

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 16:24
 Operator : DD\AJ
 Sample : L4510-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-5

Manual Integrations
 APPROVED

Ankita
 10/27/2020 10:05:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:10:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	37059084	63657187	21.545	21.662
28)	SA Decachlor...	8.127	8.989	27236878	36063680	16.978	17.231
Target Compounds							
12)	B 4,4'-DDE	5.551	6.277	6533684	11521450	3.949	3.576
17)	MA 4,4'-DDT	6.300	7.066	5175439	9036189	3.878m	4.025

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 16:24
Operator : DD\AJ
Sample : L4510-20
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
COMP-5


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:10:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

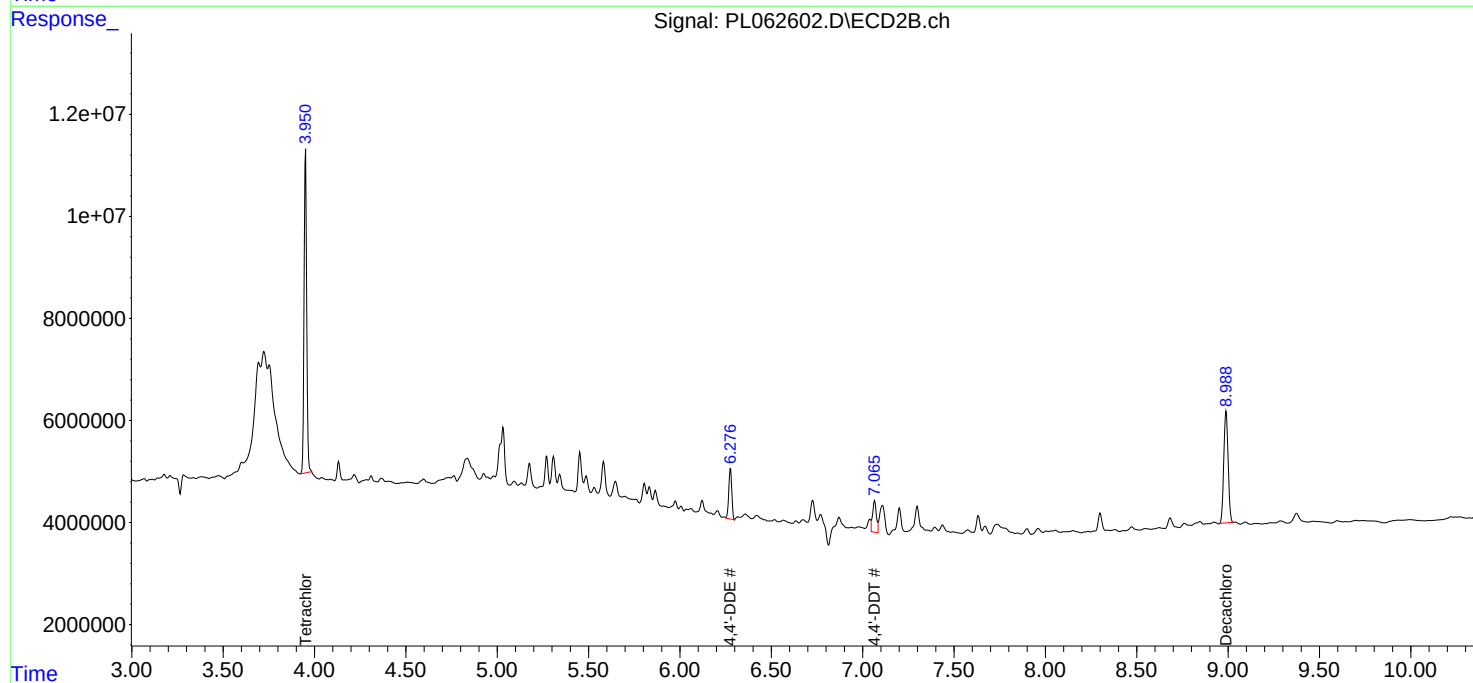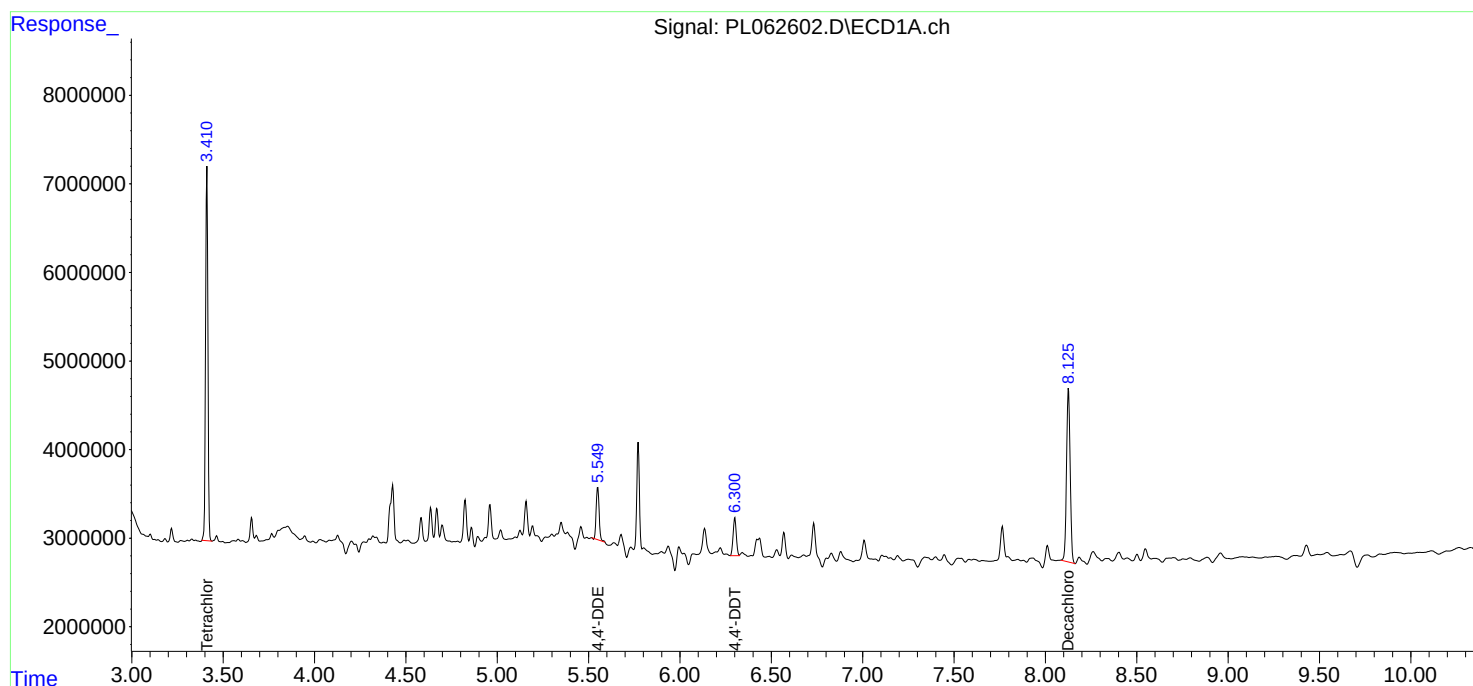

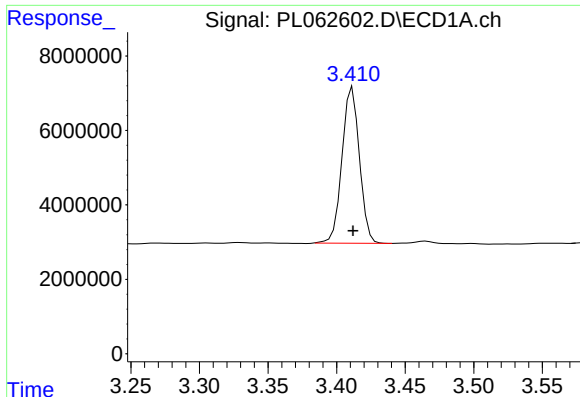


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 37059084
Conc: 21.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-5


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:27 AM

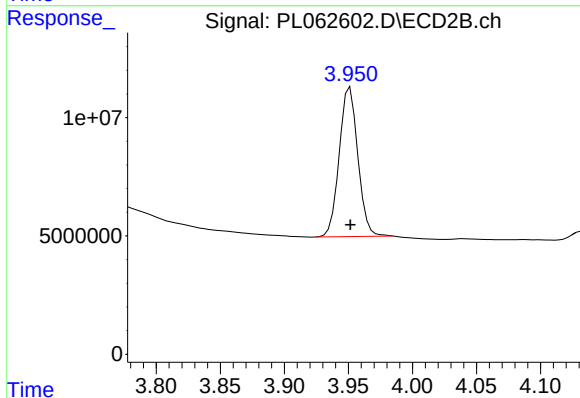


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 63657187
Conc: 21.66 ng/ml

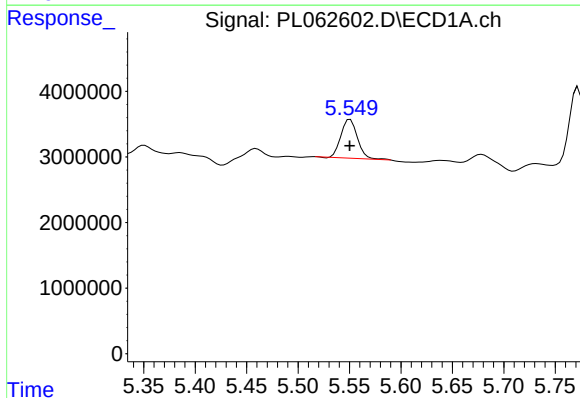


#12 4,4'-DDE

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 6533684
Conc: 3.95 ng/ml

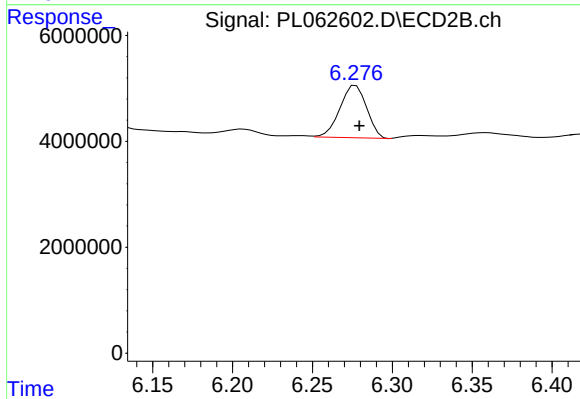

#12 4,4'-DDE

R.T.: 6.277 min
Delta R.T.: -0.002 min
Response: 11521450
Conc: 3.58 ng/ml

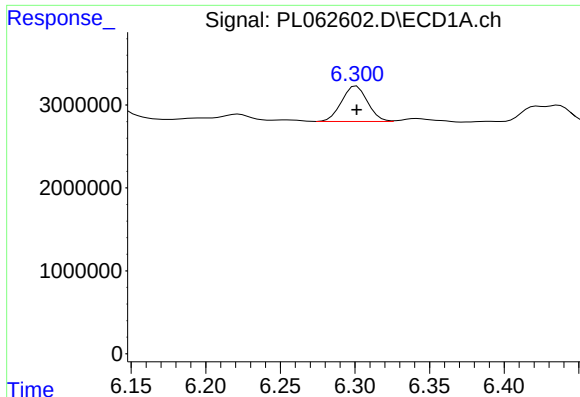


#17 4,4'-DDT

R.T.: 6.300 min
Delta R.T.: -0.001 min
Response: 5175439
Conc: 3.88 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMP-5


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:27 AM

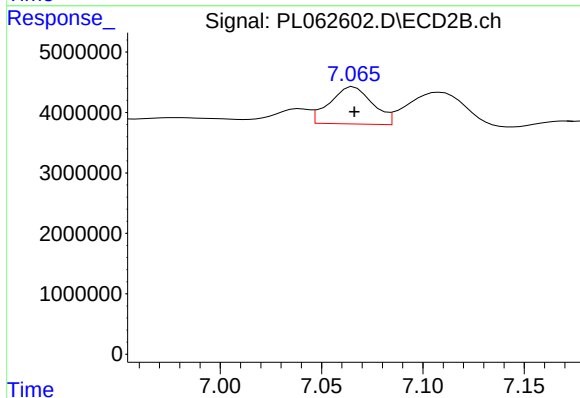


#17 4,4'-DDT

R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 9036189
Conc: 4.02 ng/ml

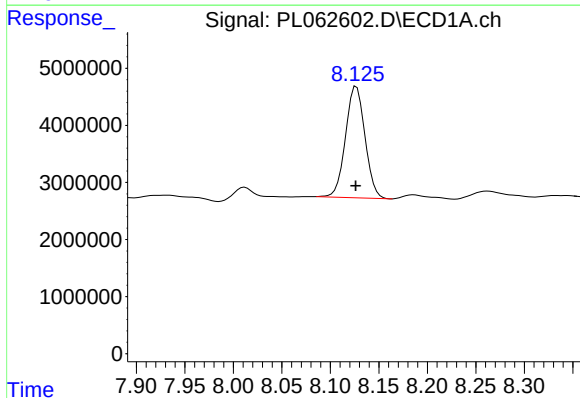

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 27236878
Conc: 16.98 ng/ml

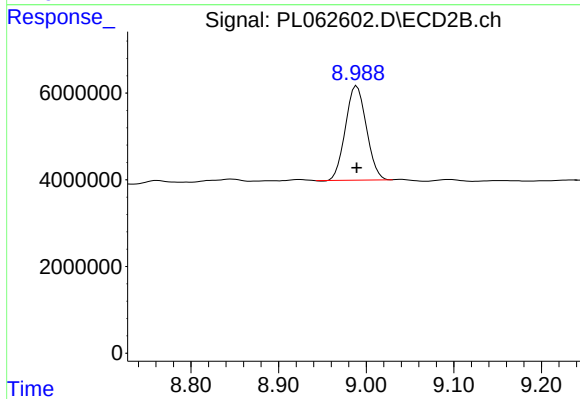

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 36063680
Conc: 17.23 ng/ml