

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 10:36
 Operator : AR\AJ
 Sample : M4340-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 13:48:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.624	5.563	10731656	31721249	21.310	20.726
28)	SA Decachlor...	10.393	11.491	12343977	24931633	16.328	17.282
Target Compounds							
2)	A alpha-BHC	5.307f	6.118f	1223396	5499555	1.762	2.354 #
3)	MA gamma-BHC...	0.000	6.535	0	1795516	N.D.	0.822 #
5)	MB Aldrin	6.488	0.000	371840	0	0.532	N.D. #
7)	B delta-BHC	0.000	7.033f	0	1497965	N.D.	0.595 #
9)	A Endosulfan I	7.494f	8.455f	901212	63600	1.338	0.034 #
10)	B gamma-Chl...	0.000	8.295	0	694846	N.D.	0.348 #
13)	MA Dieldrin	7.765	0.000	643709	0	0.916	N.D. #
15)	B Endosulfa...	0.000	9.217f	0	1251314	N.D.	0.813 #
20)	A Methoxychlor	9.093f	0.000	447268	0	1.103	N.D. #
21)	B Endrin ke...	0.000	10.044f	0	3788865	N.D.	2.187 #
25)	Chlordane-3	0.000	8.295	0	694846	N.D.	2.600 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 10:36
Operator : AR\AJ
Sample : M4340-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 13:48:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

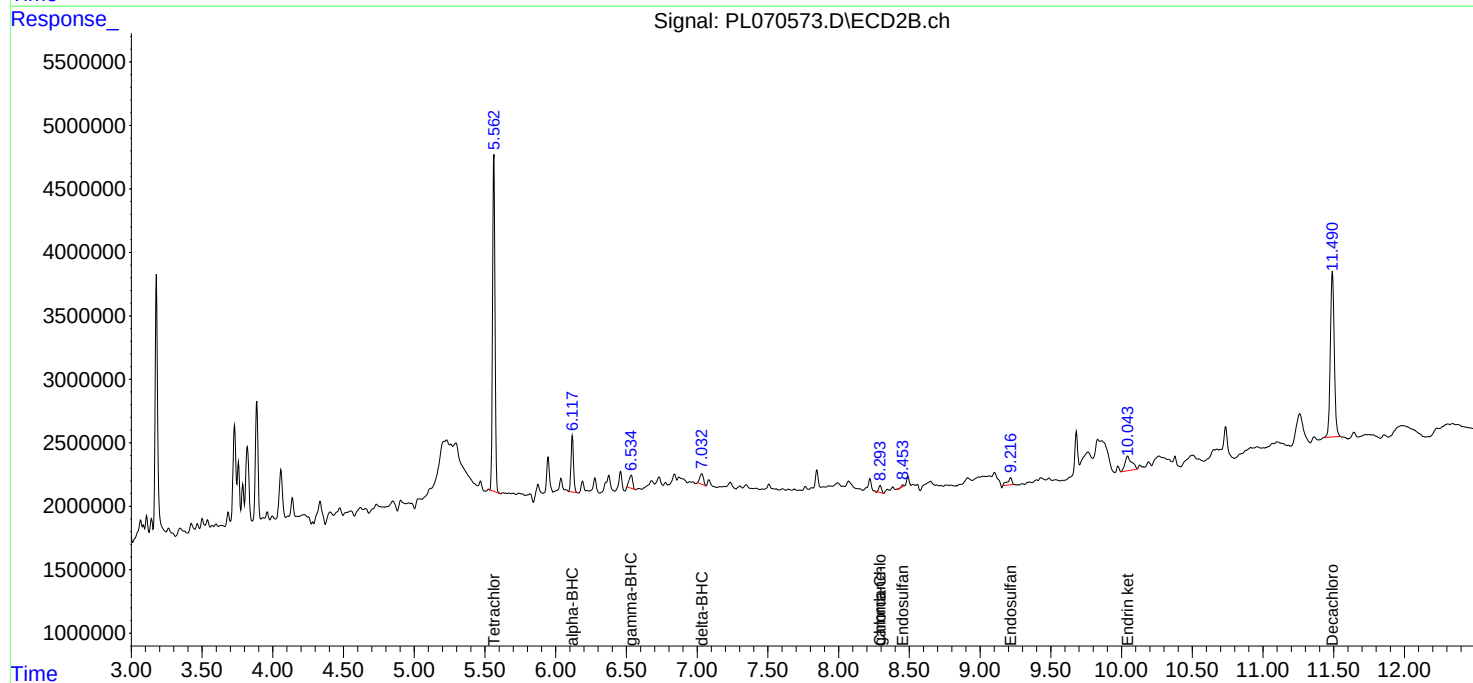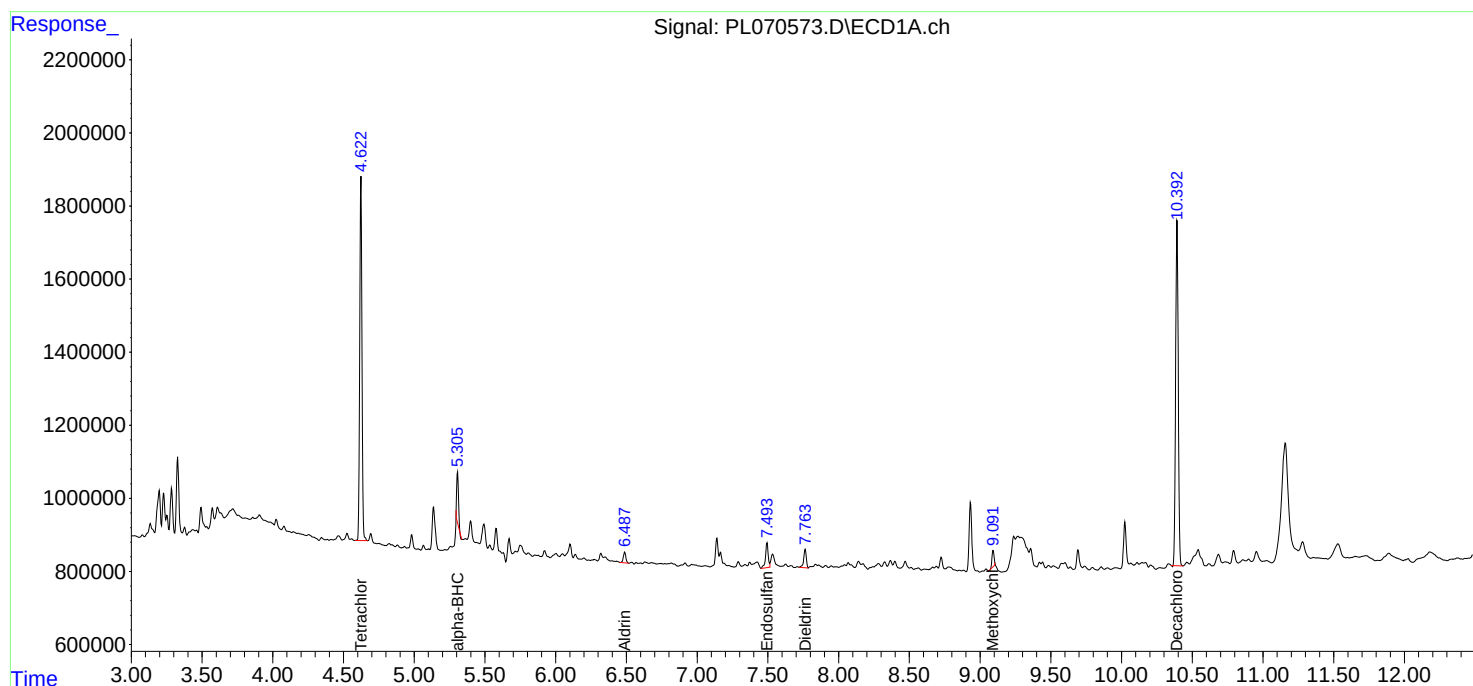

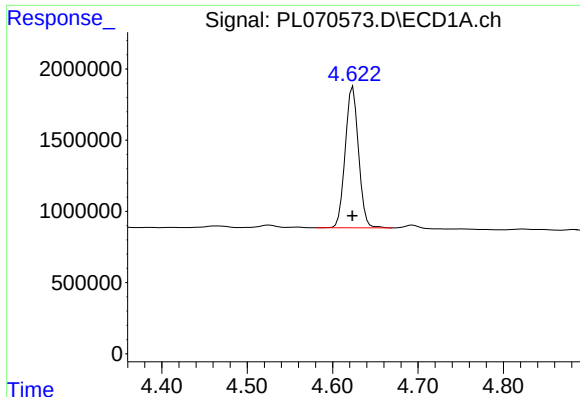


#1 Tetrachloro-m-xylene

R.T.: 4.624 min
Delta R.T.: 0.000 min
Response: 10731656
Conc: 21.31 ng/ml

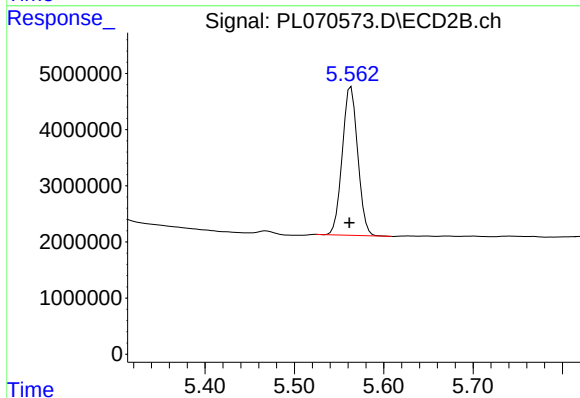


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: 0.002 min
Response: 31721249
Conc: 20.73 ng/ml

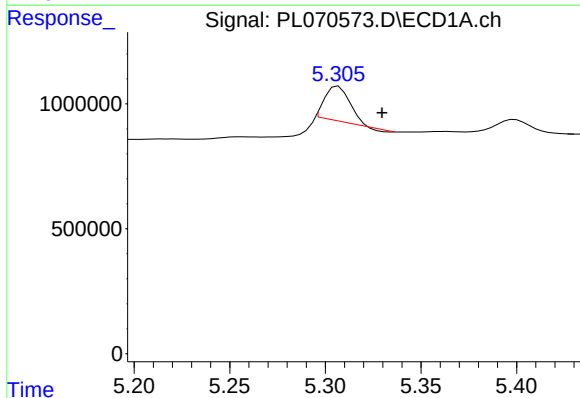


#2 alpha-BHC

R.T.: 5.307 min
Delta R.T.: -0.023 min
Response: 1223396
Conc: 1.76 ng/ml

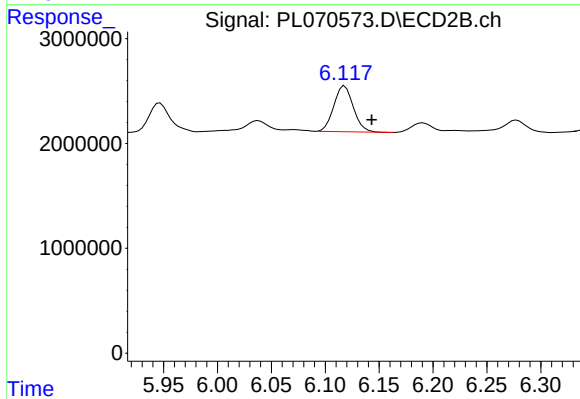


#2 alpha-BHC

R.T.: 6.118 min
Delta R.T.: -0.025 min
Response: 5499555
Conc: 2.35 ng/ml

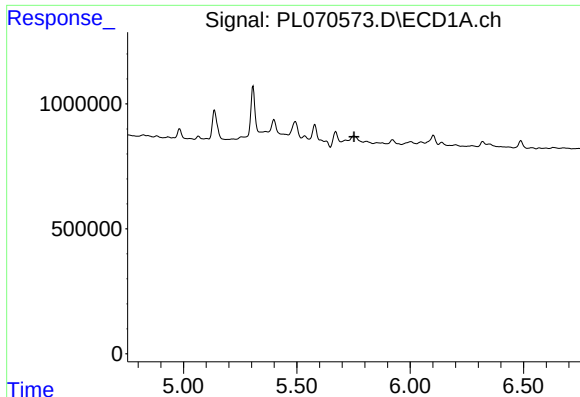


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.753 min
Response: 0
Conc: N.D.

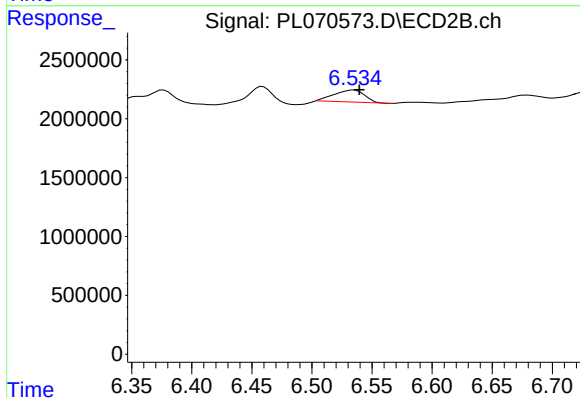


#3 gamma-BHC (Lindane)

R.T.: 6.535 min
Delta R.T.: -0.005 min
Response: 1795516
Conc: 0.82 ng/ml

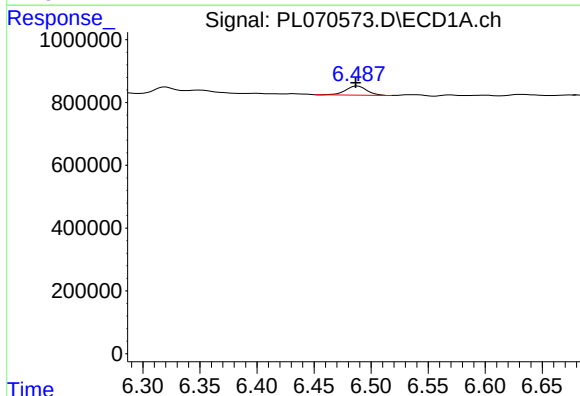


#5 Aldrin

R.T.: 6.488 min
Delta R.T.: 0.002 min
Response: 371840
Conc: 0.53 ng/ml

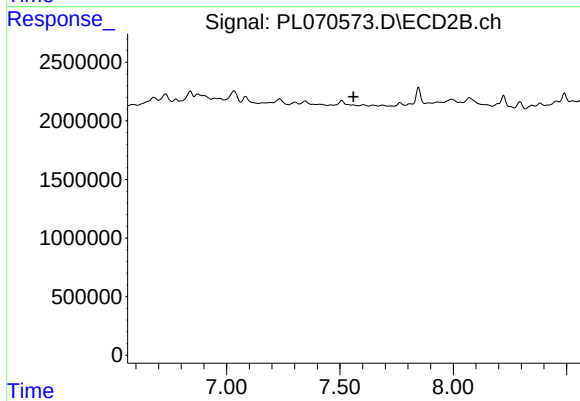


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.560 min
Response: 0
Conc: N.D.

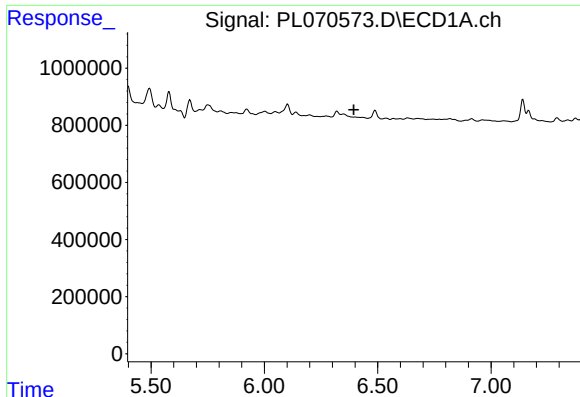


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

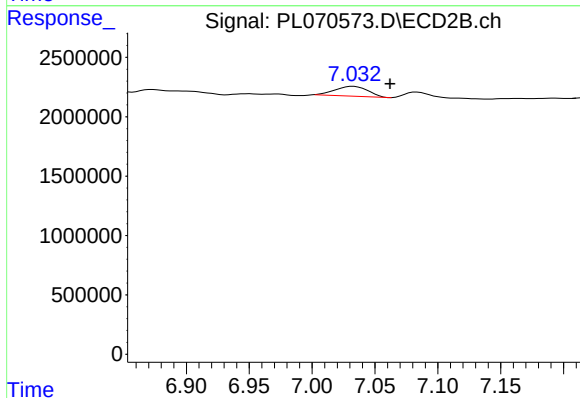


#7 delta-BHC

R.T.: 7.033 min
Delta R.T.: -0.029 min
Response: 1497965
Conc: 0.60 ng/ml

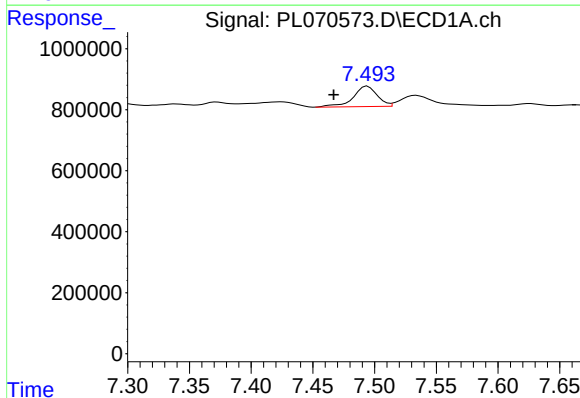


#9 Endosulfan I

R.T.: 7.494 min
Delta R.T.: 0.027 min
Response: 901212
Conc: 1.34 ng/ml

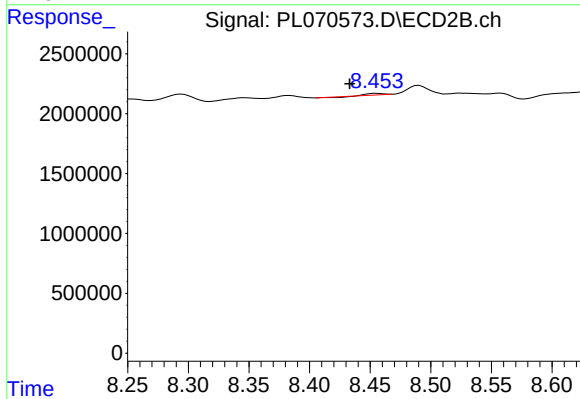


#9 Endosulfan I

R.T.: 8.455 min
Delta R.T.: 0.022 min
Response: 63600
Conc: 0.03 ng/ml

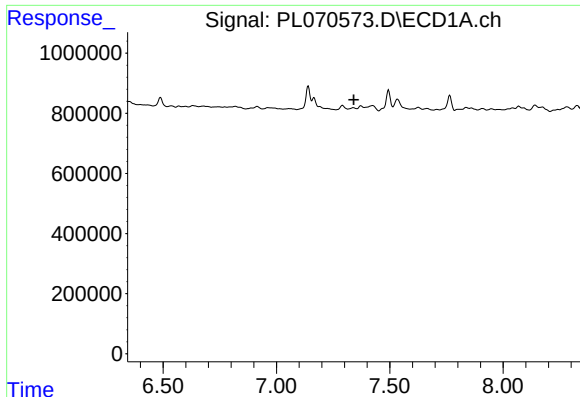


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

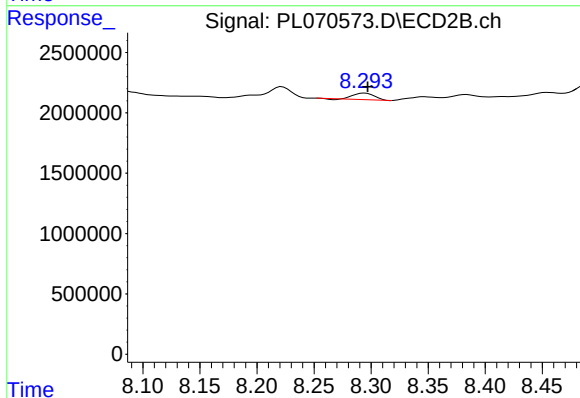


#10 gamma-Chlordane

R.T.: 8.295 min
Delta R.T.: -0.002 min
Response: 694846
Conc: 0.35 ng/ml

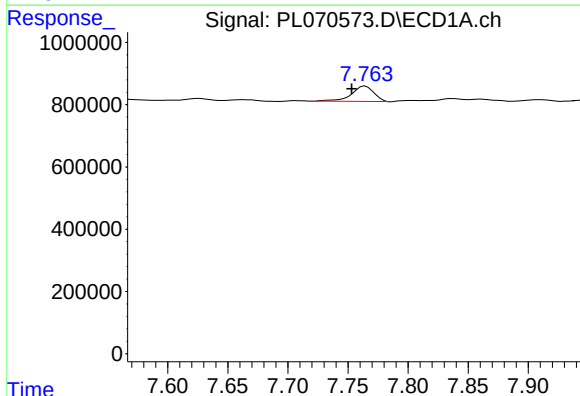


#13 Dieldrin

R.T.: 7.765 min
Delta R.T.: 0.011 min
Response: 643709
Conc: 0.92 ng/ml

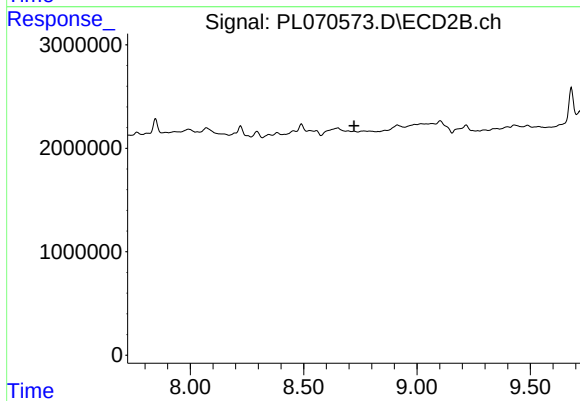


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.723 min
Response: 0
Conc: N.D.

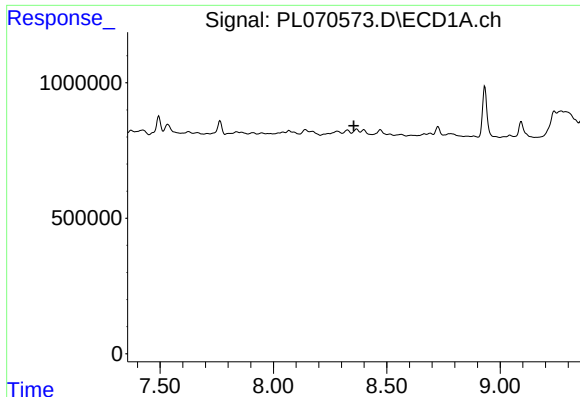


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.355 min
Response: 0
Conc: N.D.

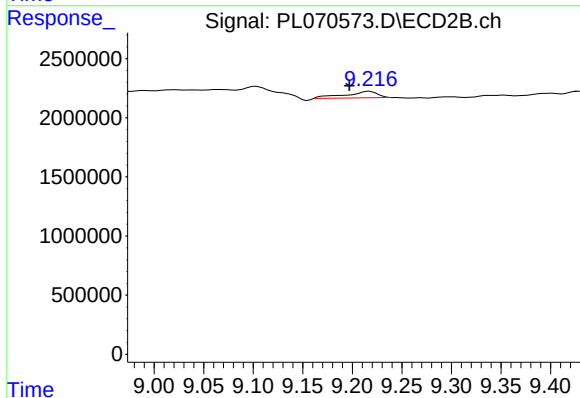


#15 Endosulfan II

R.T.: 9.217 min
Delta R.T.: 0.020 min
Response: 1251314
Conc: 0.81 ng/ml

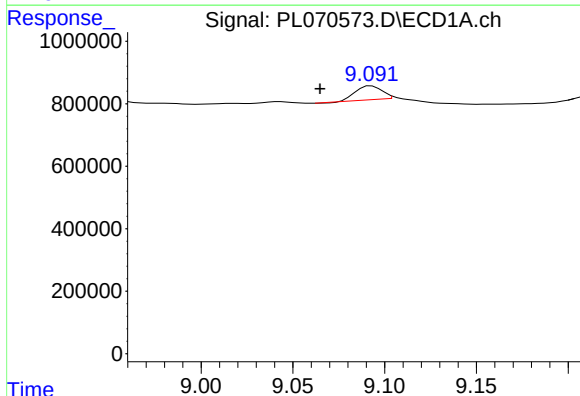


#20 Methoxychlor

R.T.: 9.093 min
Delta R.T.: 0.028 min
Response: 447268
Conc: 1.10 ng/ml

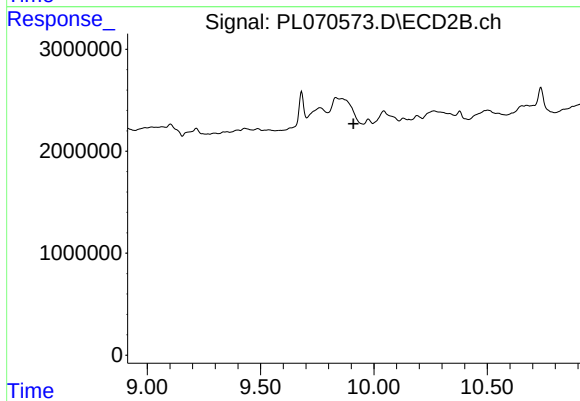


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.910 min
Response: 0
Conc: N.D.

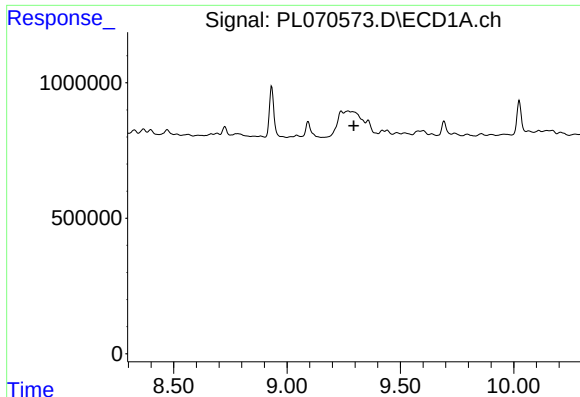


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

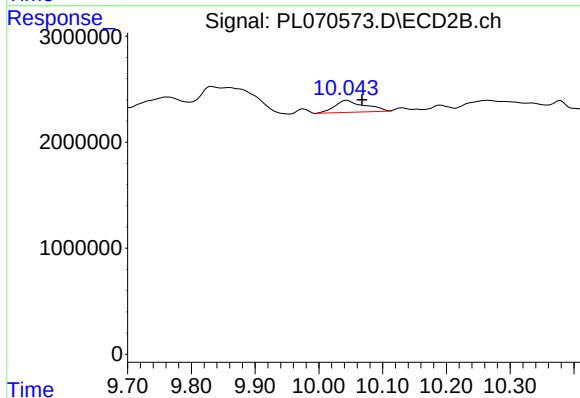


#21 Endrin ketone

R.T.: 10.044 min
Delta R.T.: -0.024 min
Response: 3788865
Conc: 2.19 ng/ml

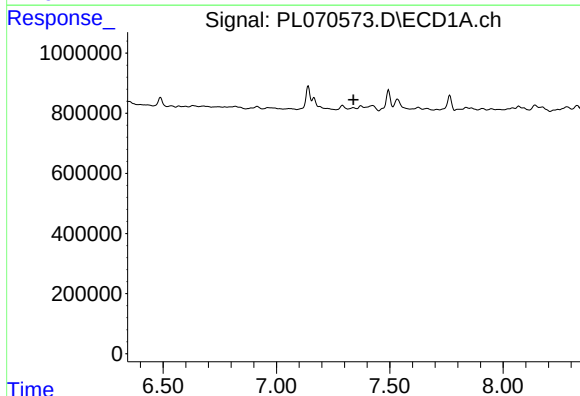


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.340 min
Response: 0
Conc: N.D.

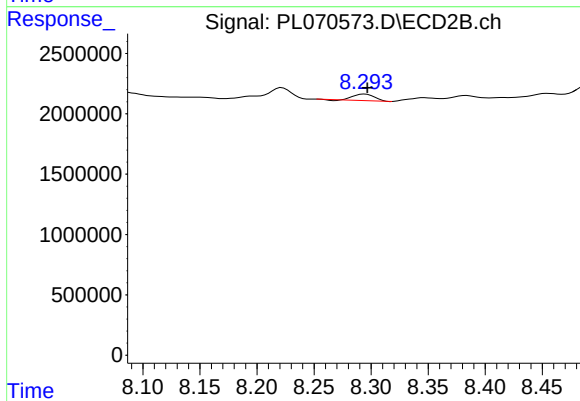


#25 Chlordane-3

R.T.: 8.295 min
Delta R.T.: -0.002 min
Response: 694846
Conc: 2.60 ng/ml

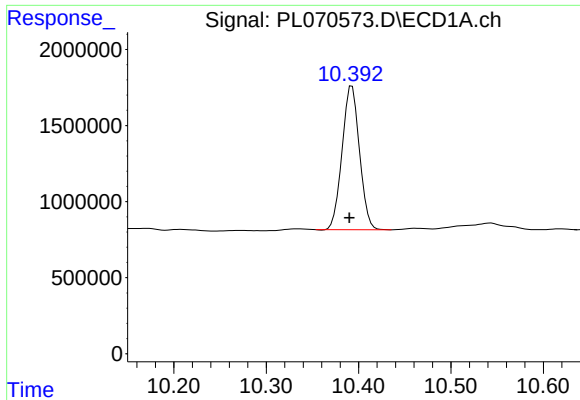

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.003 min
Response: 12343977
Conc: 16.33 ng/ml

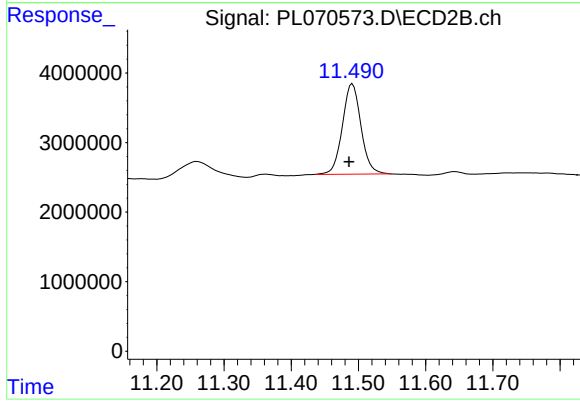

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.005 min
Response: 24931633
Conc: 17.28 ng/ml