

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 13:13
 Operator : AR\AJ
 Sample : M4348-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 17:05:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.622	5.561	5865590	16351046	11.647	10.683
28)	SA Decachlor...	10.388	11.483	5174674	9060820	6.845	6.281
Target Compounds							
3)	MA gamma-BHC...	5.751	0.000	942498	0	1.343	N.D. #
7)	B delta-BHC	0.000	7.079f	0	730074	N.D.	0.290 #
10)	B gamma-Chl...	0.000	8.295	0	965309	N.D.	0.484 #
11)	B alpha-Chl...	0.000	8.378	0	1317590	N.D.	0.673 #
12)	B 4,4'-DDE	7.622	0.000	340461	0	0.525	N.D. #
16)	A 4,4'-DDD	0.000	9.103	0	771818	N.D.	0.505 #
17)	MA 4,4'-DDT	8.466	0.000	655674	0	1.027	N.D. #
23)	Chlordane-1	0.000	6.969f	0	903179	N.D.	15.954 #
25)	Chlordane-3	0.000	8.295	0	965309	N.D.	3.612 #
26)	Chlordane-4	0.000	8.378	0	1317590	N.D.	4.156 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 13:13
Operator : AR\AJ
Sample : M4348-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 17:05:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

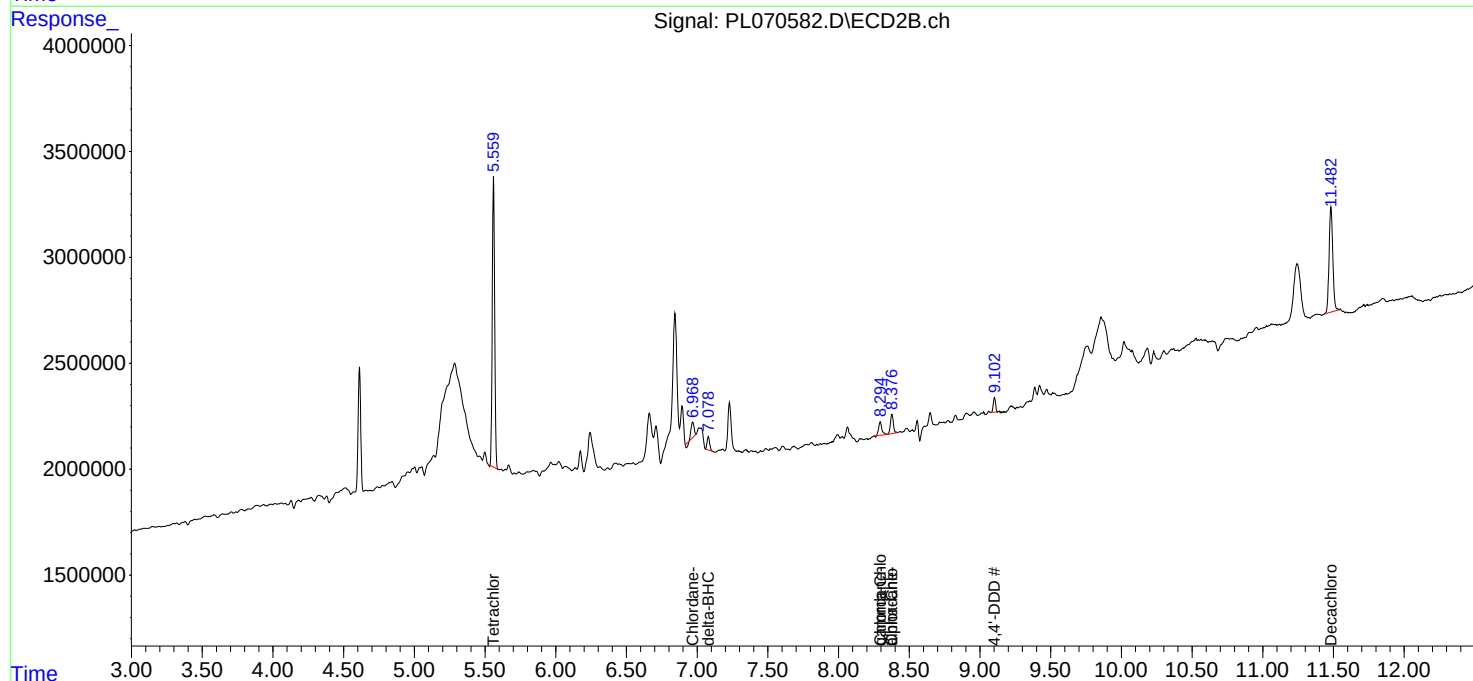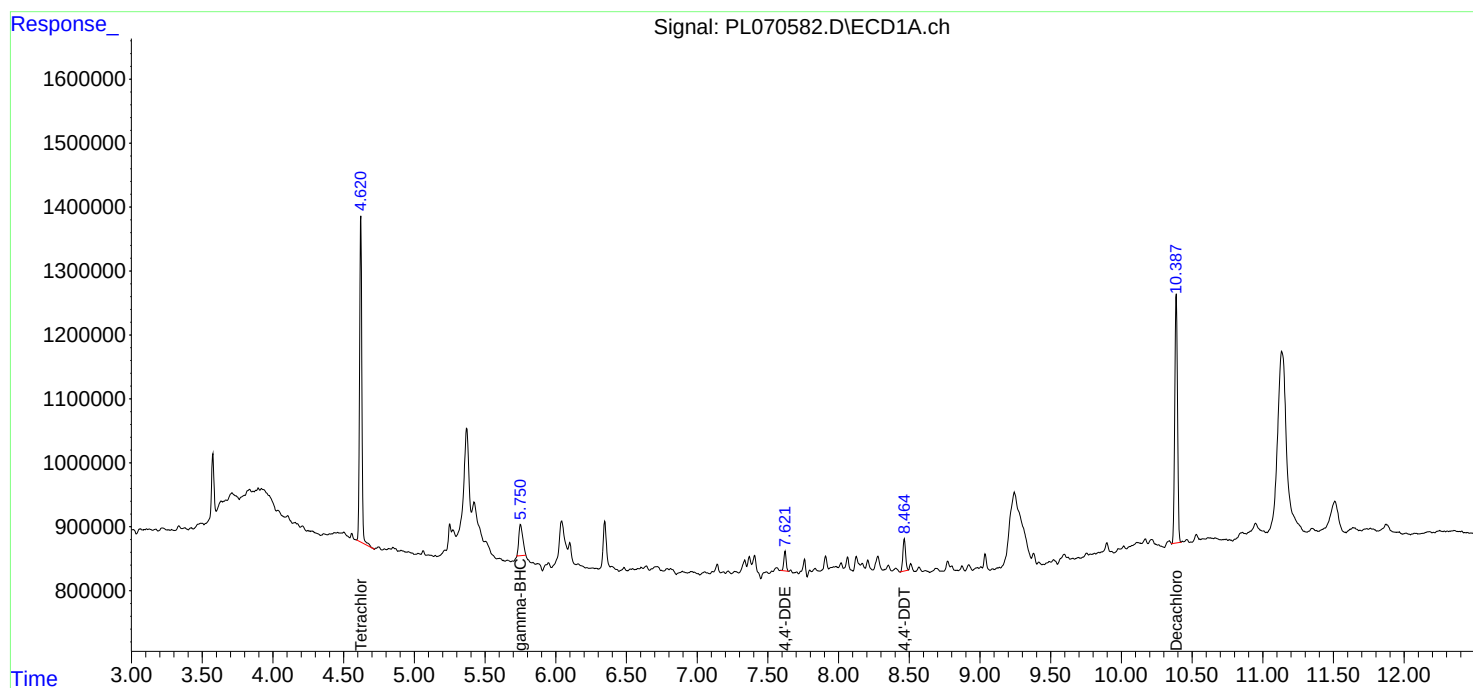

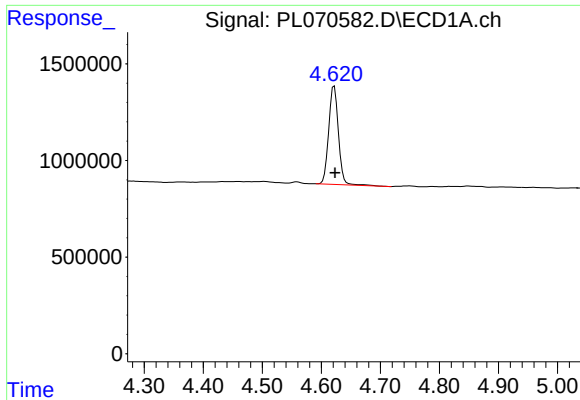


#1 Tetrachloro-m-xylene

R.T.: 4.622 min
Delta R.T.: -0.001 min
Response: 5865590
Conc: 11.65 ng/ml

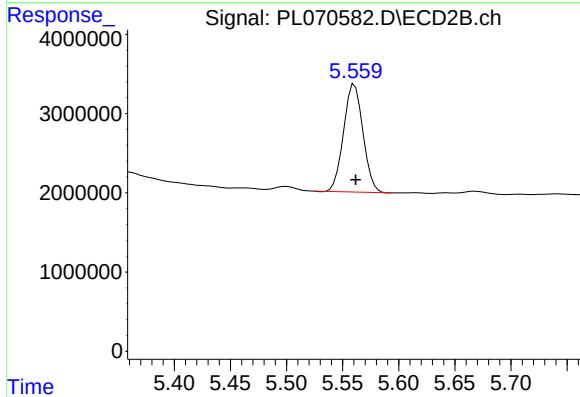


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: -0.001 min
Response: 16351046
Conc: 10.68 ng/ml

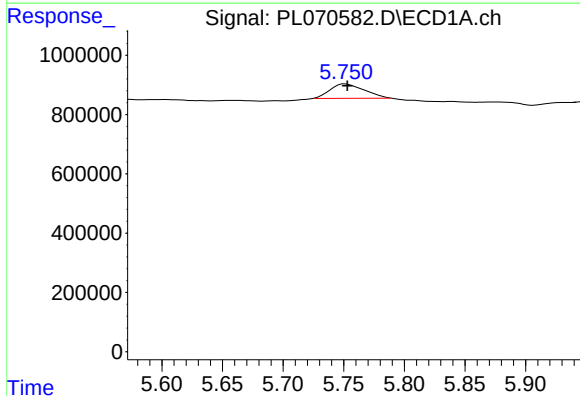


#3 gamma-BHC (Lindane)

R.T.: 5.751 min
Delta R.T.: -0.002 min
Response: 942498
Conc: 1.34 ng/ml

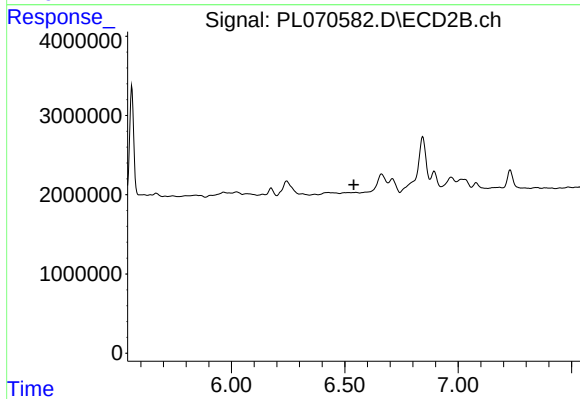


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 6.540 min
Response: 0
Conc: N.D.

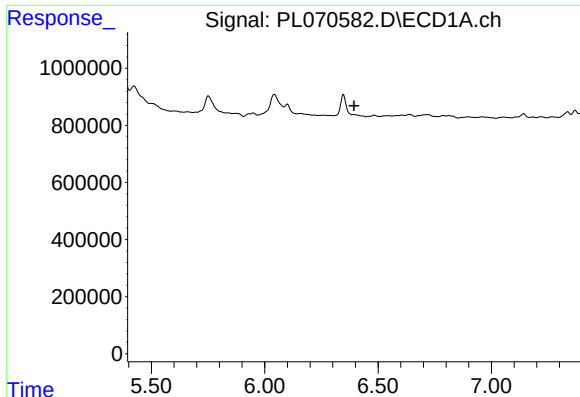


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

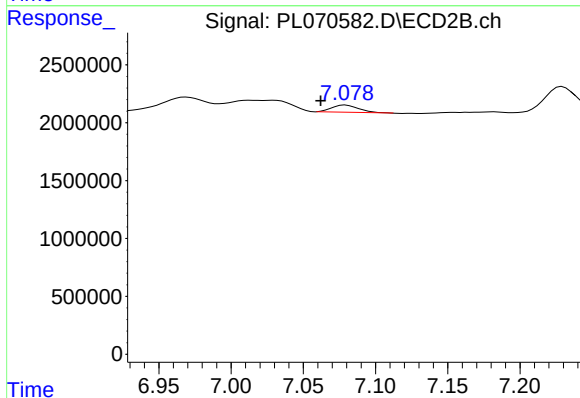


#7 delta-BHC

R.T.: 7.079 min
Delta R.T.: 0.017 min
Response: 730074
Conc: 0.29 ng/ml

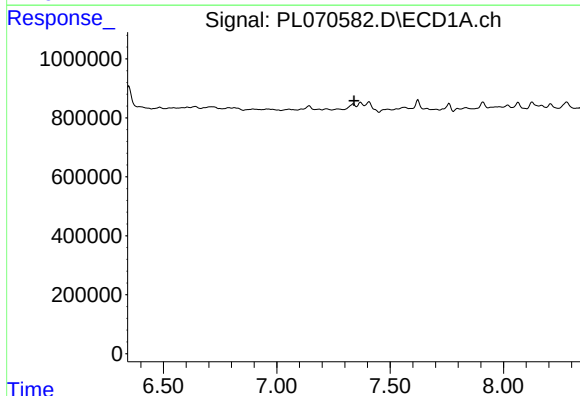


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

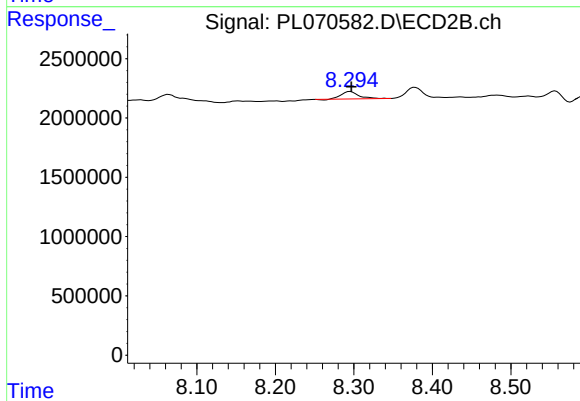


#10 gamma-Chlordane

R.T.: 8.295 min
Delta R.T.: -0.002 min
Response: 965309
Conc: 0.48 ng/ml

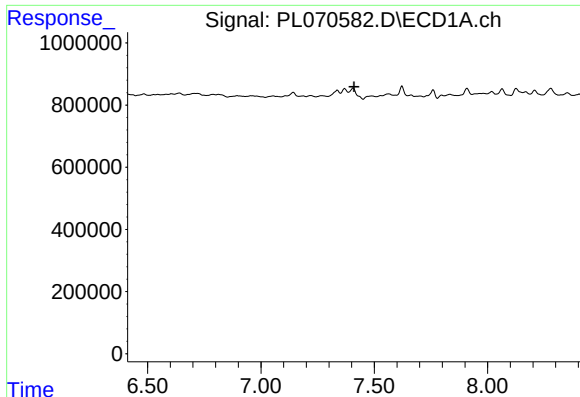


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

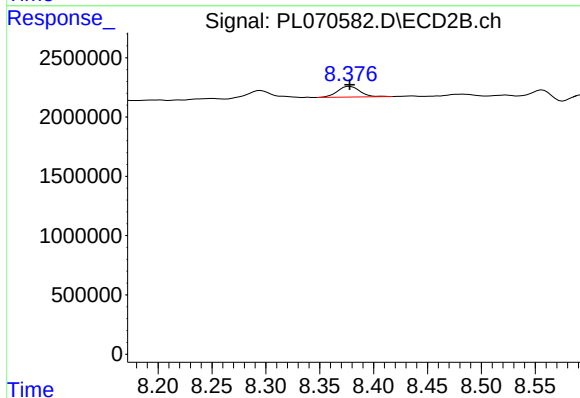


#11 alpha-Chlordane

R.T.: 8.378 min
Delta R.T.: 0.000 min
Response: 1317590
Conc: 0.67 ng/ml

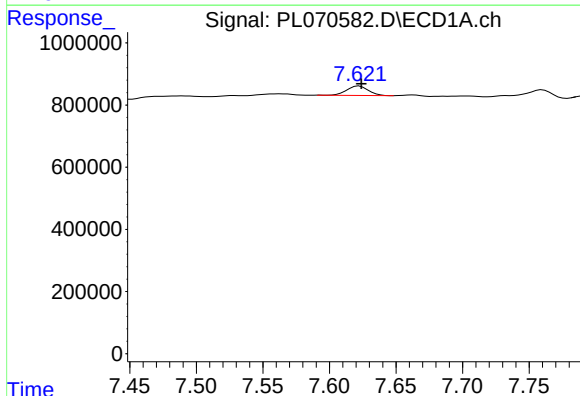


#12 4,4'-DDE

R.T.: 7.622 min
Delta R.T.: -0.002 min
Response: 340461
Conc: 0.53 ng/ml

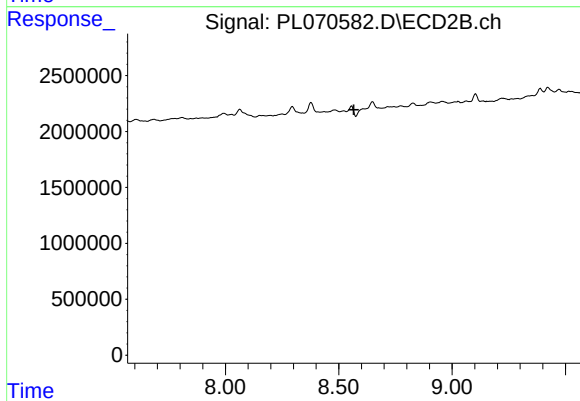


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.566 min
Response: 0
Conc: N.D.

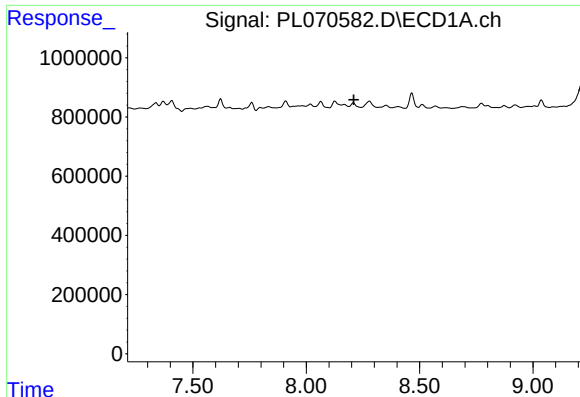


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.210 min
Response: 0
Conc: N.D.

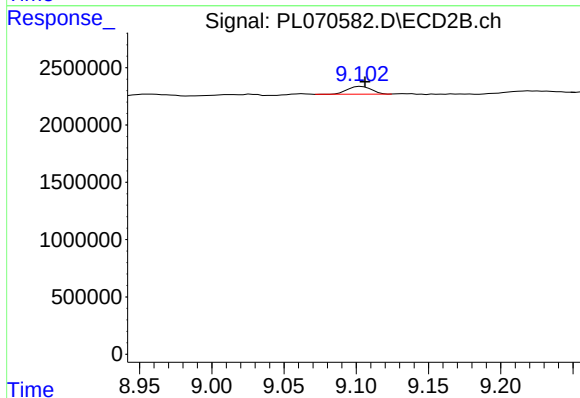


#16 4,4'-DDD

R.T.: 9.103 min
Delta R.T.: -0.003 min
Response: 771818
Conc: 0.50 ng/ml

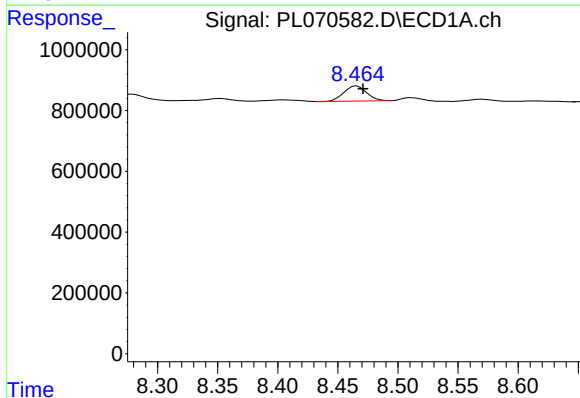


#17 4,4'-DDT

R.T.: 8.466 min
Delta R.T.: -0.005 min
Response: 655674
Conc: 1.03 ng/ml

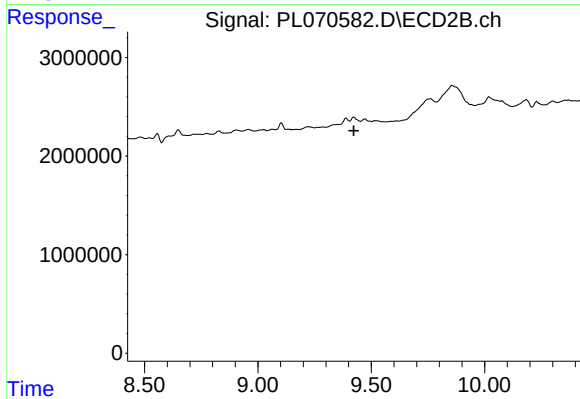


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 9.424 min
Response: 0
Conc: N.D.

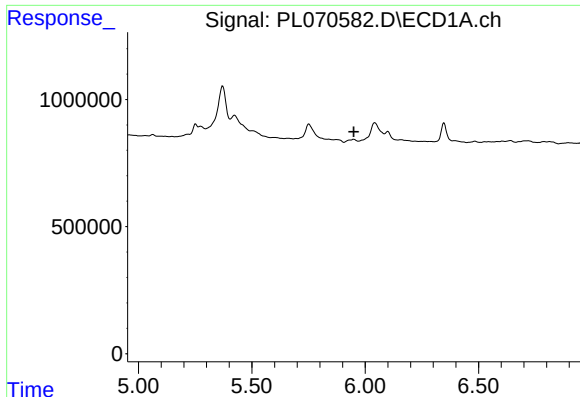


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.950 min
Response: 0
Conc: N.D.

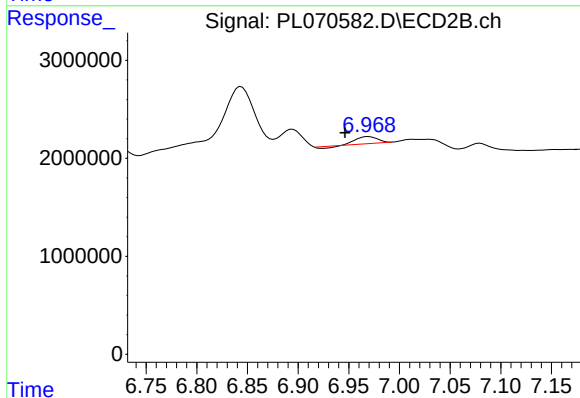


#23 Chlordane-1

R.T.: 6.969 min
Delta R.T.: 0.023 min
Response: 903179
Conc: 15.95 ng/ml

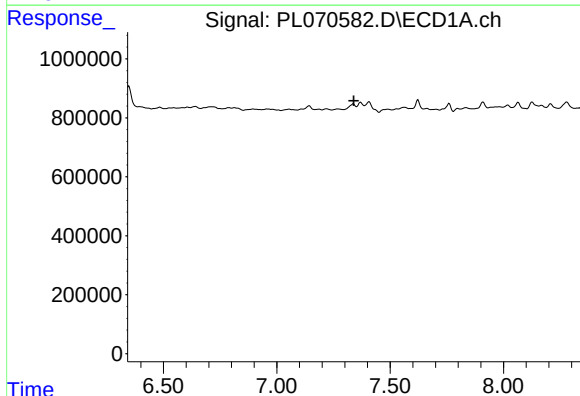


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.340 min
Response: 0
Conc: N.D.

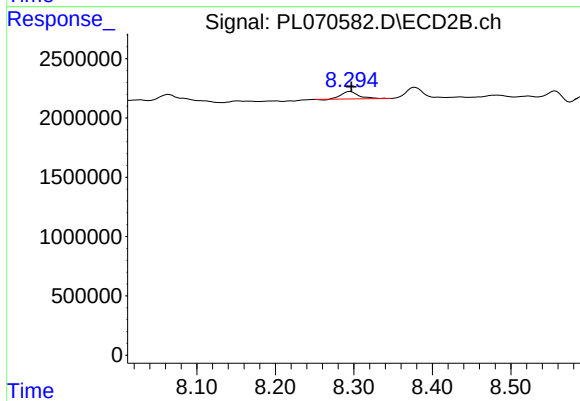


#25 Chlordane-3

R.T.: 8.295 min
Delta R.T.: -0.001 min
Response: 965309
Conc: 3.61 ng/ml

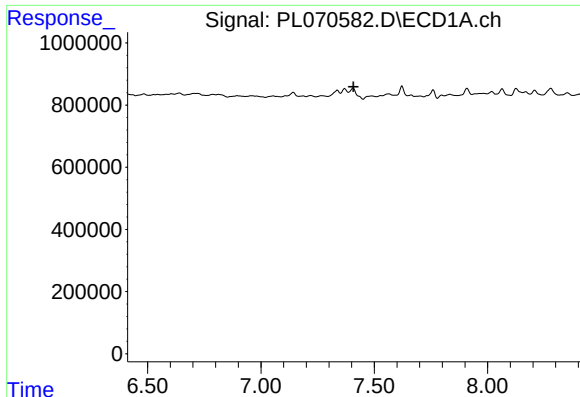


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.409 min
Response: 0
Conc: N.D.

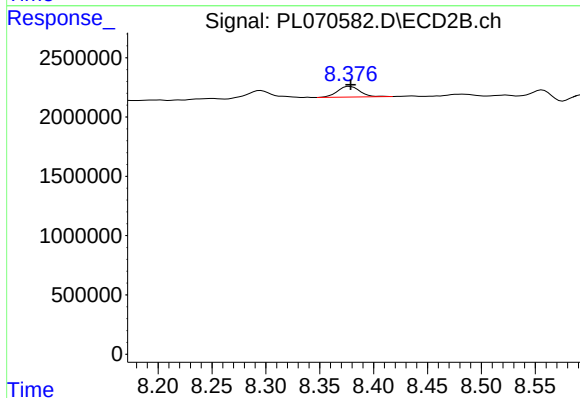


#26 Chlordane-4

R.T.: 8.378 min
Delta R.T.: -0.001 min
Response: 1317590
Conc: 4.16 ng/ml

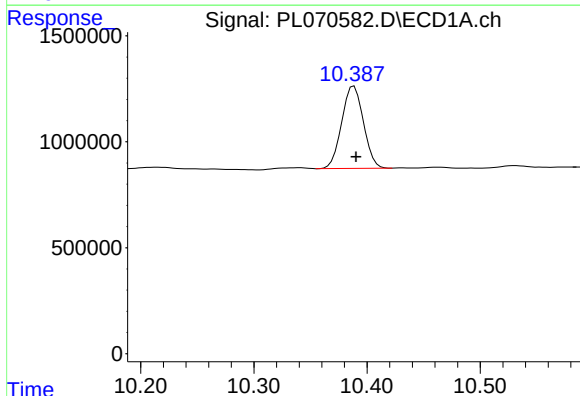

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.002 min
Response: 5174674
Conc: 6.84 ng/ml

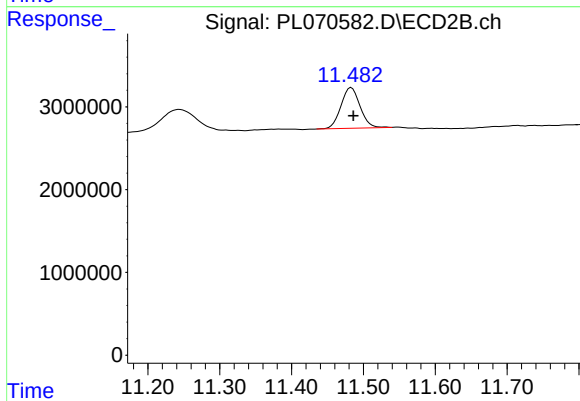

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.003 min
Response: 9060820
Conc: 6.28 ng/ml