

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 18:22
 Operator : AR\AJ
 Sample : M4358-07
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 04:13:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.622	5.560	6747151	20240078	13.398	13.224
28)	SA Decachlor...	10.387	11.482	7934042	14023803	10.495	9.721
Target Compounds							
7)	B delta-BHC	0.000	7.079f	0	766861	N.D.	0.305 #
10)	B gamma-Chl...	0.000	8.293	0	223079	N.D.	0.112 #
11)	B alpha-Chl...	0.000	8.375	0	1183120	N.D.	0.604 #
14)	MA Endrin	0.000	8.987f	0	873633	N.D.	0.538 #
16)	A 4,4'-DDD	0.000	9.099	0	947539	N.D.	0.619 #
17)	MA 4,4'-DDT	8.464	9.421	1153927	355447	1.807	0.206 #
19)	B Endosulfa...	8.772	0.000	642420	0	0.941	N.D. #
25)	Chlordane-3	0.000	8.293	0	223079	N.D.	0.835 #
26)	Chlordane-4	0.000	8.375	0	1183120	N.D.	3.732 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 18:22
Operator : AR\AJ
Sample : M4358-07
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 04:13:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

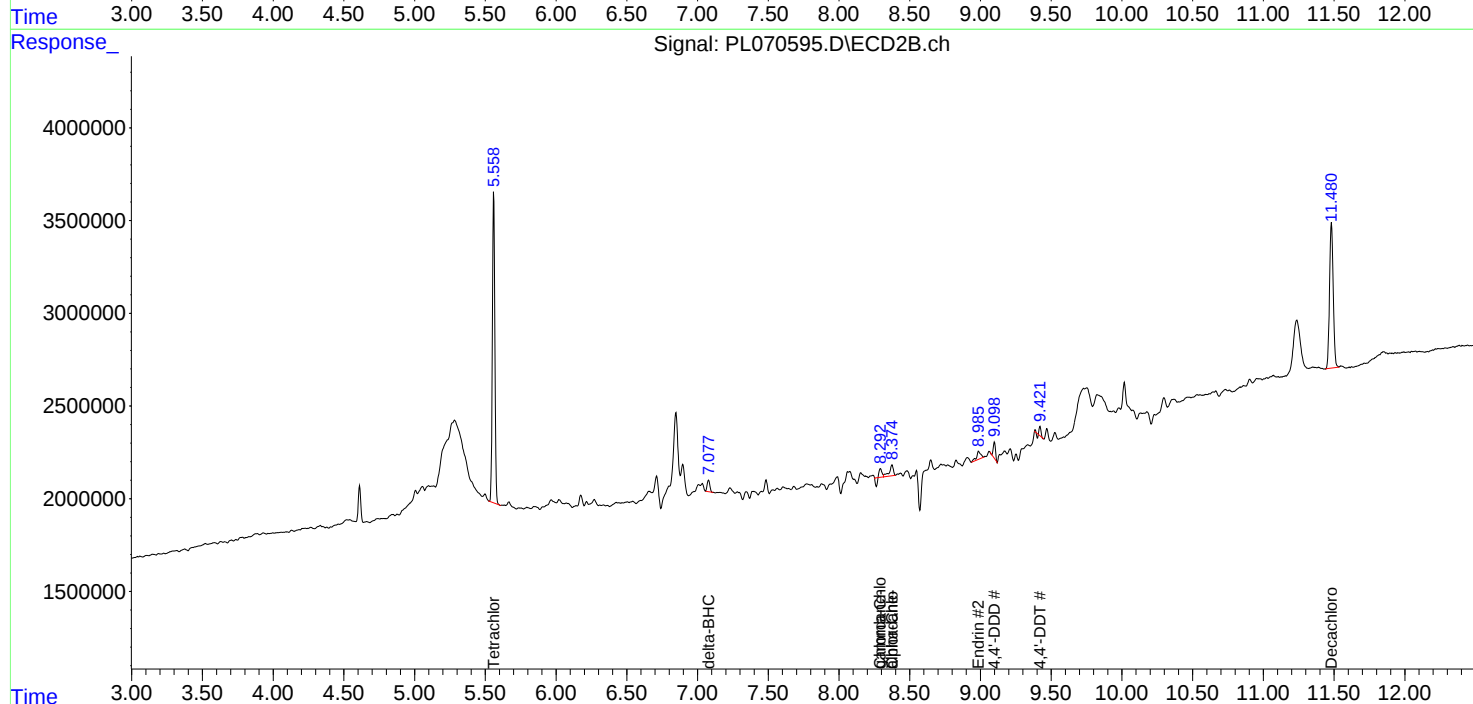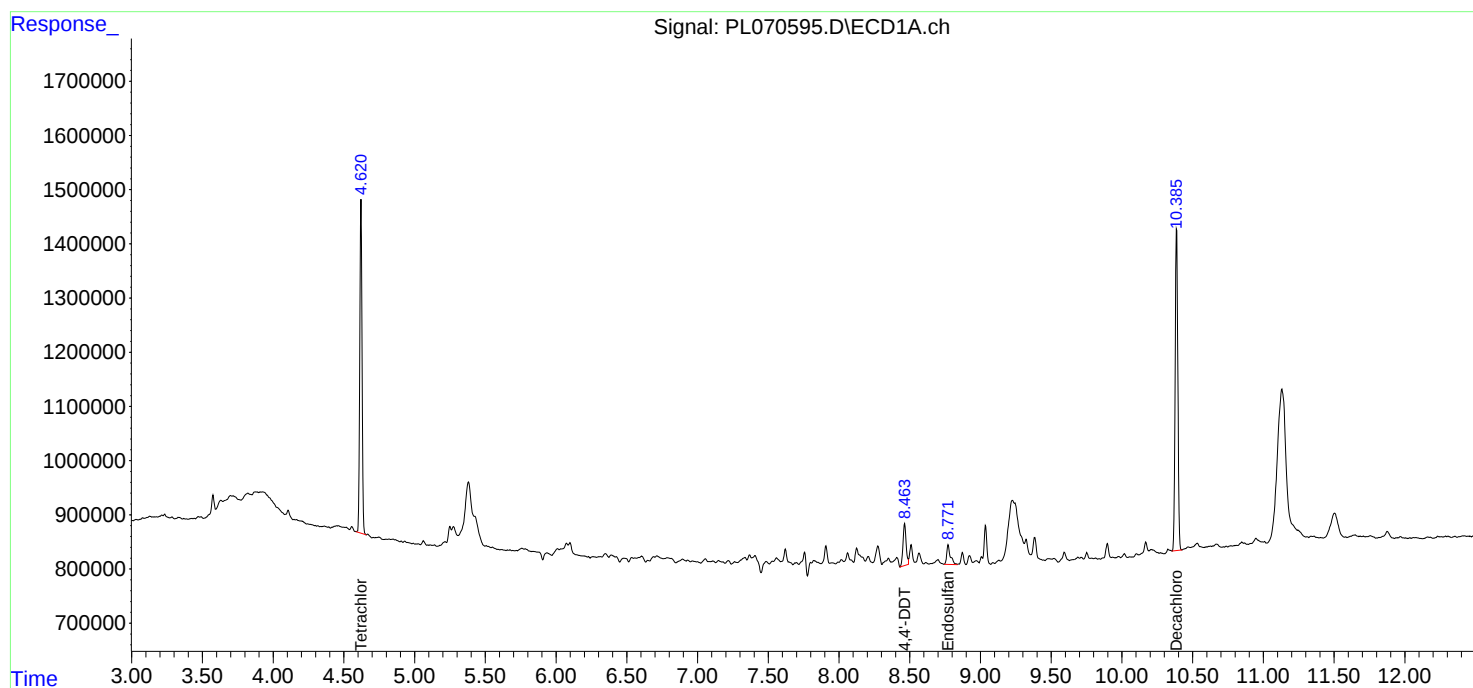

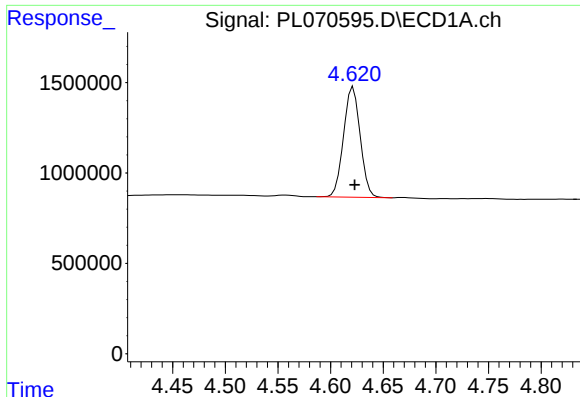


#1 Tetrachloro-m-xylene

R.T.: 4.622 min
Delta R.T.: -0.001 min
Response: 6747151
Conc: 13.40 ng/ml

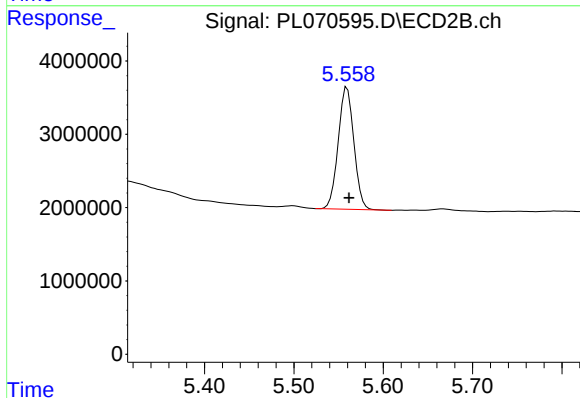


#1 Tetrachloro-m-xylene

R.T.: 5.560 min
Delta R.T.: -0.002 min
Response: 20240078
Conc: 13.22 ng/ml

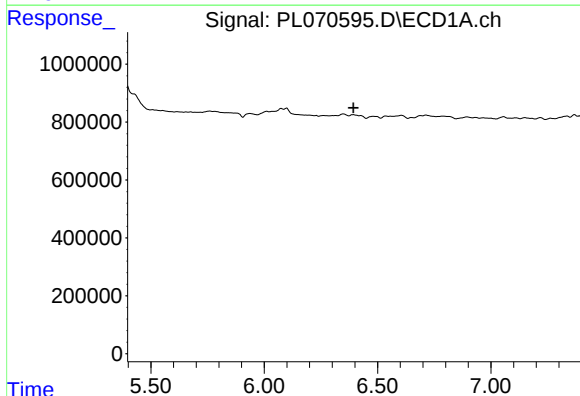


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

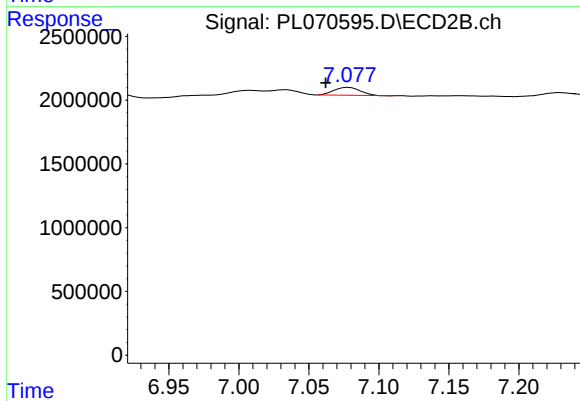


#7 delta-BHC

R.T.: 7.079 min
Delta R.T.: 0.017 min
Response: 766861
Conc: 0.30 ng/ml

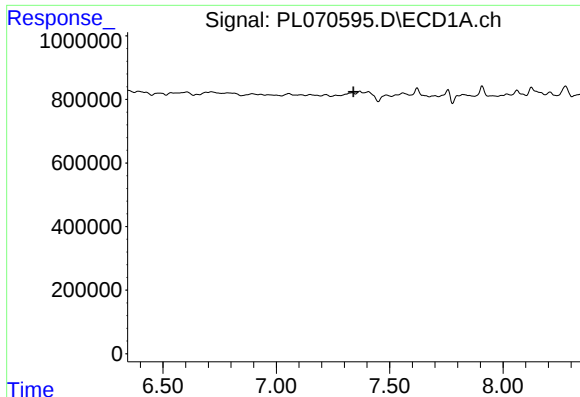


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

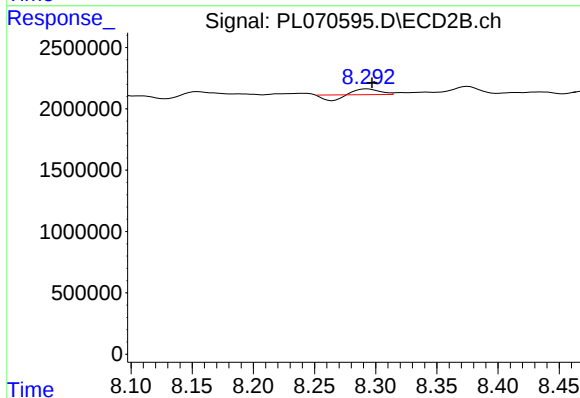


#10 gamma-Chlordane

R.T.: 8.293 min
Delta R.T.: -0.004 min
Response: 223079
Conc: 0.11 ng/ml

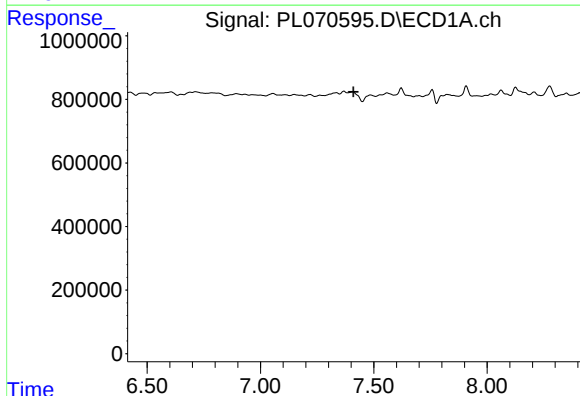


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

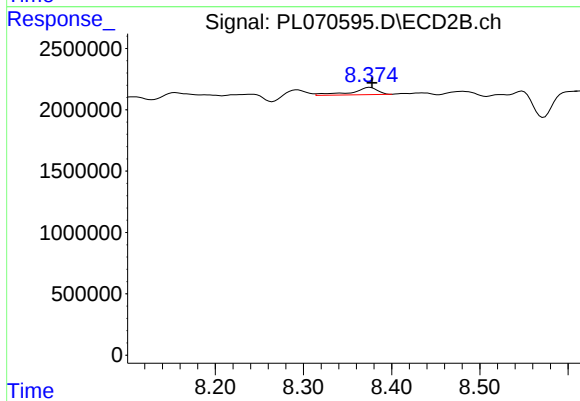


#11 alpha-Chlordane

R.T.: 8.375 min
Delta R.T.: -0.002 min
Response: 1183120
Conc: 0.60 ng/ml

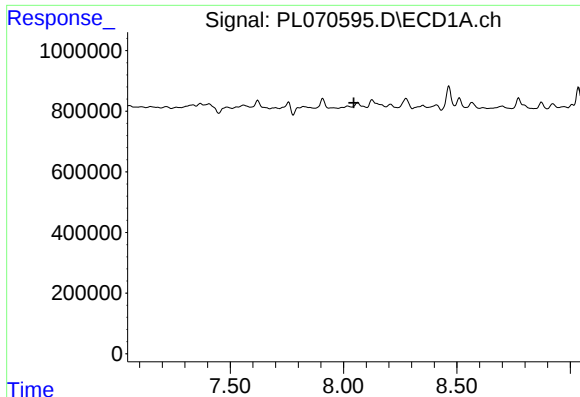


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.045 min
Response: 0
Conc: N.D.

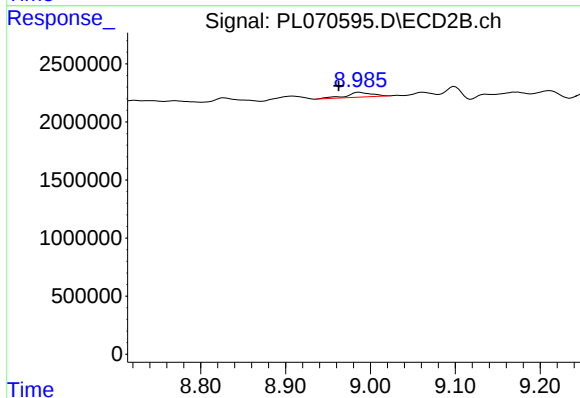


#14 Endrin

R.T.: 8.987 min
Delta R.T.: 0.024 min
Response: 873633
Conc: 0.54 ng/ml

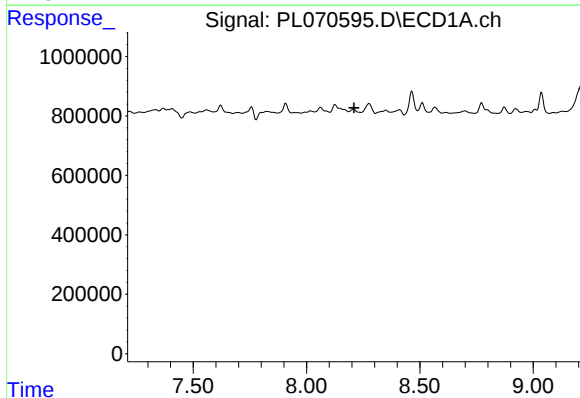


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.210 min
Response: 0
Conc: N.D.

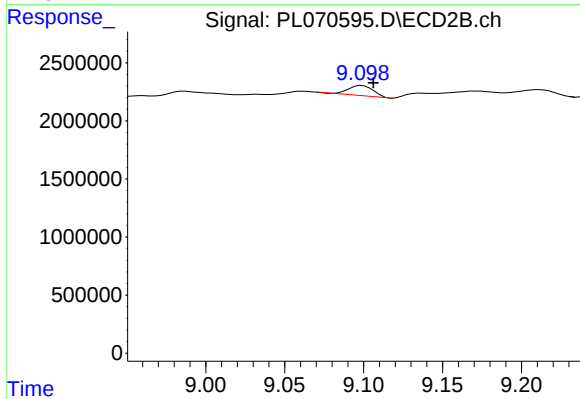


#16 4,4'-DDD

R.T.: 9.099 min
Delta R.T.: -0.007 min
Response: 947539
Conc: 0.62 ng/ml

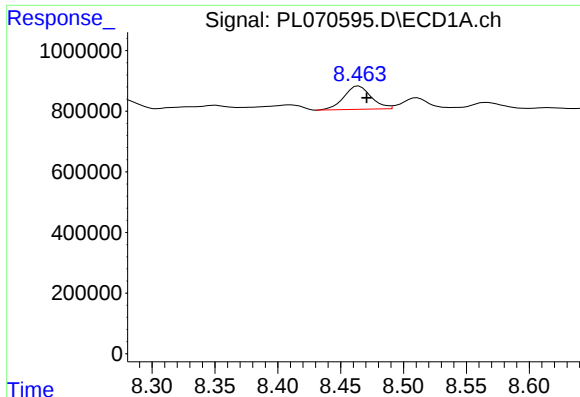


#17 4,4'-DDT

R.T.: 8.464 min
Delta R.T.: -0.006 min
Response: 1153927
Conc: 1.81 ng/ml

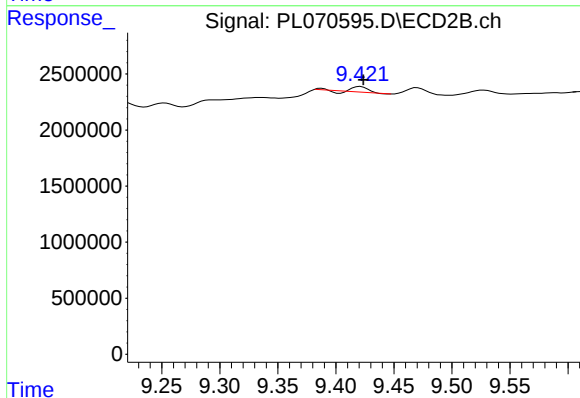


#17 4,4'-DDT

R.T.: 9.421 min
Delta R.T.: -0.002 min
Response: 355447
Conc: 0.21 ng/ml

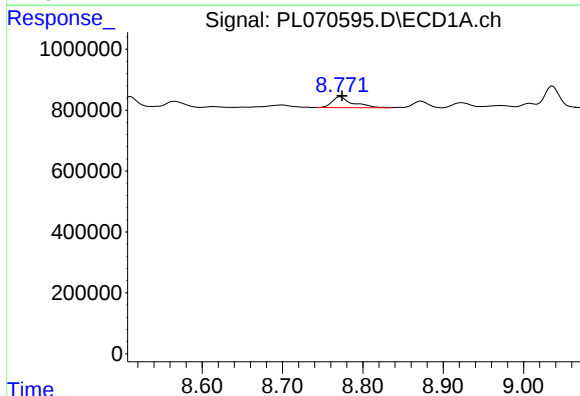


#19 Endosulfan Sulfate

R.T.: 8.772 min
Delta R.T.: -0.002 min
Response: 642420
Conc: 0.94 ng/ml

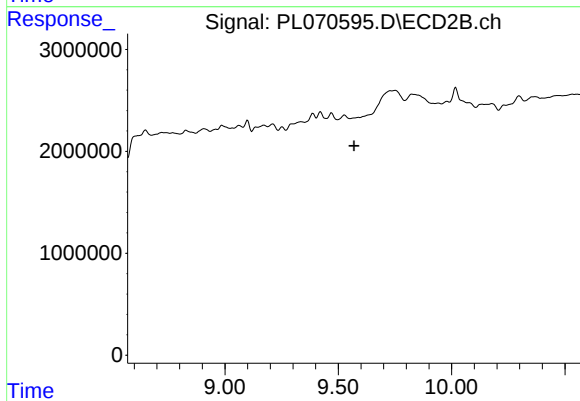


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.570 min
Response: 0
Conc: N.D.

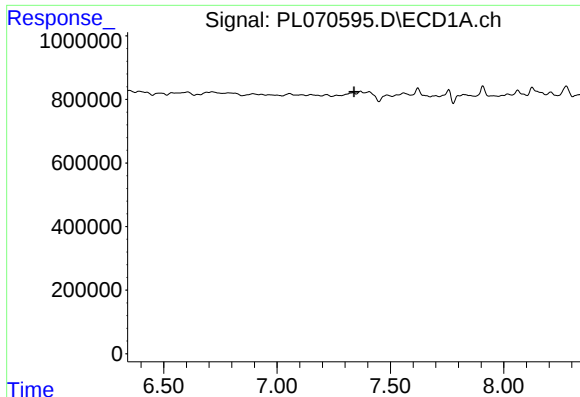


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.340 min
Response: 0
Conc: N.D.

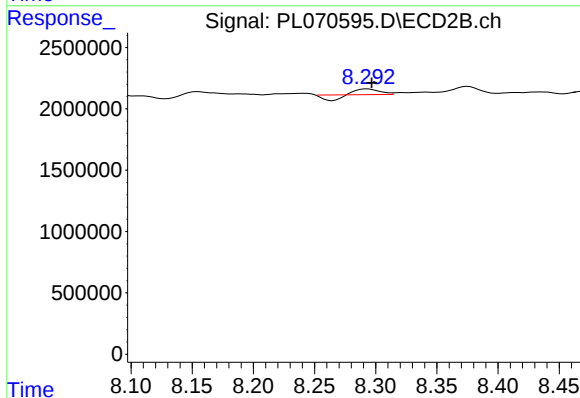


#25 Chlordane-3

R.T.: 8.293 min
Delta R.T.: -0.004 min
Response: 223079
Conc: 0.83 ng/ml

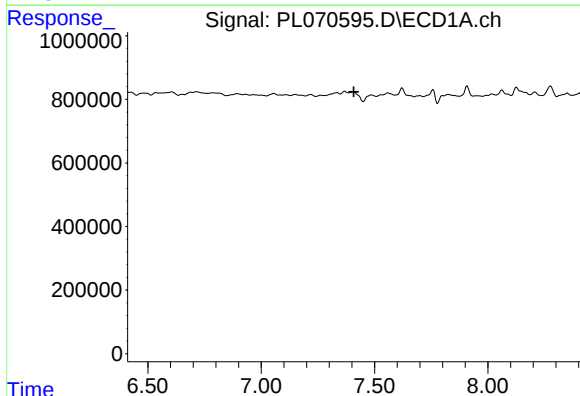


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.409 min
Response: 0
Conc: N.D.

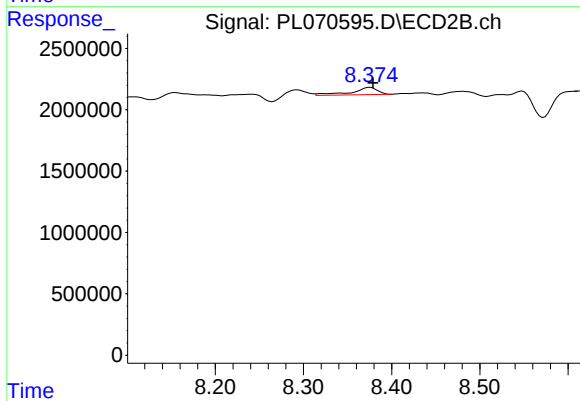


#26 Chlordane-4

R.T.: 8.375 min
Delta R.T.: -0.003 min
Response: 1183120
Conc: 3.73 ng/ml

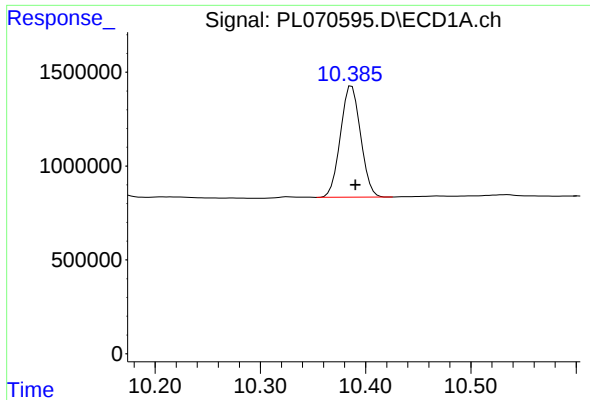

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.004 min
Response: 7934042
Conc: 10.49 ng/ml

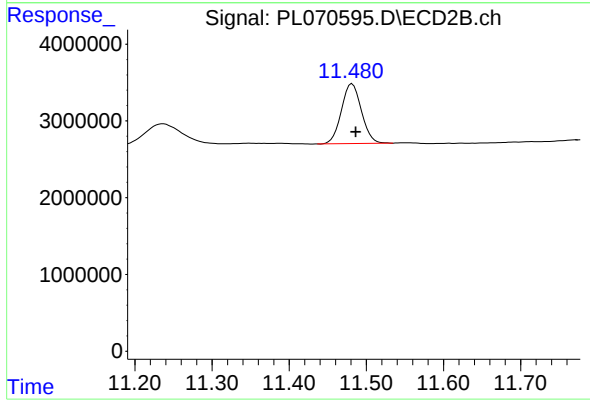

#28 Decachlorobiphenyl

R.T.: 11.482 min
Delta R.T.: -0.004 min
Response: 14023803
Conc: 9.72 ng/ml