

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 22:49
 Operator : AR\AJ
 Sample : M4367-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 04:14:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.621	5.560	6200020	18300320	12.311	11.957
28)	SA Decachlor...	10.387	11.481	8379717	14273047	11.084	9.894
Target Compounds							
7)	B delta-BHC	0.000	7.081f	0	1067965	N.D.	0.424 #
10)	B gamma-Chl...	7.338	8.293	385677	1555632	0.538	0.779 #
11)	B alpha-Chl...	7.406	8.376	723840	2449869	0.995	1.251 #
20)	A Methoxychlor	0.000	9.935f	0	74155	N.D.	0.075 #
25)	Chlordane-3	7.338	8.293	385677	1555632	5.723	5.820
26)	Chlordane-4	7.406	8.376	723840	2449869	10.080	7.727


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 22:49
Operator : AR\AJ
Sample : M4367-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 04:14:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

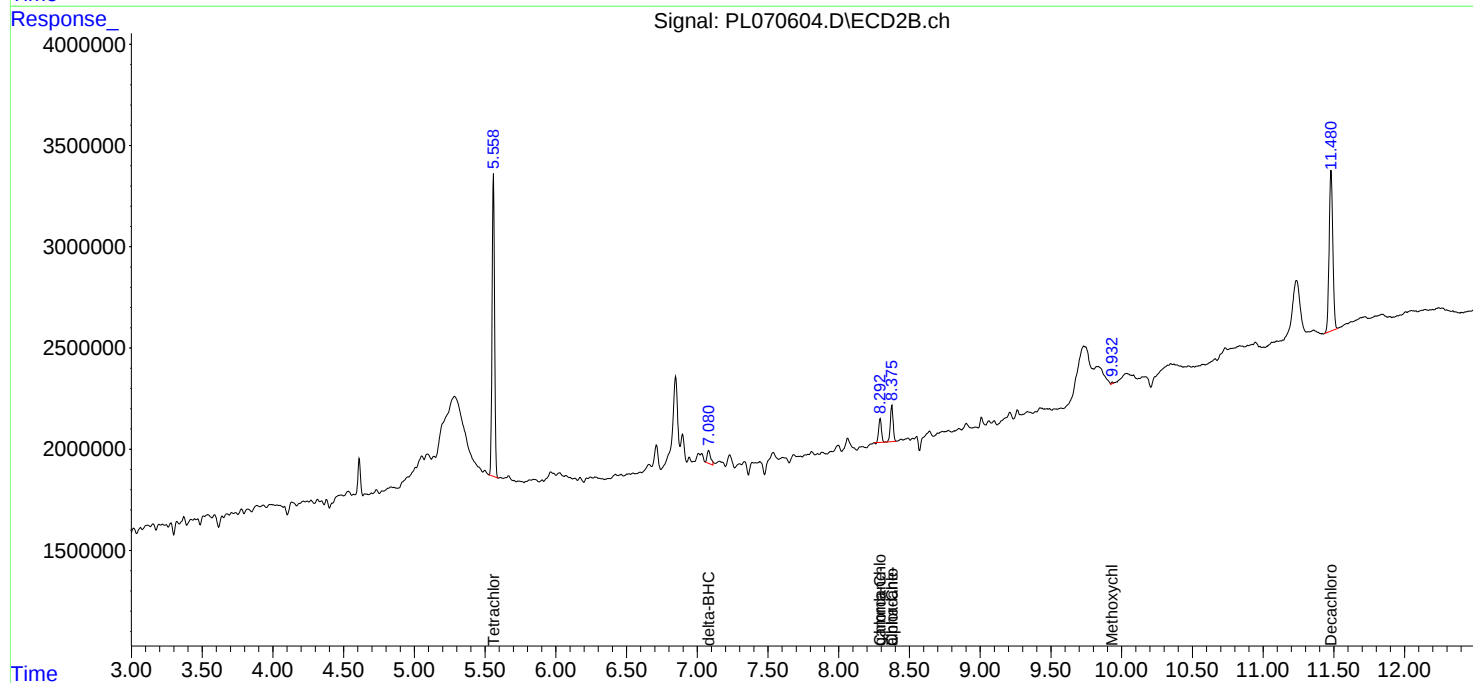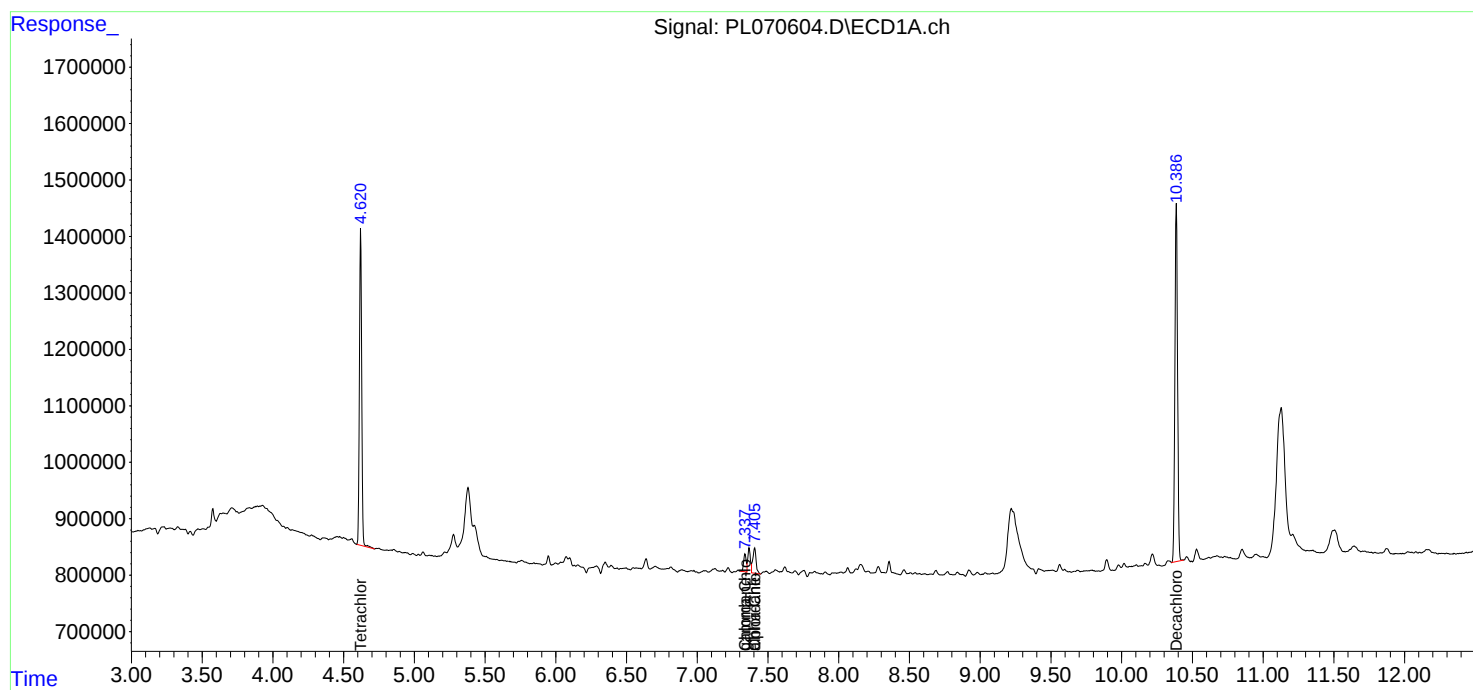

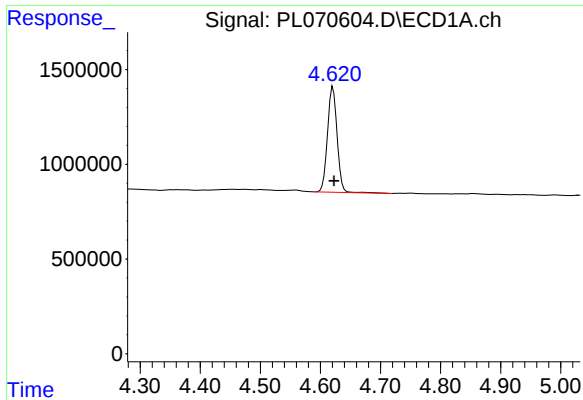


#1 Tetrachloro-m-xylene

R.T.: 4.621 min
Delta R.T.: -0.002 min
Response: 6200020
Conc: 12.31 ng/ml

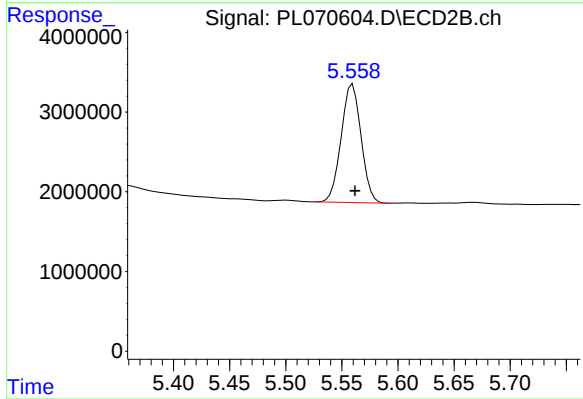


#1 Tetrachloro-m-xylene

R.T.: 5.560 min
Delta R.T.: -0.002 min
Response: 18300320
Conc: 11.96 ng/ml

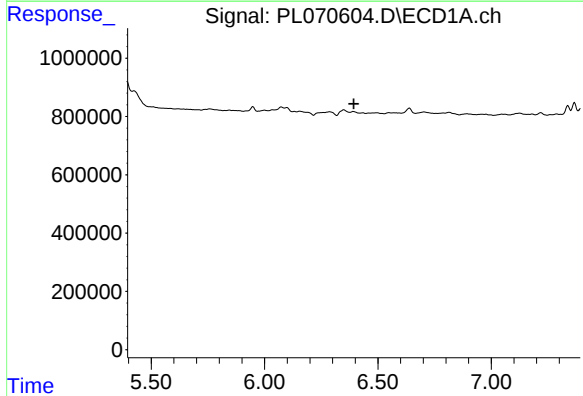


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

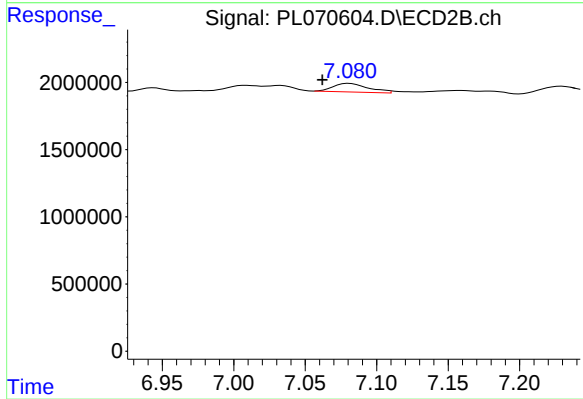


#7 delta-BHC

R.T.: 7.081 min
Delta R.T.: 0.019 min
Response: 1067965
Conc: 0.42 ng/ml

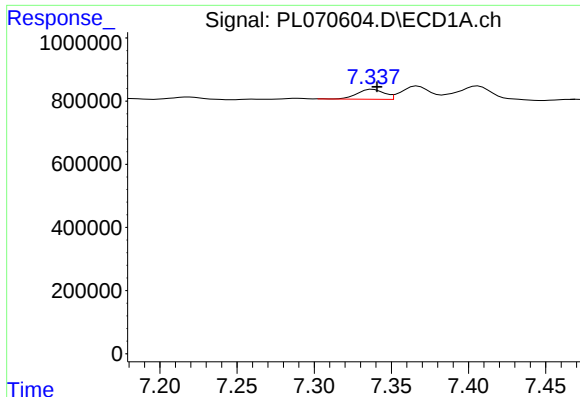


#10 gamma-Chlordane

R.T.: 7.338 min
Delta R.T.: -0.003 min
Response: 385677
Conc: 0.54 ng/ml

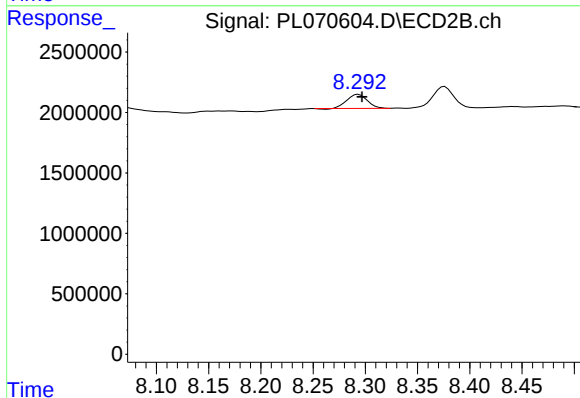


#10 gamma-Chlordane

R.T.: 8.293 min
Delta R.T.: -0.004 min
Response: 1555632
Conc: 0.78 ng/ml

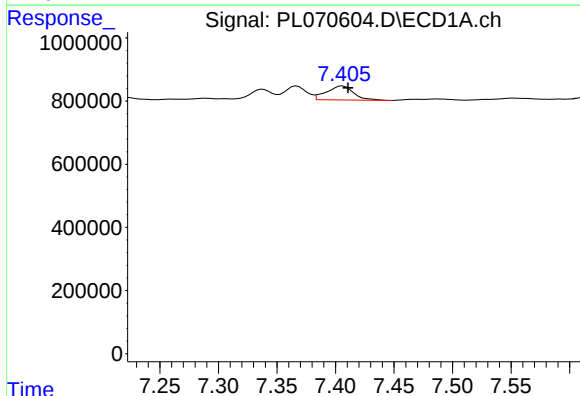


#11 alpha-Chlordane

R.T.: 7.406 min
Delta R.T.: -0.004 min
Response: 723840
Conc: 1.00 ng/ml

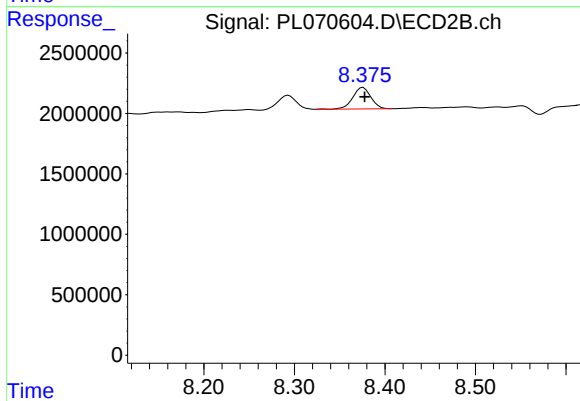


#11 alpha-Chlordane

R.T.: 8.376 min
Delta R.T.: -0.002 min
Response: 2449869
Conc: 1.25 ng/ml

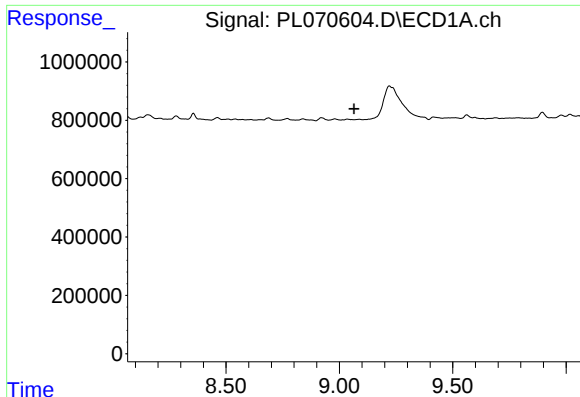


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.065 min
Response: 0
Conc: N.D.

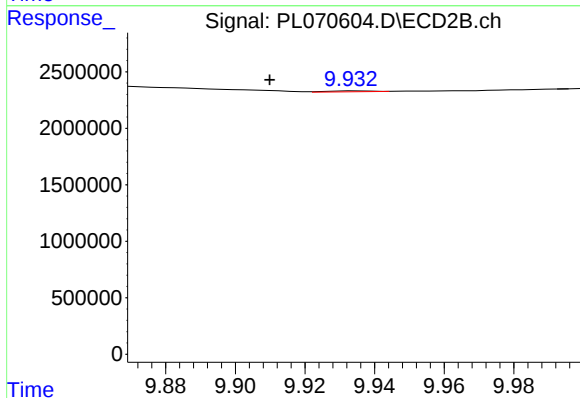


#20 Methoxychlor

R.T.: 9.935 min
Delta R.T.: 0.025 min
Response: 74155
Conc: 0.08 ng/ml

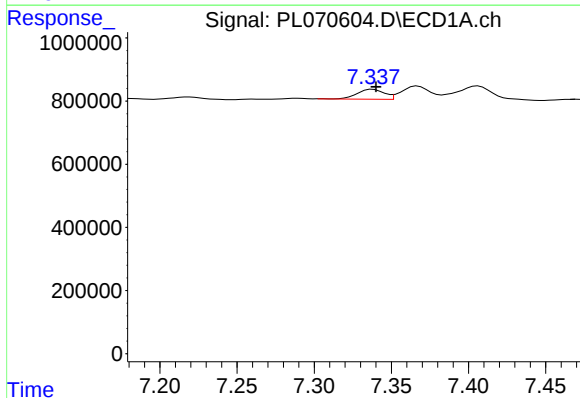


#25 Chlordane-3

R.T.: 7.338 min
Delta R.T.: -0.002 min
Response: 385677
Conc: 5.72 ng/ml

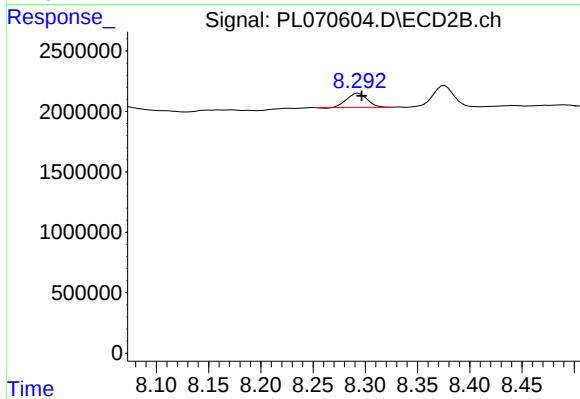


#25 Chlordane-3

R.T.: 8.293 min
Delta R.T.: -0.003 min
Response: 1555632
Conc: 5.82 ng/ml

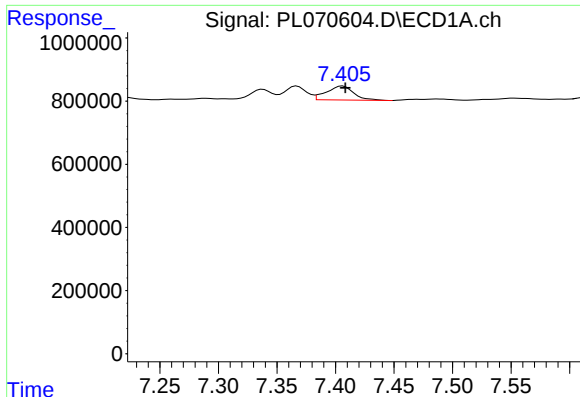


#26 Chlordane-4

R.T.: 7.406 min
Delta R.T.: -0.002 min
Response: 723840
Conc: 10.08 ng/ml

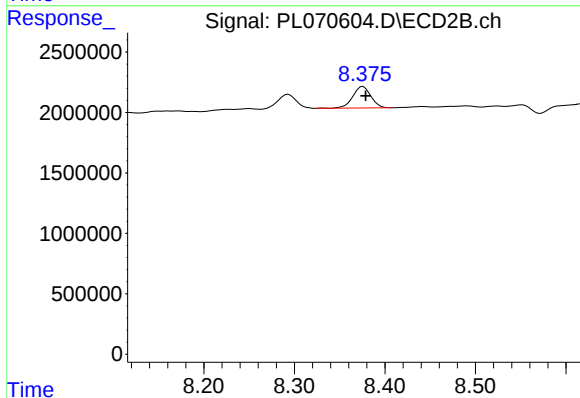


#26 Chlordane-4

R.T.: 8.376 min
Delta R.T.: -0.003 min
Response: 2449869
Conc: 7.73 ng/ml

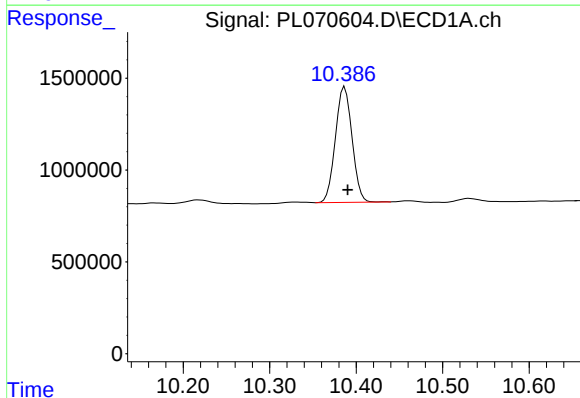

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.003 min
Response: 8379717
Conc: 11.08 ng/ml

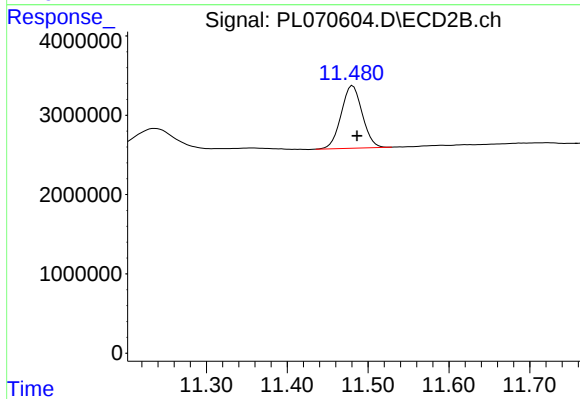

#28 Decachlorobiphenyl

R.T.: 11.481 min
Delta R.T.: -0.005 min
Response: 14273047
Conc: 9.89 ng/ml