

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070609.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 00:12
 Operator : AR\AJ
 Sample : M4372-09
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 04:15:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.622	5.561	9714285	20850246	19.289	13.623 #
28)	SA Decachlor...	10.387	11.482	10735003	21540612	14.200	14.932
Target Compounds							
2)	A alpha-BHC	5.344	6.145	-1144116	6916180	N.D.	2.960
3)	MA gamma-BHC...	0.000	6.525	0	1616102	N.D.	0.740 #
5)	MB Aldrin	0.000	7.558	0	3604132	N.D.	1.718 #
6)	B beta-BHC	0.000	6.796	0	6200778	N.D.	5.883 #
7)	B delta-BHC	0.000	7.064	0	2701007	N.D.	1.073 #
10)	B gamma-Chl...	0.000	8.292	0	1170885	N.D.	0.586 #
11)	B alpha-Chl...	7.404	0.000	469550	0	0.645	N.D. #
14)	MA Endrin	0.000	8.987f	0	327457	N.D.	0.202 #
23)	Chlordane-1	5.965f	6.957	563962	5533530	31.335	97.743 #
24)	Chlordane-2	0.000	7.558f	0	3604132	N.D.	53.589 #
25)	Chlordane-3	0.000	8.292	0	1170885	N.D.	4.381 #
26)	Chlordane-4	7.404	0.000	469550	0	6.539	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070609.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 00:12
Operator : AR\AJ
Sample : M4372-09
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 04:15:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

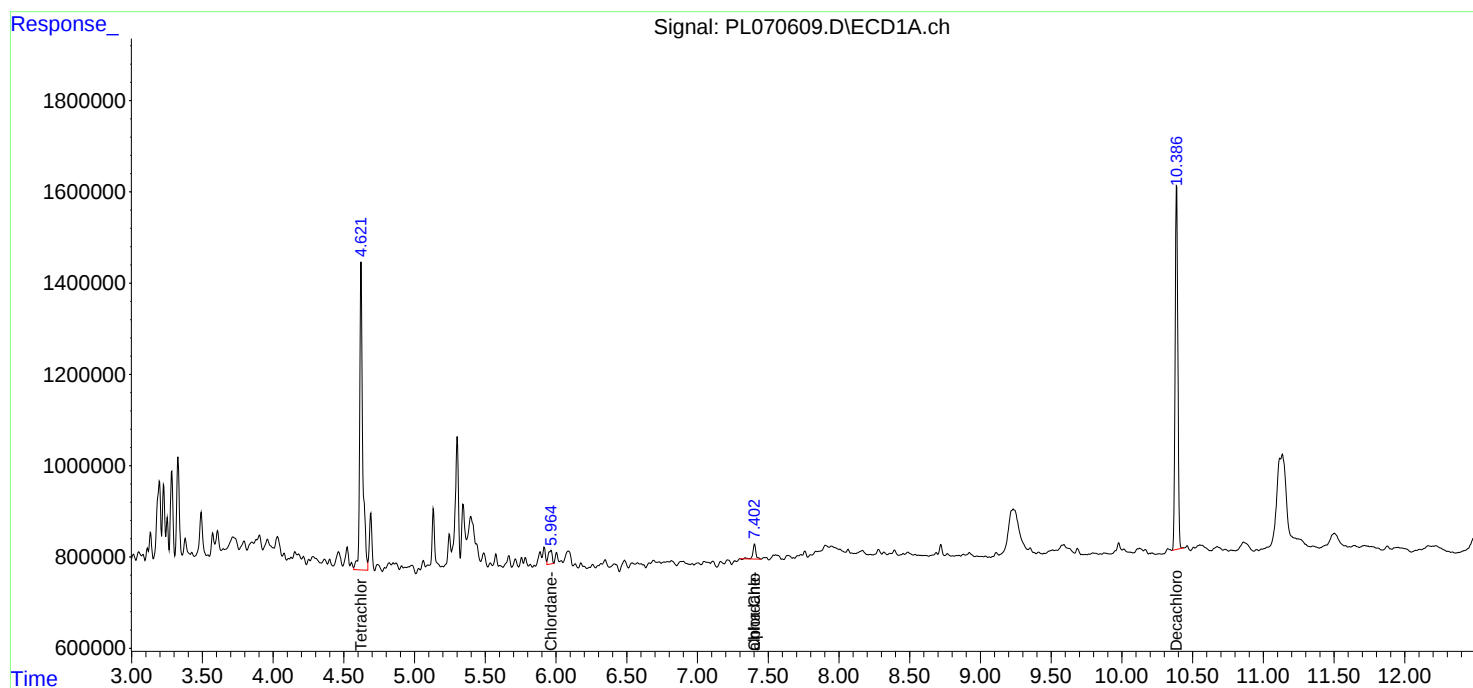

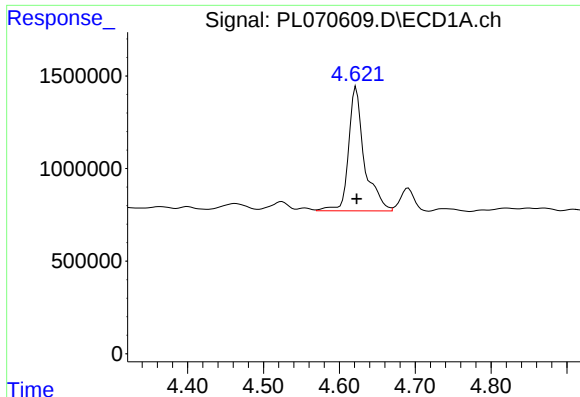


#1 Tetrachloro-m-xylene

R.T.: 4.622 min
Delta R.T.: 0.000 min
Response: 9714285
Conc: 19.29 ng/ml

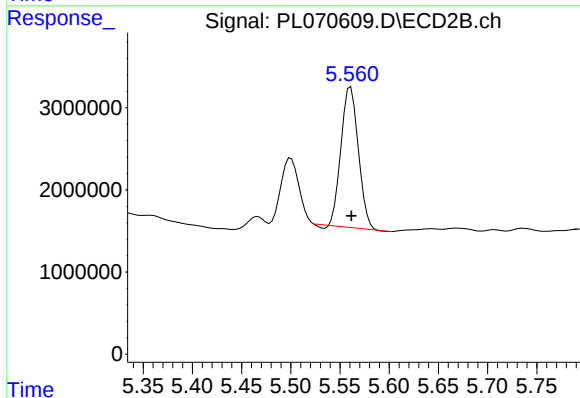


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: 0.000 min
Response: 20850246
Conc: 13.62 ng/ml

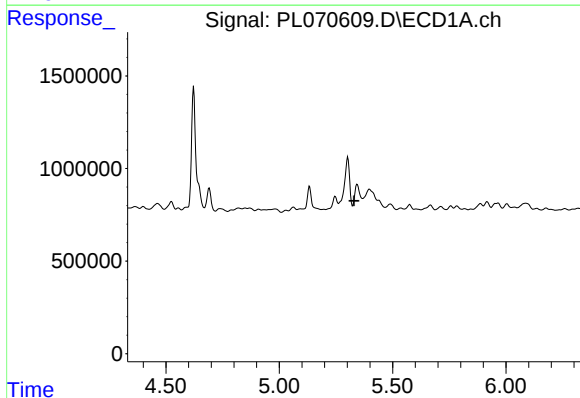


#2 alpha-BHC

R.T.: 5.344 min
Delta R.T.: 0.014 min
Response: -1144116
Conc: N.D.

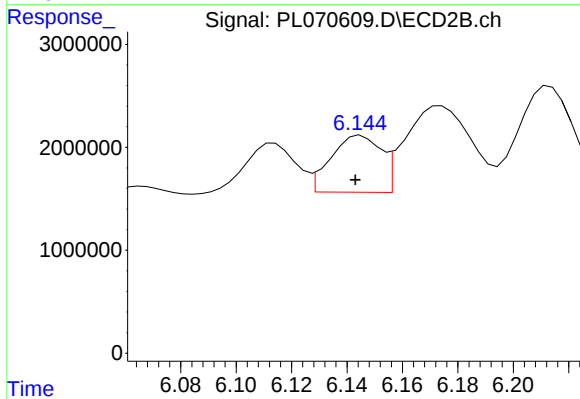


#2 alpha-BHC

R.T.: 6.145 min
Delta R.T.: 0.002 min
Response: 6916180
Conc: 2.96 ng/ml

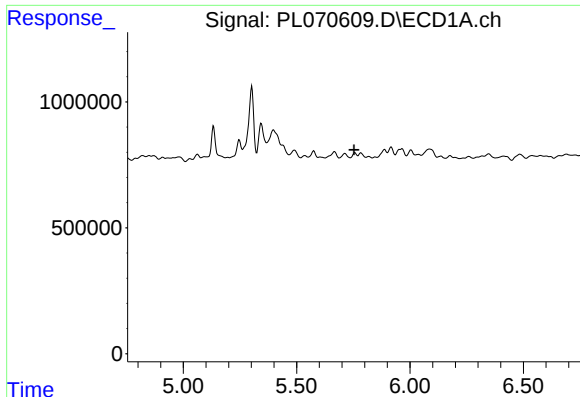


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.753 min
Response: 0
Conc: N.D.

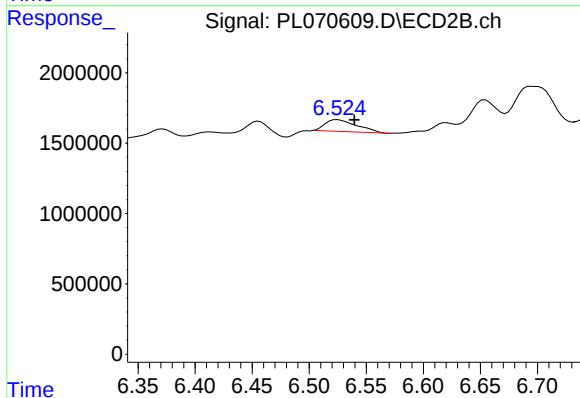


#3 gamma-BHC (Lindane)

R.T.: 6.525 min
Delta R.T.: -0.015 min
Response: 1616102
Conc: 0.74 ng/ml

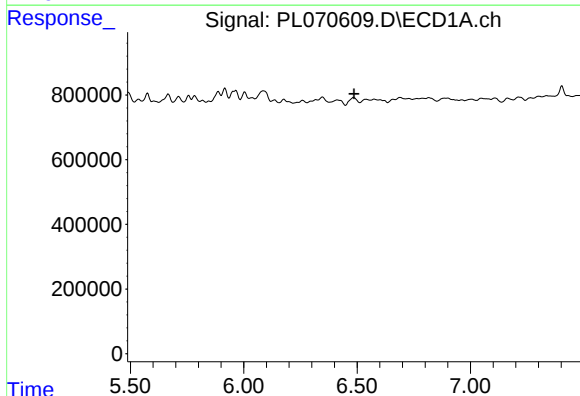


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.487 min
Response: 0
Conc: N.D.

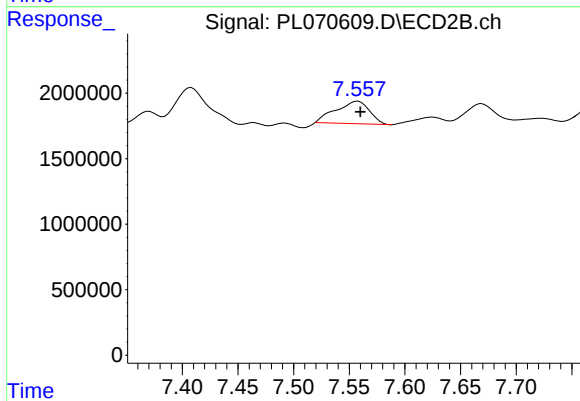


#5 Aldrin

R.T.: 7.558 min
Delta R.T.: -0.002 min
Response: 3604132
Conc: 1.72 ng/ml

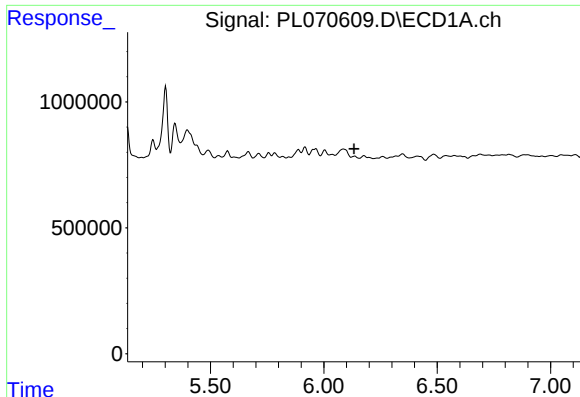


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.133 min
Response: 0
Conc: N.D.

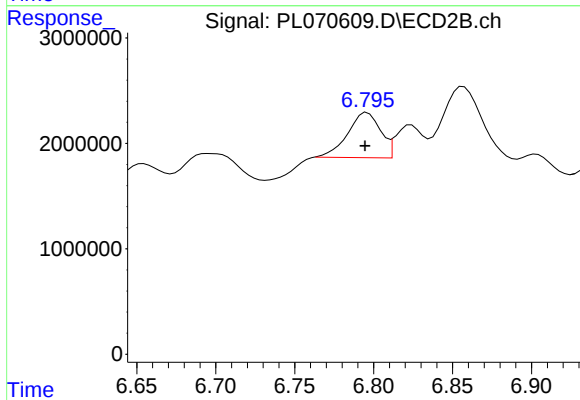


#6 beta-BHC

R.T.: 6.796 min
Delta R.T.: 0.002 min
Response: 6200778
Conc: 5.88 ng/ml

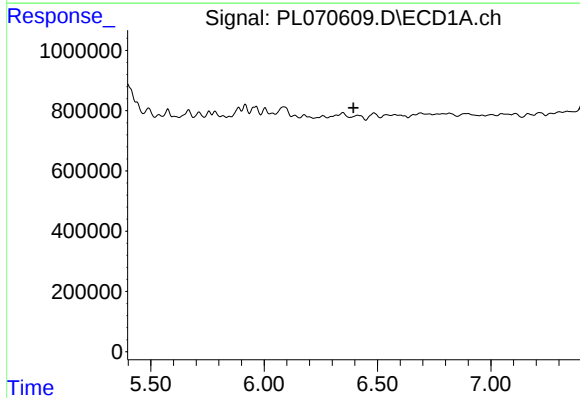


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.394 min
Response: 0
Conc: N.D.

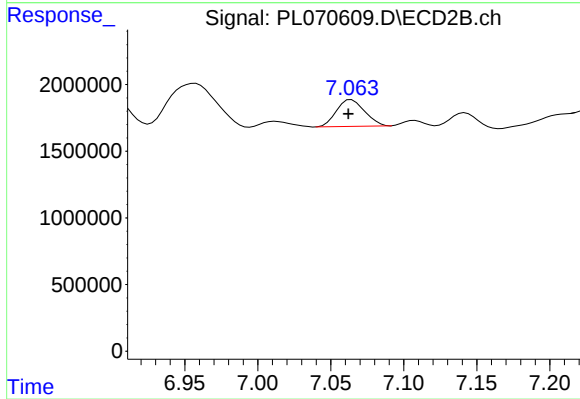


#7 delta-BHC

R.T.: 7.064 min
Delta R.T.: 0.002 min
Response: 2701007
Conc: 1.07 ng/ml

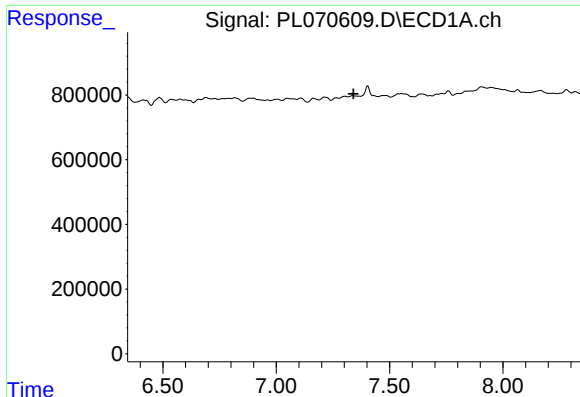


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

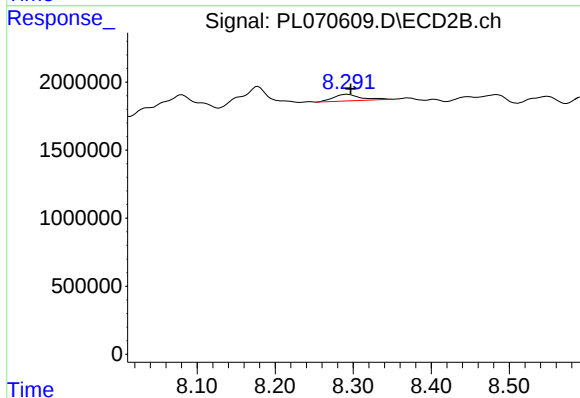


#10 gamma-Chlordane

R.T.: 8.292 min
Delta R.T.: -0.005 min
Response: 1170885
Conc: 0.59 ng/ml

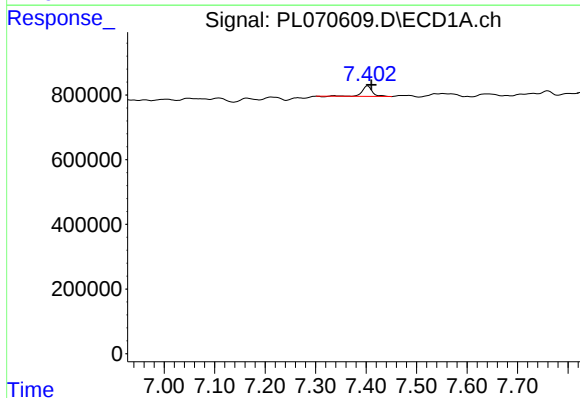


#11 alpha-Chlordane

R.T.: 7.404 min
Delta R.T.: -0.007 min
Response: 469550
Conc: 0.65 ng/ml

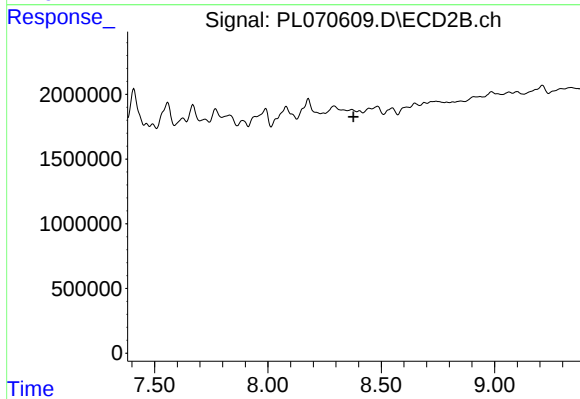


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.378 min
Response: 0
Conc: N.D.

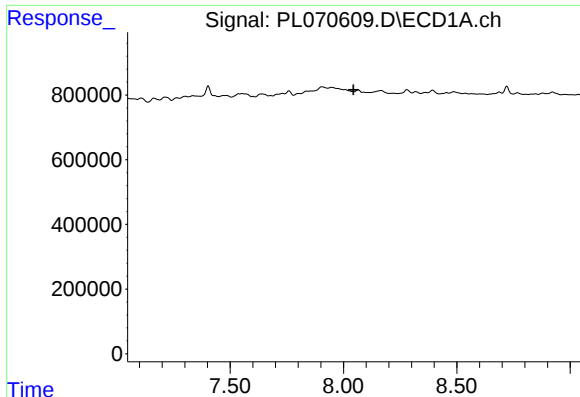


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.045 min
Response: 0
Conc: N.D.

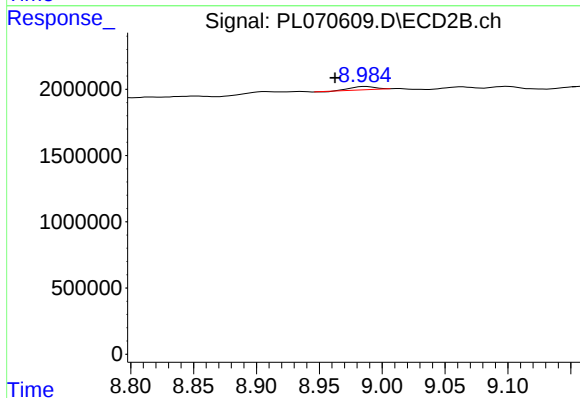


#14 Endrin

R.T.: 8.987 min
Delta R.T.: 0.024 min
Response: 327457
Conc: 0.20 ng/ml

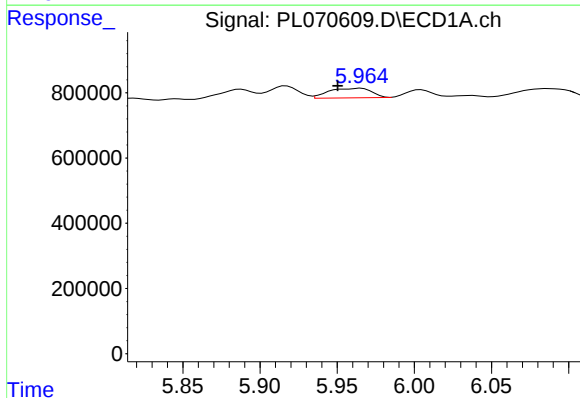


#23 Chlordane-1

R.T.: 5.965 min
Delta R.T.: 0.015 min
Response: 563962
Conc: 31.33 ng/ml

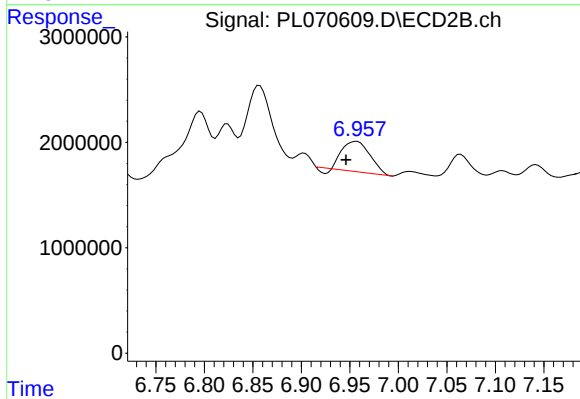


#23 Chlordane-1

R.T.: 6.957 min
Delta R.T.: 0.011 min
Response: 5533530
Conc: 97.74 ng/ml

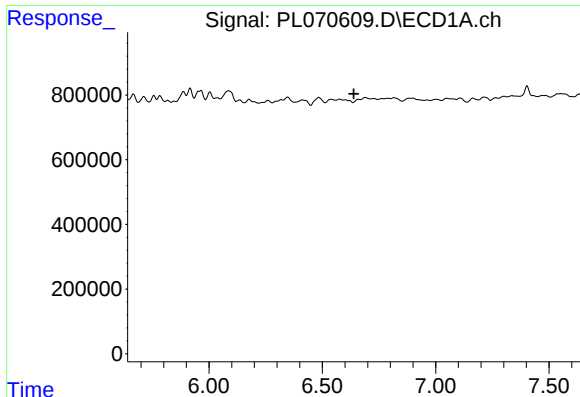


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.639 min
Response: 0
Conc: N.D.

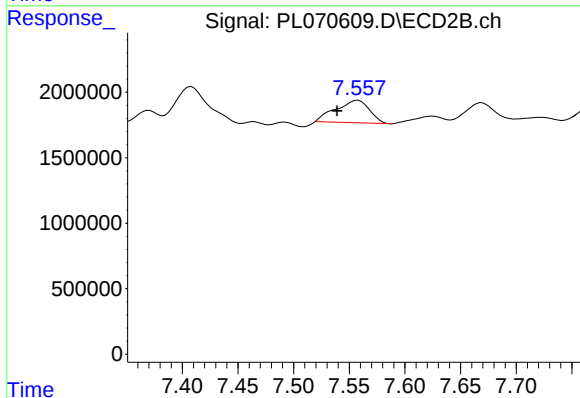


#24 Chlordane-2

R.T.: 7.558 min
Delta R.T.: 0.019 min
Response: 3604132
Conc: 53.59 ng/ml

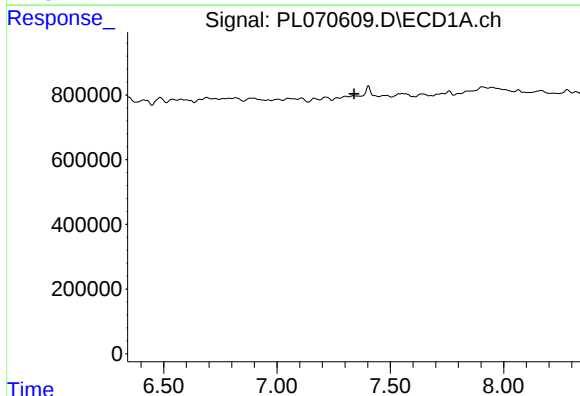


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.340 min
Response: 0
Conc: N.D.

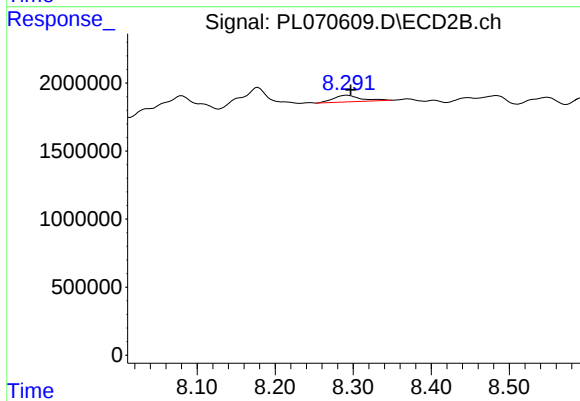


#25 Chlordane-3

R.T.: 8.292 min
Delta R.T.: -0.004 min
Response: 1170885
Conc: 4.38 ng/ml

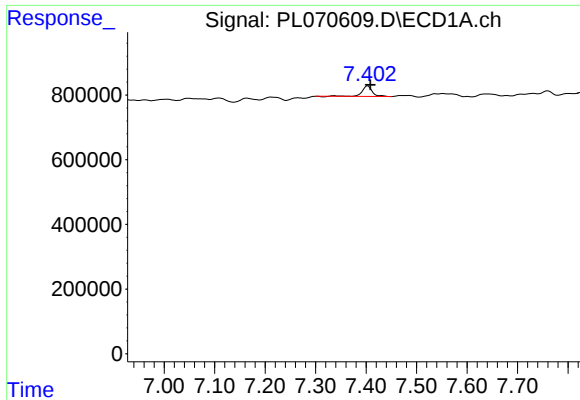


#26 Chlordane-4

R.T.: 7.404 min
Delta R.T.: -0.005 min
Response: 469550
Conc: 6.54 ng/ml

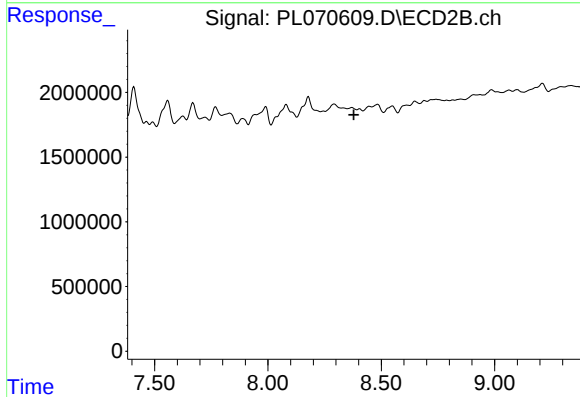


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.379 min
Response: 0
Conc: N.D.

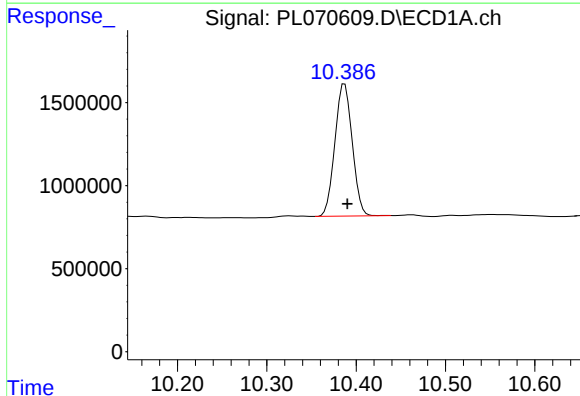

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.003 min
Response: 10735003
Conc: 14.20 ng/ml

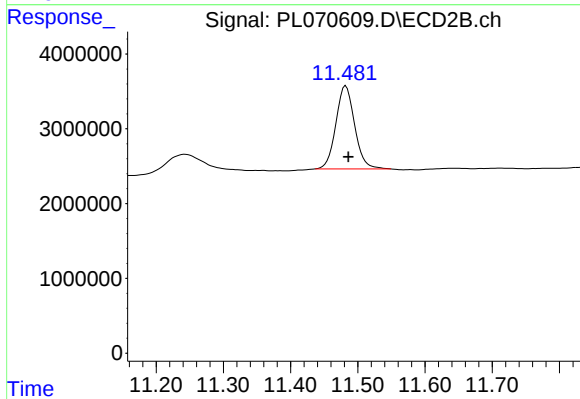

#28 Decachlorobiphenyl

R.T.: 11.482 min
Delta R.T.: -0.004 min
Response: 21540612
Conc: 14.93 ng/ml