

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 05:35
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 06:05:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 05:57:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.622	5.561	13184991	37921100	24.462	23.887
28)	SA Decachlor...	10.389	11.486	19358000	36516784	26.018	24.748
Target Compounds							
23)	Chlordane-1	5.950	6.946	4374870	13848148	240.117	233.279
24)	Chlordane-2	6.639	7.538	6225499	16546913	254.112	241.272
25)	Chlordane-3	7.340	8.297	16305931	64338431	237.722	233.360
26)	Chlordane-4	7.408	8.379	17541928	77143099	239.282	235.011
27)	Chlordane-5	8.359	9.267	6233733	13580739	237.401	233.478


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 05:35
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 06:05:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 05:57:40 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

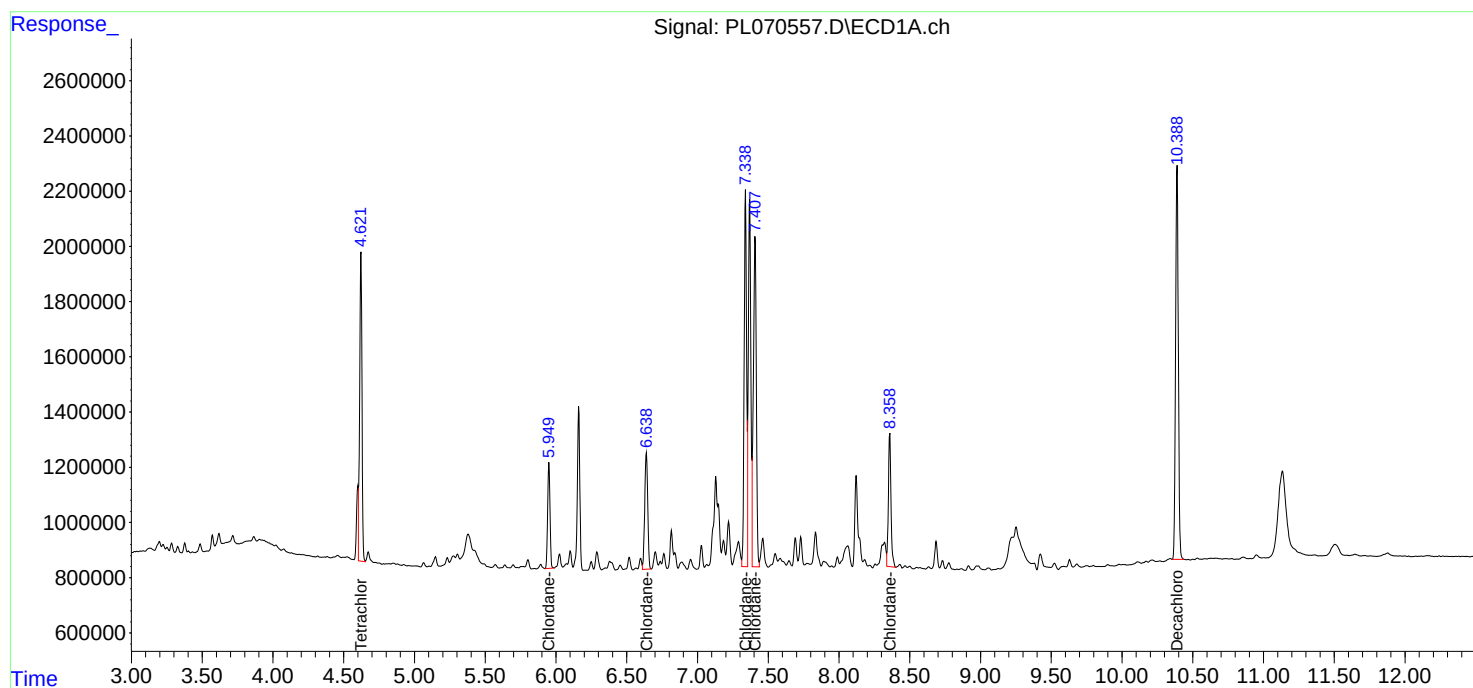


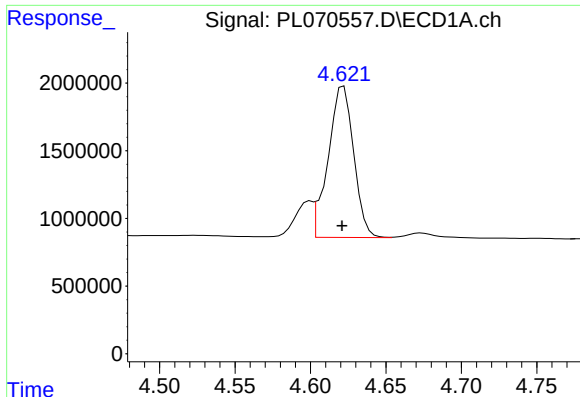

#1 Tetrachloro-m-xylene


R.T.: 4.622 min
Delta R.T.: 0.000 min
Response: 13184991
Conc: 24.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

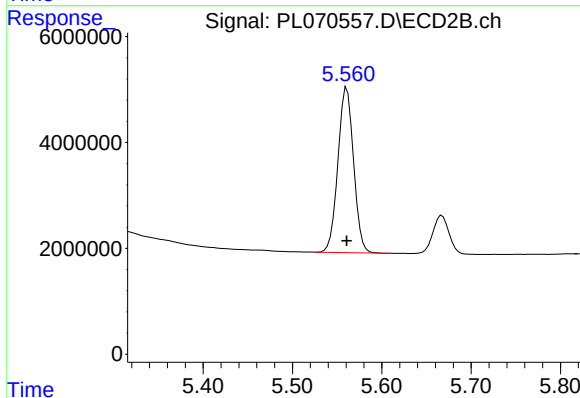


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: 0.000 min
Response: 37921100
Conc: 23.89 ng/ml

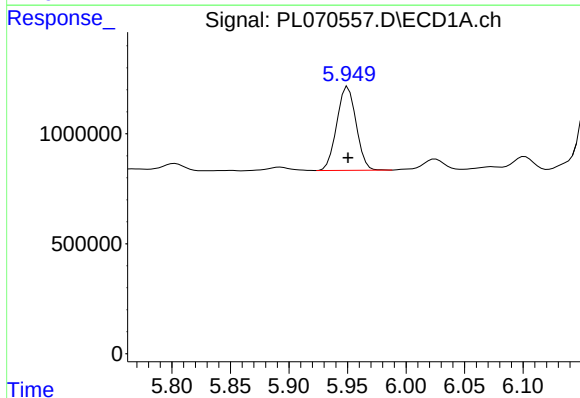


#23 Chlordane-1

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 4374870
Conc: 240.12 ng/ml

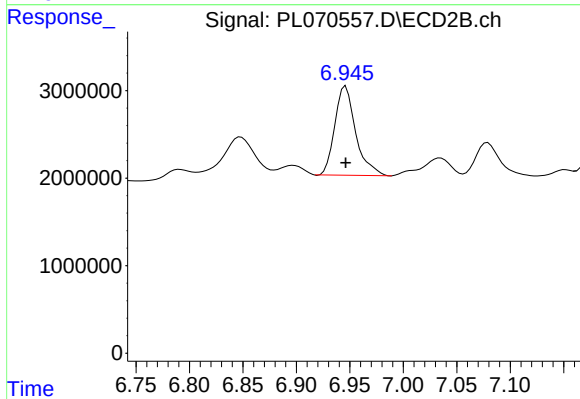

#23 Chlordane-1


R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 13848148
Conc: 233.28 ng/ml

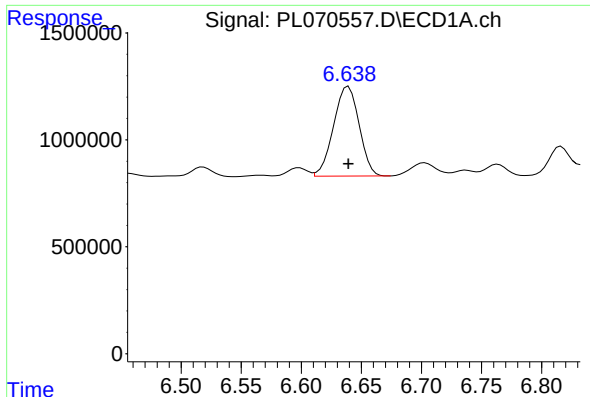

#24 Chlordane-2


R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 6225499
Conc: 254.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

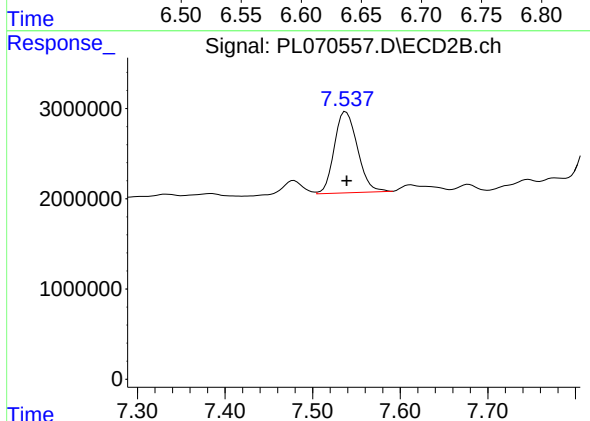


#24 Chlordane-2

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 16546913
Conc: 241.27 ng/ml

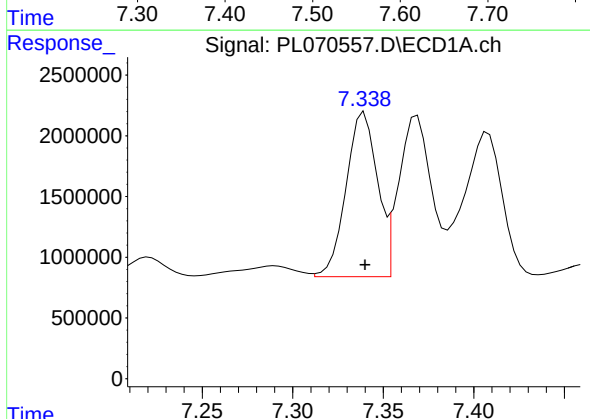


#25 Chlordane-3

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 16305931
Conc: 237.72 ng/ml

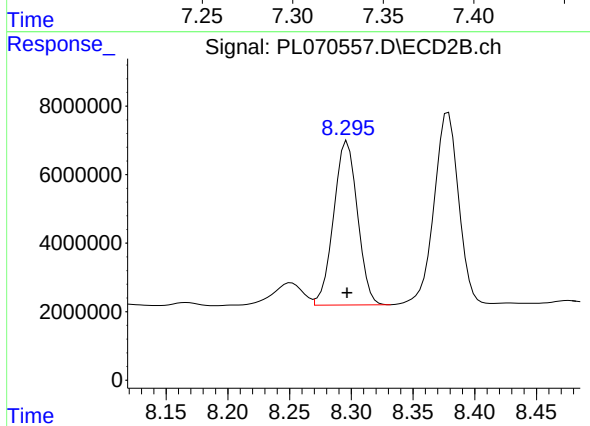

#25 Chlordane-3


R.T.: 8.297 min
Delta R.T.: 0.000 min
Response: 64338431
Conc: 233.36 ng/ml

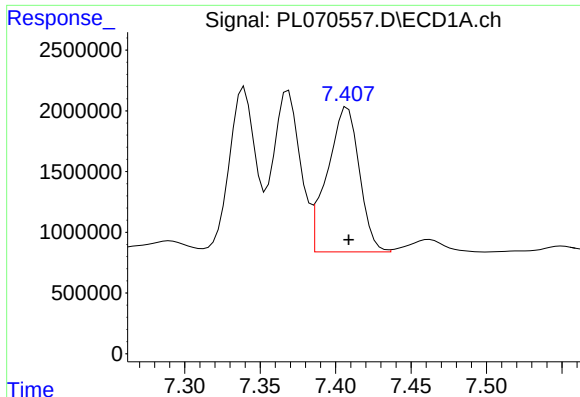

#26 Chlordane-4


R.T.: 7.408 min
Delta R.T.: 0.000 min
Response: 17541928
Conc: 239.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

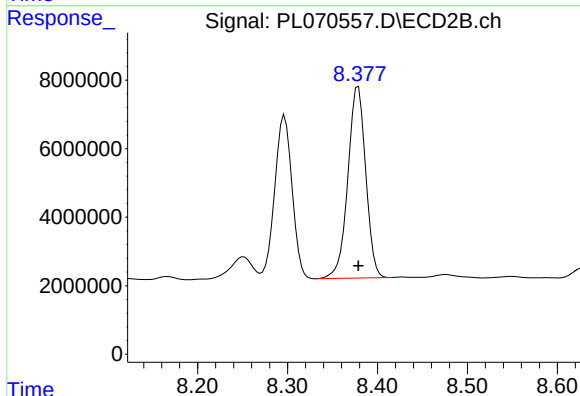


#26 Chlordane-4

R.T.: 8.379 min
Delta R.T.: 0.000 min
Response: 77143099
Conc: 235.01 ng/ml

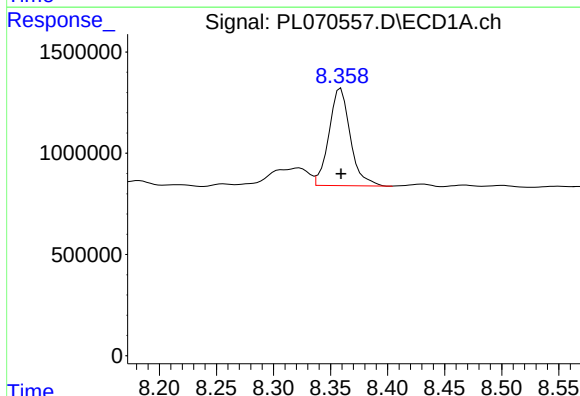


#27 Chlordane-5

R.T.: 8.359 min
Delta R.T.: 0.000 min
Response: 6233733
Conc: 237.40 ng/ml

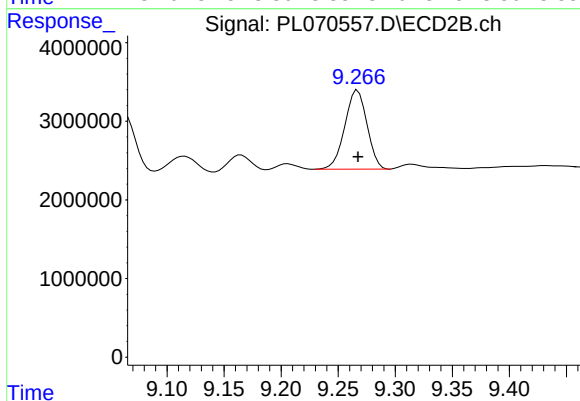

#27 Chlordane-5


R.T.: 9.267 min
Delta R.T.: 0.000 min
Response: 13580739
Conc: 233.48 ng/ml

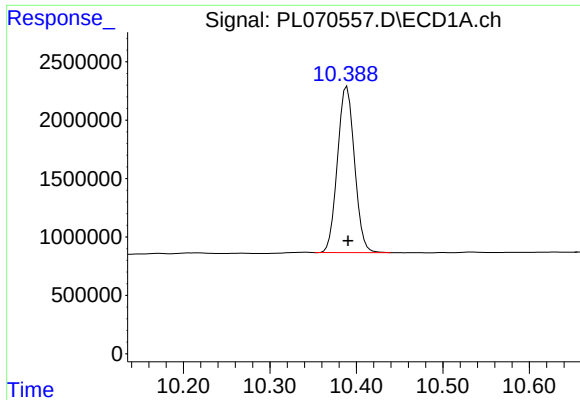

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.001 min
Response: 19358000
Conc: 26.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

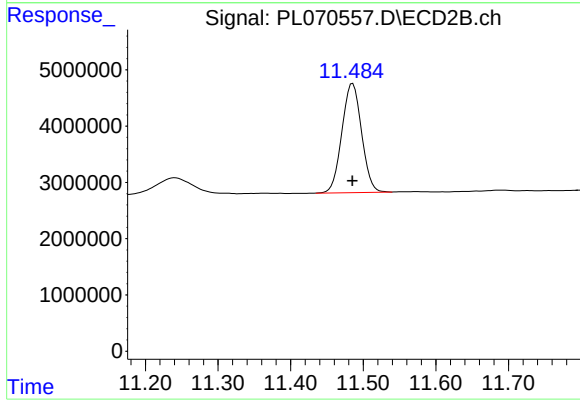

#28 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: 0.000 min
Response: 36516784
Conc: 24.75 ng/ml