

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 12:24
 Operator : AR\AJ
 Sample : M4343-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 METRO-SP

Manual Integrations
 APPROVED

mohammad
 10/28/2021 11:47:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 17:02:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.622	5.562	7209767	16632965	14.316m	10.868m
28) SA Decachlor...	10.393	11.490	9140741	16106679	12.091	11.165
Target Compounds						
11) B alpha-Chl...	7.410	8.381	6062708	15321720	8.334m	7.825
17) MA 4,4'-DDT	8.467	9.426	1676292	1172218	2.625m	0.678 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 12:24
Operator : AR\AJ
Sample : M4343-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
METRO-SP


Manual Integrations
APPROVED

mohammad
10/28/2021 11:47:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 17:02:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

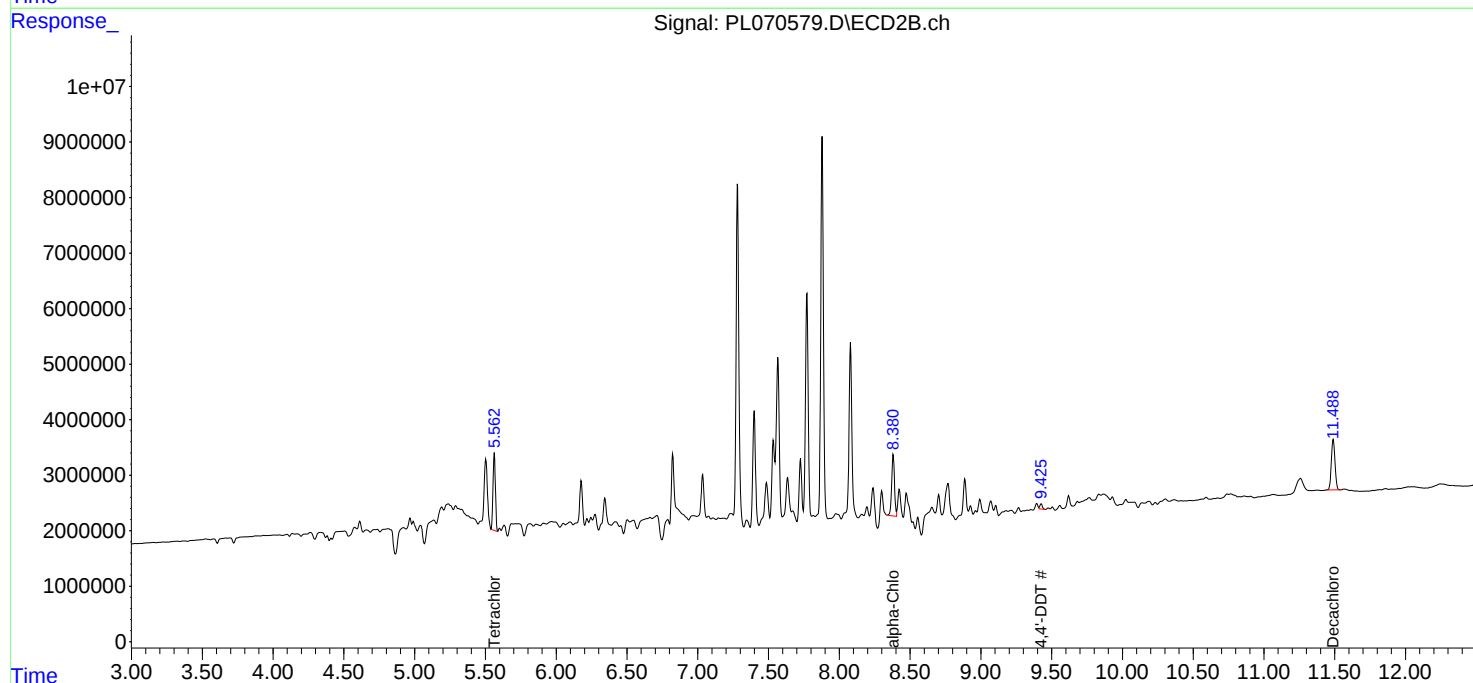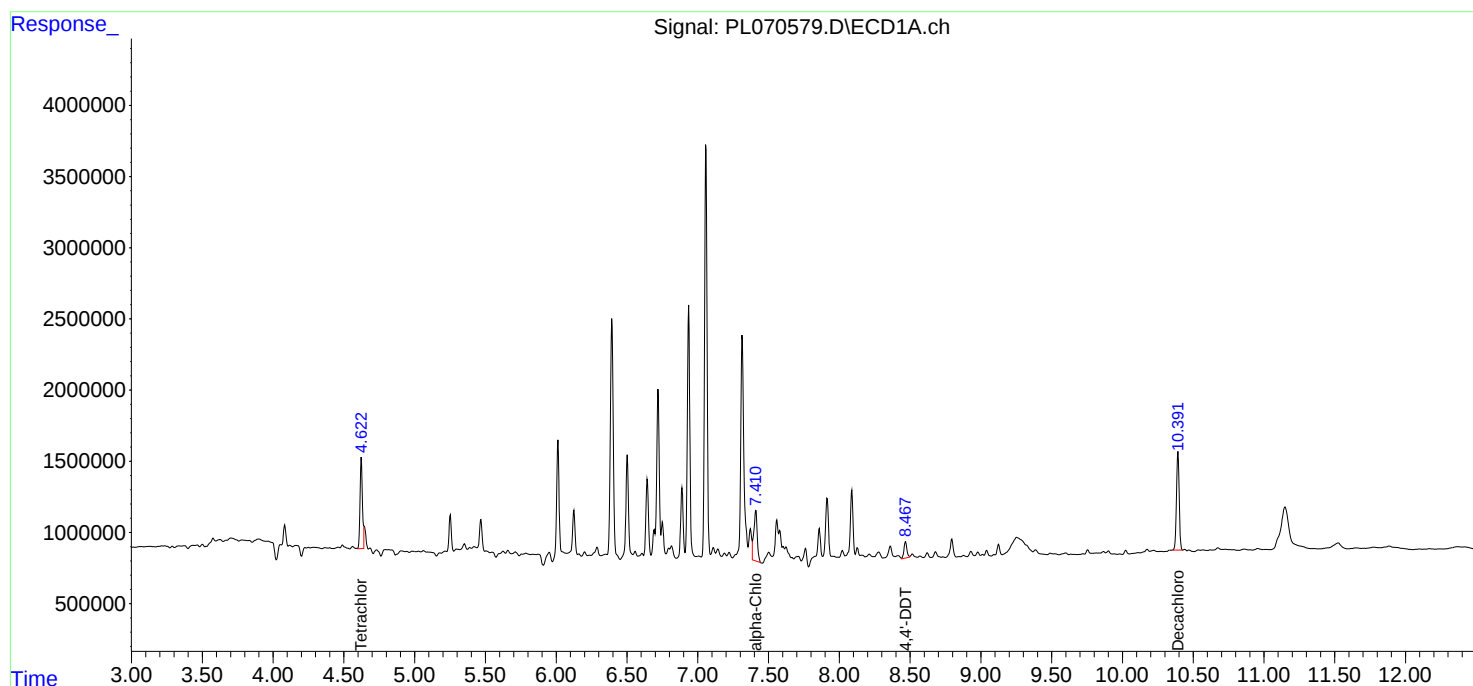

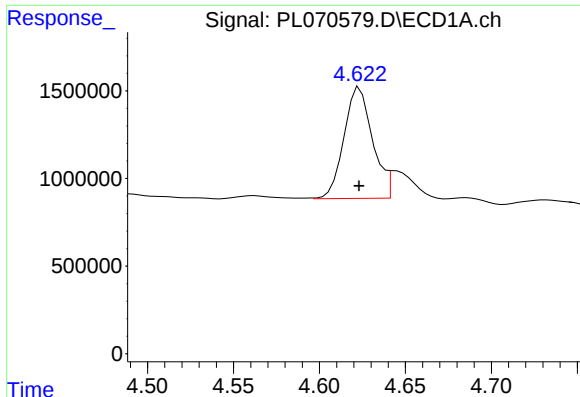


#1 Tetrachloro-m-xylene

R.T.: 4.622 min
Delta R.T.: 0.000 min
Response: 7209767
Conc: 14.32 ng/ml m

Instrument :
ECD_L
ClientSampleId :
METRO-SP


Manual Integrations
APPROVED

mohammad
10/28/2021 11:47:32 AM

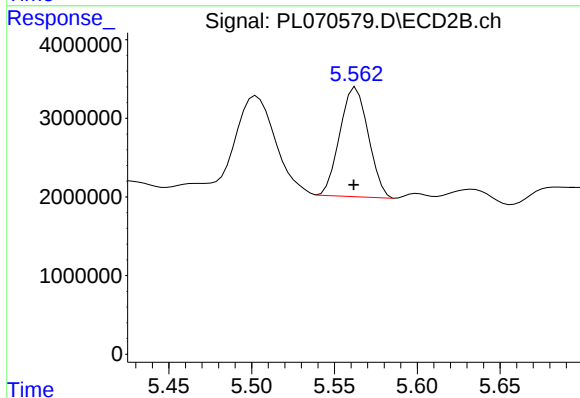


#1 Tetrachloro-m-xylene

R.T.: 5.562 min
Delta R.T.: 0.000 min
Response: 16632965
Conc: 10.87 ng/ml m

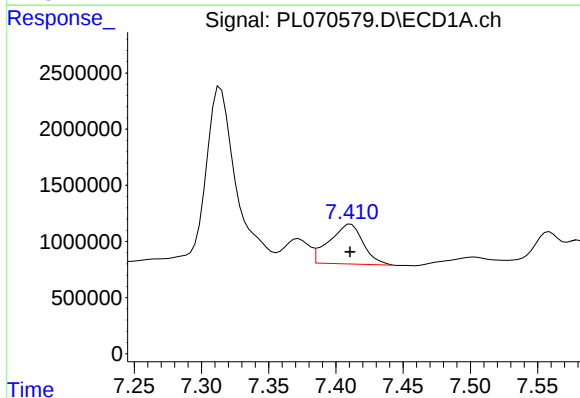


#11 alpha-Chlordane

R.T.: 7.410 min
Delta R.T.: 0.000 min
Response: 6062708
Conc: 8.33 ng/ml m

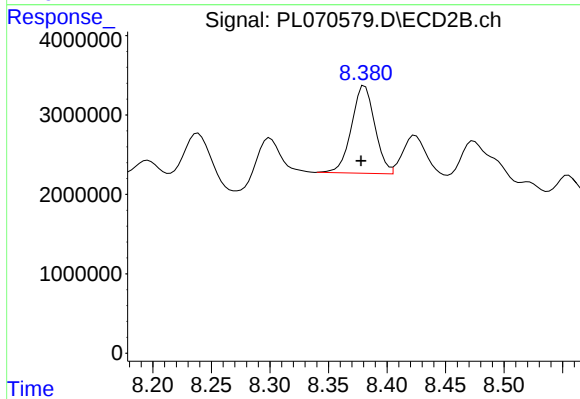

#11 alpha-Chlordane

R.T.: 8.381 min
Delta R.T.: 0.003 min
Response: 15321720
Conc: 7.83 ng/ml

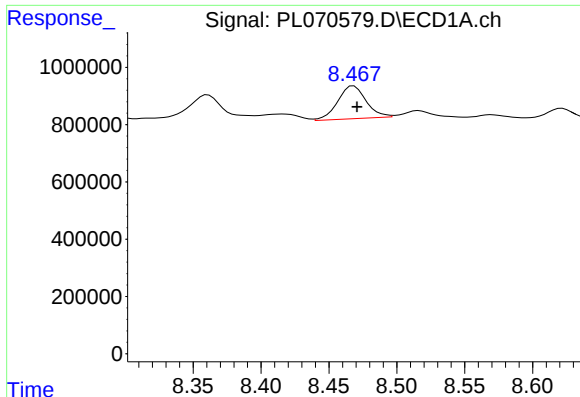


#17 4,4'-DDT

R.T.: 8.467 min
Delta R.T.: -0.004 min
Response: 1676292
Conc: 2.62 ng/ml m

Instrument :
ECD_L
ClientSampleId :
METRO-SP


Manual Integrations
APPROVED

mohammad
10/28/2021 11:47:32 AM

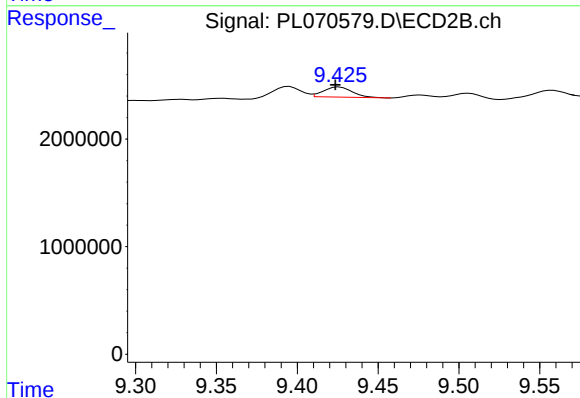


#17 4,4'-DDT

R.T.: 9.426 min
Delta R.T.: 0.002 min
Response: 1172218
Conc: 0.68 ng/ml

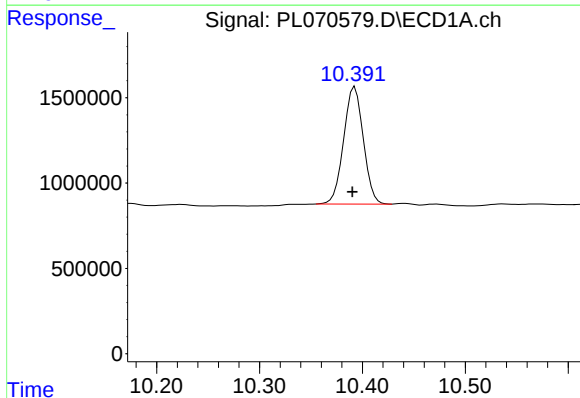

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.002 min
Response: 9140741
Conc: 12.09 ng/ml

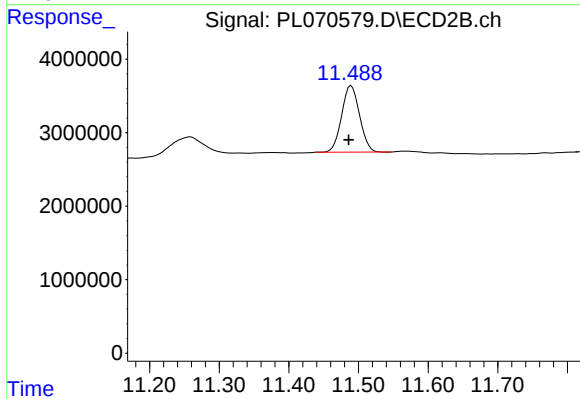

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: 0.004 min
Response: 16106679
Conc: 11.16 ng/ml