

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 13:30
 Operator : AR\AJ
 Sample : M4348-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 287

Manual Integrations
 APPROVED

mohammad
 10/28/2021 11:47:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 17:05:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.622	5.560	7268061	21777731	14.432	14.229
28) SA Decachlor...	10.388	11.483	6514500	11242383	8.617	7.793
Target Compounds						
10) B gamma-Chl...	7.340	8.294	1350798	5367553	1.885	2.688m#
11) B alpha-Chl...	7.408	8.378	2418916	9912037	3.325	5.062 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 13:30
Operator : AR\AJ
Sample : M4348-08
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
287


Manual Integrations
APPROVED

mohammad
10/28/2021 11:47:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 17:05:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

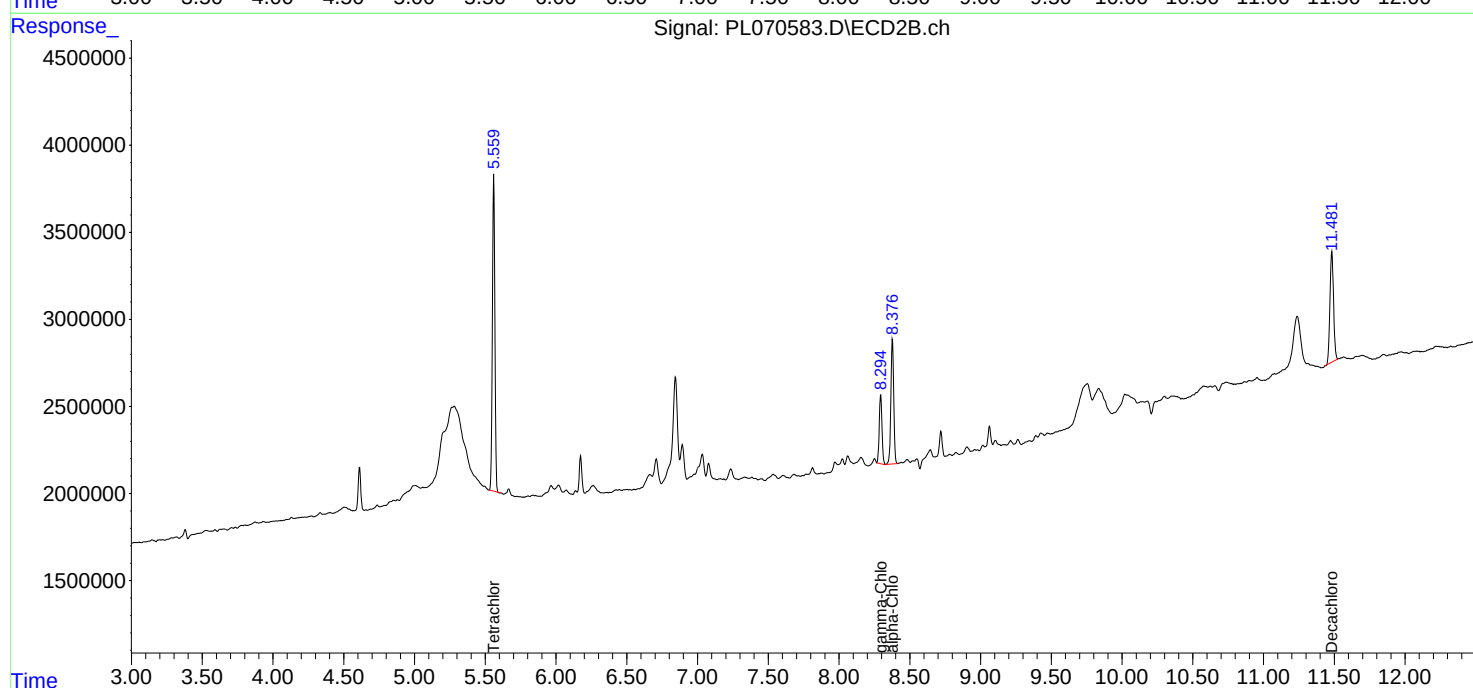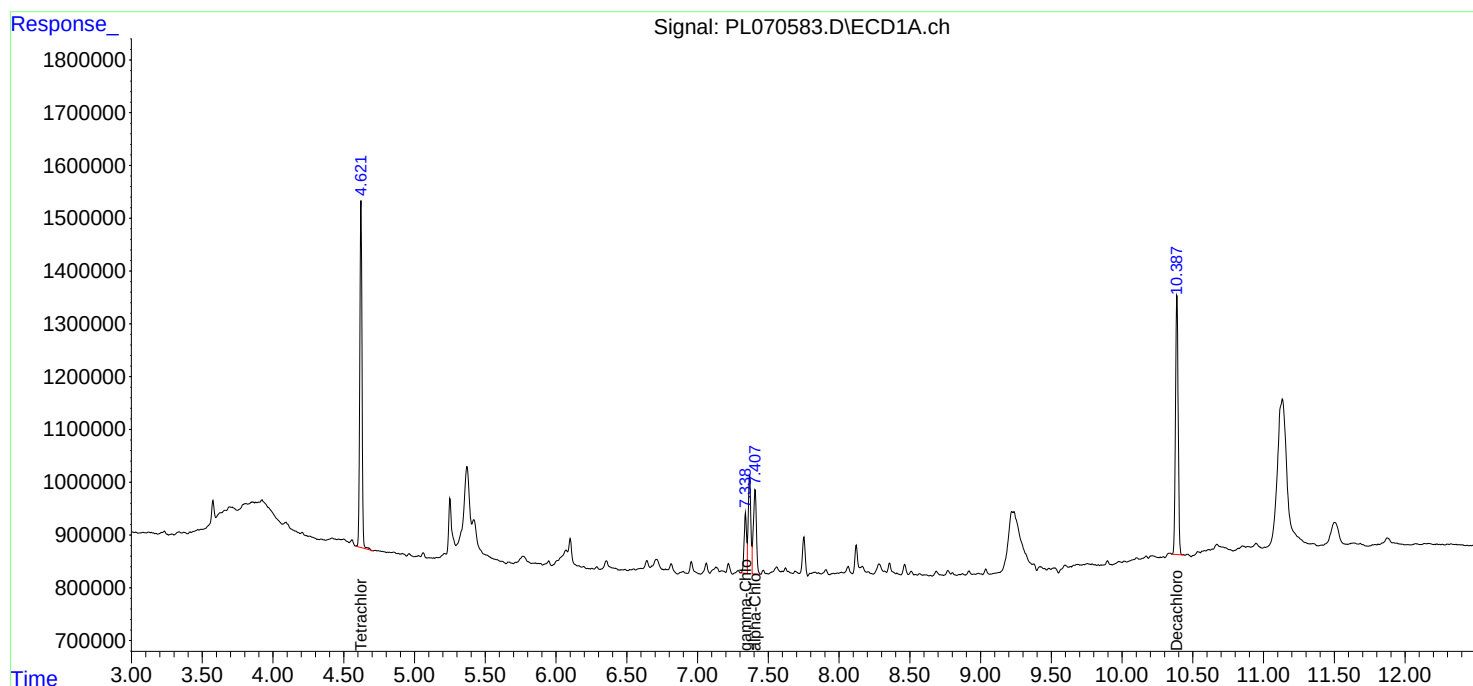

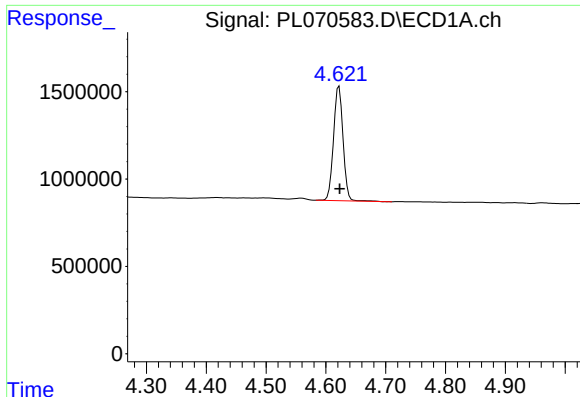


#1 Tetrachloro-m-xylene

R.T.: 4.622 min
Delta R.T.: -0.001 min
Response: 7268061
Conc: 14.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
287


Manual Integrations
APPROVED

mohammad
10/28/2021 11:47:40 AM

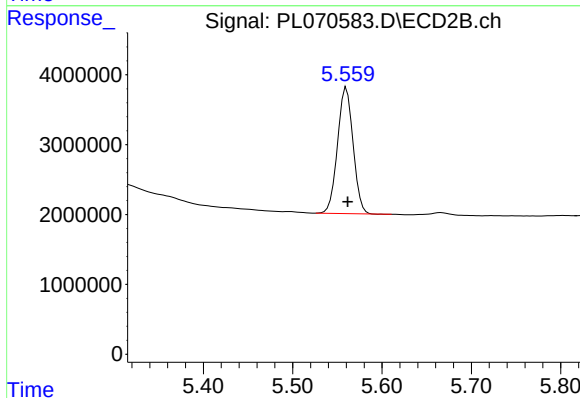


#1 Tetrachloro-m-xylene

R.T.: 5.560 min
Delta R.T.: -0.002 min
Response: 21777731
Conc: 14.23 ng/ml

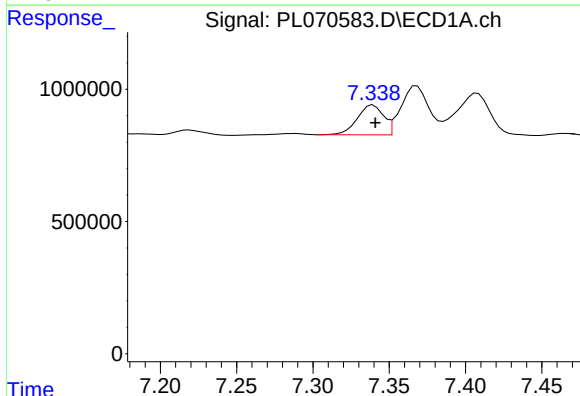


#10 gamma-Chlordane

R.T.: 7.340 min
Delta R.T.: -0.001 min
Response: 1350798
Conc: 1.89 ng/ml

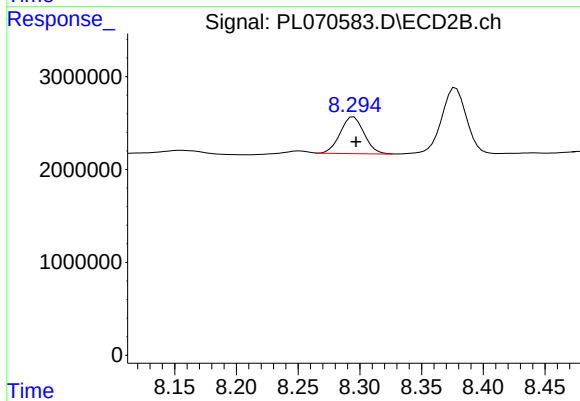

#10 gamma-Chlordane

R.T.: 8.294 min
Delta R.T.: -0.003 min
Response: 5367553
Conc: 2.69 ng/ml m

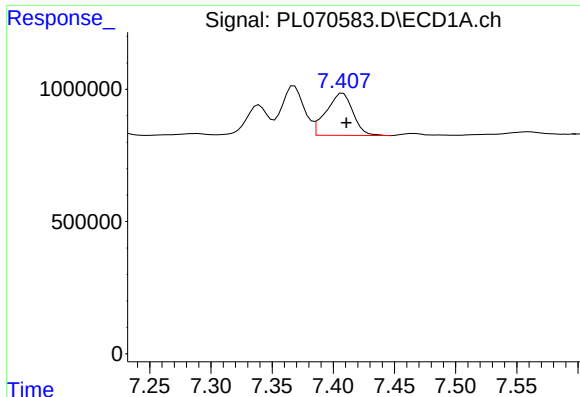


#11 alpha-Chlordane

R.T.: 7.408 min
Delta R.T.: -0.003 min
Response: 2418916
Conc: 3.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
287


Manual Integrations
APPROVED

mohammad
10/28/2021 11:47:40 AM

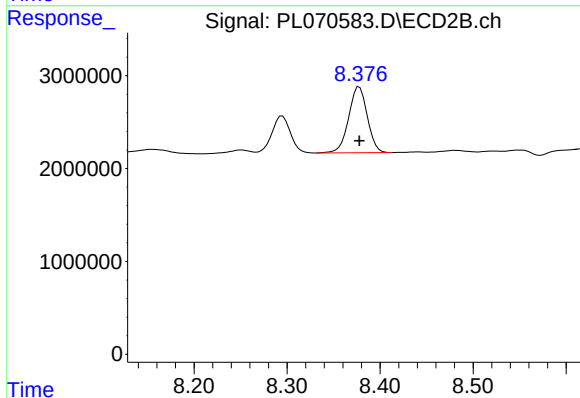


#11 alpha-Chlordane

R.T.: 8.378 min
Delta R.T.: 0.000 min
Response: 9912037
Conc: 5.06 ng/ml

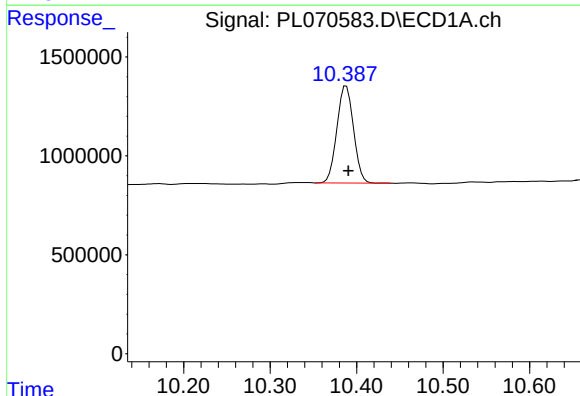

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.002 min
Response: 6514500
Conc: 8.62 ng/ml

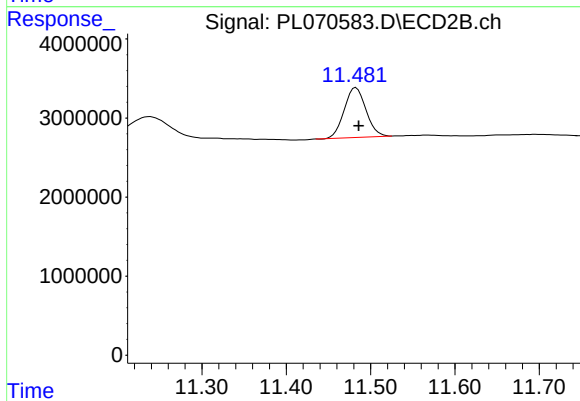

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.003 min
Response: 11242383
Conc: 7.79 ng/ml