

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 17:32
 Operator : AR\AJ
 Sample : M4356-01DL 2X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-282DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 04:13:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.622	5.560	3382664	9935342	6.717	6.492
28)	SA Decachlor...	10.389	11.483	5840796	8551871	7.726	5.928
Target Compounds							
10)	B gamma-Chl...	7.340	8.295	22241022	70595451	31.037	35.360
11)	B alpha-Chl...	7.409	8.377	47691413	154.3E6	65.560	78.781
17)	MA 4,4'-DDT	8.467	9.420	2196975	3205357	3.440	1.855 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 17:32
Operator : AR\AJ
Sample : M4356-01DL 2X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
ETGI-282DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 04:13:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

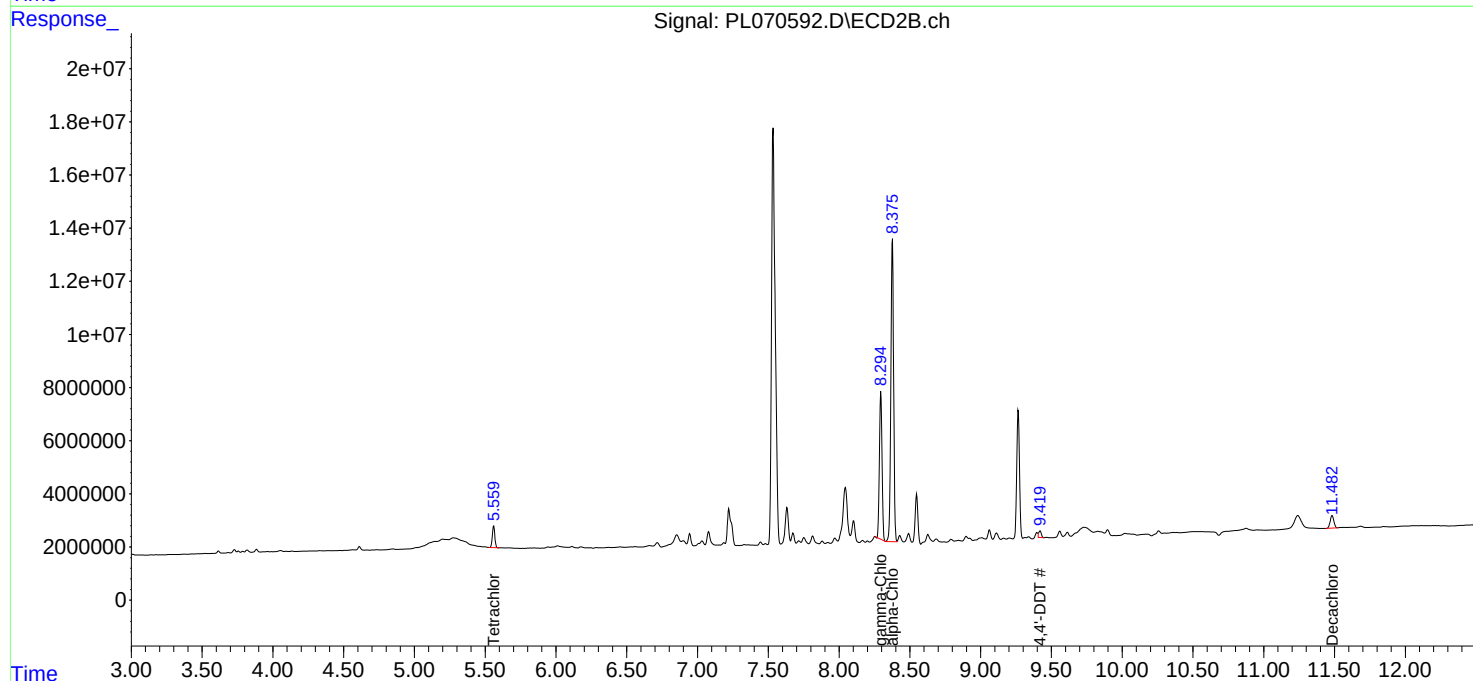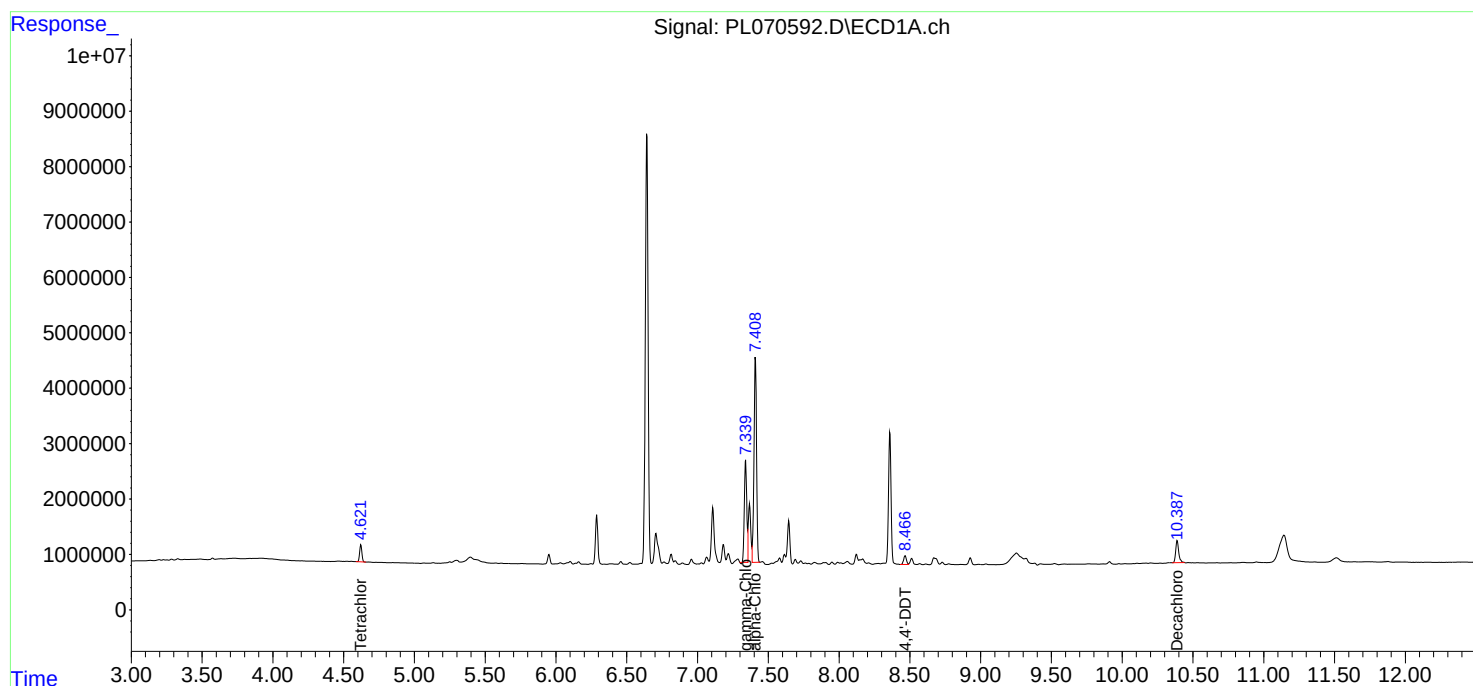


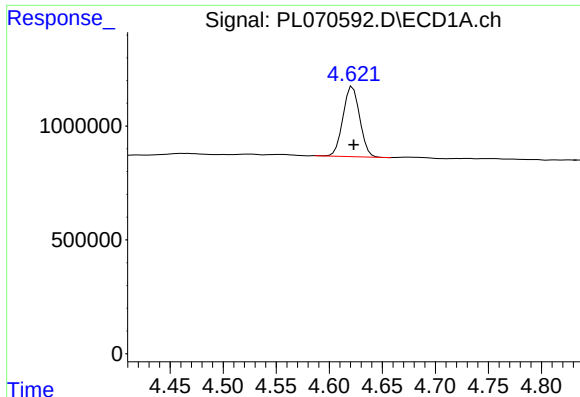

#1 Tetrachloro-m-xylene


R.T.: 4.622 min
Delta R.T.: 0.000 min
Response: 3382664
Conc: 6.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-282DL

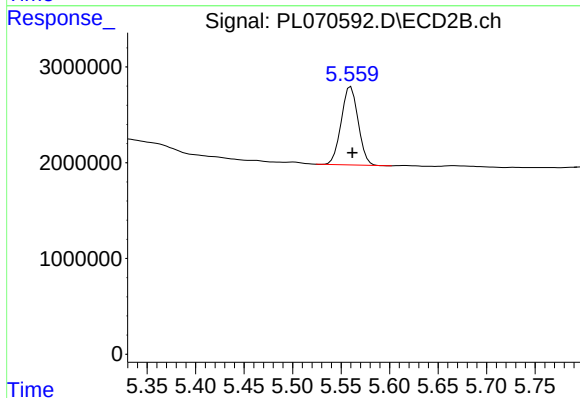


#1 Tetrachloro-m-xylene

R.T.: 5.560 min
Delta R.T.: -0.002 min
Response: 9935342
Conc: 6.49 ng/ml

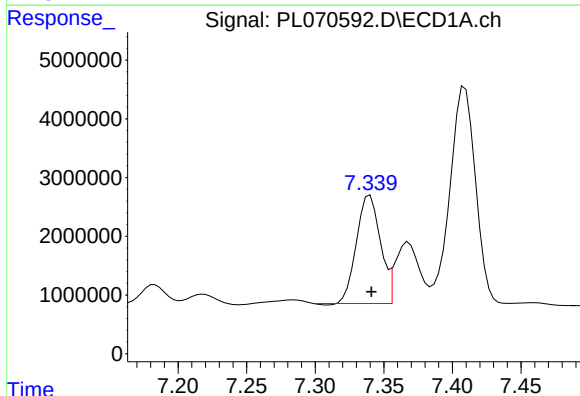


#10 gamma-Chlordane

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 22241022
Conc: 31.04 ng/ml

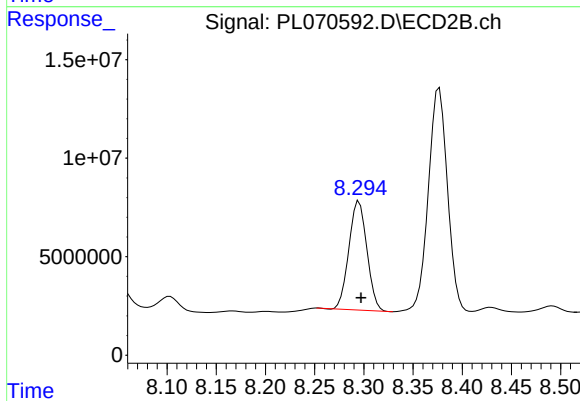

#10 gamma-Chlordane


R.T.: 8.295 min
Delta R.T.: -0.002 min
Response: 70595451
Conc: 35.36 ng/ml

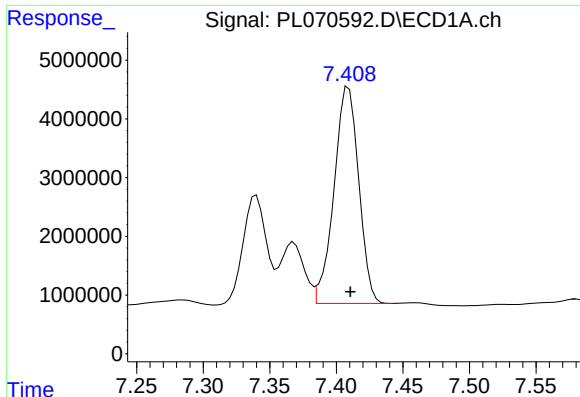

#11 alpha-Chlordane


R.T.: 7.409 min
Delta R.T.: -0.001 min
Response: 47691413
Conc: 65.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-282DL

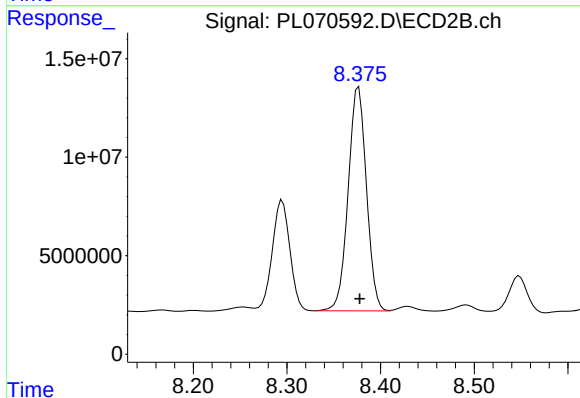


#11 alpha-Chlordane

R.T.: 8.377 min
Delta R.T.: -0.001 min
Response: 154254258
Conc: 78.78 ng/ml

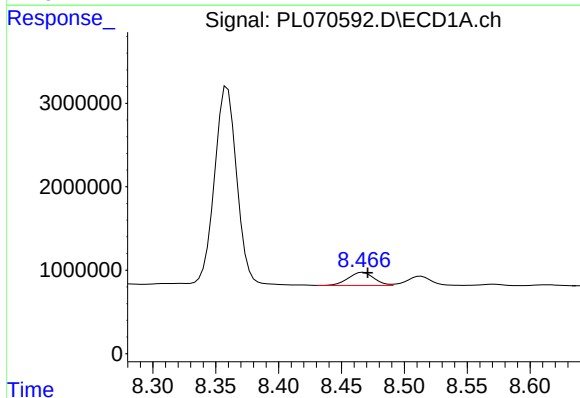


#17 4,4'-DDT

R.T.: 8.467 min
Delta R.T.: -0.004 min
Response: 2196975
Conc: 3.44 ng/ml

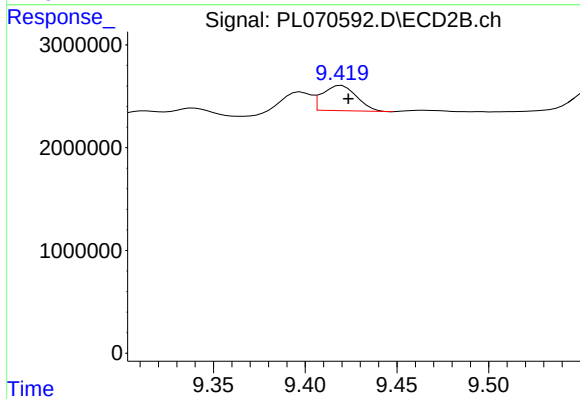

#17 4,4'-DDT


R.T.: 9.420 min
Delta R.T.: -0.004 min
Response: 3205357
Conc: 1.86 ng/ml

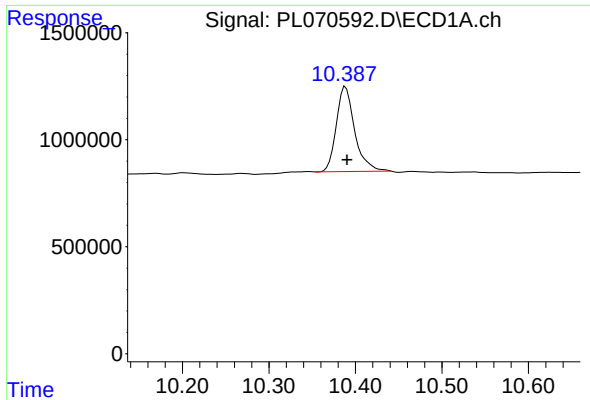

#28 Decachlorobiphenyl

R.T.: 10.389 min
Delta R.T.: -0.002 min
Response: 5840796
Conc: 7.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-282DL

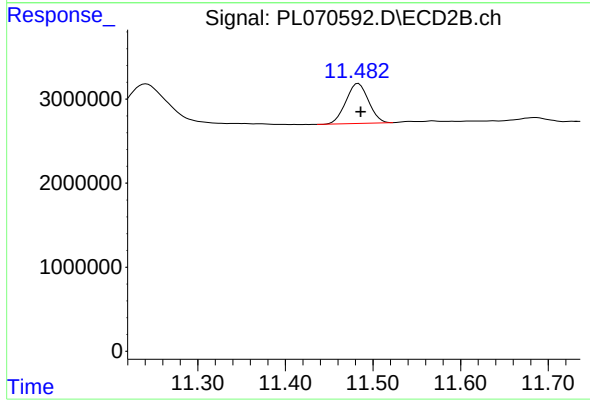

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.003 min
Response: 8551871
Conc: 5.93 ng/ml