

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
 Data File : PL070622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 03:49
 Operator : AR\AJ
 Sample : M4330-02
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JET-GROUT-SPOILS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 04:17:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.622	5.560	10483977	31034887	20.818	20.278
28)	SA Decachlor...	10.387	11.481	10962402	19553198	14.500	13.554

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102621\
Data File : PL070622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 03:49
Operator : AR\AJ
Sample : M4330-02
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JET-GROUT-SPOILS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 04:17:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

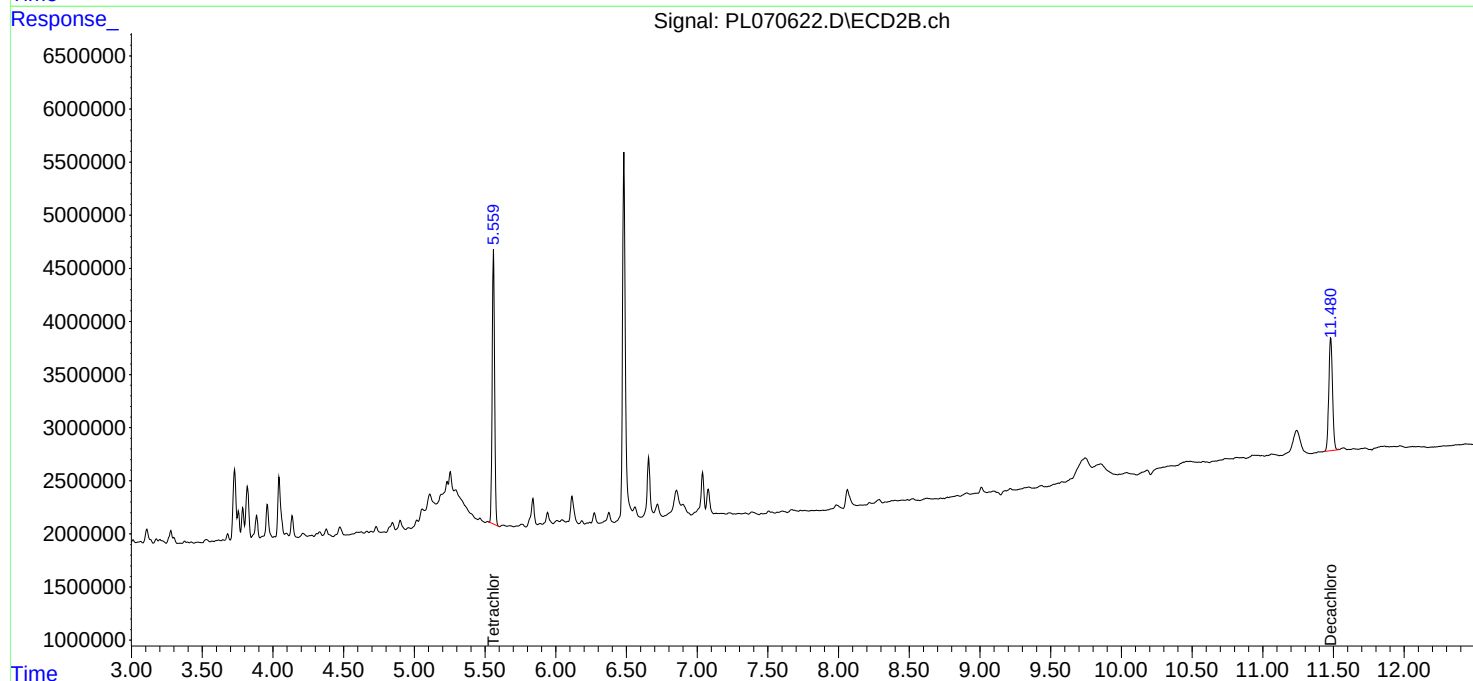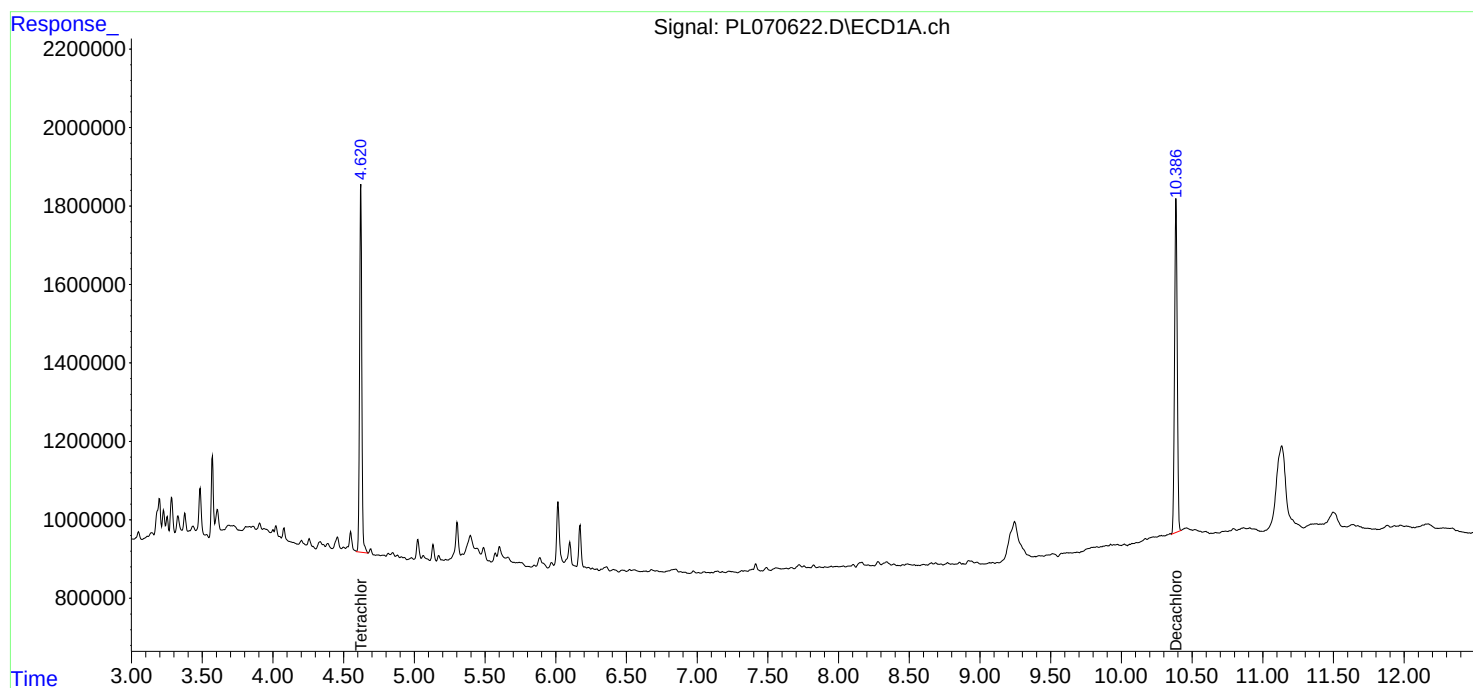


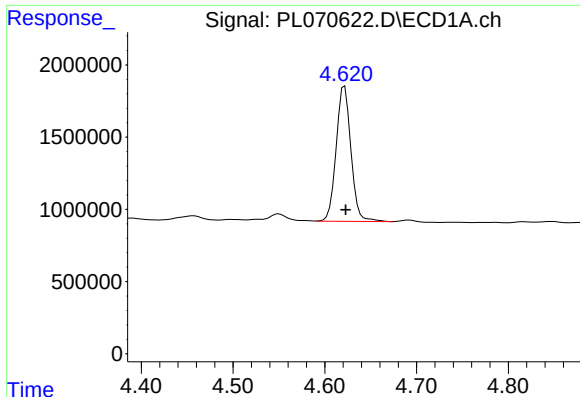

#1 Tetrachloro-m-xylene


R.T.: 4.622 min
Delta R.T.: -0.001 min
Response: 10483977
Conc: 20.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
JET-GROUT-SPOILS

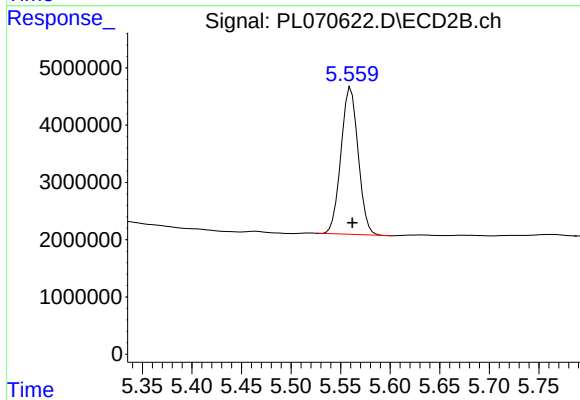


#1 Tetrachloro-m-xylene

R.T.: 5.560 min
Delta R.T.: -0.001 min
Response: 31034887
Conc: 20.28 ng/ml

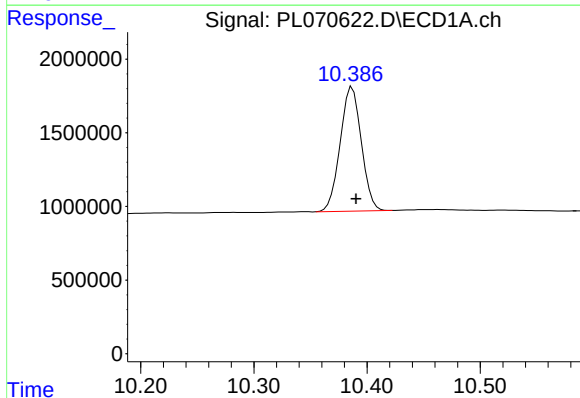

#28 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.003 min
Response: 10962402
Conc: 14.50 ng/ml

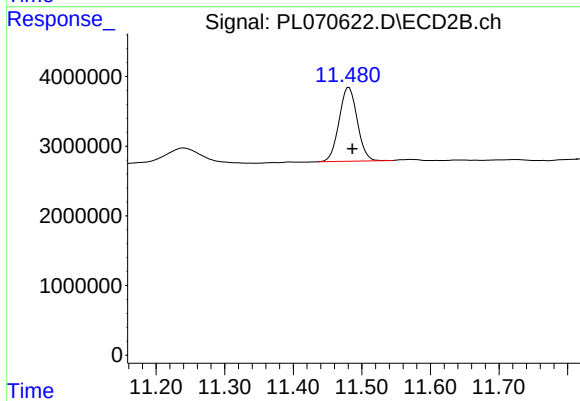

#28 Decachlorobiphenyl

R.T.: 11.481 min
Delta R.T.: -0.005 min
Response: 19553198
Conc: 13.55 ng/ml