

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102720\
 Data File : PL062618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2020 14:18
 Operator : DD\AJ
 Sample : L4523-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 05:03:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	36608004	64312925	21.283	21.885
28)	SA Decachlor...	8.128	8.989	38303027	50396793	23.875	24.079
Target Compounds							
2)	A alpha-BHC	0.000	4.309f	0	2059907	N.D.	0.464 #
7)	B delta-BHC	0.000	5.004	0	3334178	N.D.	0.953 #
8)	B Heptachlo...	0.000	5.828	0	2831793	N.D.	0.874 #
10)	B gamma-Chl...	0.000	6.070f	0	2234401	N.D.	0.664 #
15)	B Endosulfa...	0.000	6.869f	0	6188988	N.D.	2.165 #
21)	B Endrin ke...	0.000	7.670	0	2800710	N.D.	1.182 #
23)	Chlordane-1	4.277	0.000	498941	0	9.679	N.D. #
25)	Chlordane-3	0.000	6.070f	0	2234401	N.D.	5.532 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102720\
Data File : PL062618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2020 14:18
Operator : DD\AJ
Sample : L4523-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 05:03:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

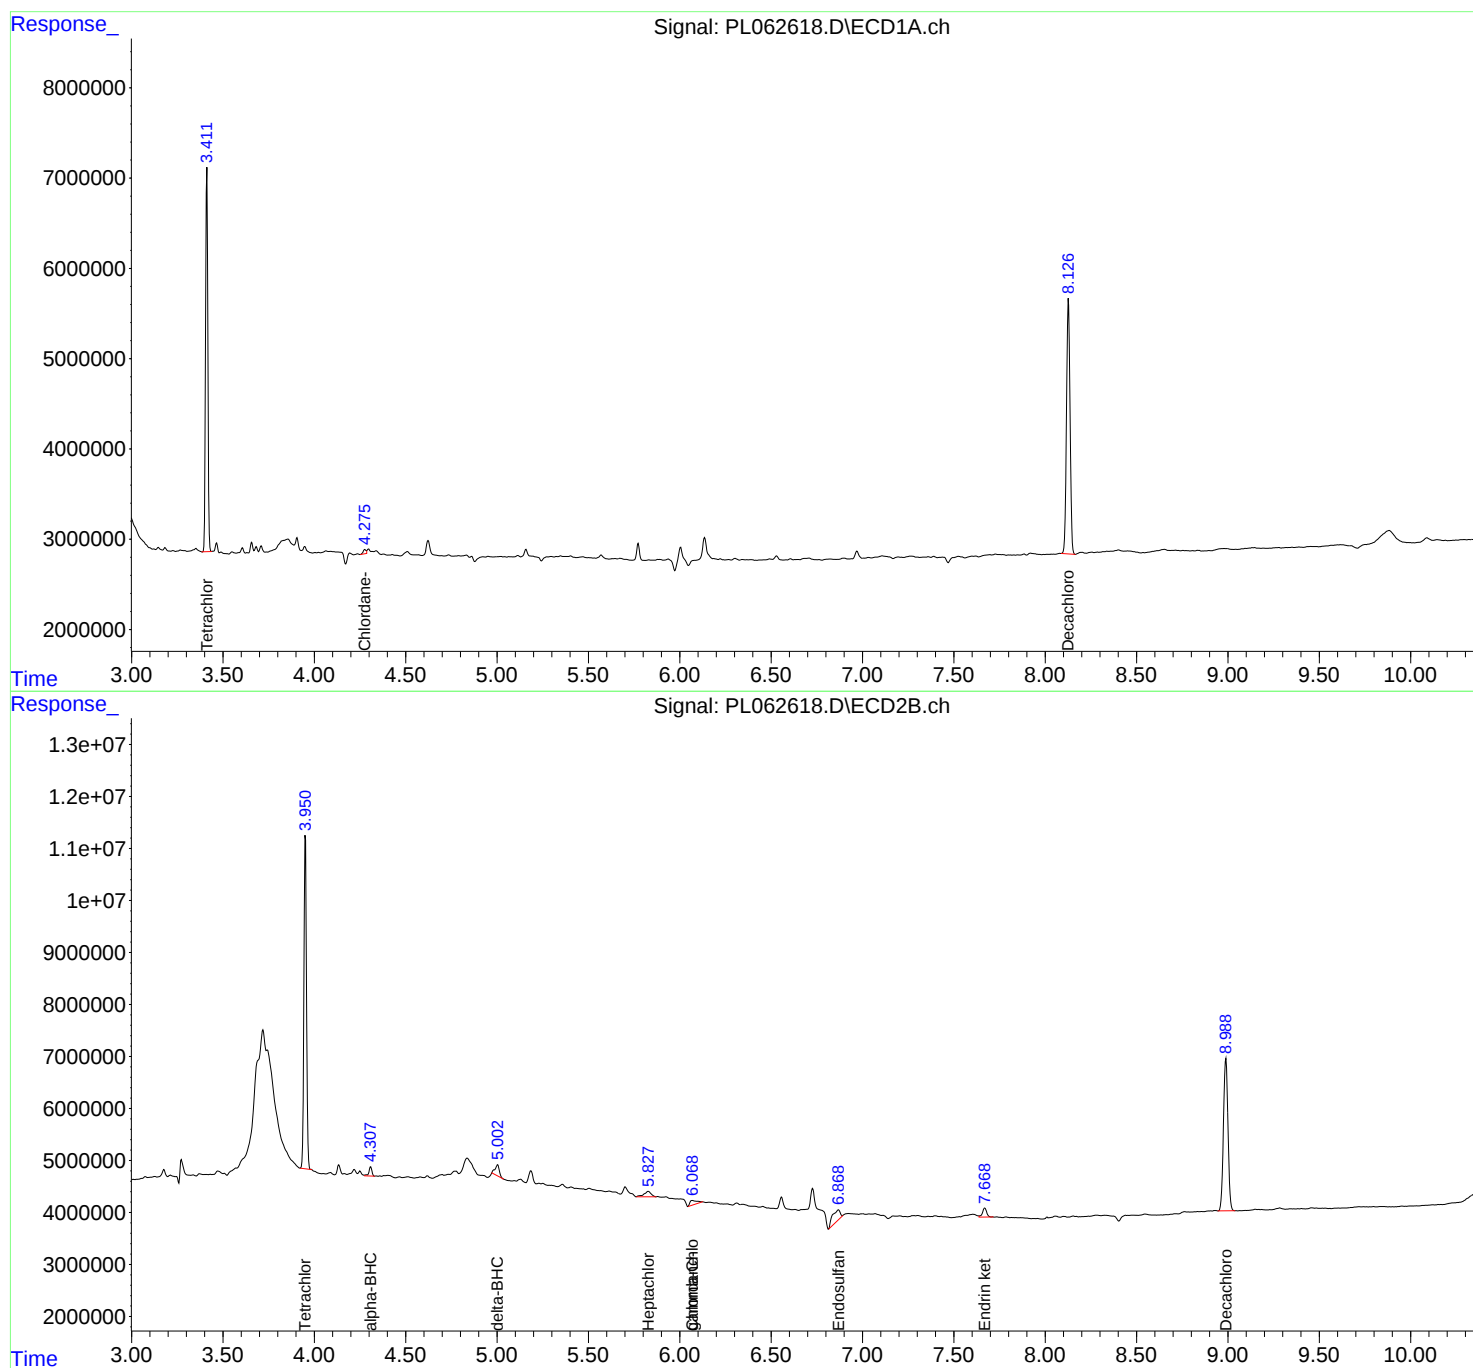


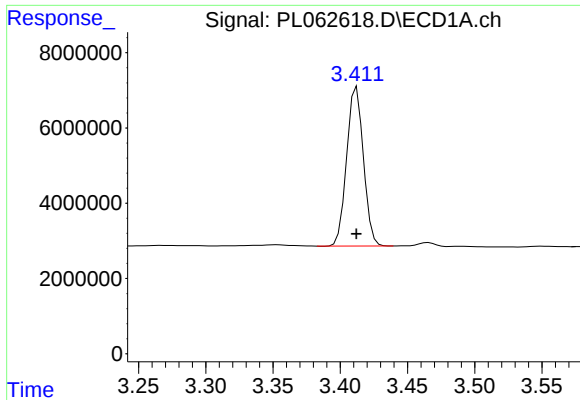

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 36608004
Conc: 21.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

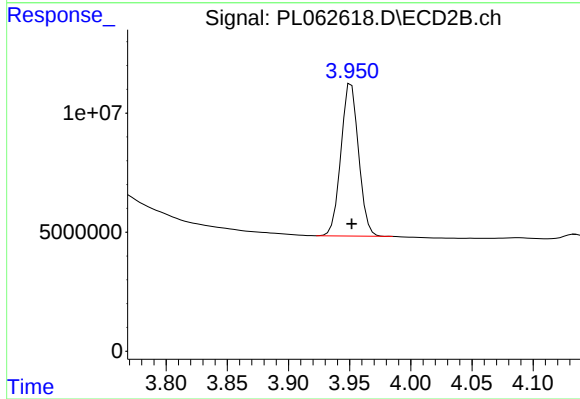


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 64312925
Conc: 21.88 ng/ml

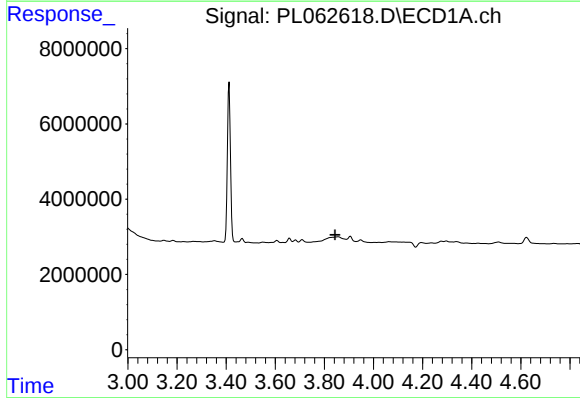


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

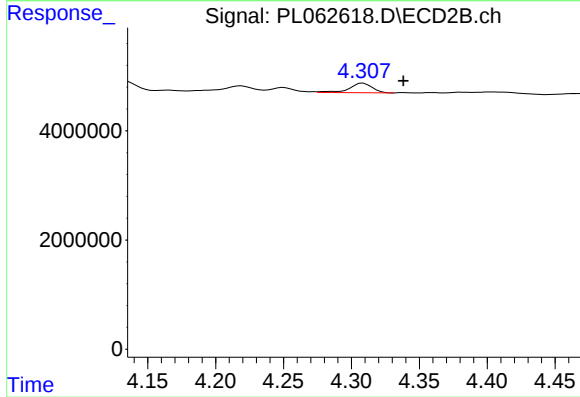

#2 alpha-BHC


R.T.: 4.309 min
Delta R.T.: -0.029 min
Response: 2059907
Conc: 0.46 ng/ml

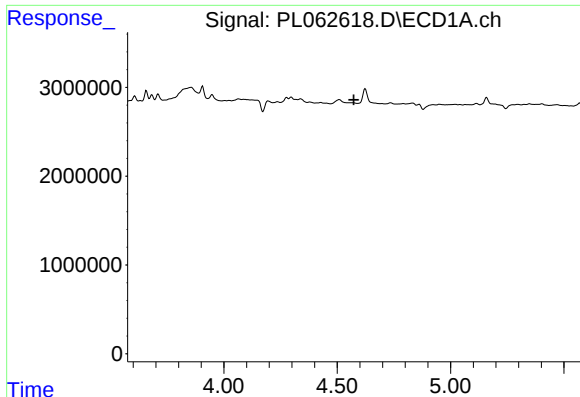

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

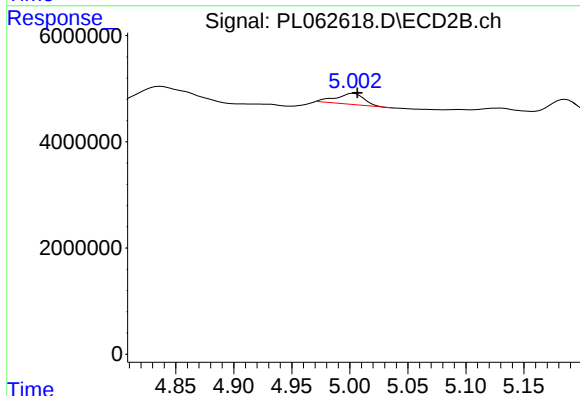


#7 delta-BHC

R.T.: 5.004 min
Delta R.T.: -0.003 min
Response: 3334178
Conc: 0.95 ng/ml

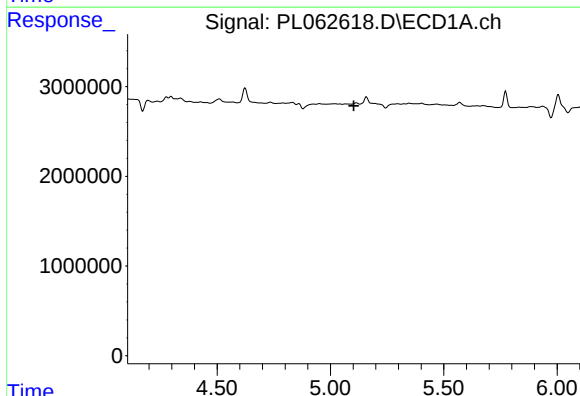


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

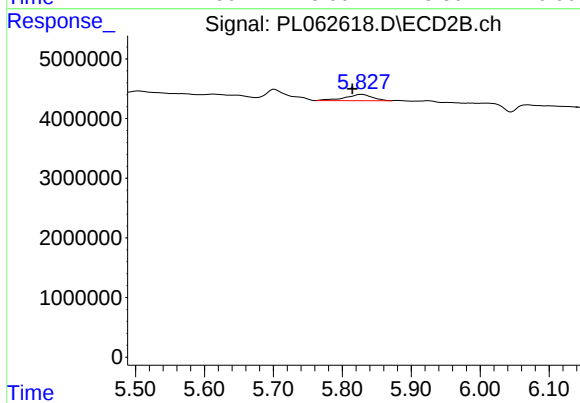

#8 Heptachlor epoxide


R.T.: 5.828 min
Delta R.T.: 0.014 min
Response: 2831793
Conc: 0.87 ng/ml

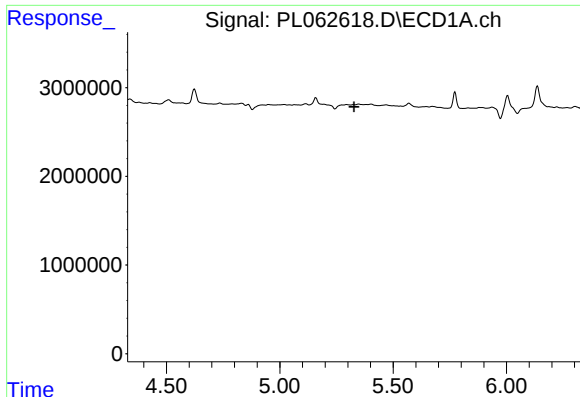

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

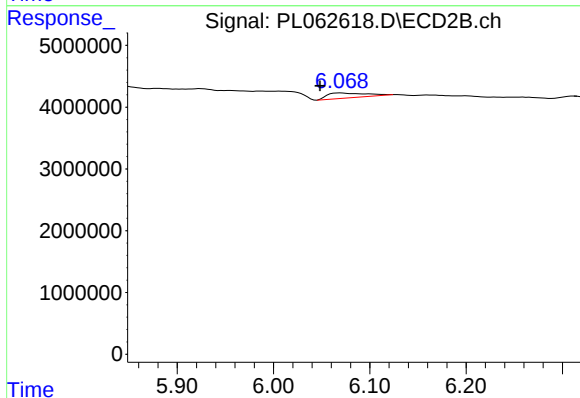


#10 gamma-Chlordane

R.T.: 6.070 min
Delta R.T.: 0.021 min
Response: 2234401
Conc: 0.66 ng/ml

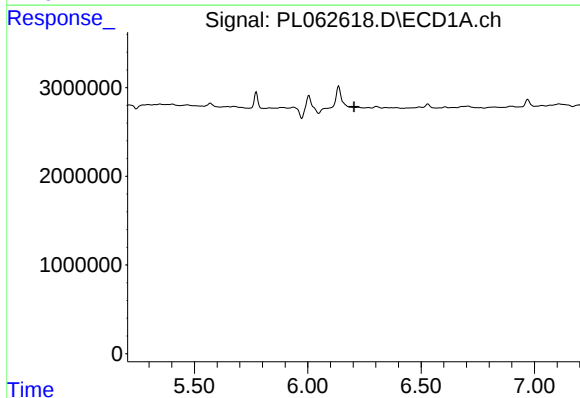


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

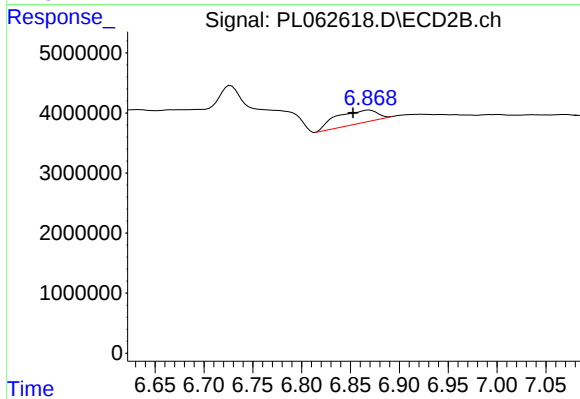

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 6188988
Conc: 2.17 ng/ml

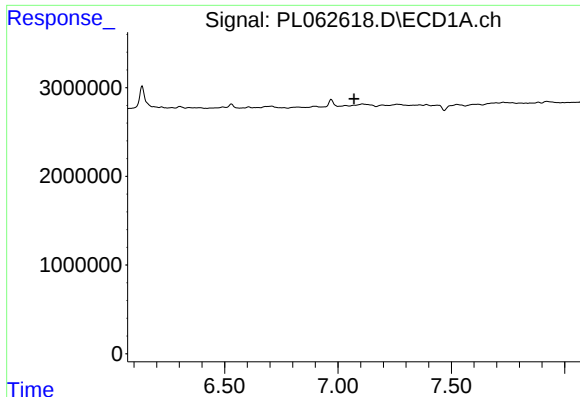

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

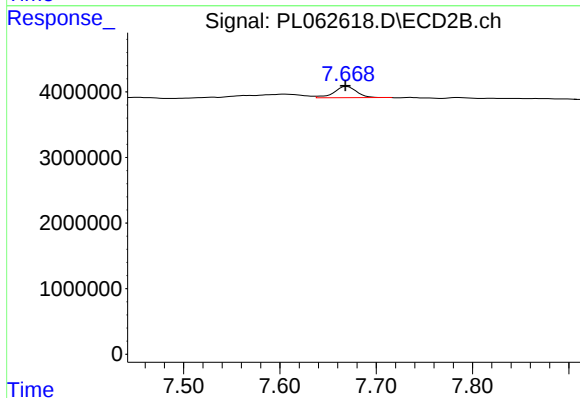


#21 Endrin ketone

R.T.: 7.670 min
Delta R.T.: 0.001 min
Response: 2800710
Conc: 1.18 ng/ml

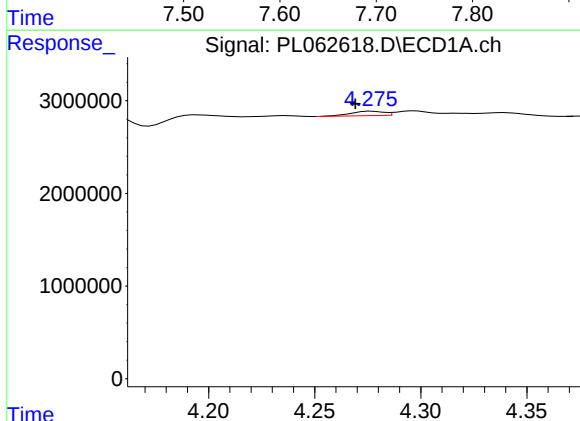


#23 Chlordane-1

R.T.: 4.277 min
Delta R.T.: 0.008 min
Response: 498941
Conc: 9.68 ng/ml

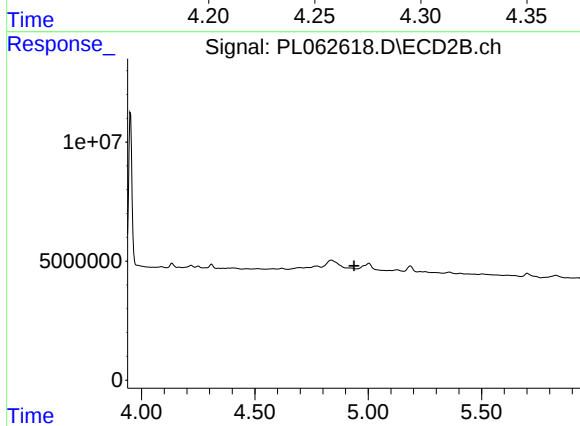

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

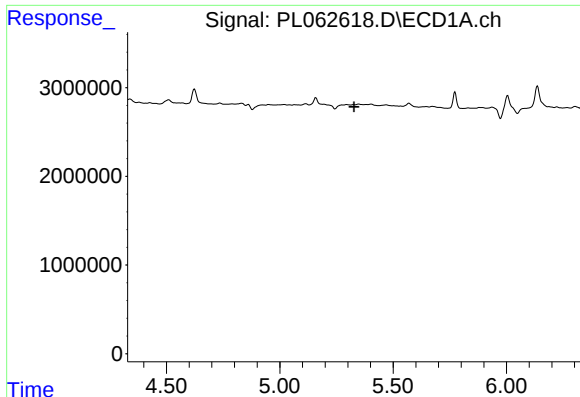

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

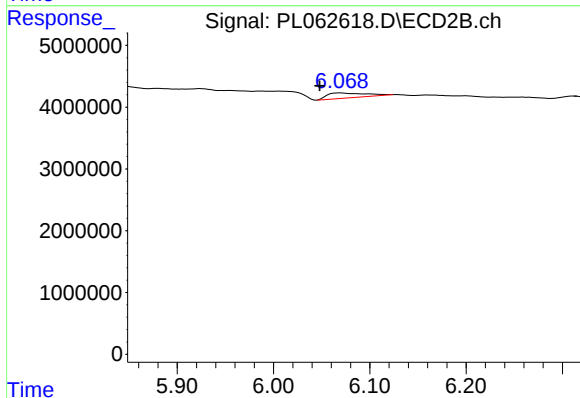


#25 Chlordane-3

R.T.: 6.070 min
Delta R.T.: 0.021 min
Response: 2234401
Conc: 5.53 ng/ml

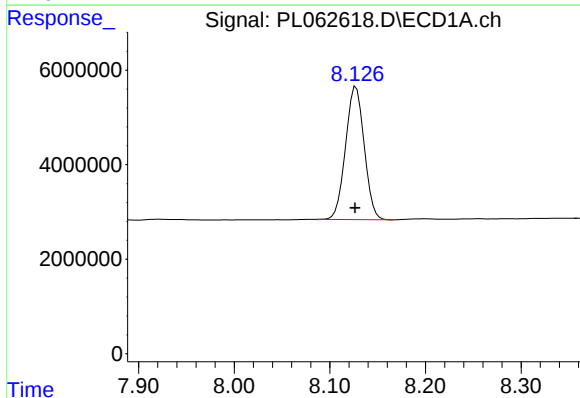

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 38303027
Conc: 23.88 ng/ml

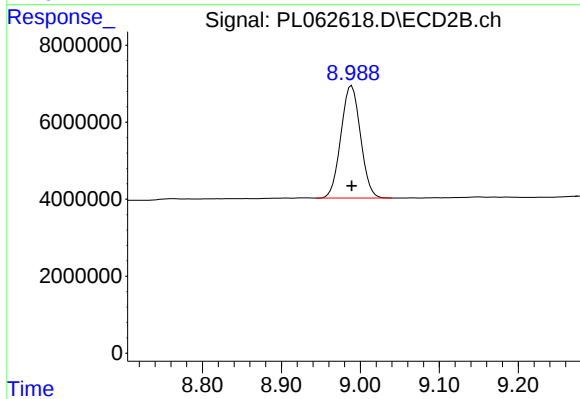

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 50396793
Conc: 24.08 ng/ml