

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102720\
 Data File : PL062626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2020 16:19
 Operator : DD\AJ
 Sample : L4520-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PS-FRAC

Manual Integrations
 APPROVED

Ankita
 10/28/2020 3:44:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:55:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	33485785	54282193	19.468	18.471
28)	SA Decachlor...	8.126	8.989	23292174	33117888	14.519	15.823
Target Compounds							
11)	B alpha-Chl...	5.374	6.120	8080411	2050802	4.470m	0.609 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102720\
Data File : PL062626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2020 16:19
Operator : DD\AJ
Sample : L4520-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PS-FRAC


Manual Integrations
APPROVED

Ankita
10/28/2020 3:44:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:55:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

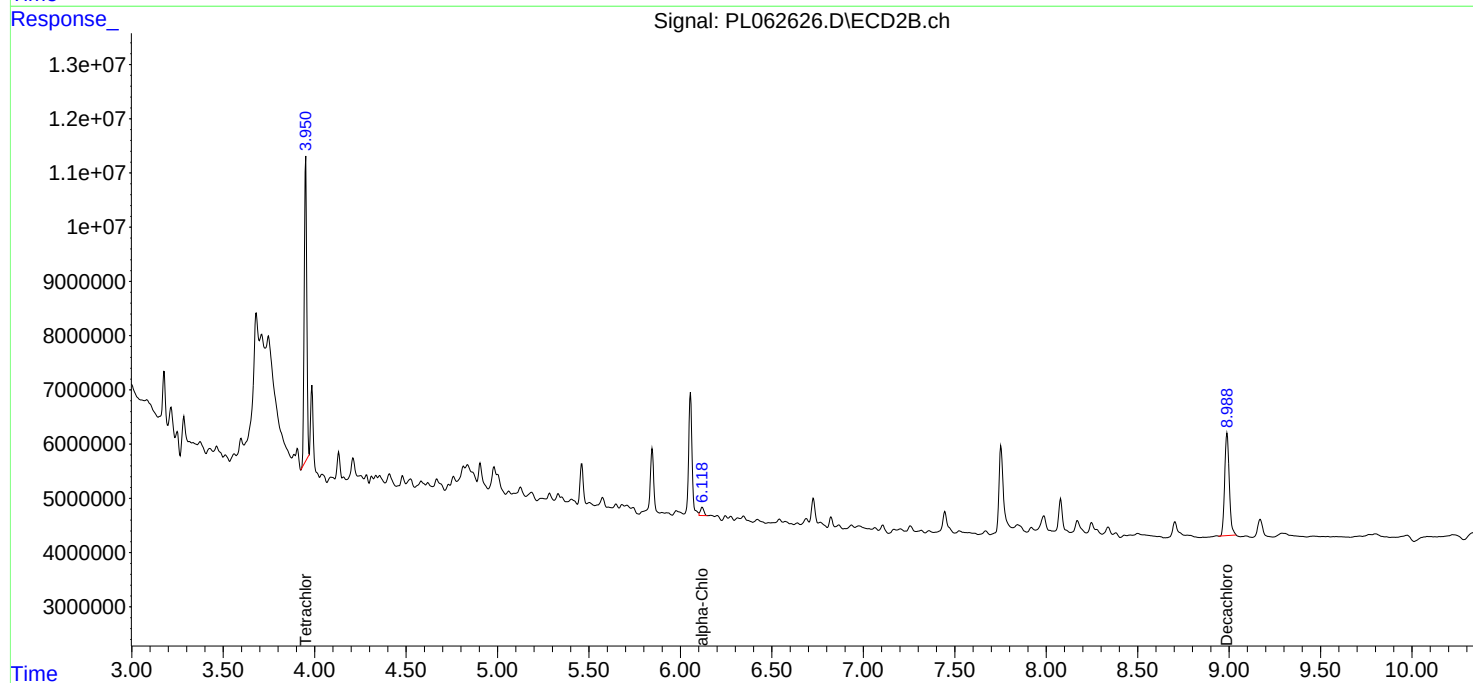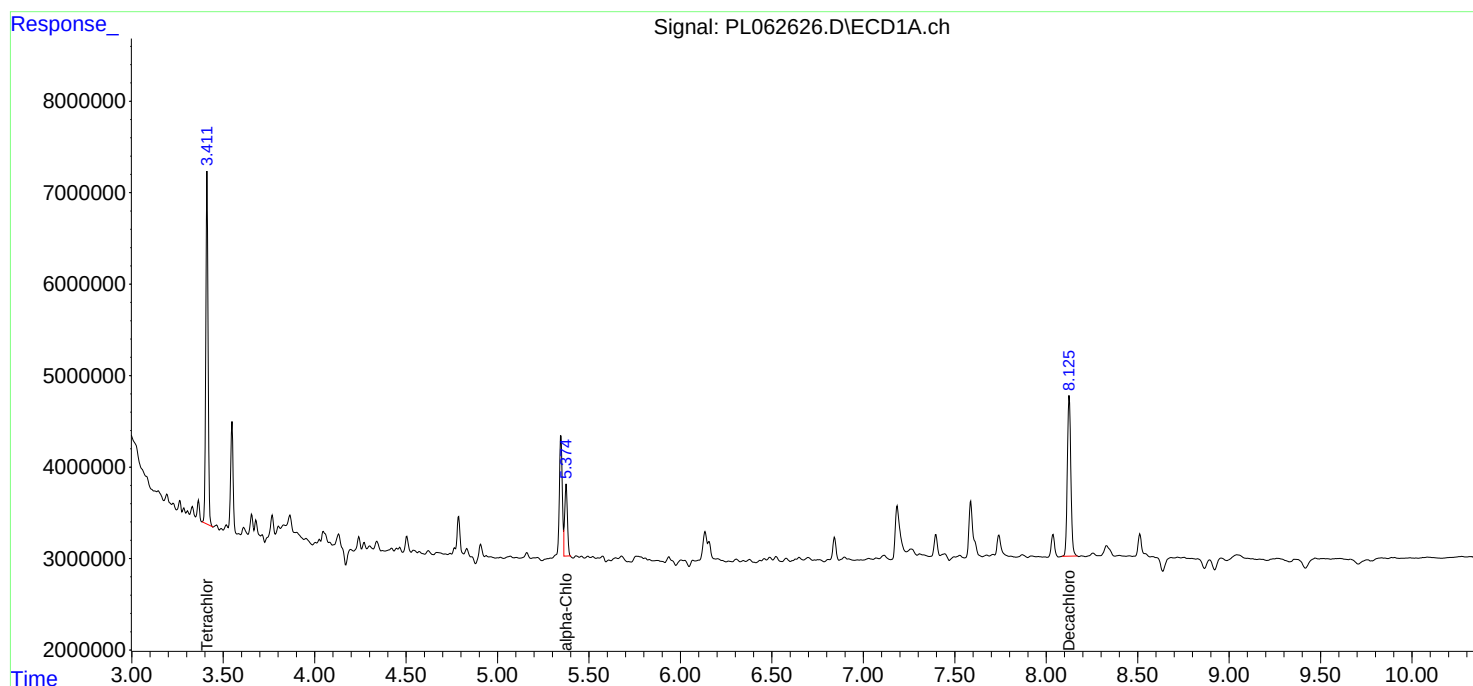

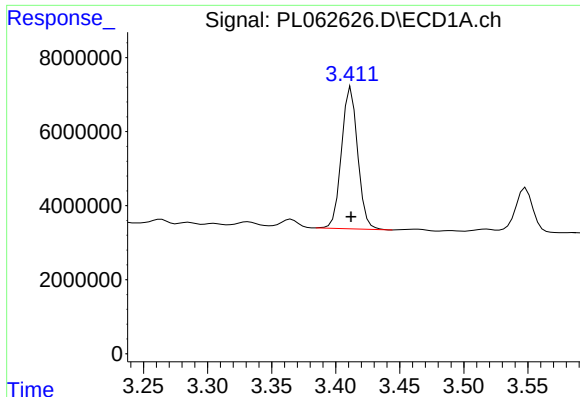


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 33485785
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-FRAC


Manual Integrations
APPROVED

Ankita
10/28/2020 3:44:47 PM

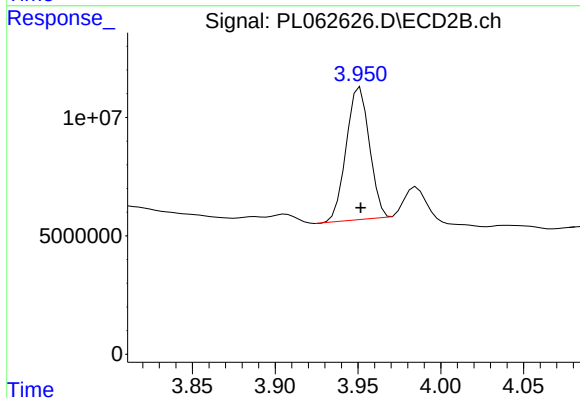


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 54282193
Conc: 18.47 ng/ml

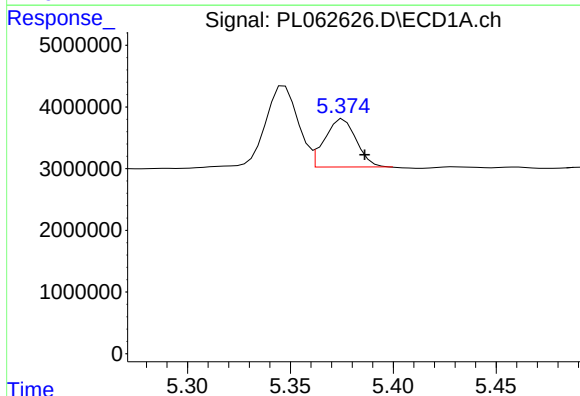


#11 alpha-Chlordane

R.T.: 5.374 min
Delta R.T.: -0.012 min
Response: 8080411
Conc: 4.47 ng/ml m

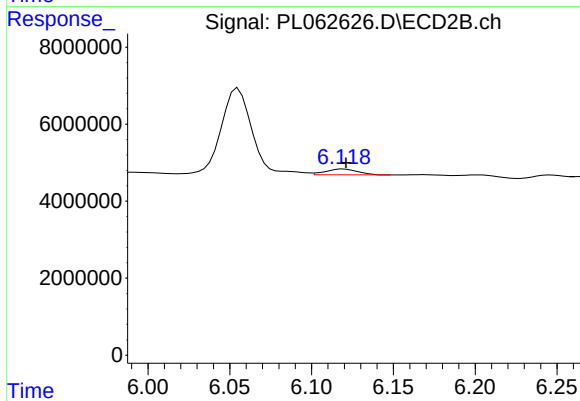

#11 alpha-Chlordane

R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 2050802
Conc: 0.61 ng/ml

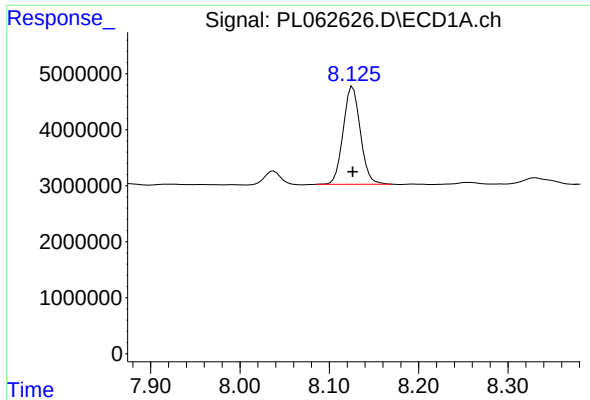


#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 23292174
Conc: 14.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-FRAC

Manual Integrations
APPROVED

Ankita
10/28/2020 3:44:47 PM

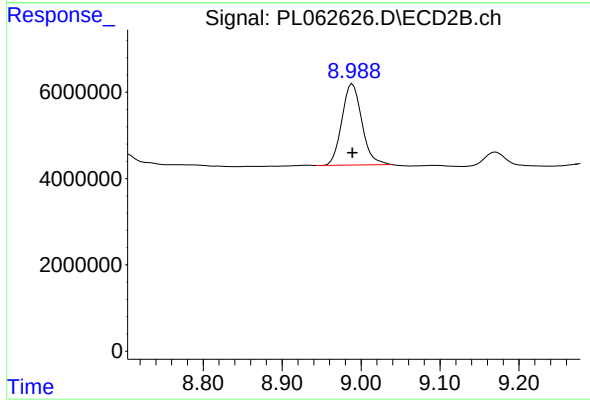

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 33117888
Conc: 15.82 ng/ml