

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102722\
 Data File : PL078552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 13:16
 Operator : AR\AJ
 Sample : PB148575BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB148575BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/27/2022
 Supervised By : Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 21:39:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.331	2.568	36124379	48747324	18.943	19.093
2) SA Decachlor...	8.786	7.645	31000808	38253598	20.607m	20.196

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102722\
Data File : PL078552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 13:16
Operator : AR\AJ
Sample : PB148575BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB148575BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/27/2022
Supervised By : Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 21:39:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

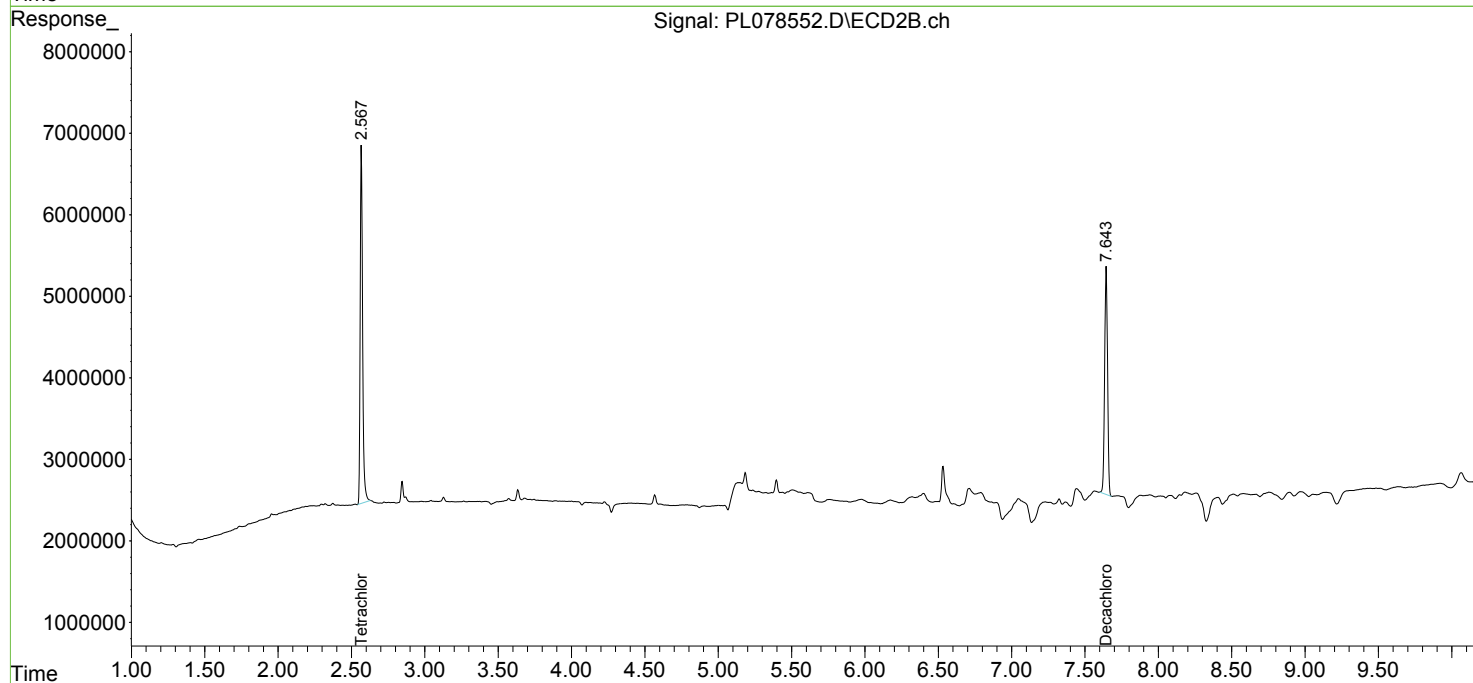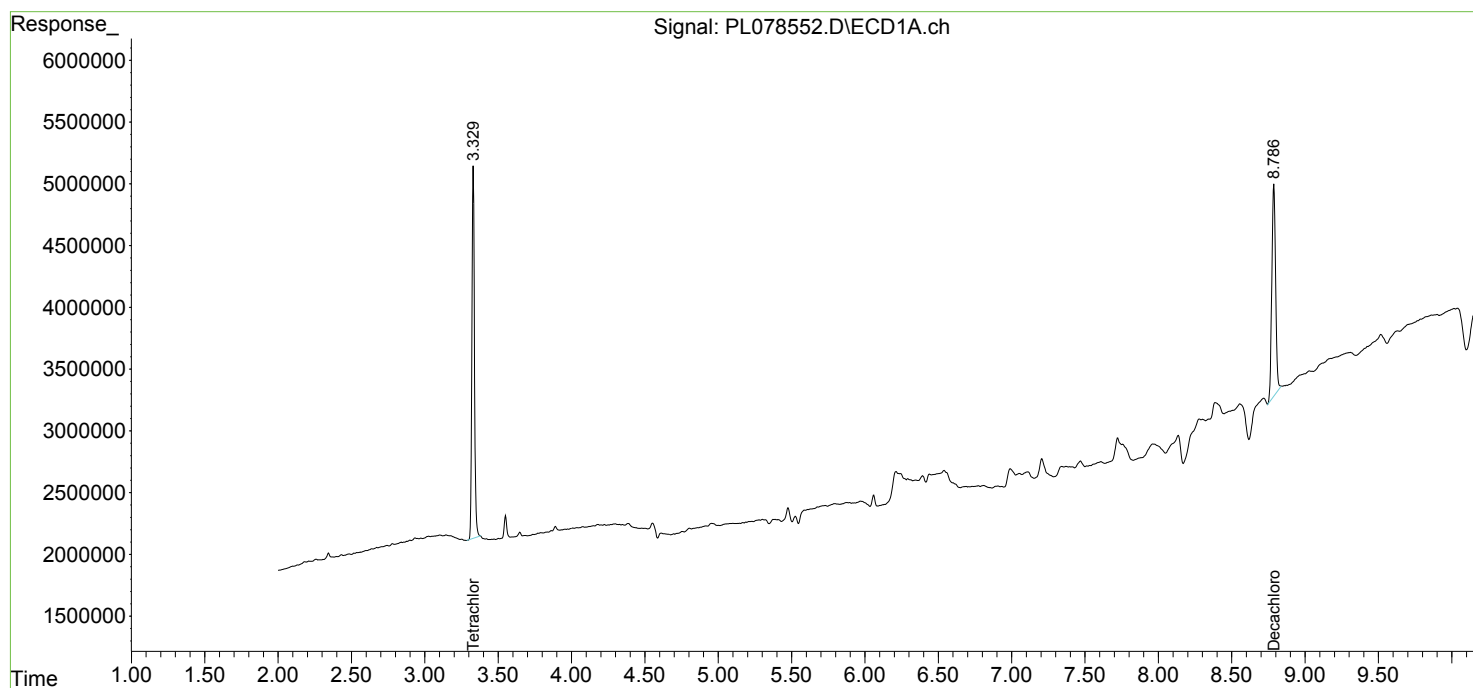

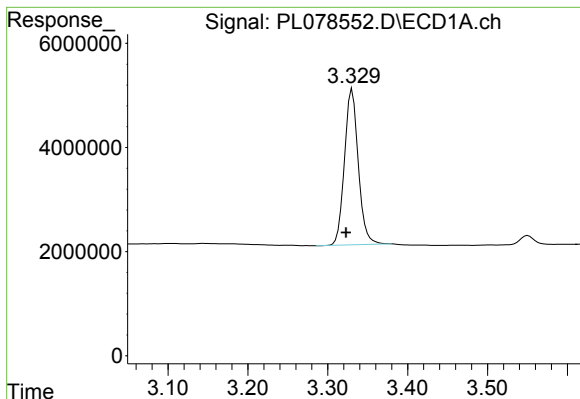

#1 Tetrachloro-m-xylene

R.T.: 3.331 min
Delta R.T.: 0.008 min
Response: 36124379
Conc: 18.94 ng/ml

Instrument :

ECD_L

ClientSampleId :


PB148575BL

Manual Integrations

APPROVED


Reviewed By :Abdul Mirza 10/27/2022

Supervised By :Ankita Jodhani 10/27/2022

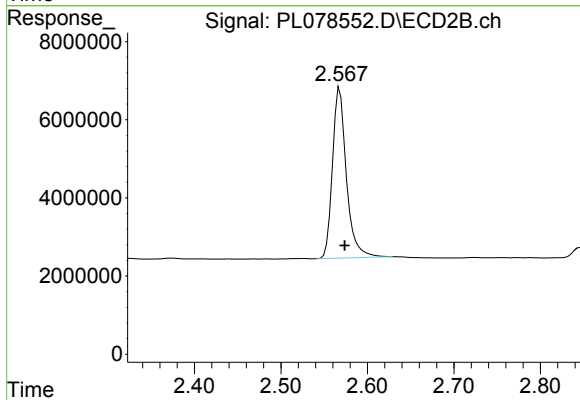


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 48747324
Conc: 19.09 ng/ml

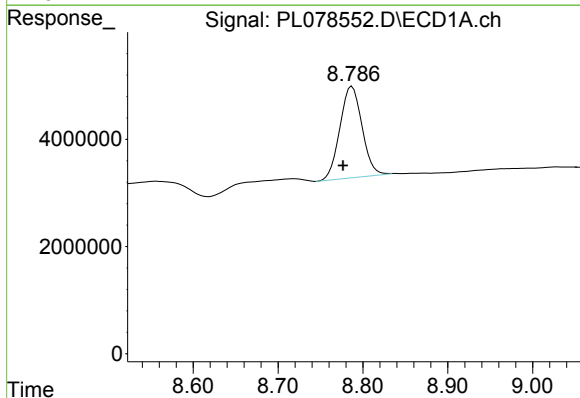

#28 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: 0.009 min
Response: 31000808
Conc: 20.61 ng/ml m

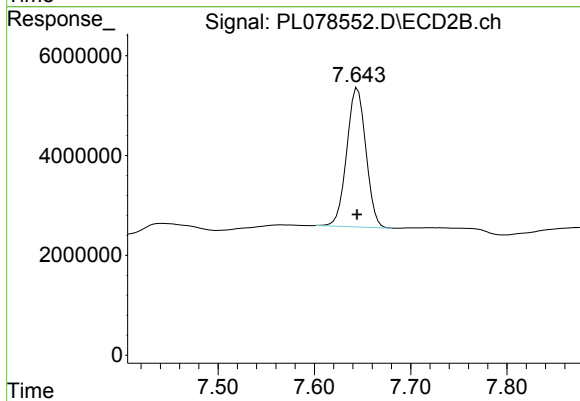

#28 Decachlorobiphenyl

R.T.: 7.645 min
Delta R.T.: 0.000 min
Response: 38253598
Conc: 20.20 ng/ml