

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102722\
 Data File : PL078563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 17:45
 Operator : AR\AJ
 Sample : N5272-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20221117-AMENDED-COMP-02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/27/2022
 Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 21:43:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.571	29544781	41757147	15.493	16.355
2)	SA Decachlor...	8.777	7.644	7969412	11074928	5.298	5.847
Target Compounds							
12)	B 4,4'-DDE	5.977	4.980	1161707	1369366	0.580	0.503m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102722\
Data File : PL078563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 17:45
Operator : AR\AJ
Sample : N5272-07
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20221117-AMENDED-COMP-02


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/27/2022
Supervised By : Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 21:43:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

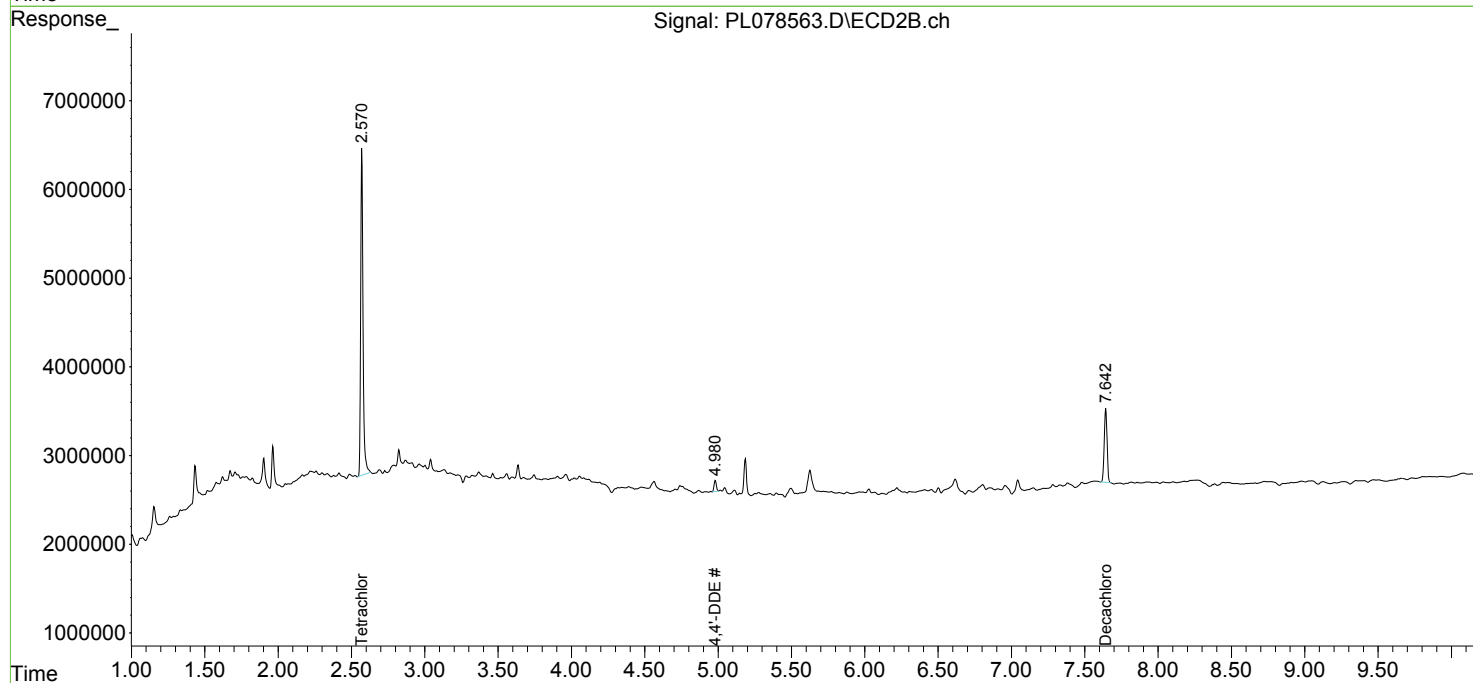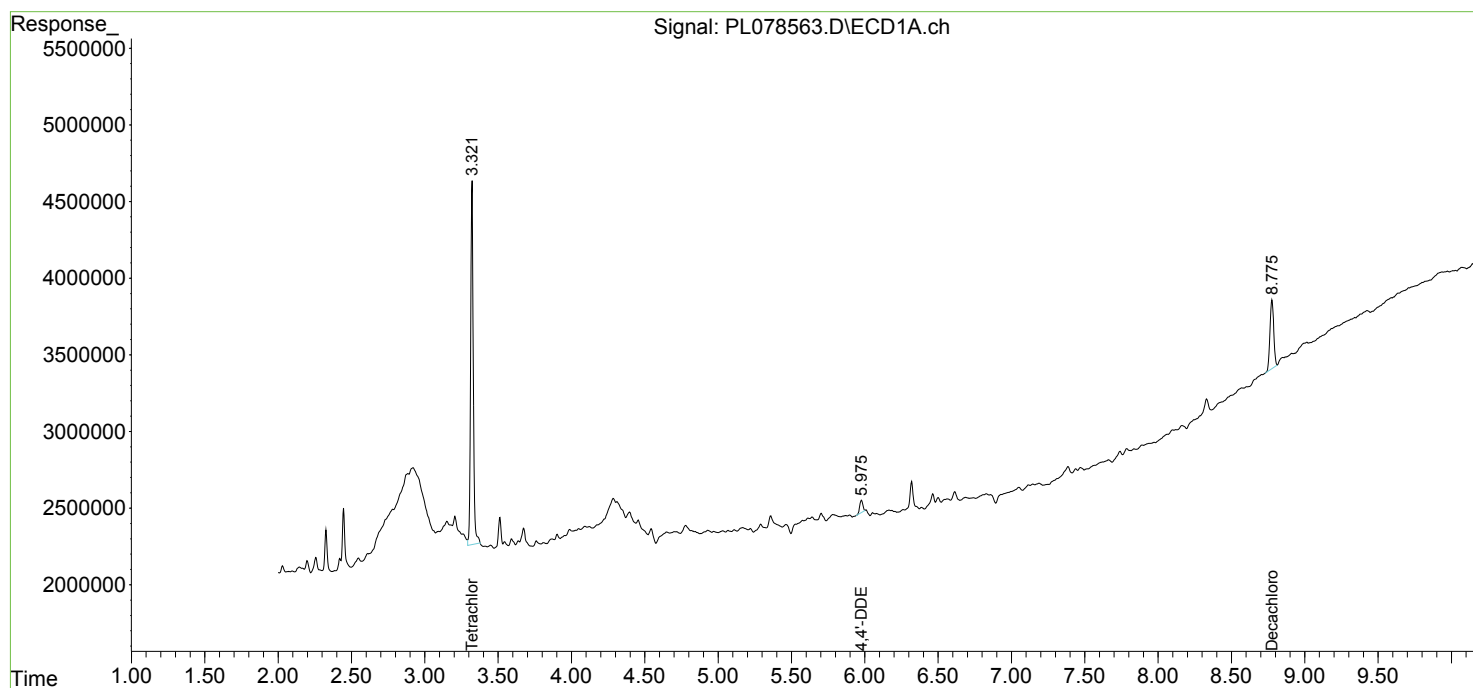

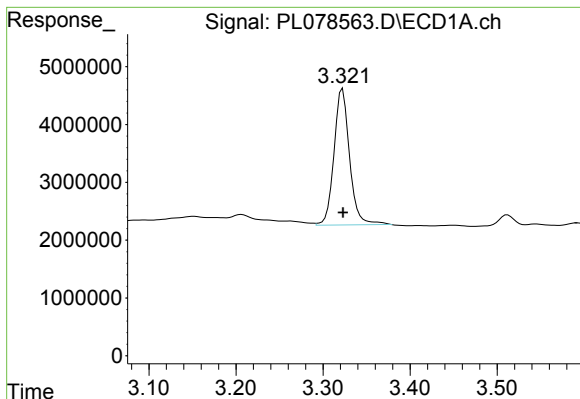


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 29544781
Conc: 15.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
20221117-AMENDED-COMP-02


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/27/2022
Supervised By :Ankita Jodhani 10/27/2022

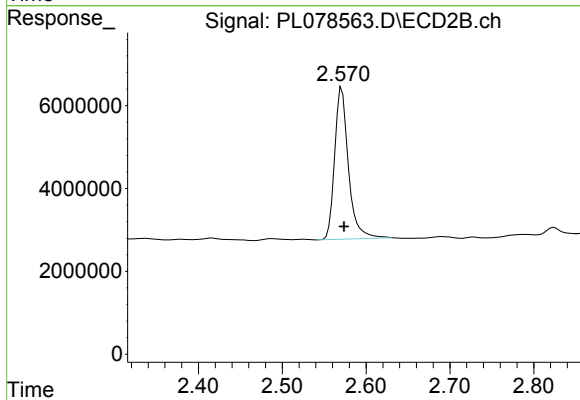


#1 Tetrachloro-m-xylene

R.T.: 2.571 min
Delta R.T.: -0.003 min
Response: 41757147
Conc: 16.35 ng/ml

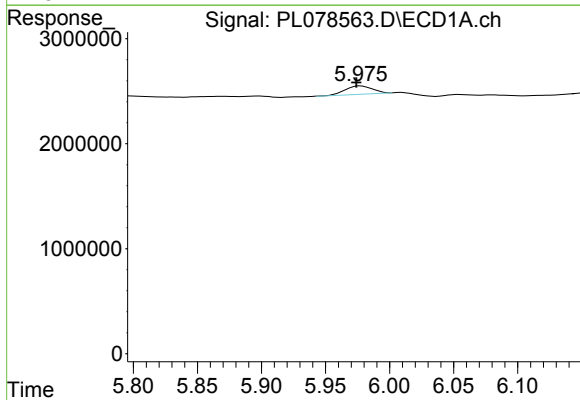


#12 4,4'-DDE

R.T.: 5.977 min
Delta R.T.: 0.003 min
Response: 1161707
Conc: 0.58 ng/ml

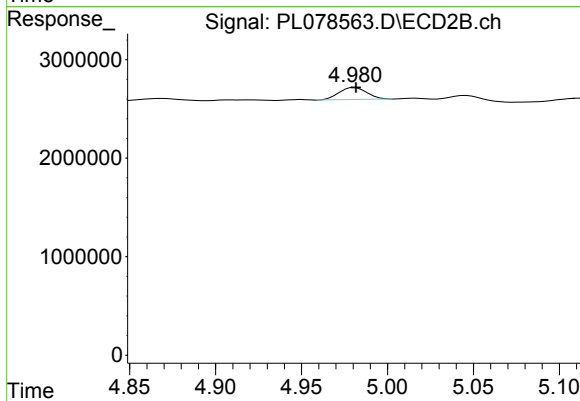

#12 4,4'-DDE

R.T.: 4.980 min
Delta R.T.: -0.002 min
Response: 1369366
Conc: 0.50 ng/ml m

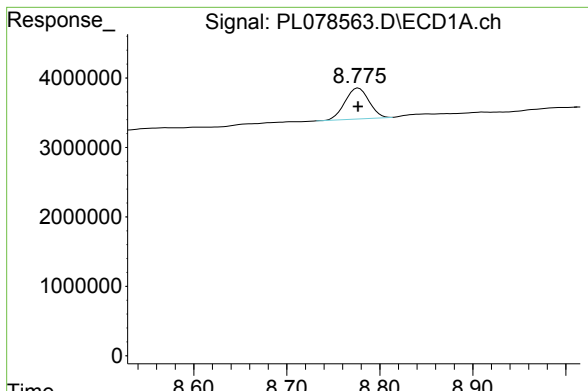


#28 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 7969412
Conc: 5.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
20221117-AMENDED-COMP-02

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/27/2022
Supervised By :Ankita Jodhani 10/27/2022

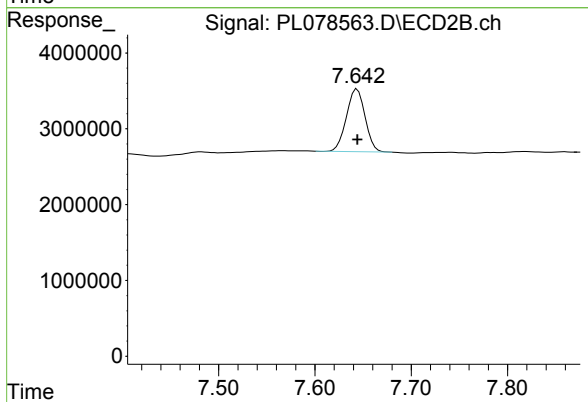

#28 Decachlorobiphenyl

R.T.: 7.644 min
Delta R.T.: 0.000 min
Response: 11074928
Conc: 5.85 ng/ml