

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102819\
 Data File : PL053848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2019 16:56
 Operator : SG\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 09:18:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.044	601.9E6	140.1E6	55.529	55.971
28)	SA Decachlor...	8.325	9.121	386.9E6	130.3E6	39.433	46.268
Target Compounds							
2)	A alpha-BHC	3.985	4.436	978.1E6	200.4E6	56.097	57.979
3)	MA gamma-BHC...	4.272	4.721	877.6E6	184.7E6	56.354	57.346
4)	MA Heptachlor	4.579	5.230	863.5E6	173.7E6	54.709	53.901
5)	MB Aldrin	4.830	5.536	813.8E6	165.2E6	56.924	55.405
6)	B beta-BHC	4.522	4.891	357.4E6	83860168	54.236	54.292
7)	B delta-BHC	4.731	5.108	849.7E6	176.3E6	55.821	58.376
8)	B Heptachlo...	5.276	5.922	742.9E6	157.0E6	55.035	53.850
9)	A Endosulfan I	5.618	6.279	671.8E6	140.0E6	54.649	51.635
10)	B gamma-Chl...	5.505	6.156	757.5E6	150.0E6	55.522	51.404
11)	B alpha-Chl...	5.563	6.228	717.4E6	151.8E6	53.922	51.991
12)	B 4,4'-DDE	5.726	6.384	645.9E6	146.7E6	54.357	52.073
13)	MA Dieldrin	5.862	6.536	674.2E6	149.0E6	51.732	52.223
14)	MA Endrin	6.120	6.754	550.3E6	117.7E6	47.473	48.509
15)	B Endosulfa...	6.393	6.962	518.2E6	130.3E6	46.353	50.990
16)	A 4,4'-DDD	6.243	6.874	475.7E6	116.3E6	53.450	55.809
17)	MA 4,4'-DDT	6.486	7.173	426.6E6	106.8E6	43.067	46.193
18)	B Endrin al...	6.562	7.086	412.2E6	107.8E6	44.950	49.075
19)	B Endosulfa...	6.775	7.309	477.9E6	117.3E6	46.985	47.819
20)	A Methoxychlor	7.030	7.630	211.9E6	57014205	42.975	43.894
21)	B Endrin ke...	7.269	7.780	493.5E6	125.0E6	45.843	48.463
22)	Mirex	7.462	8.235	370.4E6	99420301	43.301	49.143
23)	Chlordane-1	4.449f	0.000	5117157	0	14.428	N.D. #
24)	Chlordane-2	0.000	5.536f	0	165.2E6	N.D.	1681.849 #
25)	Chlordane-3	5.505	6.156	757.5E6	150.0E6	657.177	410.667 #
26)	Chlordane-4	5.563	6.228	717.4E6	151.8E6	765.219	338.070 #
27)	Chlordane-5	6.393f	0.000	518.2E6	0	1417.732	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102819\
Data File : PL053848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 16:56
Operator : SG\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 09:18:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

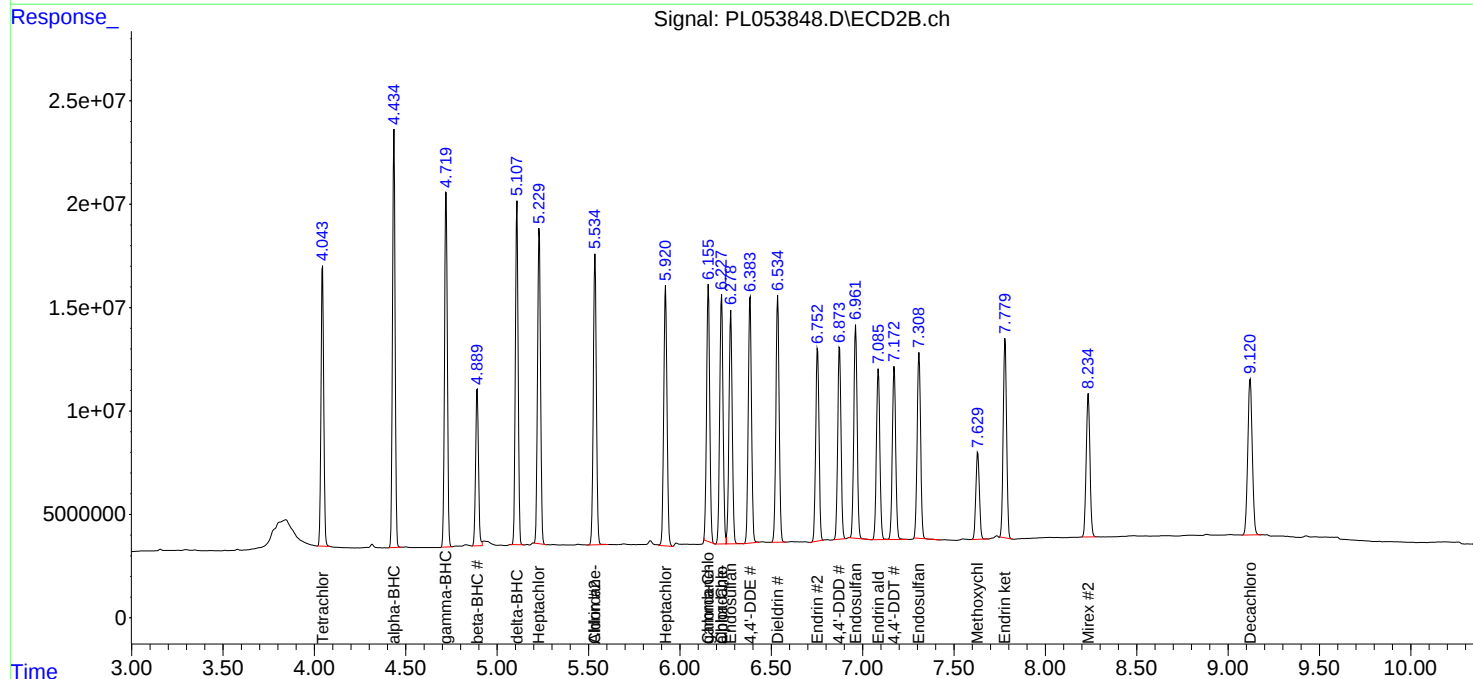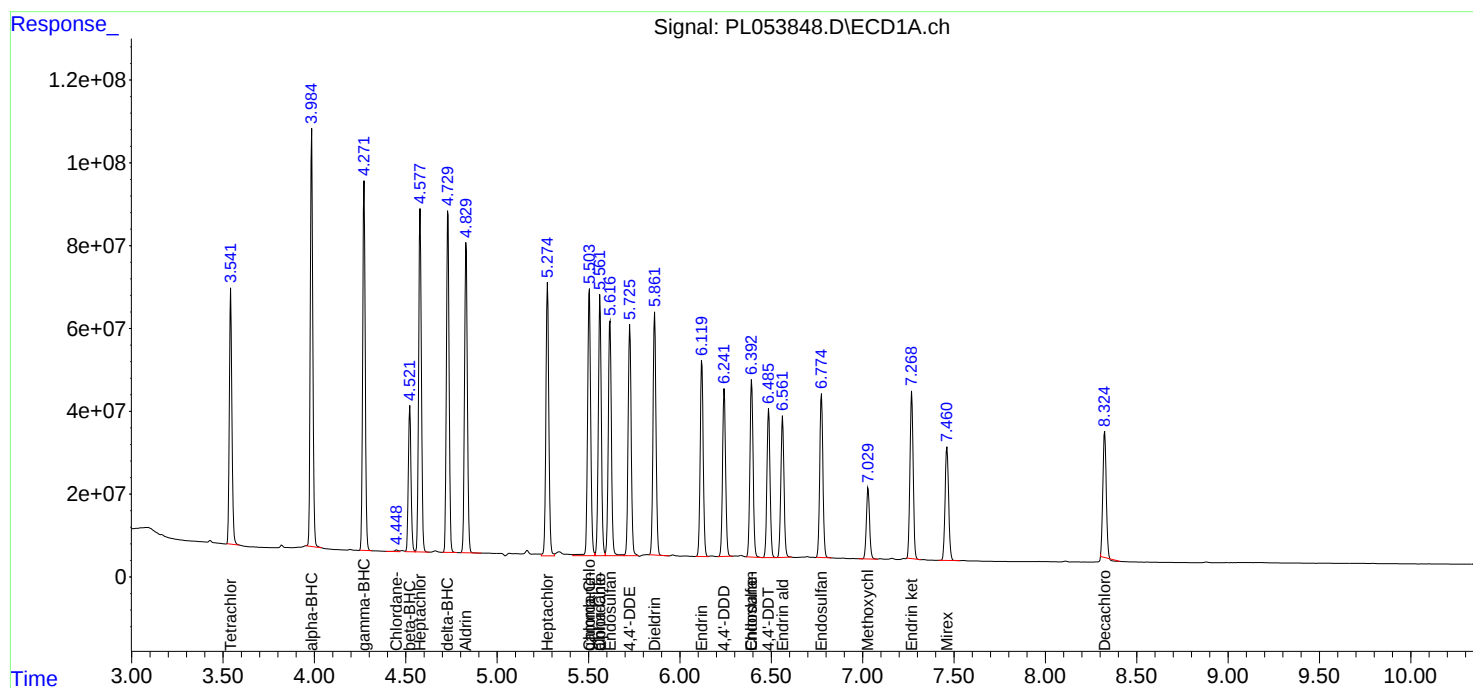


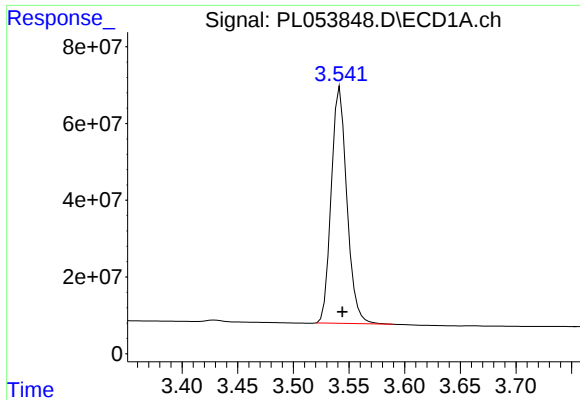

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 601902897
Conc: 55.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

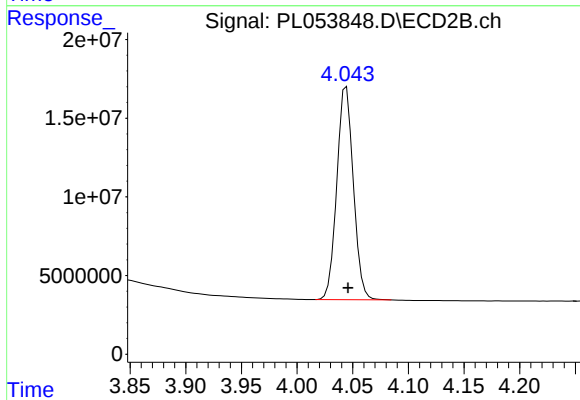


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 140060045
Conc: 55.97 ng/ml

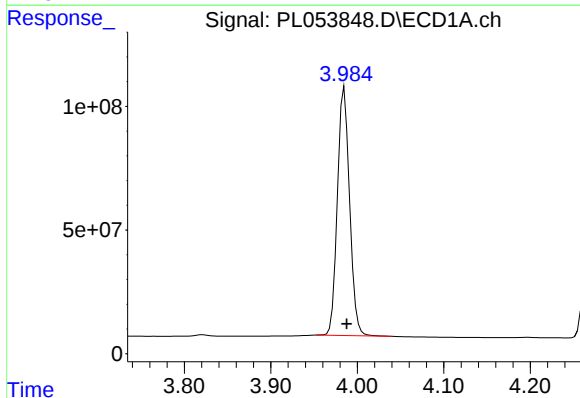


#2 alpha-BHC

R.T.: 3.985 min
Delta R.T.: -0.003 min
Response: 978130133
Conc: 56.10 ng/ml

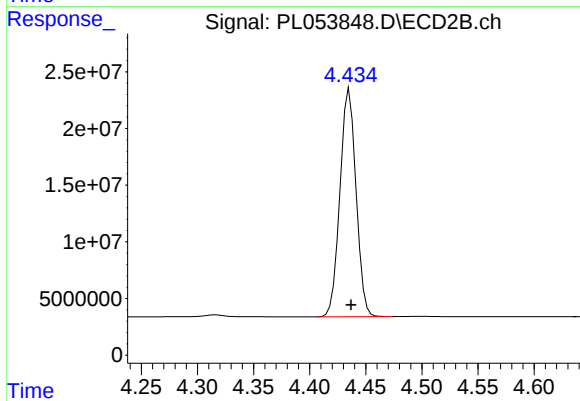

#2 alpha-BHC


R.T.: 4.436 min
Delta R.T.: -0.001 min
Response: 200437573
Conc: 57.98 ng/ml

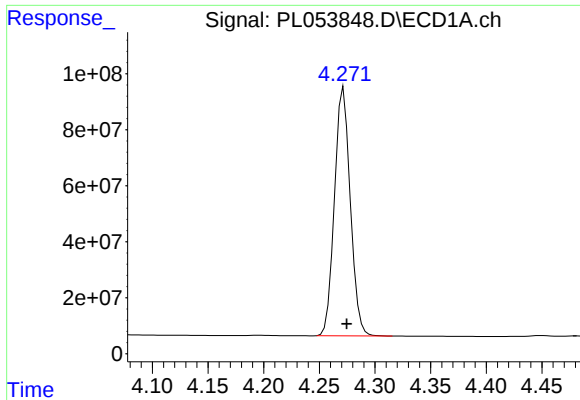

#3 gamma-BHC (Lindane)


R.T.: 4.272 min
Delta R.T.: -0.003 min
Response: 877629006
Conc: 56.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

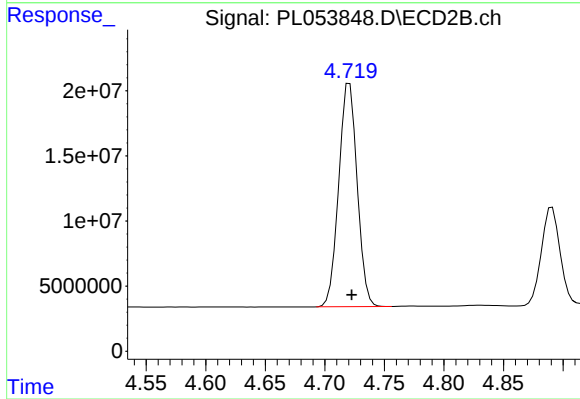


#3 gamma-BHC (Lindane)

R.T.: 4.721 min
Delta R.T.: -0.002 min
Response: 184676023
Conc: 57.35 ng/ml

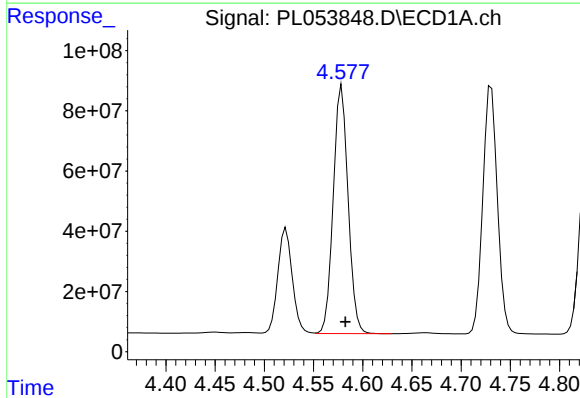


#4 Heptachlor

R.T.: 4.579 min
Delta R.T.: -0.004 min
Response: 863464042
Conc: 54.71 ng/ml

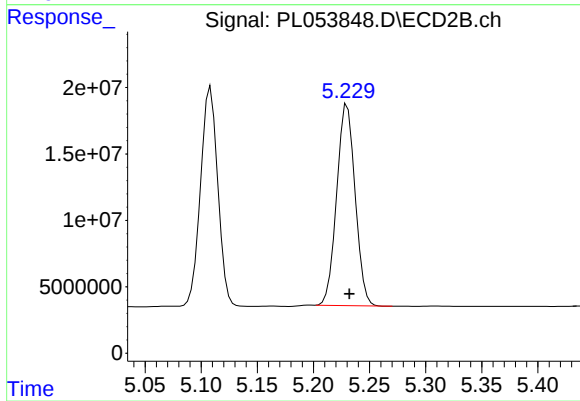

#4 Heptachlor


R.T.: 5.230 min
Delta R.T.: -0.002 min
Response: 173678362
Conc: 53.90 ng/ml

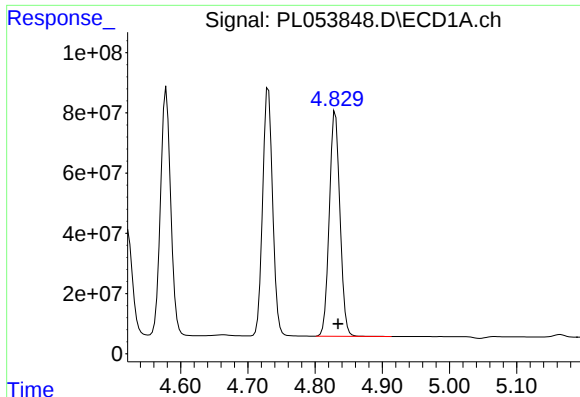

#5 Aldrin


R.T.: 4.830 min
Delta R.T.: -0.004 min
Response: 813772115
Conc: 56.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

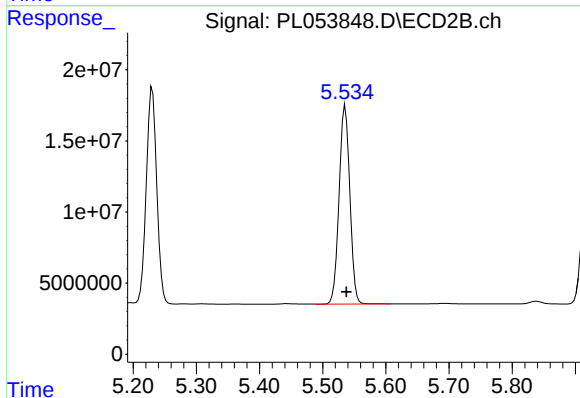


#5 Aldrin

R.T.: 5.536 min
Delta R.T.: -0.002 min
Response: 165193711
Conc: 55.41 ng/ml

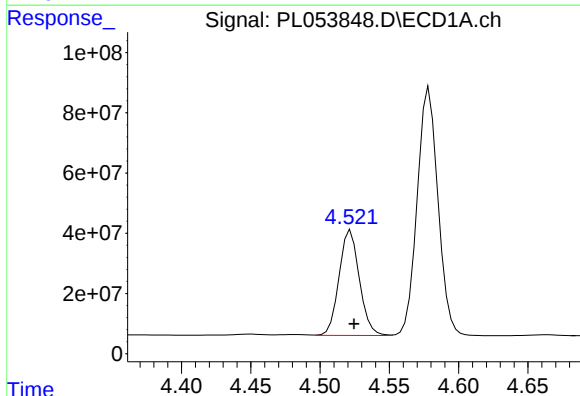


#6 beta-BHC

R.T.: 4.522 min
Delta R.T.: -0.002 min
Response: 357407987
Conc: 54.24 ng/ml

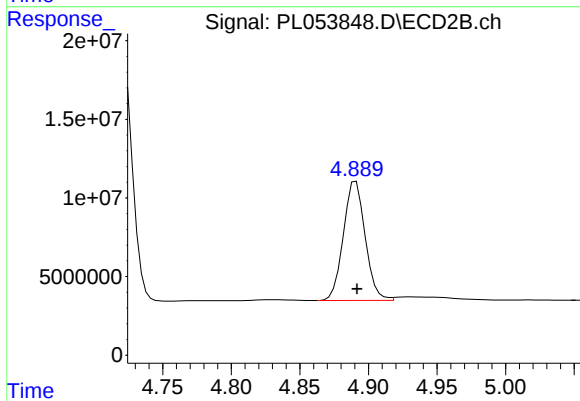

#6 beta-BHC


R.T.: 4.891 min
Delta R.T.: 0.000 min
Response: 83860168
Conc: 54.29 ng/ml

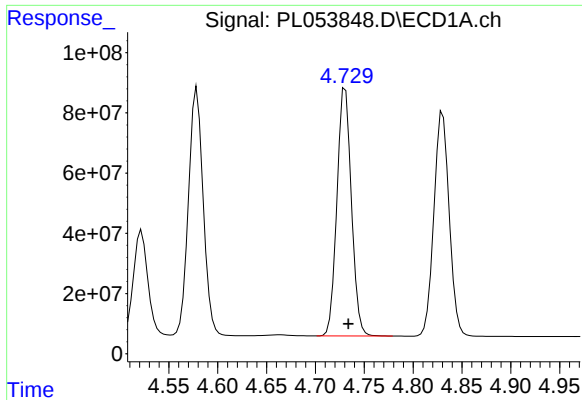

#7 delta-BHC


R.T.: 4.731 min
Delta R.T.: -0.003 min
Response: 849653521
Conc: 55.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

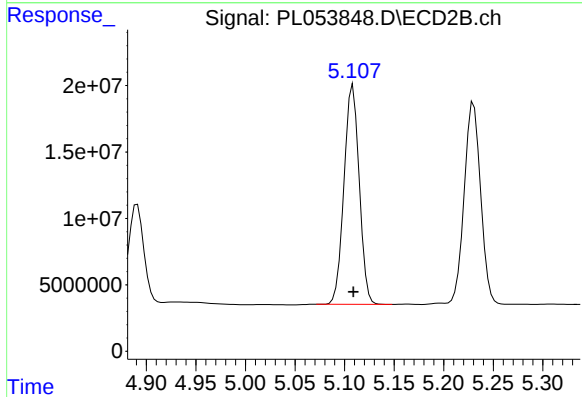


#7 delta-BHC

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 176329234
Conc: 58.38 ng/ml

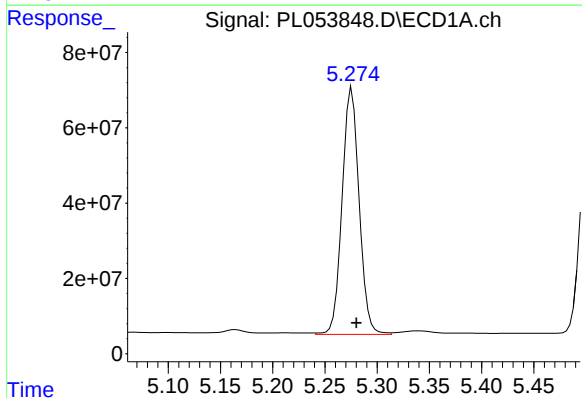


#8 Heptachlor epoxide

R.T.: 5.276 min
Delta R.T.: -0.004 min
Response: 742933021
Conc: 55.04 ng/ml

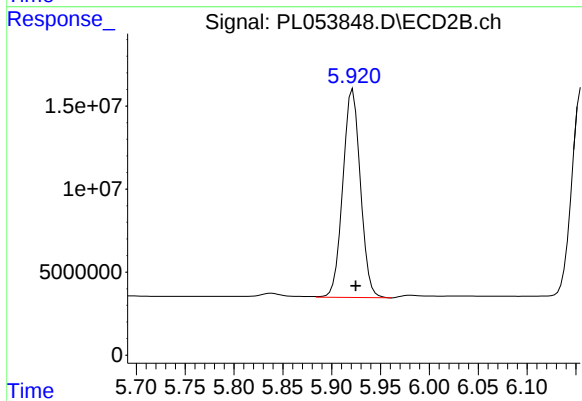

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.003 min
Response: 157047679
Conc: 53.85 ng/ml

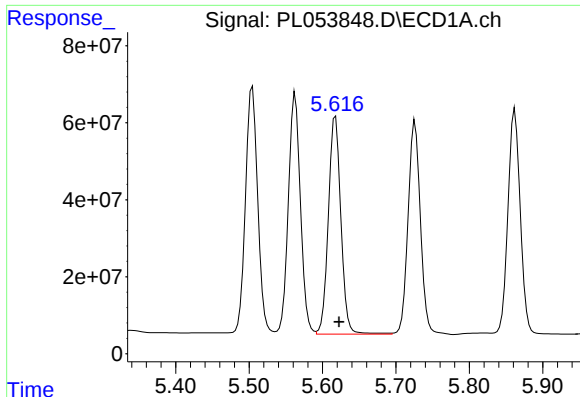

#9 Endosulfan I


R.T.: 5.618 min
Delta R.T.: -0.005 min
Response: 671753277
Conc: 54.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

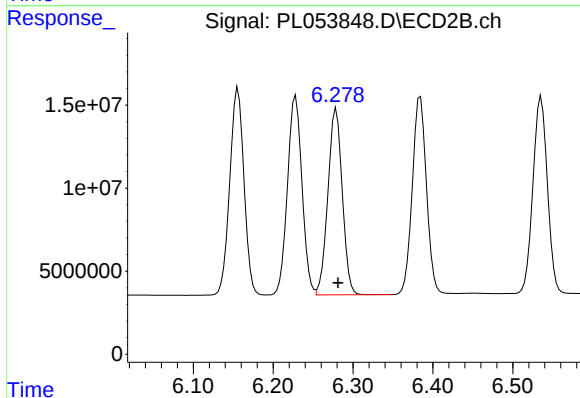


#9 Endosulfan I

R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 139995969
Conc: 51.64 ng/ml

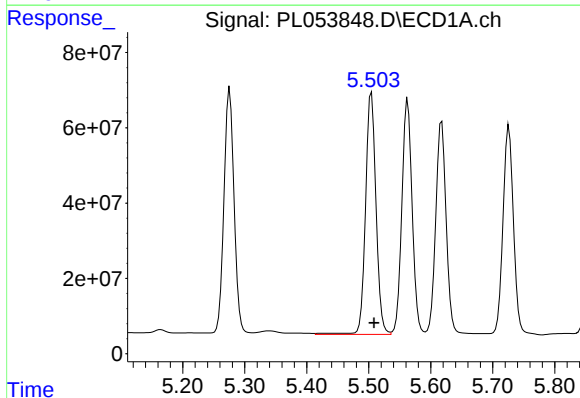


#10 gamma-Chlordane

R.T.: 5.505 min
Delta R.T.: -0.004 min
Response: 757519258
Conc: 55.52 ng/ml

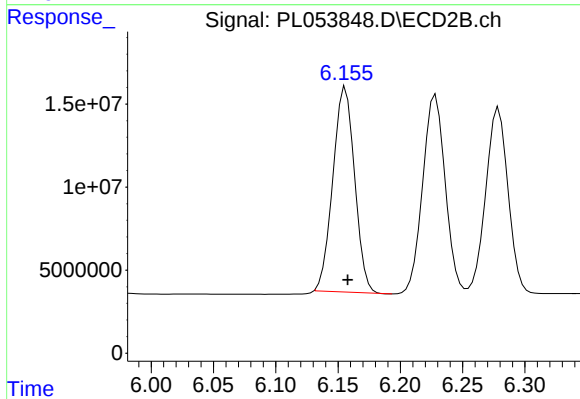

#10 gamma-Chlordane


R.T.: 6.156 min
Delta R.T.: -0.002 min
Response: 149987946
Conc: 51.40 ng/ml

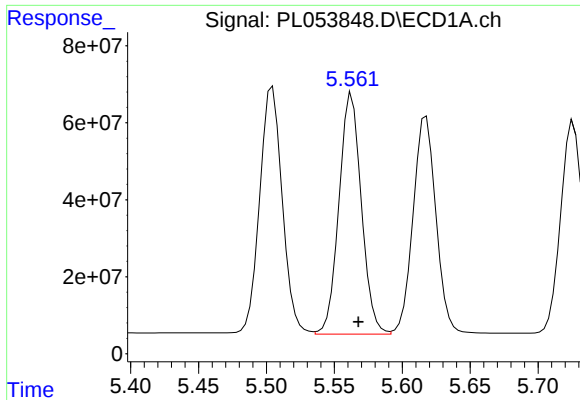

#11 alpha-Chlordane


R.T.: 5.563 min
Delta R.T.: -0.005 min
Response: 717355645
Conc: 53.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

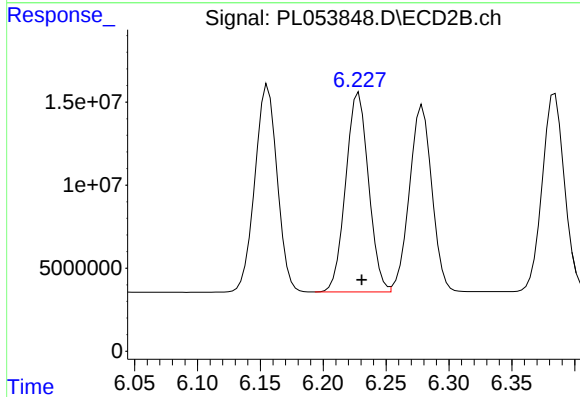


#11 alpha-Chlordane

R.T.: 6.228 min
Delta R.T.: -0.002 min
Response: 151772122
Conc: 51.99 ng/ml

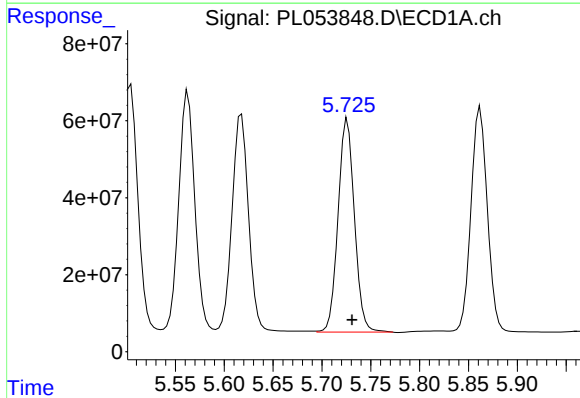


#12 4,4'-DDE

R.T.: 5.726 min
Delta R.T.: -0.005 min
Response: 645880481
Conc: 54.36 ng/ml

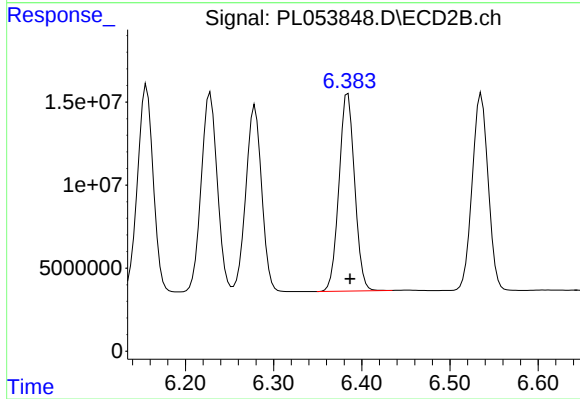

#12 4,4'-DDE


R.T.: 6.384 min
Delta R.T.: -0.003 min
Response: 146655054
Conc: 52.07 ng/ml

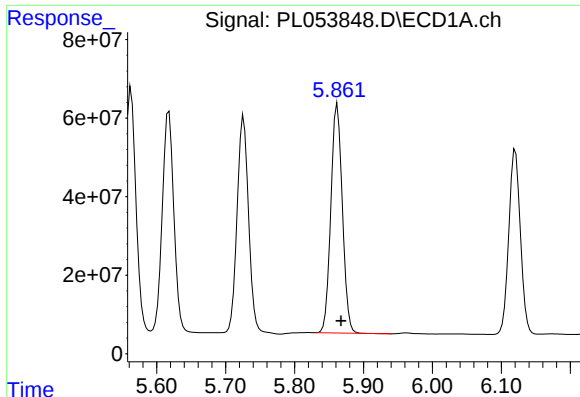

#13 Dieldrin


R.T.: 5.862 min
Delta R.T.: -0.006 min
Response: 674246690
Conc: 51.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

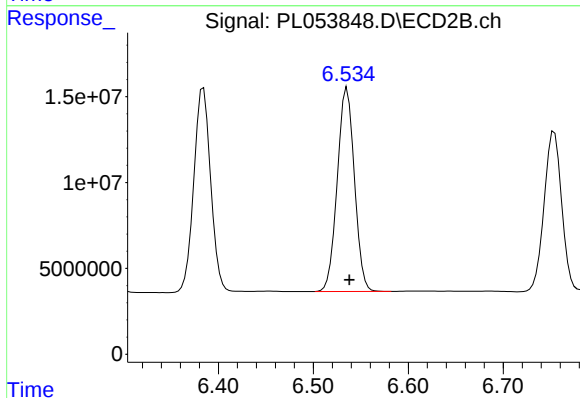


#13 Dieldrin

R.T.: 6.536 min
Delta R.T.: -0.003 min
Response: 149026390
Conc: 52.22 ng/ml

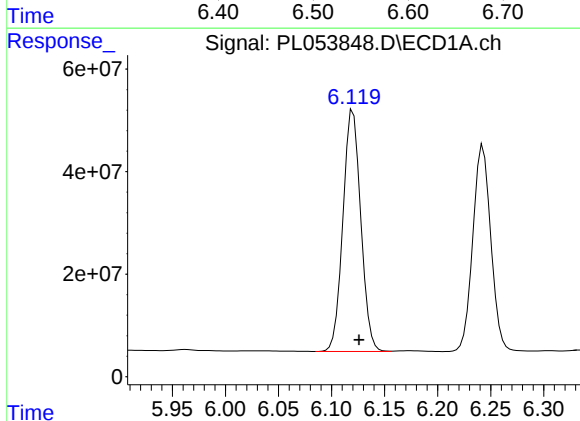


#14 Endrin

R.T.: 6.120 min
Delta R.T.: -0.006 min
Response: 550266178
Conc: 47.47 ng/ml

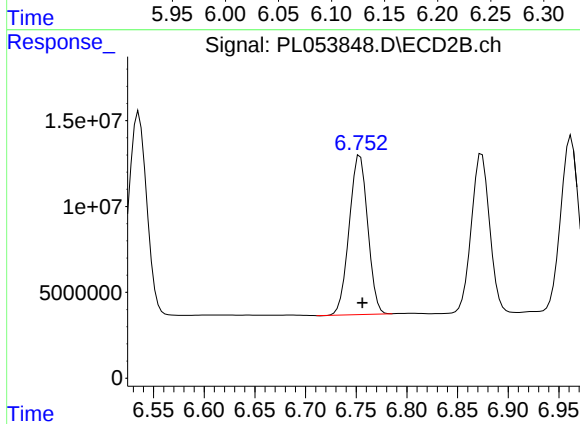

#14 Endrin


R.T.: 6.754 min
Delta R.T.: -0.002 min
Response: 117741583
Conc: 48.51 ng/ml

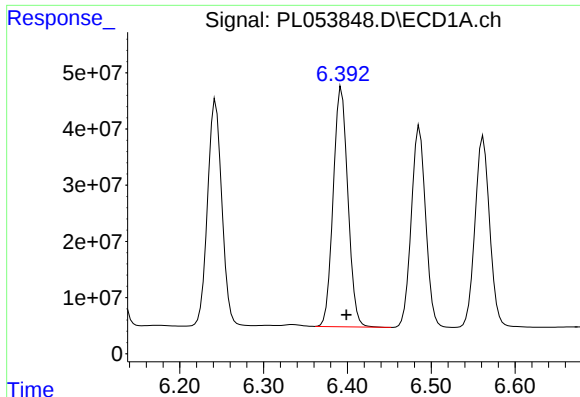

#15 Endosulfan II


R.T.: 6.393 min
Delta R.T.: -0.006 min
Response: 518243931
Conc: 46.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

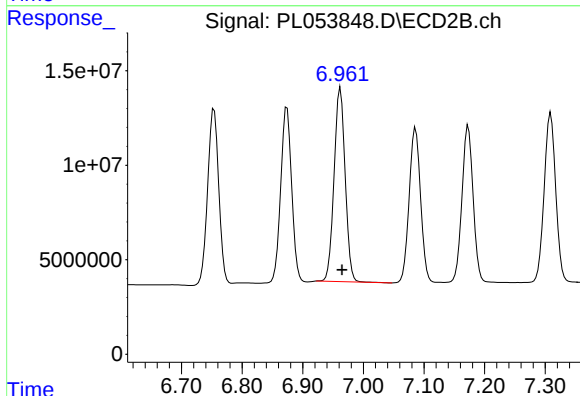


#15 Endosulfan II

R.T.: 6.962 min
Delta R.T.: -0.003 min
Response: 130253619
Conc: 50.99 ng/ml

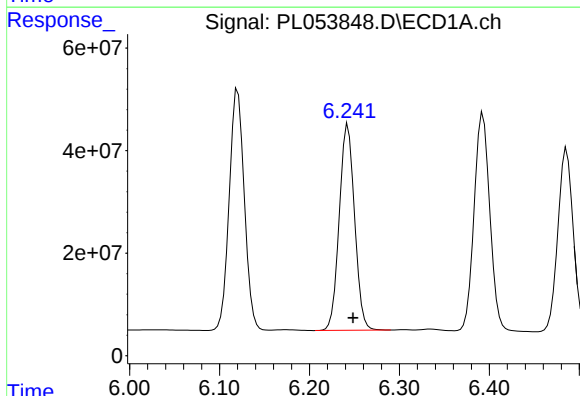


#16 4,4'-DDD

R.T.: 6.243 min
Delta R.T.: -0.006 min
Response: 475697131
Conc: 53.45 ng/ml

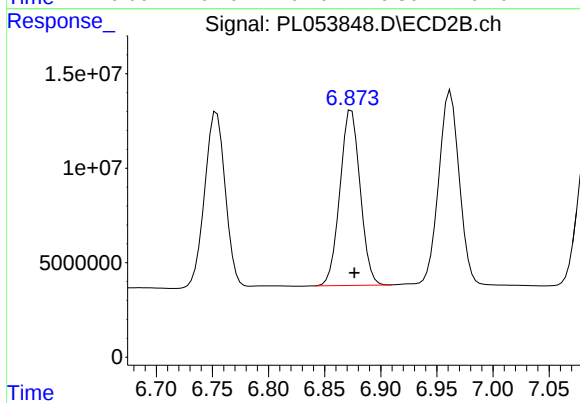

#16 4,4'-DDD


R.T.: 6.874 min
Delta R.T.: -0.003 min
Response: 116303656
Conc: 55.81 ng/ml

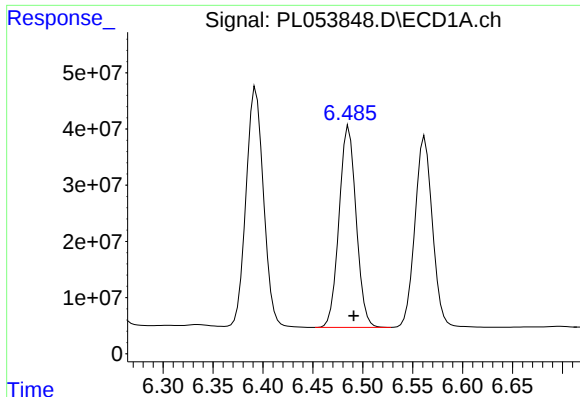

#17 4,4'-DDT


R.T.: 6.486 min
Delta R.T.: -0.005 min
Response: 426635664
Conc: 43.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

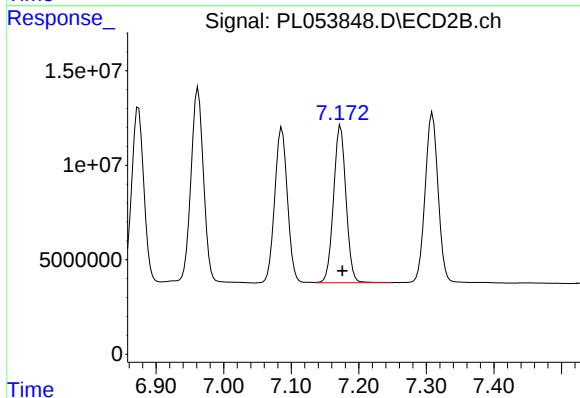


#17 4,4'-DDT

R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 106820737
Conc: 46.19 ng/ml

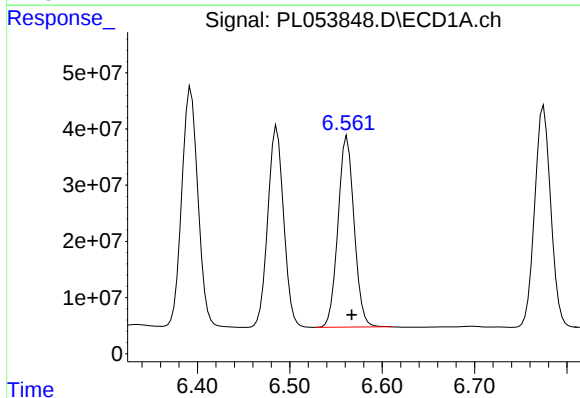


#18 Endrin aldehyde

R.T.: 6.562 min
Delta R.T.: -0.005 min
Response: 412155285
Conc: 44.95 ng/ml

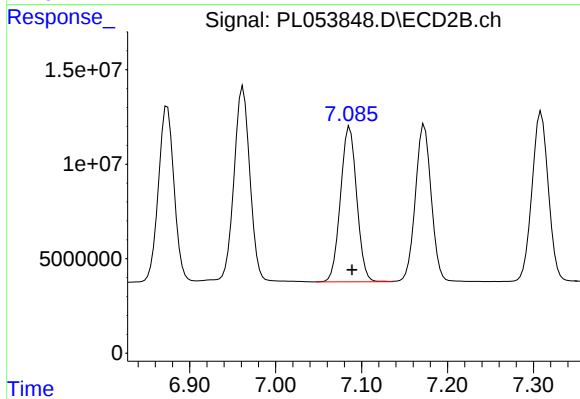

#18 Endrin aldehyde


R.T.: 7.086 min
Delta R.T.: -0.003 min
Response: 107807261
Conc: 49.08 ng/ml

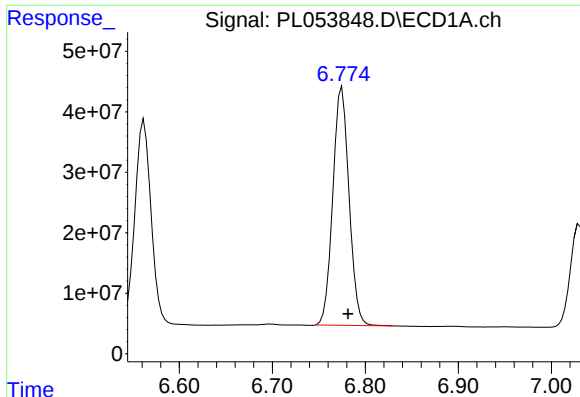

#19 Endosulfan Sulfate


R.T.: 6.775 min
Delta R.T.: -0.006 min
Response: 477914281
Conc: 46.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

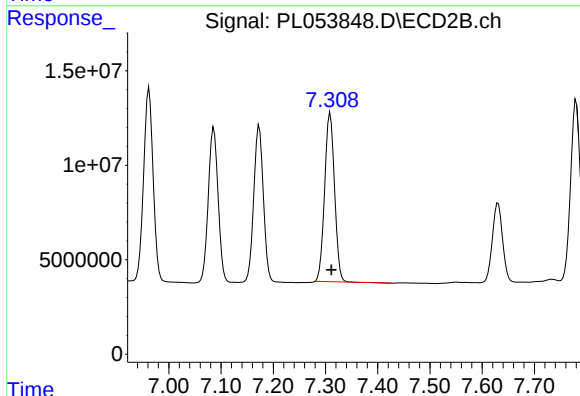


#19 Endosulfan Sulfate

R.T.: 7.309 min
Delta R.T.: -0.002 min
Response: 117329625
Conc: 47.82 ng/ml

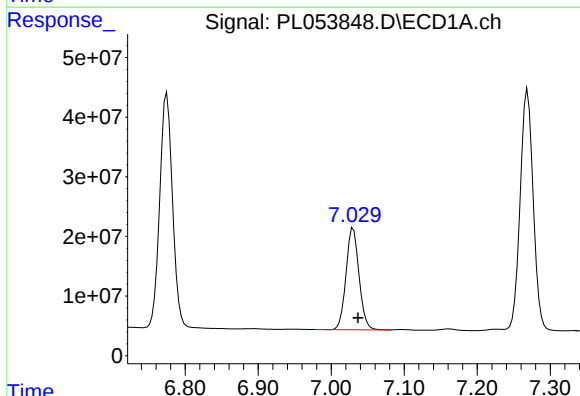


#20 Methoxychlor

R.T.: 7.030 min
Delta R.T.: -0.007 min
Response: 211880770
Conc: 42.97 ng/ml

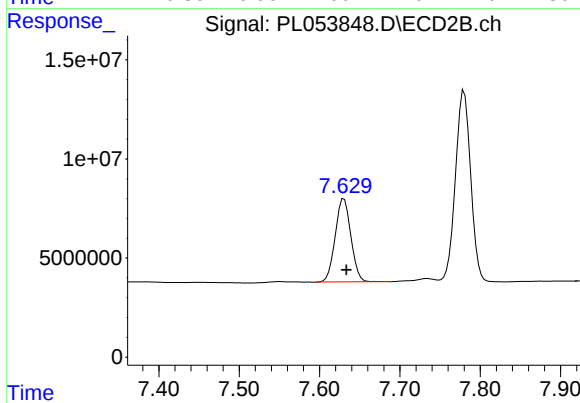

#20 Methoxychlor


R.T.: 7.630 min
Delta R.T.: -0.003 min
Response: 57014205
Conc: 43.89 ng/ml

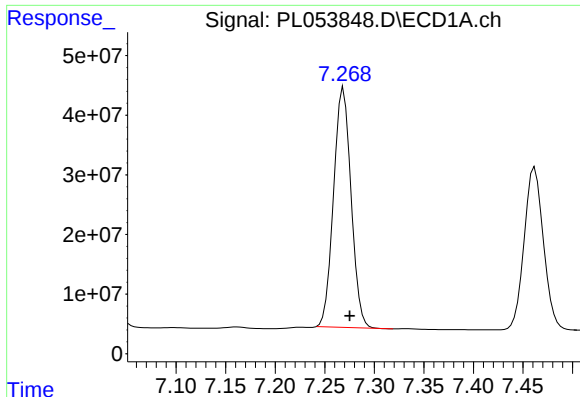

#21 Endrin ketone


R.T.: 7.269 min
Delta R.T.: -0.006 min
Response: 493510880
Conc: 45.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

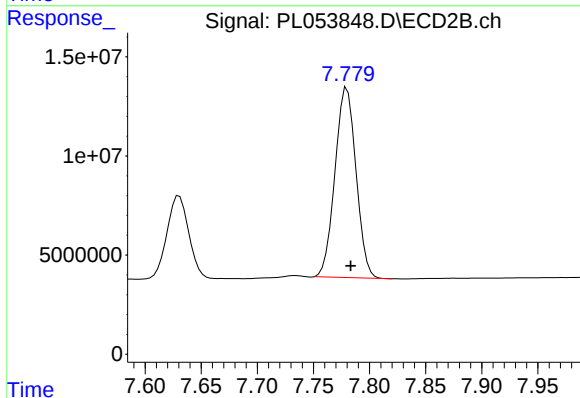


#21 Endrin ketone

R.T.: 7.780 min
Delta R.T.: -0.003 min
Response: 124960657
Conc: 48.46 ng/ml

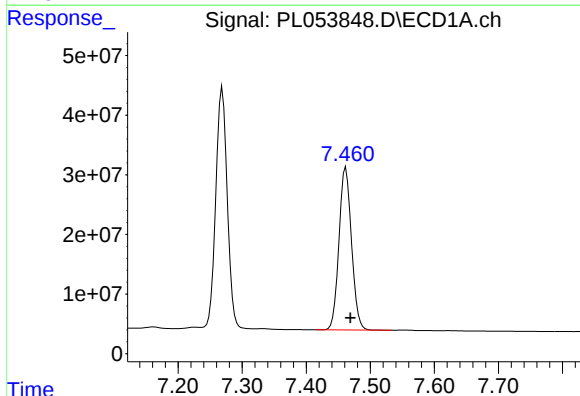


#22 Mirex

R.T.: 7.462 min
Delta R.T.: -0.007 min
Response: 370353867
Conc: 43.30 ng/ml

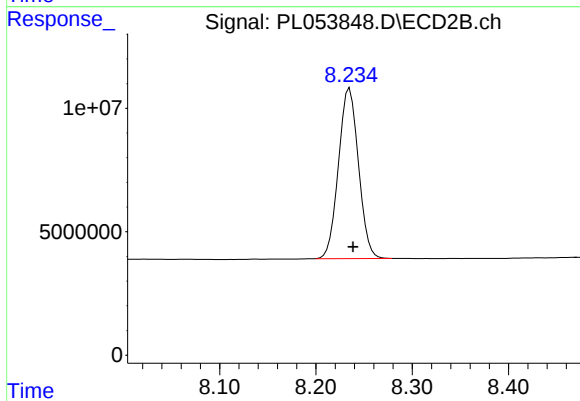

#22 Mirex


R.T.: 8.235 min
Delta R.T.: -0.003 min
Response: 99420301
Conc: 49.14 ng/ml

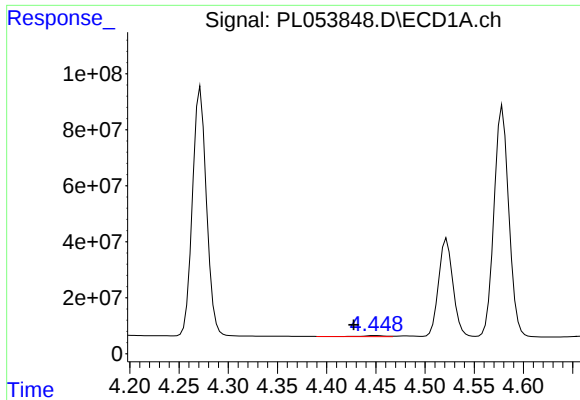

#23 Chlordane-1


R.T.: 4.449 min
Delta R.T.: 0.022 min
Response: 5117157
Conc: 14.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

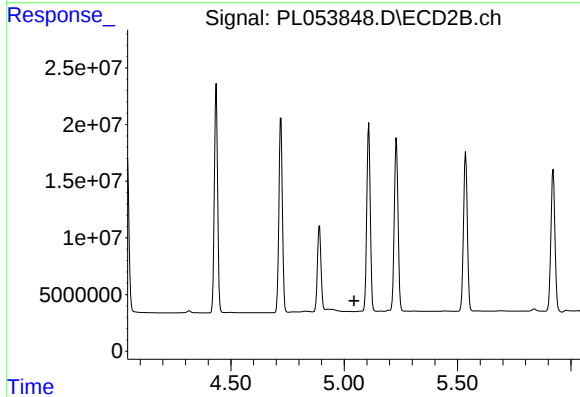


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

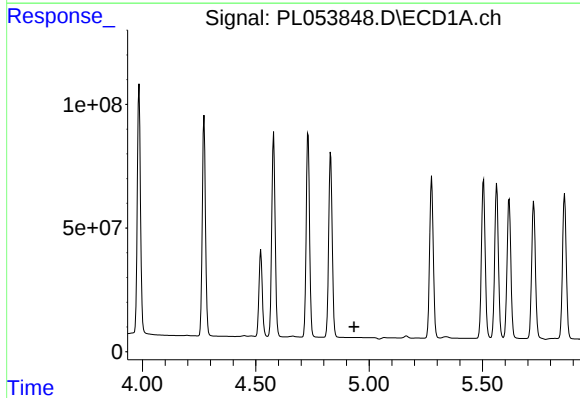


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.934 min
Response: 0
Conc: N.D.

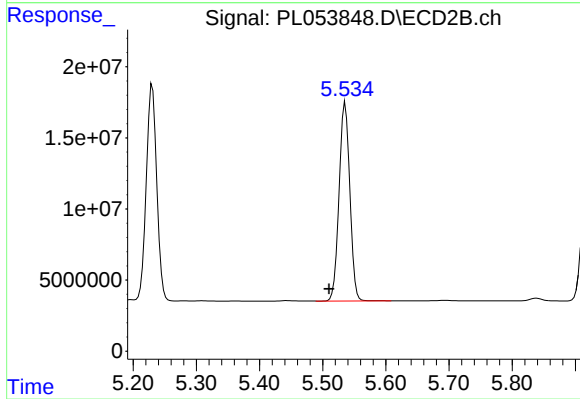

#24 Chlordane-2


R.T.: 5.536 min
Delta R.T.: 0.025 min
Response: 165193711
Conc: 1681.85 ng/ml

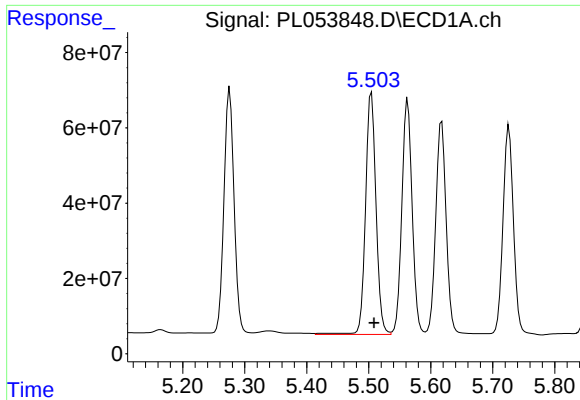

#25 Chlordane-3


R.T.: 5.505 min
Delta R.T.: -0.004 min
Response: 757519258
Conc: 657.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

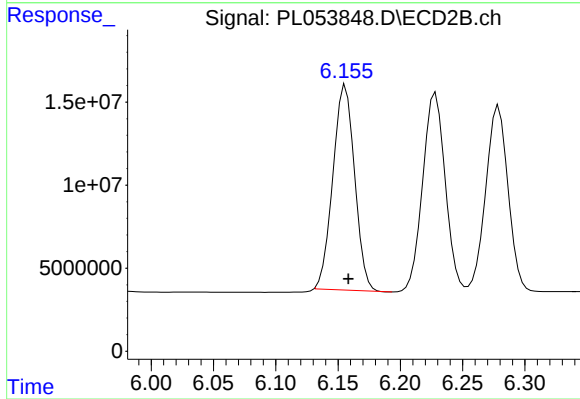


#25 Chlordane-3

R.T.: 6.156 min
Delta R.T.: -0.002 min
Response: 149987946
Conc: 410.67 ng/ml

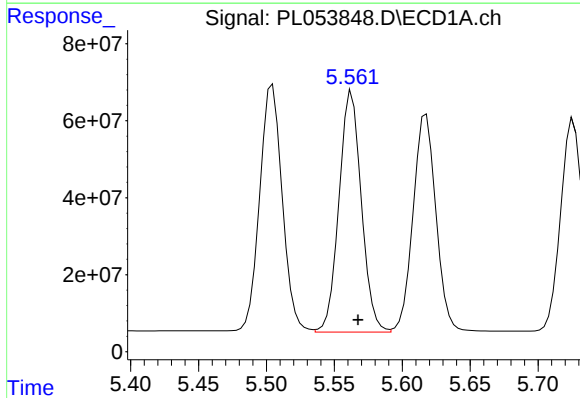


#26 Chlordane-4

R.T.: 5.563 min
Delta R.T.: -0.005 min
Response: 717355645
Conc: 765.22 ng/ml

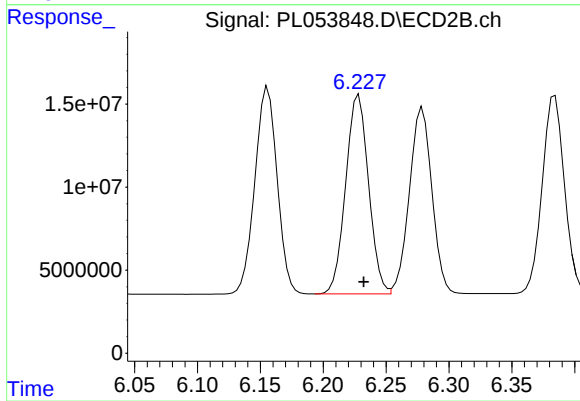

#26 Chlordane-4


R.T.: 6.228 min
Delta R.T.: -0.004 min
Response: 151772122
Conc: 338.07 ng/ml

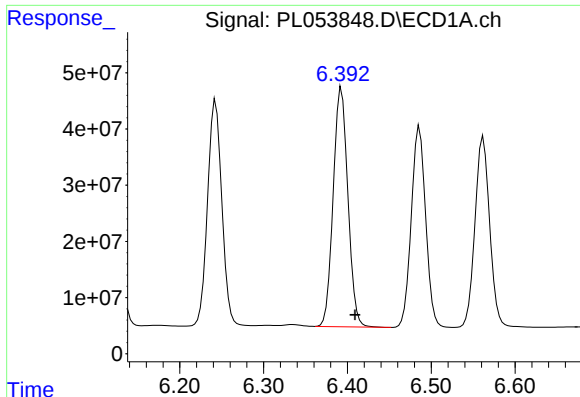

#27 Chlordane-5


R.T.: 6.393 min
Delta R.T.: -0.016 min
Response: 518243931
Conc: 1417.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

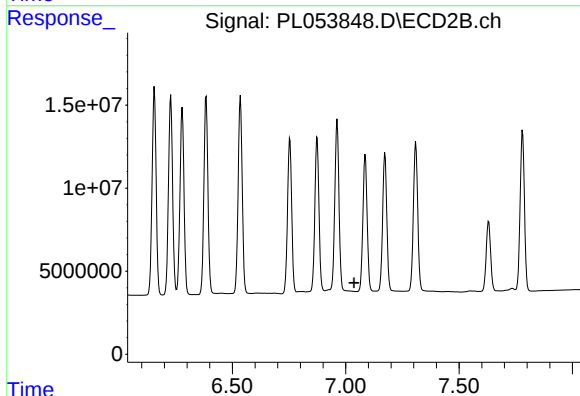


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

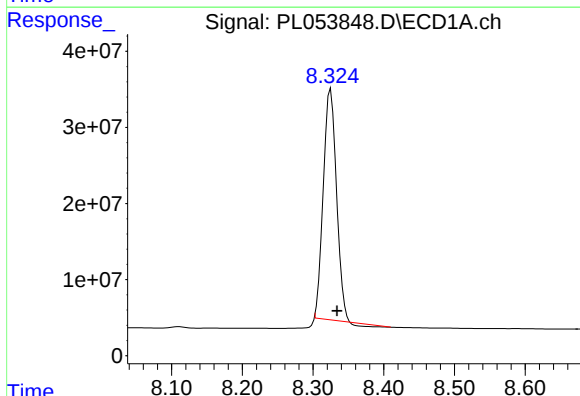

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 386899542
Conc: 39.43 ng/ml

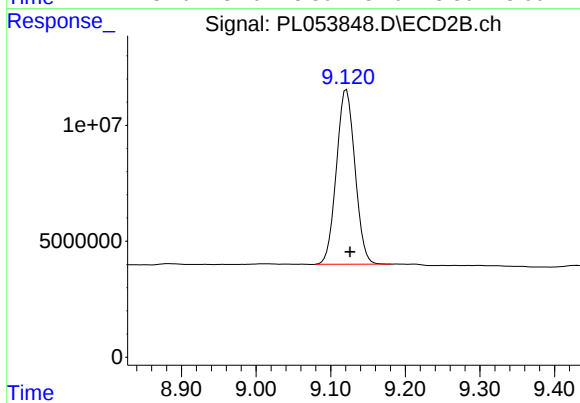

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 130292922
Conc: 46.27 ng/ml