

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102819\
 Data File : PL053849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2019 17:12
 Operator : SG\AJ
 Sample : K5544-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 09:18:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.044	202.4E6	48197435	18.670	19.261
28)	SA Decachlor...	8.328	9.123	127.8E6	41196677	13.021	14.629
Target Compounds							
10)	B gamma-Chl...	5.527f	0.000	3609694	0	0.265	N.D. #
11)	B alpha-Chl...	5.557	0.000	6565839	0	0.494	N.D. #
15)	B Endosulfa...	0.000	6.970	0	2326859	N.D.	0.911 #
23)	Chlordane-1	4.450f	0.000	4984745	0	14.055	N.D. #
25)	Chlordane-3	5.527f	0.000	3609694	0	3.132	N.D. #
26)	Chlordane-4	5.557	0.000	6565839	0	7.004	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102819\
Data File : PL053849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 17:12
Operator : SG\AJ
Sample : K5544-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
N-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 09:18:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

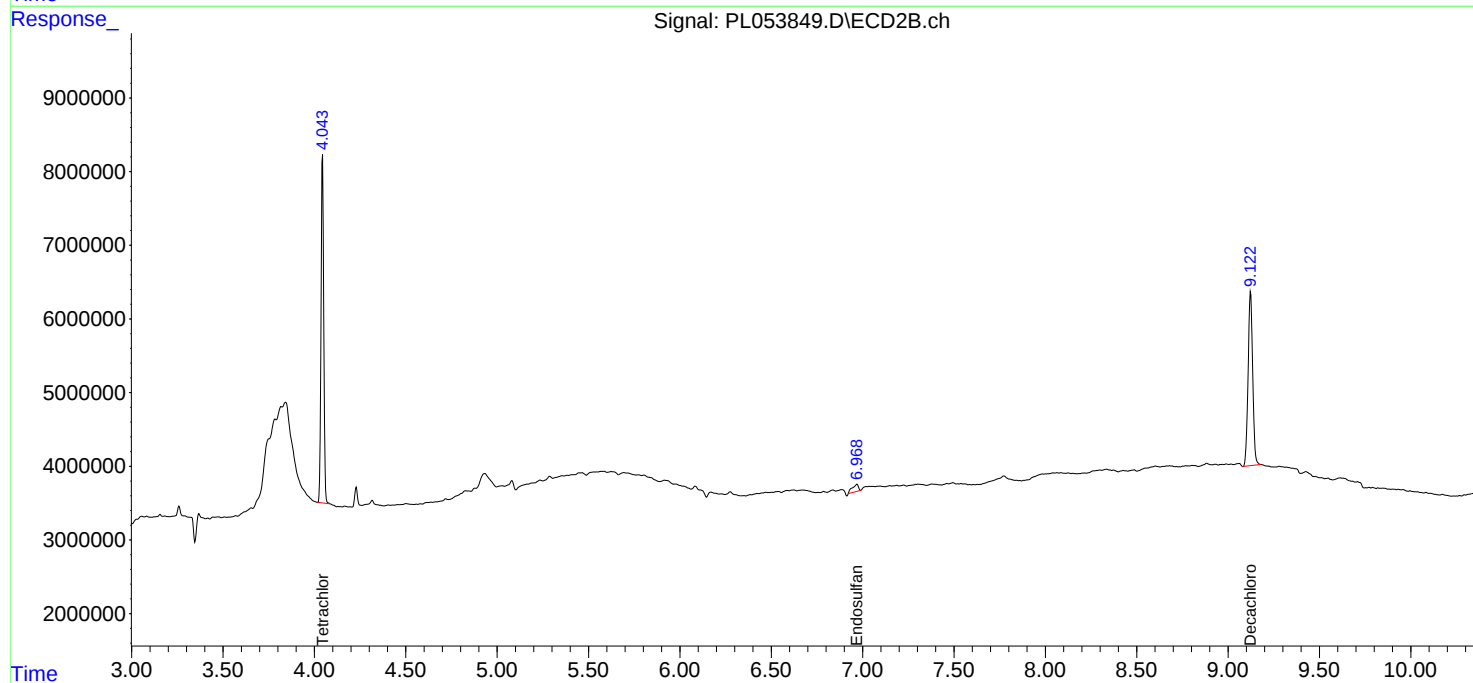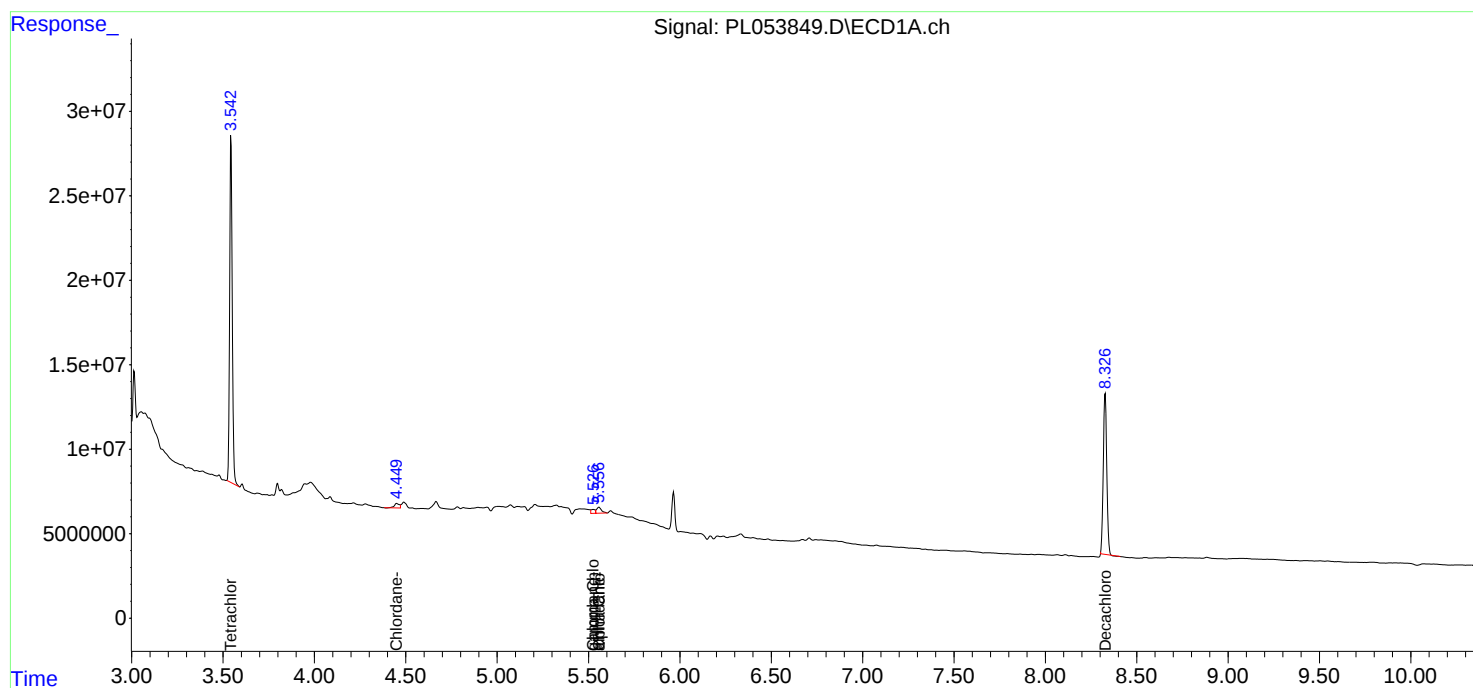


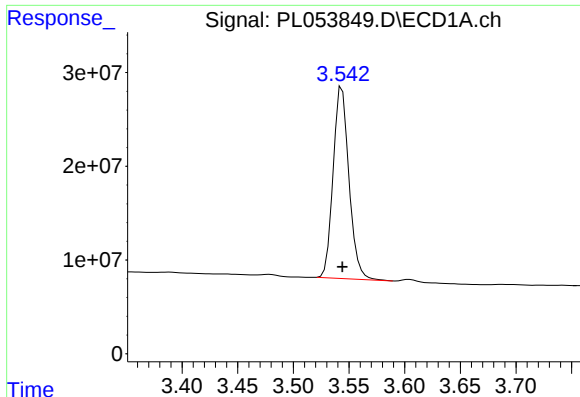

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 202372803
Conc: 18.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
N-1

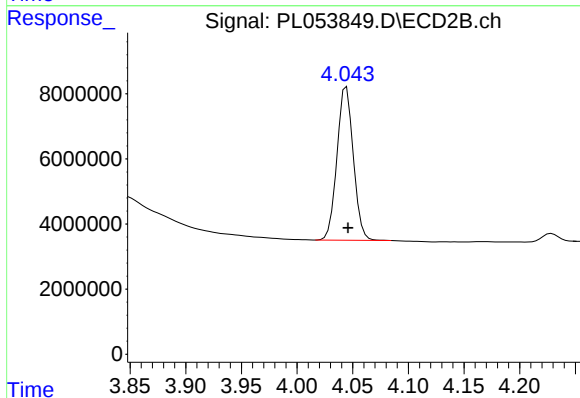


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 48197435
Conc: 19.26 ng/ml

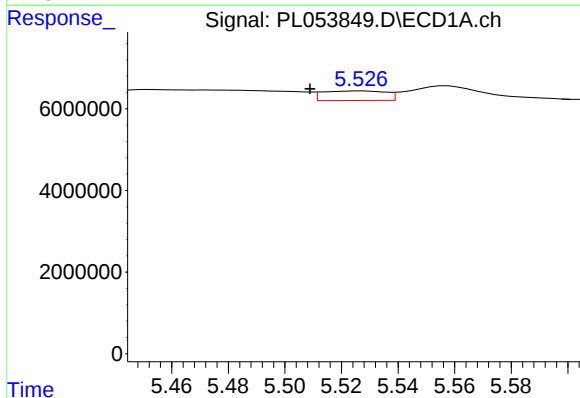


#10 gamma-Chlordane

R.T.: 5.527 min
Delta R.T.: 0.018 min
Response: 3609694
Conc: 0.26 ng/ml

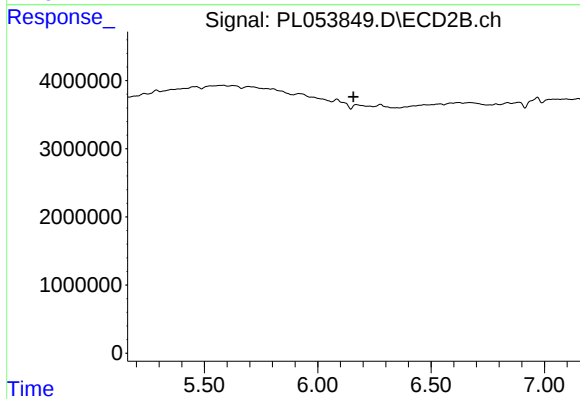

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

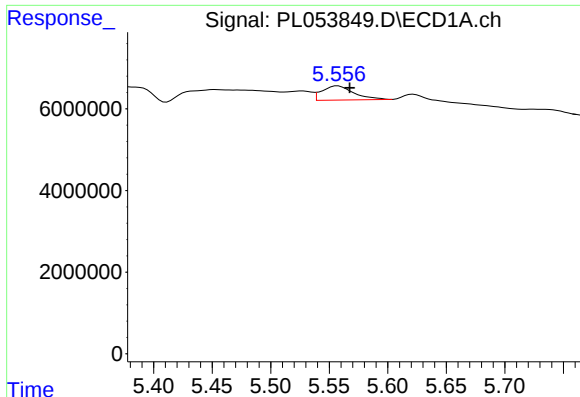

#11 alpha-Chlordane


R.T.: 5.557 min
Delta R.T.: -0.010 min
Response: 6565839
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
N-1

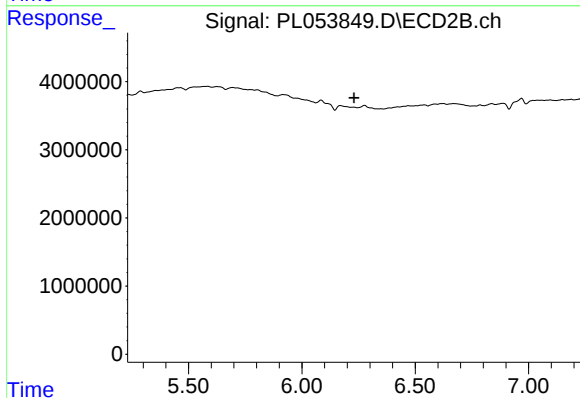


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

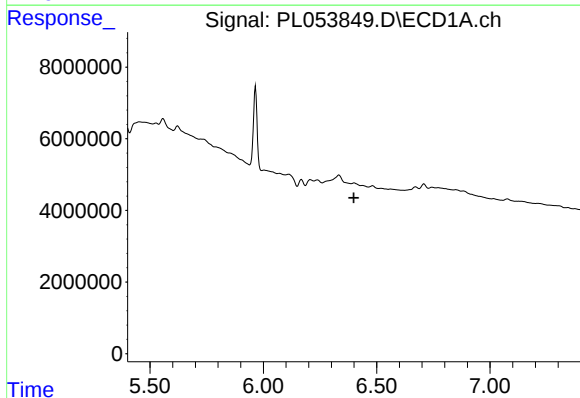


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

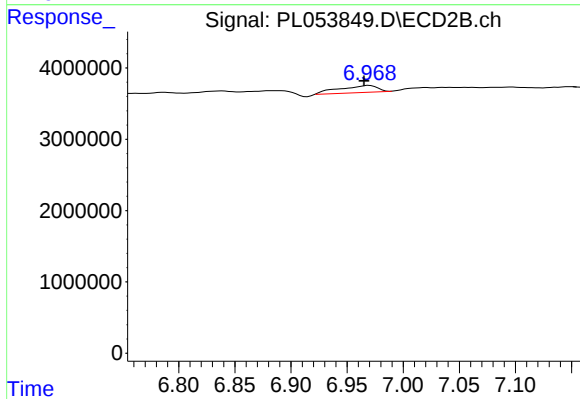

#15 Endosulfan II


R.T.: 6.970 min
Delta R.T.: 0.005 min
Response: 2326859
Conc: 0.91 ng/ml

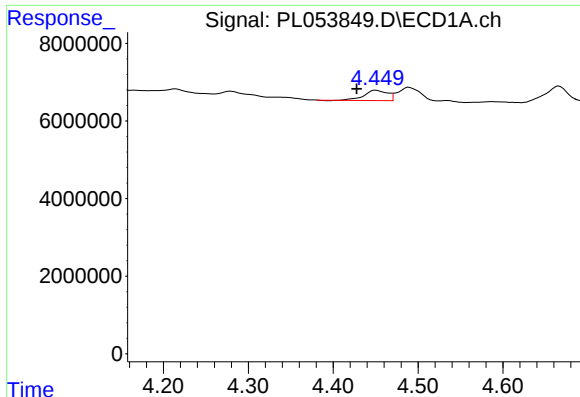

#23 Chlordane-1


R.T.: 4.450 min
Delta R.T.: 0.023 min
Response: 4984745
Conc: 14.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
N-1

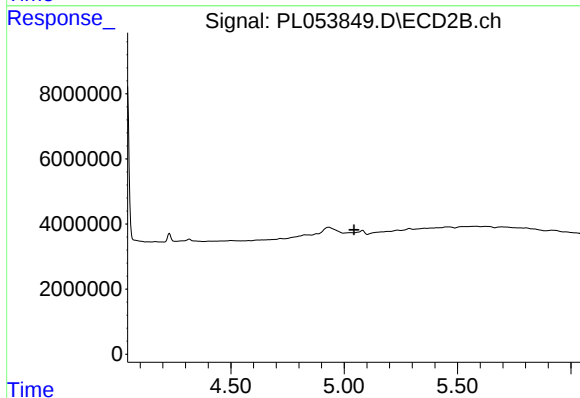


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

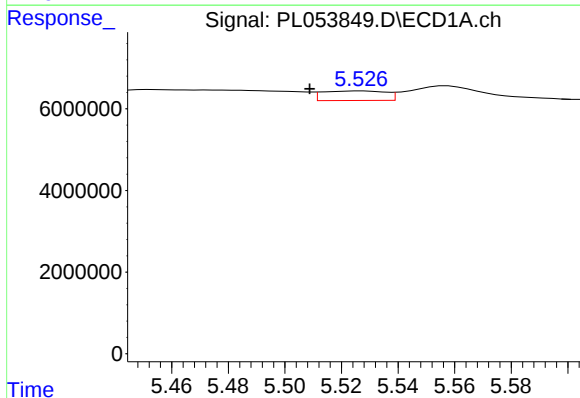


#25 Chlordane-3

R.T.: 5.527 min
Delta R.T.: 0.018 min
Response: 3609694
Conc: 3.13 ng/ml

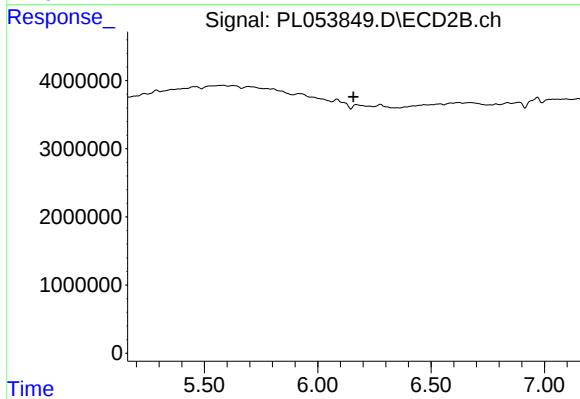

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

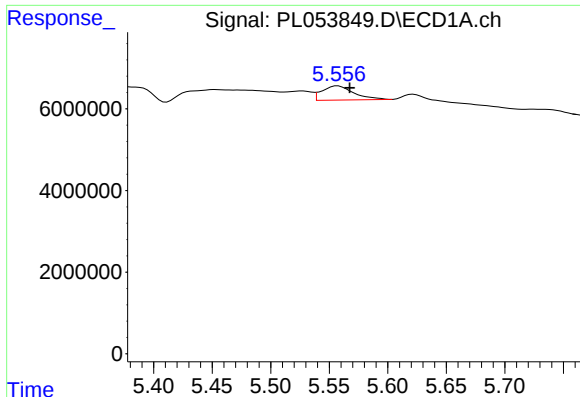

#26 Chlordane-4


R.T.: 5.557 min
Delta R.T.: -0.010 min
Response: 6565839
Conc: 7.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
N-1

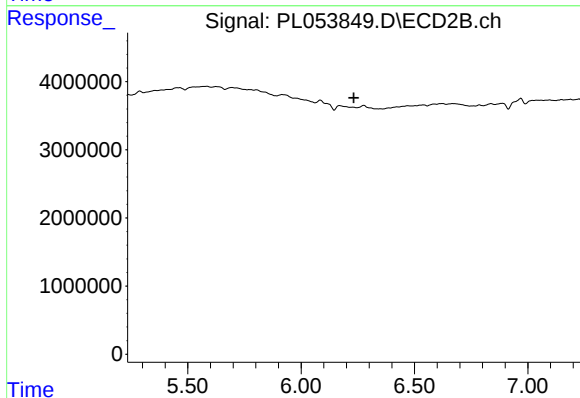


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.232 min
Response: 0
Conc: N.D.

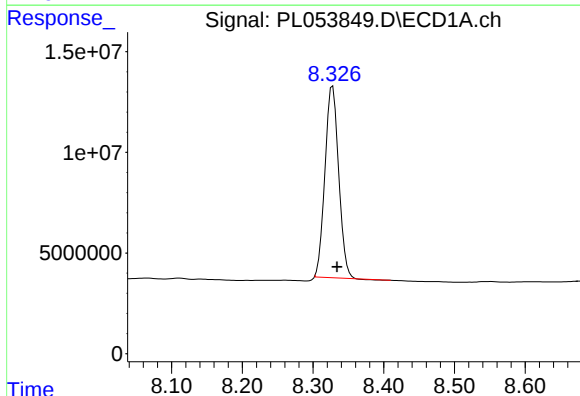

#28 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: -0.006 min
Response: 127758928
Conc: 13.02 ng/ml

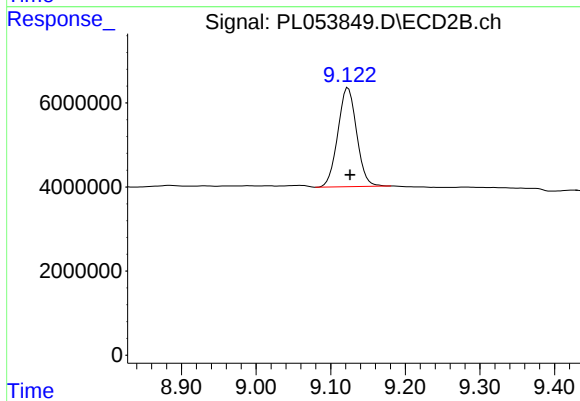

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 41196677
Conc: 14.63 ng/ml