

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102820\
 Data File : PL062660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 17:51
 Operator : DD\AJ
 Sample : L4537-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 06:33:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	22972623	37128168	13.356	12.634
28)	SA Decachlor...	8.127	8.991	18085694	24581635	11.273	11.745
Target Compounds							
5)	MB Aldrin	4.660	0.000	1513127	0	0.793	N.D. #
6)	B beta-BHC	0.000	4.818f	0	1596988	N.D.	0.848 #
8)	B Heptachlo...	0.000	5.828	0	3987118	N.D.	1.231 #
9)	A Endosulfan I	5.451	0.000	1511219	0	0.904	N.D. #
10)	B gamma-Chl...	0.000	6.048	0	2987359	N.D.	0.887 #
11)	B alpha-Chl...	0.000	6.099f	0	4361406	N.D.	1.295 #
23)	Chlordane-1	4.266	0.000	2160709	0	41.915	N.D. #
24)	Chlordane-2	0.000	5.397	0	363919	N.D.	3.338 #
25)	Chlordane-3	0.000	6.048	0	2987359	N.D.	7.396 #
26)	Chlordane-4	0.000	6.099f	0	4361406	N.D.	9.006 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102820\
Data File : PL062660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 17:51
Operator : DD\AJ
Sample : L4537-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 06:33:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

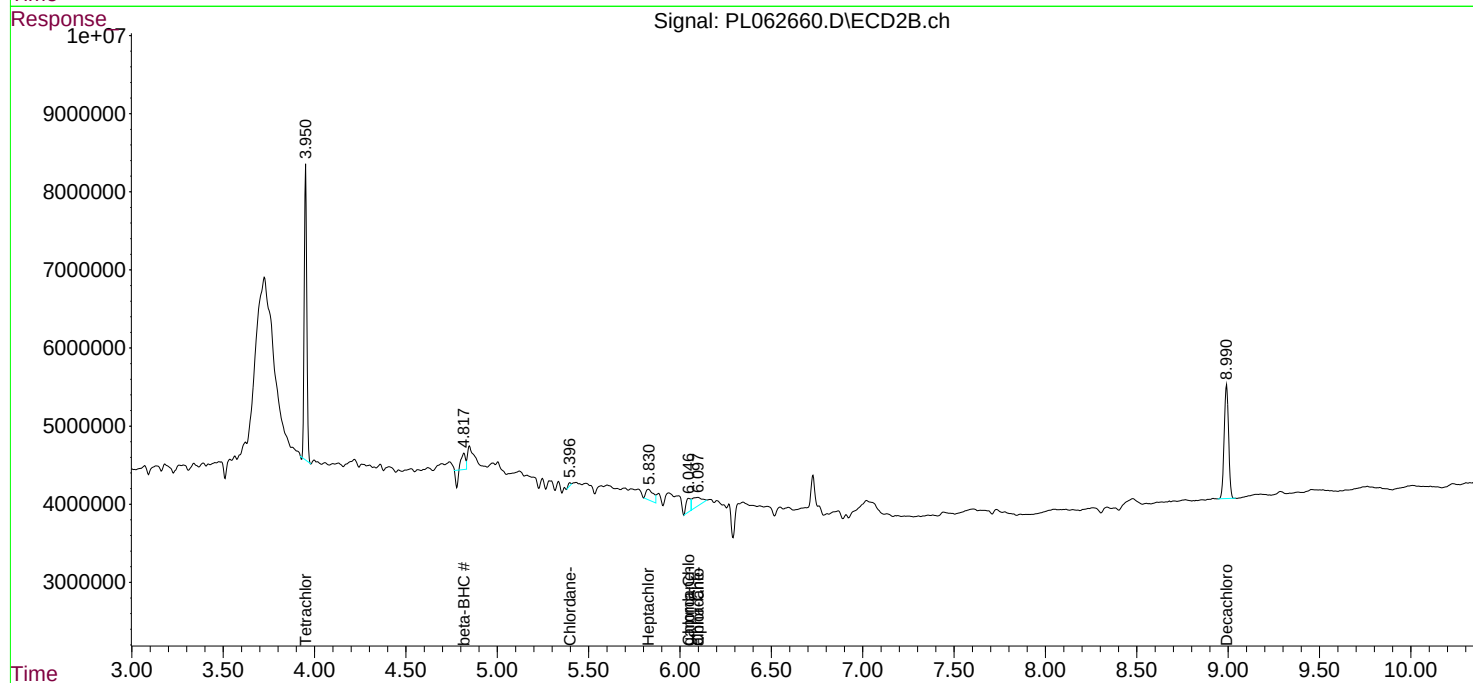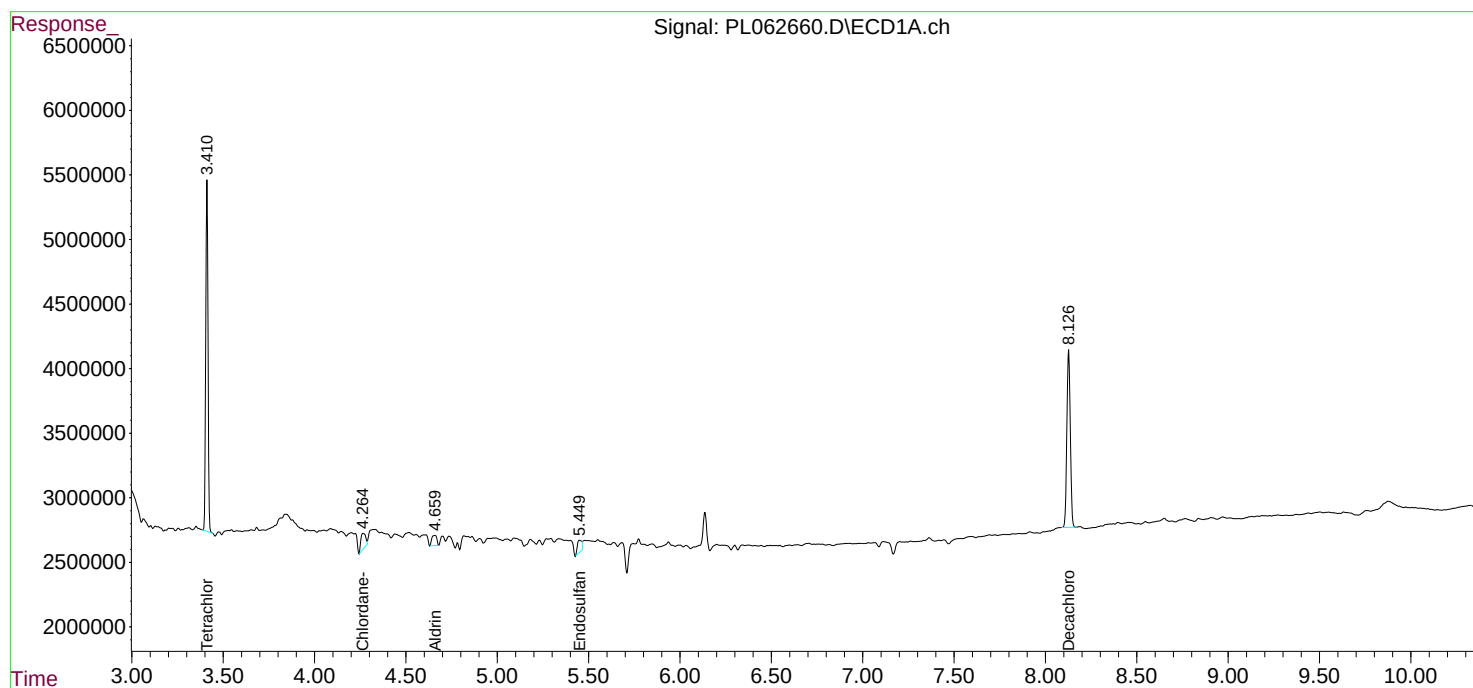


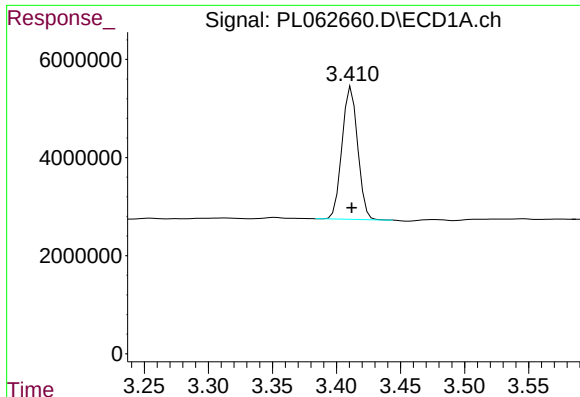

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 22972623
Conc: 13.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

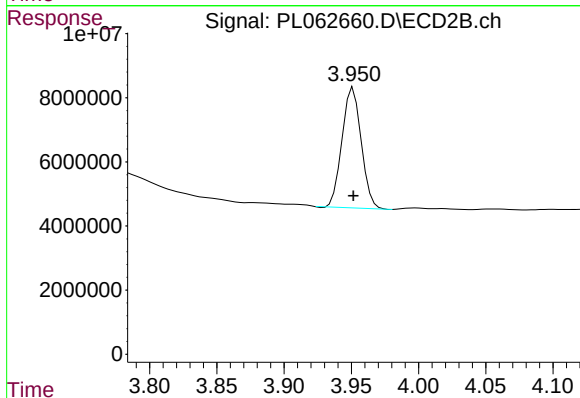


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 37128168
Conc: 12.63 ng/ml

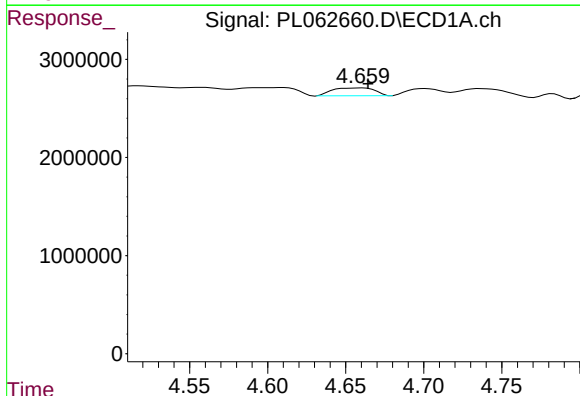


#5 Aldrin

R.T.: 4.660 min
Delta R.T.: -0.004 min
Response: 1513127
Conc: 0.79 ng/ml

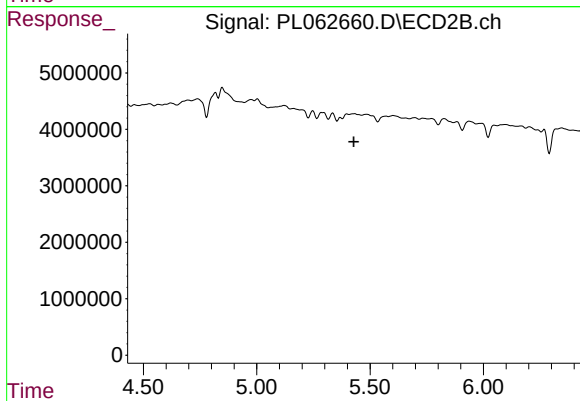

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.429 min
Response: 0
Conc: N.D.

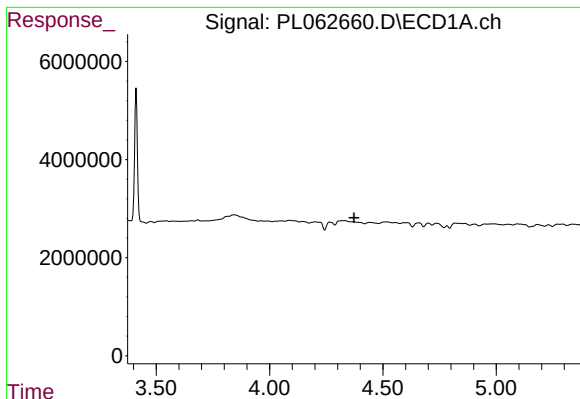

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

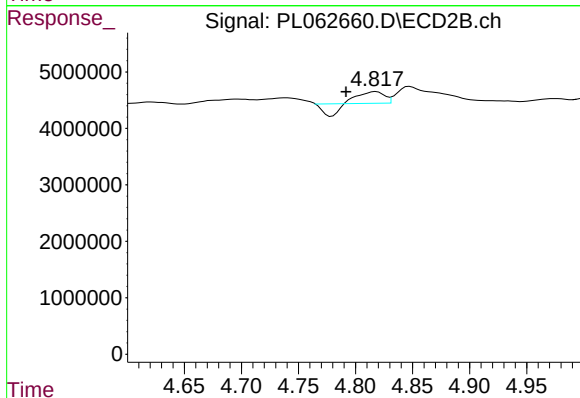


#6 beta-BHC

R.T.: 4.818 min
Delta R.T.: 0.026 min
Response: 1596988
Conc: 0.85 ng/ml

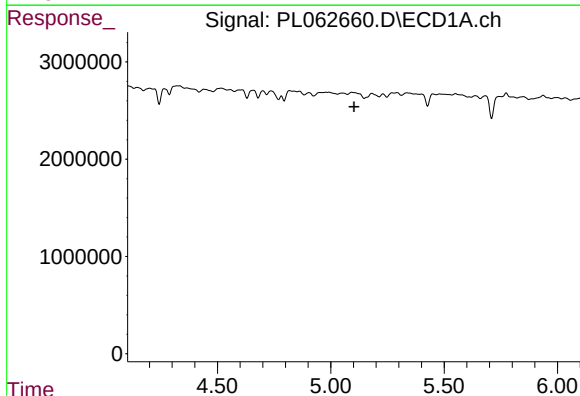


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

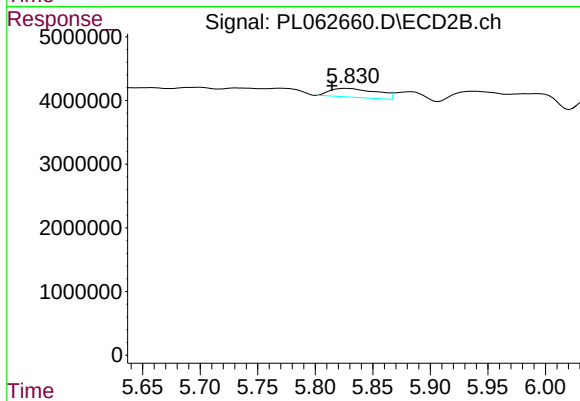

#8 Heptachlor epoxide


R.T.: 5.828 min
Delta R.T.: 0.013 min
Response: 3987118
Conc: 1.23 ng/ml

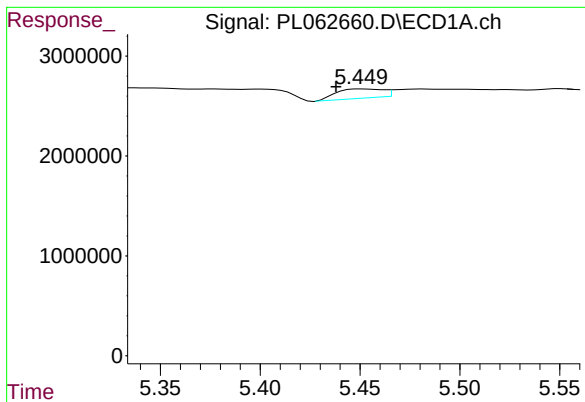

#9 Endosulfan I


R.T.: 5.451 min
Delta R.T.: 0.013 min
Response: 1511219
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

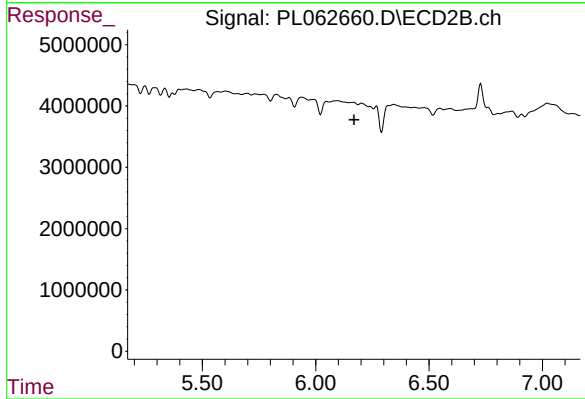


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

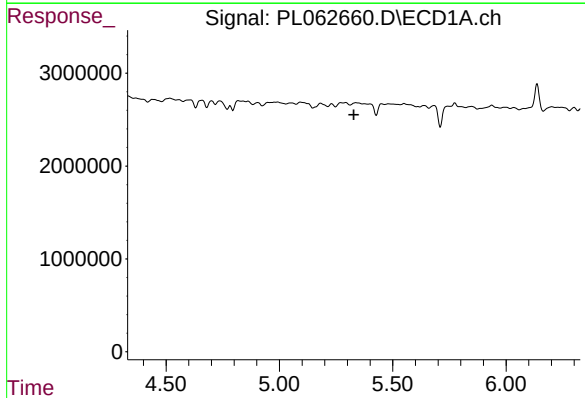


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

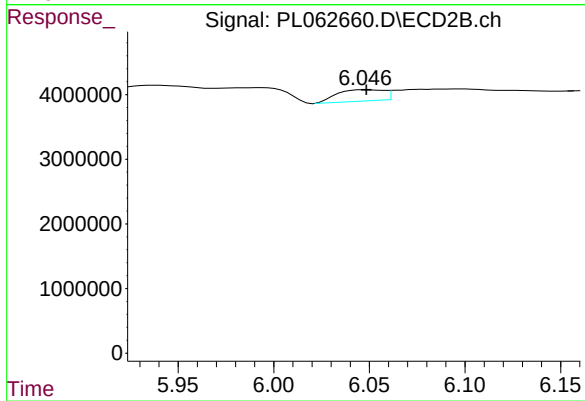

#10 gamma-Chlordane


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 2987359
Conc: 0.89 ng/ml

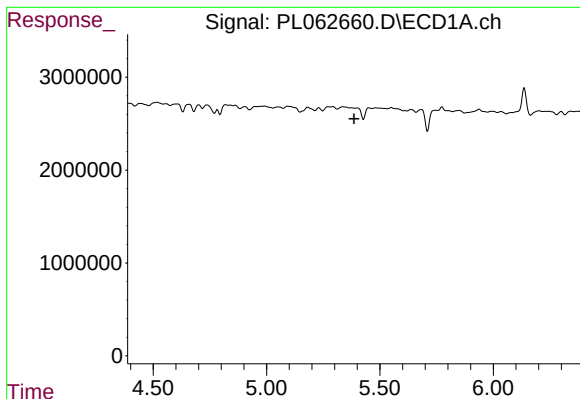

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

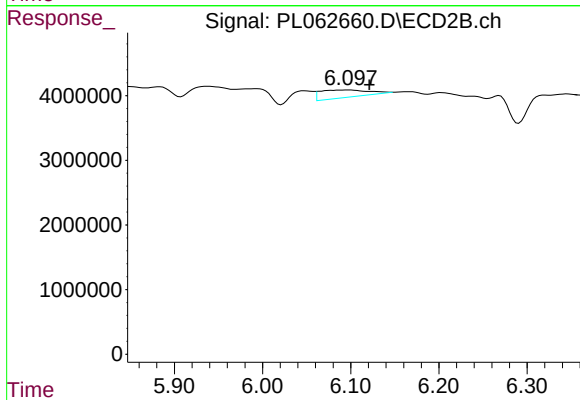


#11 alpha-Chlordane

R.T.: 6.099 min
Delta R.T.: -0.022 min
Response: 4361406
Conc: 1.29 ng/ml

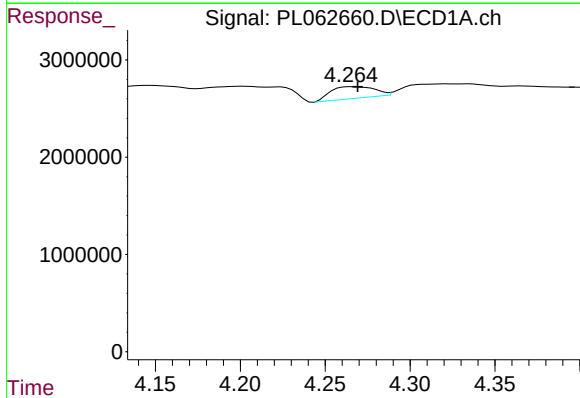


#23 Chlordane-1

R.T.: 4.266 min
Delta R.T.: -0.004 min
Response: 2160709
Conc: 41.91 ng/ml

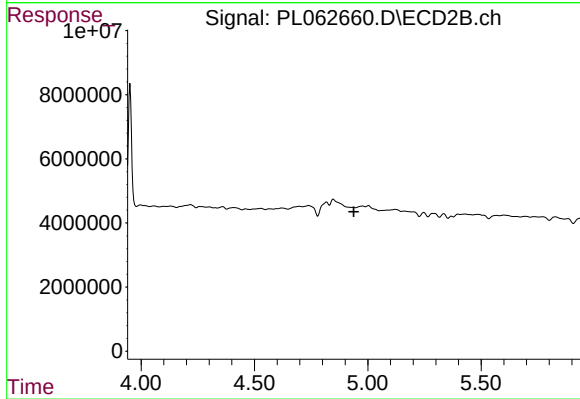

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.938 min
Response: 0
Conc: N.D.

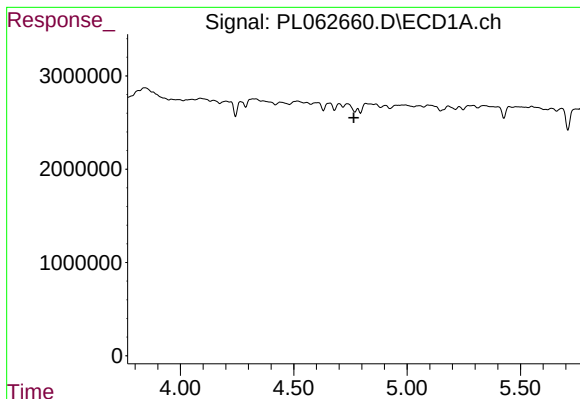

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

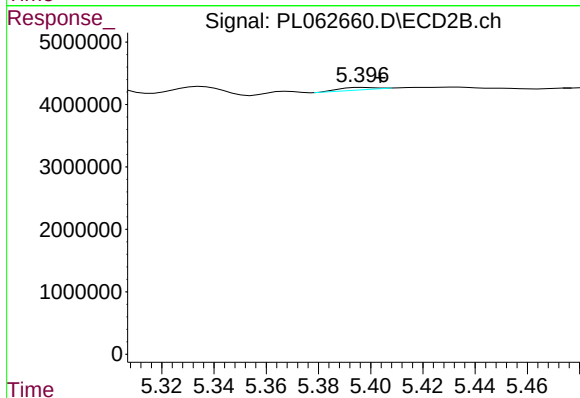


#24 Chlordane-2

R.T.: 5.397 min
Delta R.T.: -0.006 min
Response: 363919
Conc: 3.34 ng/ml

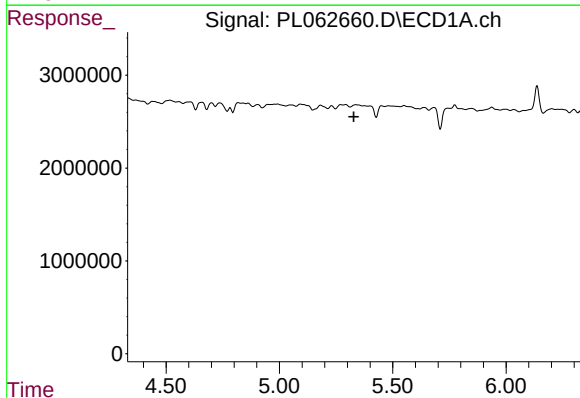


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

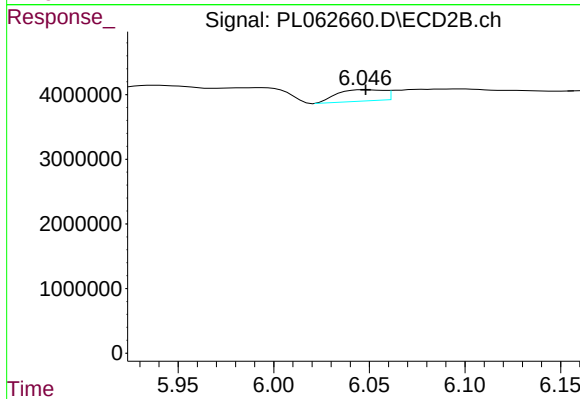

#25 Chlordane-3


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 2987359
Conc: 7.40 ng/ml

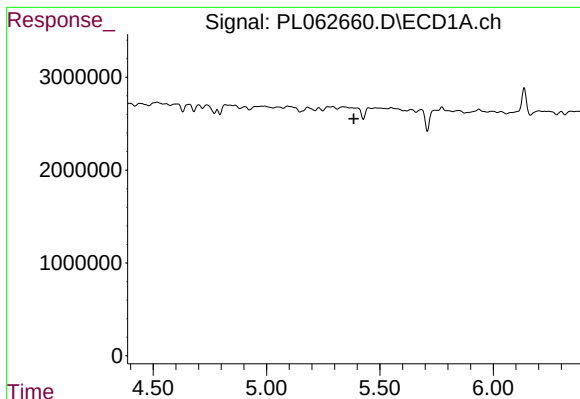

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

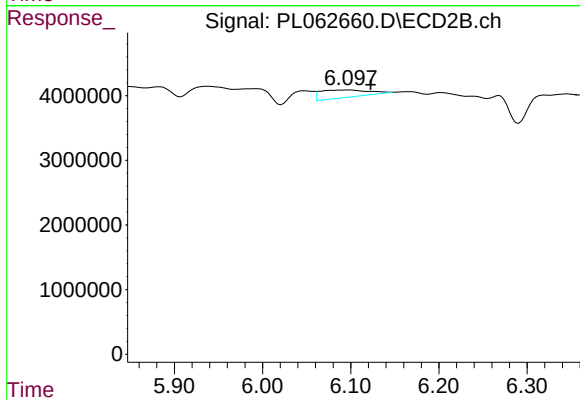


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: -0.024 min
Response: 4361406
Conc: 9.01 ng/ml

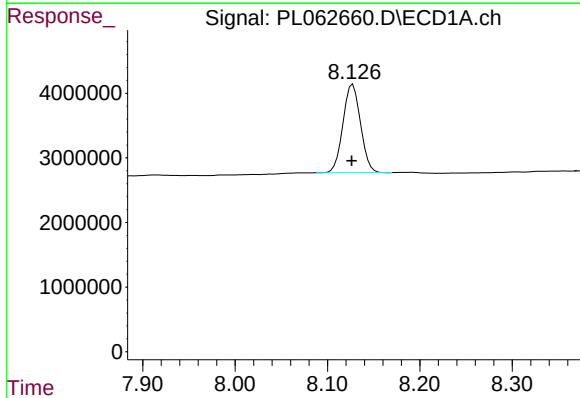

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.001 min
Response: 18085694
Conc: 11.27 ng/ml

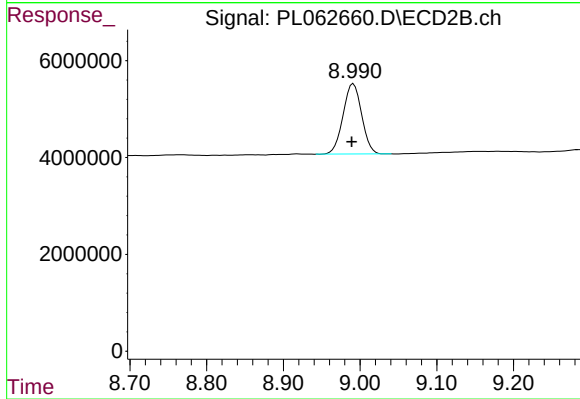

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 24581635
Conc: 11.74 ng/ml