

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102820\
 Data File : PL062674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 21:10
 Operator : DD\AJ
 Sample : L4527-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 06:37:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	29569546	51337940	17.191	17.470
28)	SA Decachlor...	8.128	8.992	33346629	46598649	20.786	22.264
Target Compounds							
3)	MA gamma-BHC...	0.000	4.597f	0	1780266	N.D.	0.426 #
7)	B delta-BHC	0.000	4.983f	0	997741	N.D.	0.285 #
8)	B Heptachlo...	5.082f	0.000	3650954	0	2.001	N.D. #
15)	B Endosulfa...	0.000	6.870f	0	3238601	N.D.	1.133 #
19)	B Endosulfa...	6.606f	0.000	2418421	0	1.465	N.D. #
23)	Chlordane-1	4.281	0.000	2869016	0	55.655	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102820\
Data File : PL062674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 21:10
Operator : DD\AJ
Sample : L4527-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 06:37:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

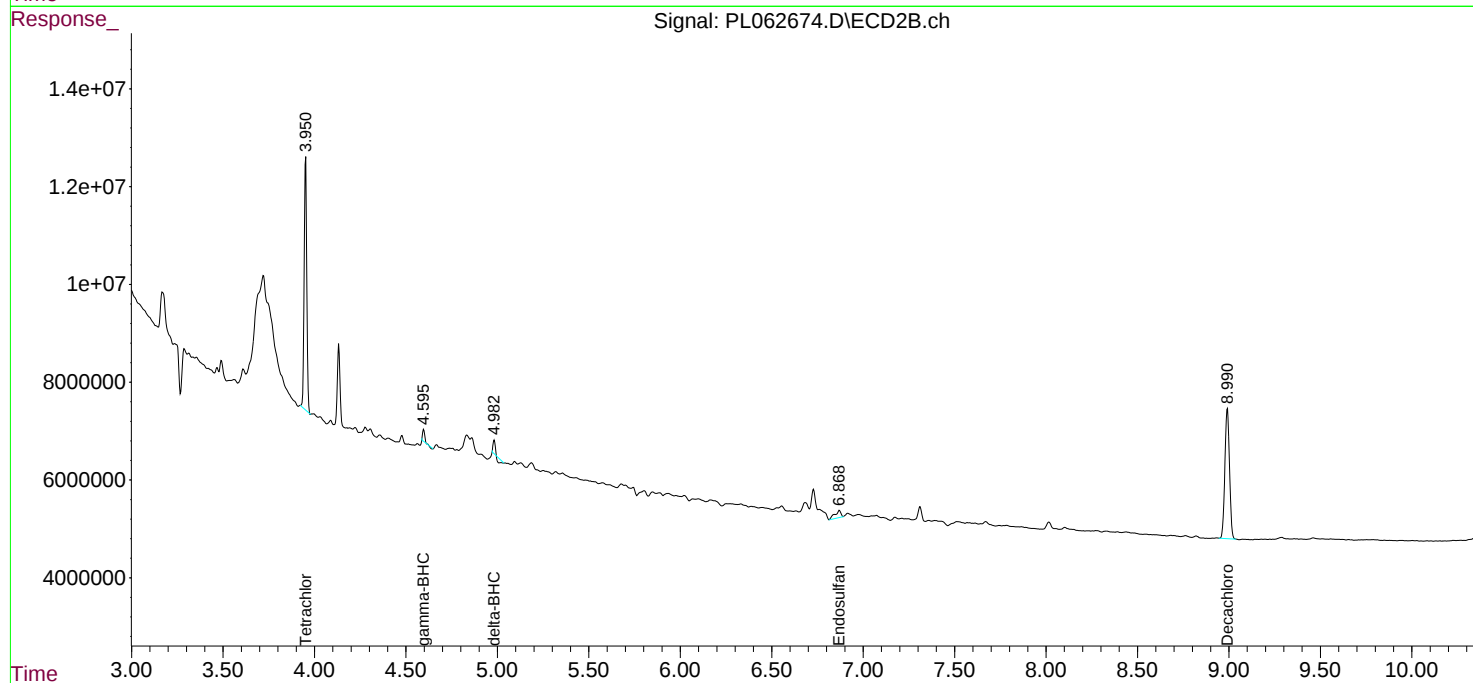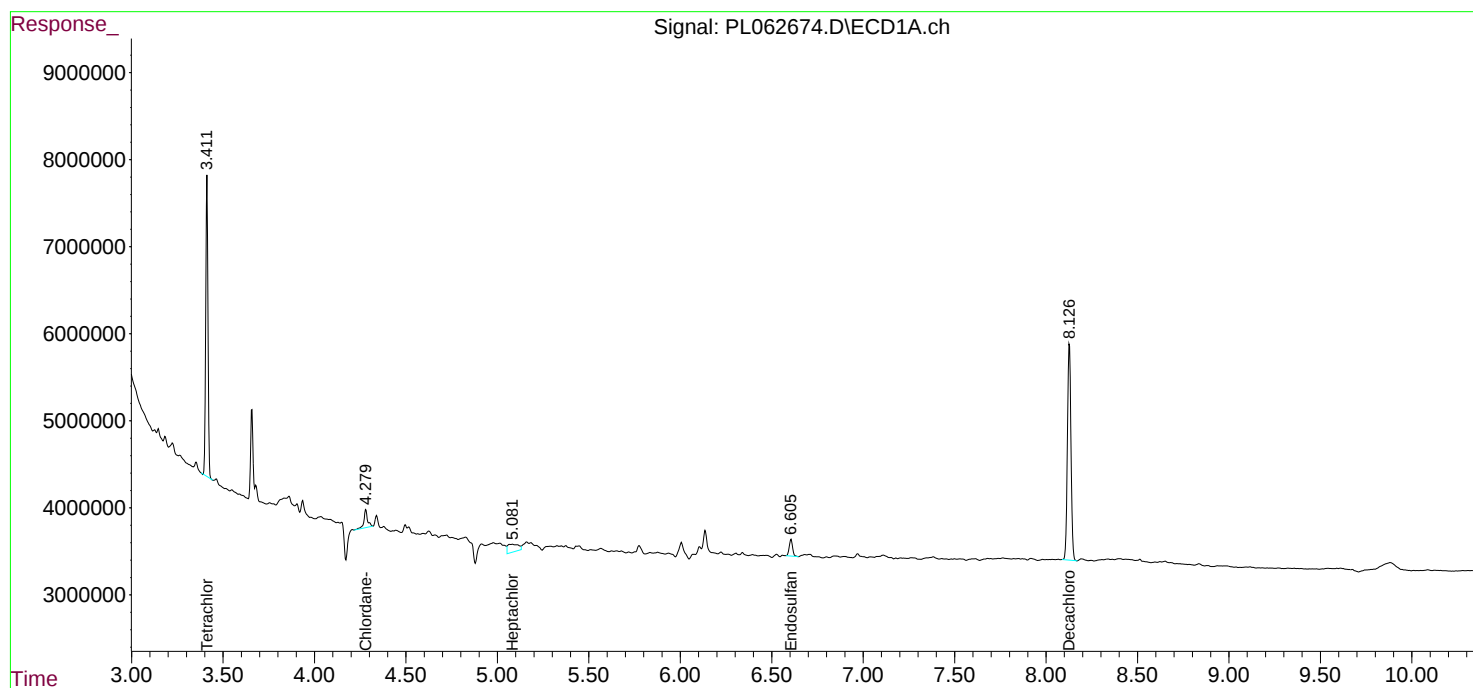


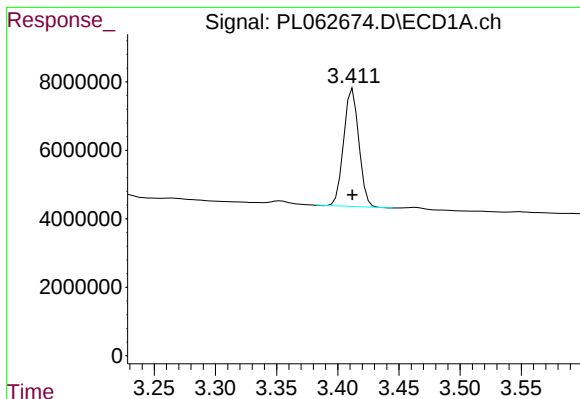

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 29569546
Conc: 17.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

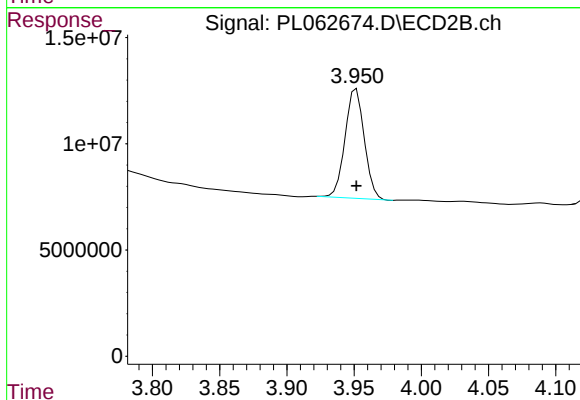


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 51337940
Conc: 17.47 ng/ml

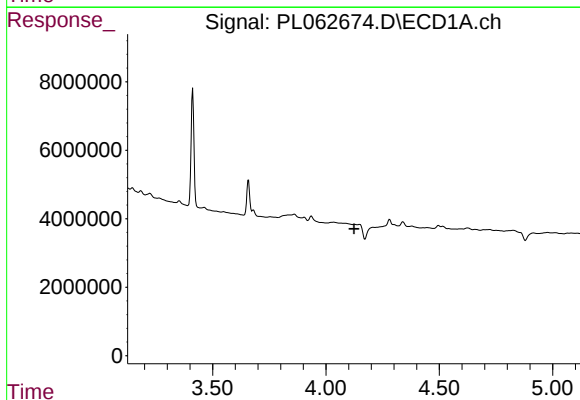


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.124 min
Response: 0
Conc: N.D.

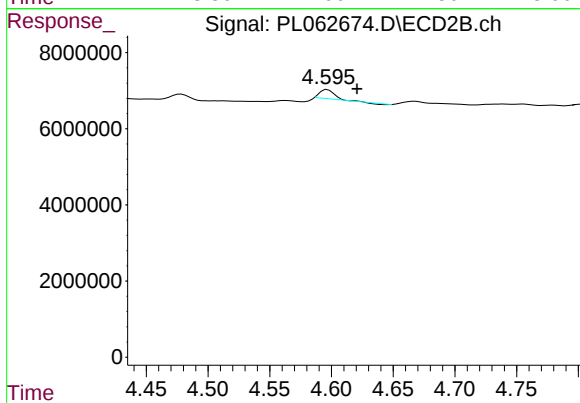

#3 gamma-BHC (Lindane)


R.T.: 4.597 min
Delta R.T.: -0.024 min
Response: 1780266
Conc: 0.43 ng/ml

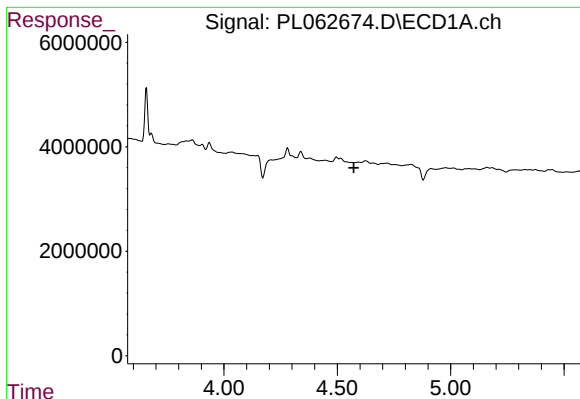

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

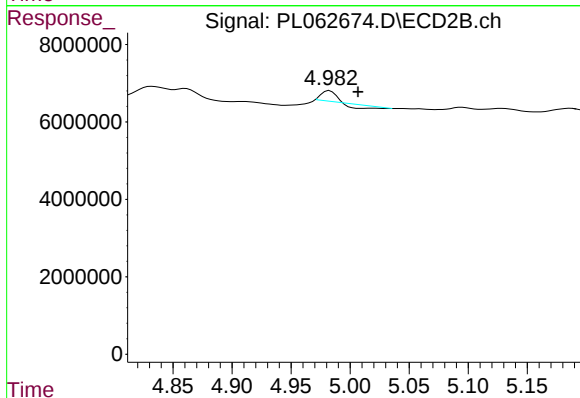


#7 delta-BHC

R.T.: 4.983 min
Delta R.T.: -0.024 min
Response: 997741
Conc: 0.29 ng/ml

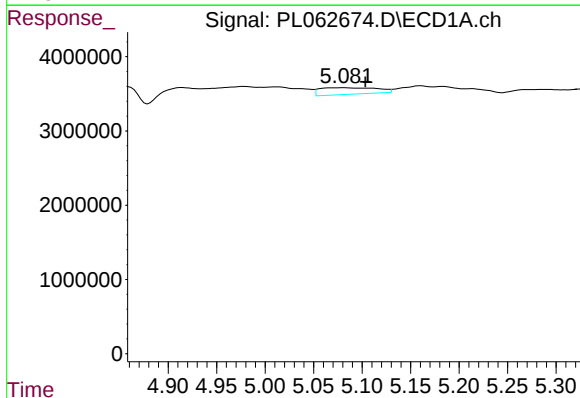


#8 Heptachlor epoxide

R.T.: 5.082 min
Delta R.T.: -0.021 min
Response: 3650954
Conc: 2.00 ng/ml

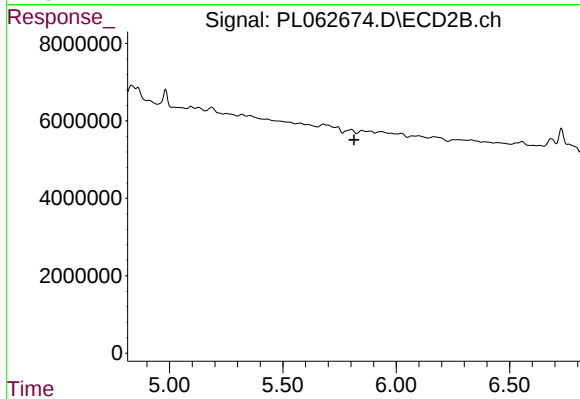

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

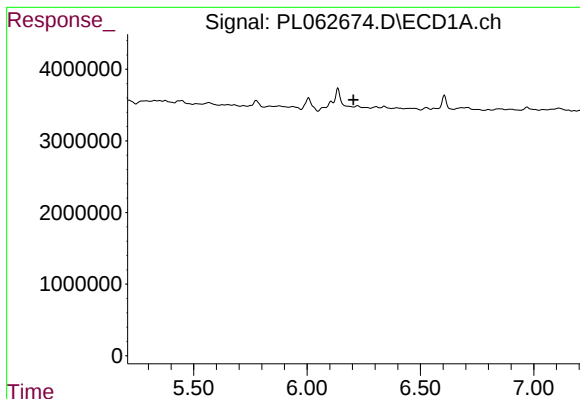

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

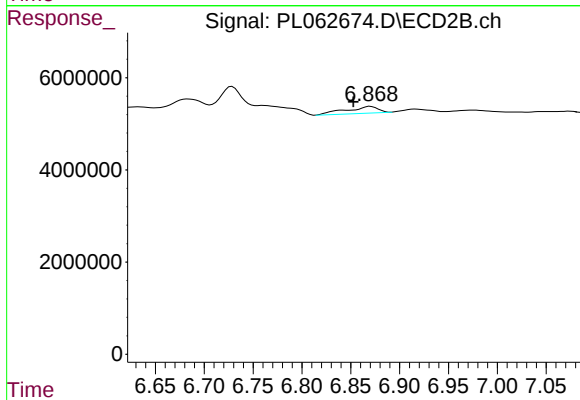


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.017 min
Response: 3238601
Conc: 1.13 ng/ml

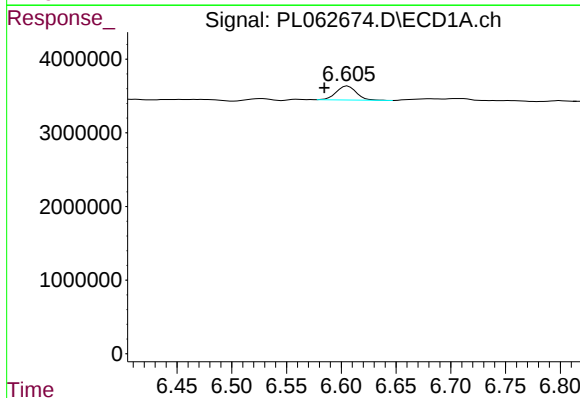


#19 Endosulfan Sulfate

R.T.: 6.606 min
Delta R.T.: 0.021 min
Response: 2418421
Conc: 1.47 ng/ml

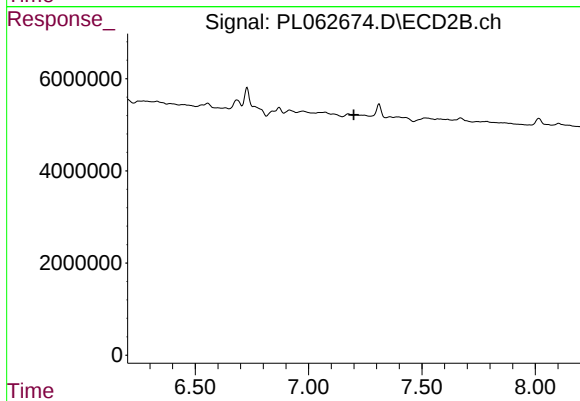

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

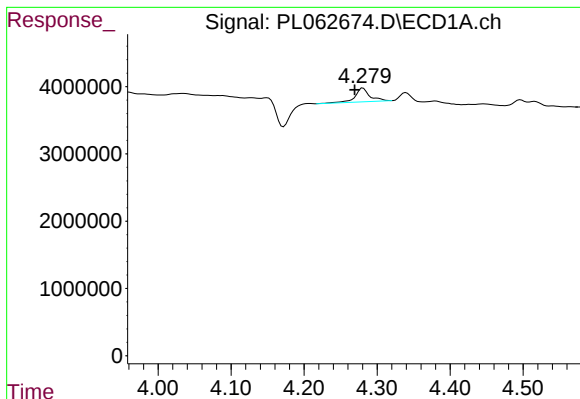

#23 Chlordane-1


R.T.: 4.281 min
Delta R.T.: 0.012 min
Response: 2869016
Conc: 55.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

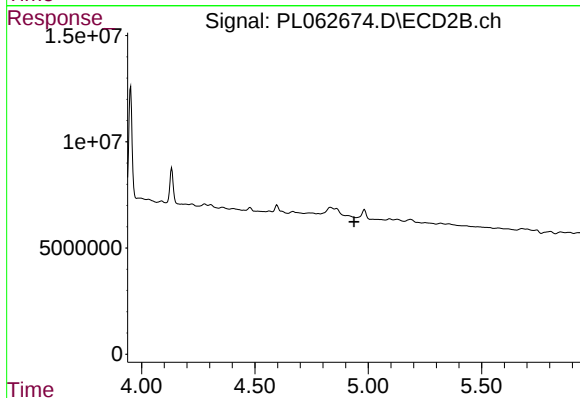


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

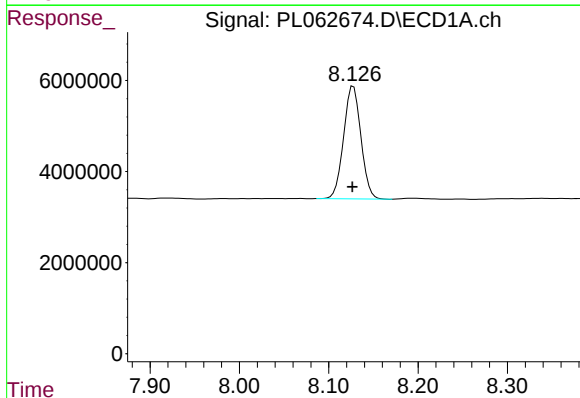

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 33346629
Conc: 20.79 ng/ml

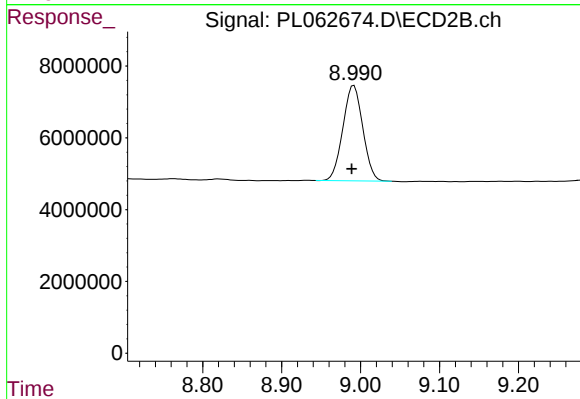

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 46598649
Conc: 22.26 ng/ml