

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102820\
 Data File : PL062656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 16:54
 Operator : DD\AJ
 Sample : L4528-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-24245

Manual Integrations
 APPROVED

Ankita
 10/29/2020 12:02:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 06:32:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	25899214	44005090	15.057	14.974
28)	SA Decachlor...	8.131	8.994	17985808	26210530	11.211	12.523
Target Compounds							
12)	B 4,4'-DDE	5.552	6.280	2200373	5702221	1.330m	1.770 #
17)	MA 4,4'-DDT	6.302	7.067	6384134	6436671	4.784m	2.867m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102820\
Data File : PL062656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 16:54
Operator : DD\AJ
Sample : L4528-03
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-24245


Manual Integrations
APPROVED

Ankita
10/29/2020 12:02:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 06:32:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

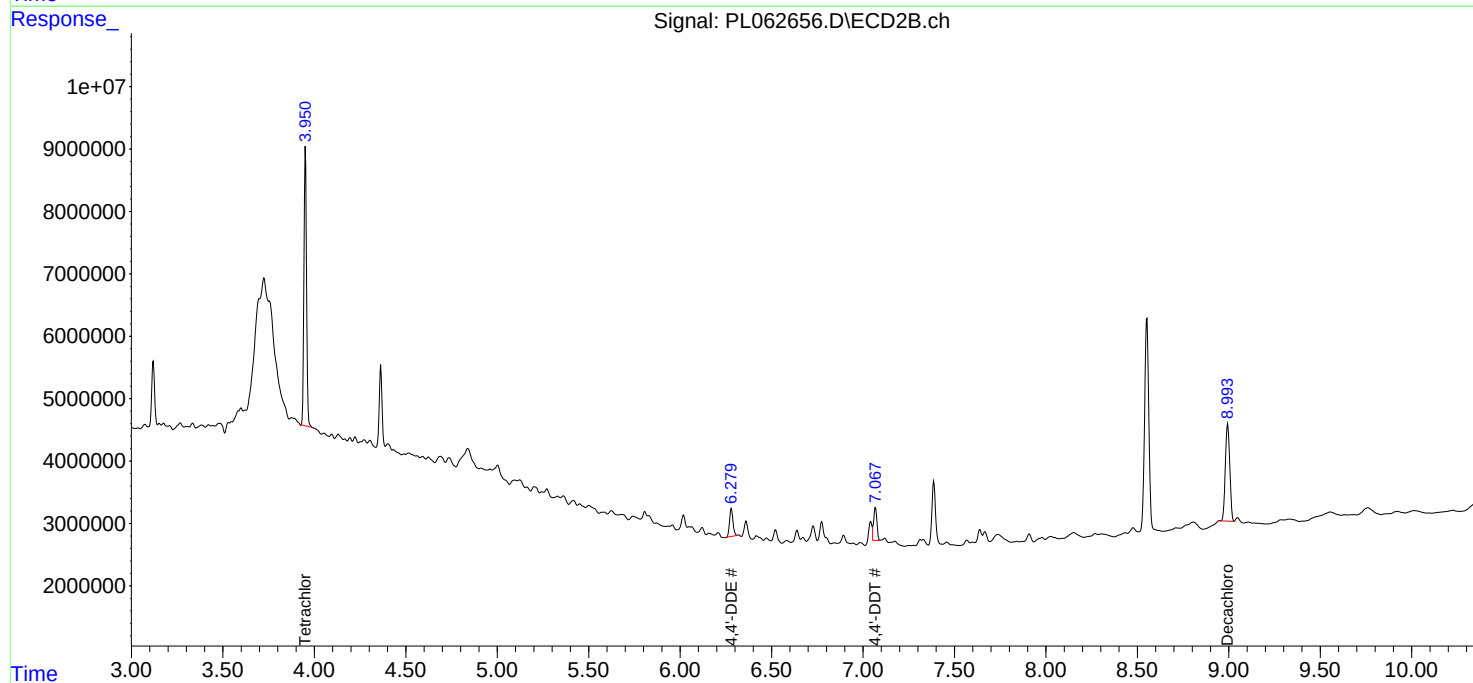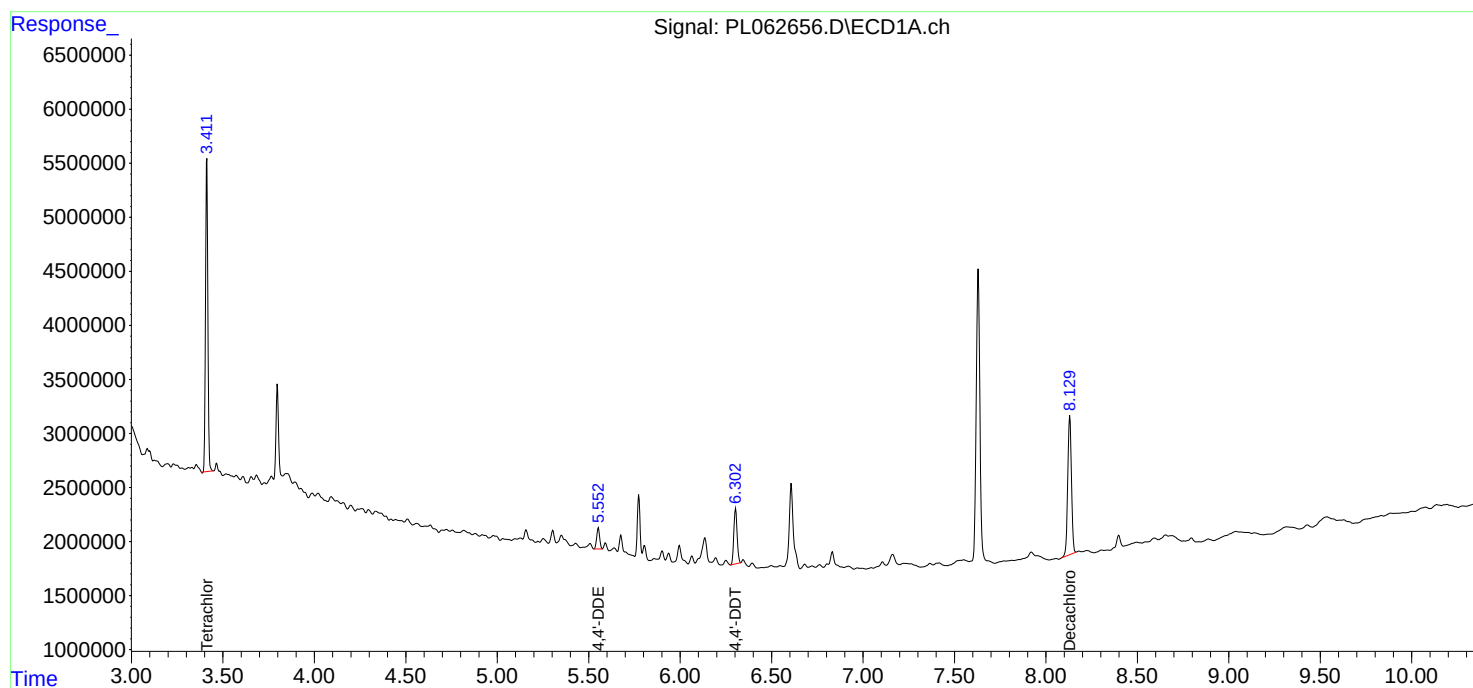

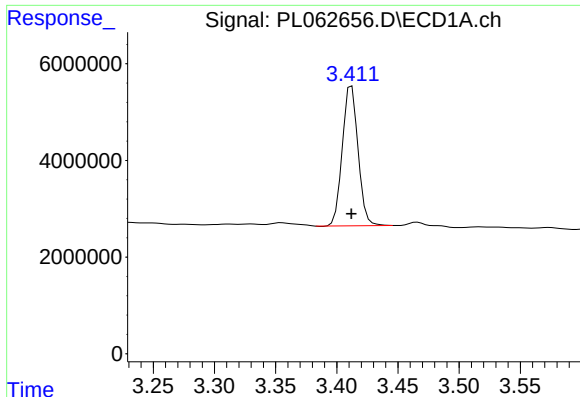


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 25899214
Conc: 15.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-24245


Manual Integrations
APPROVED

Ankita
10/29/2020 12:02:27 PM

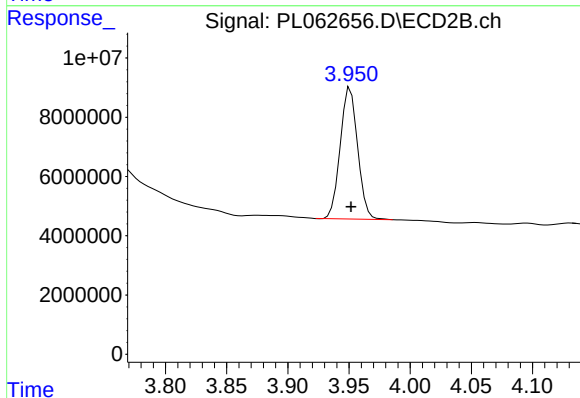


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 44005090
Conc: 14.97 ng/ml

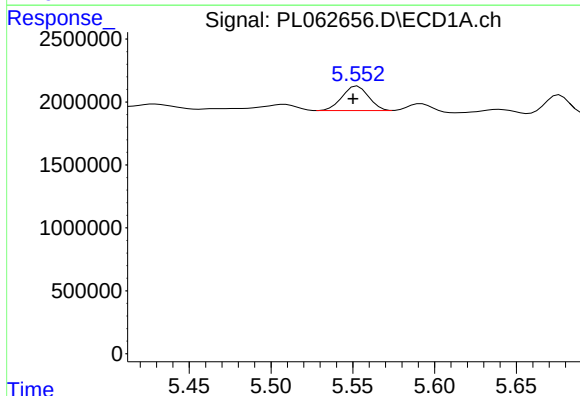


#12 4,4'-DDE

R.T.: 5.552 min
Delta R.T.: 0.001 min
Response: 2200373
Conc: 1.33 ng/ml m

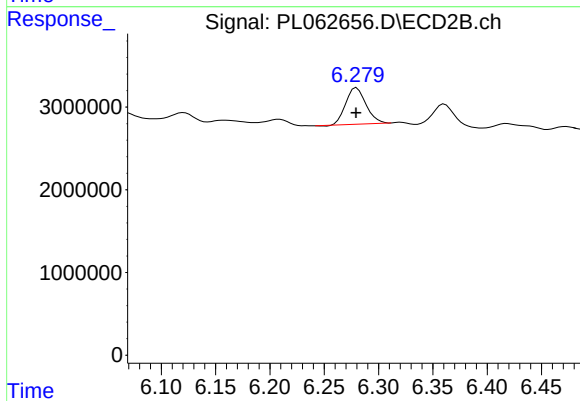

#12 4,4'-DDE

R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 5702221
Conc: 1.77 ng/ml

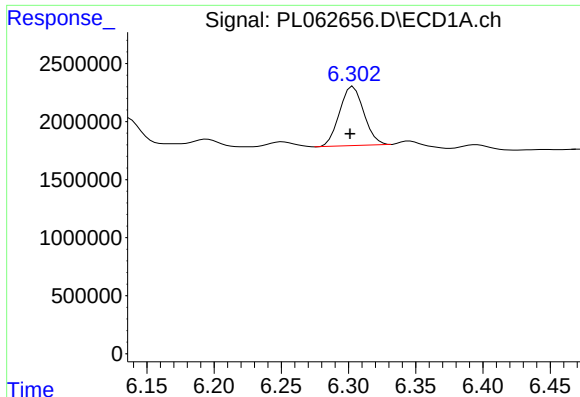


#17 4,4'-DDT

R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 6384134
Conc: 4.78 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CHRT-24245


Manual Integrations
APPROVED

Ankita
10/29/2020 12:02:27 PM

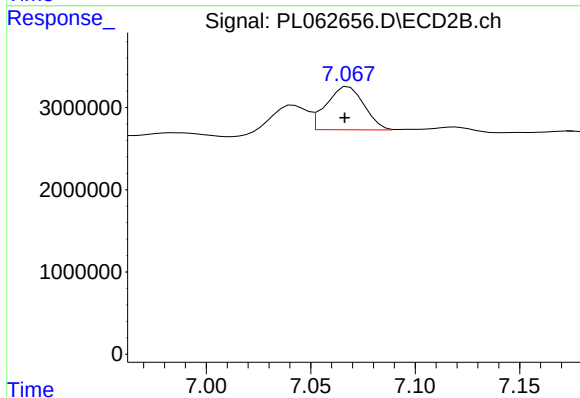


#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 6436671
Conc: 2.87 ng/ml m

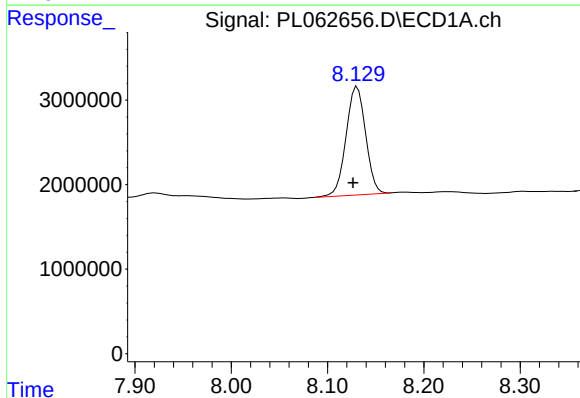

#28 Decachlorobiphenyl

R.T.: 8.131 min
Delta R.T.: 0.005 min
Response: 17985808
Conc: 11.21 ng/ml

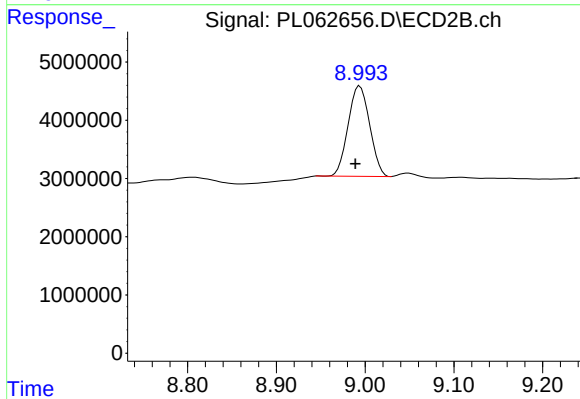

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.005 min
Response: 26210530
Conc: 12.52 ng/ml