

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102821\
 Data File : PL070633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 13:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:21:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.623	5.561	10326174	26402753	20.504	17.251
28)	SA Decachlor...	10.388	11.483	13730934	24540809	18.162	17.011
Target Compounds							
4)	MA Heptachlor	6.138f	0.000	457187	0	0.595	N.D. #
6)	B beta-BHC	6.138	0.000	457187	0	1.305	N.D. #
7)	B delta-BHC	0.000	7.078f	0	5389168	N.D.	2.142 #
10)	B gamma-Chl...	0.000	8.288	0	940630	N.D.	0.471 #
14)	MA Endrin	0.000	8.971	0	383059	N.D.	0.236 #
15)	B Endosulfa...	8.326f	0.000	1341610	0	2.106	N.D. #
21)	B Endrin ke...	0.000	10.049f	0	1913831	N.D.	1.105 #
25)	Chlordane-3	0.000	8.288	0	940630	N.D.	3.519 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102821\
Data File : PL070633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 13:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:21:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

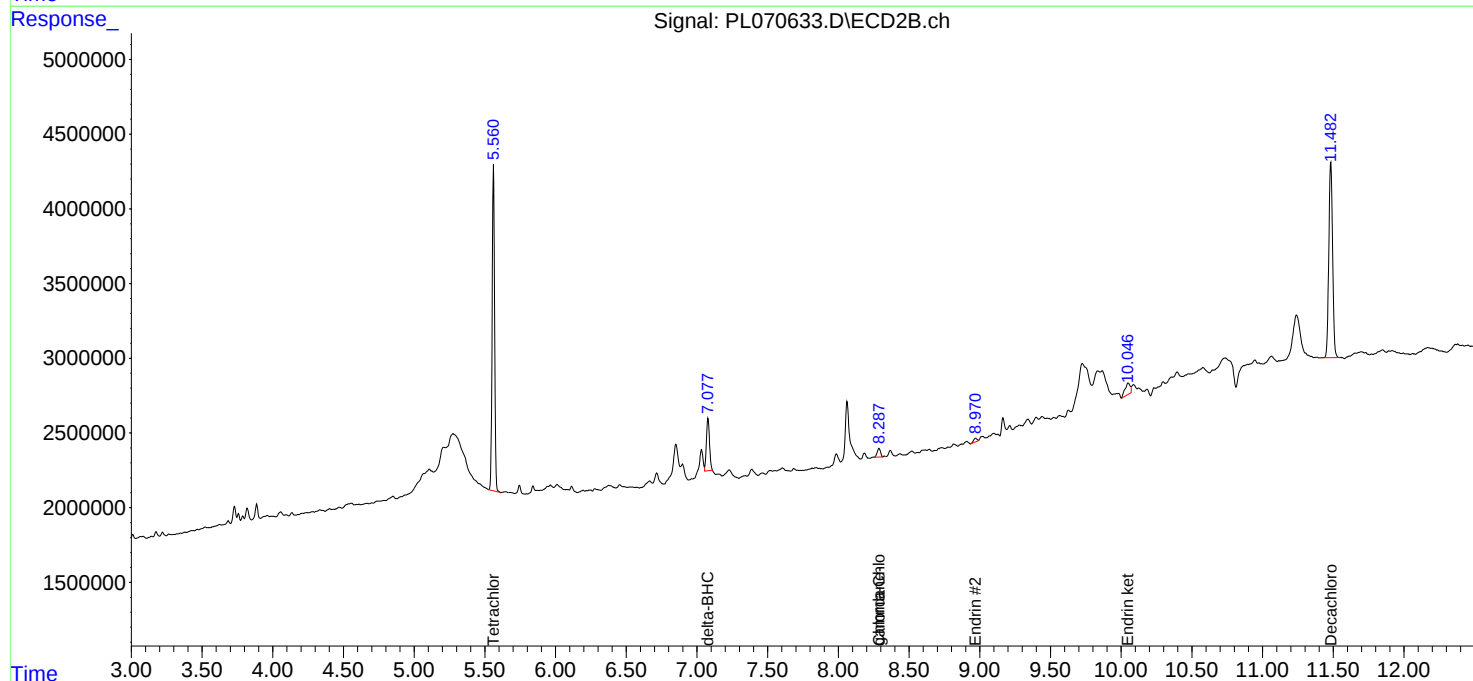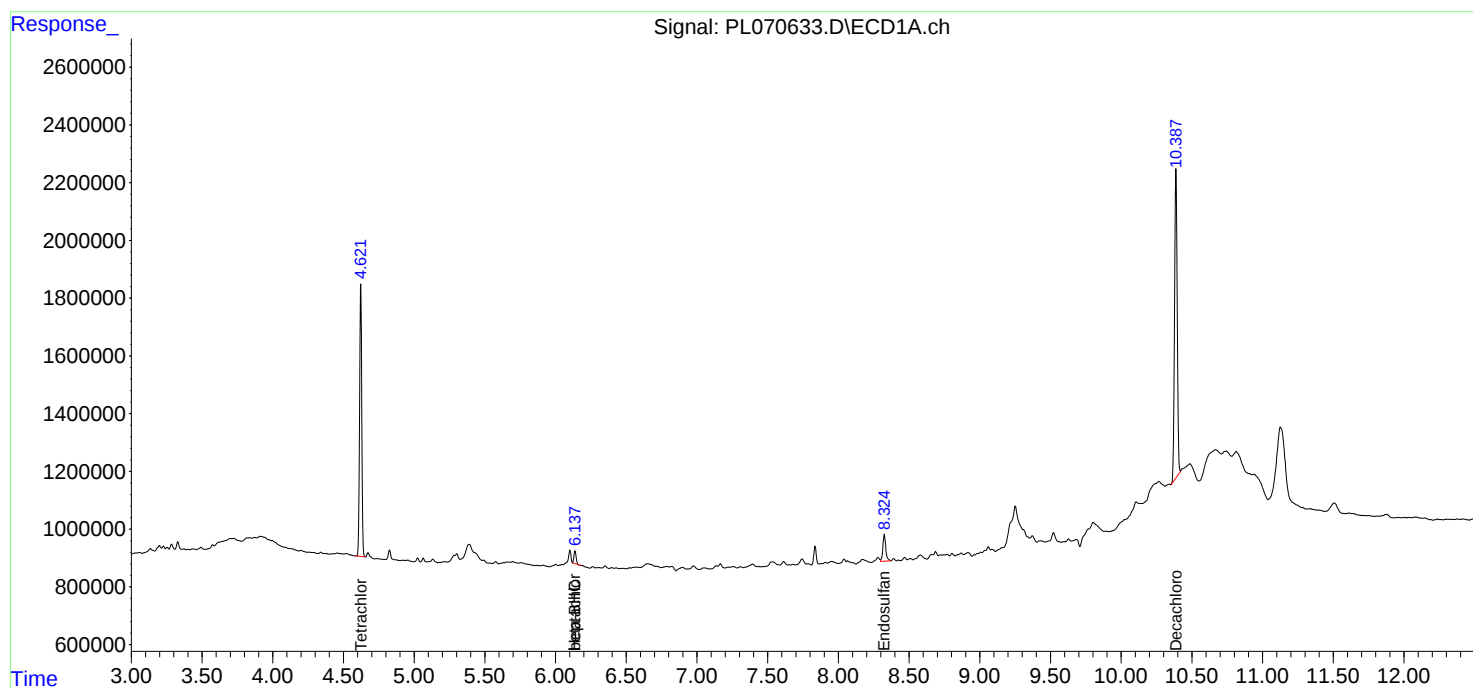


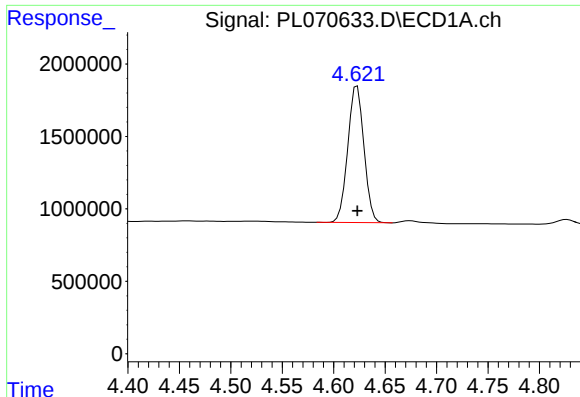

#1 Tetrachloro-m-xylene


R.T.: 4.623 min
Delta R.T.: 0.000 min
Response: 10326174
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

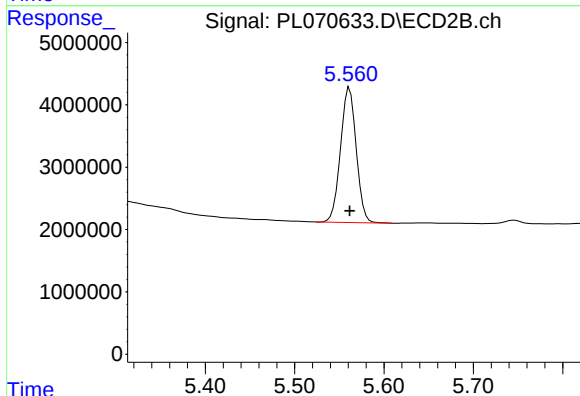


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: 0.000 min
Response: 26402753
Conc: 17.25 ng/ml

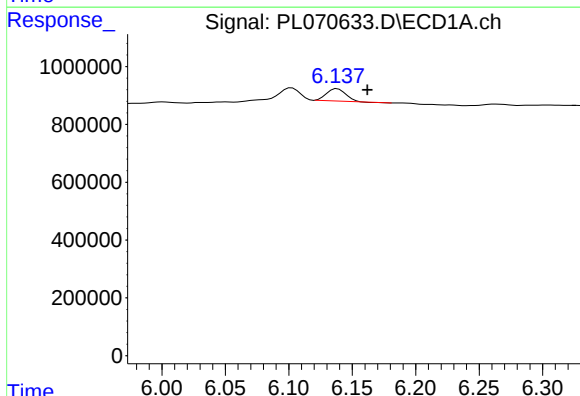


#4 Heptachlor

R.T.: 6.138 min
Delta R.T.: -0.024 min
Response: 457187
Conc: 0.60 ng/ml

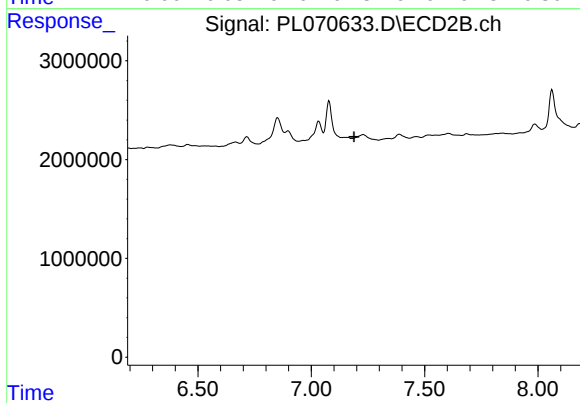

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.189 min
Response: 0
Conc: N.D.

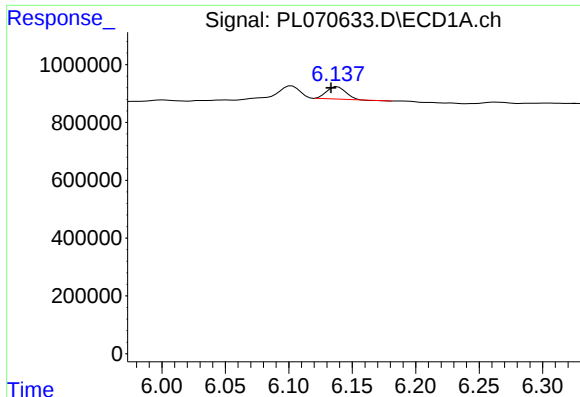

#6 beta-BHC


R.T.: 6.138 min
Delta R.T.: 0.005 min
Response: 457187
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

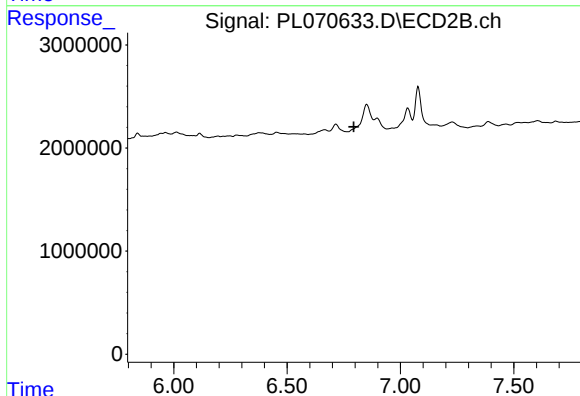


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.795 min
Response: 0
Conc: N.D.

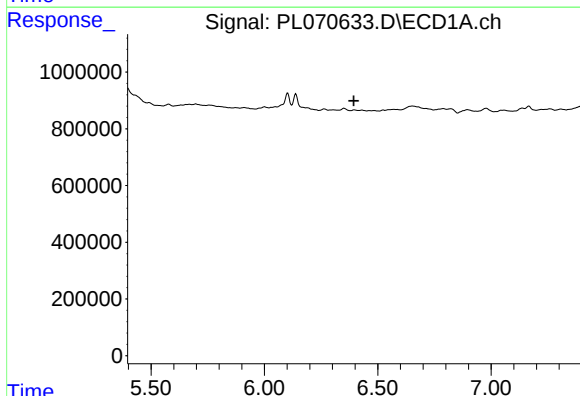


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

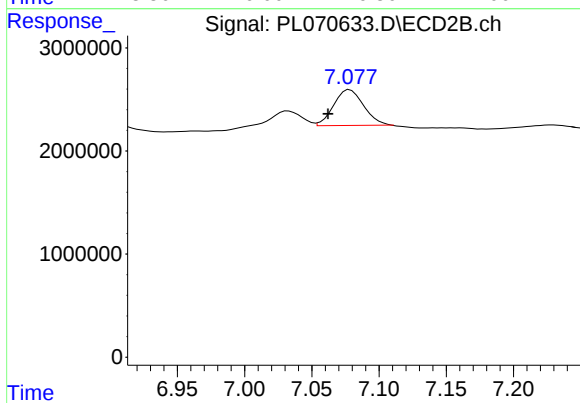

#7 delta-BHC


R.T.: 7.078 min
Delta R.T.: 0.016 min
Response: 5389168
Conc: 2.14 ng/ml

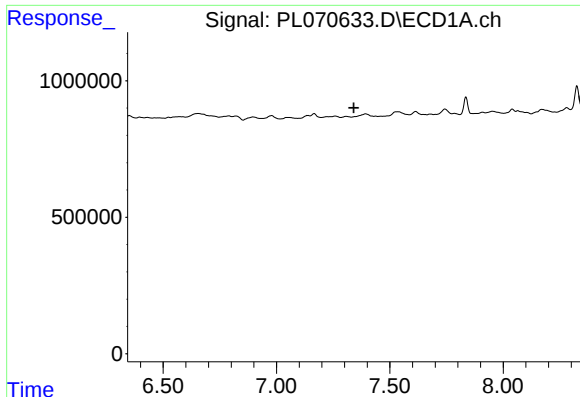

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

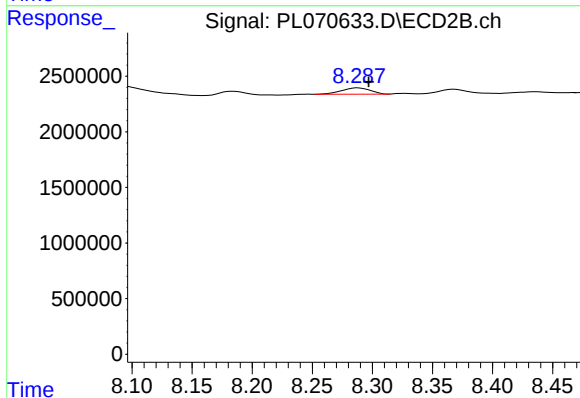


#10 gamma-Chlordane

R.T.: 8.288 min
Delta R.T.: -0.009 min
Response: 940630
Conc: 0.47 ng/ml

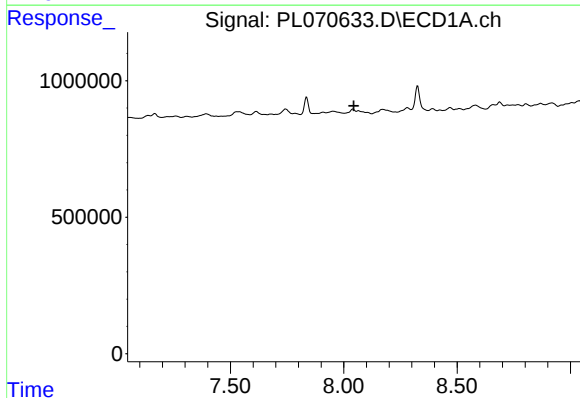


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.045 min
Response: 0
Conc: N.D.

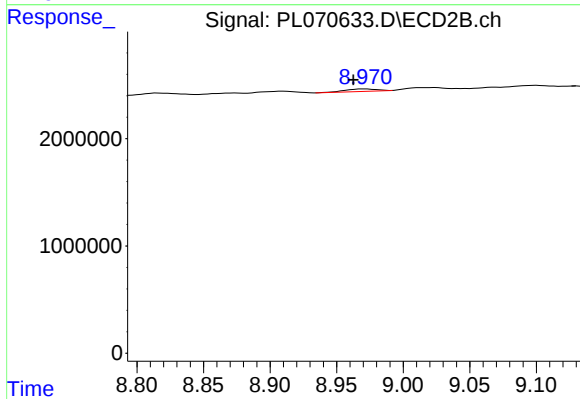

#14 Endrin


R.T.: 8.971 min
Delta R.T.: 0.009 min
Response: 383059
Conc: 0.24 ng/ml

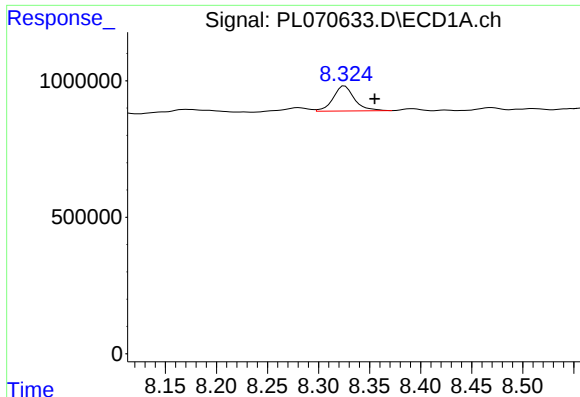

#15 Endosulfan II


R.T.: 8.326 min
Delta R.T.: -0.029 min
Response: 1341610
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

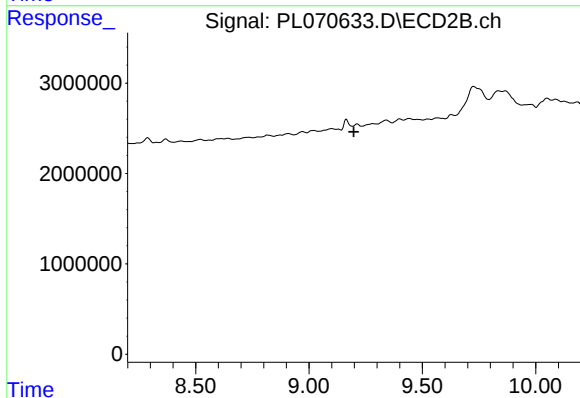


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

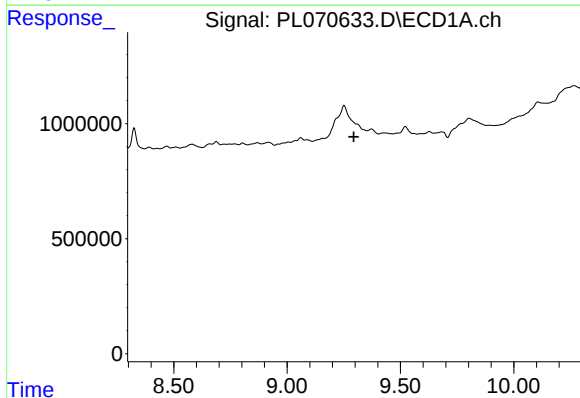


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

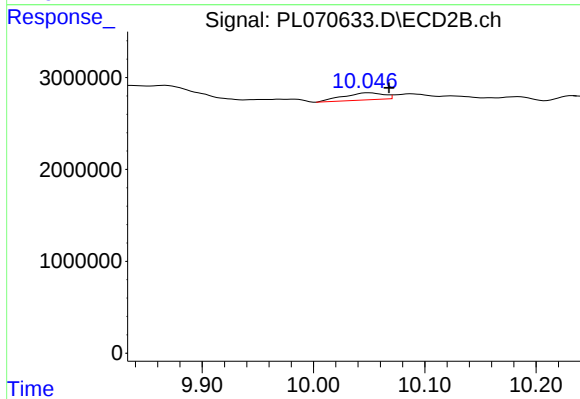

#21 Endrin ketone


R.T.: 10.049 min
Delta R.T.: -0.019 min
Response: 1913831
Conc: 1.10 ng/ml

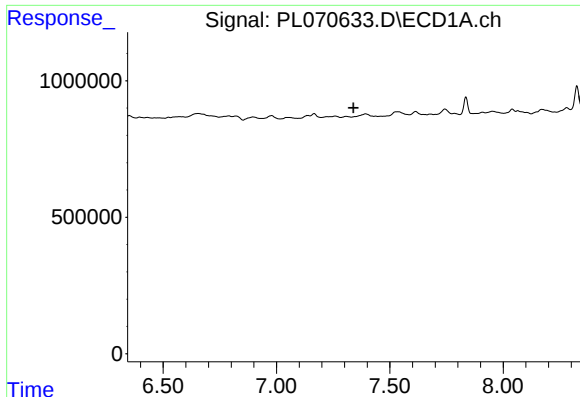

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

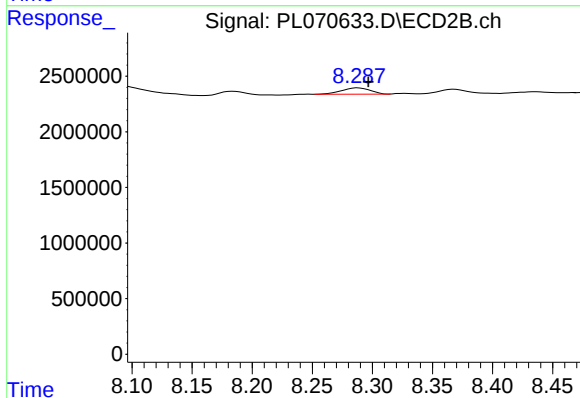


#25 Chlordane-3

R.T.: 8.288 min
Delta R.T.: -0.009 min
Response: 940630
Conc: 3.52 ng/ml

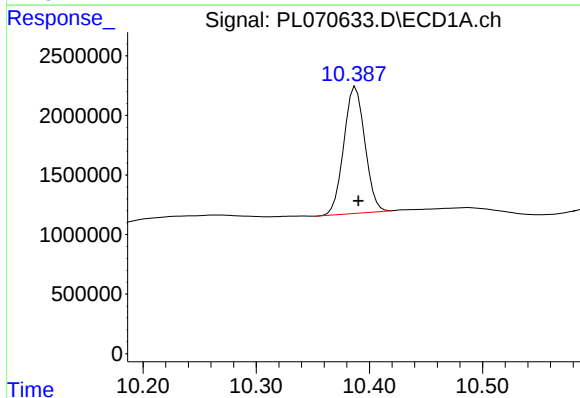

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.002 min
Response: 13730934
Conc: 18.16 ng/ml

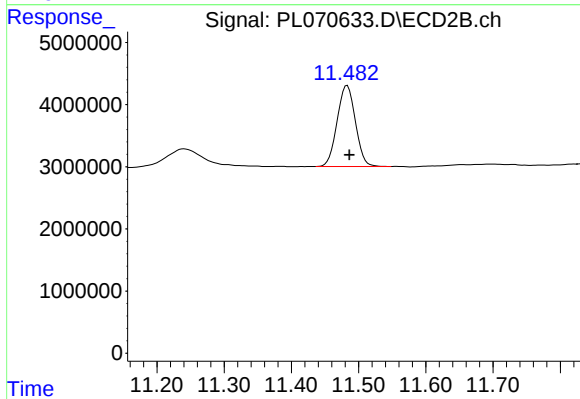

#28 Decachlorobiphenyl

R.T.: 11.483 min
Delta R.T.: -0.003 min
Response: 24540809
Conc: 17.01 ng/ml