

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102821\
 Data File : PL070632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 13:13
 Operator : AR\AJ
 Sample : M4373-03 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-04-102621

Manual Integrations
 APPROVED

mohammad
 10/29/2021 8:58:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:21:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 07:49:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.623	5.560	830948	1870366	1.650	1.222m#
28)	SA Decachlor...	10.388	11.481	1111792	1443560	1.471	1.001m#
Target Compounds							
16)	A 4,4'-DDD	8.208	9.100	393293	763740	0.691	0.499m#
17)	MA 4,4'-DDT	8.469	9.422	566995	1389597	0.888	0.804

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102821\
Data File : PL070632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 13:13
Operator : AR\AJ
Sample : M4373-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SU-04-102621


Manual Integrations
APPROVED

mohammad
10/29/2021 8:58:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:21:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102621.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 07:49:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

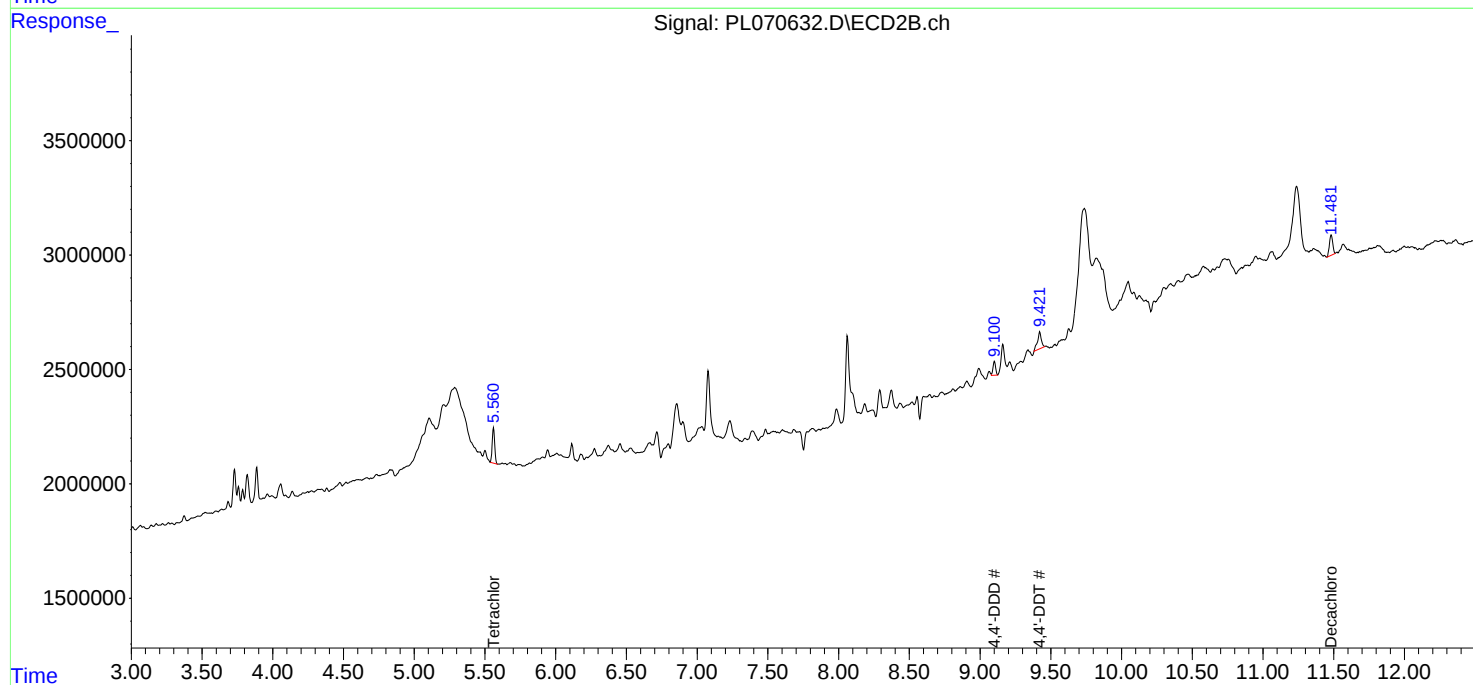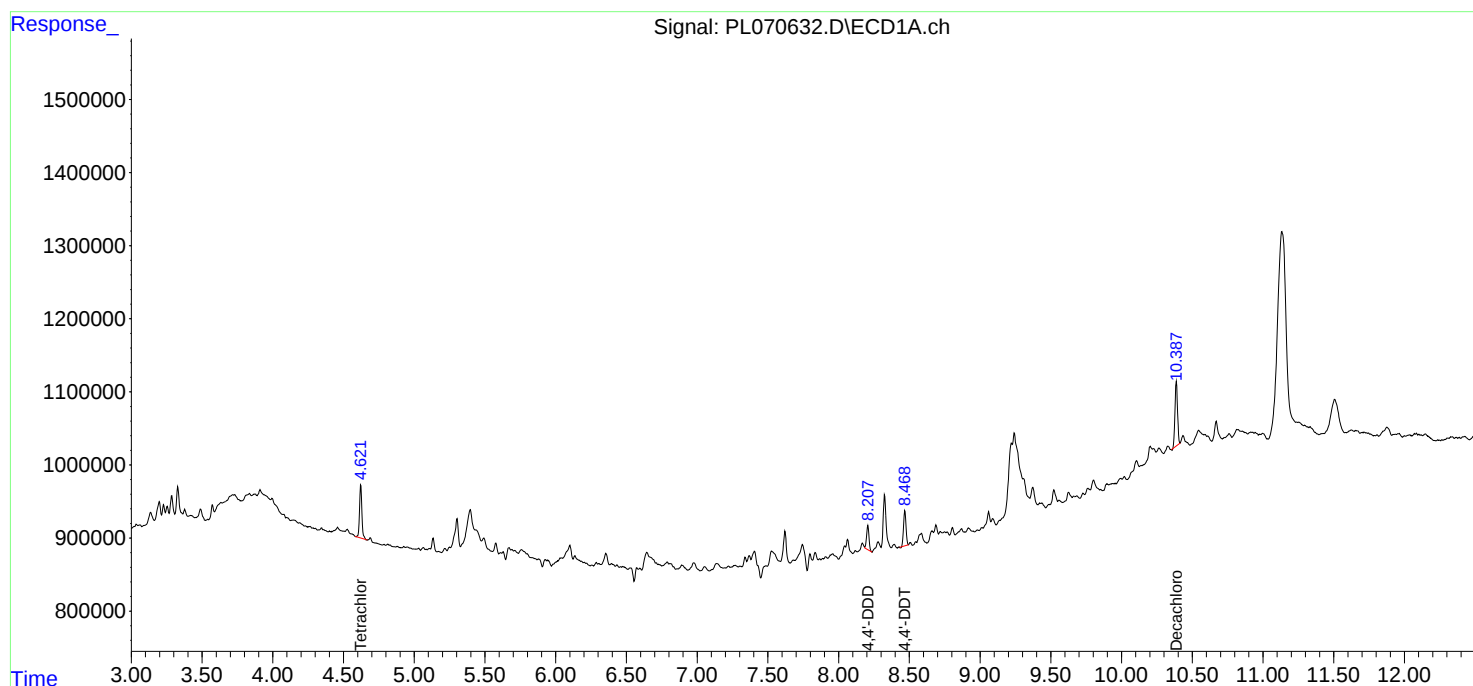

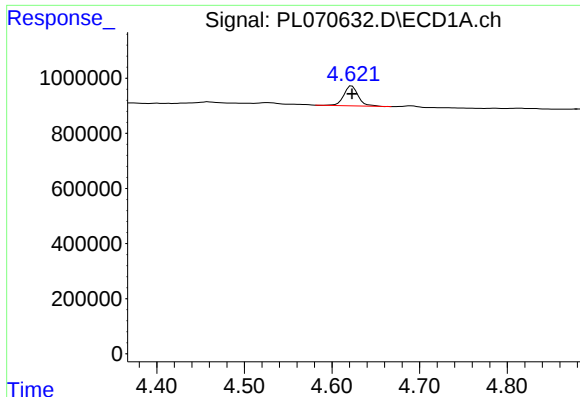


#1 Tetrachloro-m-xylene

R.T.: 4.623 min
Delta R.T.: 0.000 min
Response: 830948
Conc: 1.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-102621


Manual Integrations
APPROVED

mohammad
10/29/2021 8:58:08 AM

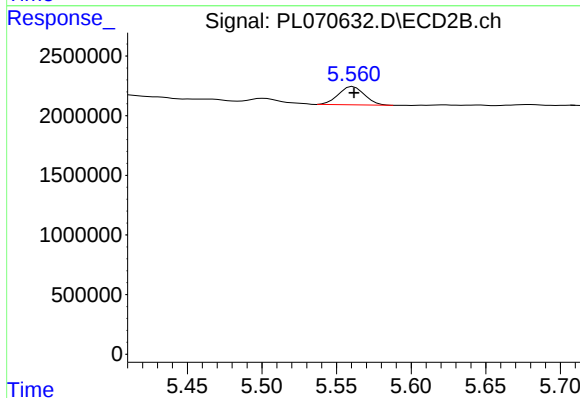


#1 Tetrachloro-m-xylene

R.T.: 5.560 min
Delta R.T.: -0.002 min
Response: 1870366
Conc: 1.22 ng/ml m

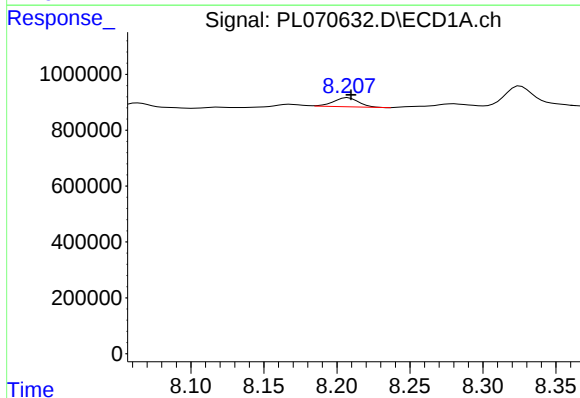


#16 4,4'-DDD

R.T.: 8.208 min
Delta R.T.: -0.002 min
Response: 393293
Conc: 0.69 ng/ml

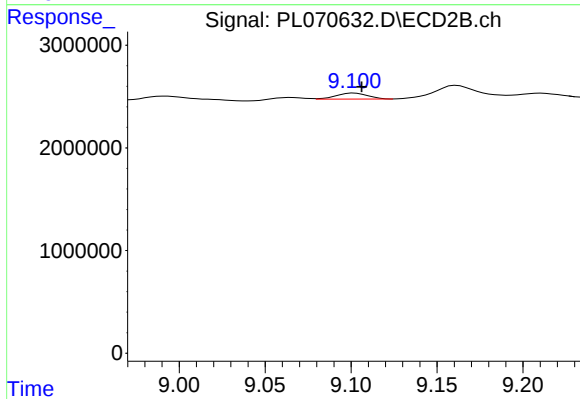

#16 4,4'-DDD

R.T.: 9.100 min
Delta R.T.: -0.006 min
Response: 763740
Conc: 0.50 ng/ml m

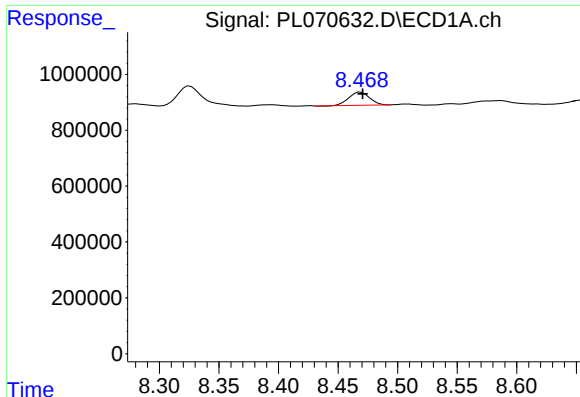


#17 4,4'-DDT

R.T.: 8.469 min
Delta R.T.: -0.002 min
Response: 566995
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-102621


Manual Integrations
APPROVED

mohammad
10/29/2021 8:58:08 AM

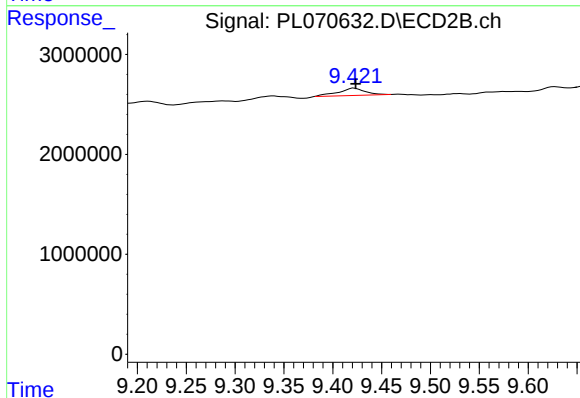


#17 4,4'-DDT

R.T.: 9.422 min
Delta R.T.: -0.002 min
Response: 1389597
Conc: 0.80 ng/ml

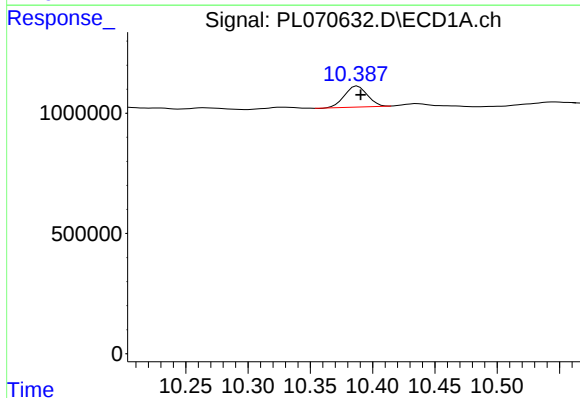

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.002 min
Response: 1111792
Conc: 1.47 ng/ml

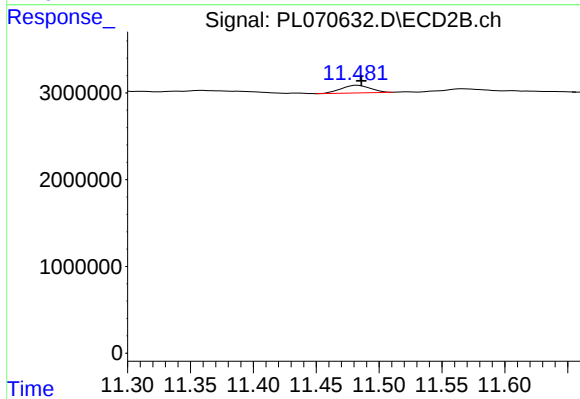

#28 Decachlorobiphenyl

R.T.: 11.481 min
Delta R.T.: -0.005 min
Response: 1443560
Conc: 1.00 ng/ml m