

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102822\
 Data File : PL078596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2022 19:05
 Operator : AR\AJ
 Sample : N5273-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LIDEN-GAS-PIPELINE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:23:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	2.591f	41494129	52086828	21.759	20.401
28)	SA Decachlor...	8.773	7.661f	37523193	36652281	24.943	19.351

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102822\
Data File : PL078596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2022 19:05
Operator : AR\AJ
Sample : N5273-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LIDEN-GAS-PIPELINE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:23:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

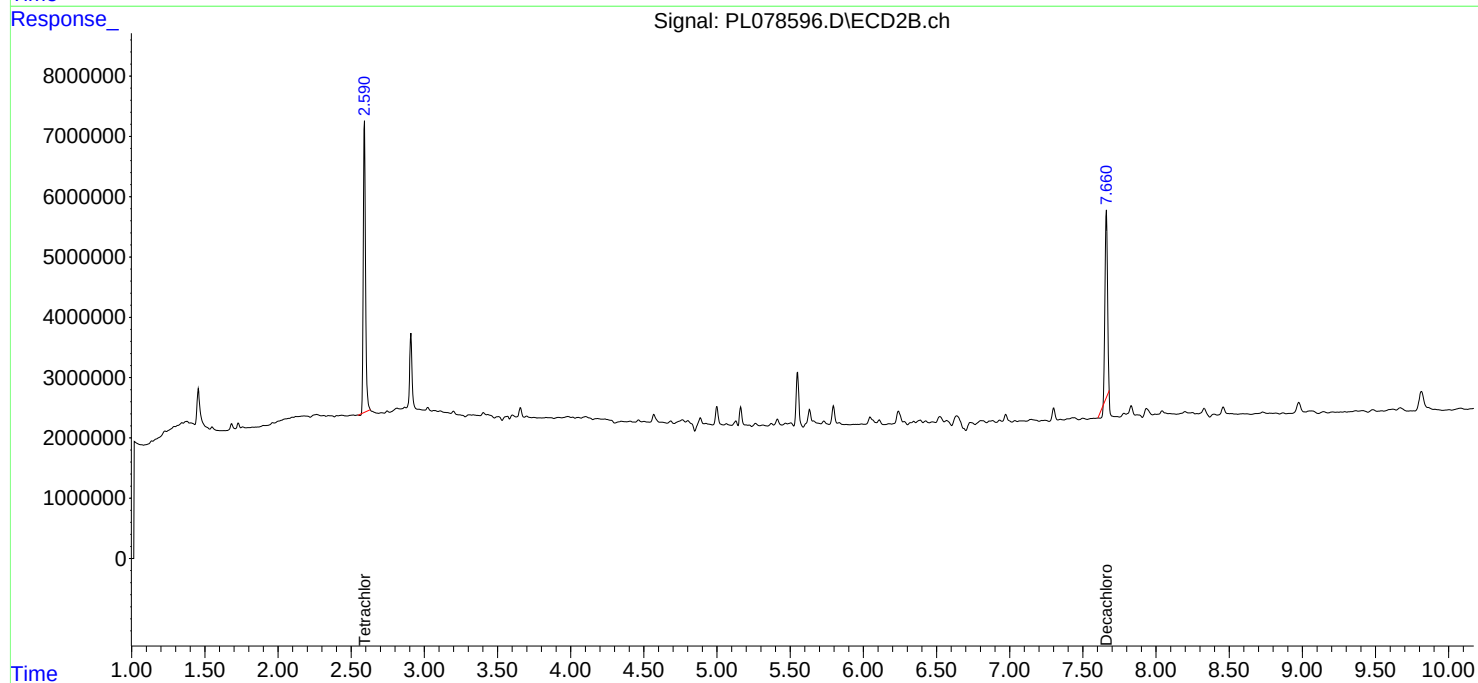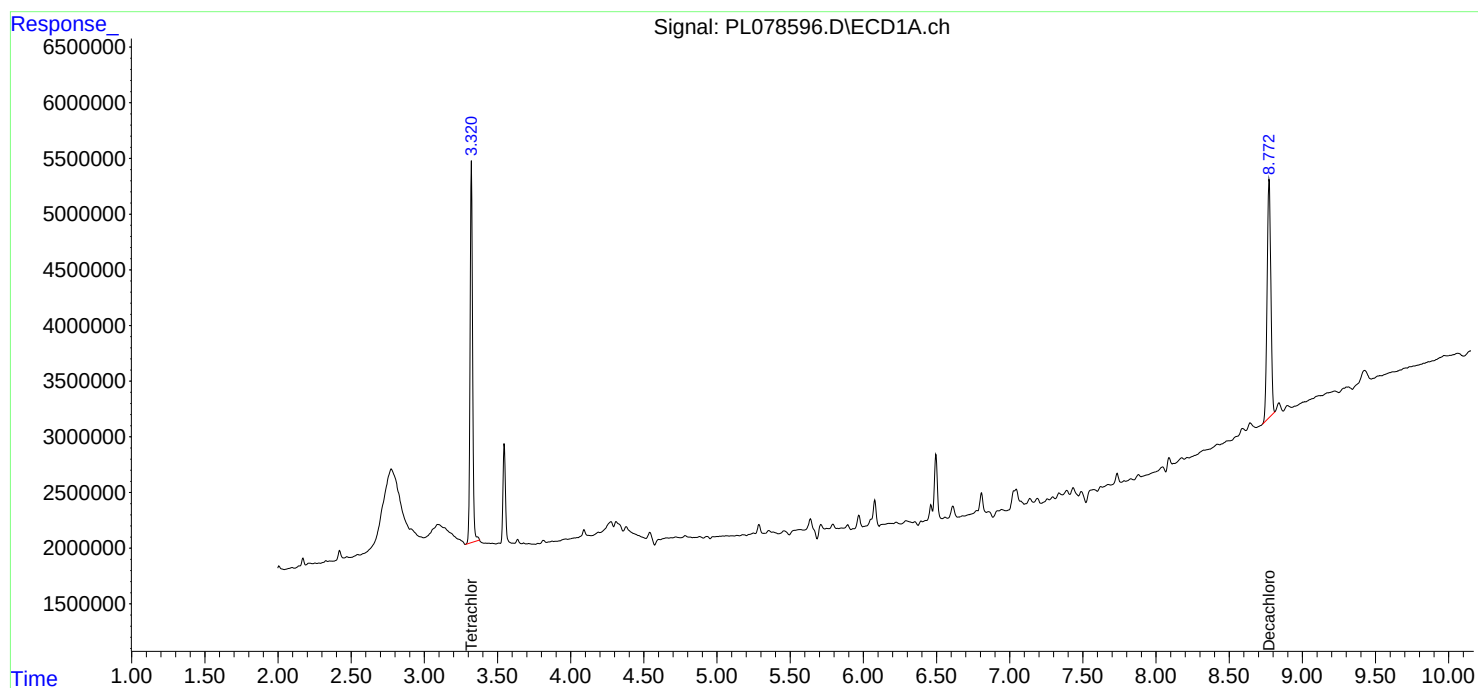


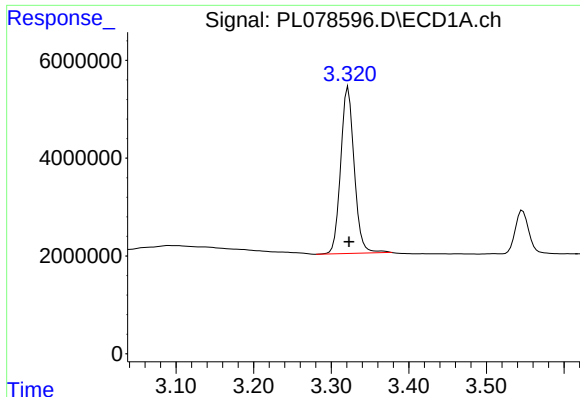

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 41494129
Conc: 21.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
LIDEN-GAS-PIPELINE

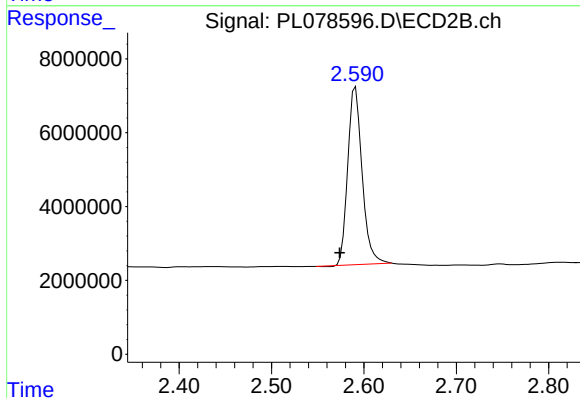


#1 Tetrachloro-m-xylene

R.T.: 2.591 min
Delta R.T.: 0.017 min
Response: 52086828
Conc: 20.40 ng/ml

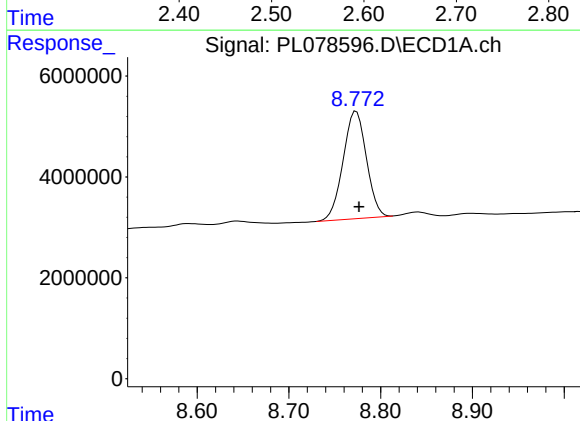

#28 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: -0.003 min
Response: 37523193
Conc: 24.94 ng/ml

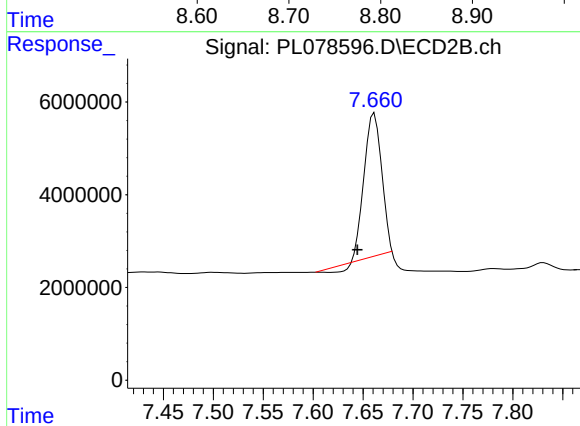

#28 Decachlorobiphenyl

R.T.: 7.661 min
Delta R.T.: 0.017 min
Response: 36652281
Conc: 19.35 ng/ml