

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 16:30
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 16:59:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 16:53:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.777	58497597	77854264	25.481	24.086
2) SA Decachlor...	9.054	7.916	47238786	67136507	26.442	25.263
Target Compounds						
23) Chlordane-1	4.701	3.776	27231061	25274086	257.672	239.800
24) Chlordane-2	5.231	4.353	28443684	29936970	261.453	248.294
25) Chlordane-3	5.941	4.982	94052852	85720881	252.753	235.491
26) Chlordane-4	6.023	5.046	116.0E6	82832502	253.851	236.282
27) Chlordane-5	6.872	5.941	23829277	29958197	260.601	241.304



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 16:30
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 16:59:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 16:53:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

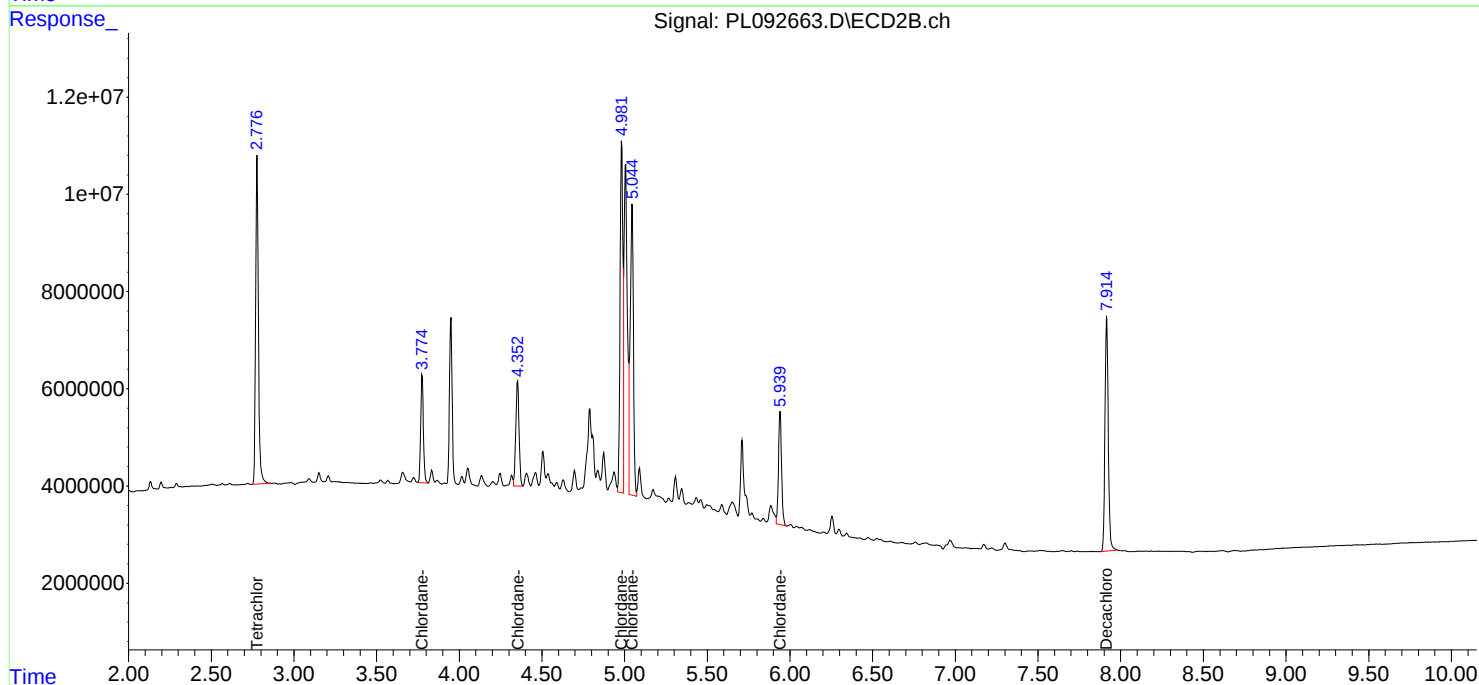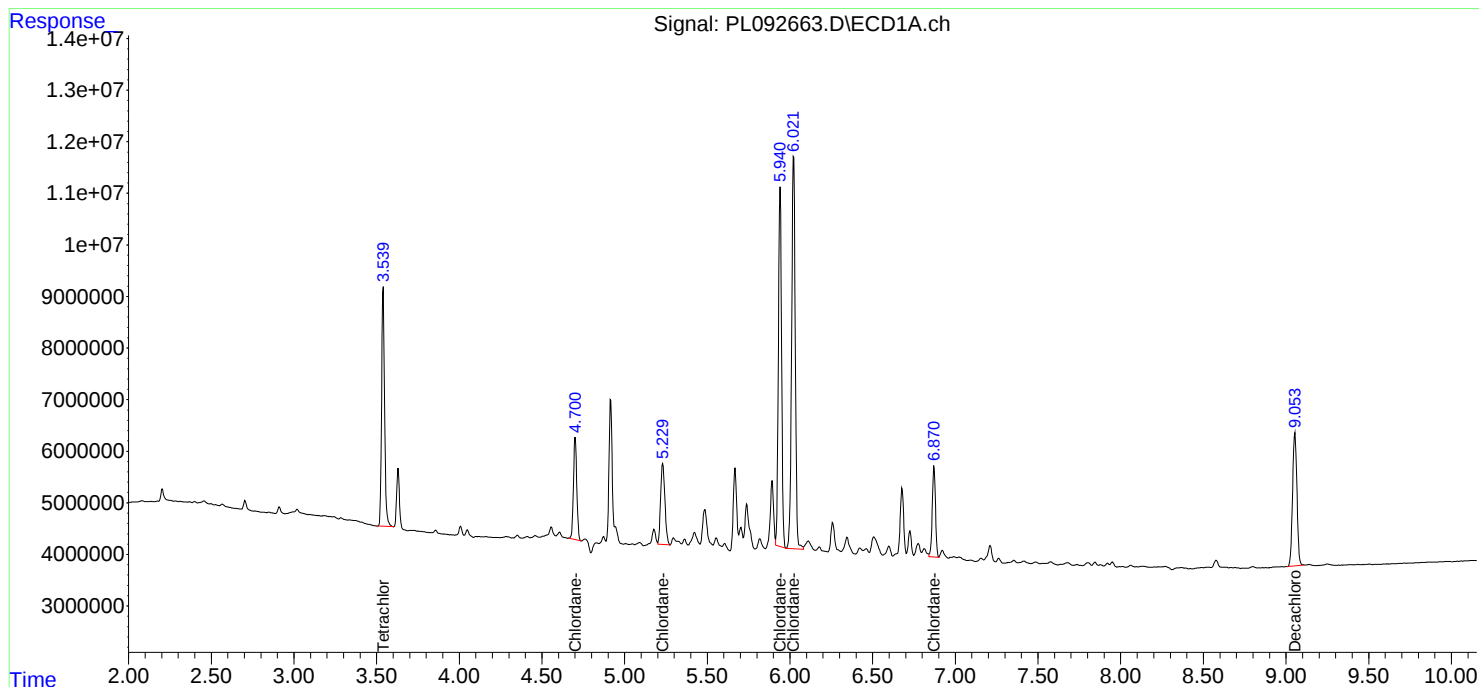


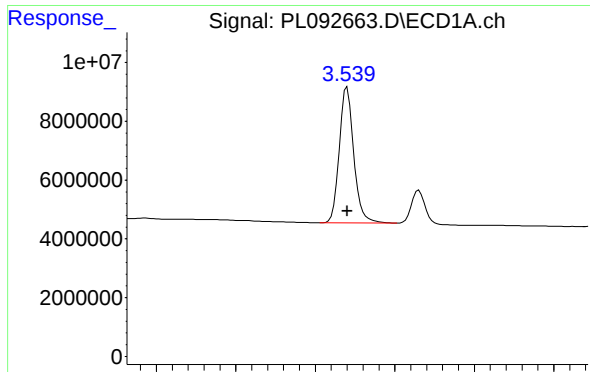

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 58497597
Conc: 25.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

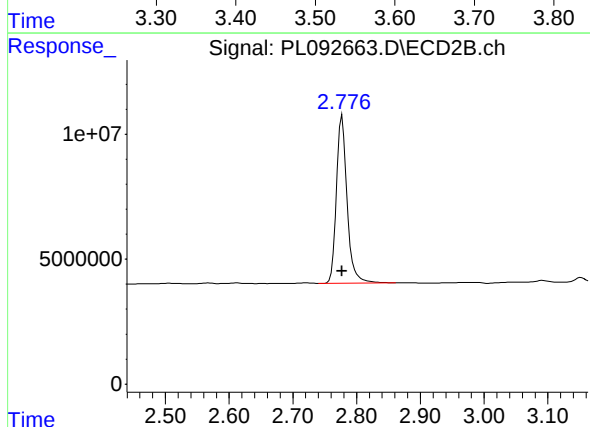


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 77854264
Conc: 24.09 ng/ml

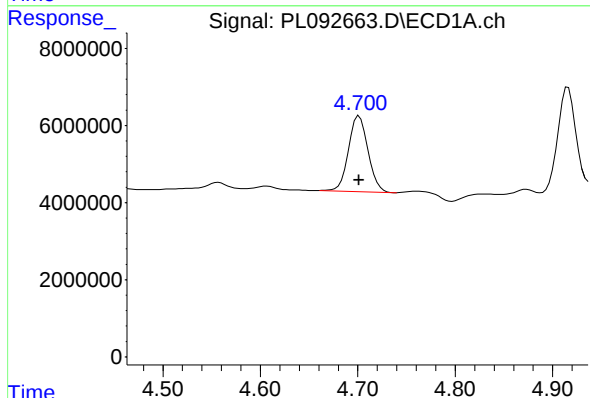


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 27231061
Conc: 257.67 ng/ml

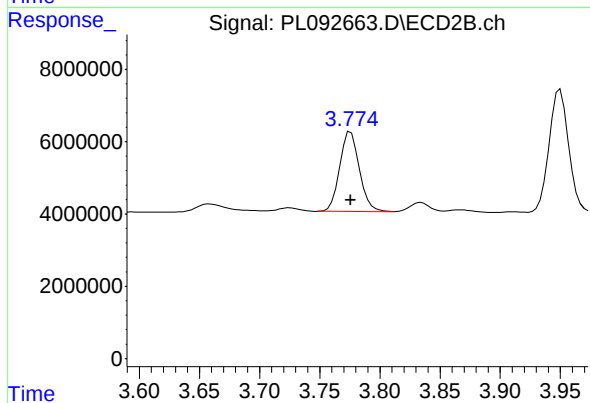

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 25274086
Conc: 239.80 ng/ml

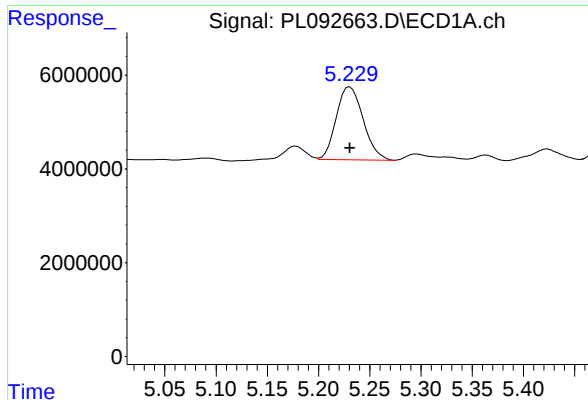

#24 Chlordane-2


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 28443684
Conc: 261.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

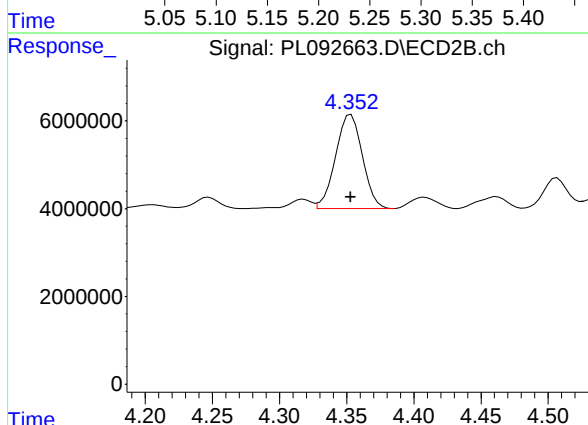


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 29936970
Conc: 248.29 ng/ml

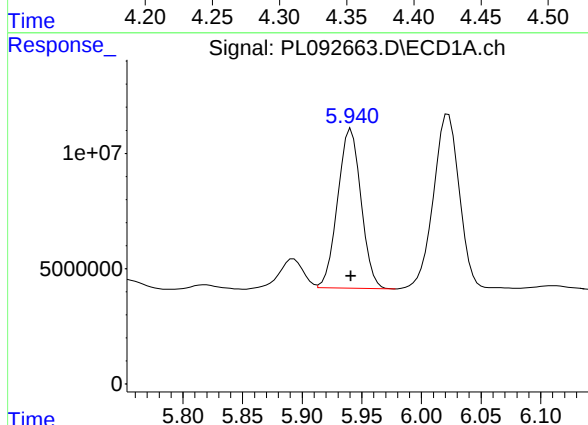


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 94052852
Conc: 252.75 ng/ml

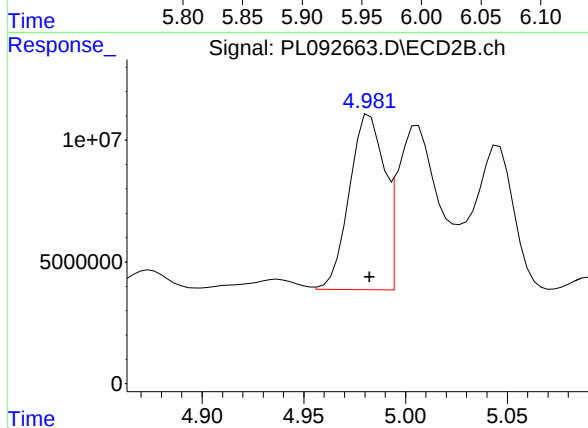

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 85720881
Conc: 235.49 ng/ml

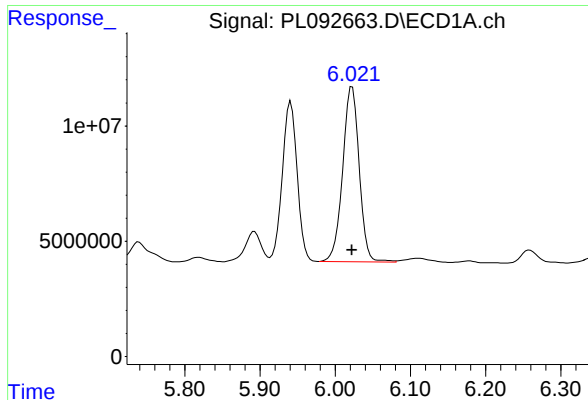

#26 Chlordane-4


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 115961405
Conc: 253.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

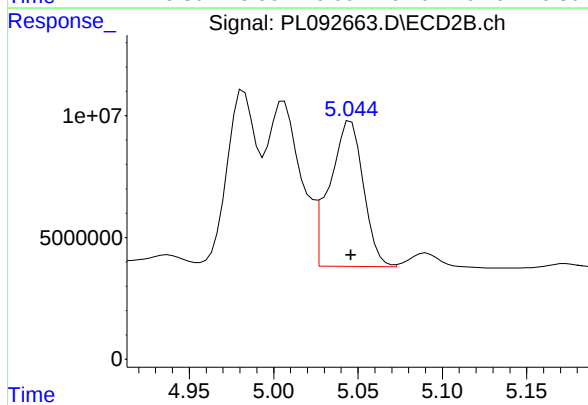


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 82832502
Conc: 236.28 ng/ml

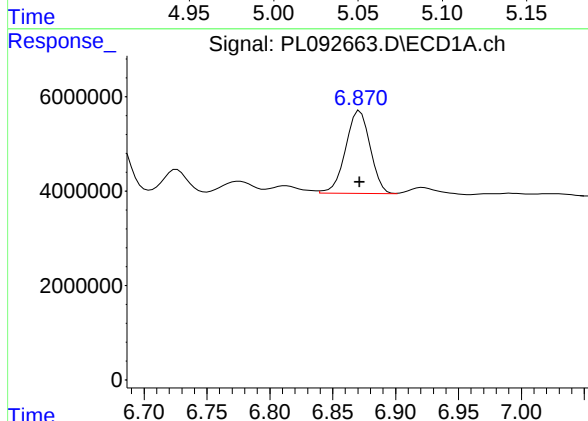


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 23829277
Conc: 260.60 ng/ml

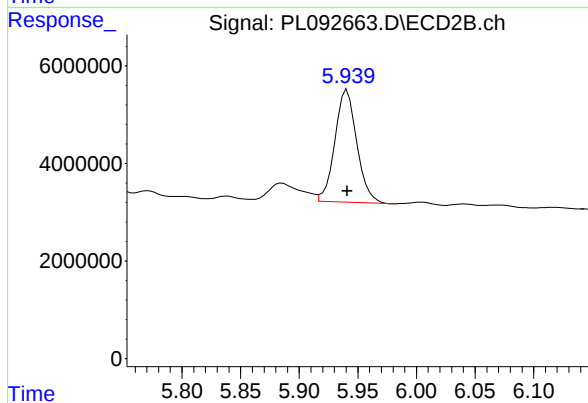

#27 Chlordane-5


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 29958197
Conc: 241.30 ng/ml

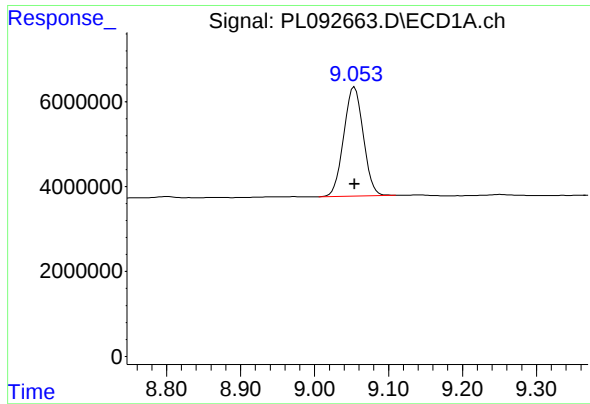

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 47238786
Conc: 26.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

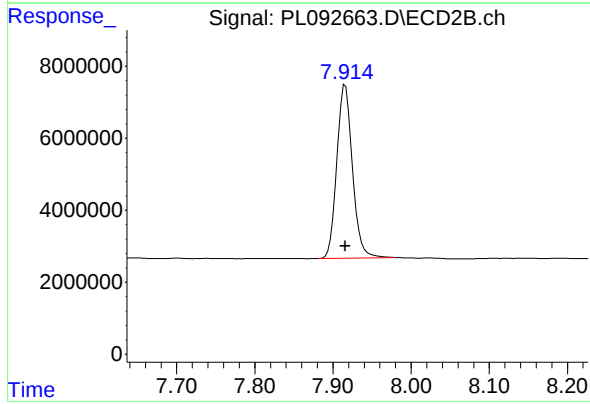

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 67136507
Conc: 25.26 ng/ml