

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 16:43
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:01:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 16:53:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.778	14129112	16871301	5.883	5.174
28) SA Decachlor...	9.052	7.916	11626851	15638742	6.138	5.684
Target Compounds						
23) Chlordane-1	4.701	3.776	6361268	5459234	57.835	51.427
24) Chlordane-2	5.231	4.353	6895253	6849165	60.161	55.301
25) Chlordane-3	5.941	4.983	23156223	17868929	59.327	49.269
26) Chlordane-4	6.023	5.045	28139408	17340131	58.868	49.570
27) Chlordane-5	6.871	5.941	5377074	6871733	56.804	54.190



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 16:43
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:01:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 16:53:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

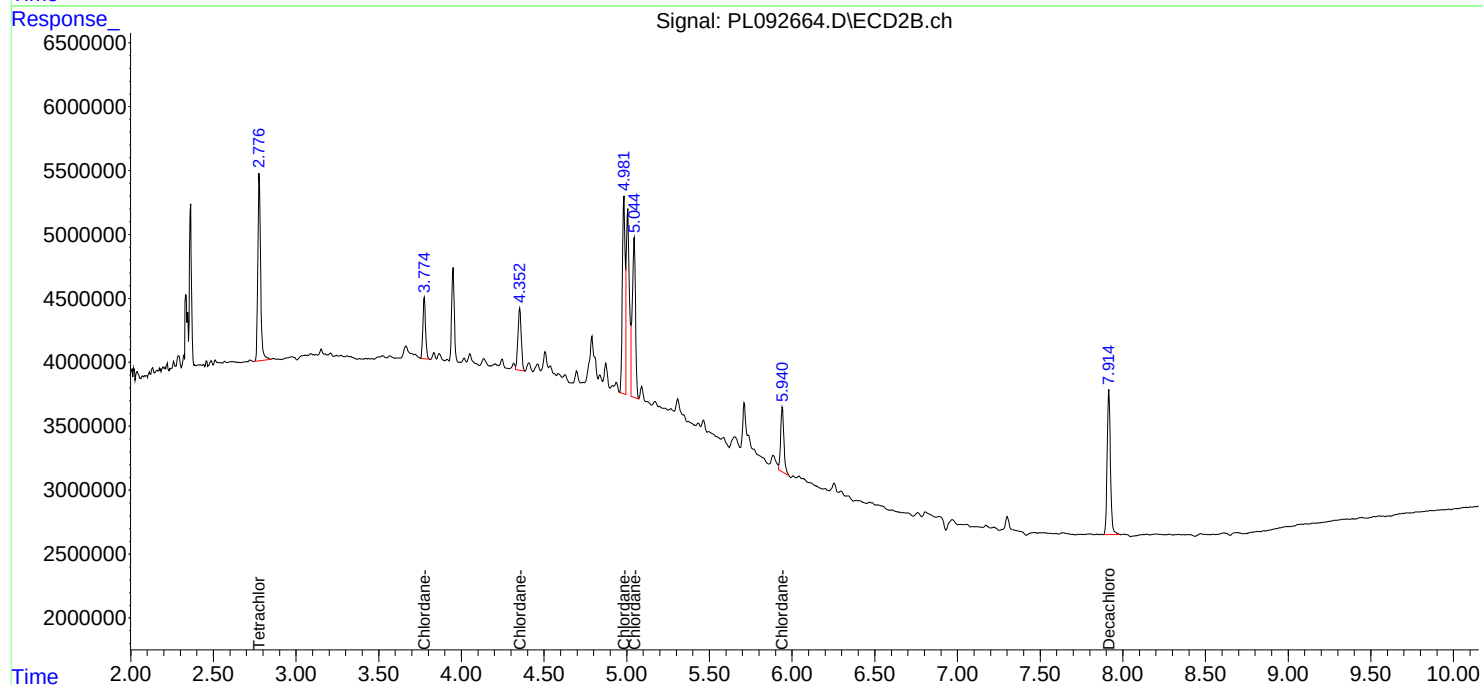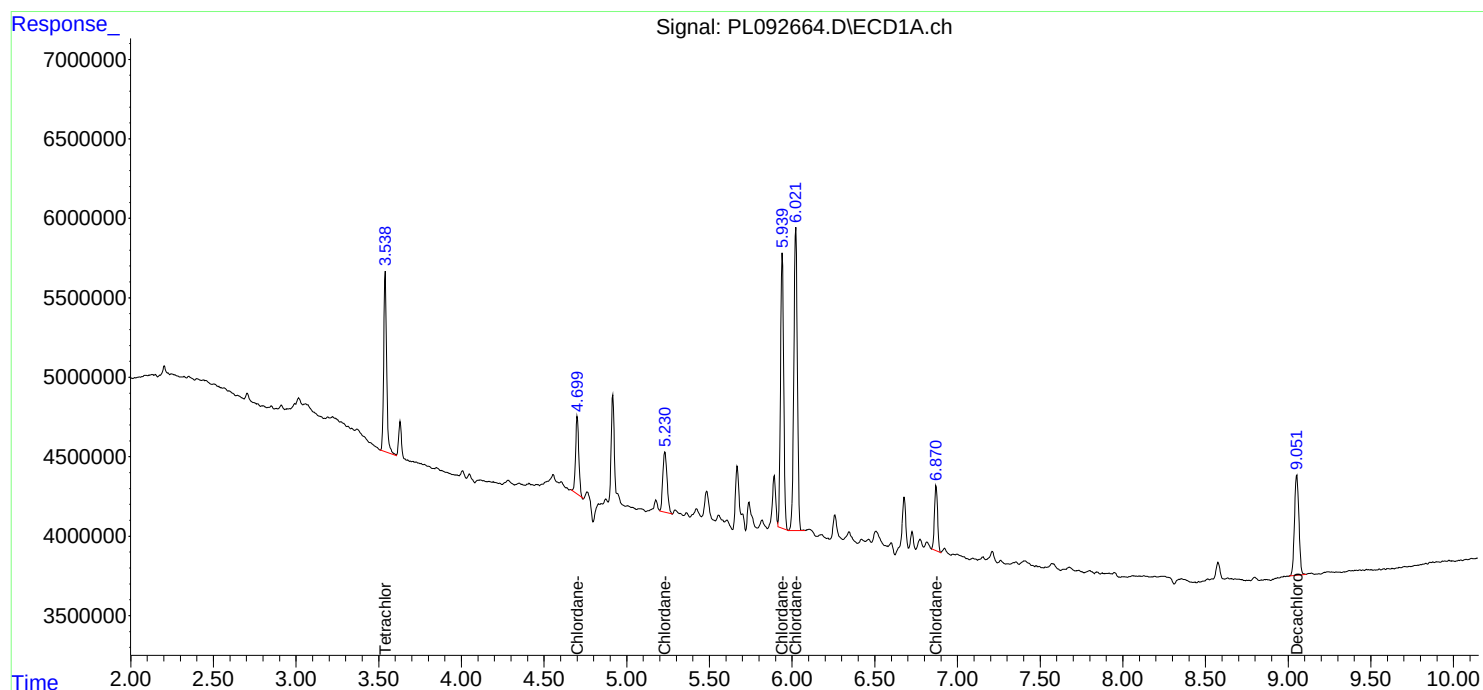


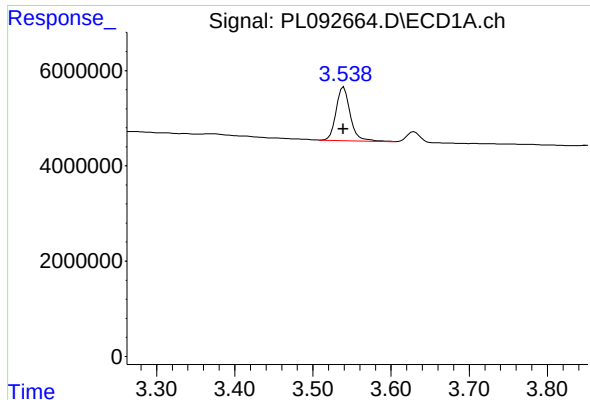

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 14129112
Conc: 5.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

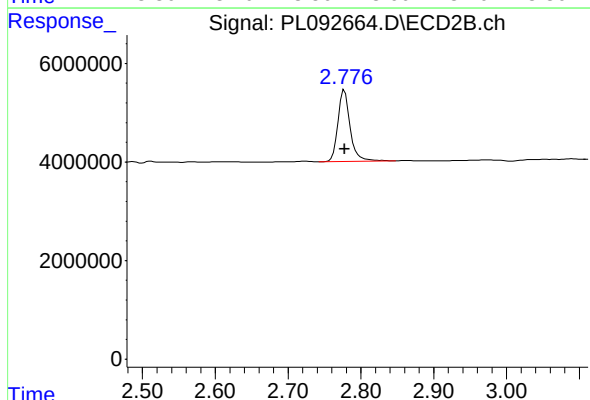


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 16871301
Conc: 5.17 ng/ml

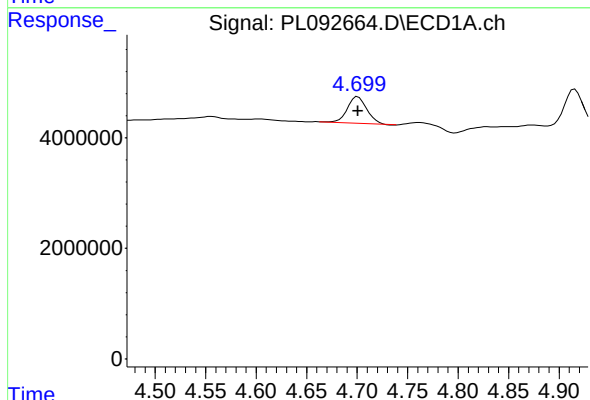


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 6361268
Conc: 57.84 ng/ml

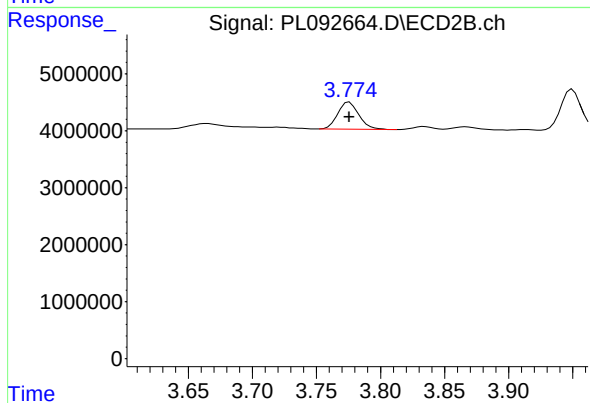

#23 Chlordane-1


R.T.: 3.776 min
Delta R.T.: 0.000 min
Response: 5459234
Conc: 51.43 ng/ml

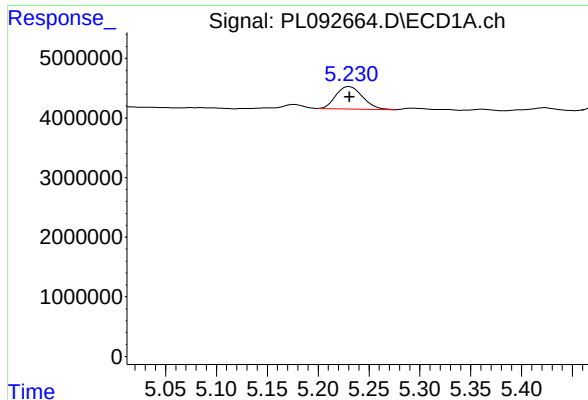

#24 Chlordane-2


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 6895253
Conc: 60.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

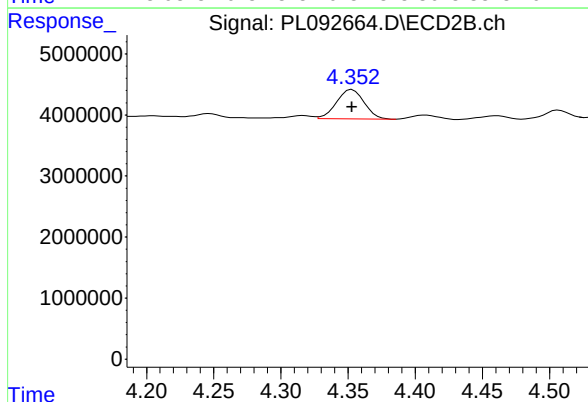


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 6849165
Conc: 55.30 ng/ml

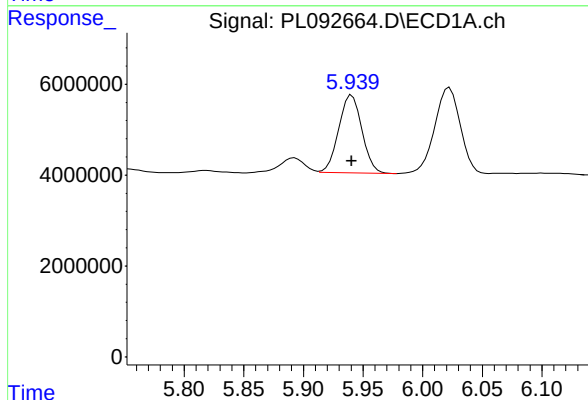


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 23156223
Conc: 59.33 ng/ml

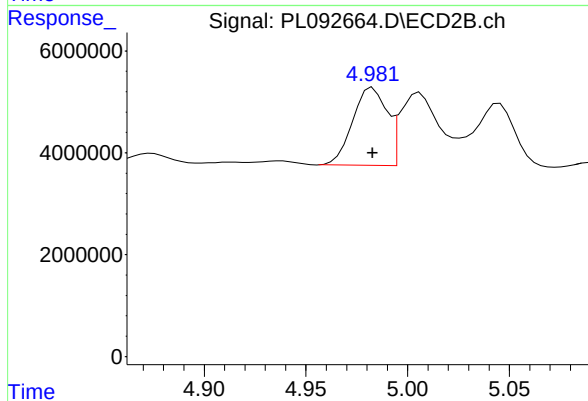

#25 Chlordane-3


R.T.: 4.983 min
Delta R.T.: 0.000 min
Response: 17868929
Conc: 49.27 ng/ml

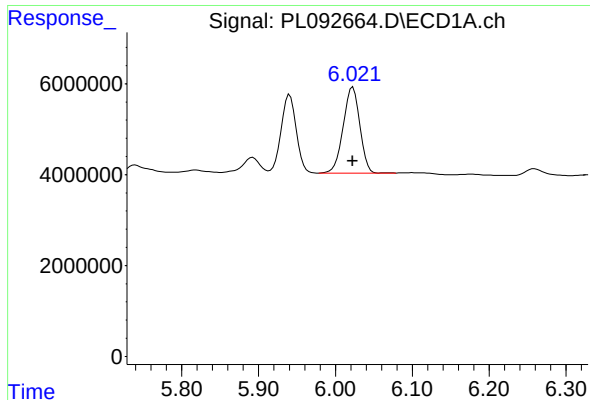

#26 Chlordane-4


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 28139408
Conc: 58.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

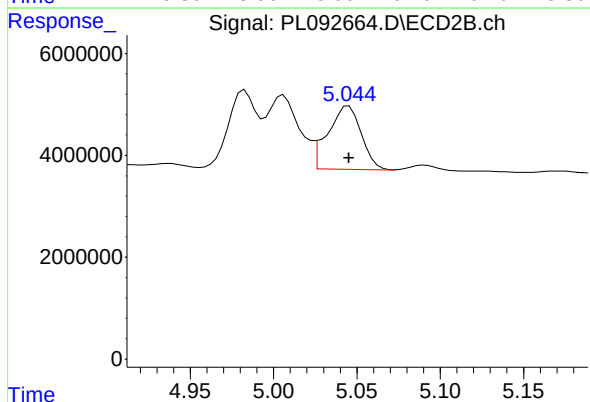


#26 Chlordane-4

R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 17340131
Conc: 49.57 ng/ml

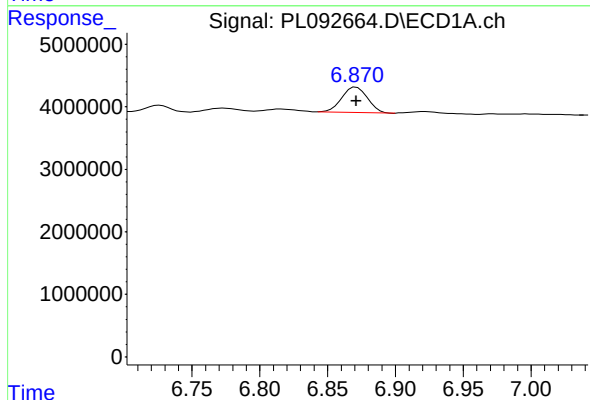


#27 Chlordane-5

R.T.: 6.871 min
Delta R.T.: 0.000 min
Response: 5377074
Conc: 56.80 ng/ml

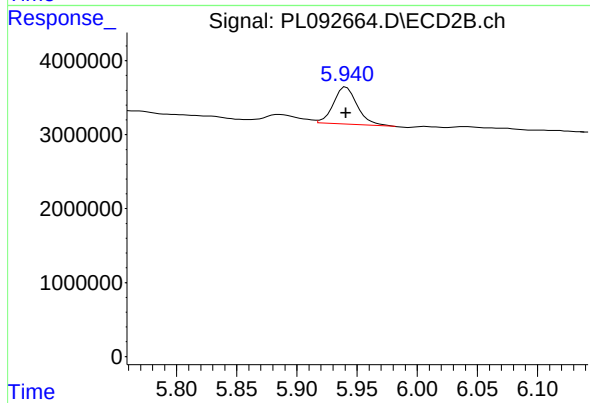

#27 Chlordane-5


R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 6871733
Conc: 54.19 ng/ml

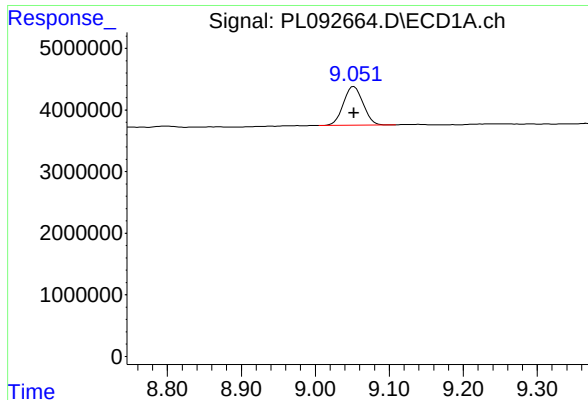

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: 0.000 min
Response: 11626851
Conc: 6.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

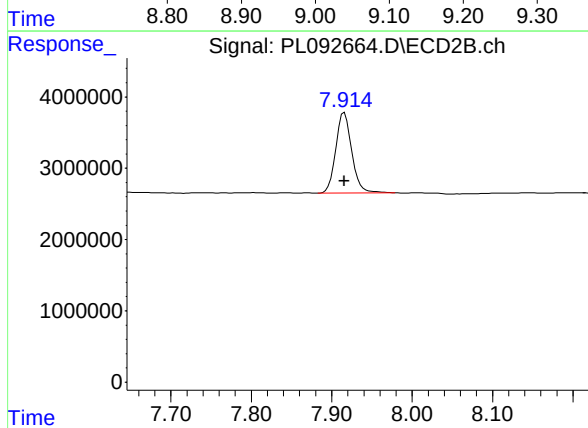

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 15638742
Conc: 5.68 ng/ml