

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 18:30
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL102824CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 18:55:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:55:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.777	116.2E6	162.6E6	48.370	49.862
28) SA Decachlor...	9.053	7.915	91212958	135.8E6	48.151	49.359
Target Compounds						
23) Chlordane-1	4.701	3.775	53586597	53029458	487.196	499.551
24) Chlordane-2	5.231	4.352	54950332	60704270	479.439	490.132
25) Chlordane-3	5.941	4.982	186.4E6	180.0E6	477.568	496.319
26) Chlordane-4	6.022	5.045	229.4E6	173.9E6	479.933	497.043
27) Chlordane-5	6.872	5.940	46544927	61748302	491.706	486.943



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 18:30
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL102824CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 18:55:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:55:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

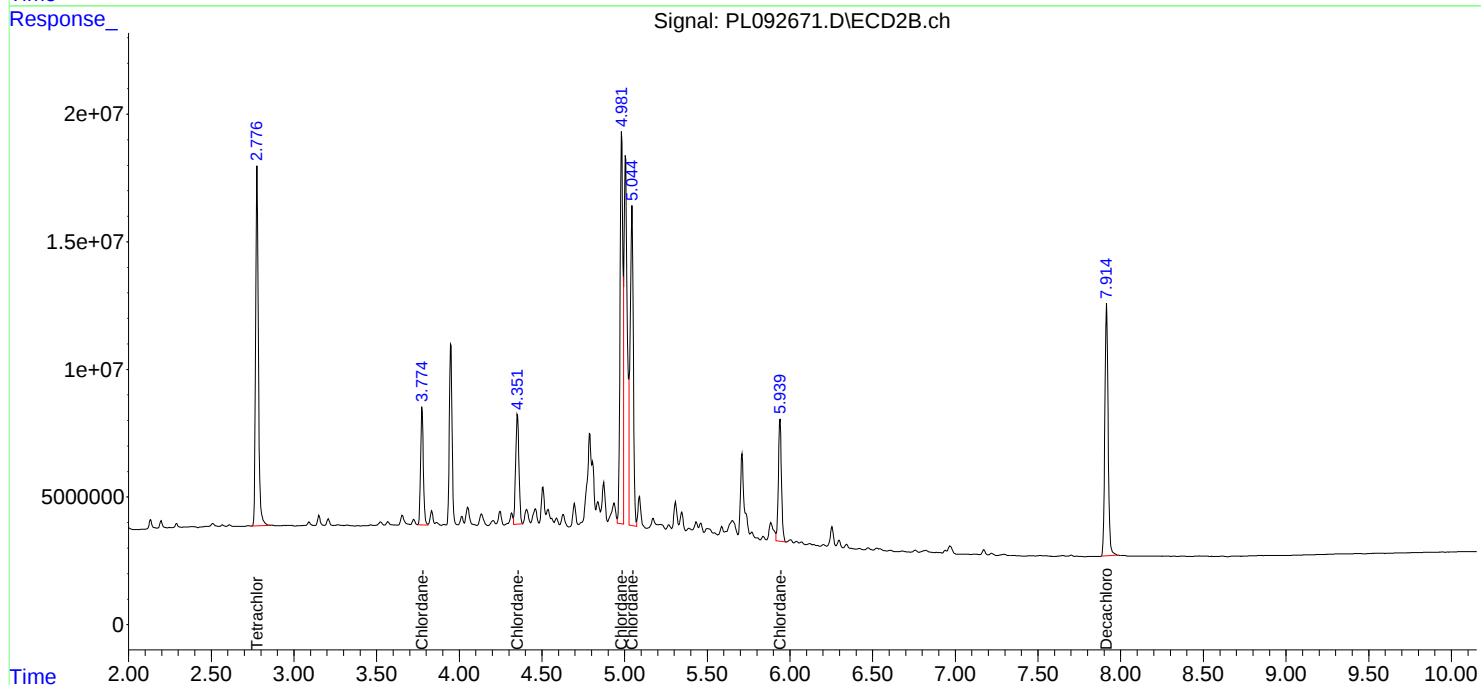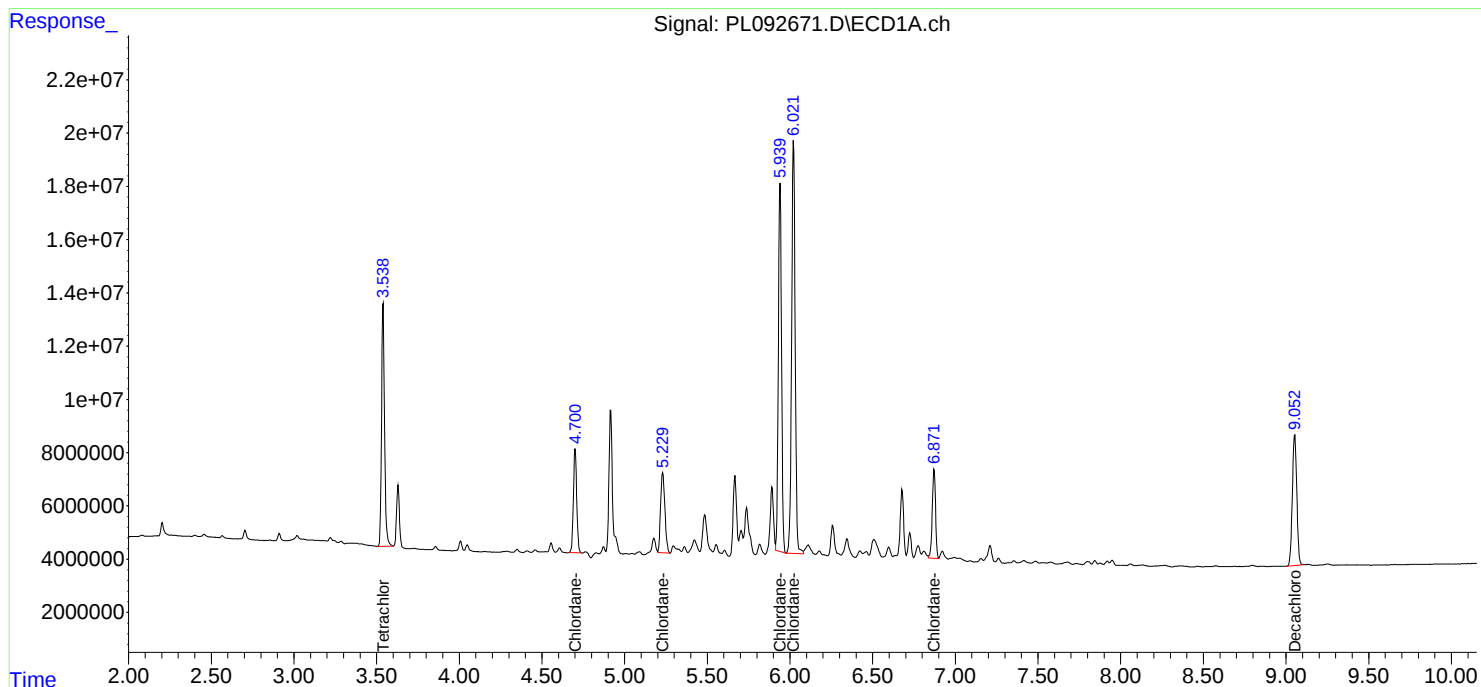


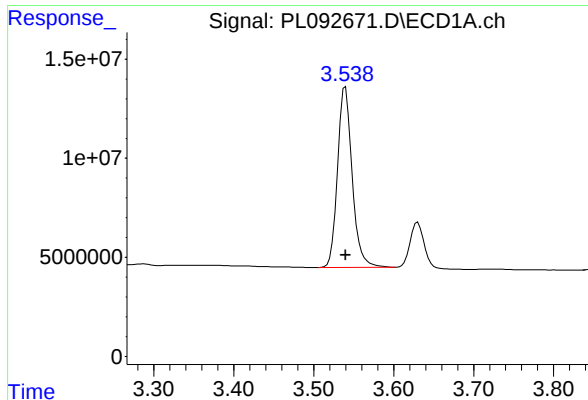

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 116172113
Conc: 48.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102824CHLOR

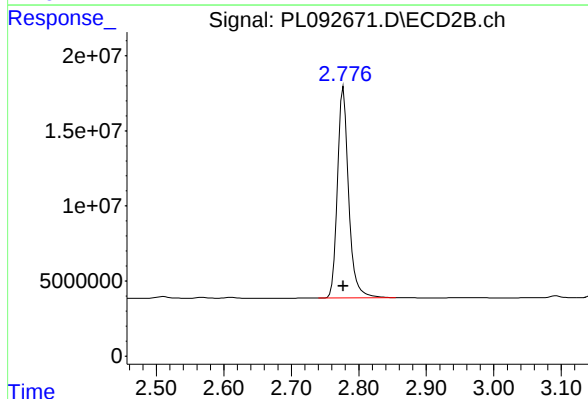


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 162586552
Conc: 49.86 ng/ml

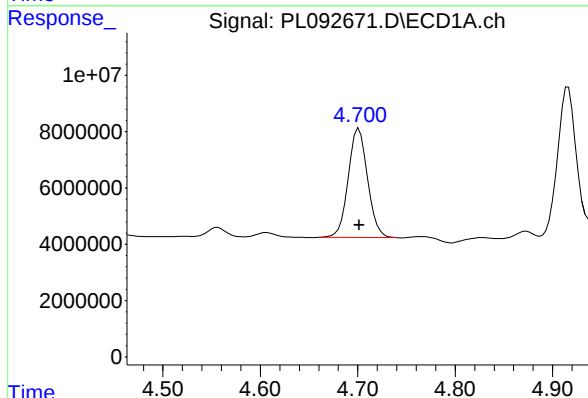


#23 Chlordane-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 53586597
Conc: 487.20 ng/ml

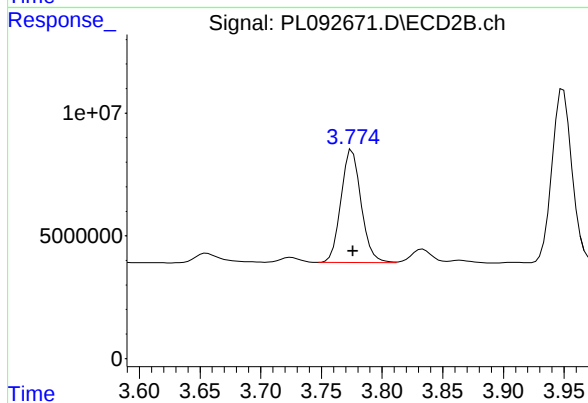

#23 Chlordane-1


R.T.: 3.775 min
Delta R.T.: 0.000 min
Response: 53029458
Conc: 499.55 ng/ml

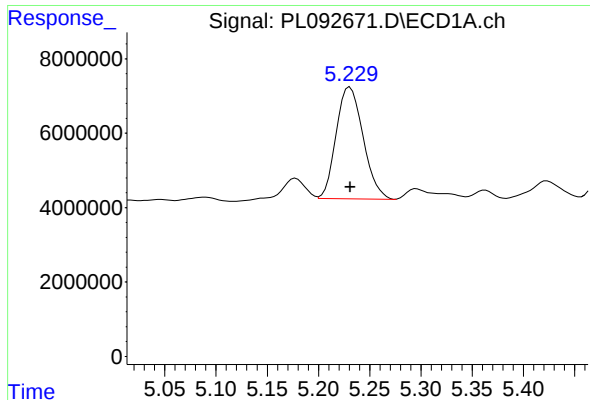

#24 Chlordane-2


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 54950332
Conc: 479.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102824CHLOR

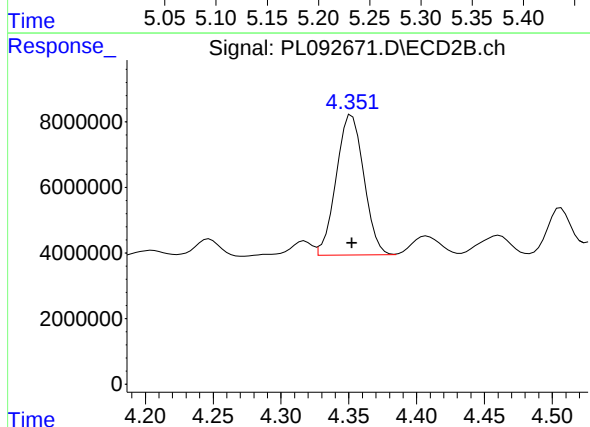


#24 Chlordane-2

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 60704270
Conc: 490.13 ng/ml

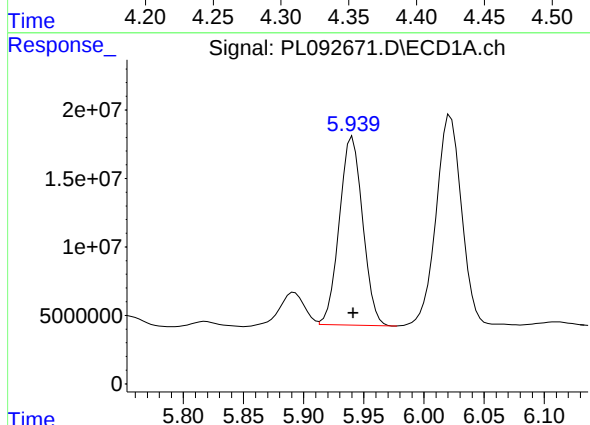


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 186402299
Conc: 477.57 ng/ml

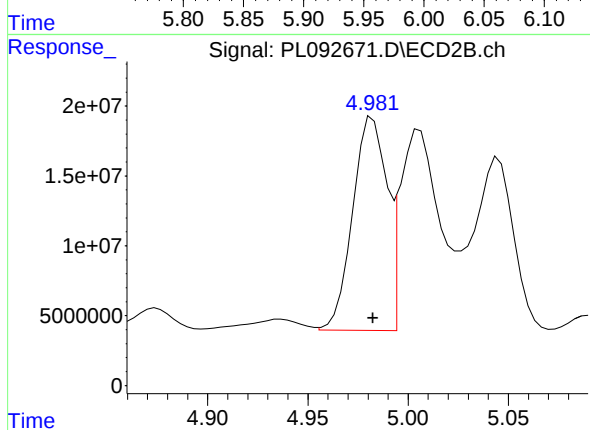

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 180006321
Conc: 496.32 ng/ml

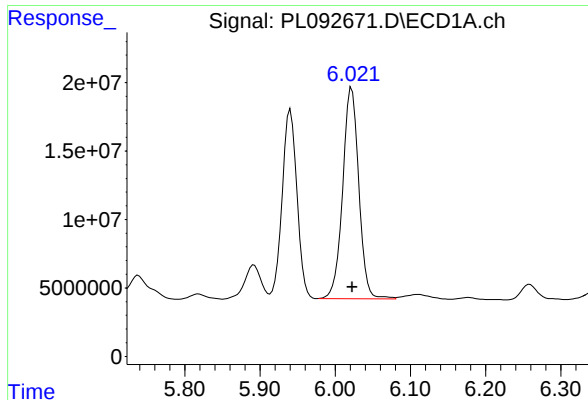

#26 Chlordane-4


R.T.: 6.022 min
Delta R.T.: -0.001 min
Response: 229410745
Conc: 479.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102824CHLOR

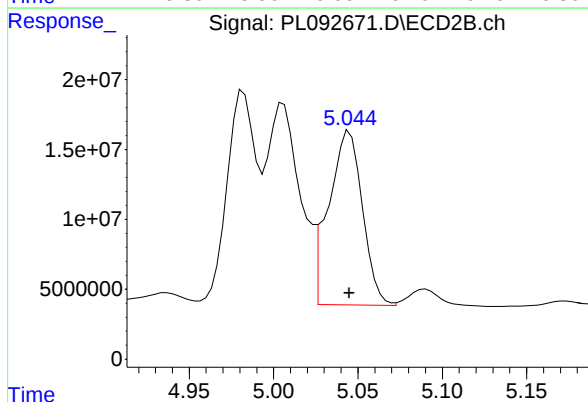


#26 Chlordane-4

R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 173872534
Conc: 497.04 ng/ml

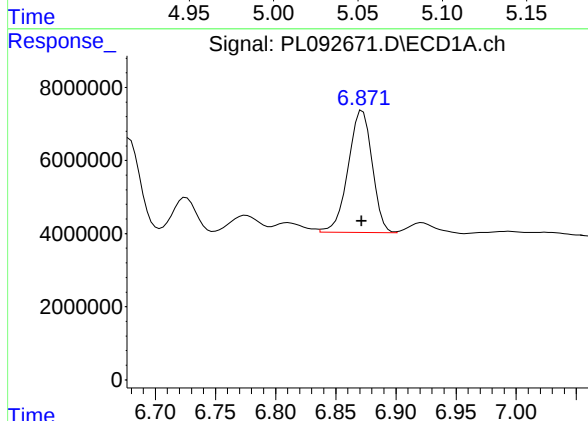


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 46544927
Conc: 491.71 ng/ml

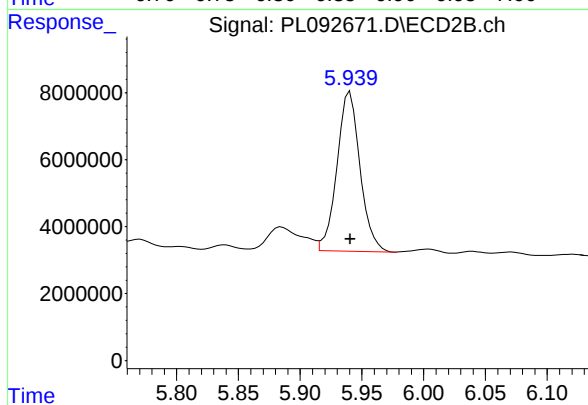

#27 Chlordane-5


R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 61748302
Conc: 486.94 ng/ml

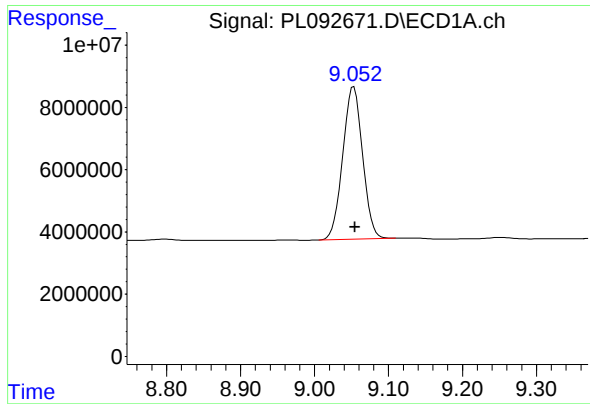

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.002 min
Response: 91212958
Conc: 48.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL102824CHLOR

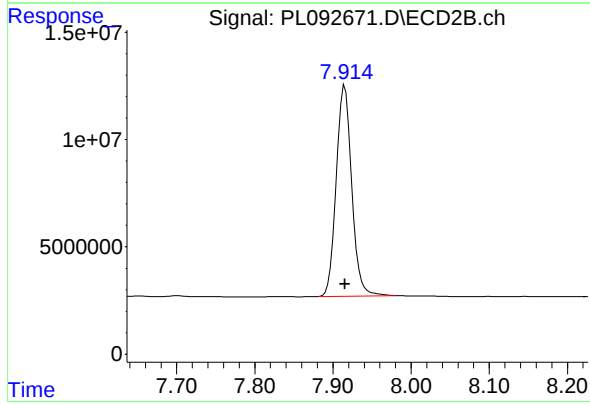

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 135815823
Conc: 49.36 ng/ml