

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 22:58
 Operator : AR\AJ
 Sample : P4561-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BP-F-18

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/29/2024
 Supervised By :Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:50:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.777	47203417	53930779	19.265m	19.819m
28) SA Decachlor...	9.052	7.915	32894990	46880189	17.092m	17.177

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 22:58
Operator : AR\AJ
Sample : P4561-05
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BP-F-18


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/29/2024
Supervised By : Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:50:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

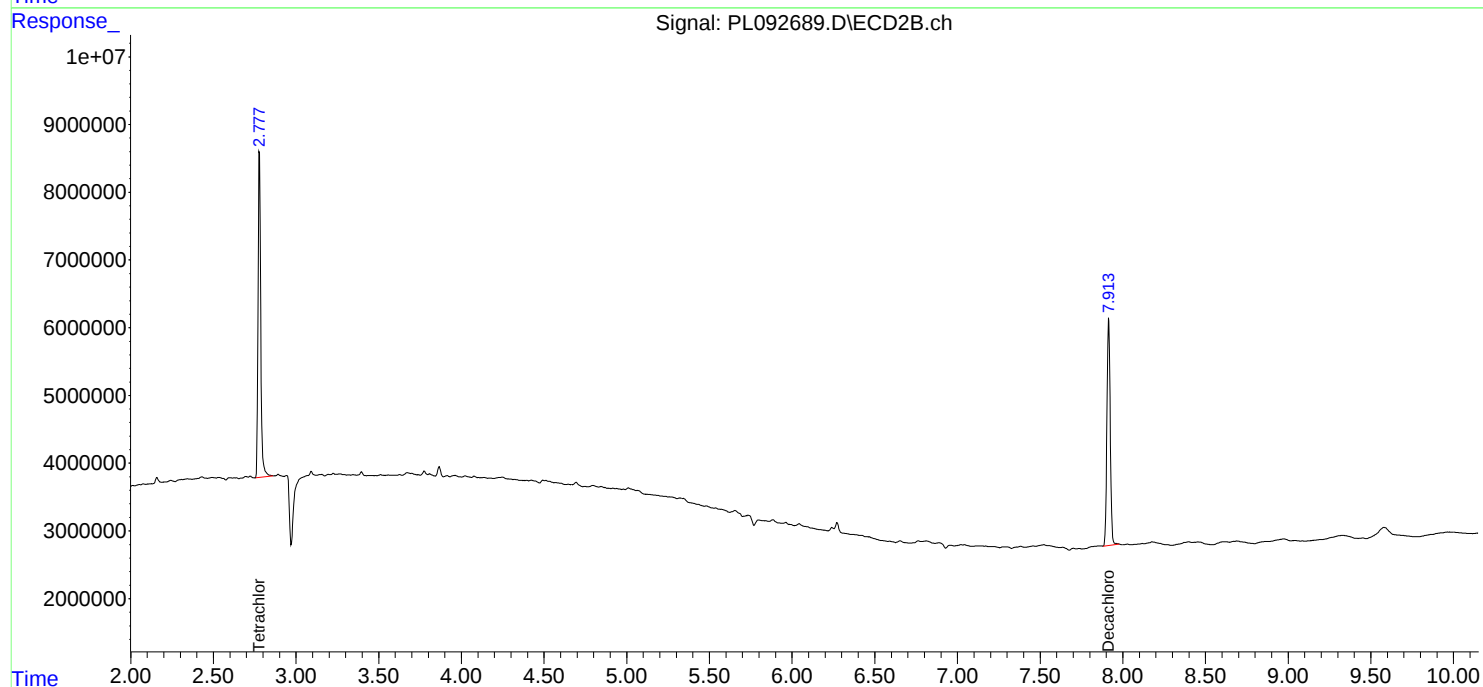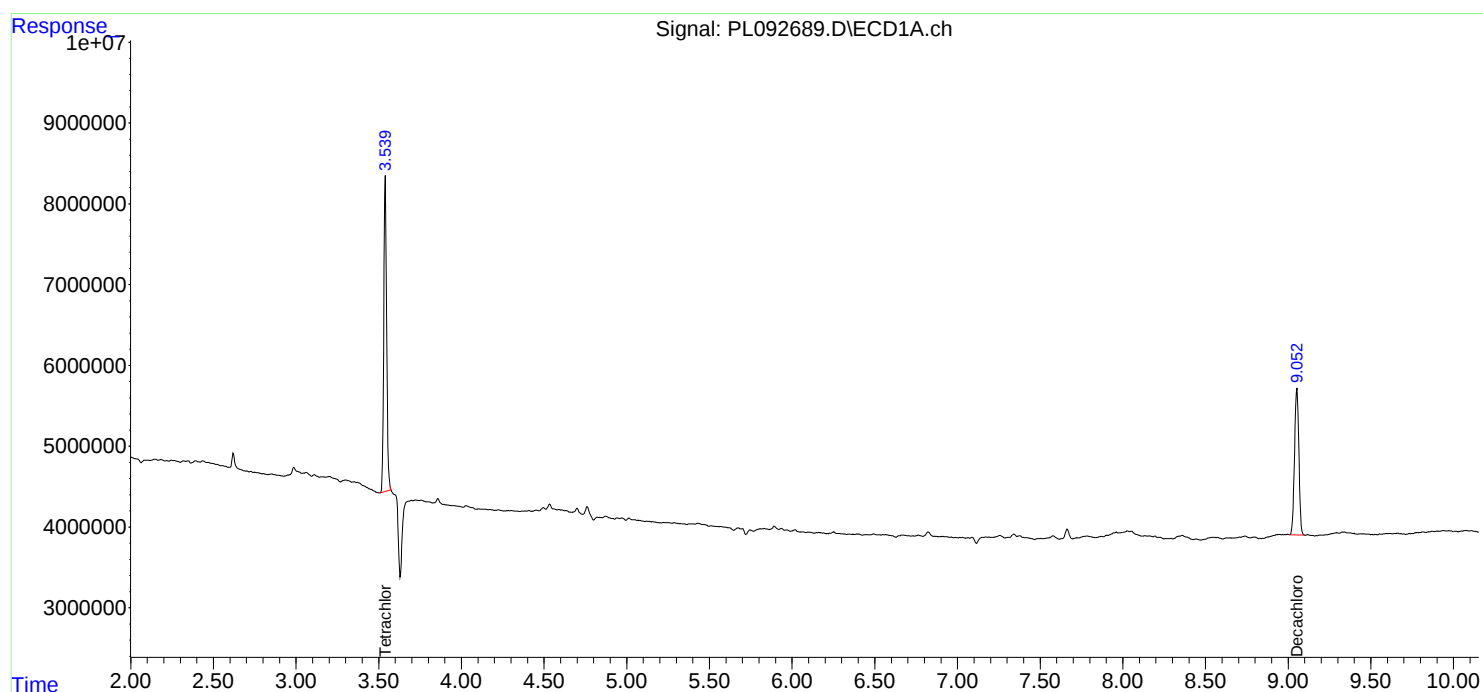

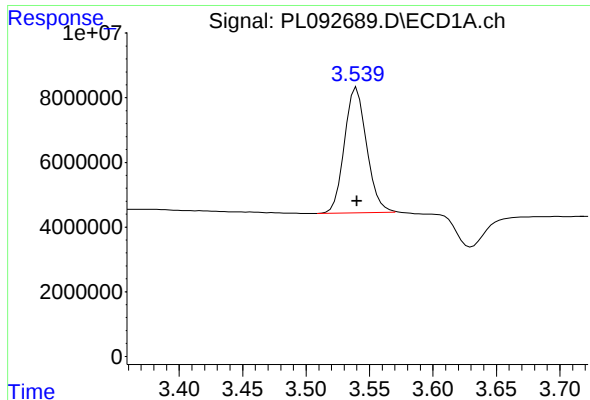


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.001 min
Response: 47203417
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
BP-F-18


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/29/2024
Supervised By :Ankita Jodhani 10/29/2024

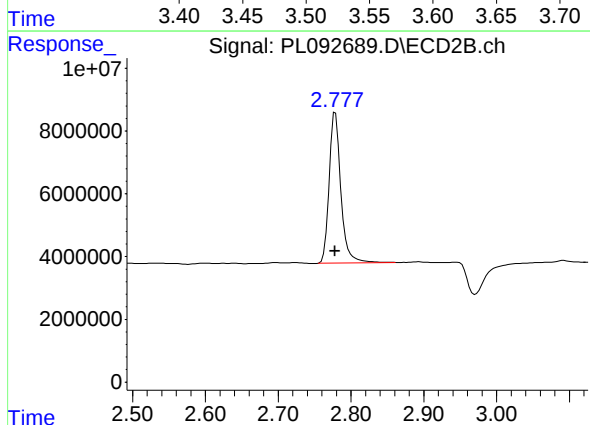


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 53930779
Conc: 19.82 ng/ml

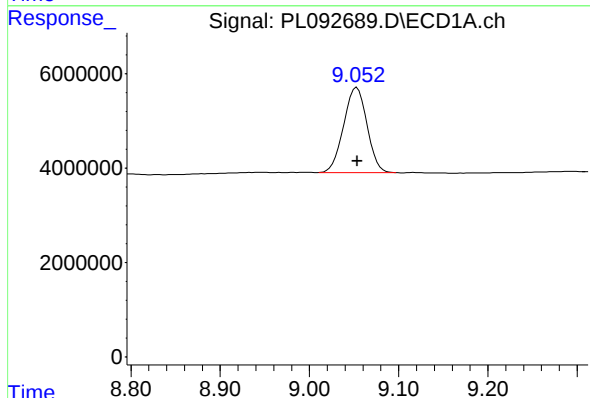

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.002 min
Response: 32894990
Conc: 17.09 ng/ml

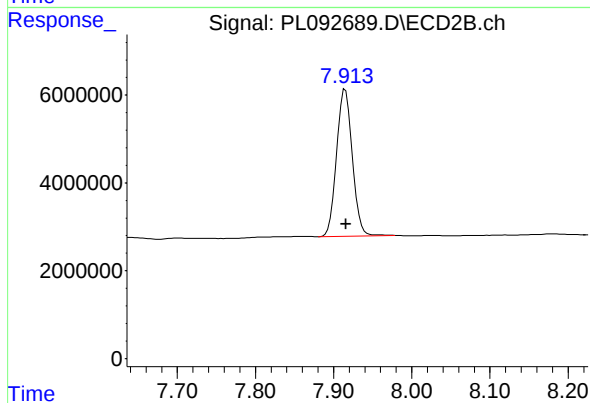

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 46880189
Conc: 17.18 ng/ml