

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
 Data File : PL097638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 14:44
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:16:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 17:14:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	2.822	68653611	102.2E6	16.778	16.983
28)	SA Decachlor...	8.993	7.979	55990964	100.3E6	18.819	18.769
Target Compounds							
9)	A Endosulfan I	6.028	5.159	36611647	60316785	7.260	8.012
10)	B gamma-Chl...	5.900	5.040	40477496	84144133	7.383	9.723 #
12)	B 4,4'-DDE	6.151	5.292	71991085	121.8E6	15.686	15.884
13)	MA Dieldrin	6.300	5.423	82160157	124.7E6	15.324	15.515
18)	B Endrin al...	0.000	6.168	0	9995432	N.D.	1.737 #
19)	B Endosulfa...	7.102	6.391	62699483	107.9E6	16.038	15.988
20)	A Methoxychlor	7.447	6.669	158.5E6	283.7E6	77.677	76.355
21)	B Endrin ke...	7.581	6.895	66312303	118.5E6	15.930	15.916
25)	Chlordane-3	5.900	5.040	40477496	84144133	48.636	94.365 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
Data File : PL097638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 14:44
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:16:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 17:14:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

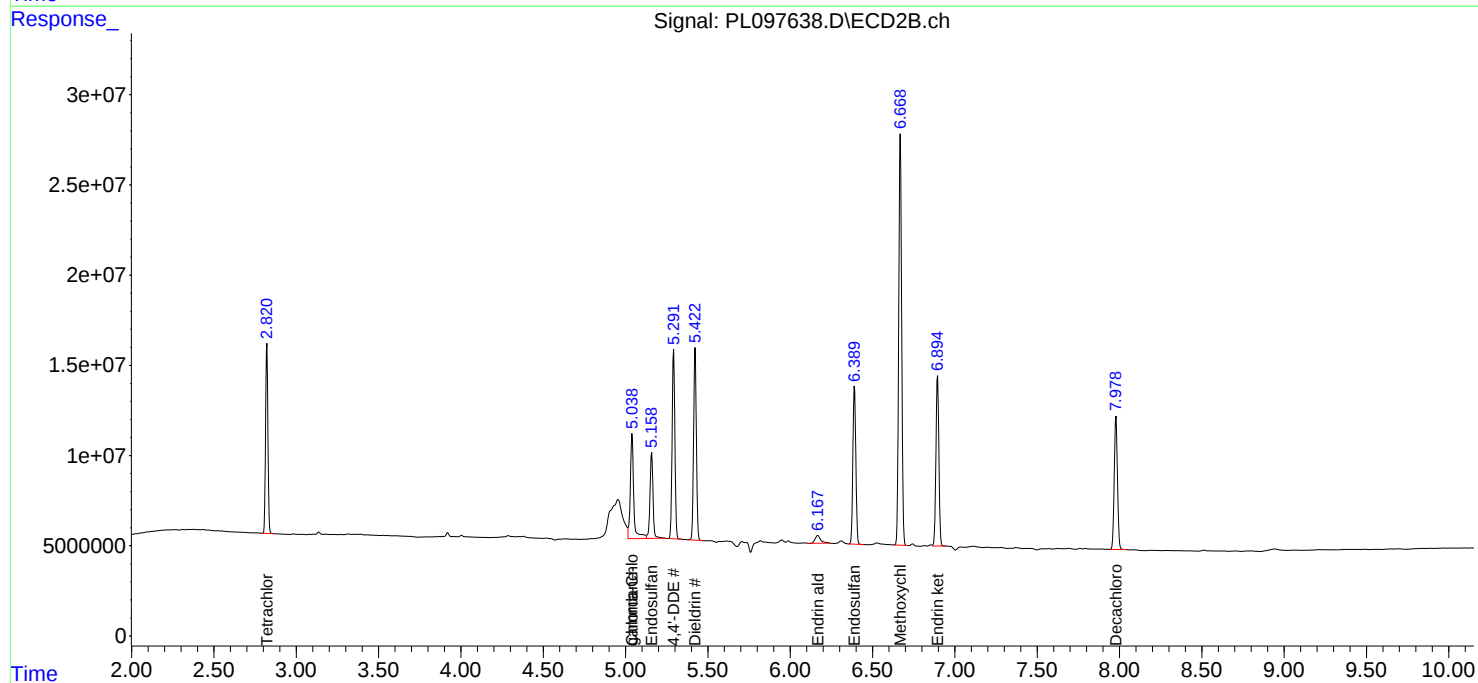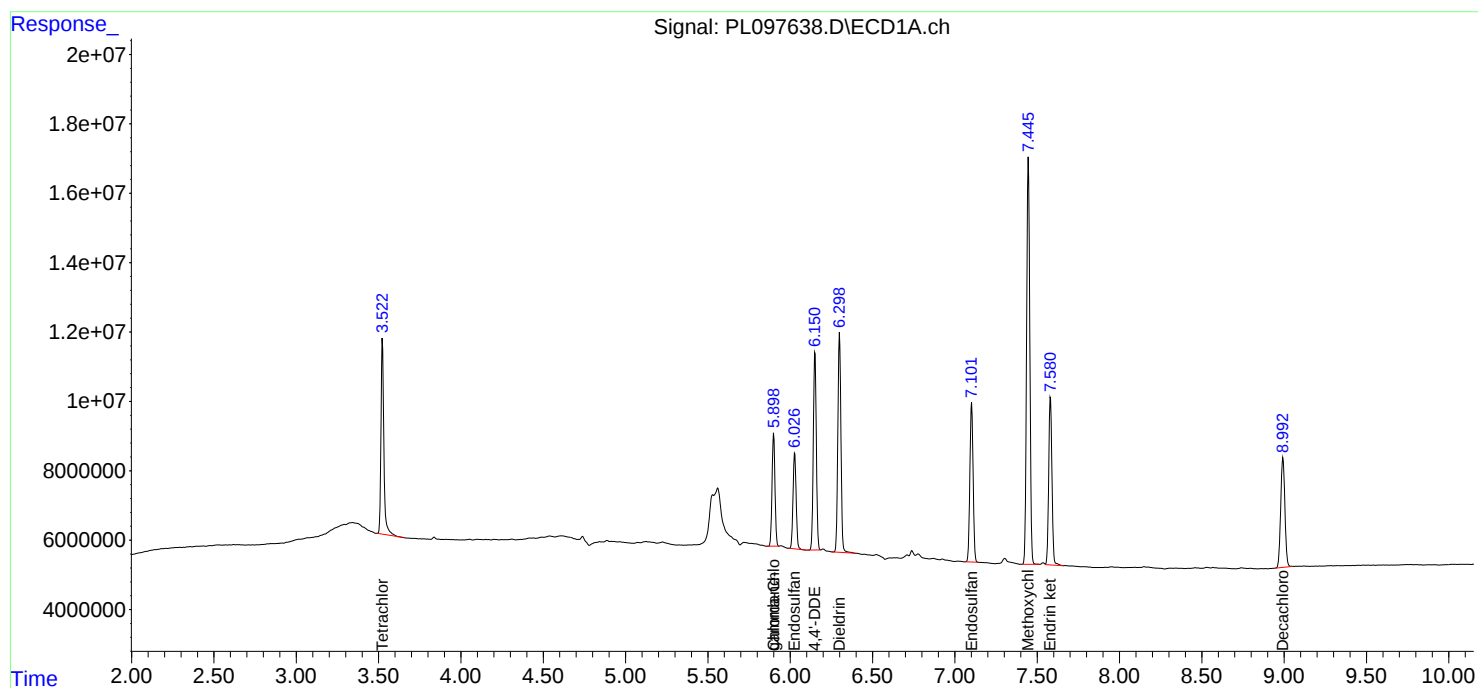


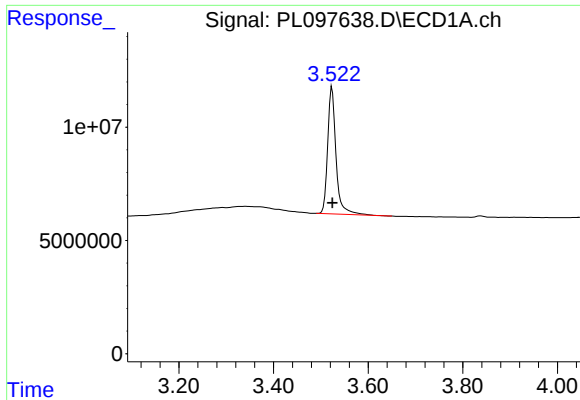

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 68653611
Conc: 16.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

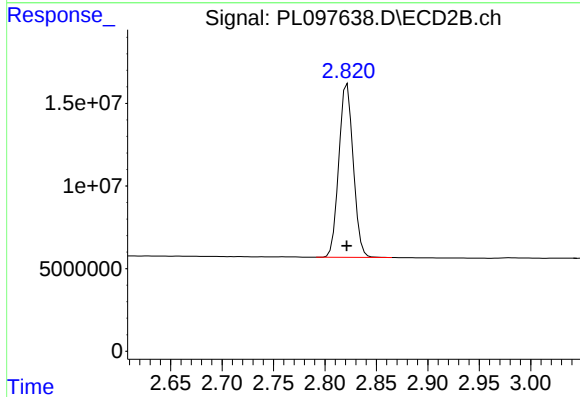


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 102218408
Conc: 16.98 ng/ml

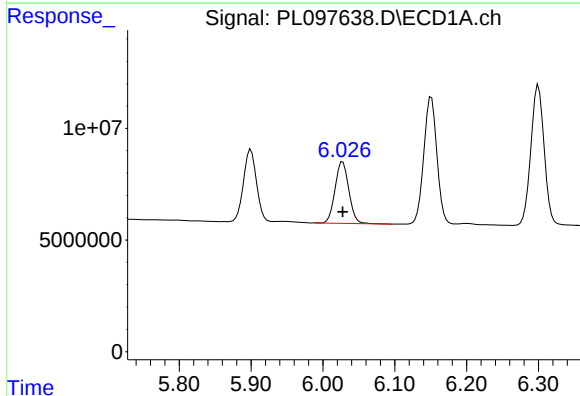


#9 Endosulfan I

R.T.: 6.028 min
Delta R.T.: 0.000 min
Response: 36611647
Conc: 7.26 ng/ml

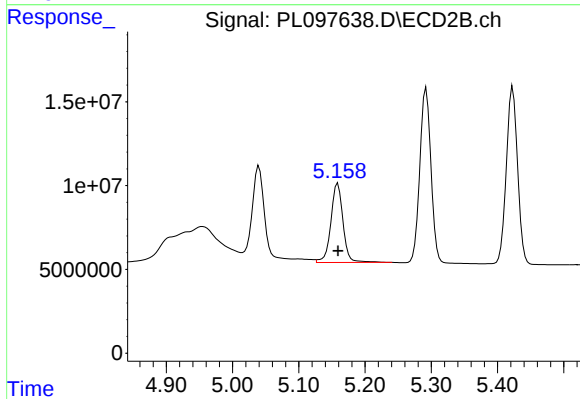

#9 Endosulfan I


R.T.: 5.159 min
Delta R.T.: 0.000 min
Response: 60316785
Conc: 8.01 ng/ml

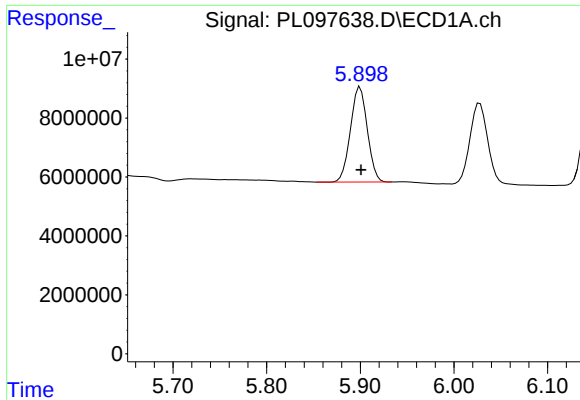

#10 gamma-Chlordane


R.T.: 5.900 min
Delta R.T.: -0.001 min
Response: 40477496
Conc: 7.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

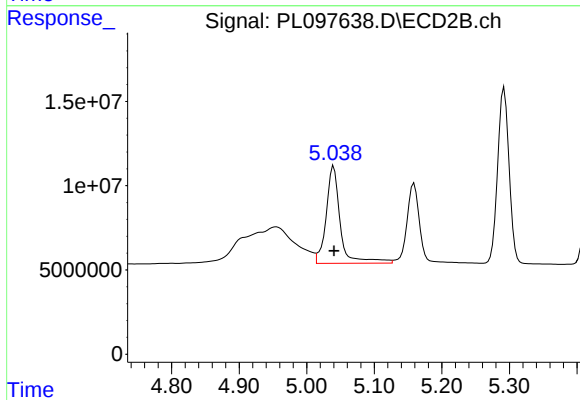


#10 gamma-Chlordane

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 84144133
Conc: 9.72 ng/ml

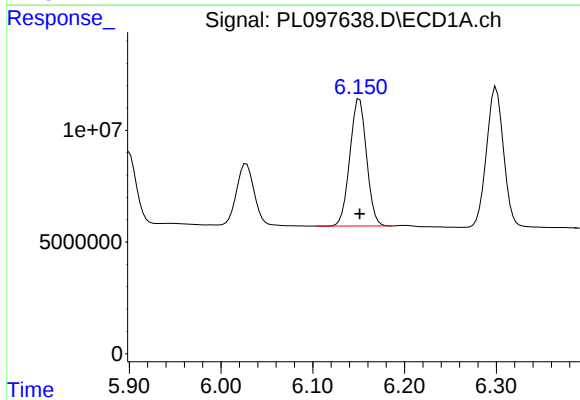


#12 4,4'-DDE

R.T.: 6.151 min
Delta R.T.: 0.000 min
Response: 71991085
Conc: 15.69 ng/ml

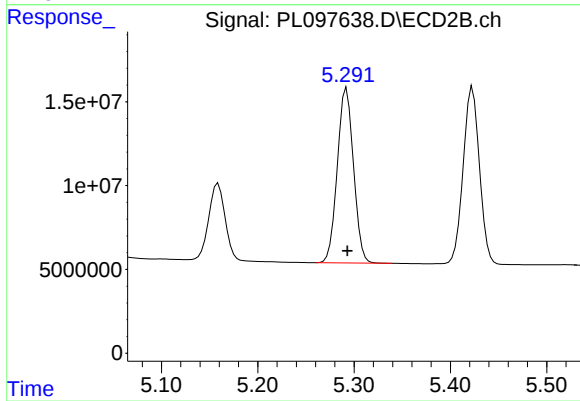

#12 4,4'-DDE


R.T.: 5.292 min
Delta R.T.: 0.000 min
Response: 121753063
Conc: 15.88 ng/ml

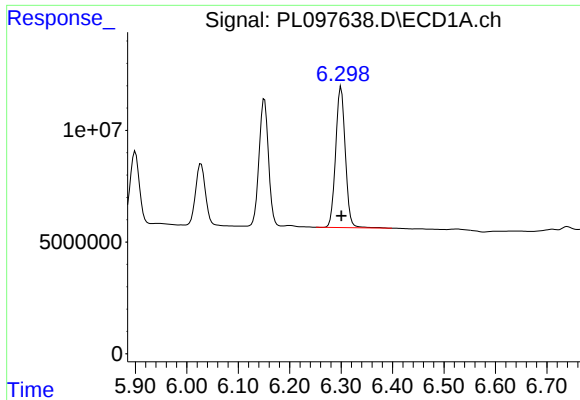

#13 Dieldrin


R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 82160157
Conc: 15.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

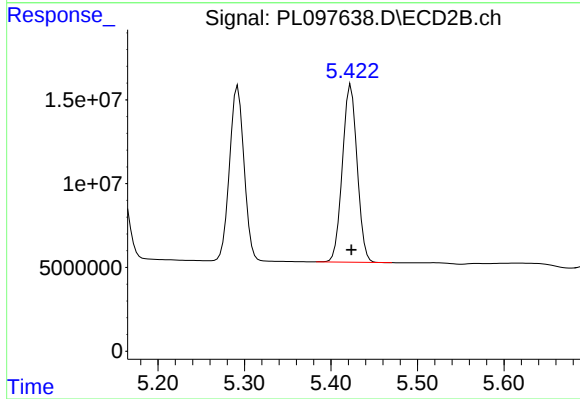


#13 Dieldrin

R.T.: 5.423 min
Delta R.T.: 0.000 min
Response: 124735883
Conc: 15.52 ng/ml

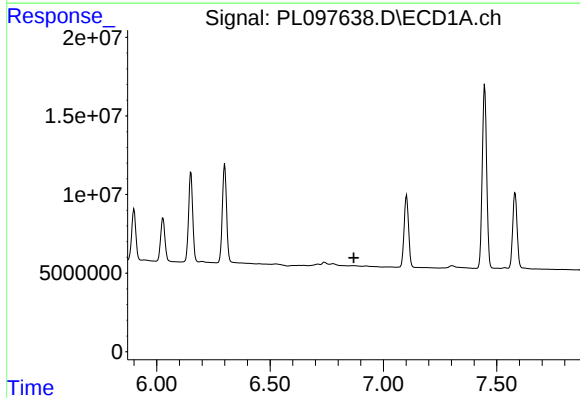


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.869 min
Response: 0
Conc: N.D.

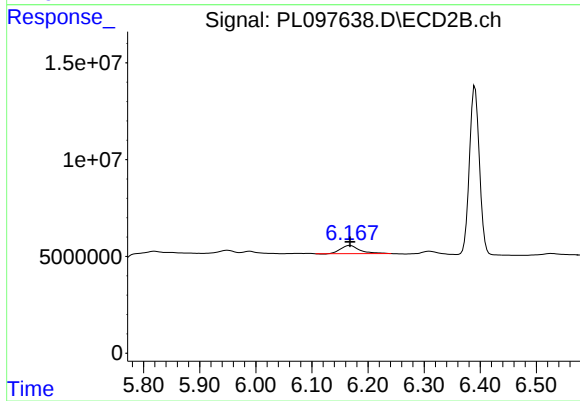

#18 Endrin aldehyde


R.T.: 6.168 min
Delta R.T.: 0.000 min
Response: 9995432
Conc: 1.74 ng/ml

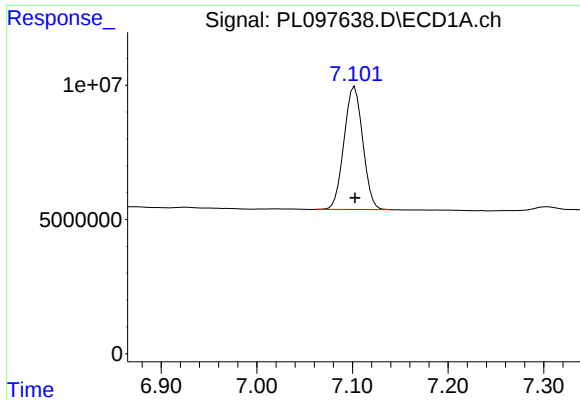

#19 Endosulfan Sulfate


R.T.: 7.102 min
Delta R.T.: 0.000 min
Response: 62699483
Conc: 16.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

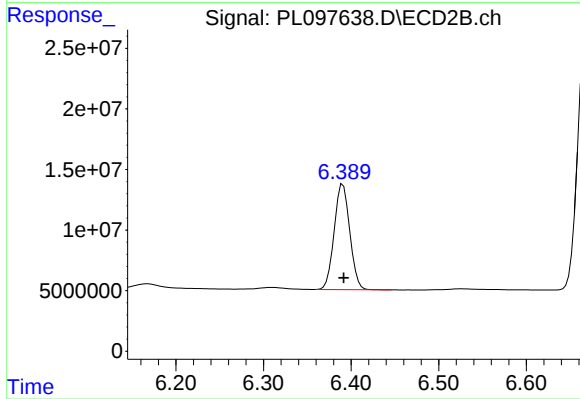


#19 Endosulfan Sulfate

R.T.: 6.391 min
Delta R.T.: 0.000 min
Response: 107859245
Conc: 15.99 ng/ml

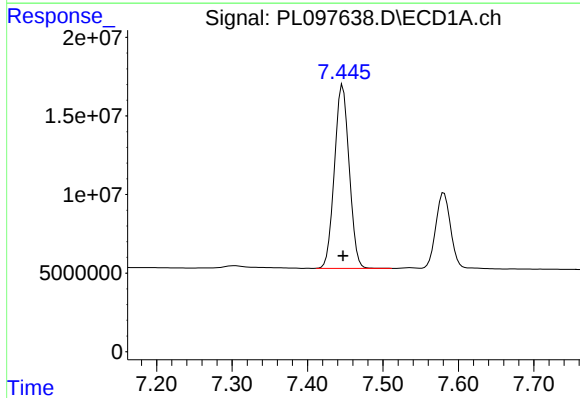


#20 Methoxychlor

R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 158524994
Conc: 77.68 ng/ml

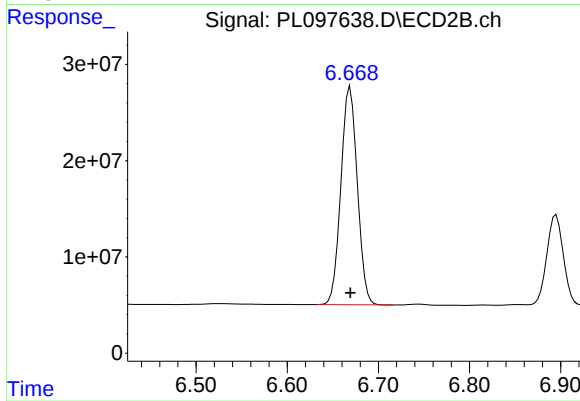

#20 Methoxychlor


R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 283678129
Conc: 76.35 ng/ml

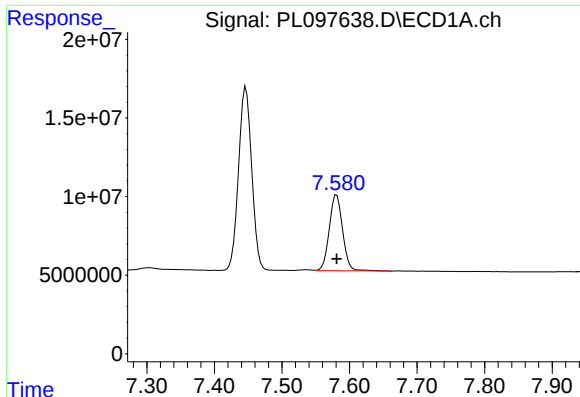

#21 Endrin ketone


R.T.: 7.581 min
Delta R.T.: 0.000 min
Response: 66312303
Conc: 15.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

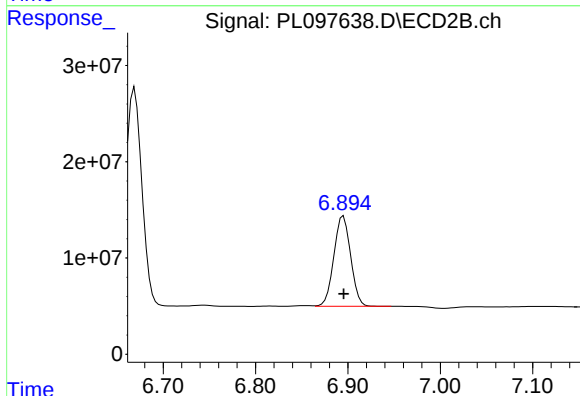


#21 Endrin ketone

R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 118479033
Conc: 15.92 ng/ml

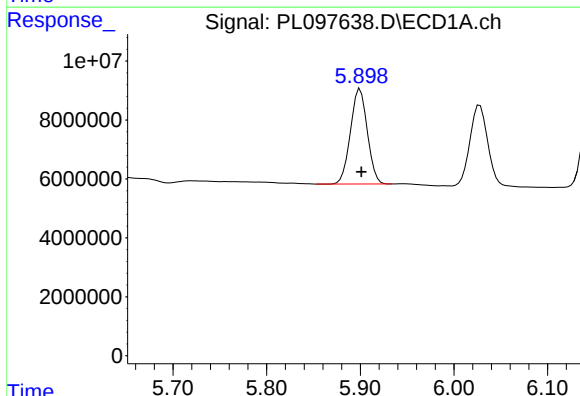


#25 Chlordane-3

R.T.: 5.900 min
Delta R.T.: -0.001 min
Response: 40477496
Conc: 48.64 ng/ml

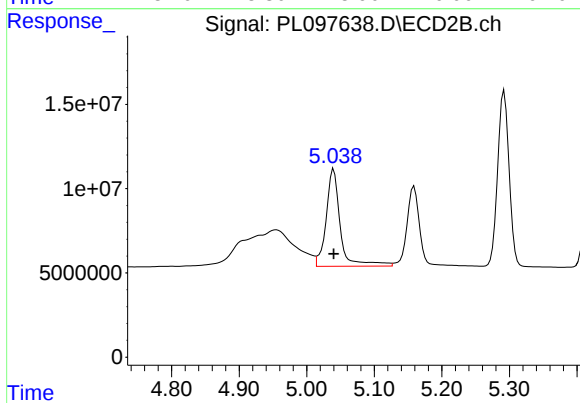

#25 Chlordane-3

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 84144133
Conc: 94.37 ng/ml

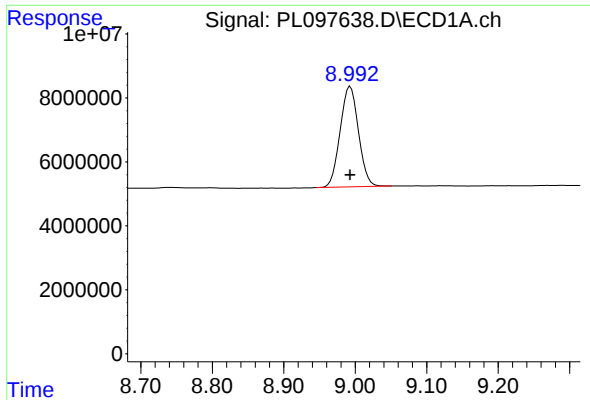

#28 Decachlorobiphenyl


R.T.: 8.993 min

Delta R.T.: 0.000 min

Response: 55990964

Conc: 18.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

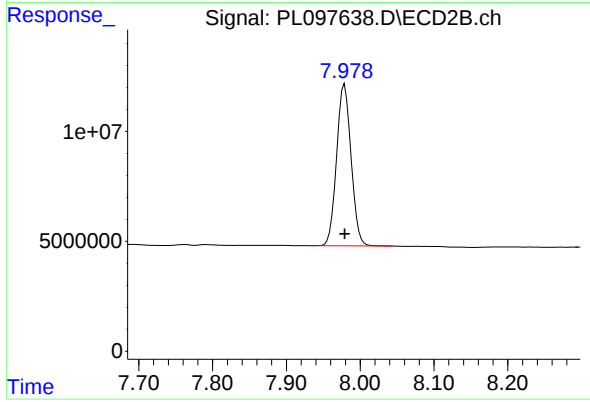

#28 Decachlorobiphenyl

R.T.: 7.979 min

Delta R.T.: 0.000 min

Response: 100316045

Conc: 18.77 ng/ml