

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
 Data File : PL097644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 16:05
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 16:59:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 16:57:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	2.821	358.5E6	658.5E6	99.614	99.648
28)	SA Decachlor...	8.993	7.979	244.9E6	440.5E6	98.133	97.500
Target Compounds							
23)	Chlordane-1	4.675	3.830	197.4E6	236.2E6	999.520	1001.508
24)	Chlordane-2	5.199	4.408	208.0E6	256.7E6	974.239	982.573
25)	Chlordane-3	5.901	5.041	807.0E6	822.6E6	1001.278	995.008
26)	Chlordane-4	5.986	5.104	977.0E6	723.4E6	993.286	996.984
27)	Chlordane-5	6.822	5.997	159.8E6	282.6E6	1001.396	1001.053



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
Data File : PL097644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 16:05
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 16:59:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 16:57:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

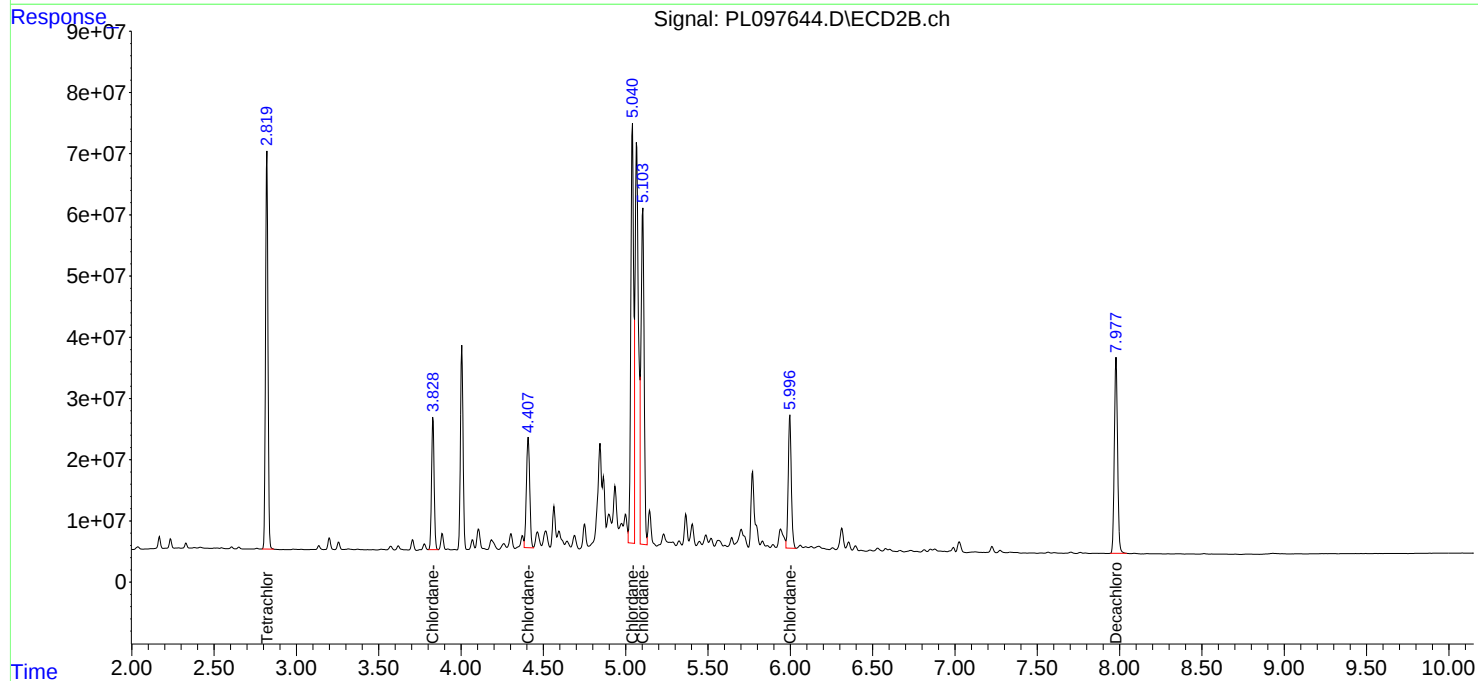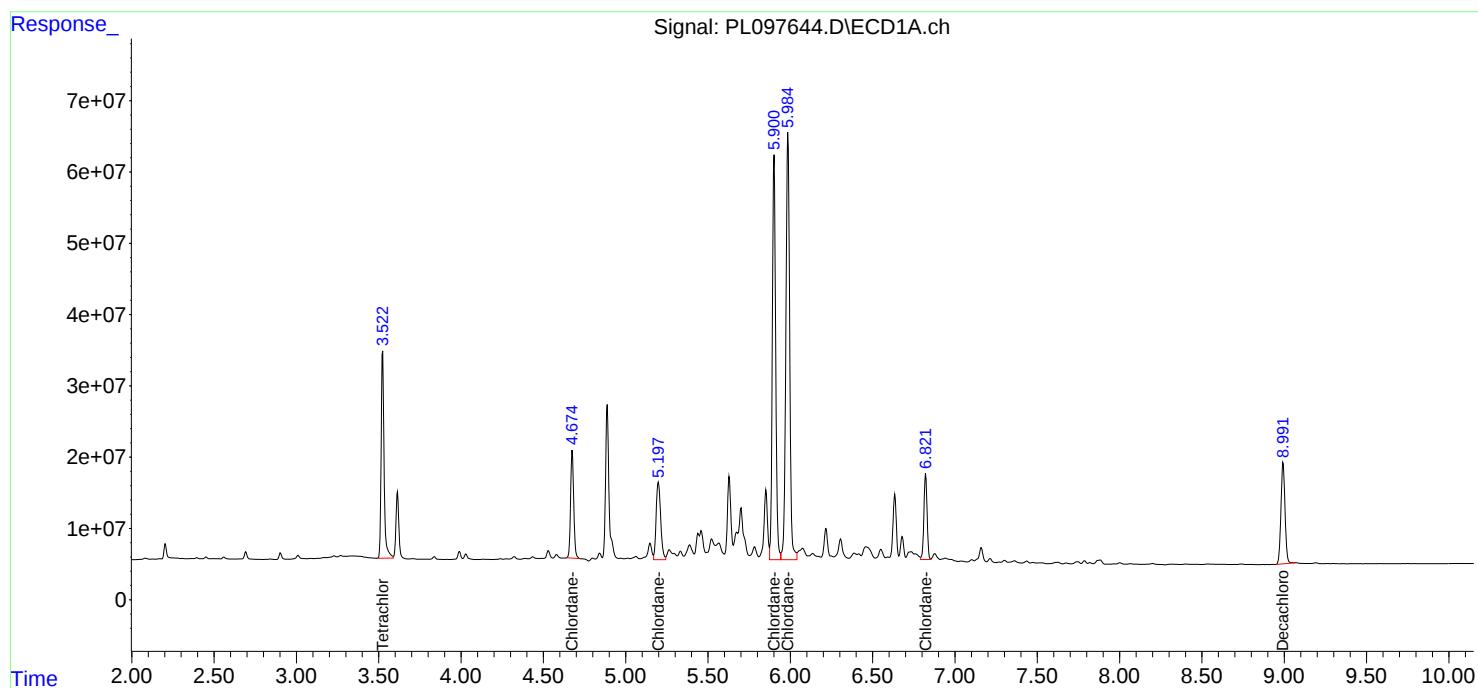


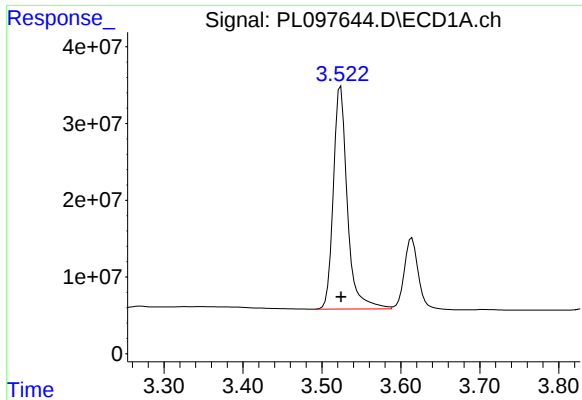

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 358504524
Conc: 99.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

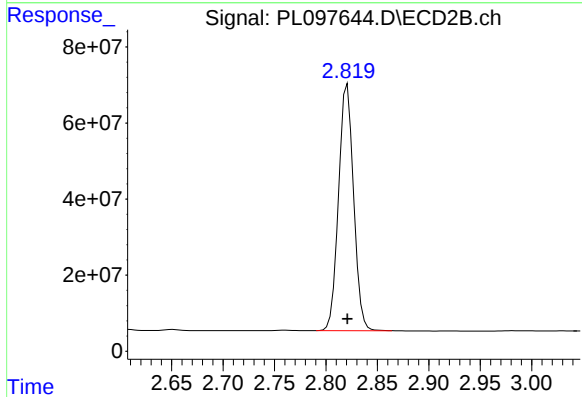


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: 0.000 min
Response: 658512299
Conc: 99.65 ng/ml

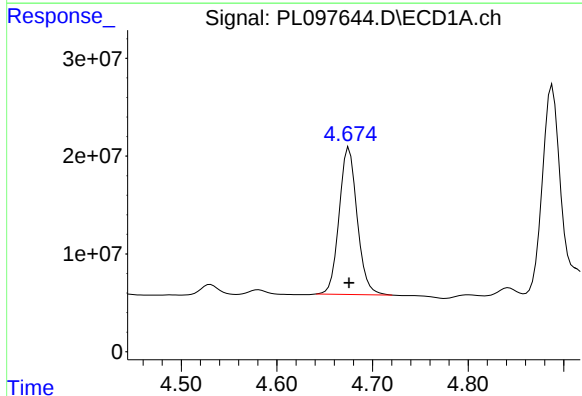


#23 Chlordane-1

R.T.: 4.675 min
Delta R.T.: 0.000 min
Response: 197396631
Conc: 999.52 ng/ml

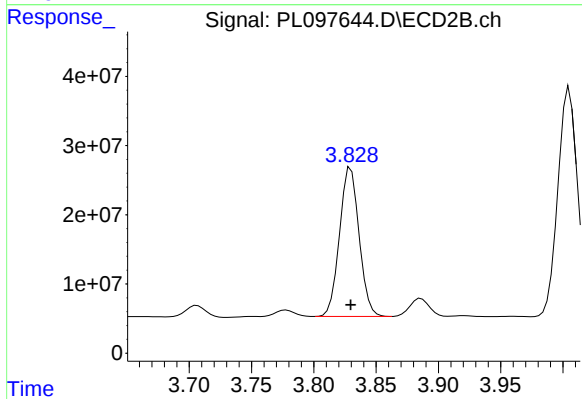

#23 Chlordane-1


R.T.: 3.830 min
Delta R.T.: 0.000 min
Response: 236206193
Conc: 1001.51 ng/ml

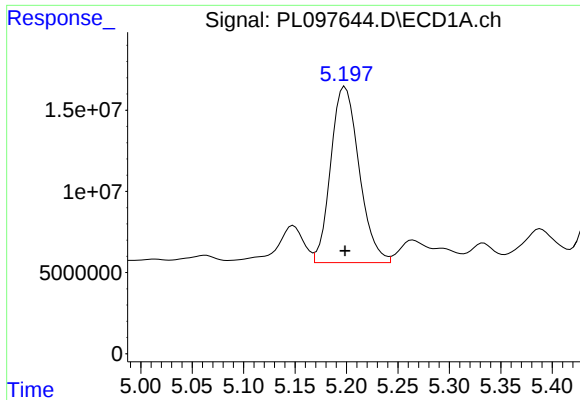

#24 Chlordane-2


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 208034304
Conc: 974.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

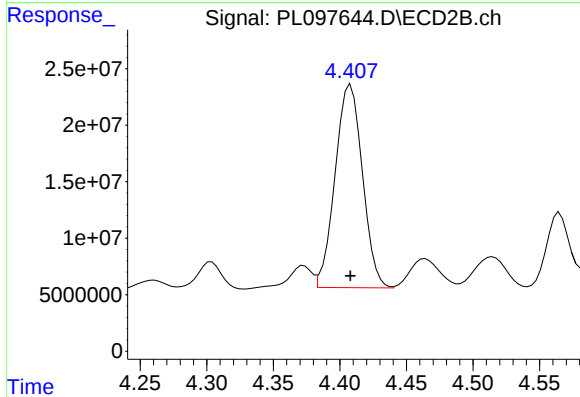


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 256723075
Conc: 982.57 ng/ml

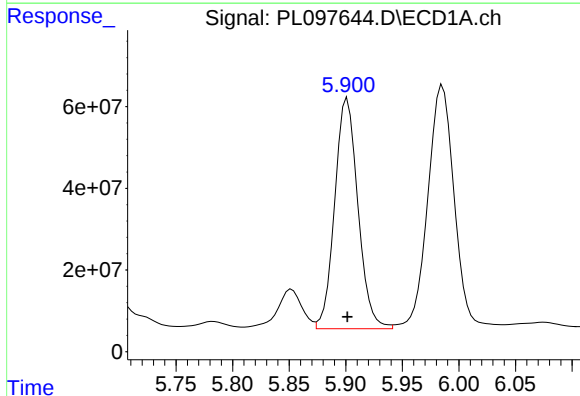


#25 Chlordane-3

R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 807041018
Conc: 1001.28 ng/ml

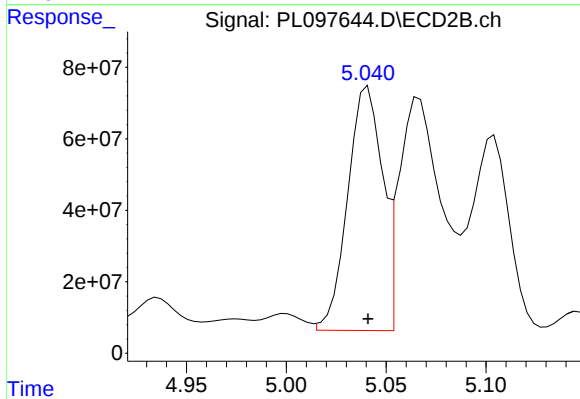

#25 Chlordane-3


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 822573104
Conc: 995.01 ng/ml

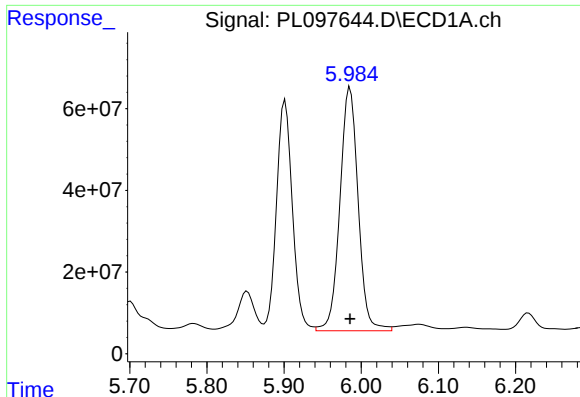

#26 Chlordane-4


R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 977013995
Conc: 993.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

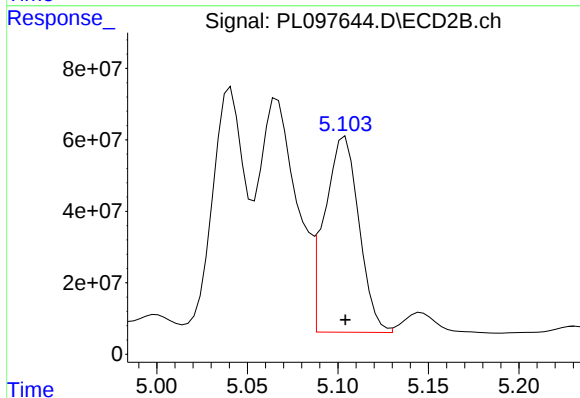


#26 Chlordane-4

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 723371281
Conc: 996.98 ng/ml

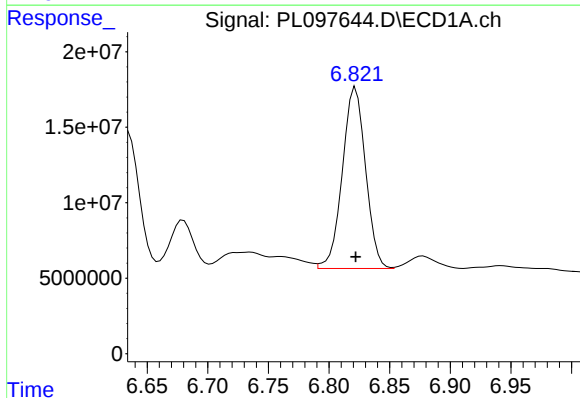


#27 Chlordane-5

R.T.: 6.822 min
Delta R.T.: 0.000 min
Response: 159775022
Conc: 1001.40 ng/ml

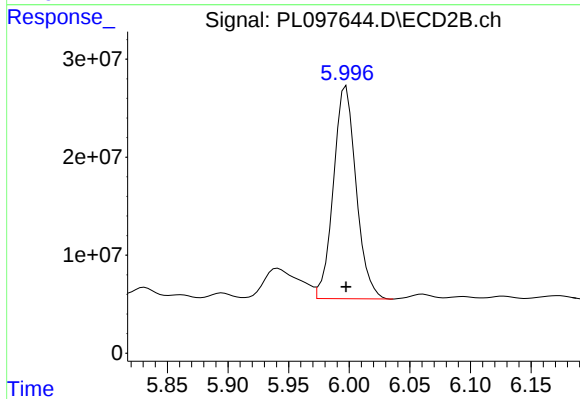

#27 Chlordane-5


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 282626296
Conc: 1001.05 ng/ml

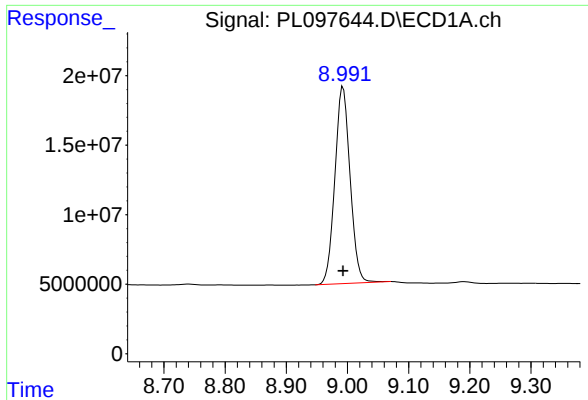

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 244873290
Conc: 98.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

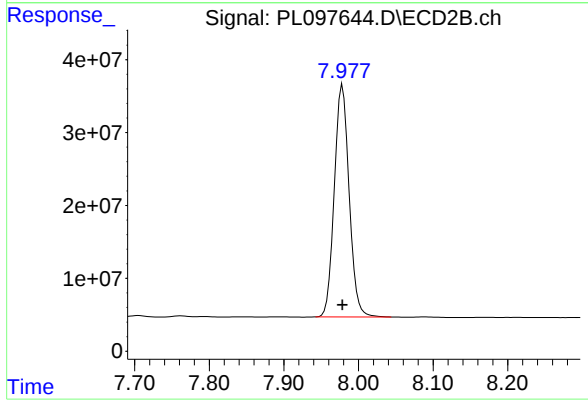

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: 0.000 min
Response: 440525910
Conc: 97.50 ng/ml