

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
 Data File : PL097646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 16:32
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 16:57:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 16:57:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.523	2.821	180.6E6	331.6E6	50.000	50.000
28)	SA Decachlor...	8.993	7.979	127.1E6	231.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.675	3.830	98793108	117.7E6	500.000	500.000
24)	Chlordane-2	5.198	4.408	109.5E6	132.9E6	500.000	500.000
25)	Chlordane-3	5.901	5.041	402.5E6	415.4E6	500.000	500.000
26)	Chlordane-4	5.986	5.104	495.1E6	363.9E6	500.000	500.000
27)	Chlordane-5	6.822	5.998	79664775	141.0E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
Data File : PL097646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 16:32
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 16:57:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 16:57:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

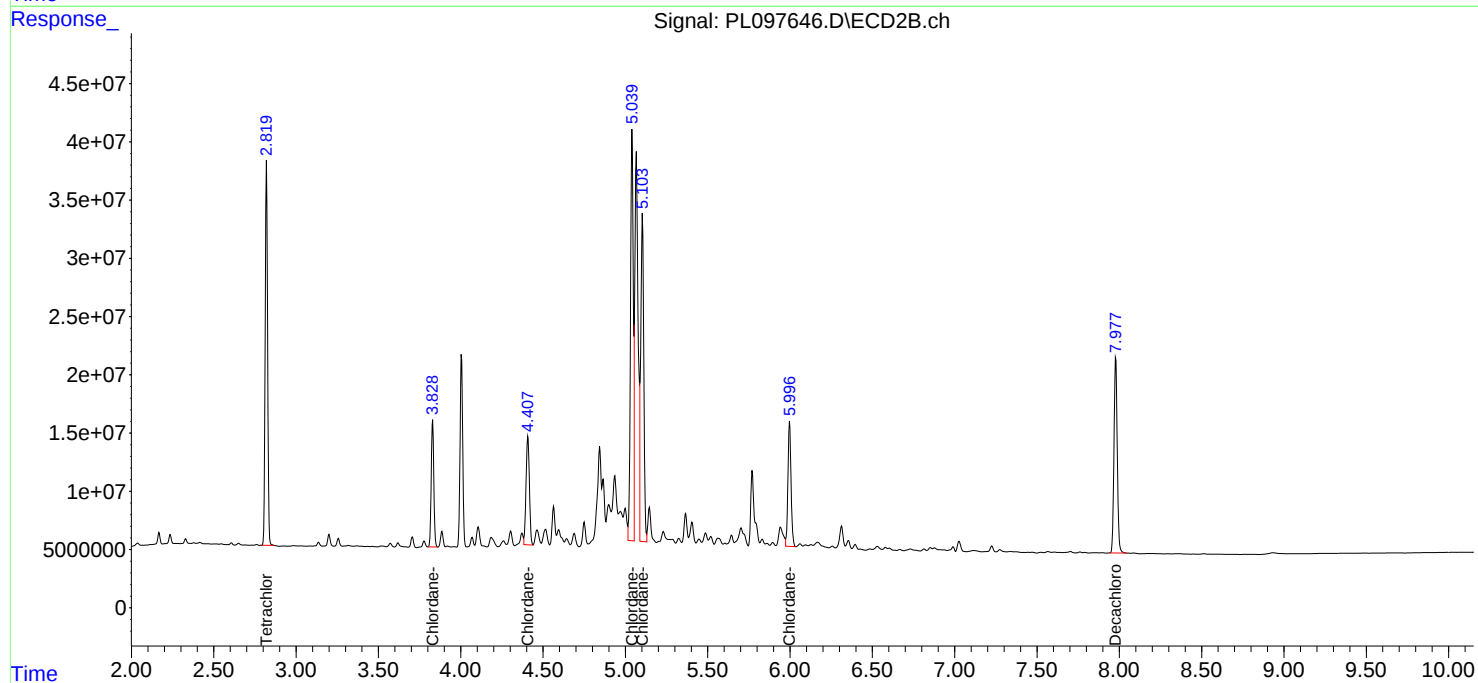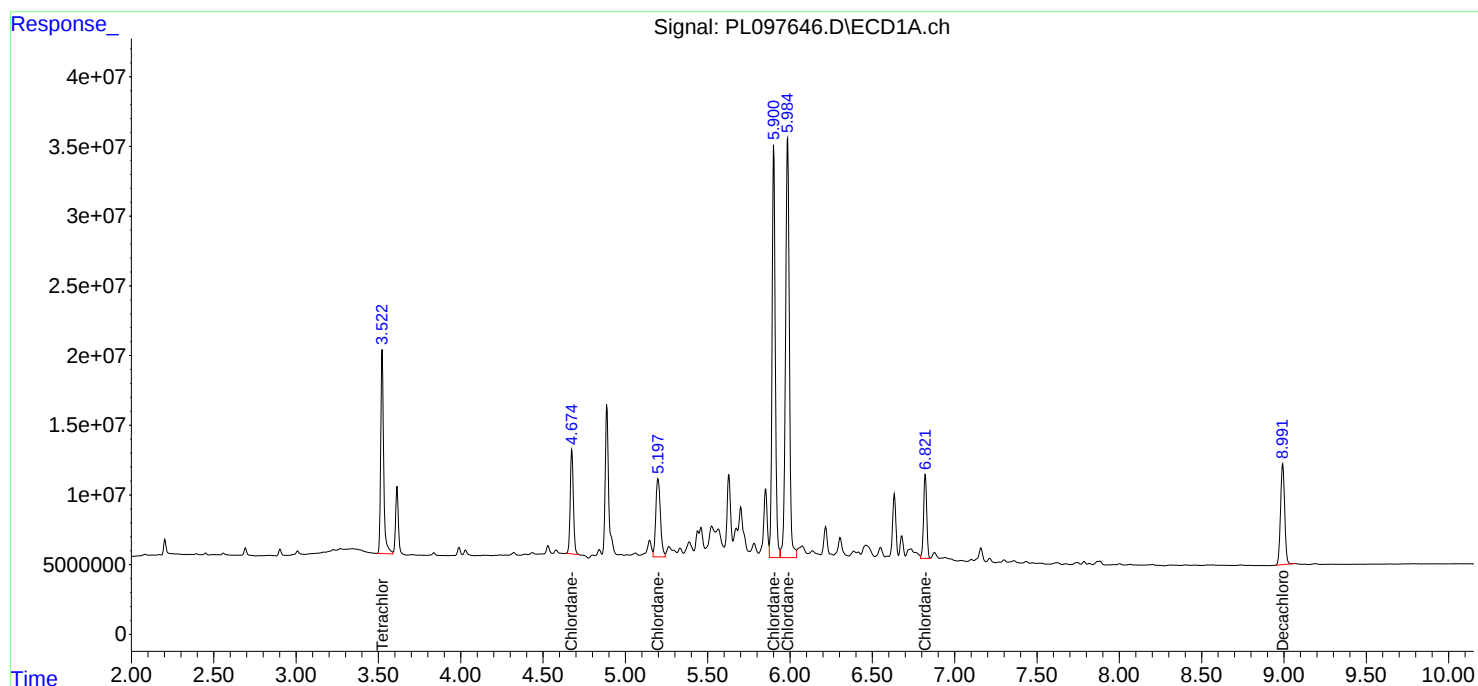


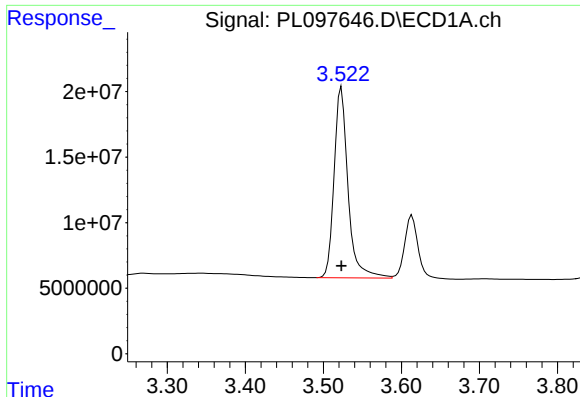

#1 Tetrachloro-m-xylene


R.T.: 3.523 min
Delta R.T.: 0.000 min
Response: 180640387
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

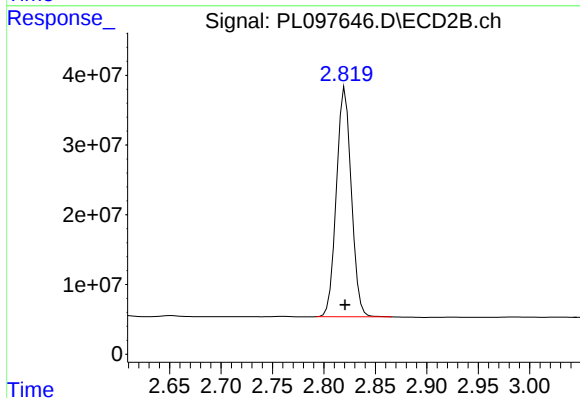


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: 0.000 min
Response: 331582273
Conc: 50.00 ng/ml

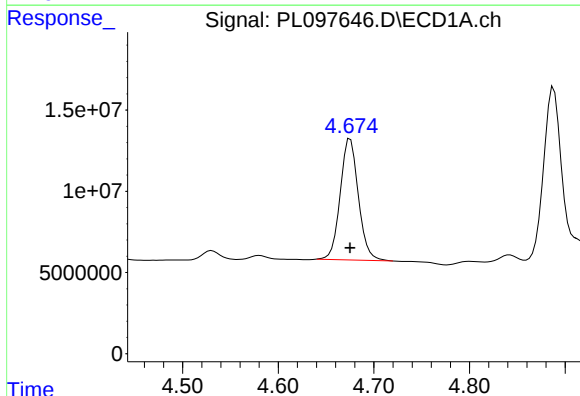


#23 Chlordane-1

R.T.: 4.675 min
Delta R.T.: 0.000 min
Response: 98793108
Conc: 500.00 ng/ml

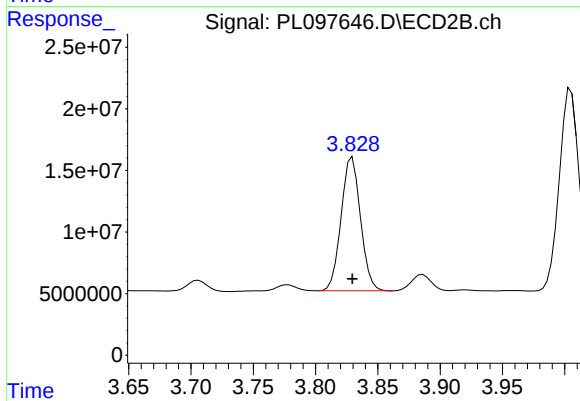

#23 Chlordane-1


R.T.: 3.830 min
Delta R.T.: 0.000 min
Response: 117747356
Conc: 500.00 ng/ml

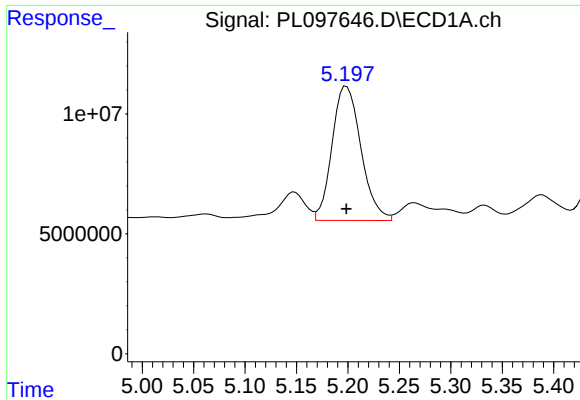

#24 Chlordane-2


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 109518052
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

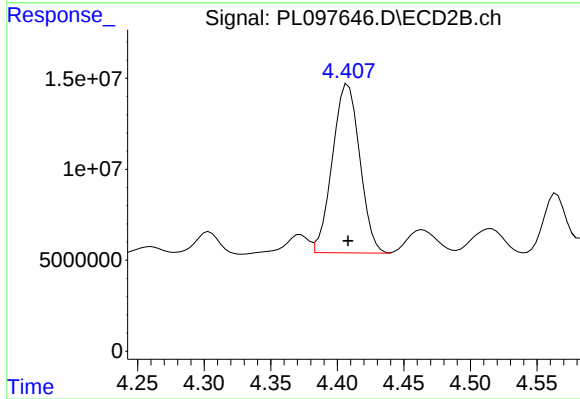


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 132914793
Conc: 500.00 ng/ml

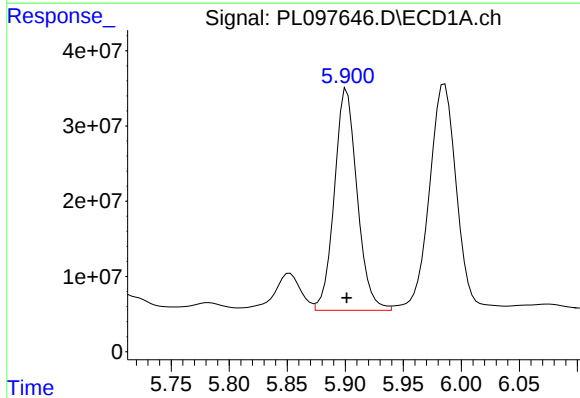


#25 Chlordane-3

R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 402490085
Conc: 500.00 ng/ml

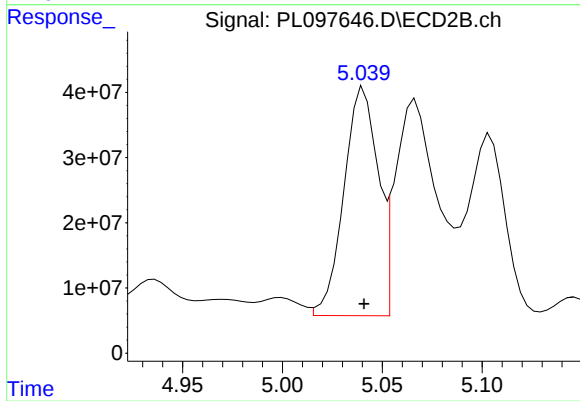

#25 Chlordane-3


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 415413489
Conc: 500.00 ng/ml

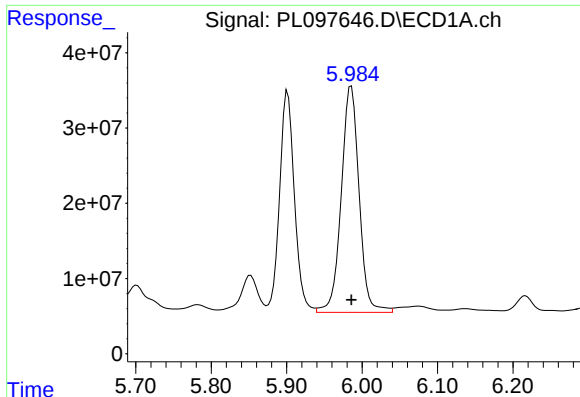

#26 Chlordane-4


R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 495110564
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

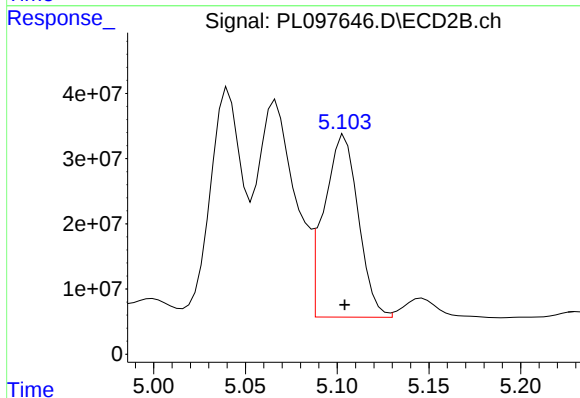


#26 Chlordane-4

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 363873782
Conc: 500.00 ng/ml

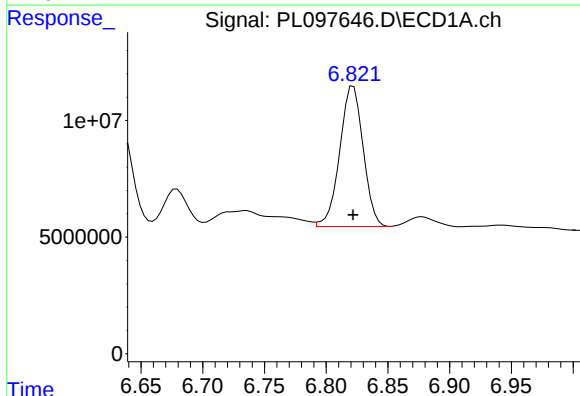


#27 Chlordane-5

R.T.: 6.822 min
Delta R.T.: 0.000 min
Response: 79664775
Conc: 500.00 ng/ml

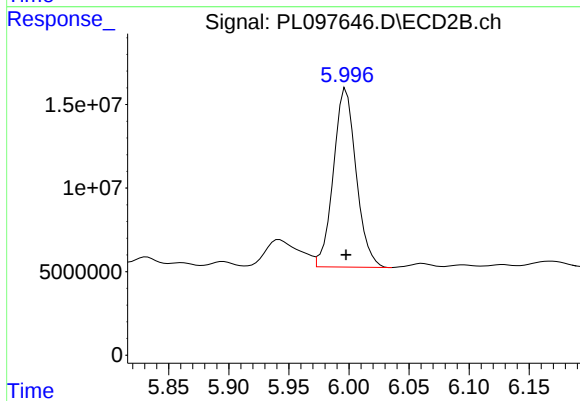

#27 Chlordane-5


R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 141015797
Conc: 500.00 ng/ml

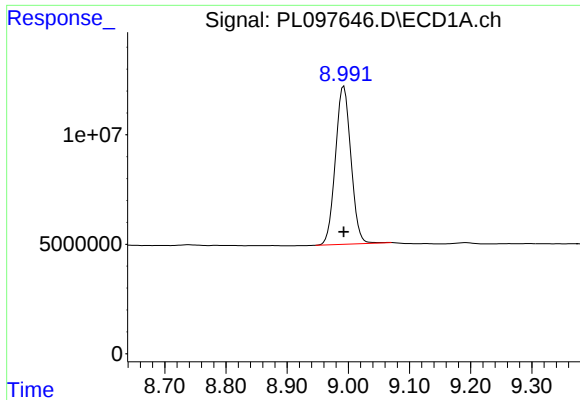

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 127095178
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

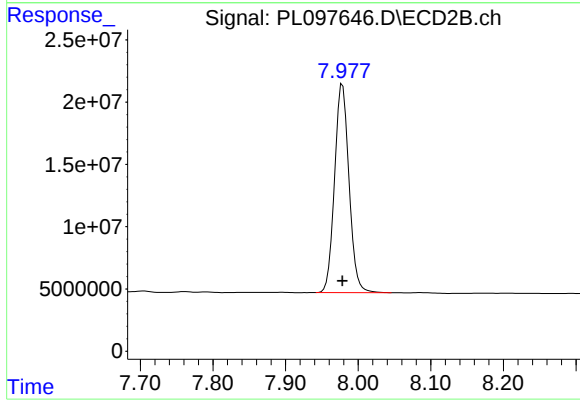

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: 0.000 min
Response: 231560692
Conc: 50.00 ng/ml