

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
 Data File : PL097647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 16:46
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:03:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 28 16:57:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	2.821	91873337	168.2E6	25.310	25.182
28)	SA Decachlor...	8.994	7.978	82116425	141.8E6	30.446	29.478
Target Compounds							
23)	Chlordane-1	4.675	3.829	50245126	60567882	252.245	253.446
24)	Chlordane-2	5.198	4.408	53959536	70249518	251.031	262.538
25)	Chlordane-3	5.902	5.040	194.8E6	216.7E6	242.371	257.119
26)	Chlordane-4	5.985	5.104	236.0E6	187.7E6	241.315	255.360
27)	Chlordane-5	6.822	5.997	40131576	72782581	249.364	254.168



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102825\
Data File : PL097647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 16:46
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:03:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102825.M
Quant Title : GC Extractables
QLast Update : Tue Oct 28 16:57:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

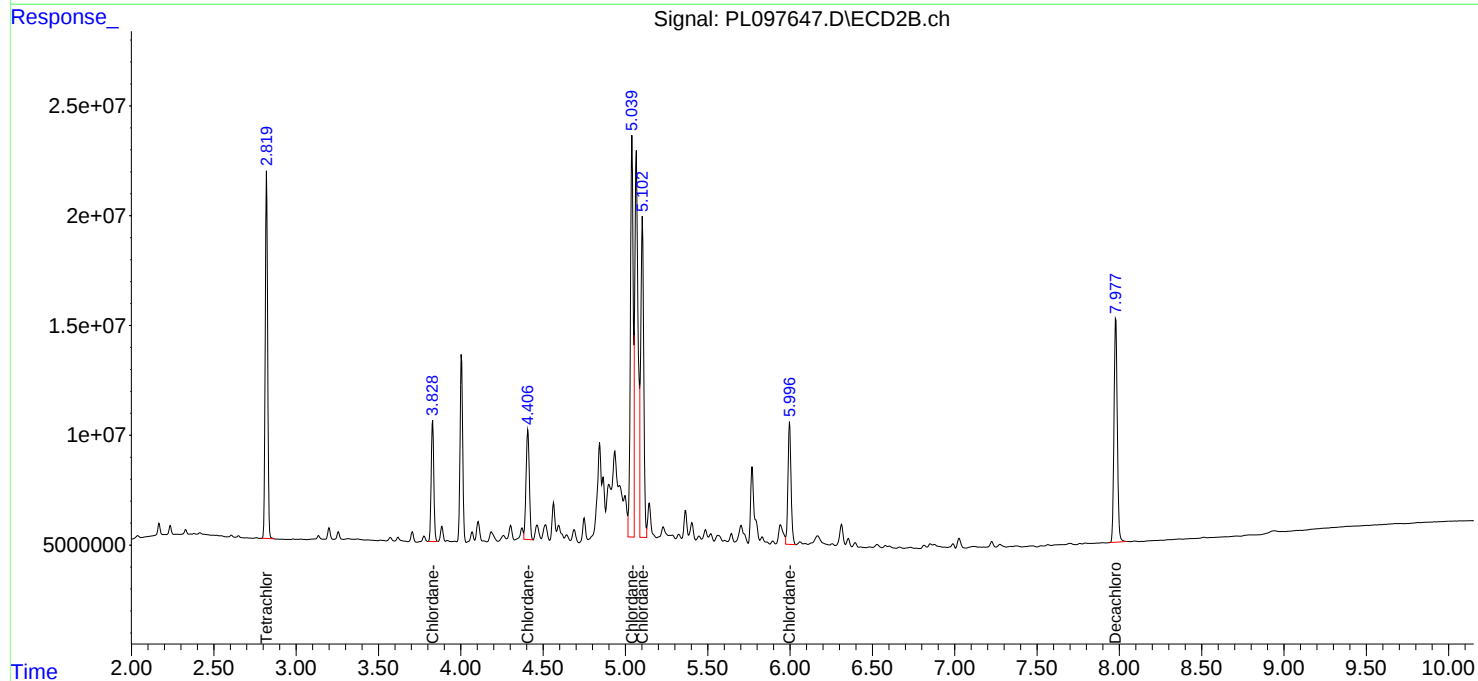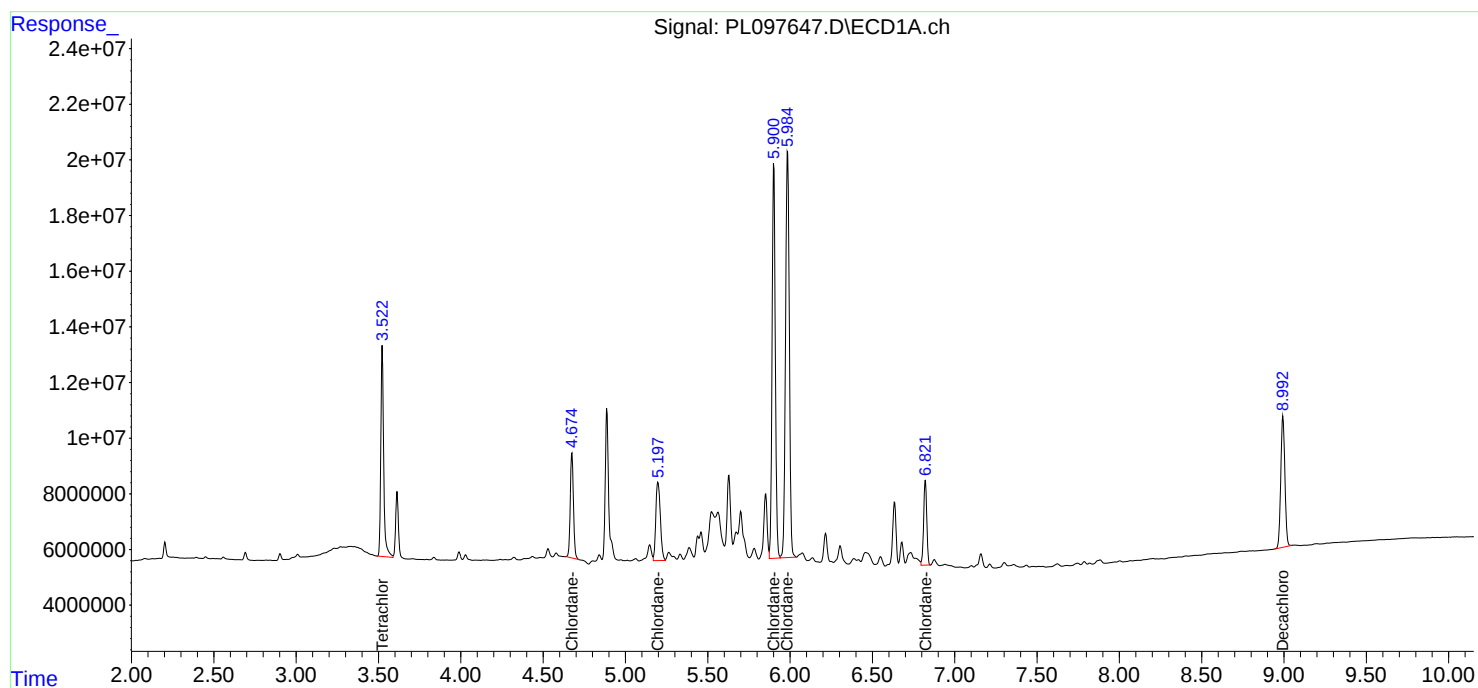


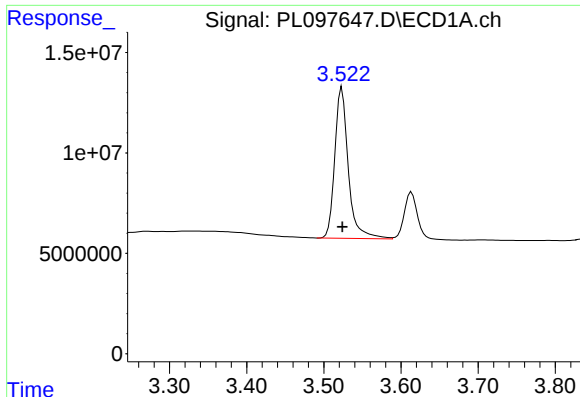

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 91873337
Conc: 25.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

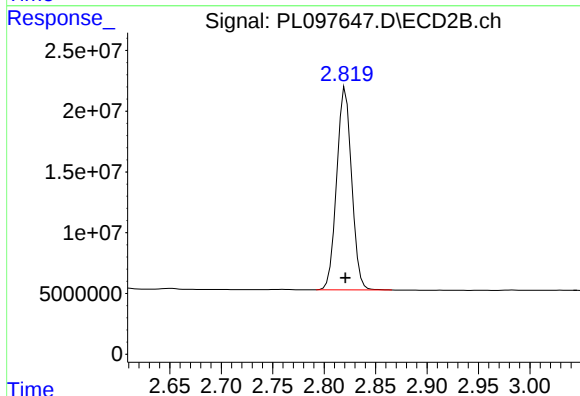


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: 0.000 min
Response: 168158836
Conc: 25.18 ng/ml

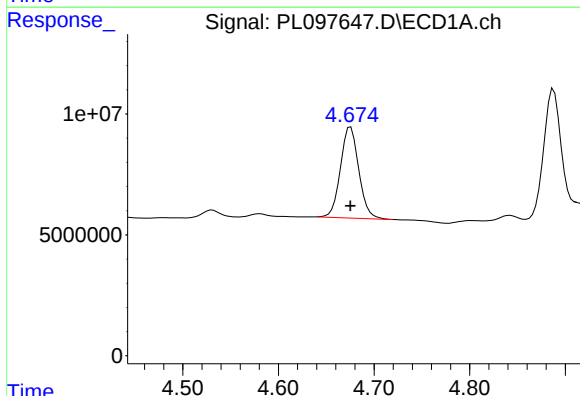


#23 Chlordane-1

R.T.: 4.675 min
Delta R.T.: 0.000 min
Response: 50245126
Conc: 252.25 ng/ml

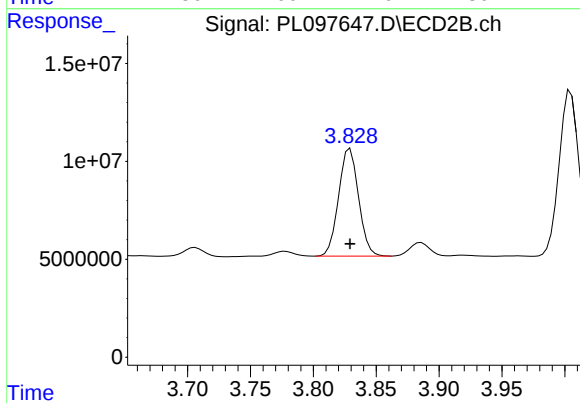

#23 Chlordane-1


R.T.: 3.829 min
Delta R.T.: 0.000 min
Response: 60567882
Conc: 253.45 ng/ml

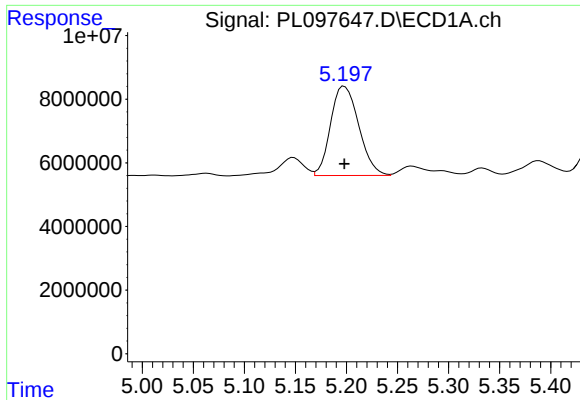

#24 Chlordane-2


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 53959536
Conc: 251.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

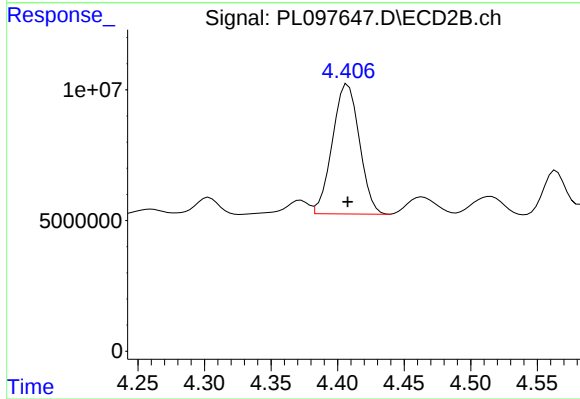


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 70249518
Conc: 262.54 ng/ml

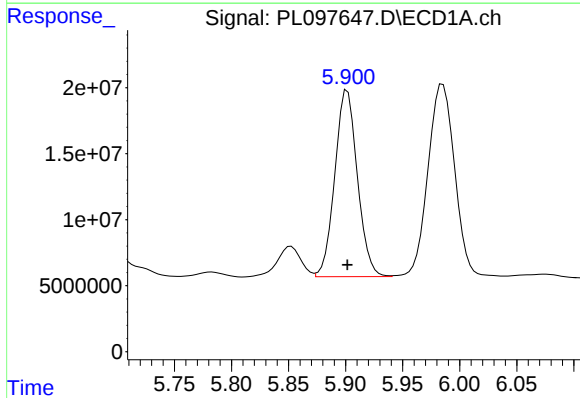


#25 Chlordane-3

R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 194754820
Conc: 242.37 ng/ml

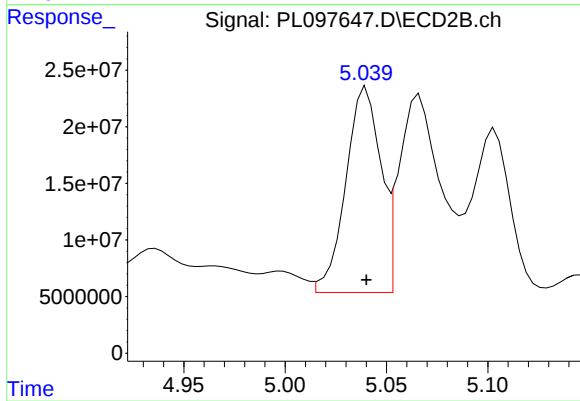

#25 Chlordane-3


R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 216704589
Conc: 257.12 ng/ml

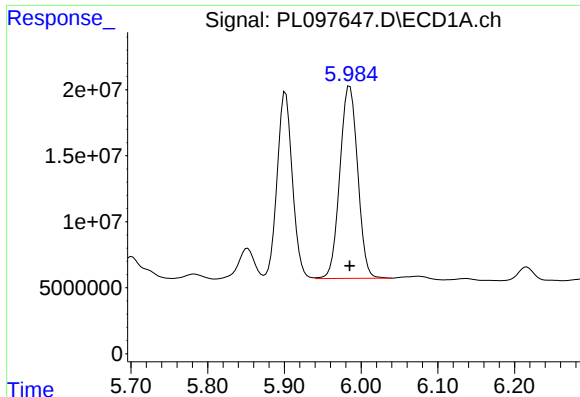

#26 Chlordane-4


R.T.: 5.985 min
Delta R.T.: 0.000 min
Response: 235959549
Conc: 241.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

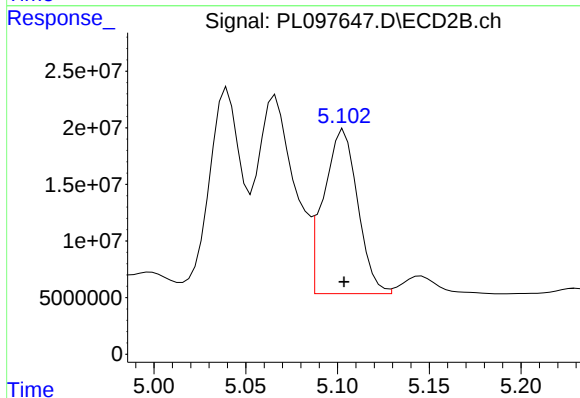


#26 Chlordane-4

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 187707411
Conc: 255.36 ng/ml

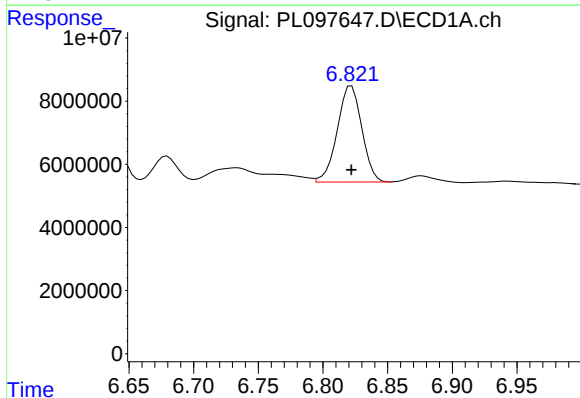


#27 Chlordane-5

R.T.: 6.822 min
Delta R.T.: 0.000 min
Response: 40131576
Conc: 249.36 ng/ml

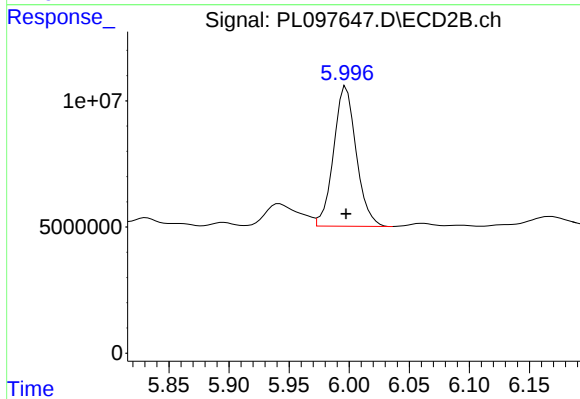

#27 Chlordane-5


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 72782581
Conc: 254.17 ng/ml

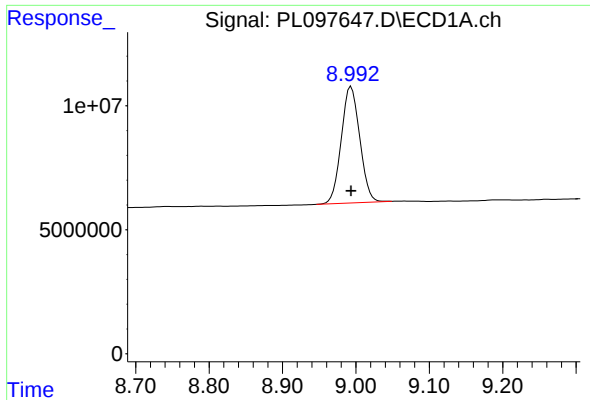

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 82116425
Conc: 30.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

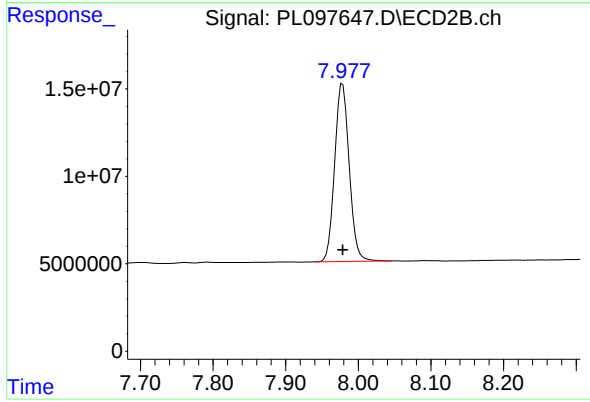

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: 0.000 min
Response: 141784972
Conc: 29.48 ng/ml