

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 13:45
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:38:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.104	140.1E6	67755463	21.988	21.997
28)	SA Decachlor...	8.219	9.237	146.1E6	55930868	22.059	21.830
Target Compounds							
10)	B gamma-Chl...	5.419	0.000	4289363	0	0.527	N.D. #
11)	B alpha-Chl...	5.419f	0.000	4289363	0	0.530	N.D. #
15)	B Endosulfa...	6.317	0.000	4241781	0	0.614	N.D. #
16)	A 4,4'-DDD	6.150	0.000	1524414	0	0.262	N.D. #
20)	A Methoxychlor	6.918	0.000	1300839	0	0.387	N.D. #
25)	Chlordane-3	5.419	0.000	4289363	0	4.813	N.D. #
26)	Chlordane-4	5.419	0.000	4289363	0	5.478	N.D. #
27)	Chlordane-5	6.317	0.000	4241781	0	17.010	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 13:45
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:38:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

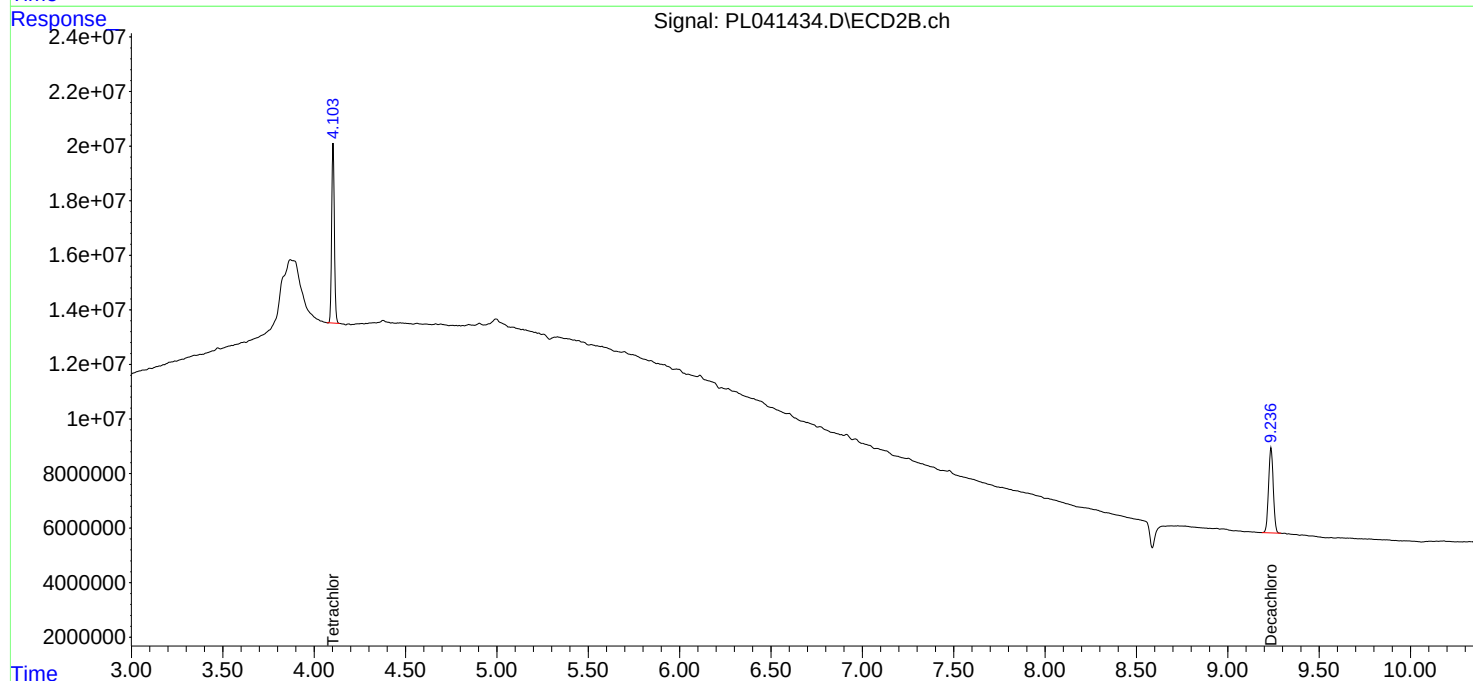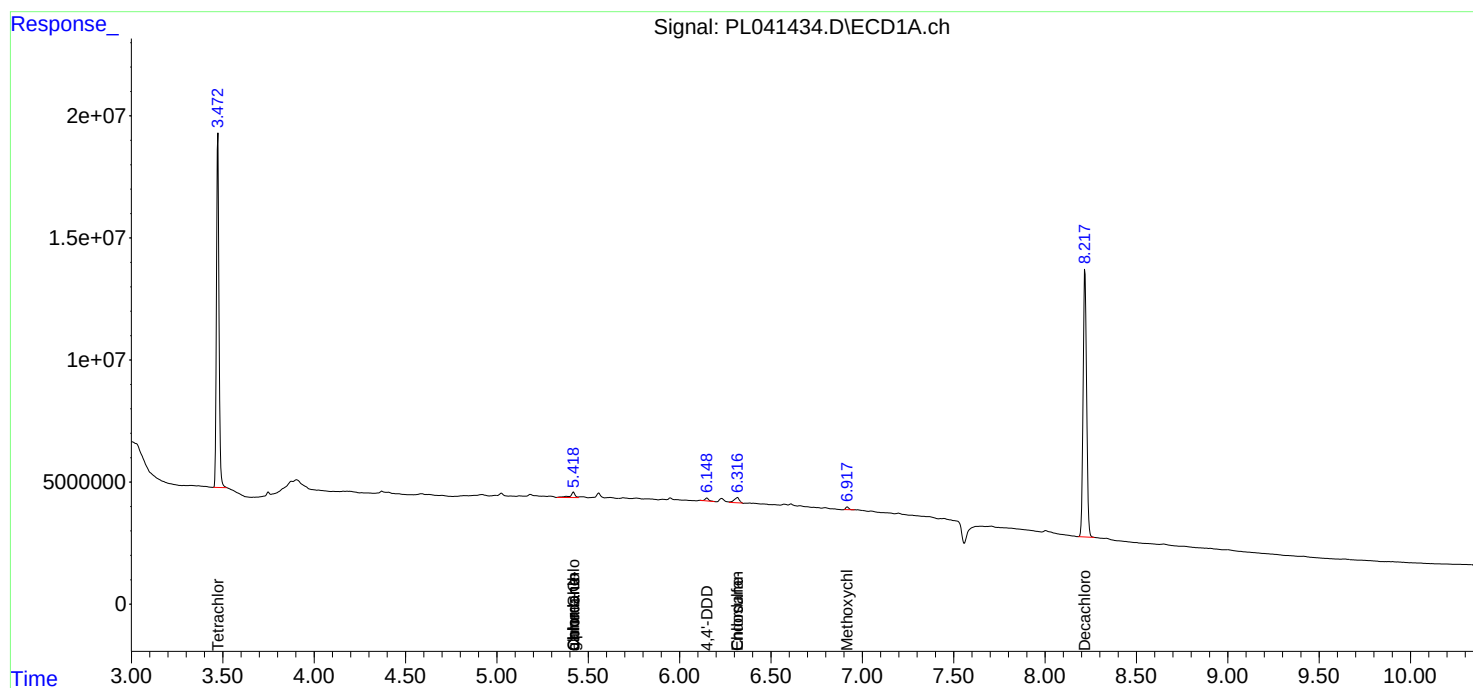


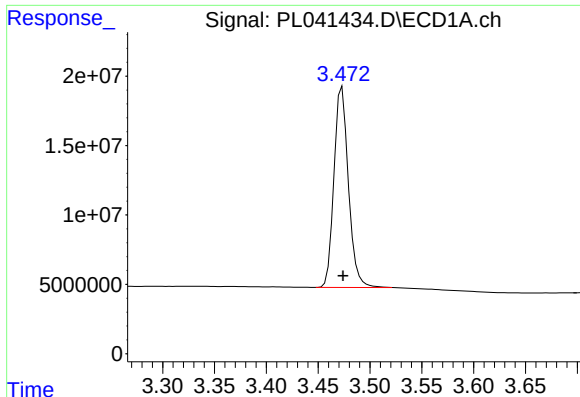

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 140068677
Conc: 21.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

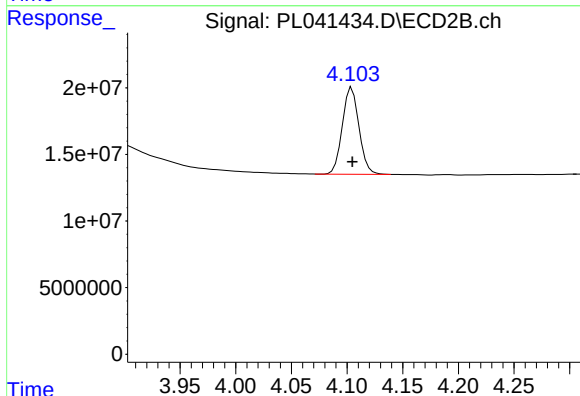


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 67755463
Conc: 22.00 ng/ml

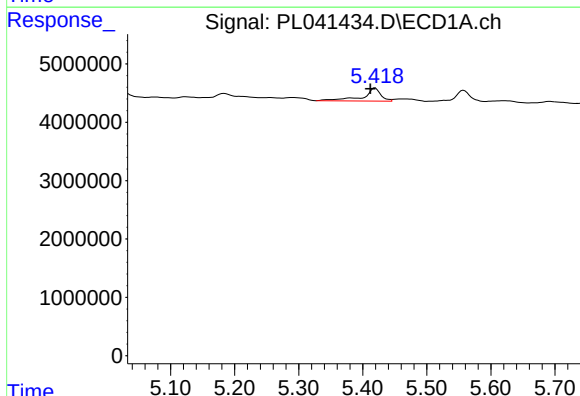


#10 gamma-Chlordane

R.T.: 5.419 min
Delta R.T.: 0.007 min
Response: 4289363
Conc: 0.53 ng/ml

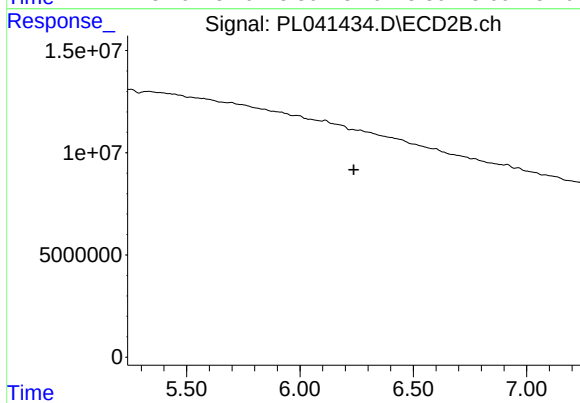

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

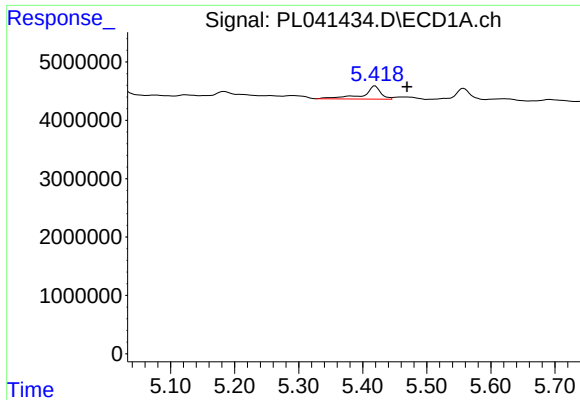

#11 alpha-Chlordane


R.T.: 5.419 min
Delta R.T.: -0.050 min
Response: 4289363
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

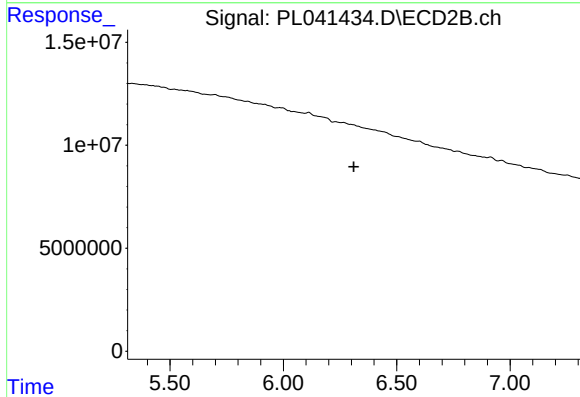


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

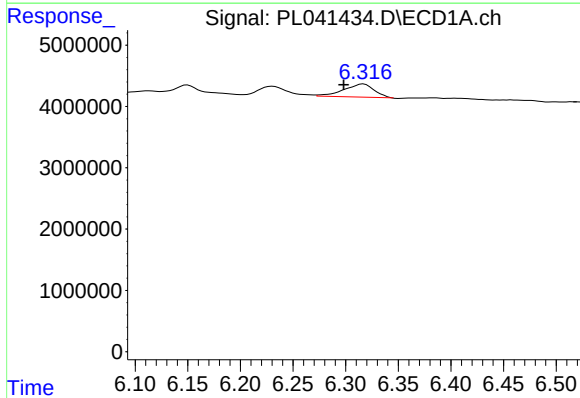


#15 Endosulfan II

R.T.: 6.317 min
Delta R.T.: 0.019 min
Response: 4241781
Conc: 0.61 ng/ml

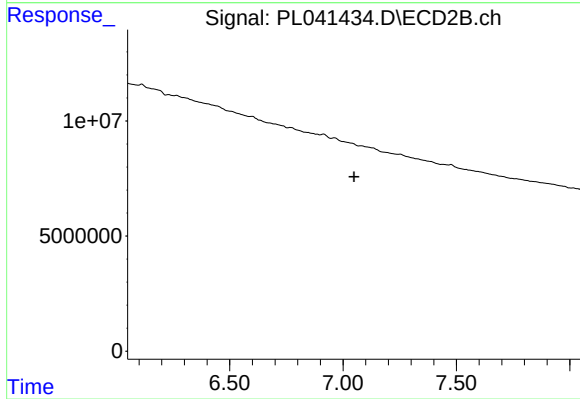

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

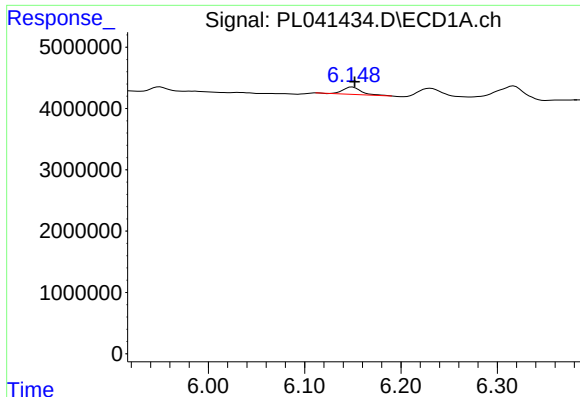

#16 4,4'-DDD


R.T.: 6.150 min
Delta R.T.: -0.002 min
Response: 1524414
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

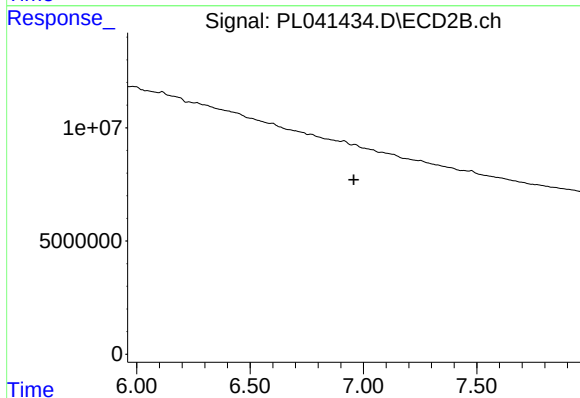


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

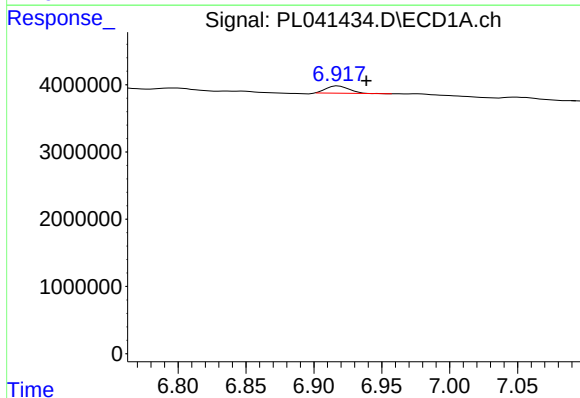


#20 Methoxychlor

R.T.: 6.918 min
Delta R.T.: -0.021 min
Response: 1300839
Conc: 0.39 ng/ml

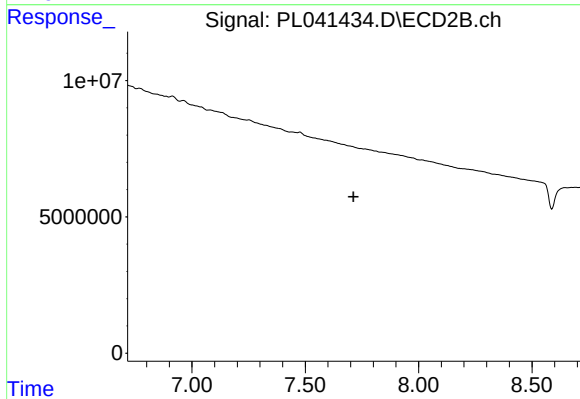

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.713 min
Response: 0
Conc: N.D.

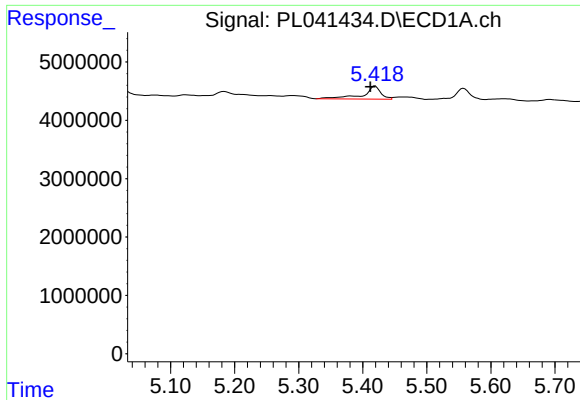

#25 Chlordane-3


R.T.: 5.419 min
Delta R.T.: 0.007 min
Response: 4289363
Conc: 4.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

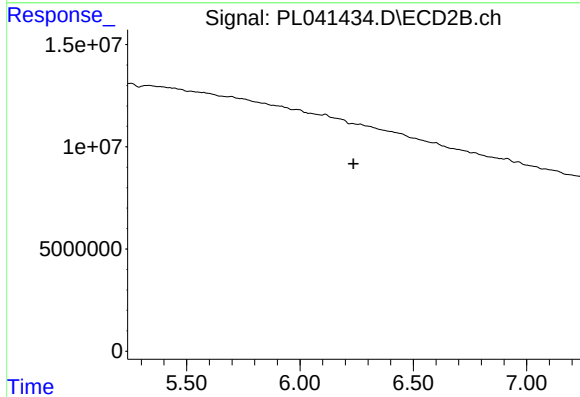


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

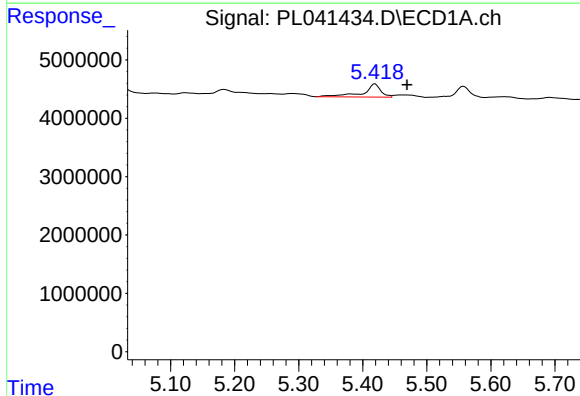


#26 Chlordane-4

R.T.: 5.419 min
Delta R.T.: -0.050 min
Response: 4289363
Conc: 5.48 ng/ml

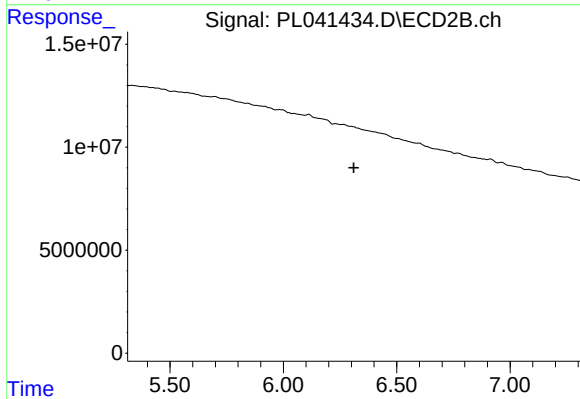

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

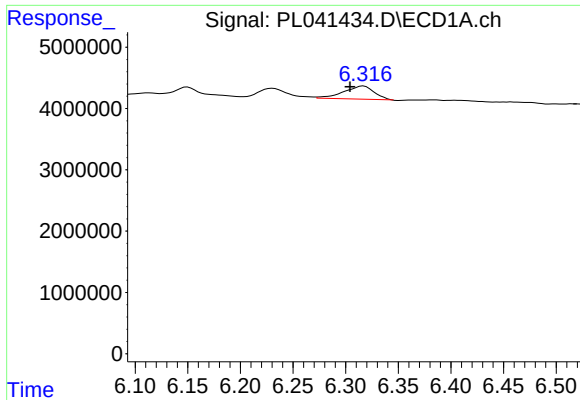

#27 Chlordane-5


R.T.: 6.317 min
Delta R.T.: 0.013 min
Response: 4241781
Conc: 17.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

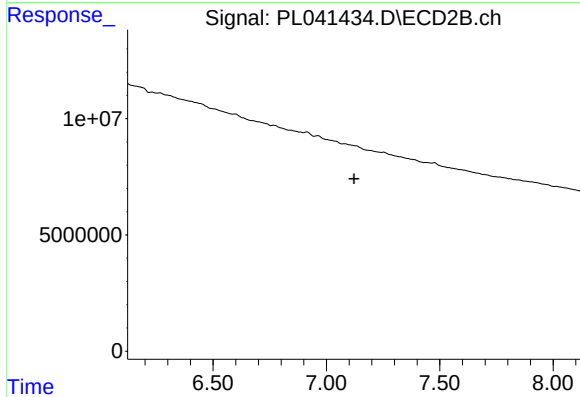


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.123 min
Response: 0
Conc: N.D.

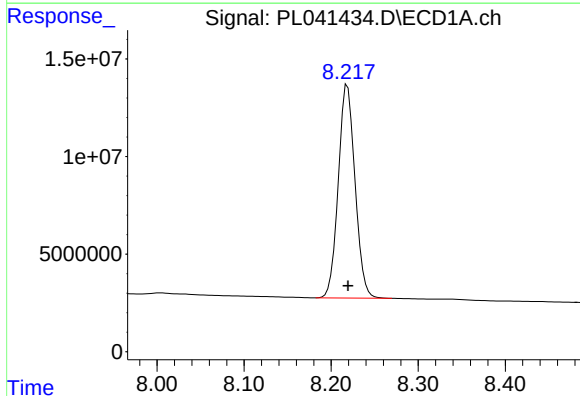

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 146117924
Conc: 22.06 ng/ml

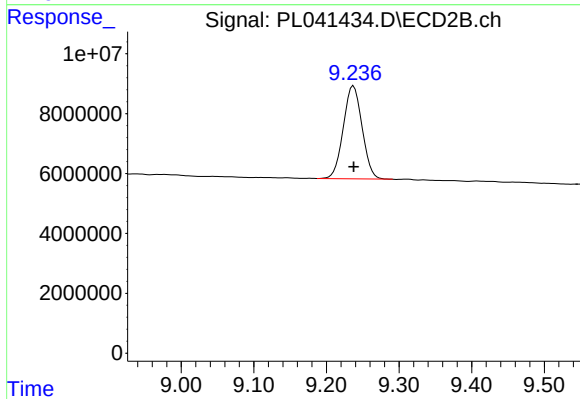

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 55930868
Conc: 21.83 ng/ml