

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 15:37
 Operator : AJ\SJ
 Sample : PCHLORICCC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:24:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:20:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.105	317.1E6	143.9E6	50.000	50.000
28)	SA Decachlor...	8.219	9.238	308.9E6	120.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.344	5.115	141.8E6	69444947	500.000	500.000
24)	Chlordane-2	4.844	5.586	147.2E6	66442266	500.000	500.000
25)	Chlordane-3	5.412	6.237	445.6E6	225.0E6	500.000	500.000
26)	Chlordane-4	5.469	6.311	391.5E6	261.4E6	500.000	500.000
27)	Chlordane-5	6.304	7.123	124.7E6	48830633	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 15:37
Operator : AJ\SJ
Sample : PCHLORICCC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:24:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:20:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

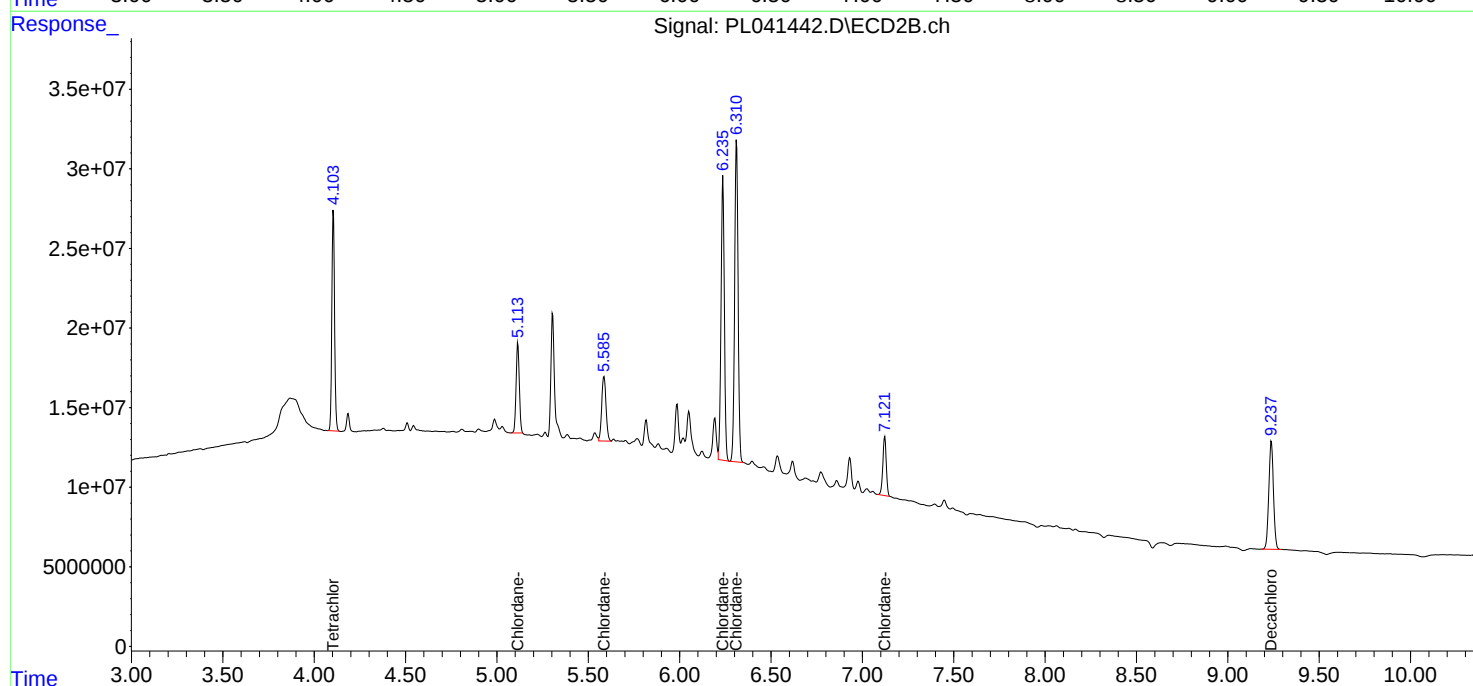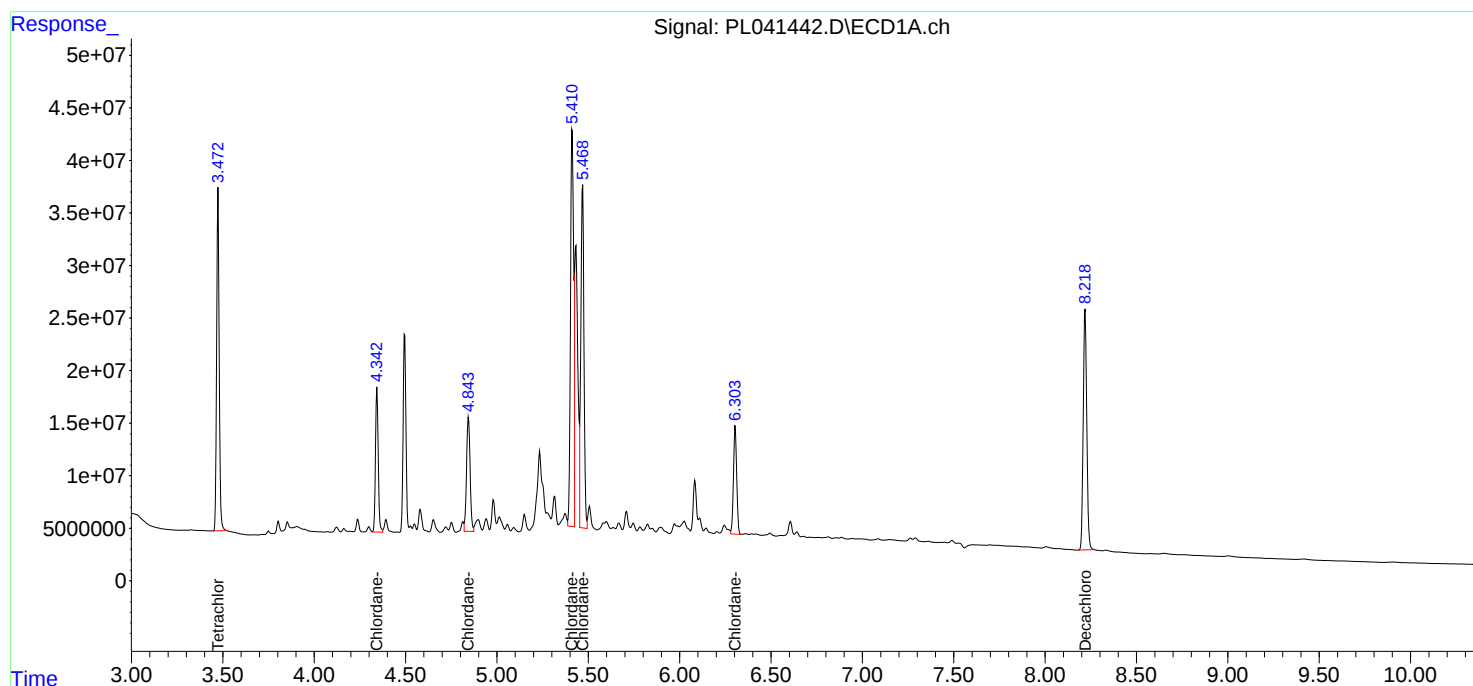


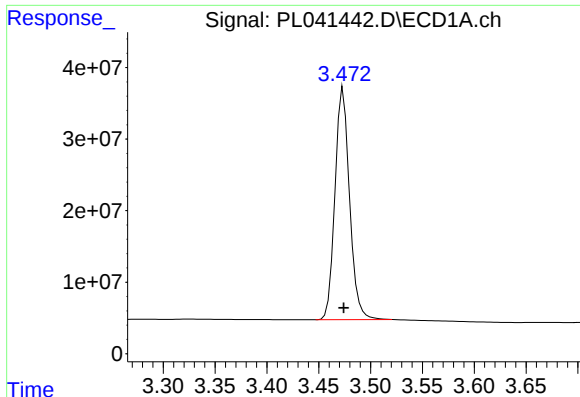

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 317084976
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

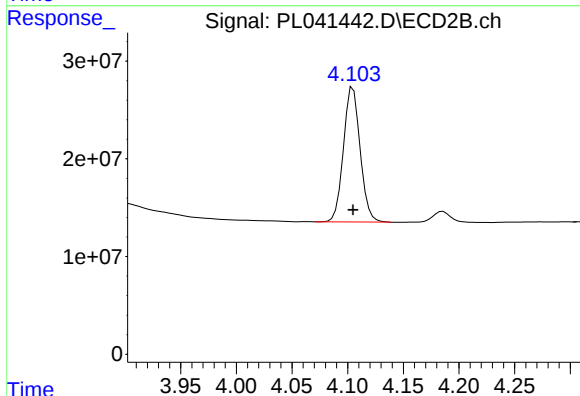


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 143939706
Conc: 50.00 ng/ml

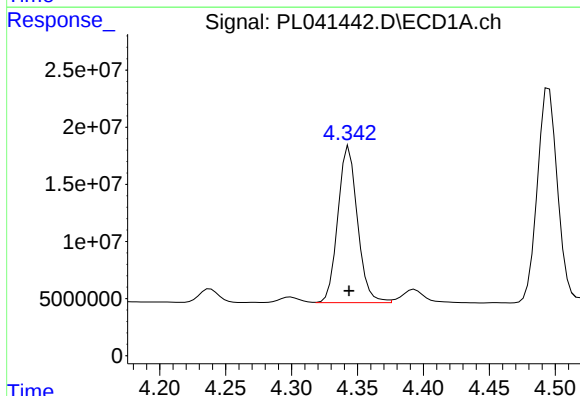


#23 Chlordane-1

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 141768779
Conc: 500.00 ng/ml

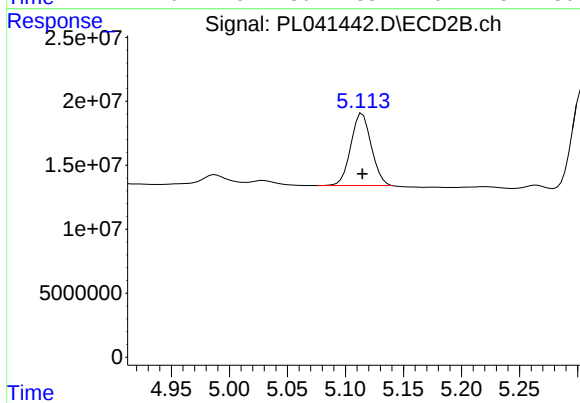

#23 Chlordane-1


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 69444947
Conc: 500.00 ng/ml

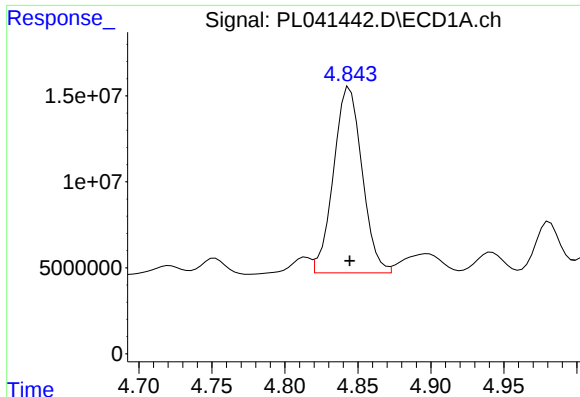

#24 Chlordane-2


R.T.: 4.844 min
Delta R.T.: 0.000 min
Response: 147247818
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

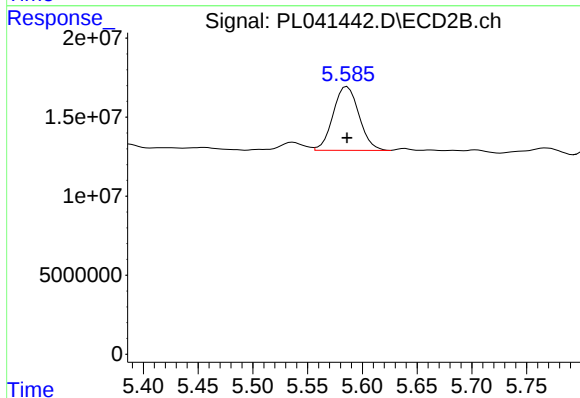


#24 Chlordane-2

R.T.: 5.586 min
Delta R.T.: 0.000 min
Response: 66442266
Conc: 500.00 ng/ml

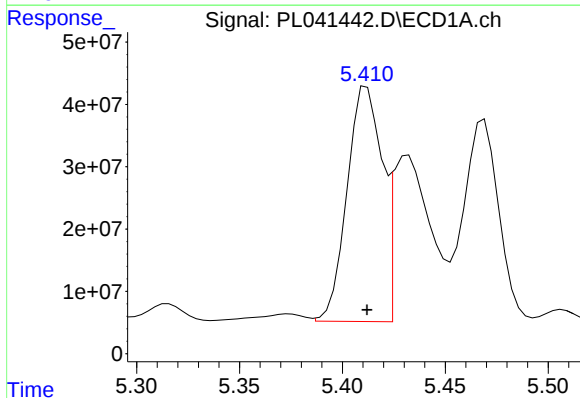


#25 Chlordane-3

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 445642563
Conc: 500.00 ng/ml

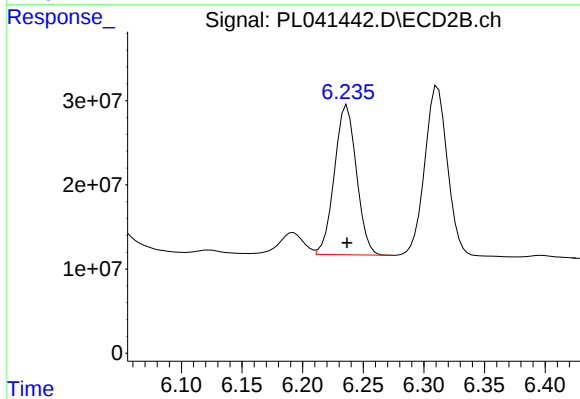

#25 Chlordane-3


R.T.: 6.237 min
Delta R.T.: 0.000 min
Response: 225014404
Conc: 500.00 ng/ml

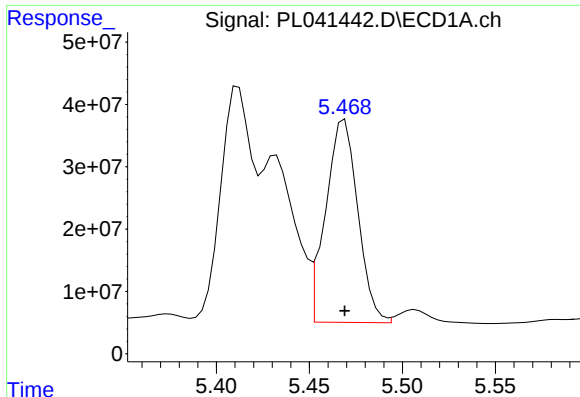

#26 Chlordane-4


R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 391476317
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

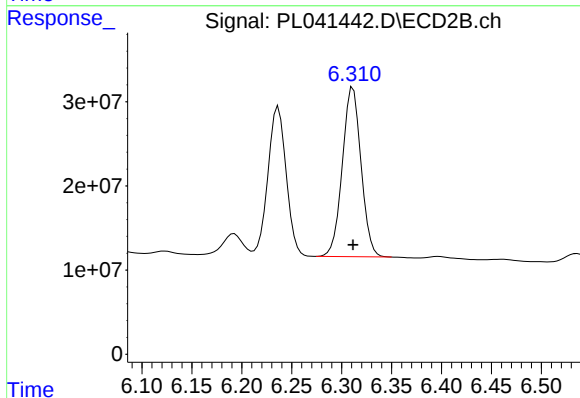


#26 Chlordane-4

R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 261410401
Conc: 500.00 ng/ml

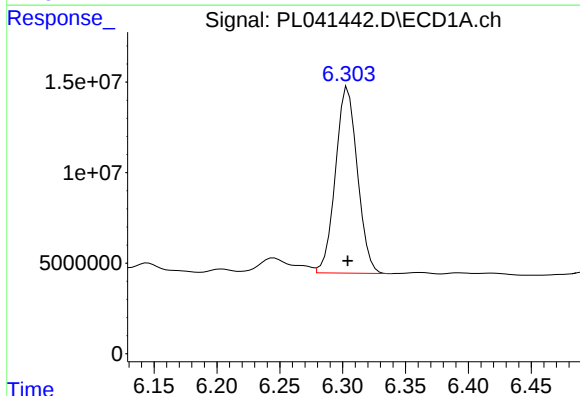


#27 Chlordane-5

R.T.: 6.304 min
Delta R.T.: 0.000 min
Response: 124681893
Conc: 500.00 ng/ml

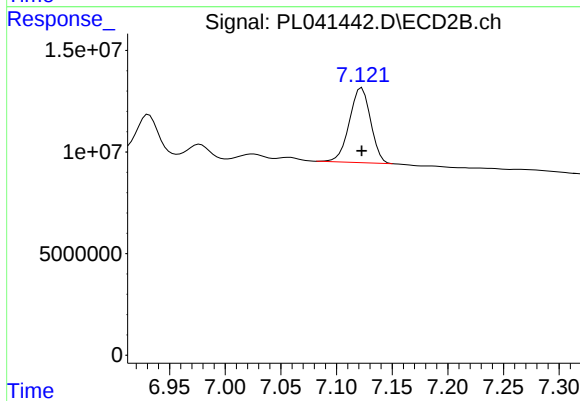

#27 Chlordane-5


R.T.: 7.123 min
Delta R.T.: 0.000 min
Response: 48830633
Conc: 500.00 ng/ml

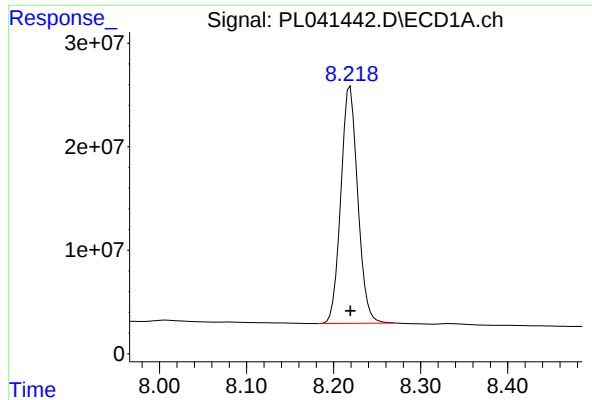

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 308943230
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

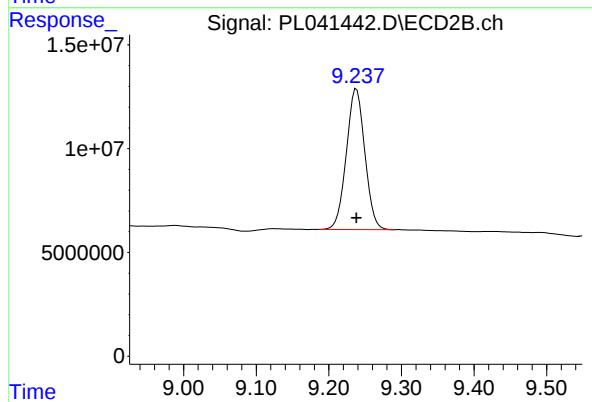

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.000 min
Response: 120041490
Conc: 50.00 ng/ml