

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 17:44
 Operator : AJ\SJ
 Sample : J5697-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-58-66-98-92

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 02:32:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.104	62600736	31096428	9.827	10.096
28)	SA Decachlor...	8.219	9.237	83128680	31093261	12.550	12.136
Target Compounds							
2)	A alpha-BHC	3.867f	0.000	85764	0	0.009	N.D. #
6)	B beta-BHC	4.407f	4.976	5078361	-1404452	1.347	N.D. #
10)	B gamma-Chl...	5.430	0.000	983383	0	0.121	N.D. #
11)	B alpha-Chl...	5.430f	0.000	983383	0	0.121	N.D. #
12)	B 4,4'-DDE	5.634	6.463	4807048	3924333	0.672	1.199 #
14)	MA Endrin	6.023	6.863	5470234	1671269	0.748	0.615
17)	MA 4,4'-DDT	6.389	7.256	15452773	7760241	2.540	3.087
20)	A Methoxychlor	6.915	0.000	2172035	0	0.646	N.D. #
23)	Chlordane-1	4.407	0.000	5078361	0	17.911	N.D. #
25)	Chlordane-3	5.430	0.000	983383	0	1.103	N.D. #
26)	Chlordane-4	5.430	0.000	983383	0	1.256	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 17:44
Operator : AJ\SJ
Sample : J5697-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 02:32:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

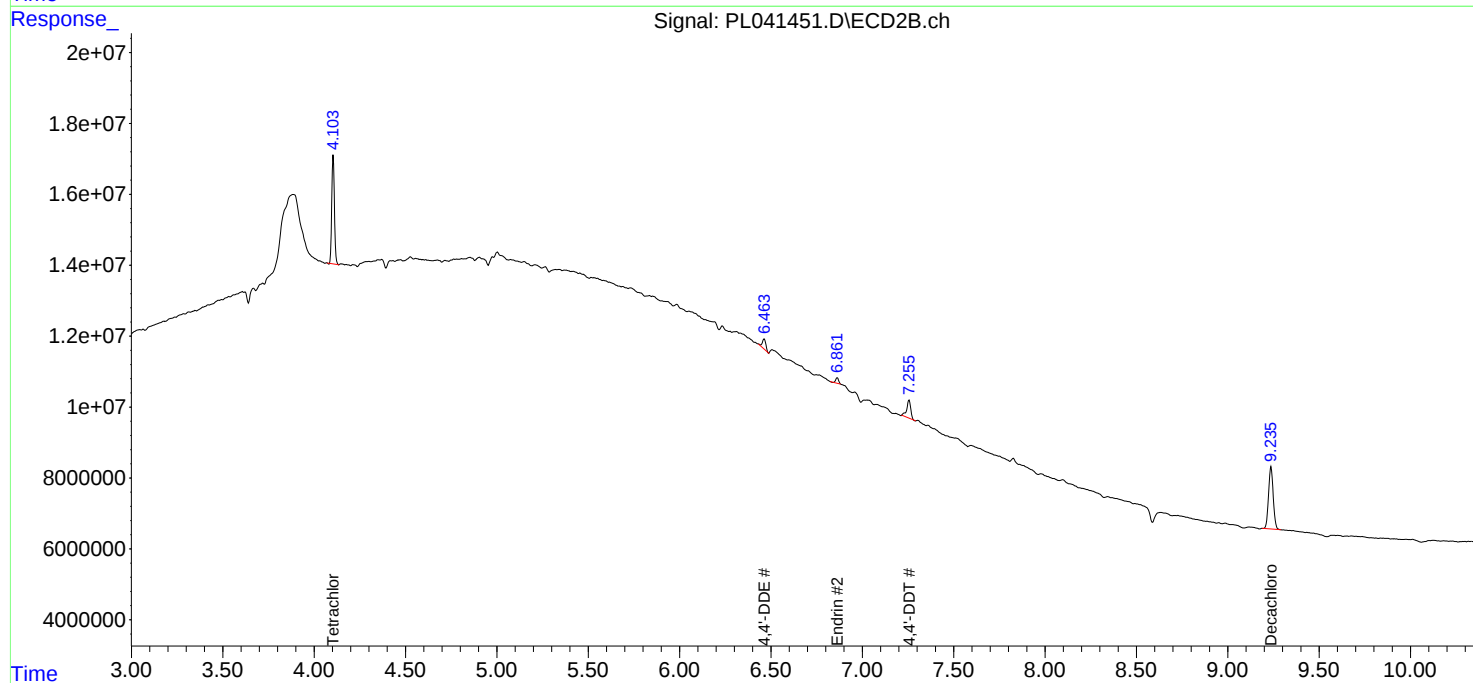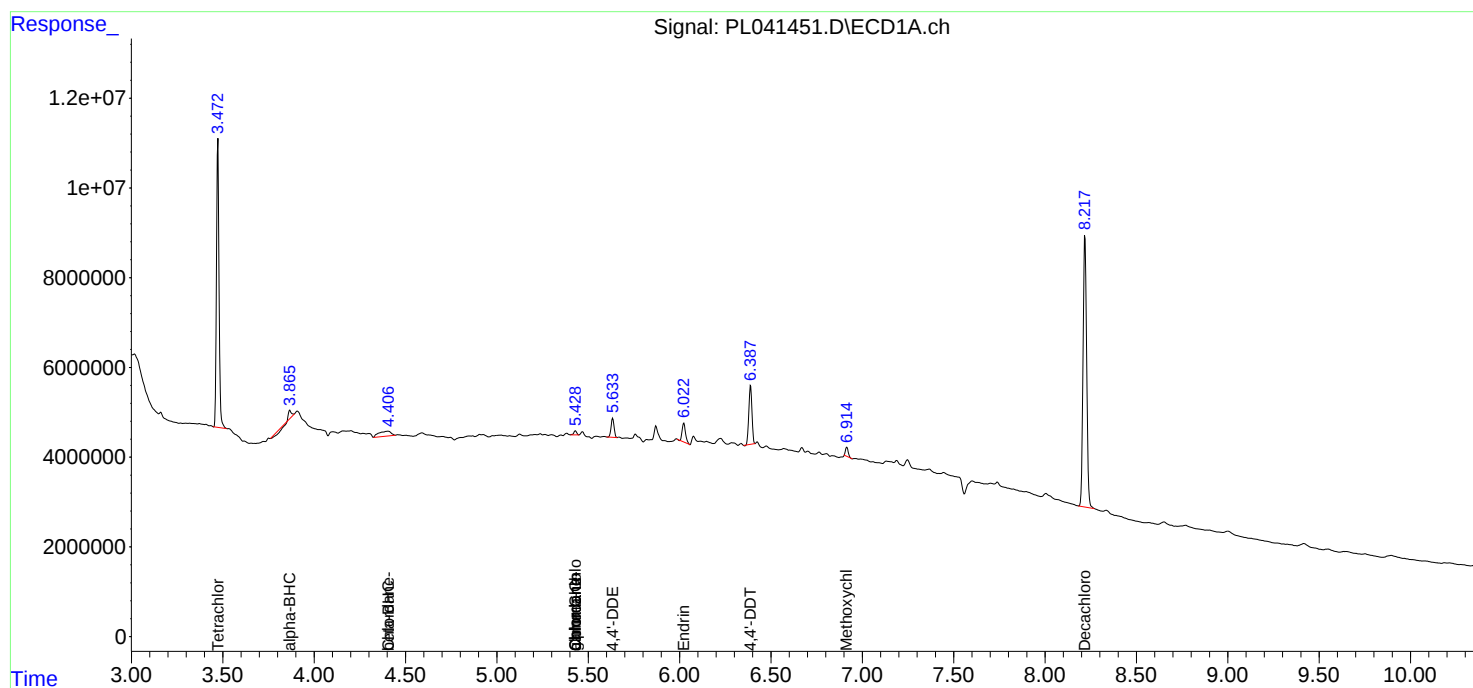


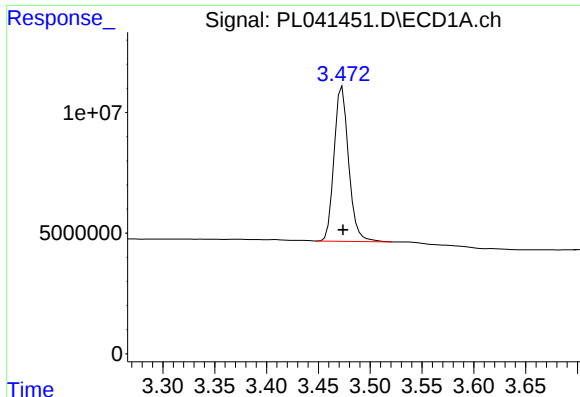

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 62600736
Conc: 9.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

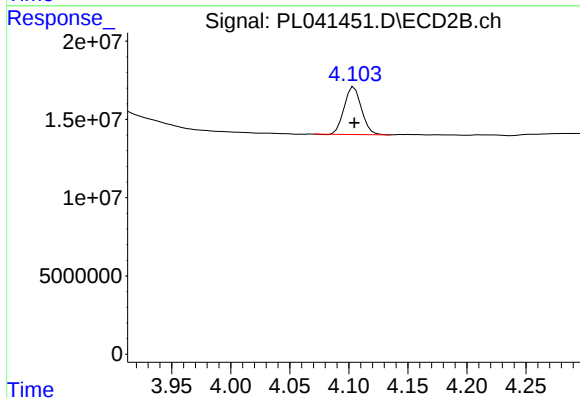


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 31096428
Conc: 10.10 ng/ml

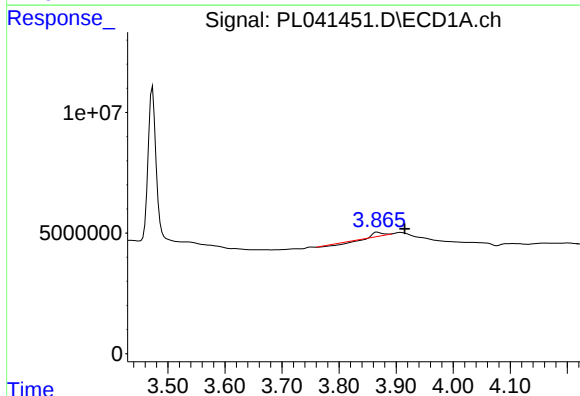


#2 alpha-BHC

R.T.: 3.867 min
Delta R.T.: -0.048 min
Response: 85764
Conc: 0.01 ng/ml

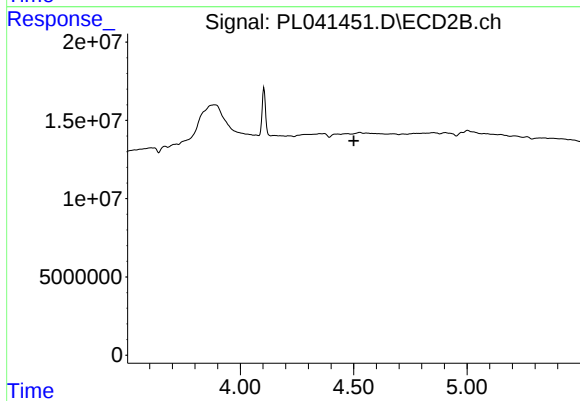

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

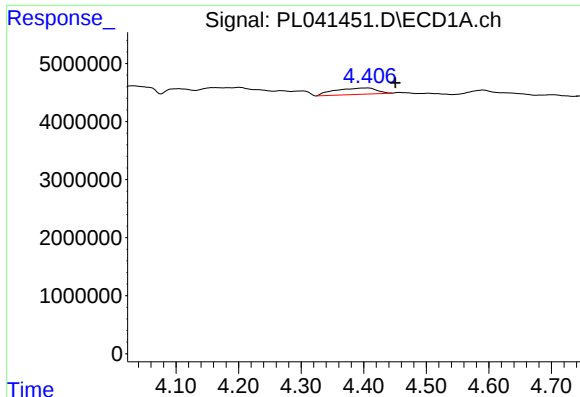

#6 beta-BHC


R.T.: 4.407 min
Delta R.T.: -0.044 min
Response: 5078361
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

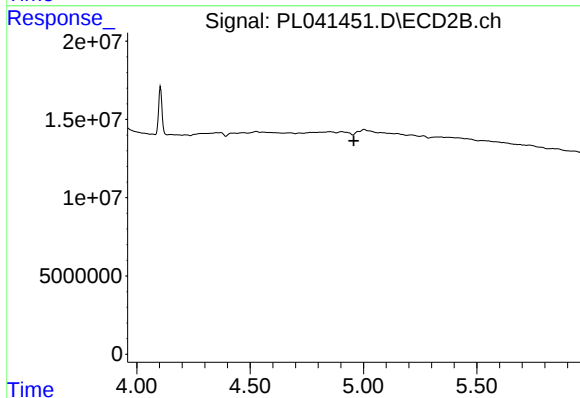


#6 beta-BHC

R.T.: 4.976 min
Delta R.T.: 0.019 min
Response: -1404452
Conc: N.D.

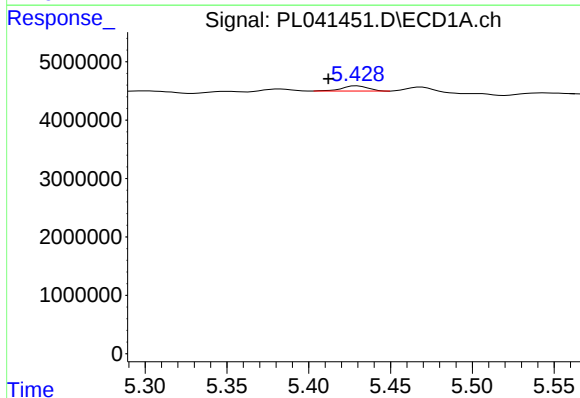


#10 gamma-Chlordane

R.T.: 5.430 min
Delta R.T.: 0.018 min
Response: 983383
Conc: 0.12 ng/ml

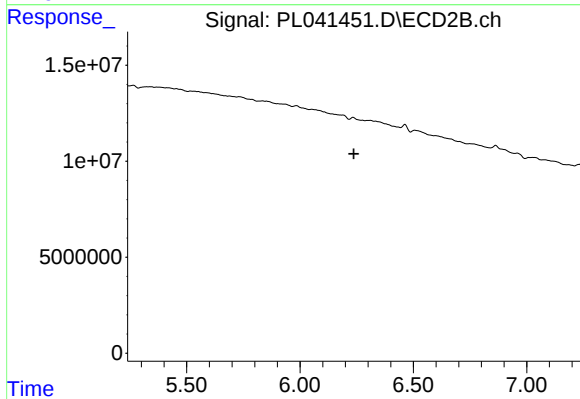

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

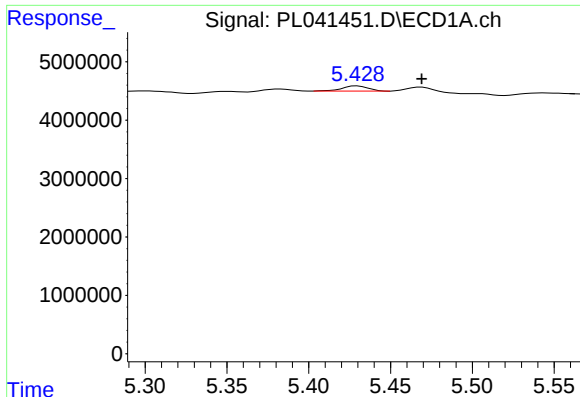

#11 alpha-Chlordane


R.T.: 5.430 min
Delta R.T.: -0.039 min
Response: 983383
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

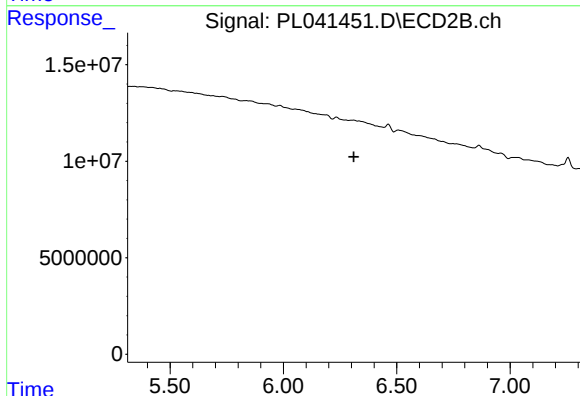


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

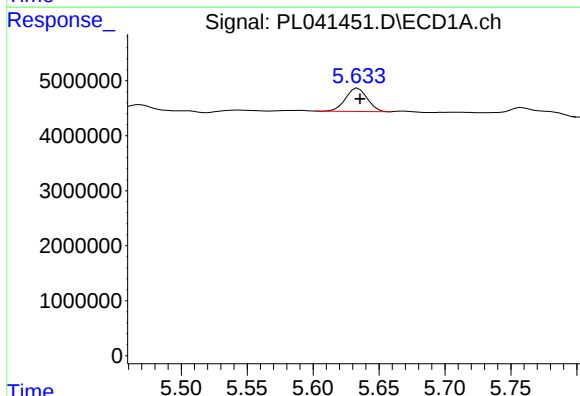


#12 4,4'-DDE

R.T.: 5.634 min
Delta R.T.: -0.001 min
Response: 4807048
Conc: 0.67 ng/ml

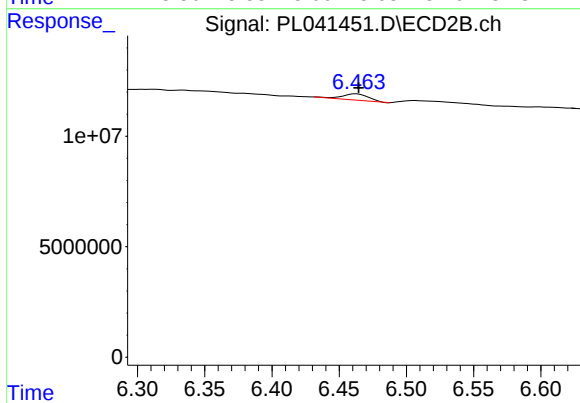

#12 4,4'-DDE


R.T.: 6.463 min
Delta R.T.: -0.002 min
Response: 3924333
Conc: 1.20 ng/ml

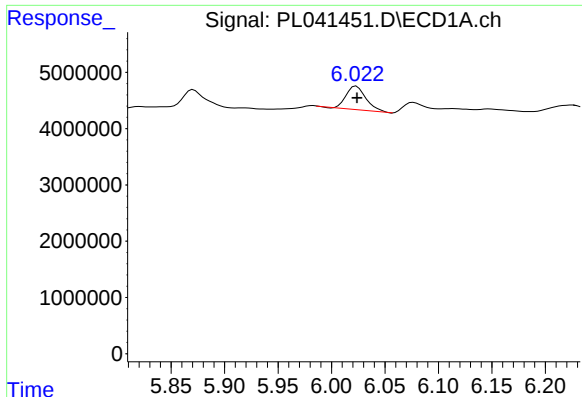

#14 Endrin


R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 5470234
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

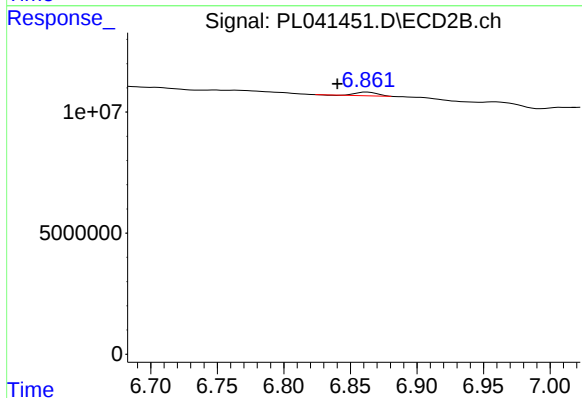


#14 Endrin

R.T.: 6.863 min
Delta R.T.: 0.023 min
Response: 1671269
Conc: 0.61 ng/ml

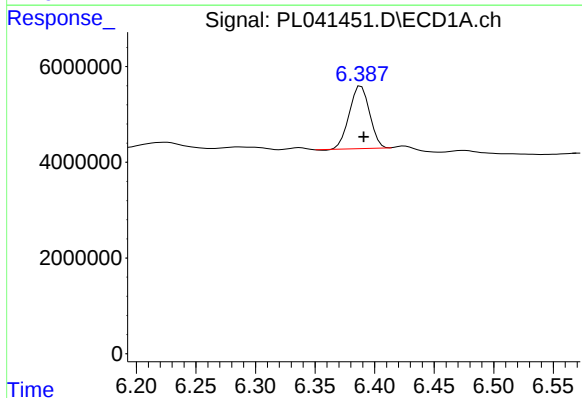


#17 4,4'-DDT

R.T.: 6.389 min
Delta R.T.: -0.002 min
Response: 15452773
Conc: 2.54 ng/ml

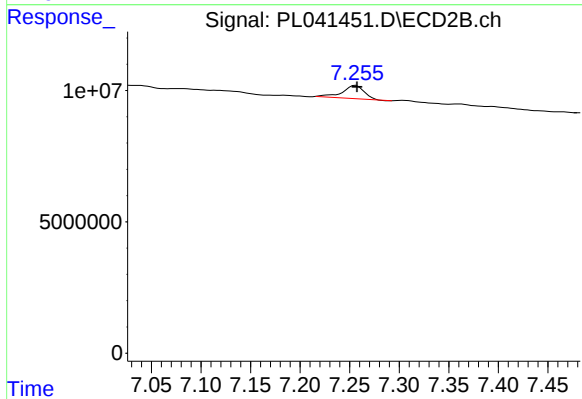

#17 4,4'-DDT


R.T.: 7.256 min
Delta R.T.: -0.001 min
Response: 7760241
Conc: 3.09 ng/ml

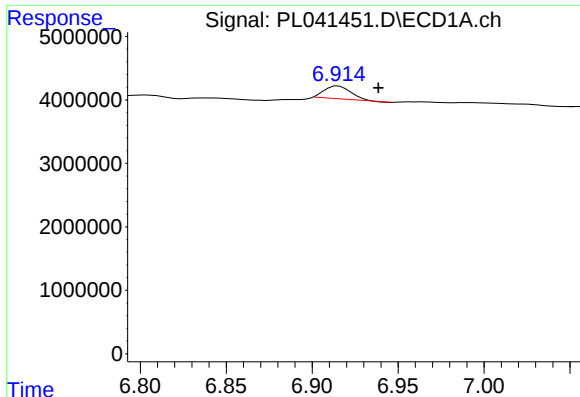

#20 Methoxychlor


R.T.: 6.915 min
Delta R.T.: -0.023 min
Response: 2172035
Conc: 0.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

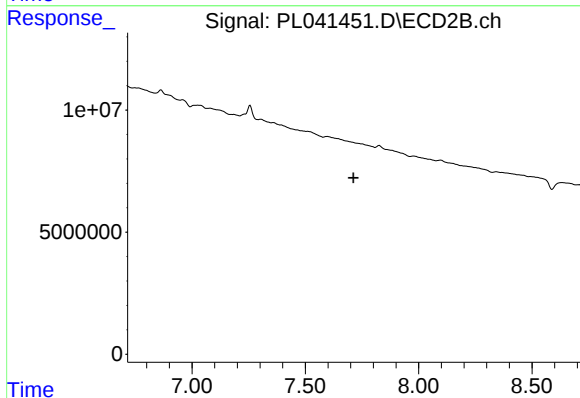


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.713 min
Response: 0
Conc: N.D.

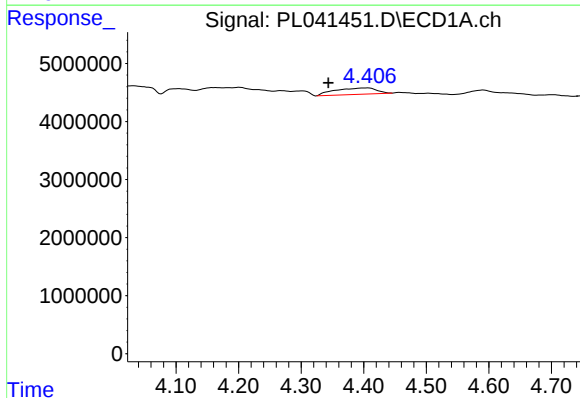


#23 Chlordane-1

R.T.: 4.407 min
Delta R.T.: 0.063 min
Response: 5078361
Conc: 17.91 ng/ml

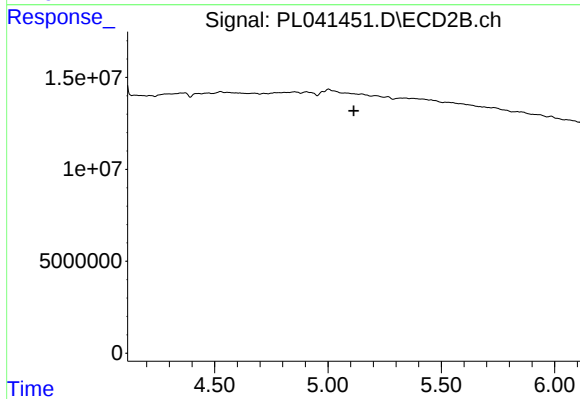

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

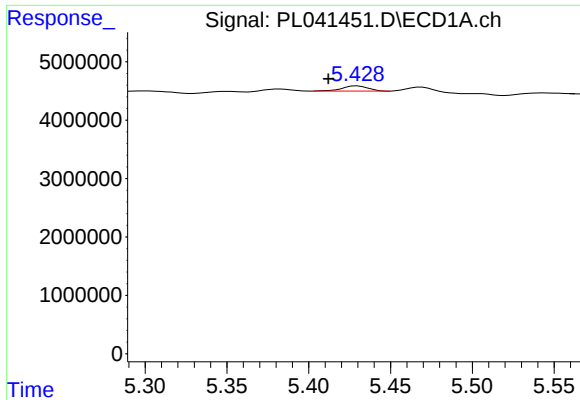

#25 Chlordane-3


R.T.: 5.430 min
Delta R.T.: 0.018 min
Response: 983383
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

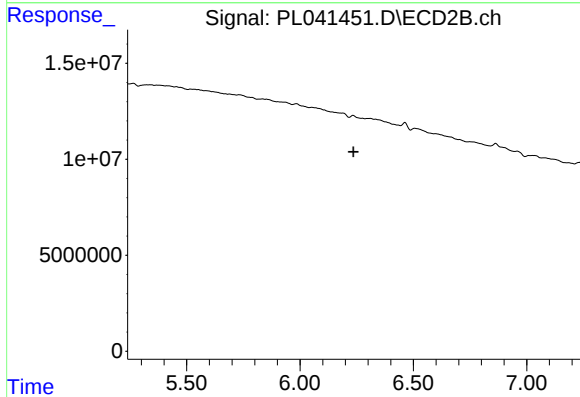


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

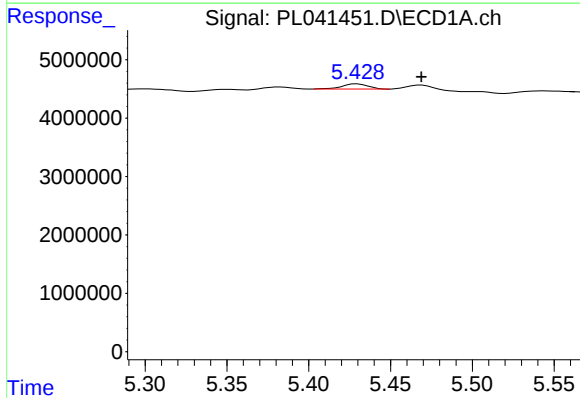


#26 Chlordane-4

R.T.: 5.430 min
Delta R.T.: -0.039 min
Response: 983383
Conc: 1.26 ng/ml

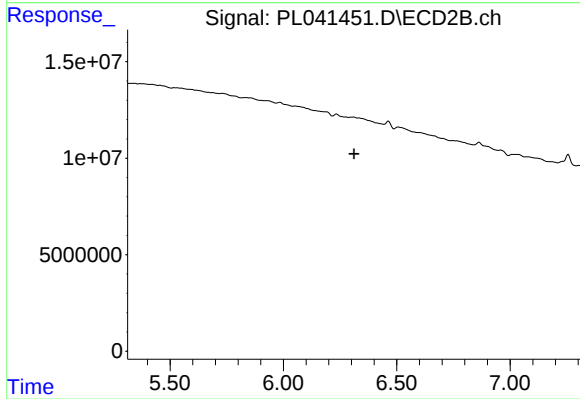

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

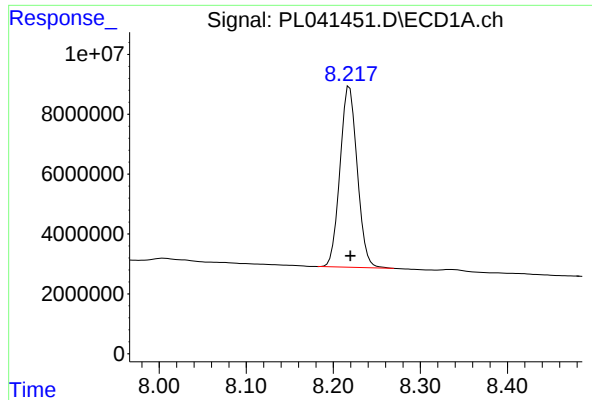

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 83128680
Conc: 12.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-58-66-98-92

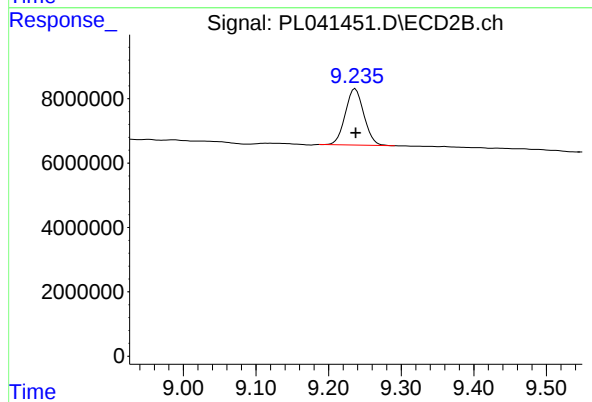

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 31093261
Conc: 12.14 ng/ml