

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 17:58
 Operator : AJ\SJ
 Sample : J5618-08RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1019-S-DH-16RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 02:33:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.104	51669495	26468498	8.111	8.593
28)	SA Decachlor...	8.218	9.236	63288713	24366279	9.554	9.510
Target Compounds							
9)	A Endosulfan I	5.468f	6.311f	2150770	3084696	0.289	0.993 #
10)	B gamma-Chl...	5.431	0.000	4890659	0	0.601	N.D. #
11)	B alpha-Chl...	5.468	6.311	2150770	3084696	0.266	0.911 #
12)	B 4,4'-DDE	5.634	6.464	35873961	18981666	5.012	5.800
14)	MA Endrin	6.023	6.862	5520737	2488056	0.755	0.915
17)	MA 4,4'-DDT	6.389	7.256	14372181	7491995	2.362	2.980 #
25)	Chlordane-3	5.431	0.000	4890659	0	5.487	N.D. #
26)	Chlordane-4	5.468	6.311	2150770	3084696	2.747	5.900 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 17:58
Operator : AJ\SJ
Sample : J5618-08RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-1019-S-DH-16RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 02:33:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

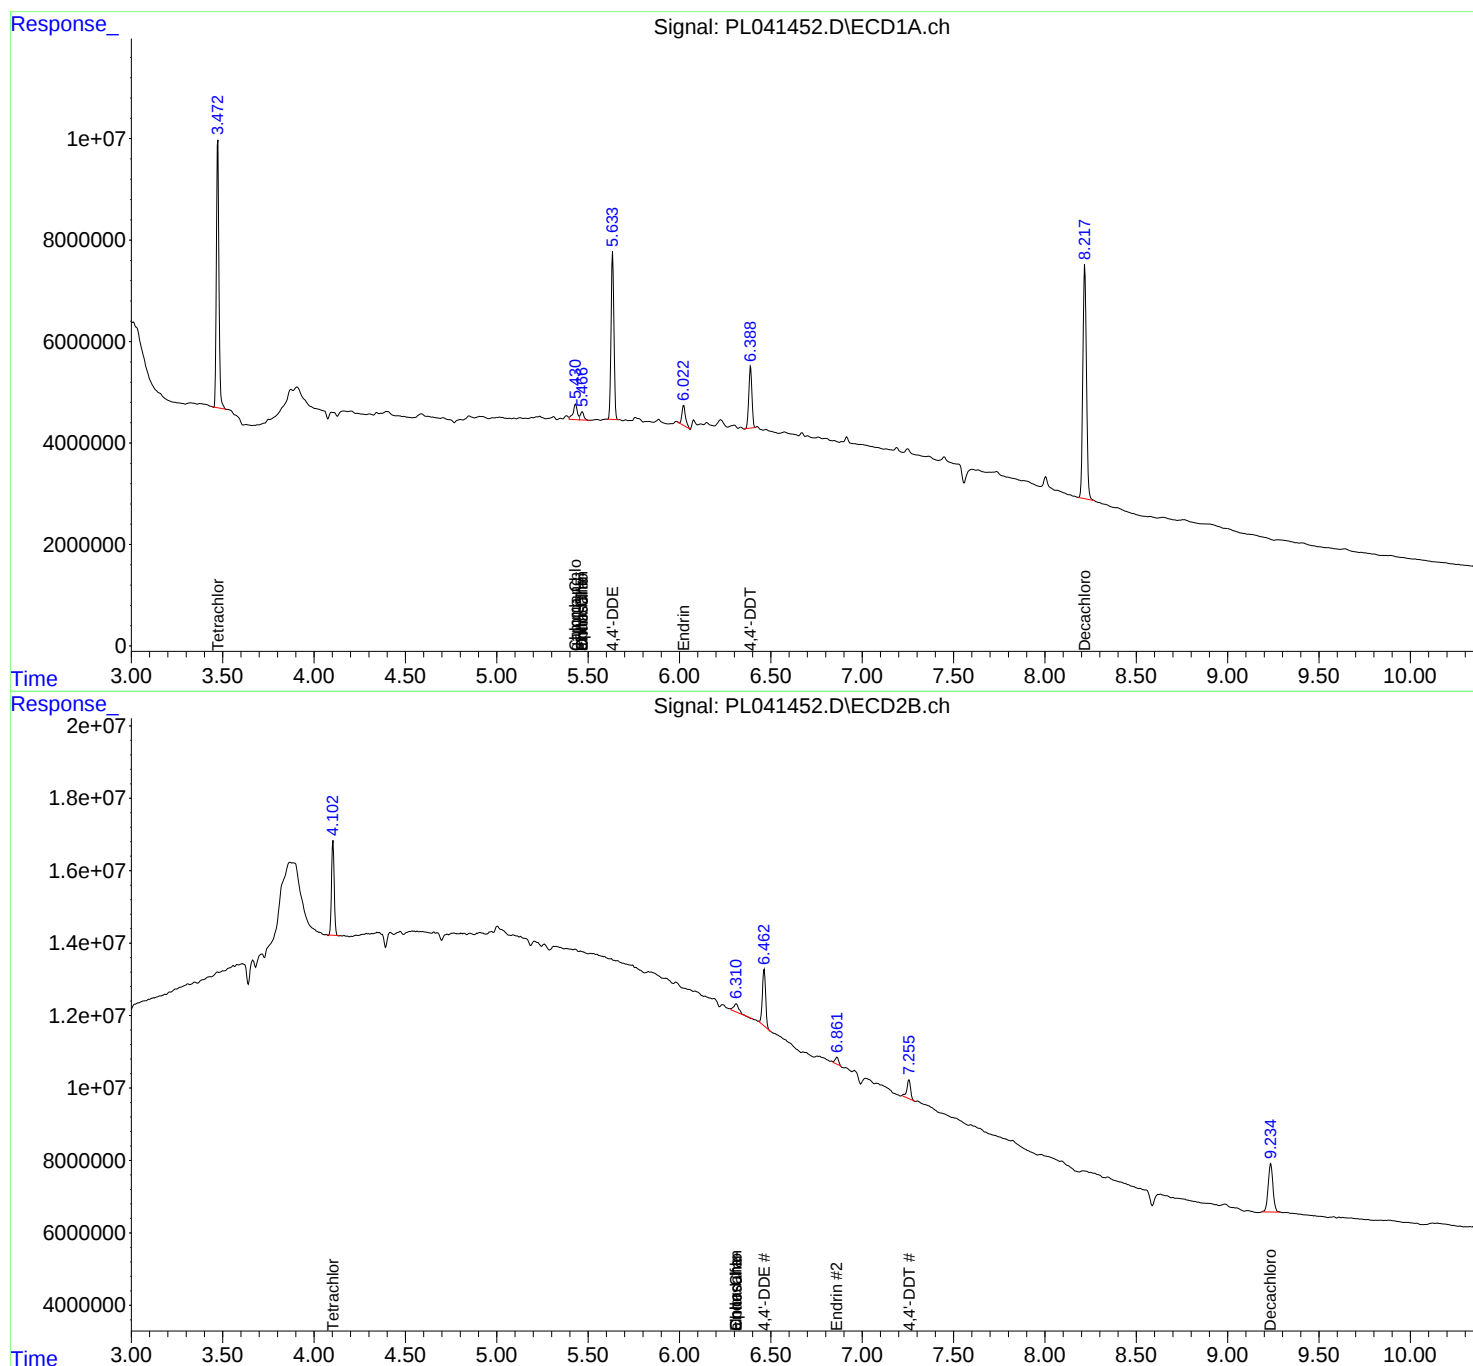


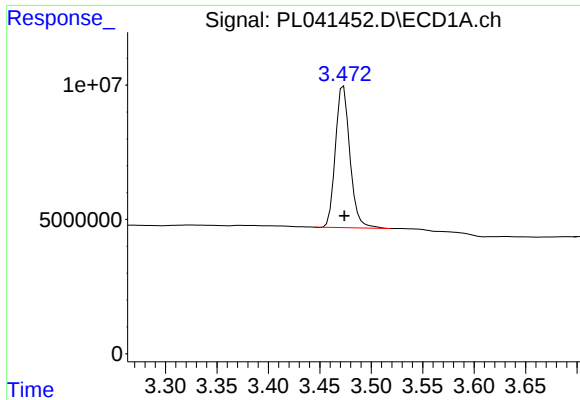

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 51669495
Conc: 8.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1019-S-DH-16RE

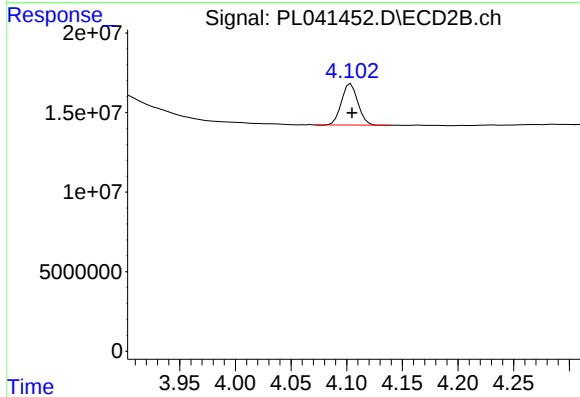


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 26468498
Conc: 8.59 ng/ml

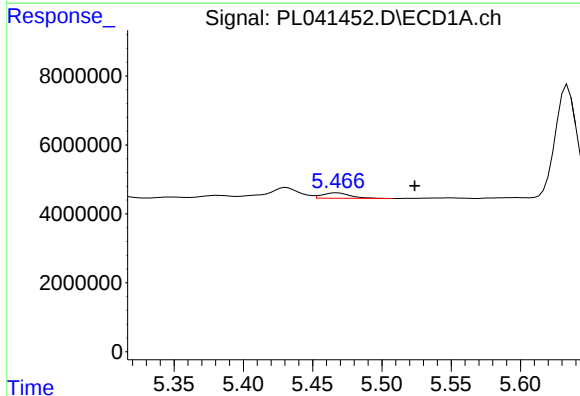


#9 Endosulfan I

R.T.: 5.468 min
Delta R.T.: -0.056 min
Response: 2150770
Conc: 0.29 ng/ml

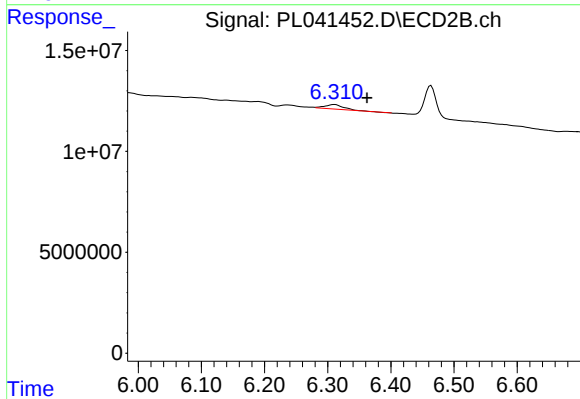

#9 Endosulfan I


R.T.: 6.311 min
Delta R.T.: -0.051 min
Response: 3084696
Conc: 0.99 ng/ml

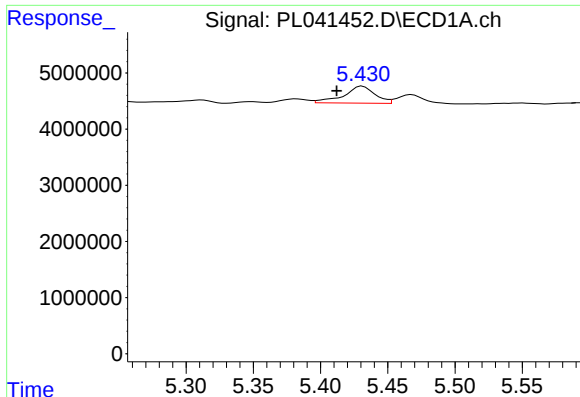

#10 gamma-Chlordane


R.T.: 5.431 min
Delta R.T.: 0.019 min
Response: 4890659
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1019-S-DH-16RE

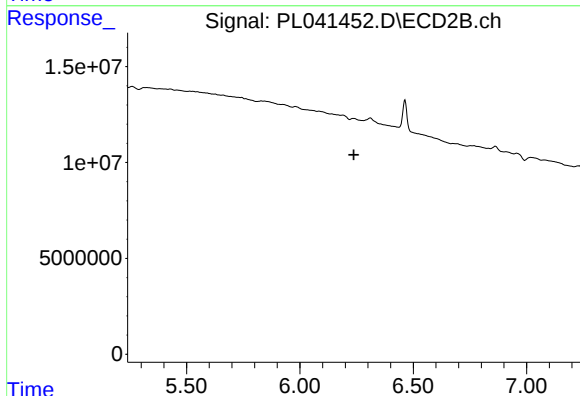


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

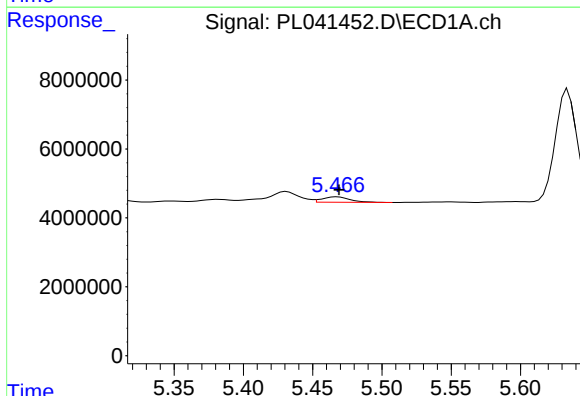


#11 alpha-Chlordane

R.T.: 5.468 min
Delta R.T.: -0.001 min
Response: 2150770
Conc: 0.27 ng/ml

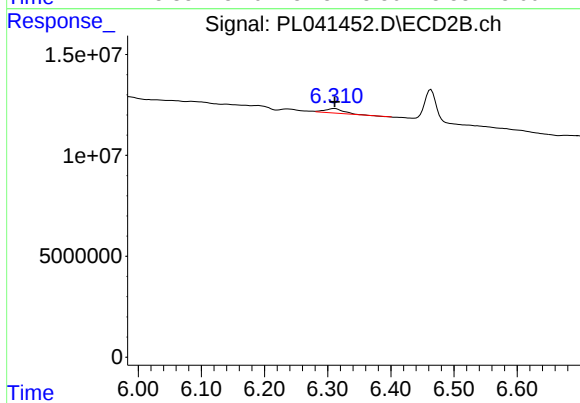

#11 alpha-Chlordane


R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 3084696
Conc: 0.91 ng/ml

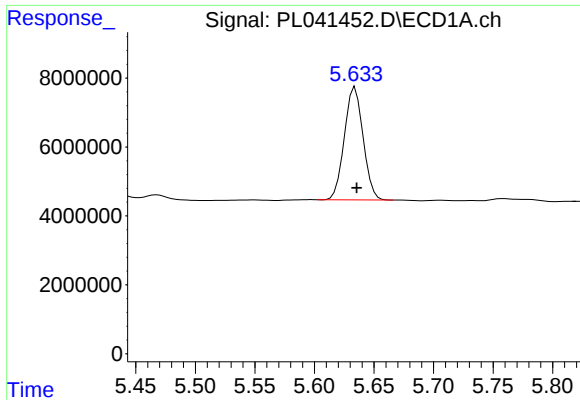

#12 4,4'-DDE


R.T.: 5.634 min
Delta R.T.: -0.001 min
Response: 35873961
Conc: 5.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1019-S-DH-16RE

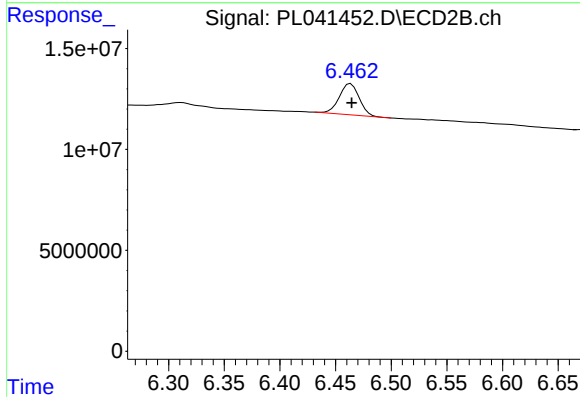


#12 4,4'-DDE

R.T.: 6.464 min
Delta R.T.: -0.001 min
Response: 18981666
Conc: 5.80 ng/ml

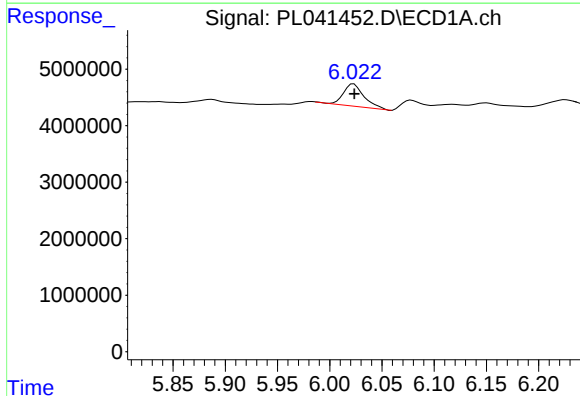


#14 Endrin

R.T.: 6.023 min
Delta R.T.: 0.000 min
Response: 5520737
Conc: 0.75 ng/ml

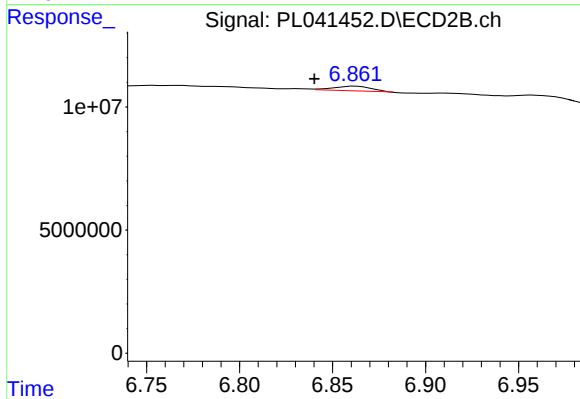

#14 Endrin


R.T.: 6.862 min
Delta R.T.: 0.022 min
Response: 2488056
Conc: 0.92 ng/ml

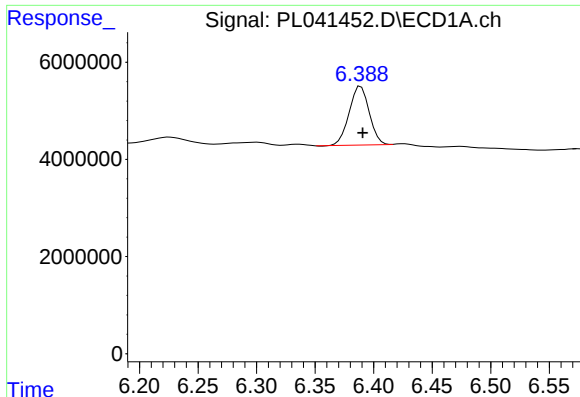

#17 4,4'-DDT


R.T.: 6.389 min
Delta R.T.: -0.002 min
Response: 14372181
Conc: 2.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1019-S-DH-16RE

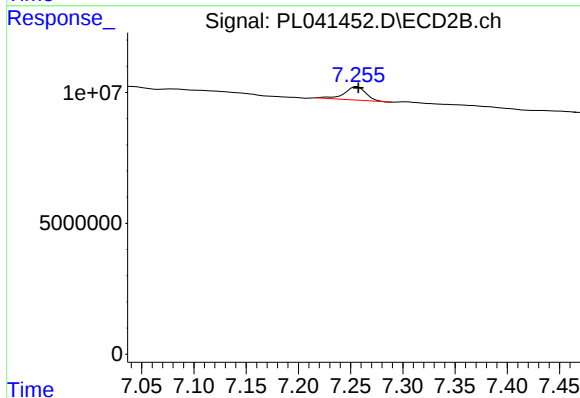


#17 4,4'-DDT

R.T.: 7.256 min
Delta R.T.: -0.001 min
Response: 7491995
Conc: 2.98 ng/ml

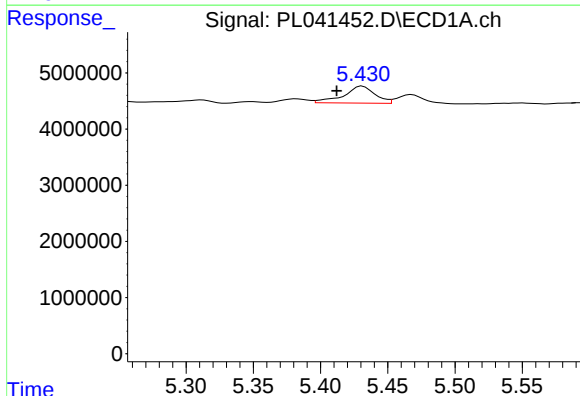


#25 Chlordane-3

R.T.: 5.431 min
Delta R.T.: 0.019 min
Response: 4890659
Conc: 5.49 ng/ml

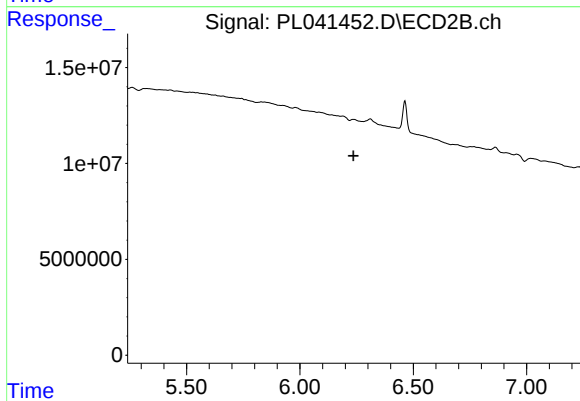

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

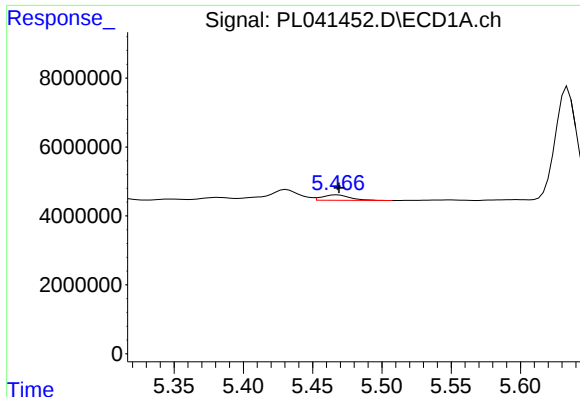

#26 Chlordane-4


R.T.: 5.468 min
Delta R.T.: -0.001 min
Response: 2150770
Conc: 2.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1019-S-DH-16RE

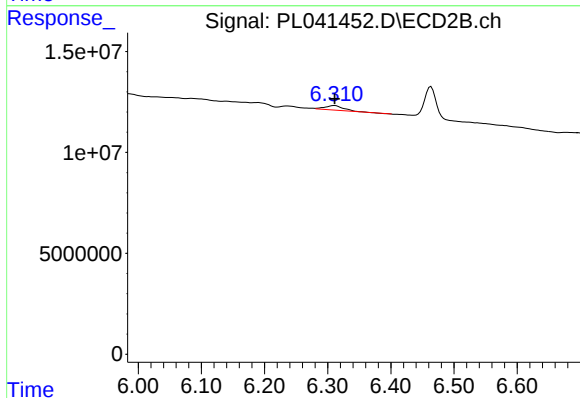


#26 Chlordane-4

R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 3084696
Conc: 5.90 ng/ml

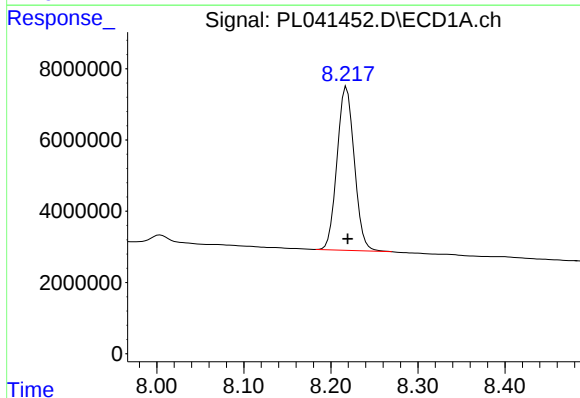

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: -0.001 min
Response: 63288713
Conc: 9.55 ng/ml

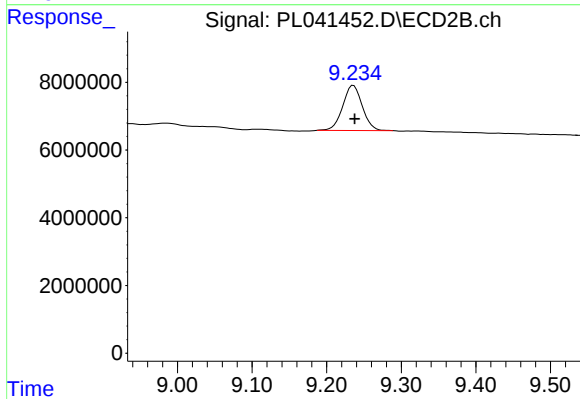

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.002 min
Response: 24366279
Conc: 9.51 ng/ml