

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 18:40
 Operator : AJ\SJ
 Sample : J5676-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 02:34:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.104	121.4E6	60311310	19.062	19.580
28)	SA Decachlor...	8.219	9.236	132.5E6	53534551	20.006	20.894
Target Compounds							
9)	A Endosulfan I	5.469f	0.000	2142292	0	0.288	N.D. #
10)	B gamma-Chl...	5.383	6.238	347077	1695510	0.043	0.502 #
11)	B alpha-Chl...	5.469	0.000	2142292	0	0.265	N.D. #
14)	MA Endrin	0.000	6.772f	0	1161452	N.D.	0.427 #
15)	B Endosulfa...	6.228f	7.038	2327751	2539685	0.337	0.939 #
23)	Chlordane-1	4.386	0.000	1453893	0	5.128	N.D. #
25)	Chlordane-3	5.383	6.238	347077	1695510	0.389	3.768 #
26)	Chlordane-4	5.469	0.000	2142292	0	2.736	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 18:40
Operator : AJ\SJ
Sample : J5676-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 02:34:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

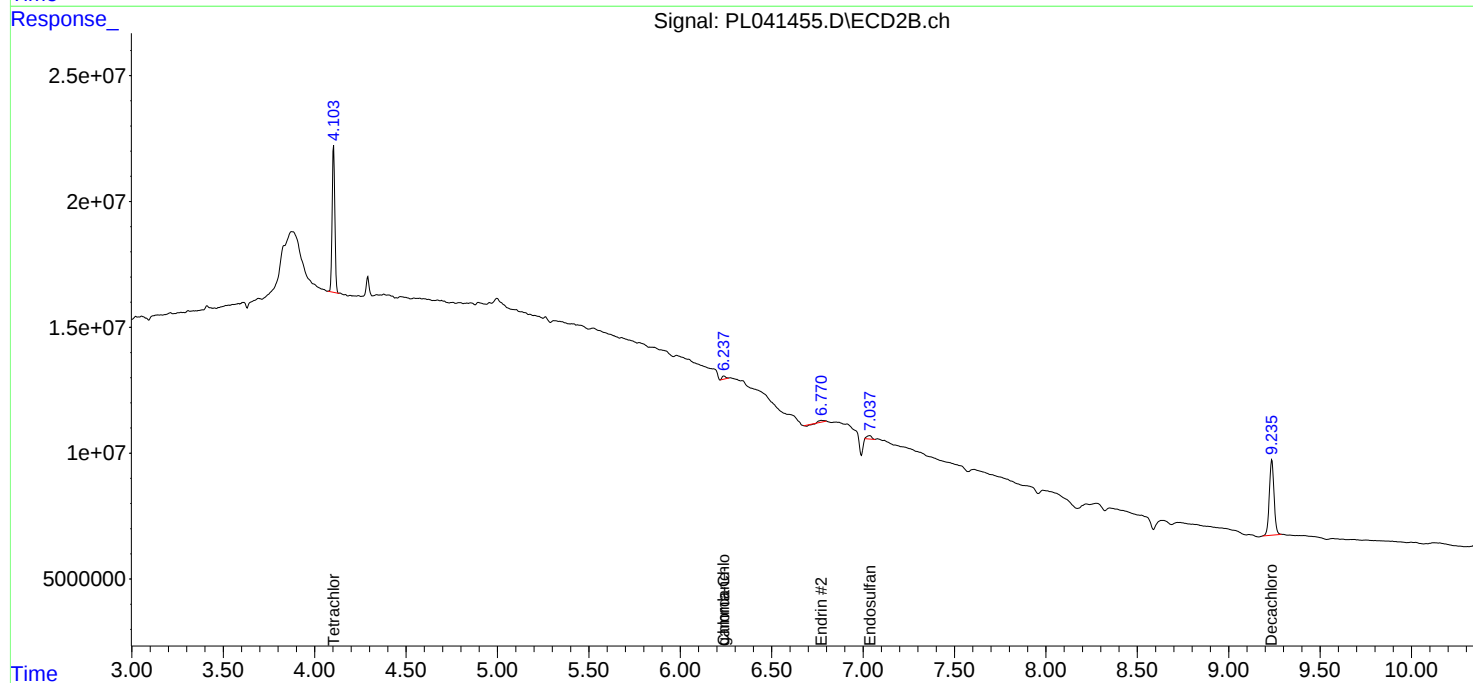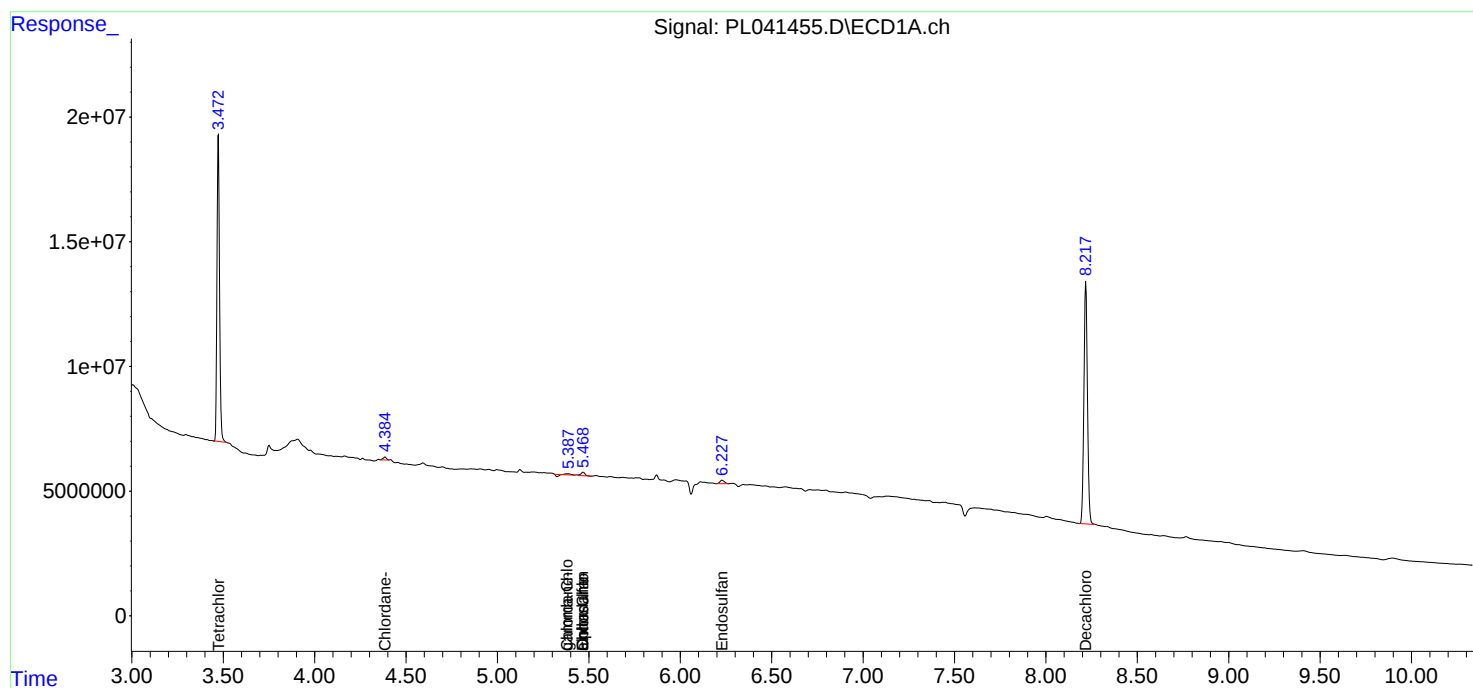


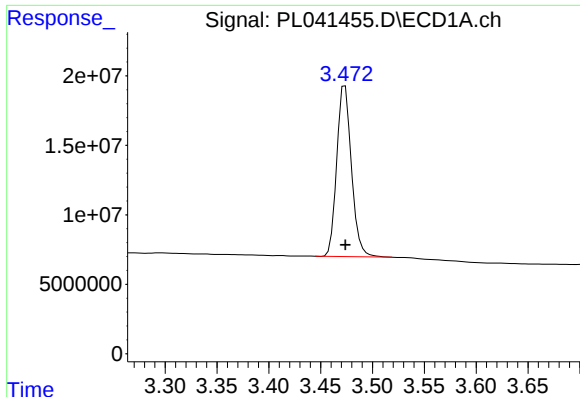

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 121428172
Conc: 19.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

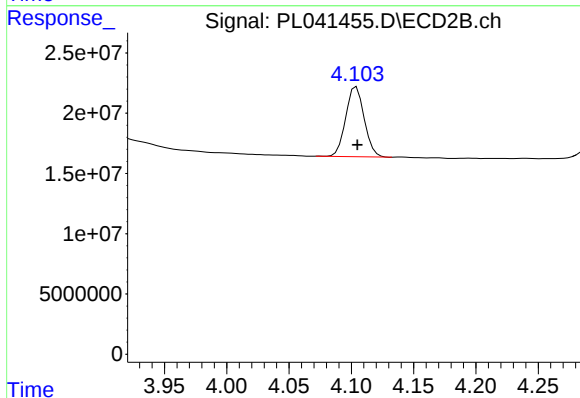


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 60311310
Conc: 19.58 ng/ml

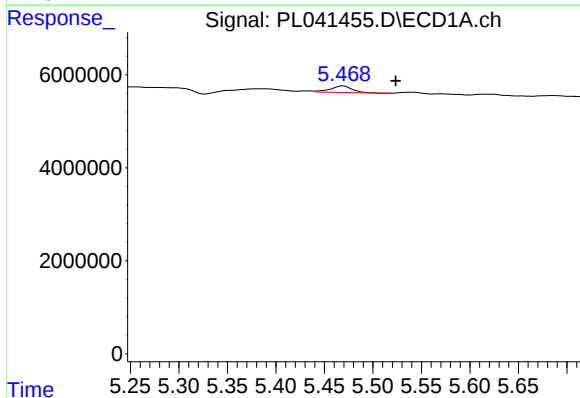


#9 Endosulfan I

R.T.: 5.469 min
Delta R.T.: -0.054 min
Response: 2142292
Conc: 0.29 ng/ml

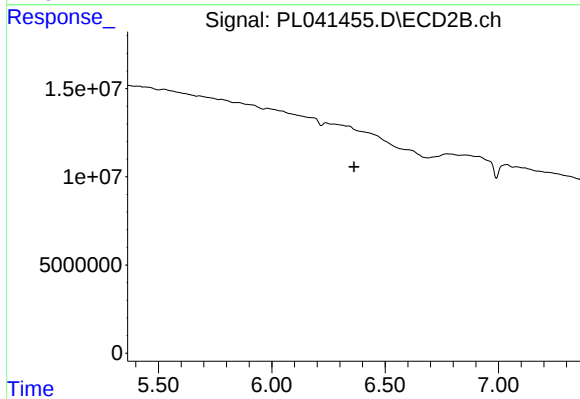

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

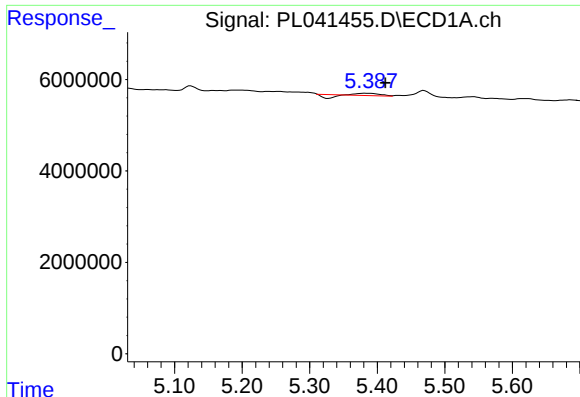

#10 gamma-Chlordane


R.T.: 5.383 min
Delta R.T.: -0.029 min
Response: 347077
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

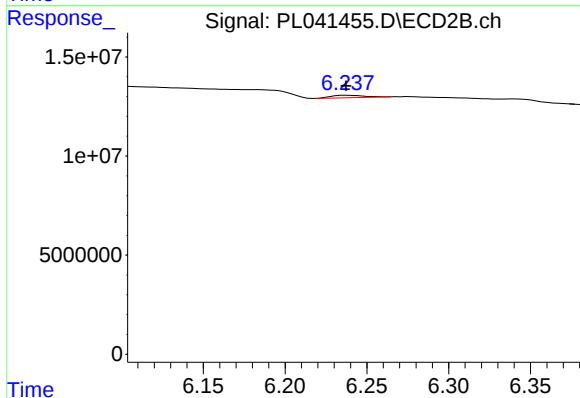


#10 gamma-Chlordane

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 1695510
Conc: 0.50 ng/ml

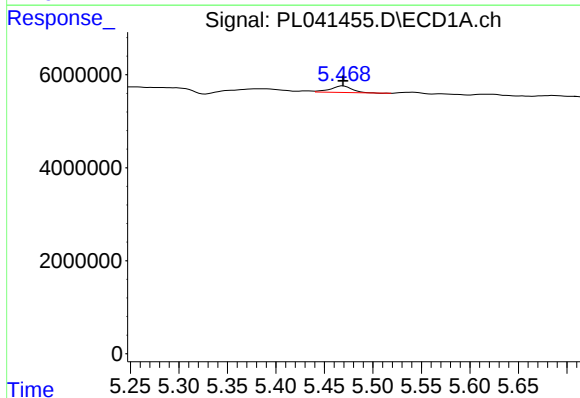


#11 alpha-Chlordane

R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 2142292
Conc: 0.26 ng/ml

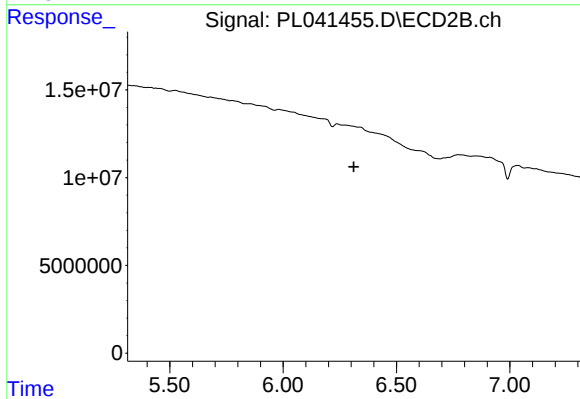

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

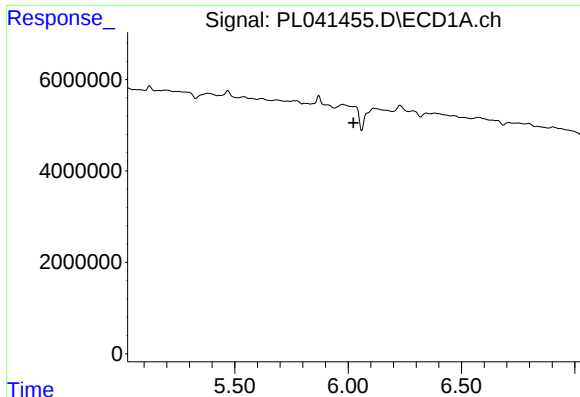

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

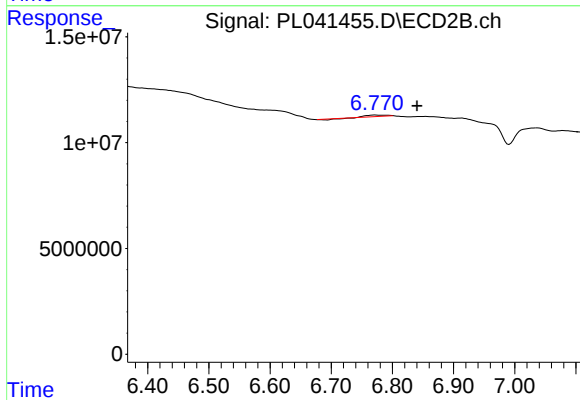


#14 Endrin

R.T.: 6.772 min
Delta R.T.: -0.068 min
Response: 1161452
Conc: 0.43 ng/ml

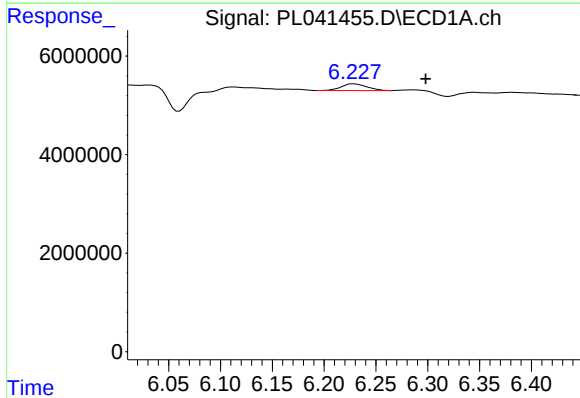


#15 Endosulfan II

R.T.: 6.228 min
Delta R.T.: -0.070 min
Response: 2327751
Conc: 0.34 ng/ml

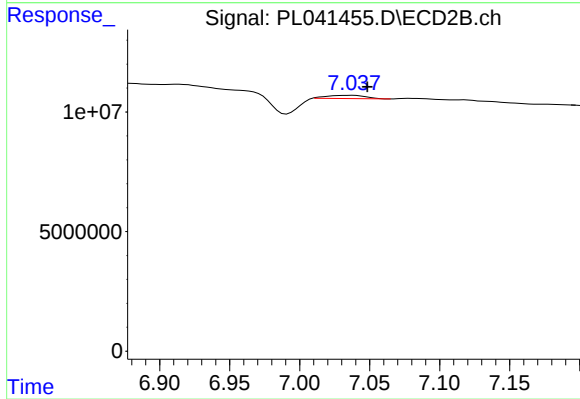

#15 Endosulfan II


R.T.: 7.038 min
Delta R.T.: -0.011 min
Response: 2539685
Conc: 0.94 ng/ml

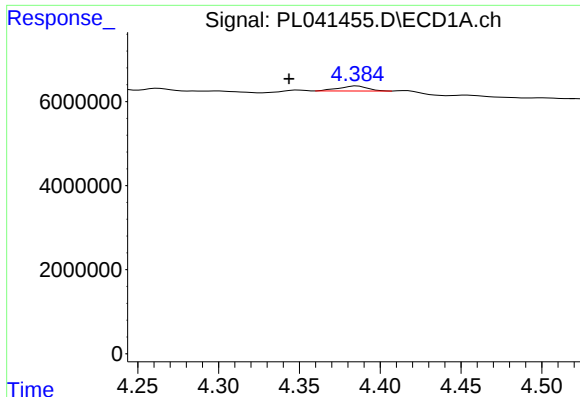

#23 Chlordane-1


R.T.: 4.386 min
Delta R.T.: 0.042 min
Response: 1453893
Conc: 5.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

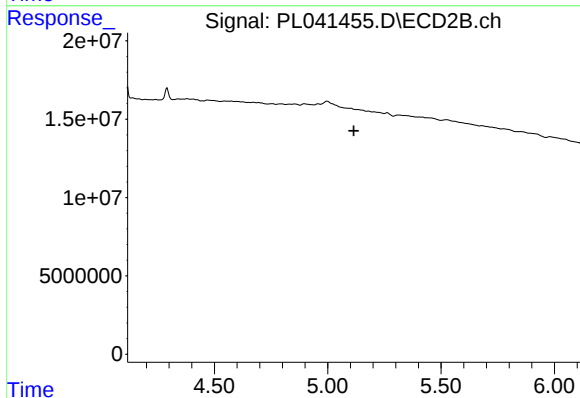


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

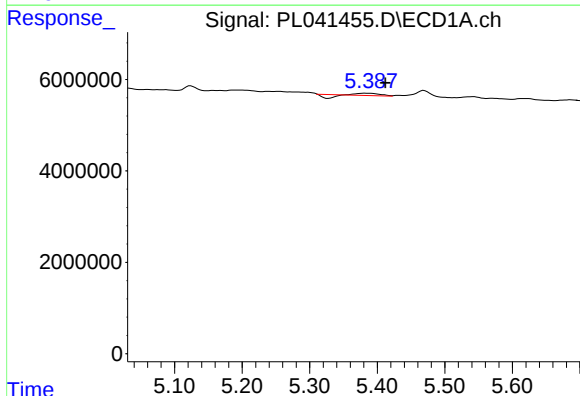


#25 Chlordane-3

R.T.: 5.383 min
Delta R.T.: -0.029 min
Response: 347077
Conc: 0.39 ng/ml

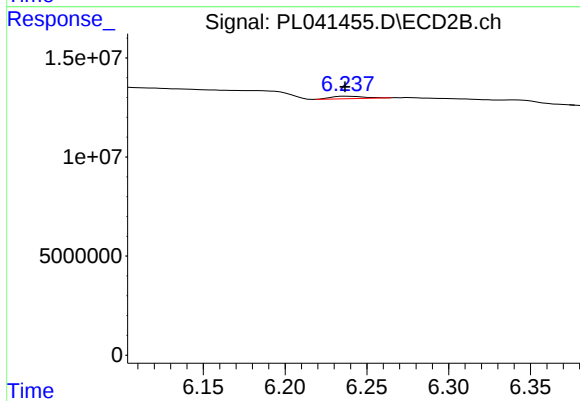

#25 Chlordane-3


R.T.: 6.238 min
Delta R.T.: 0.002 min
Response: 1695510
Conc: 3.77 ng/ml

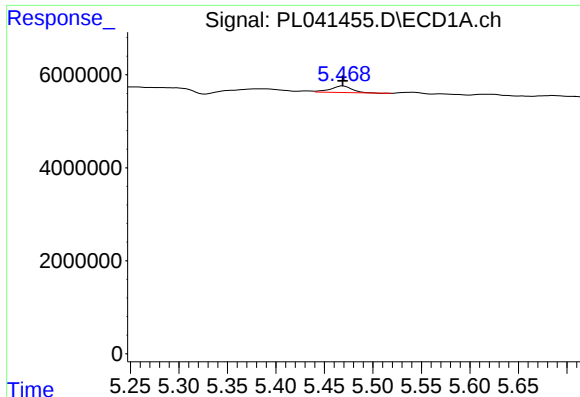

#26 Chlordane-4


R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 2142292
Conc: 2.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

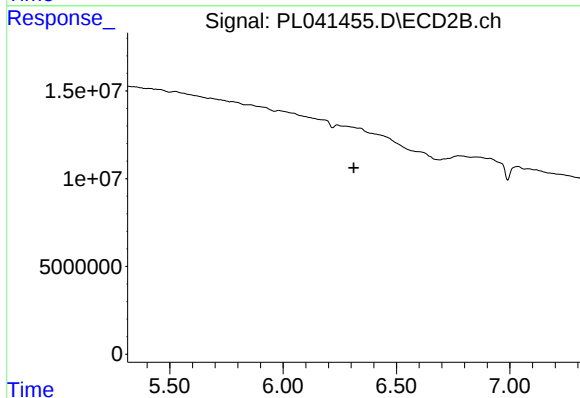


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.311 min
Response: 0
Conc: N.D.

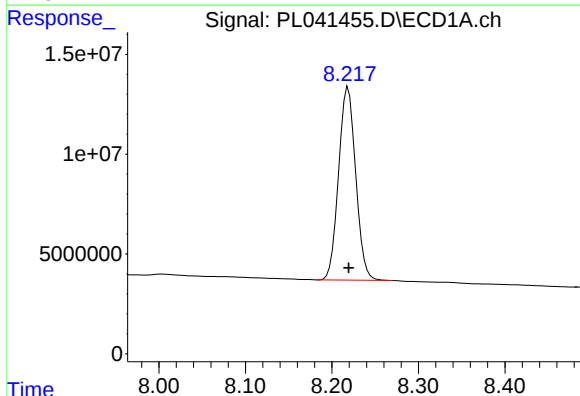

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 132521254
Conc: 20.01 ng/ml

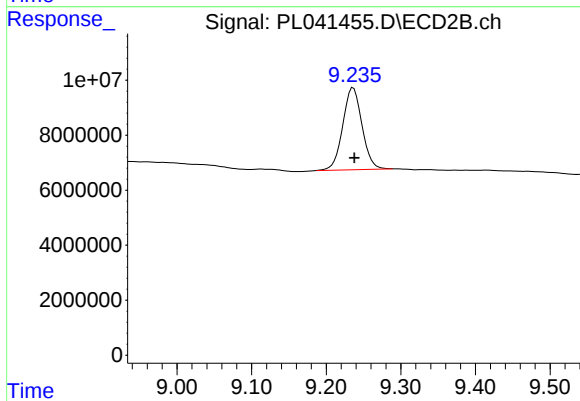

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.002 min
Response: 53534551
Conc: 20.89 ng/ml