

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 22:54
 Operator : AJ\SJ
 Sample : J5696-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EB-2018.10.25-SED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 02:41:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.104	119.0E6	57317617	18.686	18.608
28)	SA Decachlor...	8.218	9.236	90008700	34763663	13.588	13.568
Target Compounds							
2)	A alpha-BHC	3.877f	0.000	1474117	0	0.152	N.D. #
3)	MA gamma-BHC...	4.165f	0.000	49217	0	0.006	N.D. #
4)	MA Heptachlor	4.562f	0.000	1456832	0	0.159	N.D. #
6)	B beta-BHC	4.411f	0.000	1981291	0	0.526	N.D. #
7)	B delta-BHC	4.644	0.000	2804721	0	0.338	N.D. #
15)	B Endosulfa...	6.230f	0.000	2202631	0	0.319	N.D. #
19)	B Endosulfa...	6.661	0.000	4919828	0	0.770	N.D. #
23)	Chlordane-1	4.314	0.000	3552856	0	12.530	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 22:54
Operator : AJ\SJ
Sample : J5696-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EB-2018.10.25-SED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 02:41:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

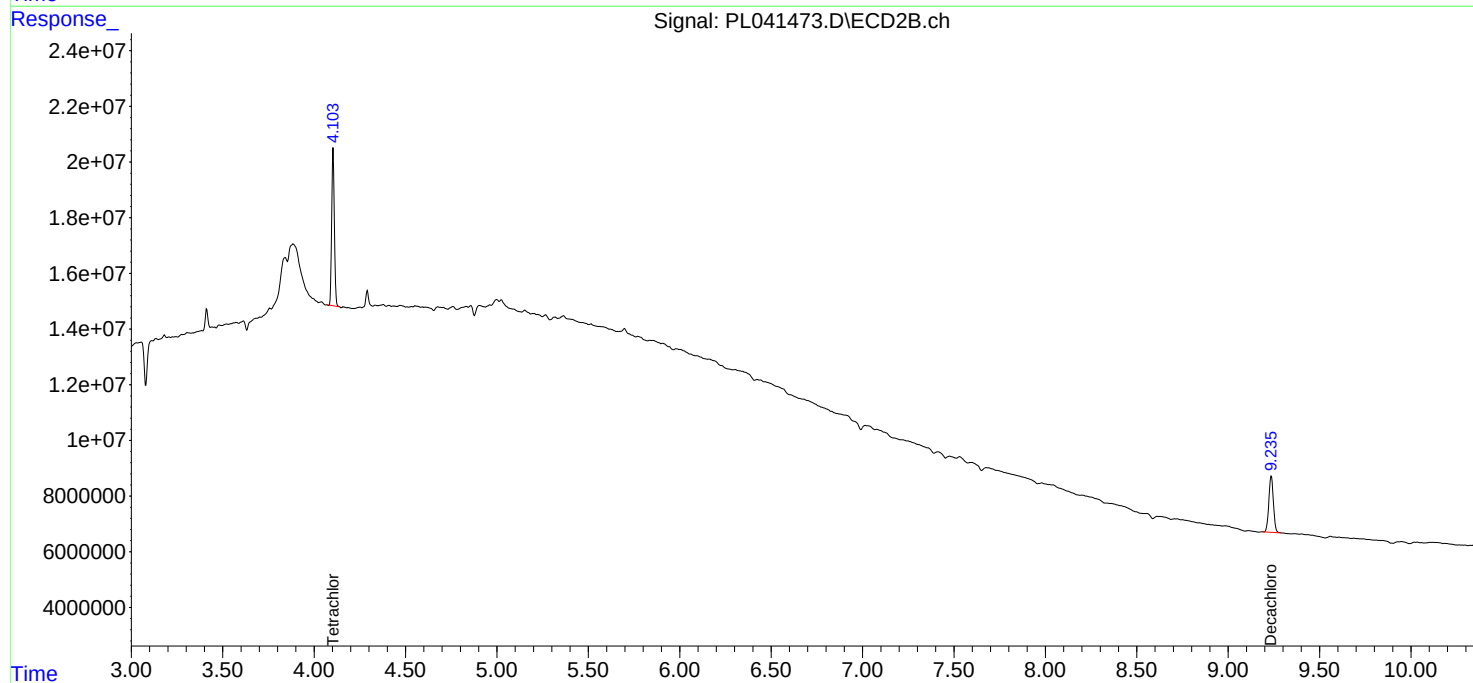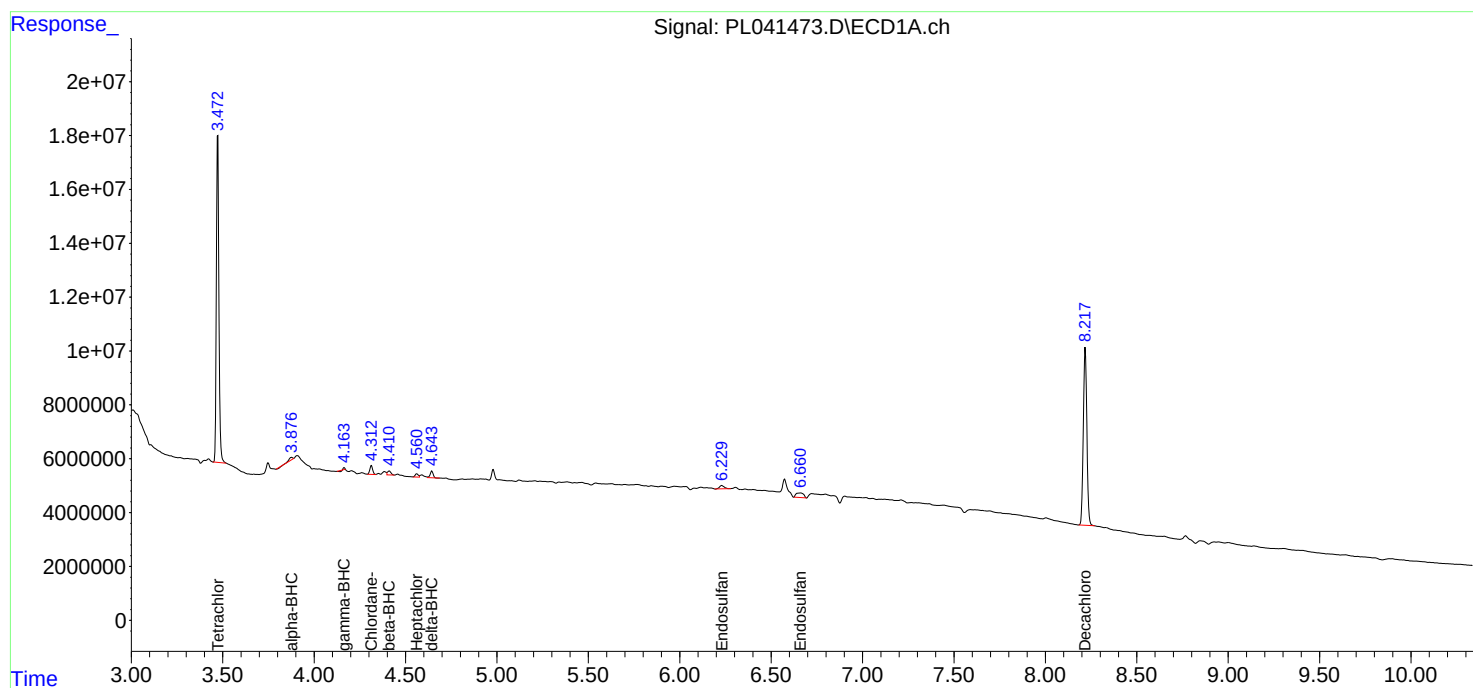


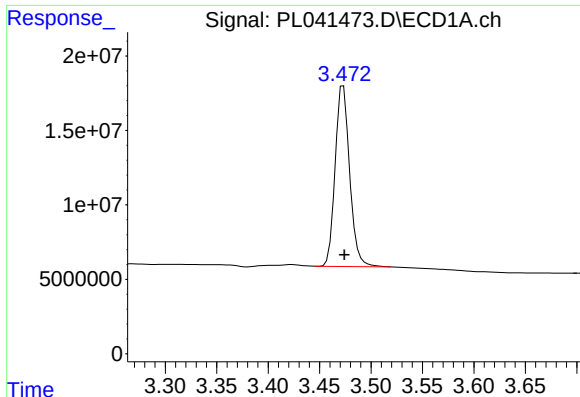

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 119035809
Conc: 18.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB-2018.10.25-SED

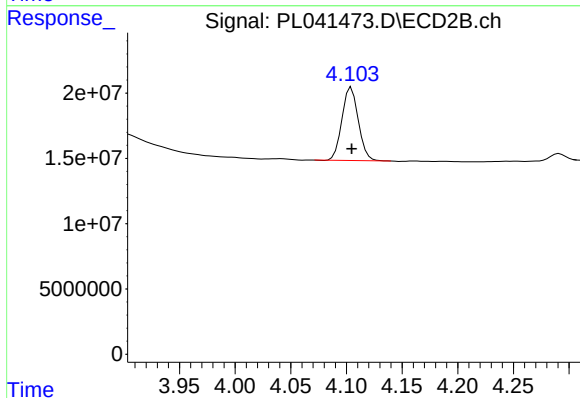


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 57317617
Conc: 18.61 ng/ml

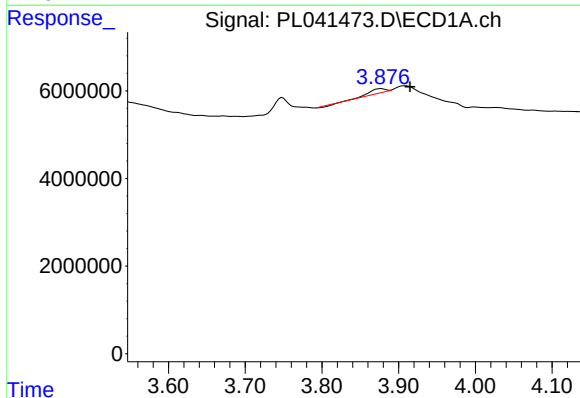


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: -0.038 min
Response: 1474117
Conc: 0.15 ng/ml

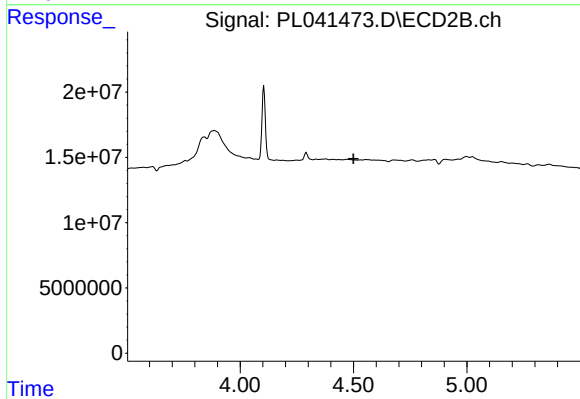

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

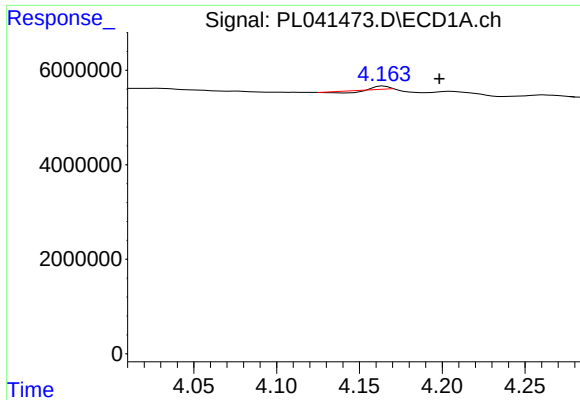

#3 gamma-BHC (Lindane)


R.T.: 4.165 min
Delta R.T.: -0.034 min
Response: 49217
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB-2018.10.25-SED

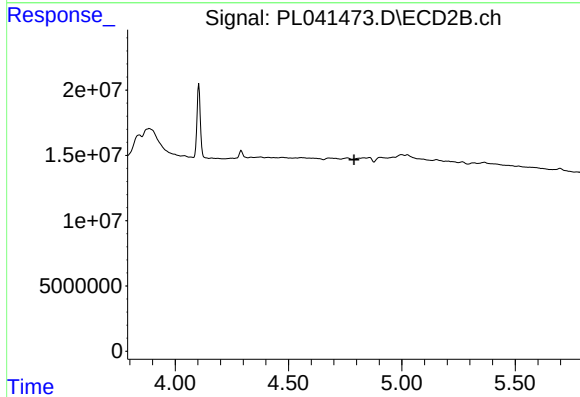


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.789 min
Response: 0
Conc: N.D.

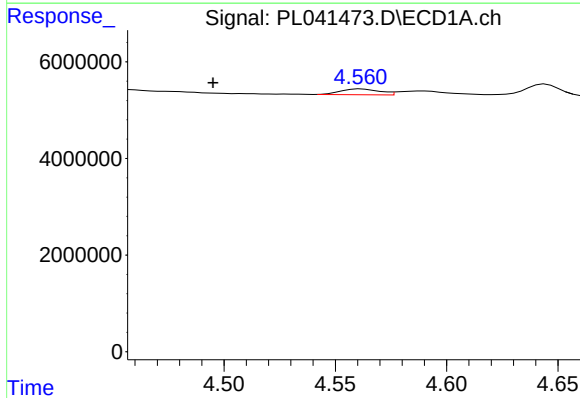


#4 Heptachlor

R.T.: 4.562 min
Delta R.T.: 0.066 min
Response: 1456832
Conc: 0.16 ng/ml

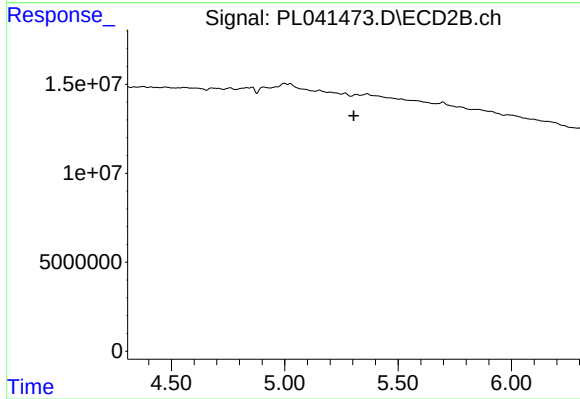

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.305 min
Response: 0
Conc: N.D.

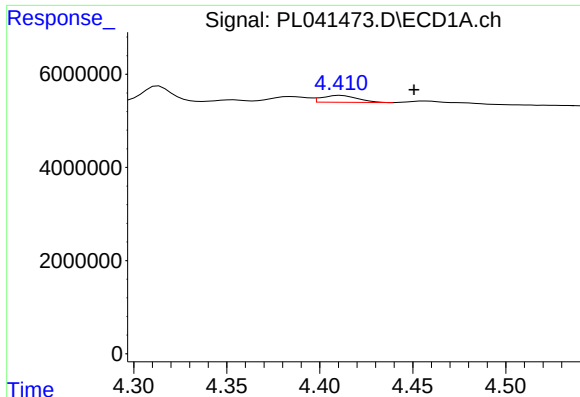

#6 beta-BHC


R.T.: 4.411 min
Delta R.T.: -0.039 min
Response: 1981291
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB-2018.10.25-SED

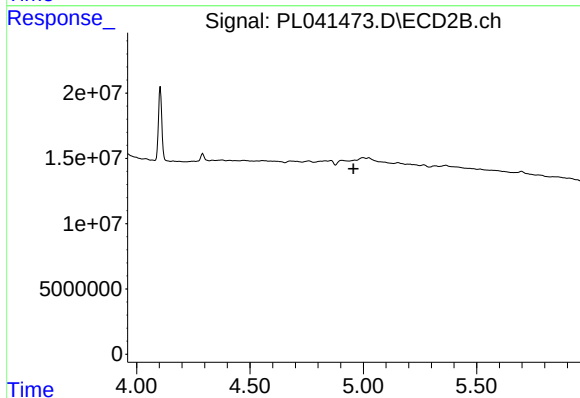


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

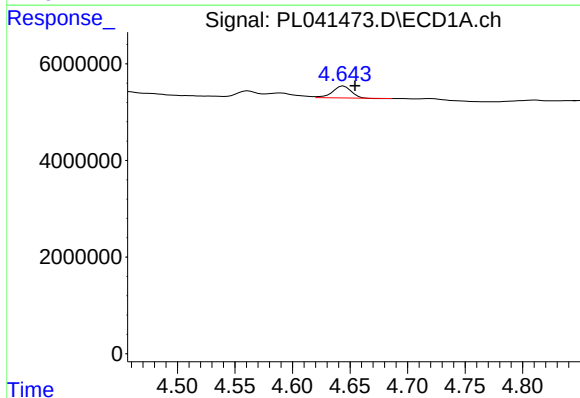


#7 delta-BHC

R.T.: 4.644 min
Delta R.T.: -0.010 min
Response: 2804721
Conc: 0.34 ng/ml

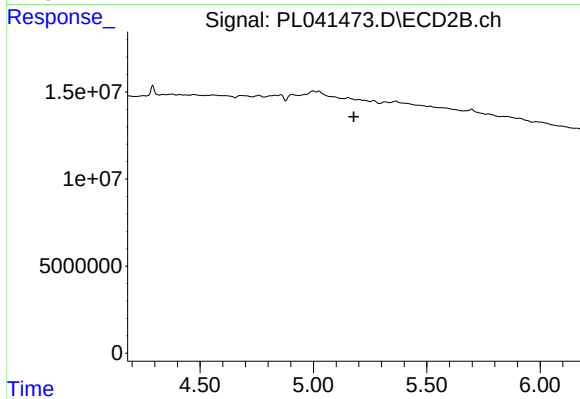

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.178 min
Response: 0
Conc: N.D.

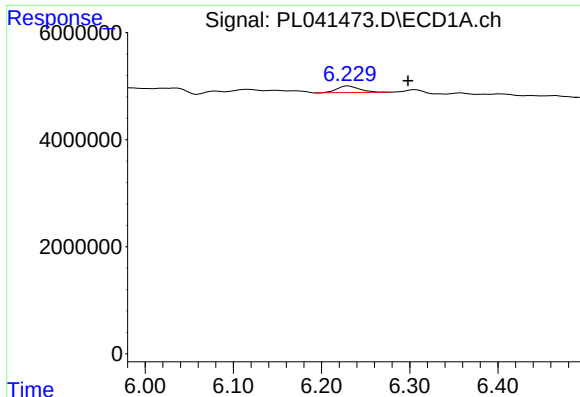

#15 Endosulfan II


R.T.: 6.230 min
Delta R.T.: -0.068 min
Response: 2202631
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB-2018.10.25-SED

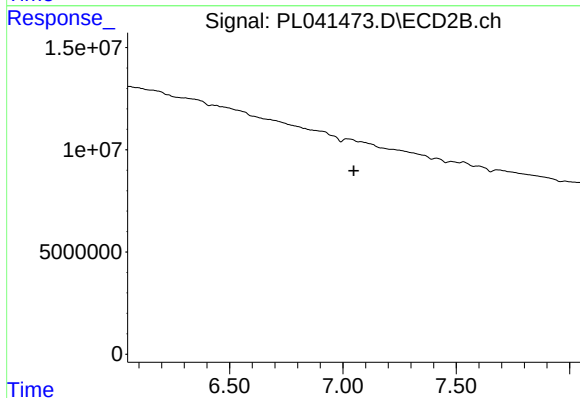


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

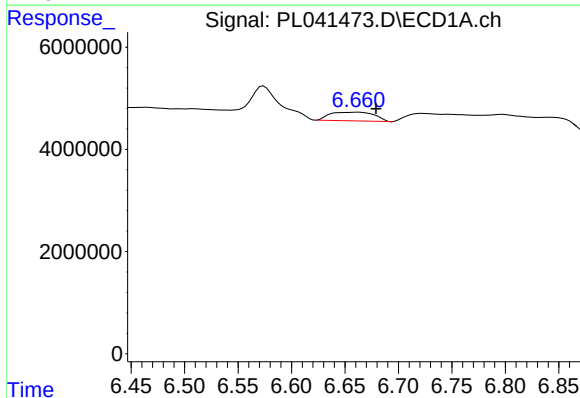


#19 Endosulfan Sulfate

R.T.: 6.661 min
Delta R.T.: -0.018 min
Response: 4919828
Conc: 0.77 ng/ml

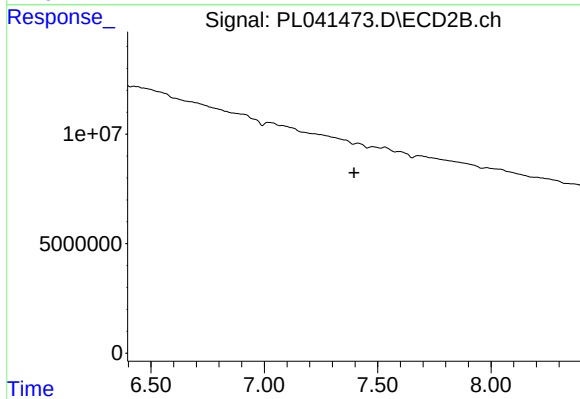

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.396 min
Response: 0
Conc: N.D.

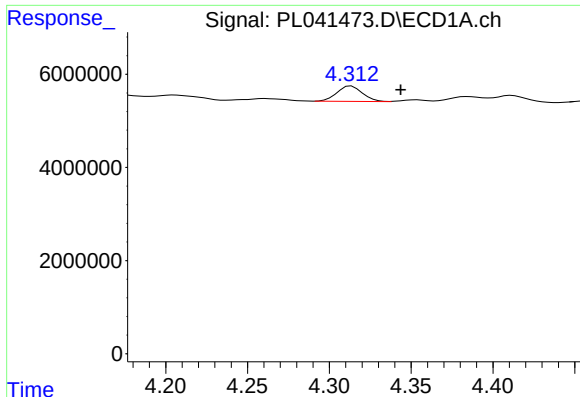

#23 Chlordane-1


R.T.: 4.314 min
Delta R.T.: -0.030 min
Response: 3552856
Conc: 12.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
EB-2018.10.25-SED

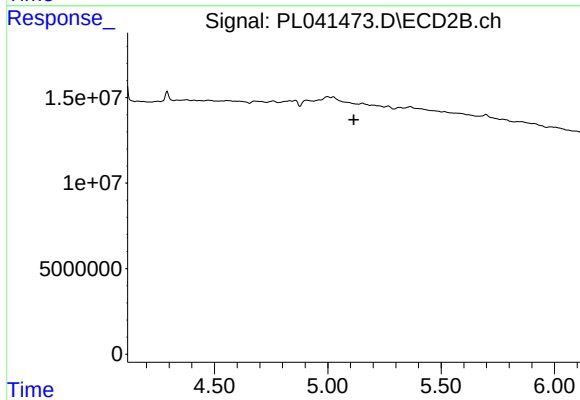


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

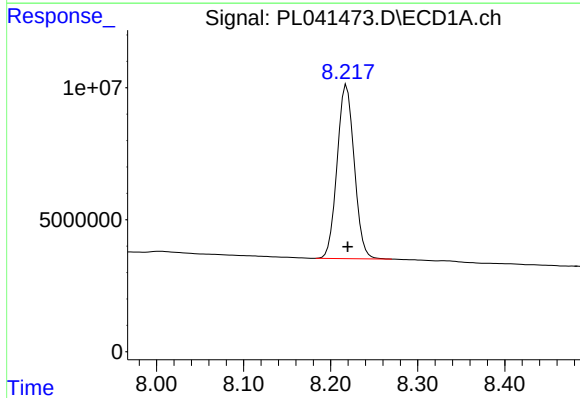

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: -0.001 min
Response: 90008700
Conc: 13.59 ng/ml

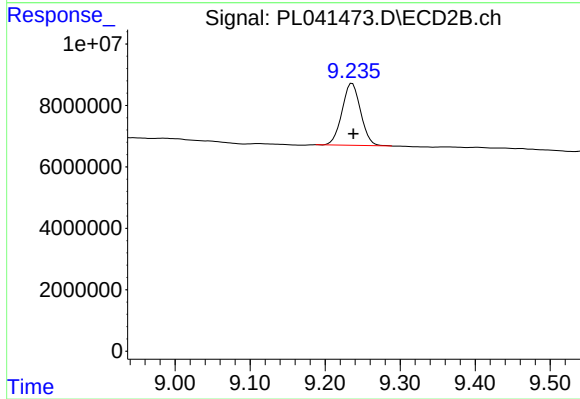

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.002 min
Response: 34763663
Conc: 13.57 ng/ml