

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 00:04
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 02:43:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.105	136.5E6	65846549	21.420	21.377
28)	SA Decachlor...	8.218	9.236	150.8E6	57851346	22.769	22.579
Target Compounds							
8)	B Heptachlo...	0.000	6.060f	0	5849841	N.D.	1.664 #
23)	Chlordane-1	4.371	0.000	413760	0	1.459	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 00:04
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 02:43:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

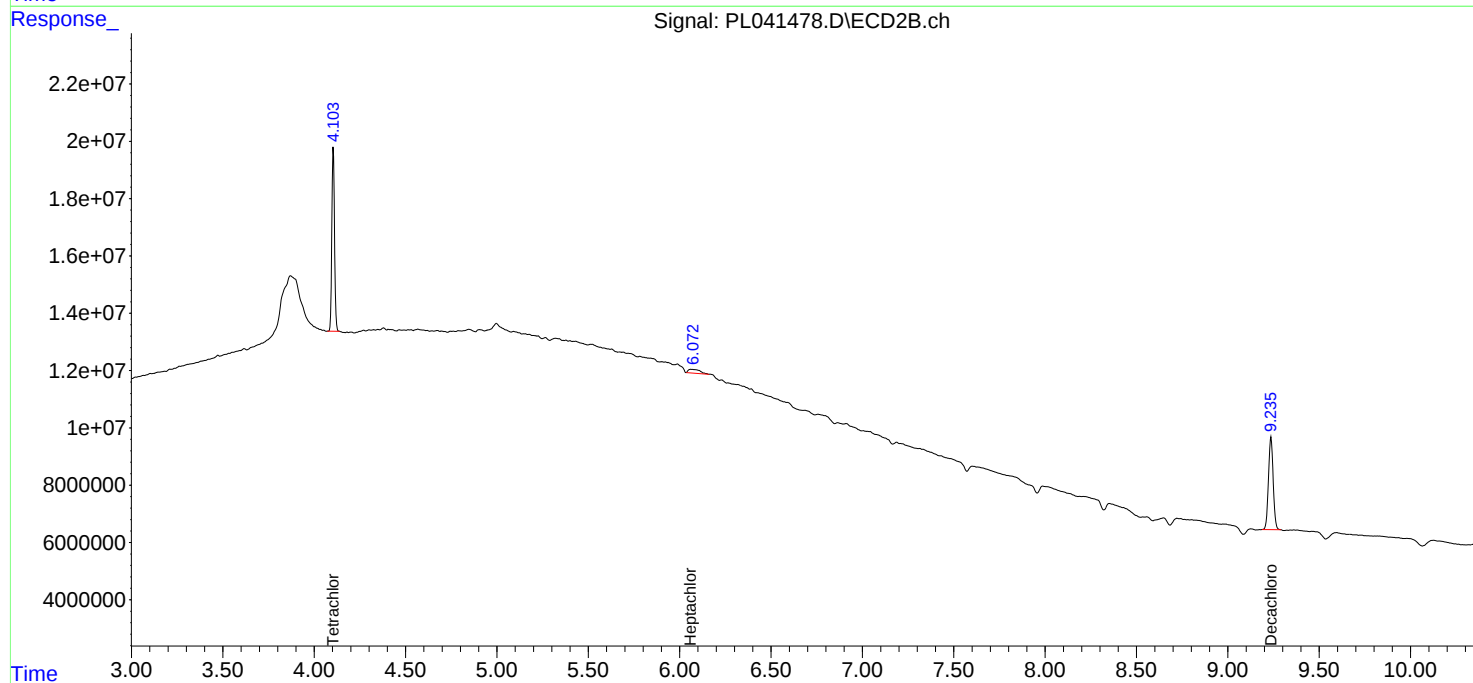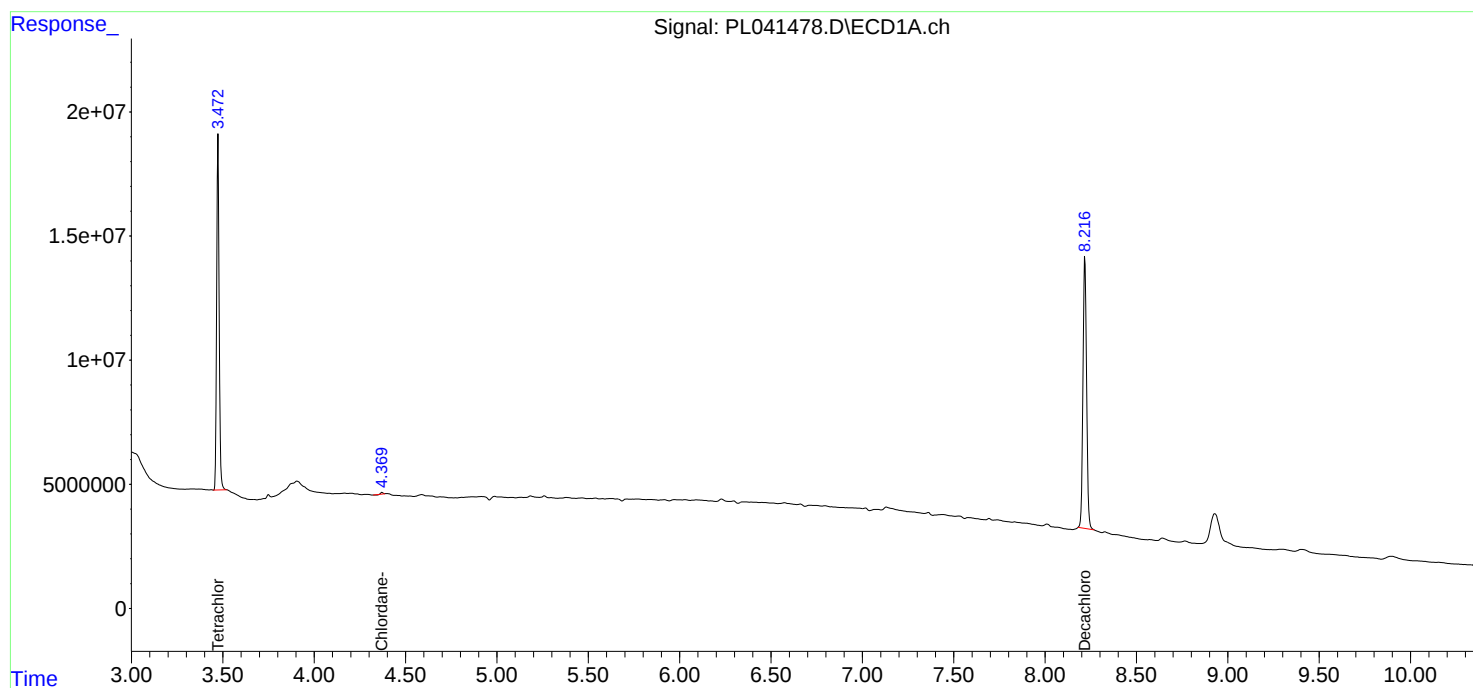


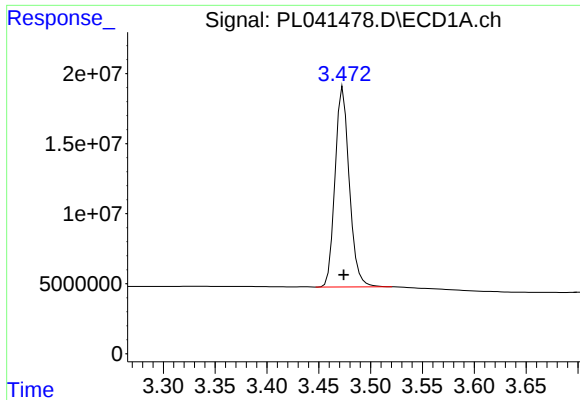

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 136451202
Conc: 21.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

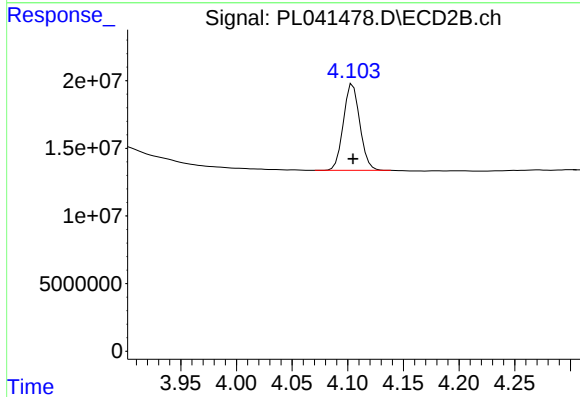


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 65846549
Conc: 21.38 ng/ml

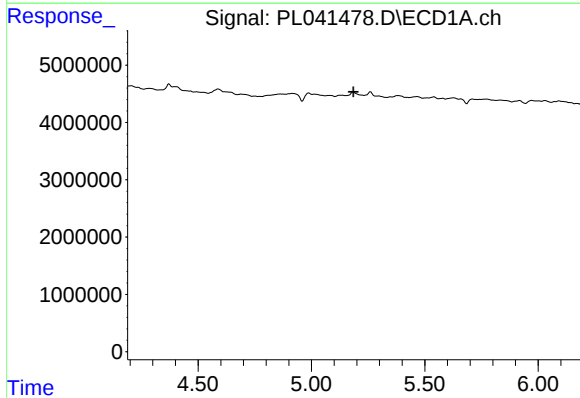


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.186 min
Response: 0
Conc: N.D.

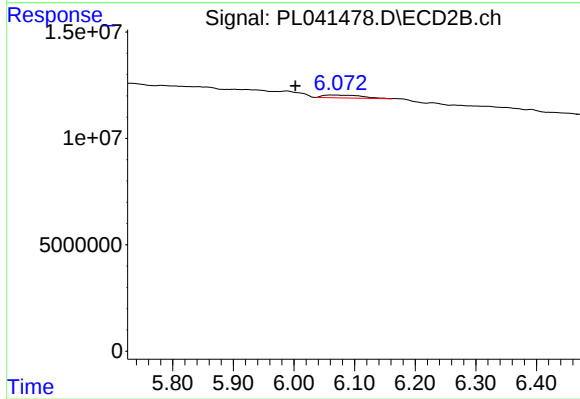

#8 Heptachlor epoxide


R.T.: 6.060 min
Delta R.T.: 0.058 min
Response: 5849841
Conc: 1.66 ng/ml

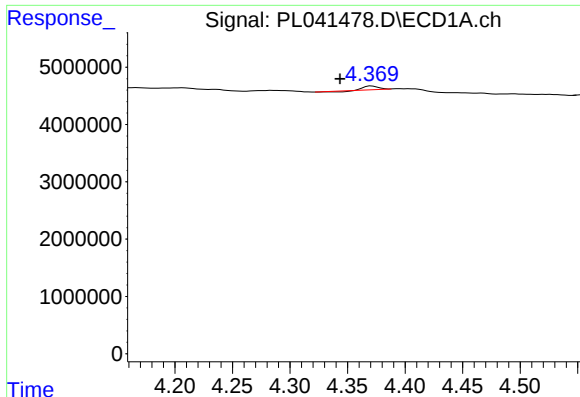

#23 Chlordane-1


R.T.: 4.371 min
Delta R.T.: 0.028 min
Response: 413760
Conc: 1.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

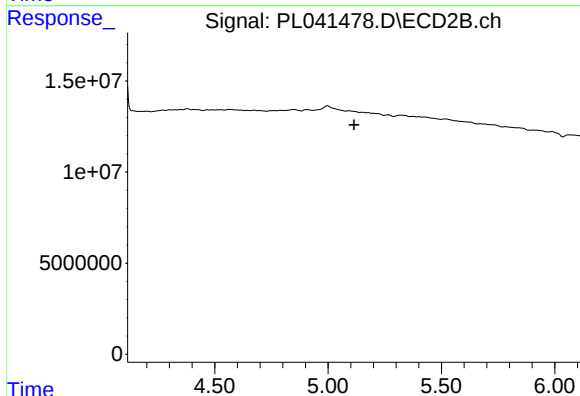


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

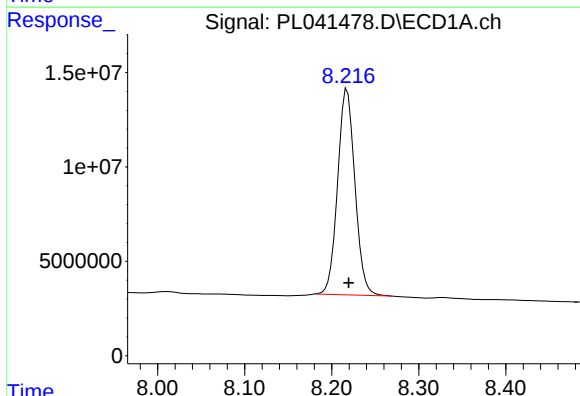

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: -0.002 min
Response: 150818825
Conc: 22.77 ng/ml

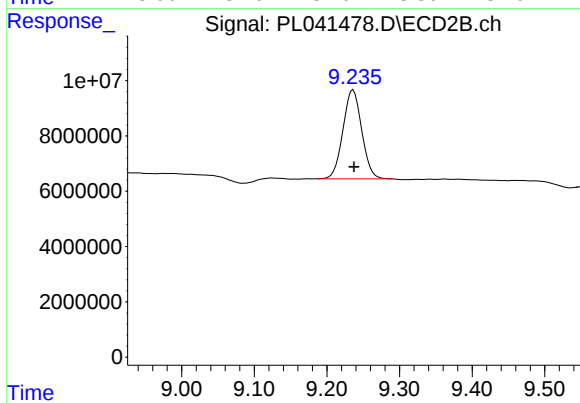

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.001 min
Response: 57851346
Conc: 22.58 ng/ml