

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
 Data File : PL041485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 01:43
 Operator : AJ\SJ
 Sample : J5194-09 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-05-102618-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 02:46:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.103	7839103	3098280	1.231	1.006
28)	SA Decachlor...	8.219	9.234	9105295	3459624	1.375	1.350
Target Compounds							
2)	A alpha-BHC	3.880f	0.000	5883425	0	0.606	N.D. #
3)	MA gamma-BHC...	4.164f	4.793	27322602	2681426	3.058	0.632 #
6)	B beta-BHC	0.000	4.968	0	6436445	N.D.	3.748 #
8)	B Heptachlo...	0.000	6.012	0	58078734	N.D.	16.520 #
10)	B gamma-Chl...	0.000	6.234	0	2352606	N.D.	0.697 #
23)	Chlordane-1	4.399	5.123	4187251	-129445	14.768	N.D. #
25)	Chlordane-3	0.000	6.234	0	2352606	N.D.	5.228 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102918\
Data File : PL041485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 01:43
Operator : AJ\SJ
Sample : J5194-09 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HR-05-102618-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 02:46:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

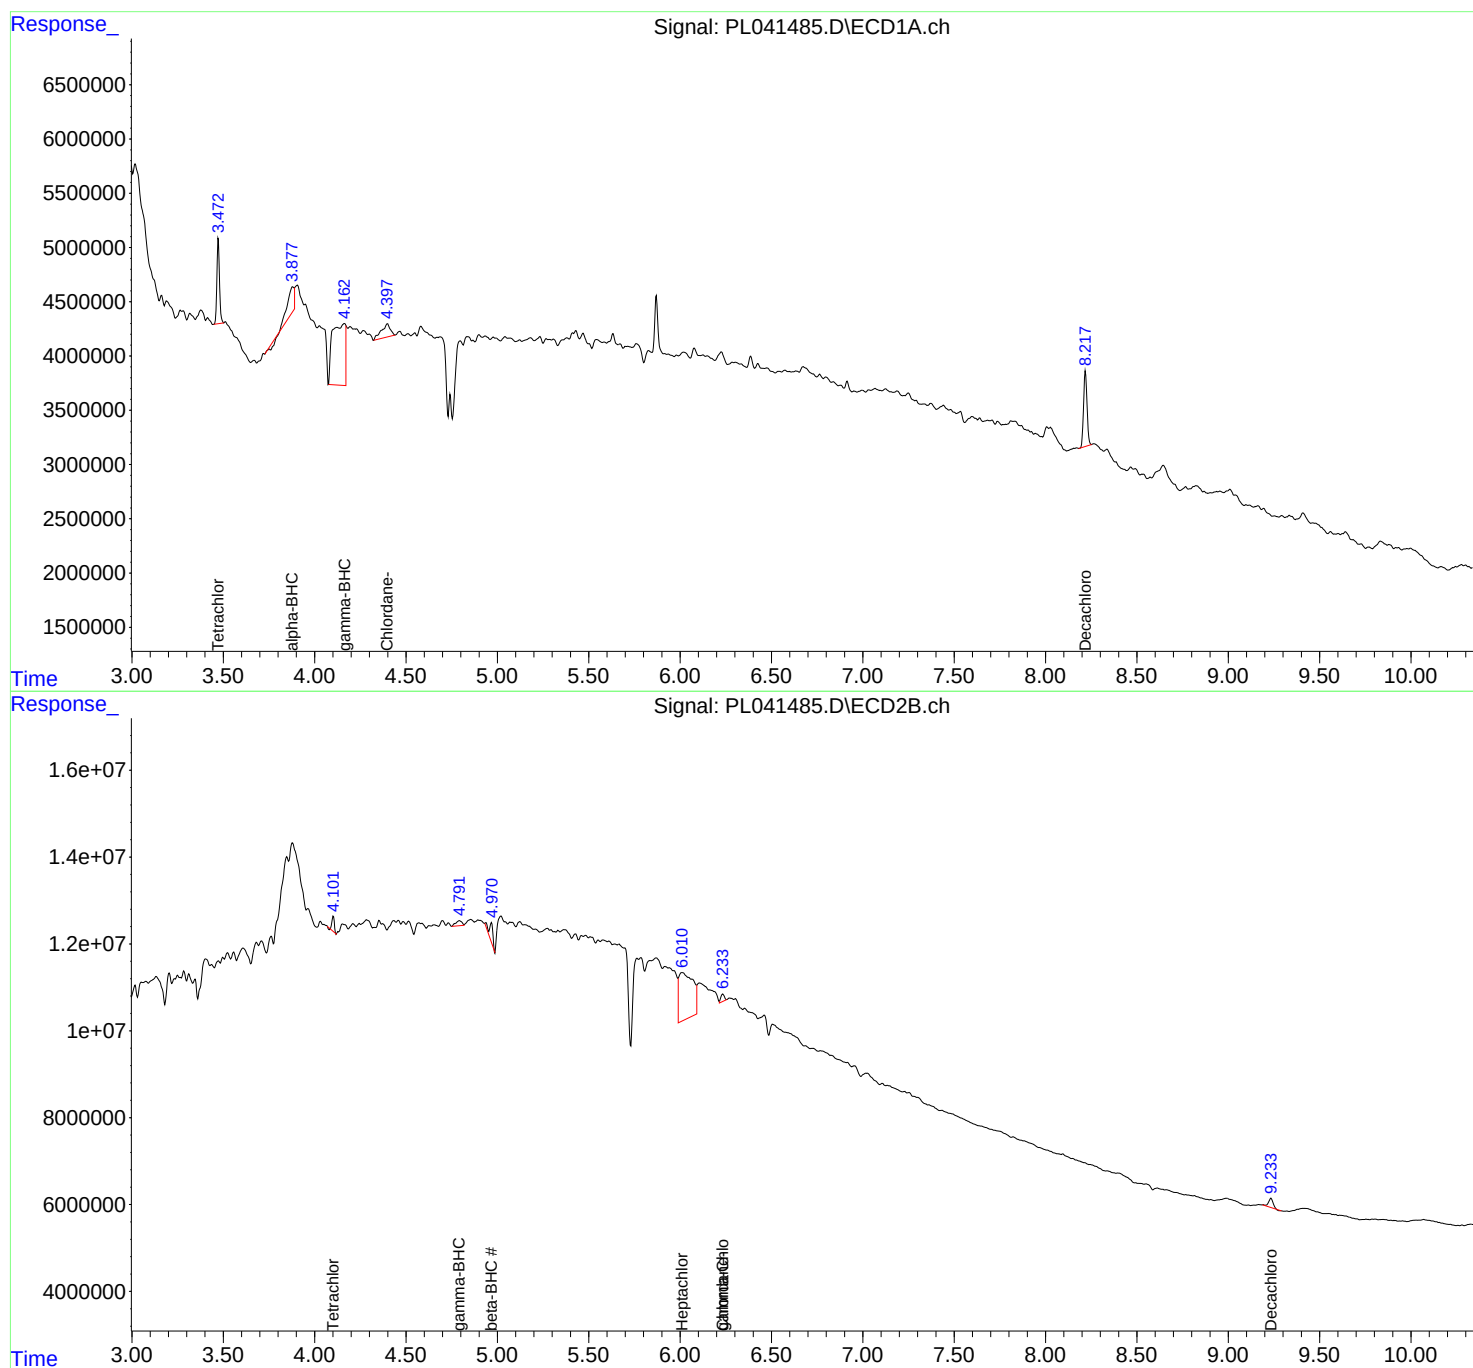


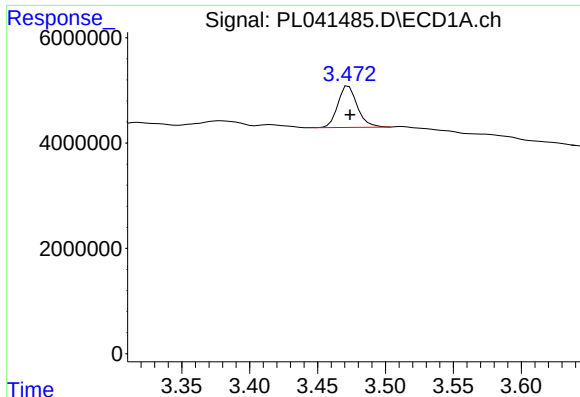

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 7839103
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-05-102618-B

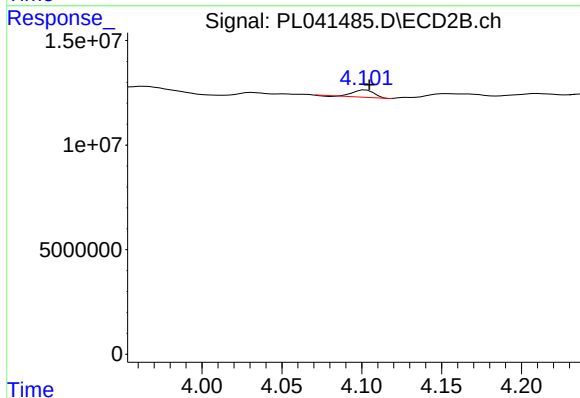


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.002 min
Response: 3098280
Conc: 1.01 ng/ml

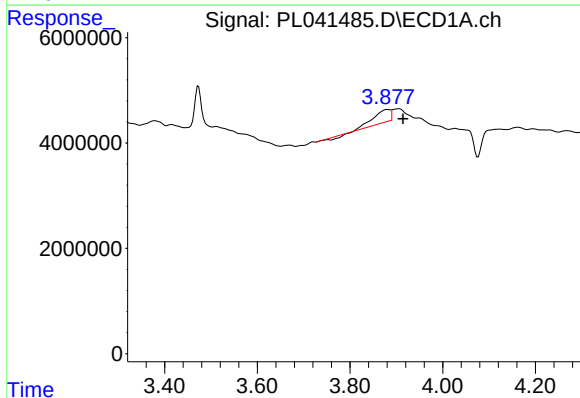


#2 alpha-BHC

R.T.: 3.880 min
Delta R.T.: -0.035 min
Response: 5883425
Conc: 0.61 ng/ml

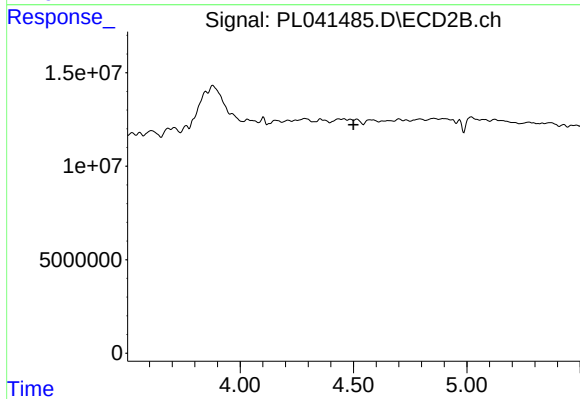

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

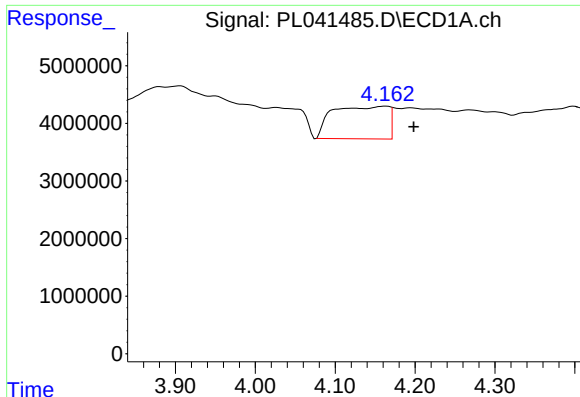

#3 gamma-BHC (Lindane)


R.T.: 4.164 min
Delta R.T.: -0.035 min
Response: 27322602
Conc: 3.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-05-102618-B

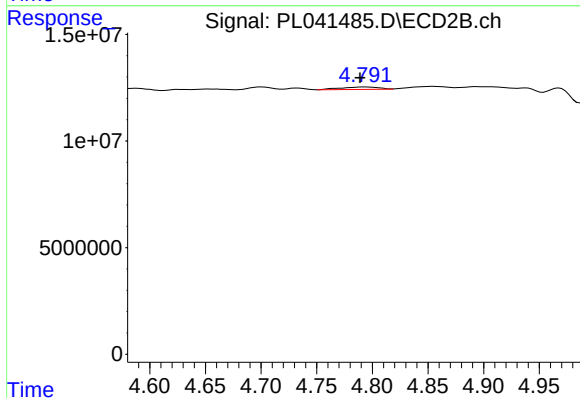


#3 gamma-BHC (Lindane)

R.T.: 4.793 min
Delta R.T.: 0.004 min
Response: 2681426
Conc: 0.63 ng/ml

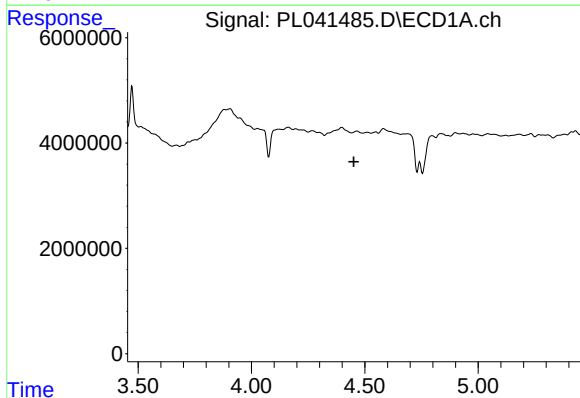


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.451 min
Response: 0
Conc: N.D.

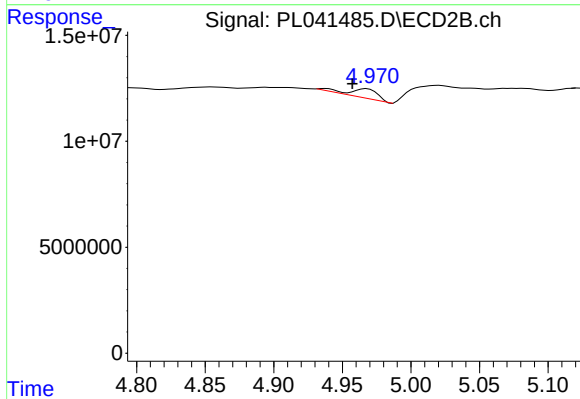

#6 beta-BHC


R.T.: 4.968 min
Delta R.T.: 0.010 min
Response: 6436445
Conc: 3.75 ng/ml

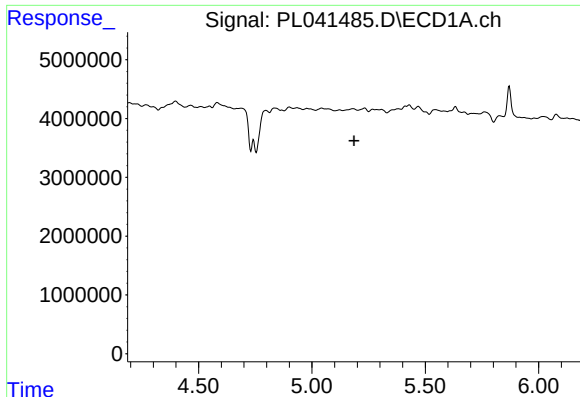

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HR-05-102618-B

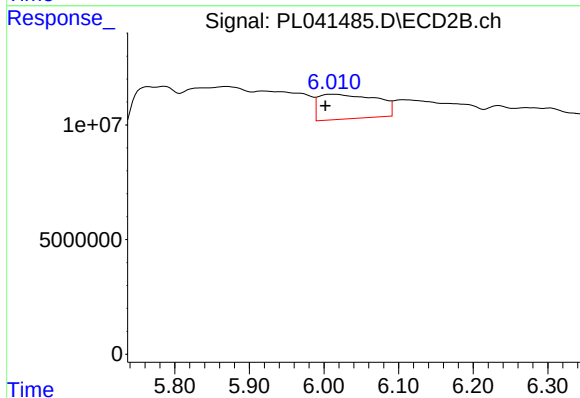


#8 Heptachlor epoxide

R.T.: 6.012 min
Delta R.T.: 0.010 min
Response: 58078734
Conc: 16.52 ng/ml

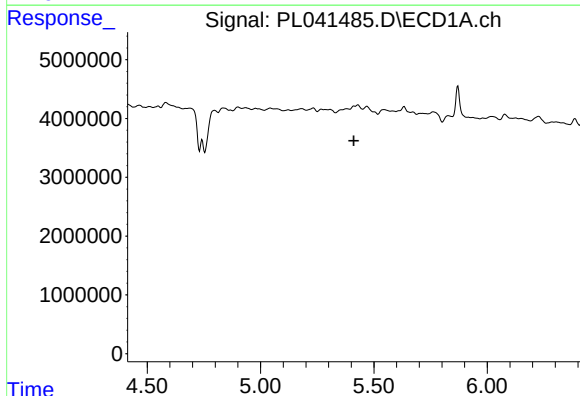


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.412 min
Response: 0
Conc: N.D.

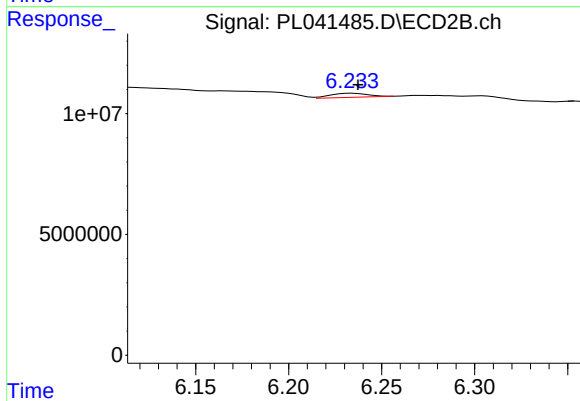

#10 gamma-Chlordane


R.T.: 6.234 min
Delta R.T.: -0.003 min
Response: 2352606
Conc: 0.70 ng/ml

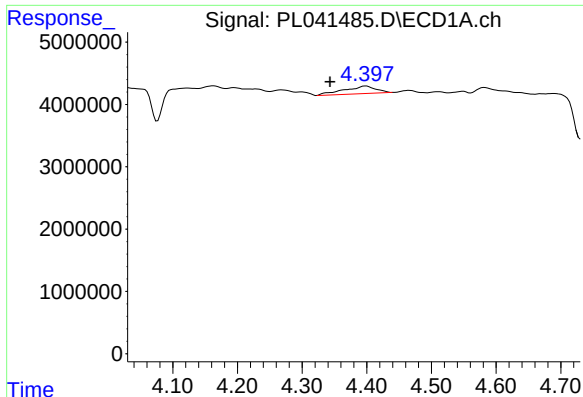

#23 Chlordane-1


R.T.: 4.399 min
Delta R.T.: 0.055 min
Response: 4187251
Conc: 14.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-05-102618-B

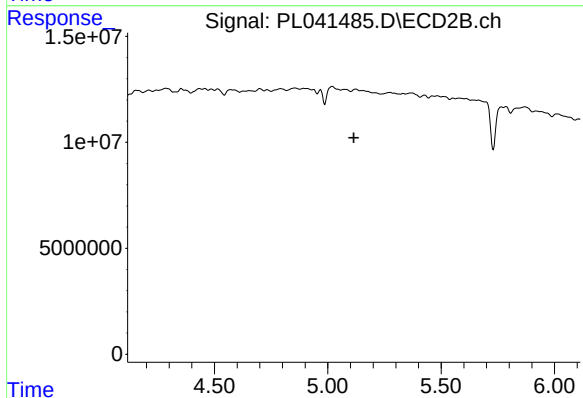


#23 Chlordane-1

R.T.: 5.123 min
Delta R.T.: 0.009 min
Response: -129445
Conc: N.D.

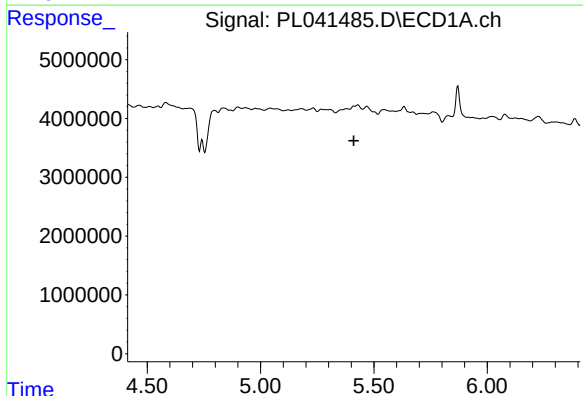


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

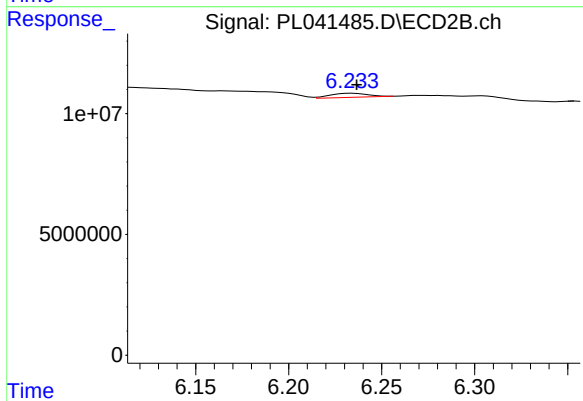

#25 Chlordane-3


R.T.: 6.234 min
Delta R.T.: -0.003 min
Response: 2352606
Conc: 5.23 ng/ml

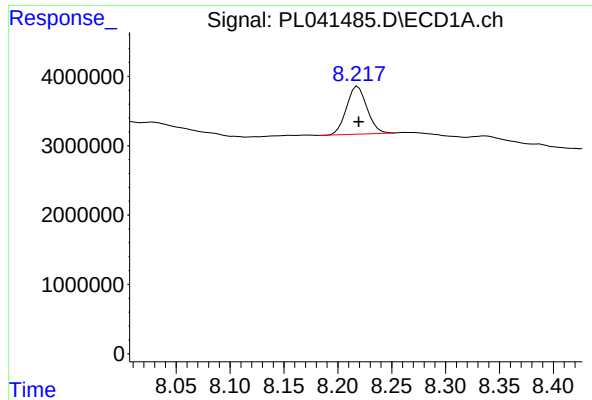

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.000 min
Response: 9105295
Conc: 1.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-05-102618-B

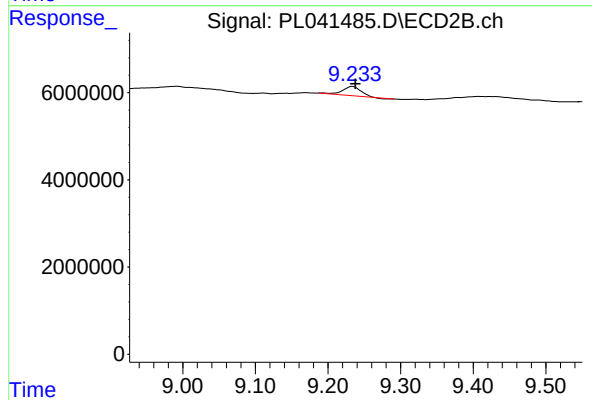

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: -0.004 min
Response: 3459624
Conc: 1.35 ng/ml