

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
 Data File : PL053857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 09:05
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 13:33:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.918	0	12317492	N.D. 4.224 #
9) A	Endosulfan I	5.634	0.000	47041467	0	3.827 N.D. #
10) B	gamma-Chl...	5.534f	0.000	64700207	0	4.742 N.D. #
14) MA	Endrin	6.129	6.746	23158078	3331201	1.998 1.372 #
18) B	Endrin al...	6.538f	0.000	11971058	0	1.306 N.D. #
25)	Chlordane-3	5.534f	0.000	64700207	0	56.130 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
Data File : PL053857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 09:05
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 13:33:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

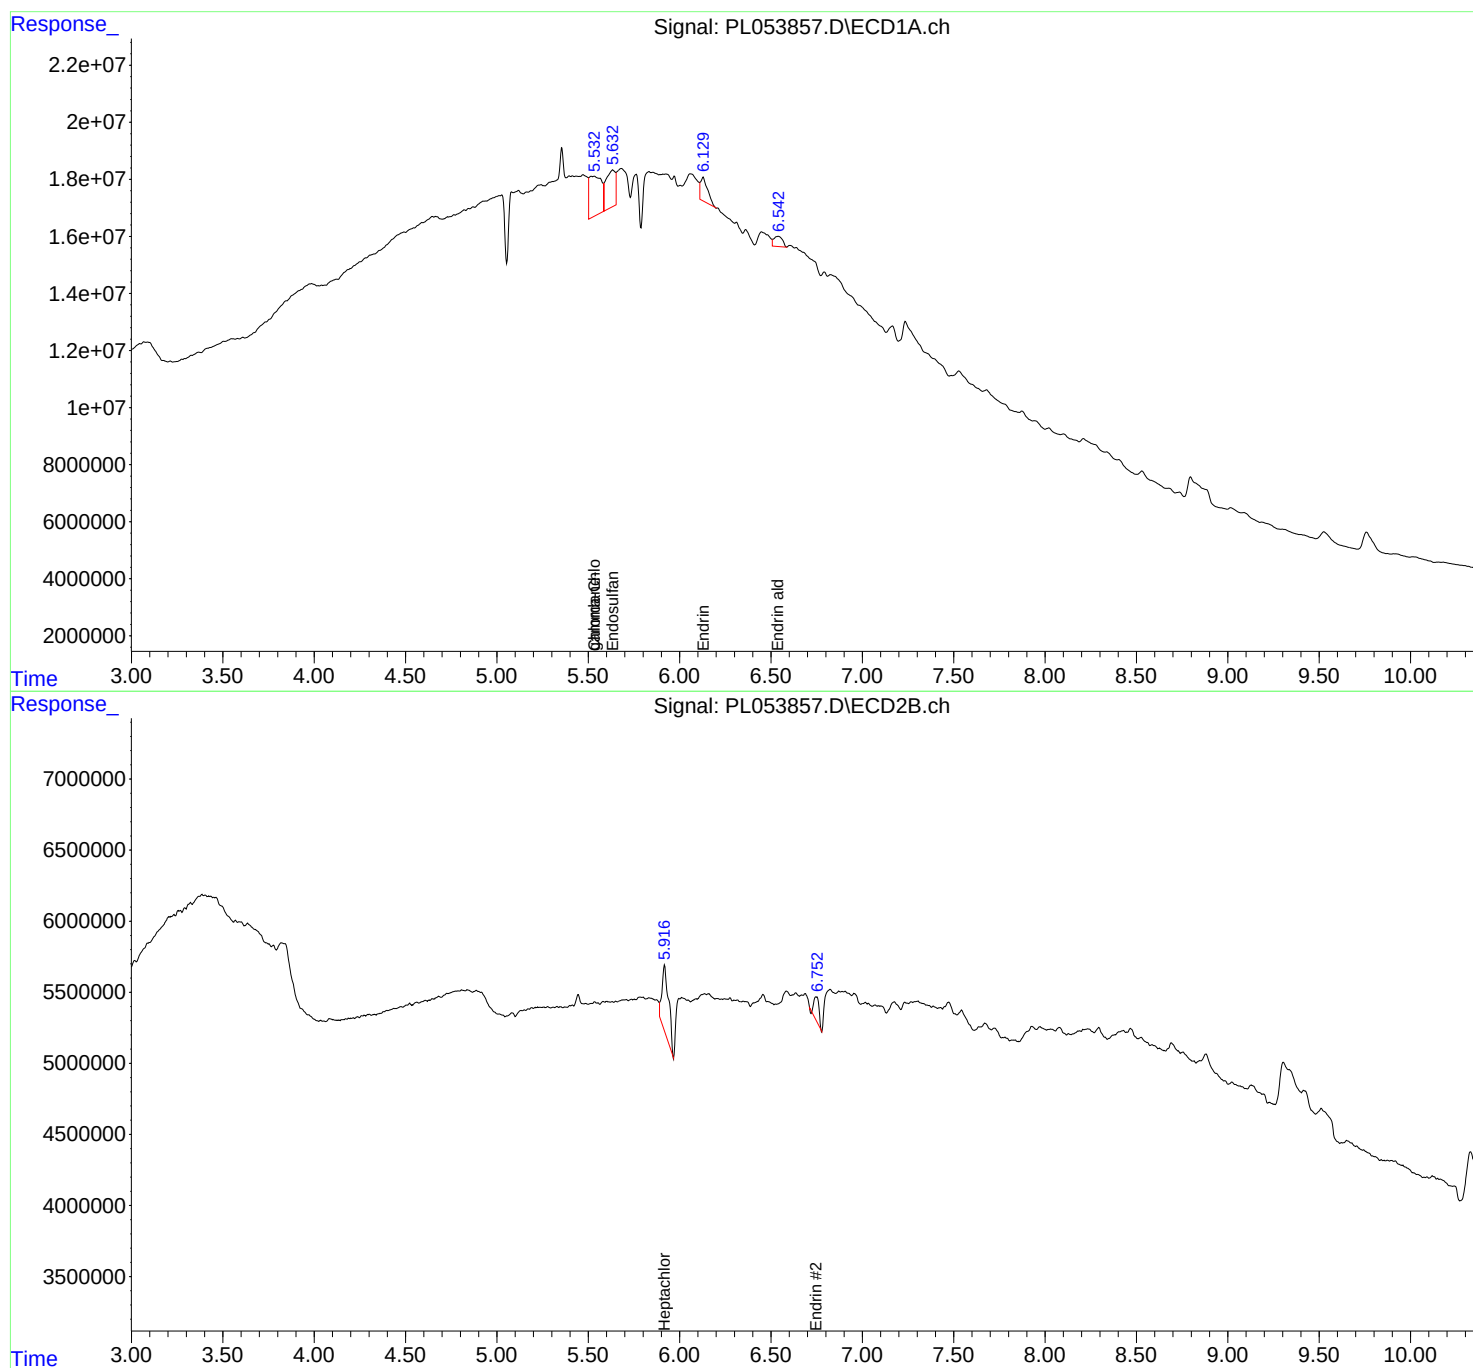


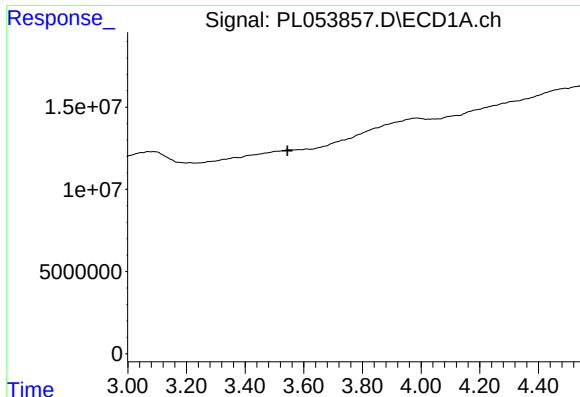

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

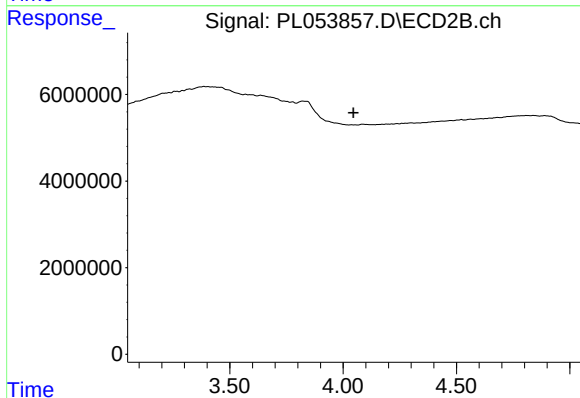


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.046 min
Response: 0
Conc: N.D.

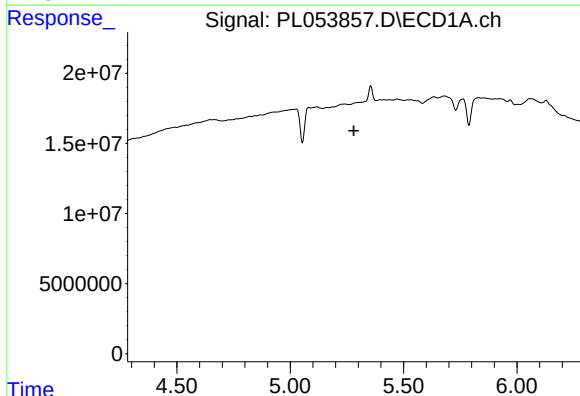


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

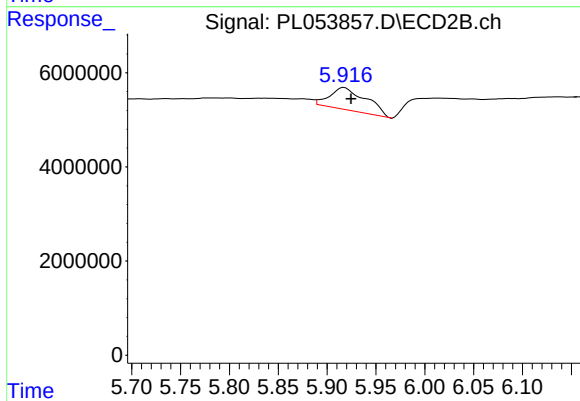

#8 Heptachlor epoxide


R.T.: 5.918 min
Delta R.T.: -0.007 min
Response: 12317492
Conc: 4.22 ng/ml

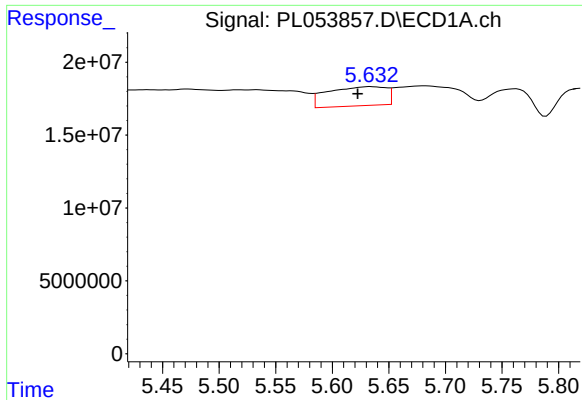

#9 Endosulfan I


R.T.: 5.634 min
Delta R.T.: 0.012 min
Response: 47041467
Conc: 3.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

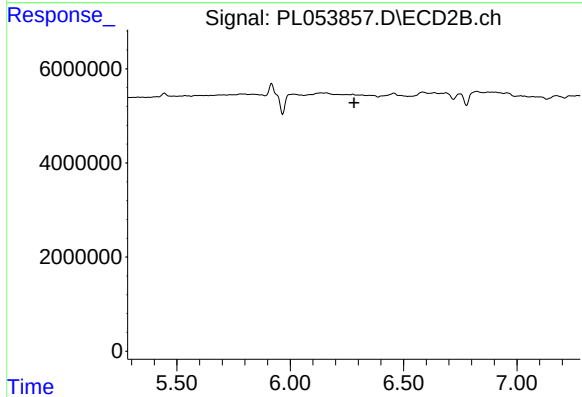


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

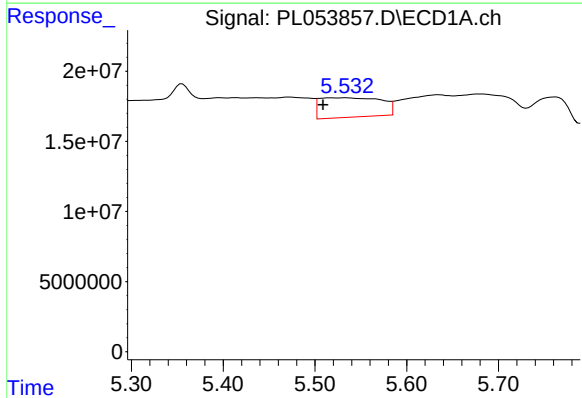


#10 gamma-Chlordane

R.T.: 5.534 min
Delta R.T.: 0.025 min
Response: 64700207
Conc: 4.74 ng/ml

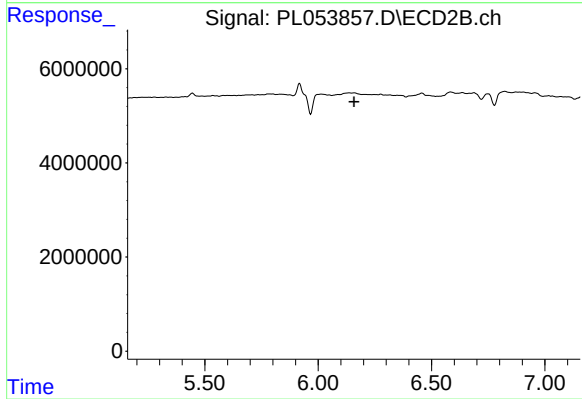

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

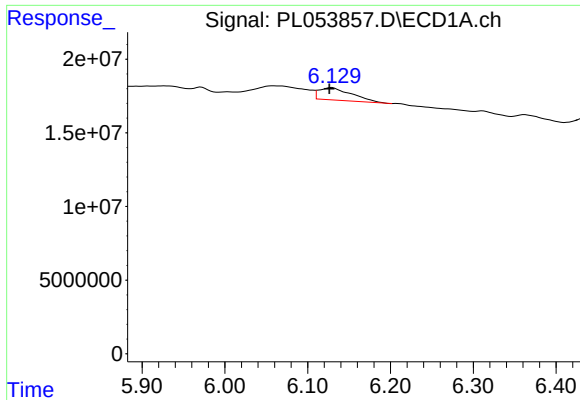

#14 Endrin


R.T.: 6.129 min
Delta R.T.: 0.003 min
Response: 23158078
Conc: 2.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

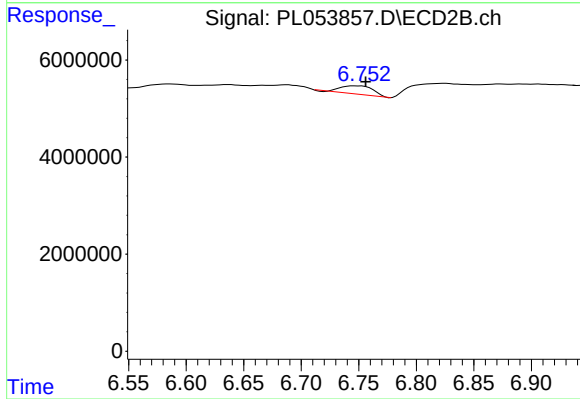


#14 Endrin

R.T.: 6.746 min
Delta R.T.: -0.010 min
Response: 3331201
Conc: 1.37 ng/ml

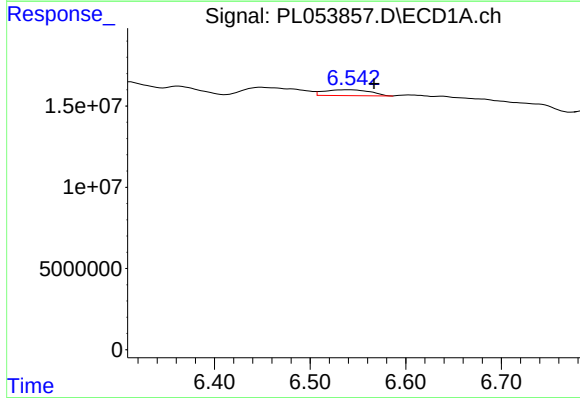


#18 Endrin aldehyde

R.T.: 6.538 min
Delta R.T.: -0.029 min
Response: 11971058
Conc: 1.31 ng/ml

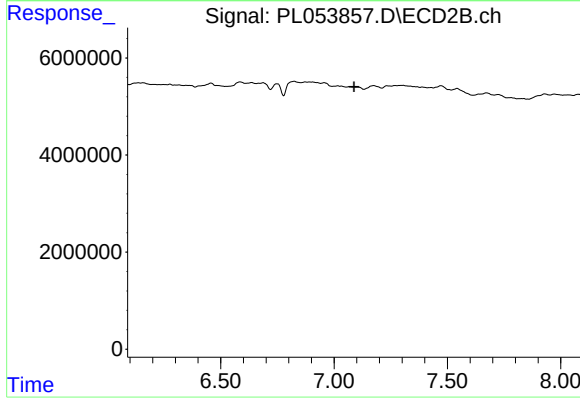

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.089 min
Response: 0
Conc: N.D.

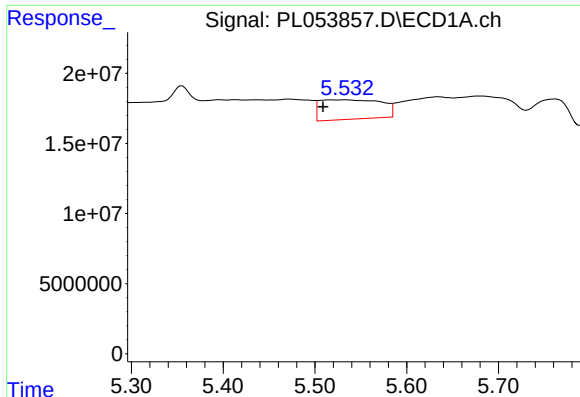

#25 Chlordane-3


R.T.: 5.534 min
Delta R.T.: 0.025 min
Response: 64700207
Conc: 56.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

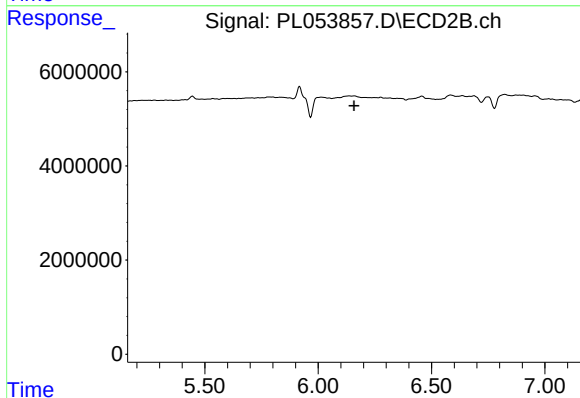


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

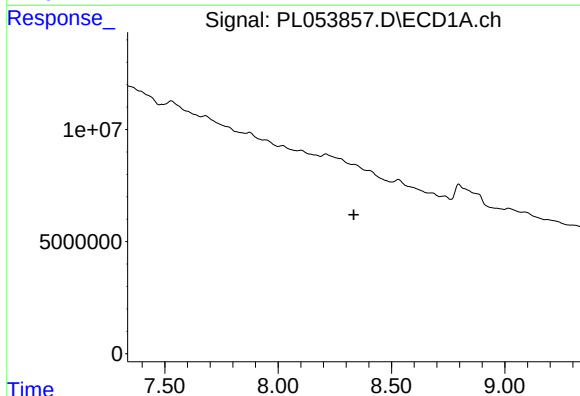

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.334 min
Response: 0
Conc: N.D.

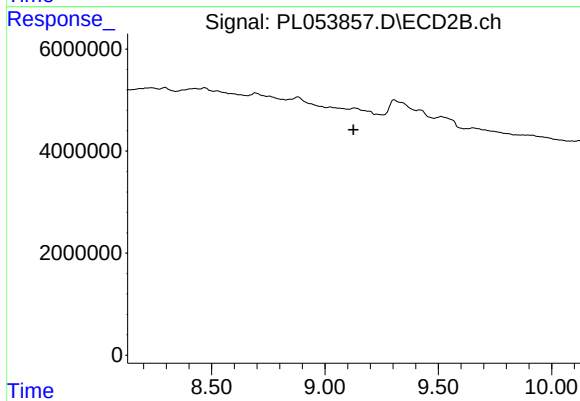

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.