

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
 Data File : PL053885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 18:53
 Operator : SG\AJ
 Sample : K5149-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-01-102819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 07:18:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.045	180.9E6	42682157	16.691	17.057
28)	SA Decachlor...	8.325	9.121	162.1E6	48944882	16.521	17.381
Target Compounds							
7)	B delta-BHC	0.000	5.081f	0	1643153	N.D.	0.544 #
8)	B Heptachlo...	0.000	5.905f	0	794366	N.D.	0.272 #
12)	B 4,4'-DDE	5.741	6.415f	5380391	1939965	0.453	0.689 #
15)	B Endosulfa...	0.000	6.971	0	3120968	N.D.	1.222 #
16)	A 4,4'-DDD	6.245	0.000	3213664	0	0.361	N.D. #
19)	B Endosulfa...	6.776	0.000	6816823	0	0.670	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
Data File : PL053885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 18:53
Operator : SG\AJ
Sample : K5149-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-01-102819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 07:18:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

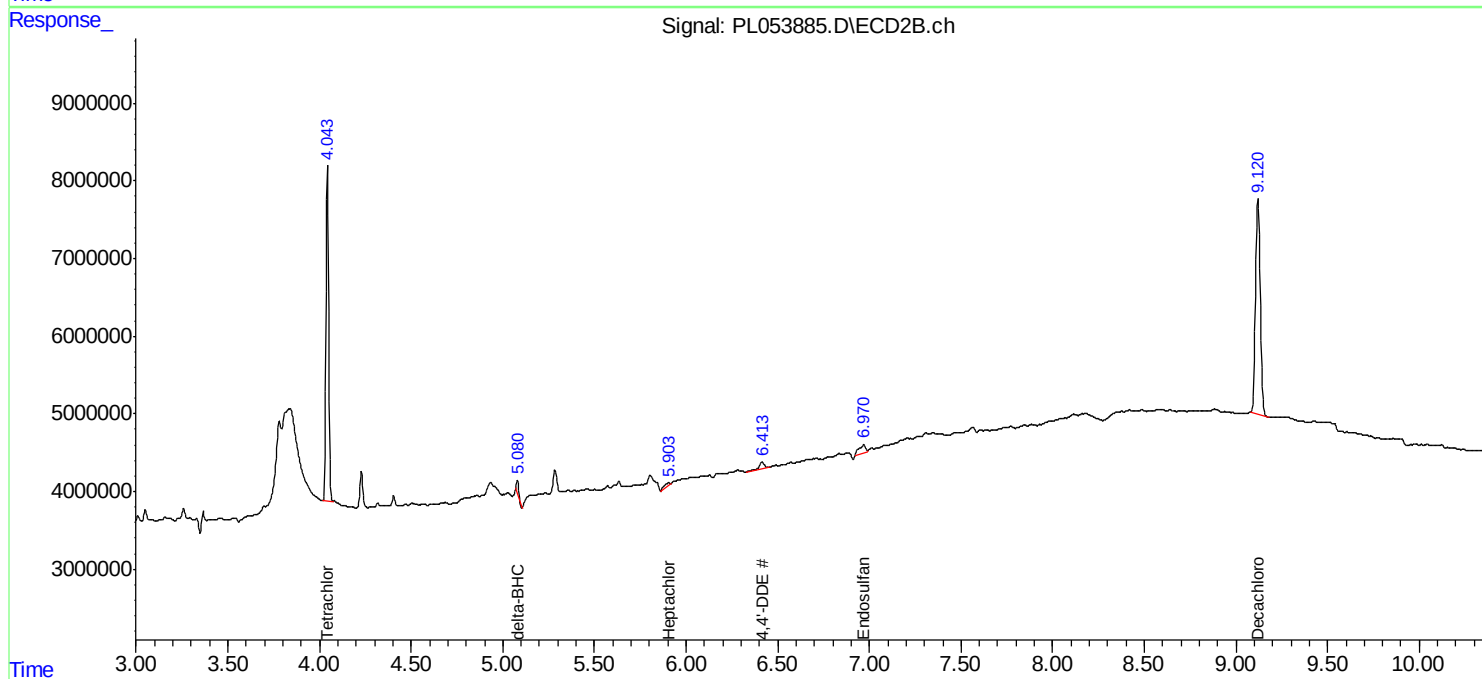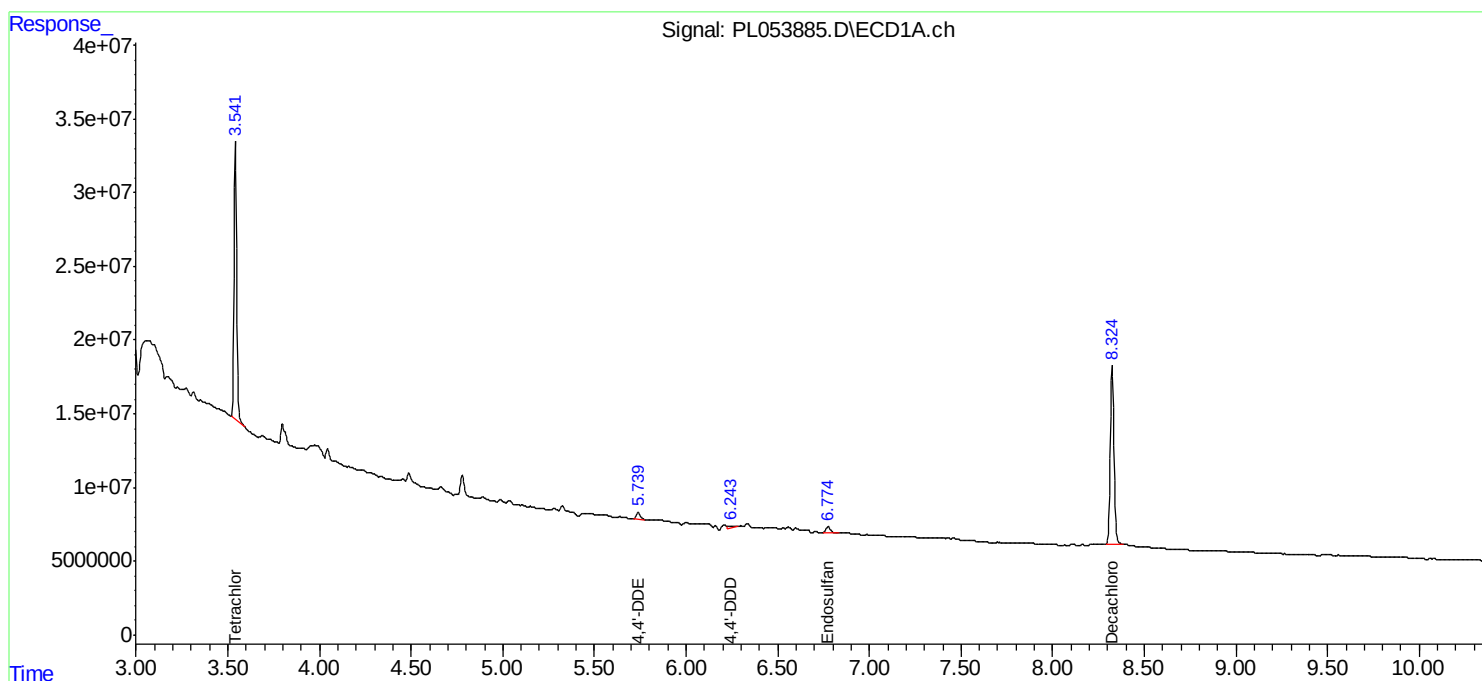


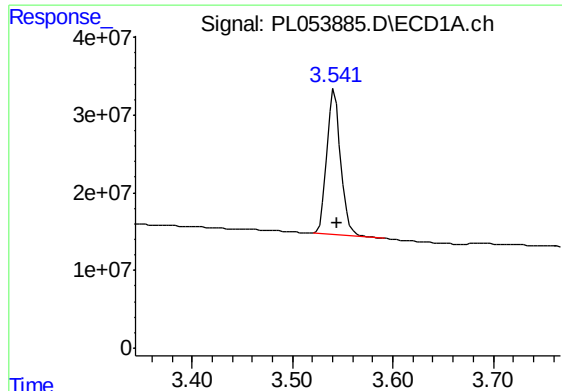

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 180923187
Conc: 16.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-102819

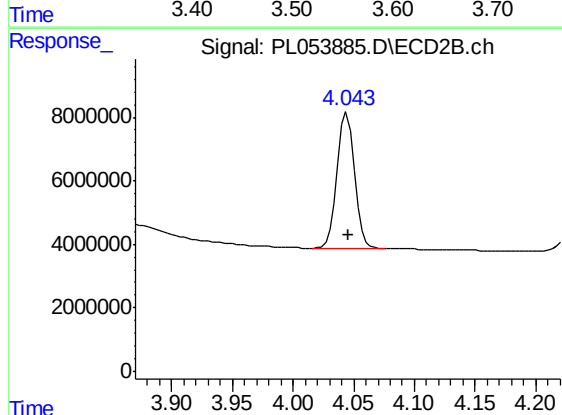


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 42682157
Conc: 17.06 ng/ml

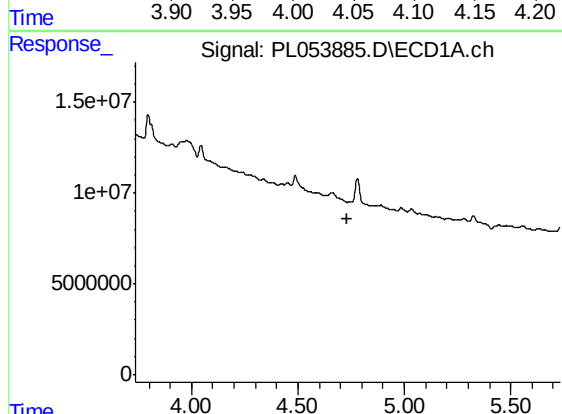


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

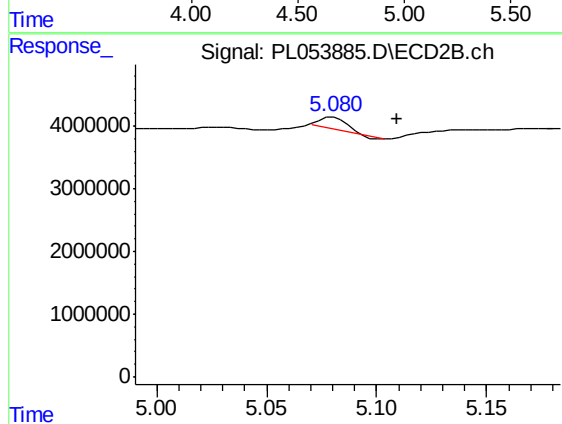

#7 delta-BHC


R.T.: 5.081 min
Delta R.T.: -0.028 min
Response: 1643153
Conc: 0.54 ng/ml

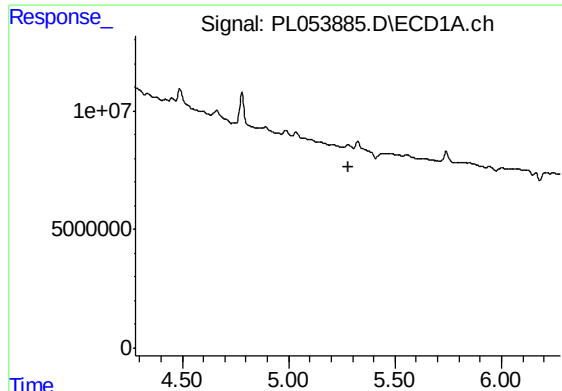

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.280 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-01-102819

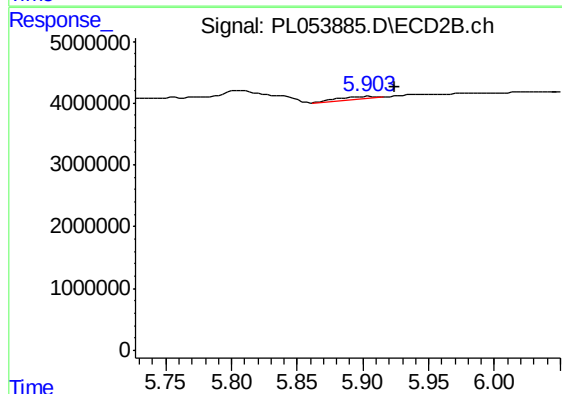


#8 Heptachlor epoxide

R.T.: 5.905 min
Delta R.T.: -0.020 min
Response: 794366
Conc: 0.27 ng/ml

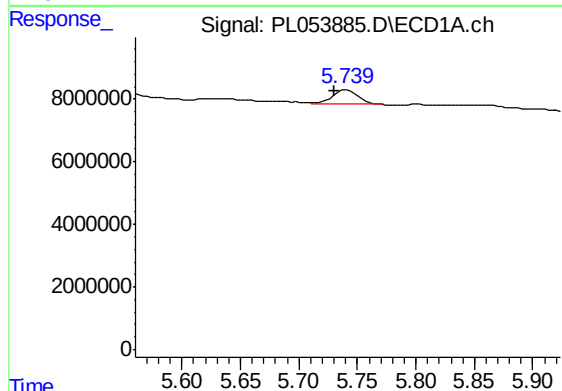


#12 4,4'-DDE

R.T.: 5.741 min
Delta R.T.: 0.010 min
Response: 5380391
Conc: 0.45 ng/ml

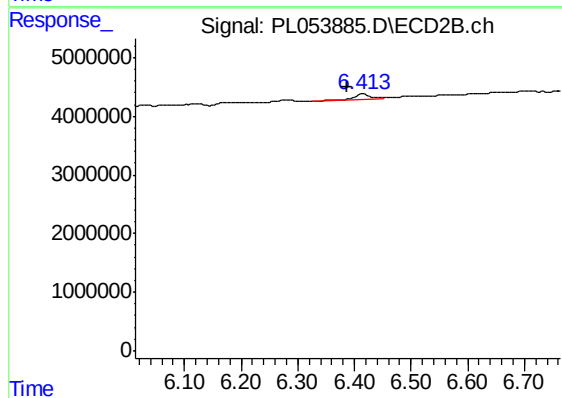

#12 4,4'-DDE


R.T.: 6.415 min
Delta R.T.: 0.028 min
Response: 1939965
Conc: 0.69 ng/ml

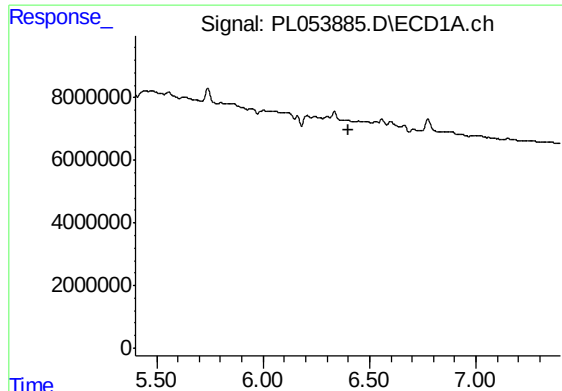

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-01-102819

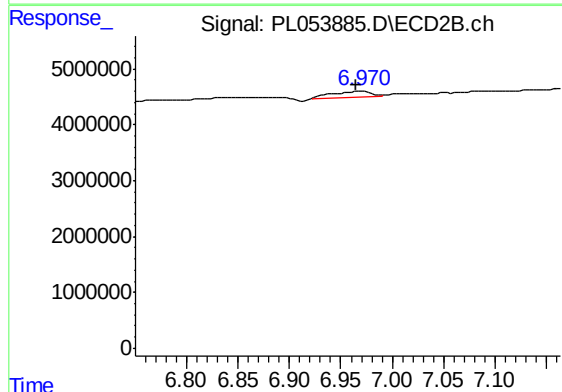


#15 Endosulfan II

R.T.: 6.971 min
Delta R.T.: 0.006 min
Response: 3120968
Conc: 1.22 ng/ml

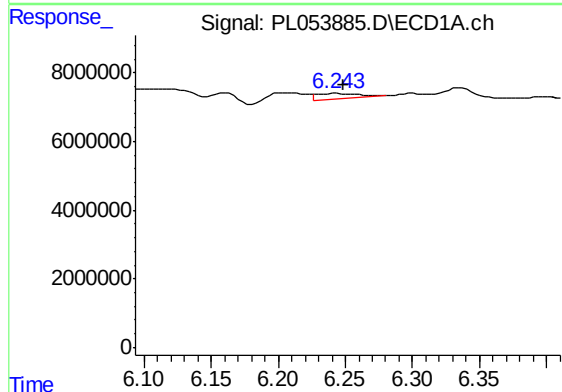


#16 4,4'-DDD

R.T.: 6.245 min
Delta R.T.: -0.004 min
Response: 3213664
Conc: 0.36 ng/ml

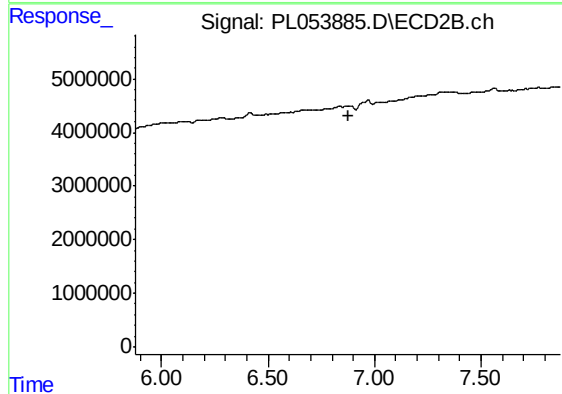

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.877 min
Response: 0
Conc: N.D.

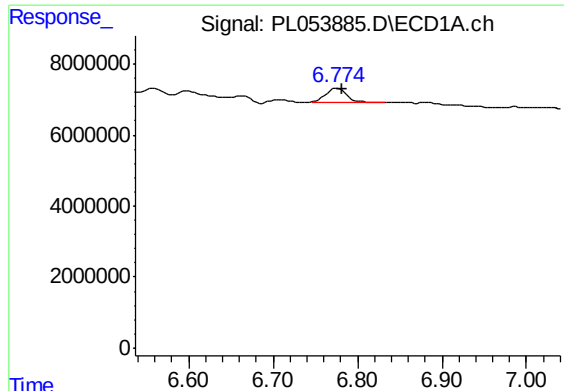

#19 Endosulfan Sulfate


R.T.: 6.776 min
Delta R.T.: -0.006 min
Response: 6816823
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-102819

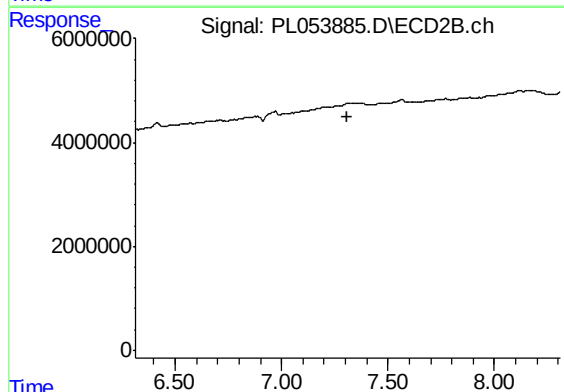


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

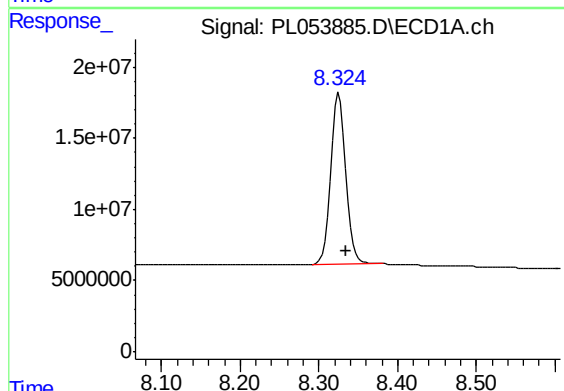

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 162095414
Conc: 16.52 ng/ml

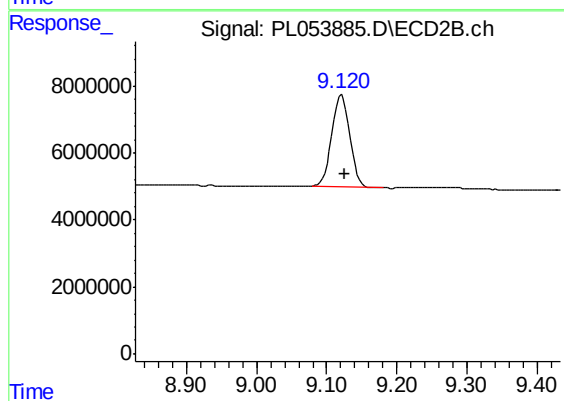

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 48944882
Conc: 17.38 ng/ml