

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
 Data File : PL053870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 14:54
 Operator : SG\AJ
 Sample : K5582-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NCQ-632

Manual Integrations
 APPROVED

Ankita
 10/30/2019 11:37:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 07:14:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.043	361.0E6	42193293	33.308m	16.861m#
28)	SA Decachlor...	8.324	9.120	152.0E6	45489443	15.488	16.154
Target Compounds							
4)	MA Heptachlor	4.582	5.229	225.3E6	102.9E6	14.274	31.945 #
15)	B Endosulfa...	6.401	6.973	2378.0E6	439.7E6	212.694	172.121m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
Data File : PL053870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 14:54
Operator : SG\AJ
Sample : K5582-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NCQ-632


Manual Integrations
APPROVED

Ankita
10/30/2019 11:37:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 07:14:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

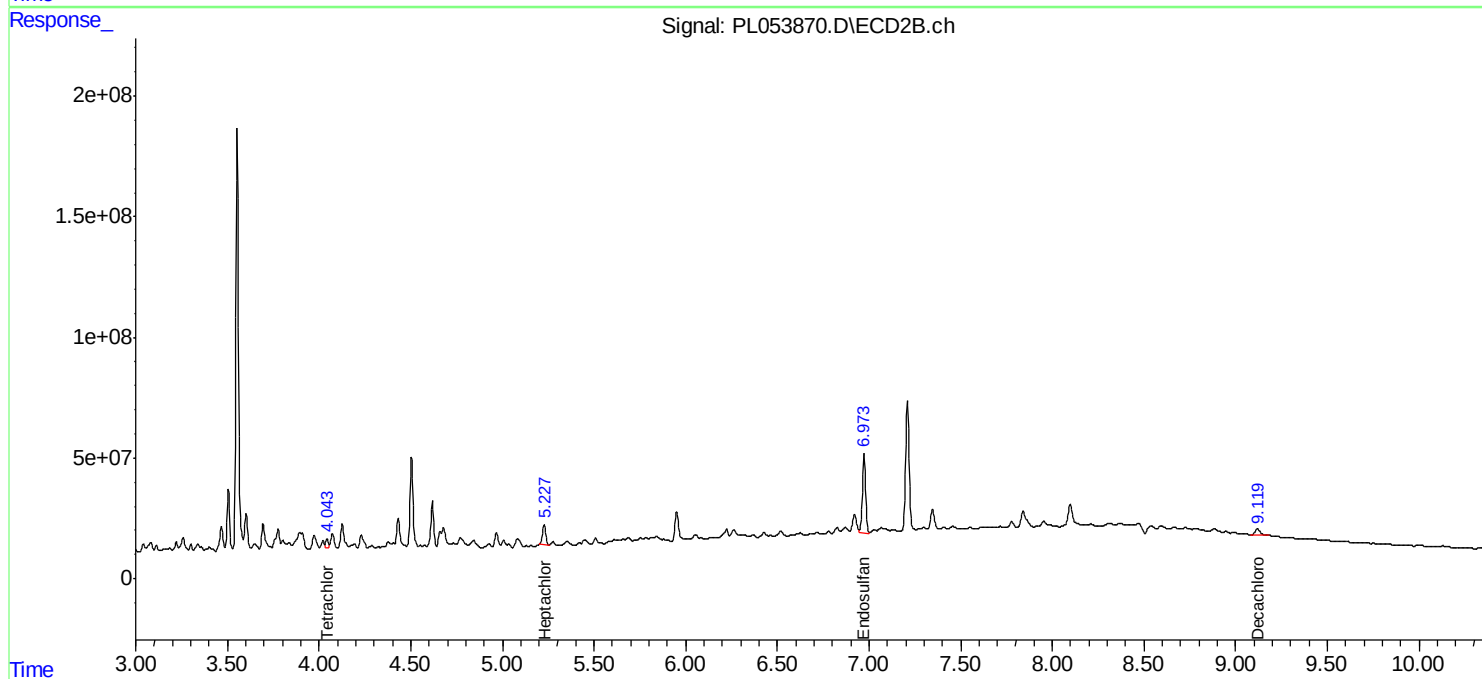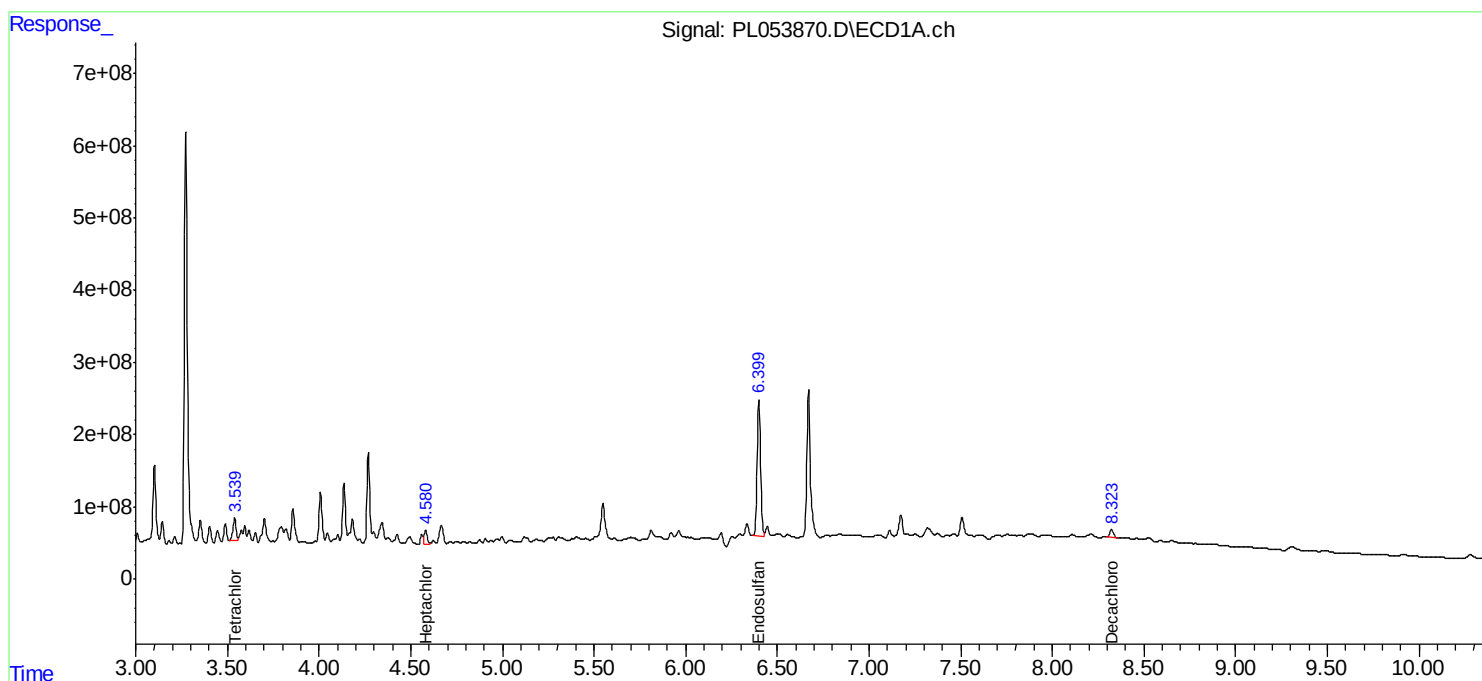

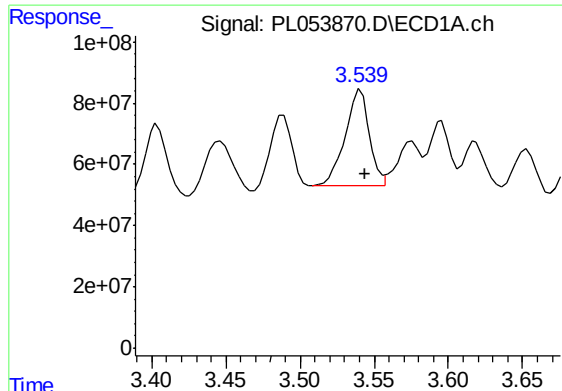


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.005 min
Response: 361039610
Conc: 33.31 ng/ml m

Instrument :
ECD_L
ClientSampleId :
NCQ-632


Manual Integrations
APPROVED

Ankita
10/30/2019 11:37:59 AM

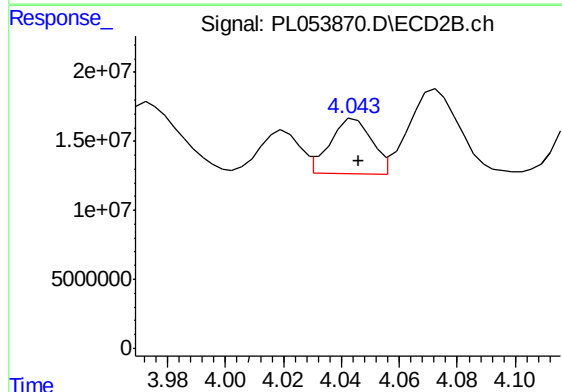


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 42193293
Conc: 16.86 ng/ml m

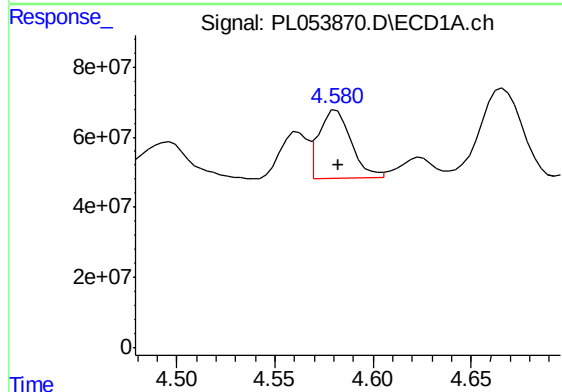


#4 Heptachlor

R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 225286296
Conc: 14.27 ng/ml

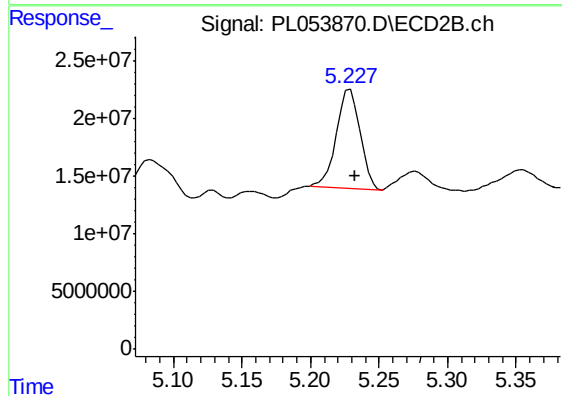

#4 Heptachlor

R.T.: 5.229 min
Delta R.T.: -0.003 min
Response: 102930964
Conc: 31.94 ng/ml

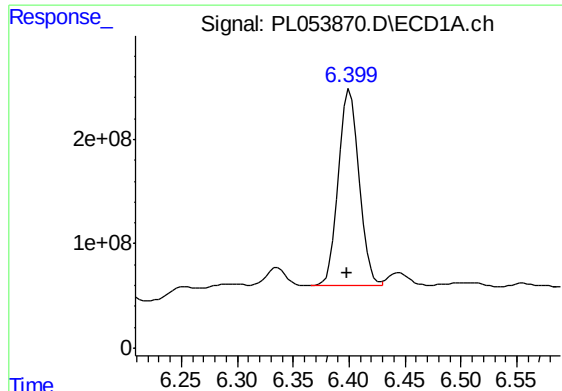


#15 Endosulfan II

R.T.: 6.401 min
Delta R.T.: 0.002 min
Response: 2377995659
Conc: 212.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
NCQ-632


Manual Integrations
APPROVED

Ankita
10/30/2019 11:37:59 AM

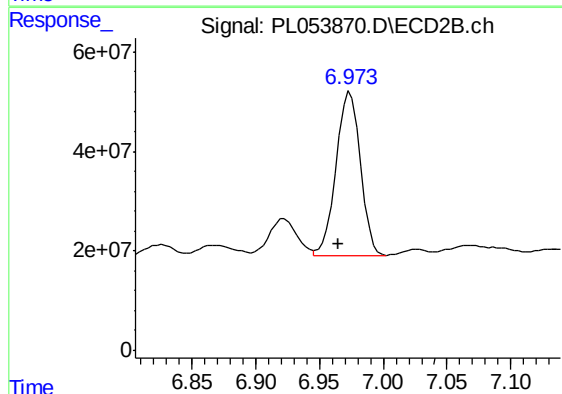


#15 Endosulfan II

R.T.: 6.973 min
Delta R.T.: 0.008 min
Response: 439681167
Conc: 172.12 ng/ml m

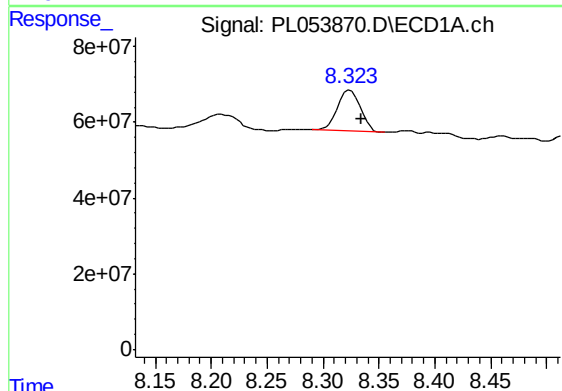

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 151956656
Conc: 15.49 ng/ml

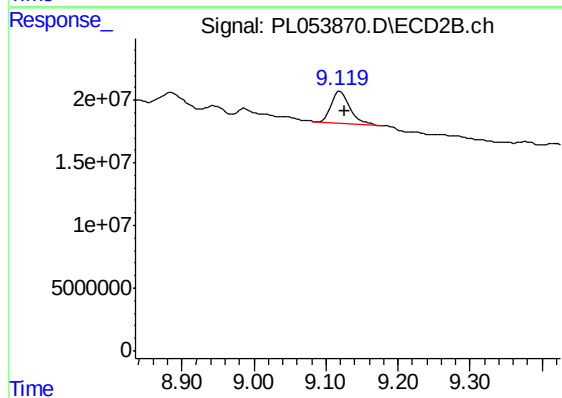

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: -0.006 min
Response: 45489443
Conc: 16.15 ng/ml