

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
 Data File : PL053878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 16:47
 Operator : SG\AJ
 Sample : K5569-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 IDW-DECON-WATER-102519

Manual Integrations
 APPROVED

Ankita
 10/30/2019 2:33:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 07:16:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.044	22482498	7657066	2.074	3.060 #
28)	SA Decachlor...	8.324	0.000	1454364	0	0.148m	N.D. d#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102919\
Data File : PL053878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 16:47
Operator : SG\AJ
Sample : K5569-02
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
IDW-DECON-WATER-102519


Manual Integrations
APPROVED

Ankita
10/30/2019 2:33:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 07:16:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

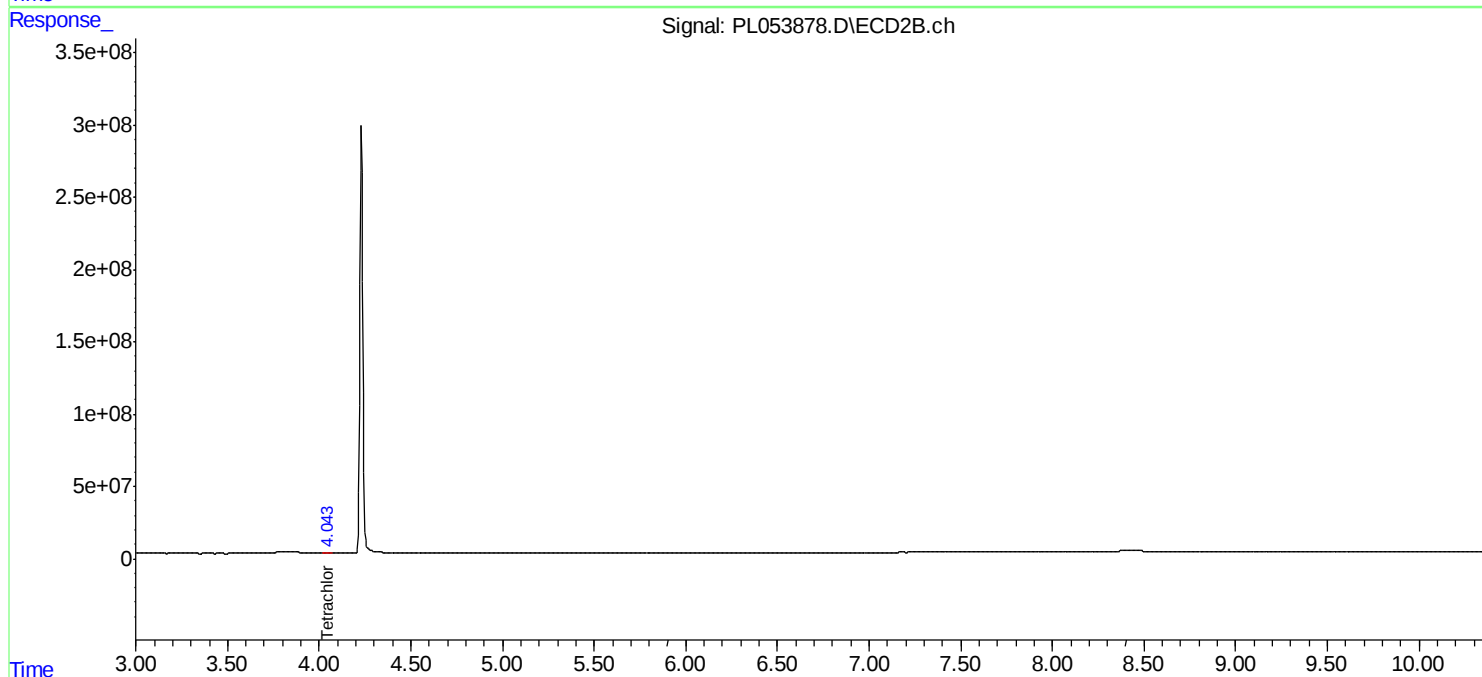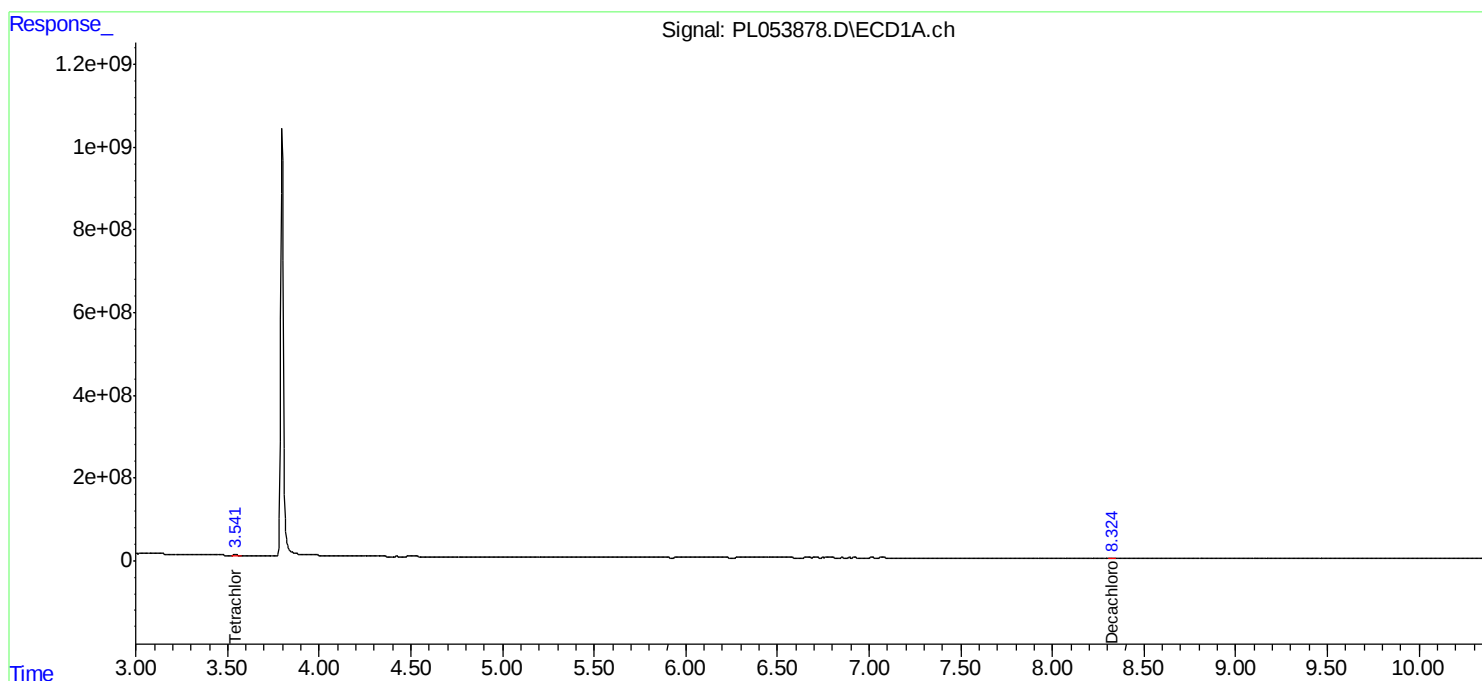

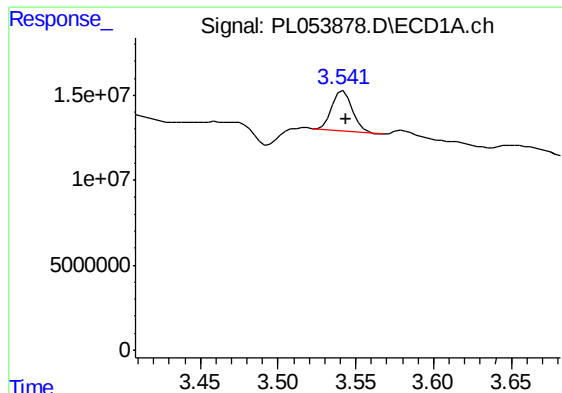


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 22482498
Conc: 2.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
IDW-DECON-WATER-102519


Manual Integrations
APPROVED

Ankita
10/30/2019 2:33:12 PM

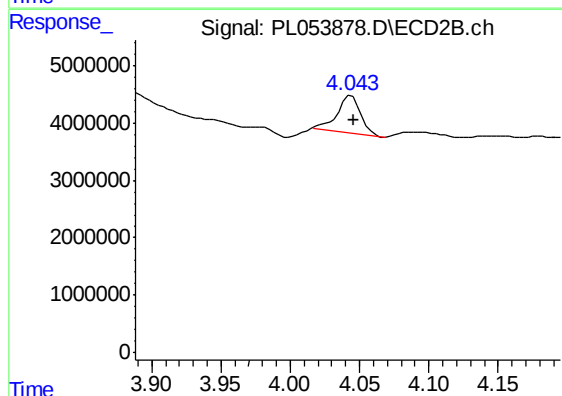


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 7657066
Conc: 3.06 ng/ml

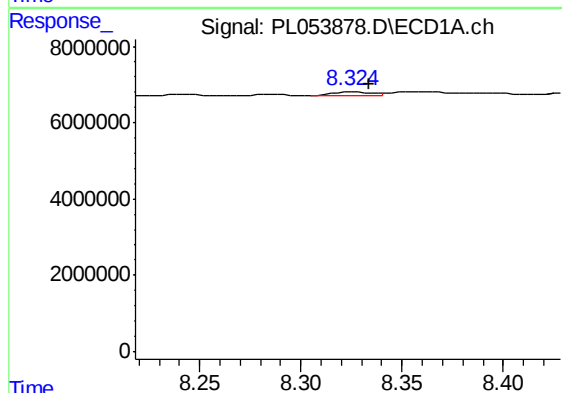

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 1454364
Conc: 0.15 ng/ml m

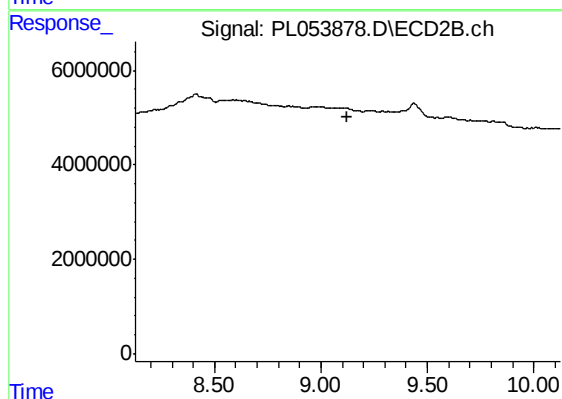

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.