

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102920\
 Data File : PL062691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2020 16:04
 Operator : DD\AJ
 Sample : L4217-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-01-102820

Manual Integrations
 APPROVED

Ankita
 10/30/2020 3:54:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:18:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	20112129	34428026	11.693	11.715
28)	SA Decachlor...	8.130	8.994	18709511	27196897	11.662	12.994
Target Compounds							
12)	B 4,4'-DDE	5.553	6.278	1514333	3606975	0.915	1.119
17)	MA 4,4'-DDT	6.300	7.067	1507154	1771917	1.129m	0.789m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102920\
Data File : PL062691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2020 16:04
Operator : DD\AJ
Sample : L4217-07
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
HR-01-102820


Manual Integrations
APPROVED

Ankita
10/30/2020 3:54:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:18:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

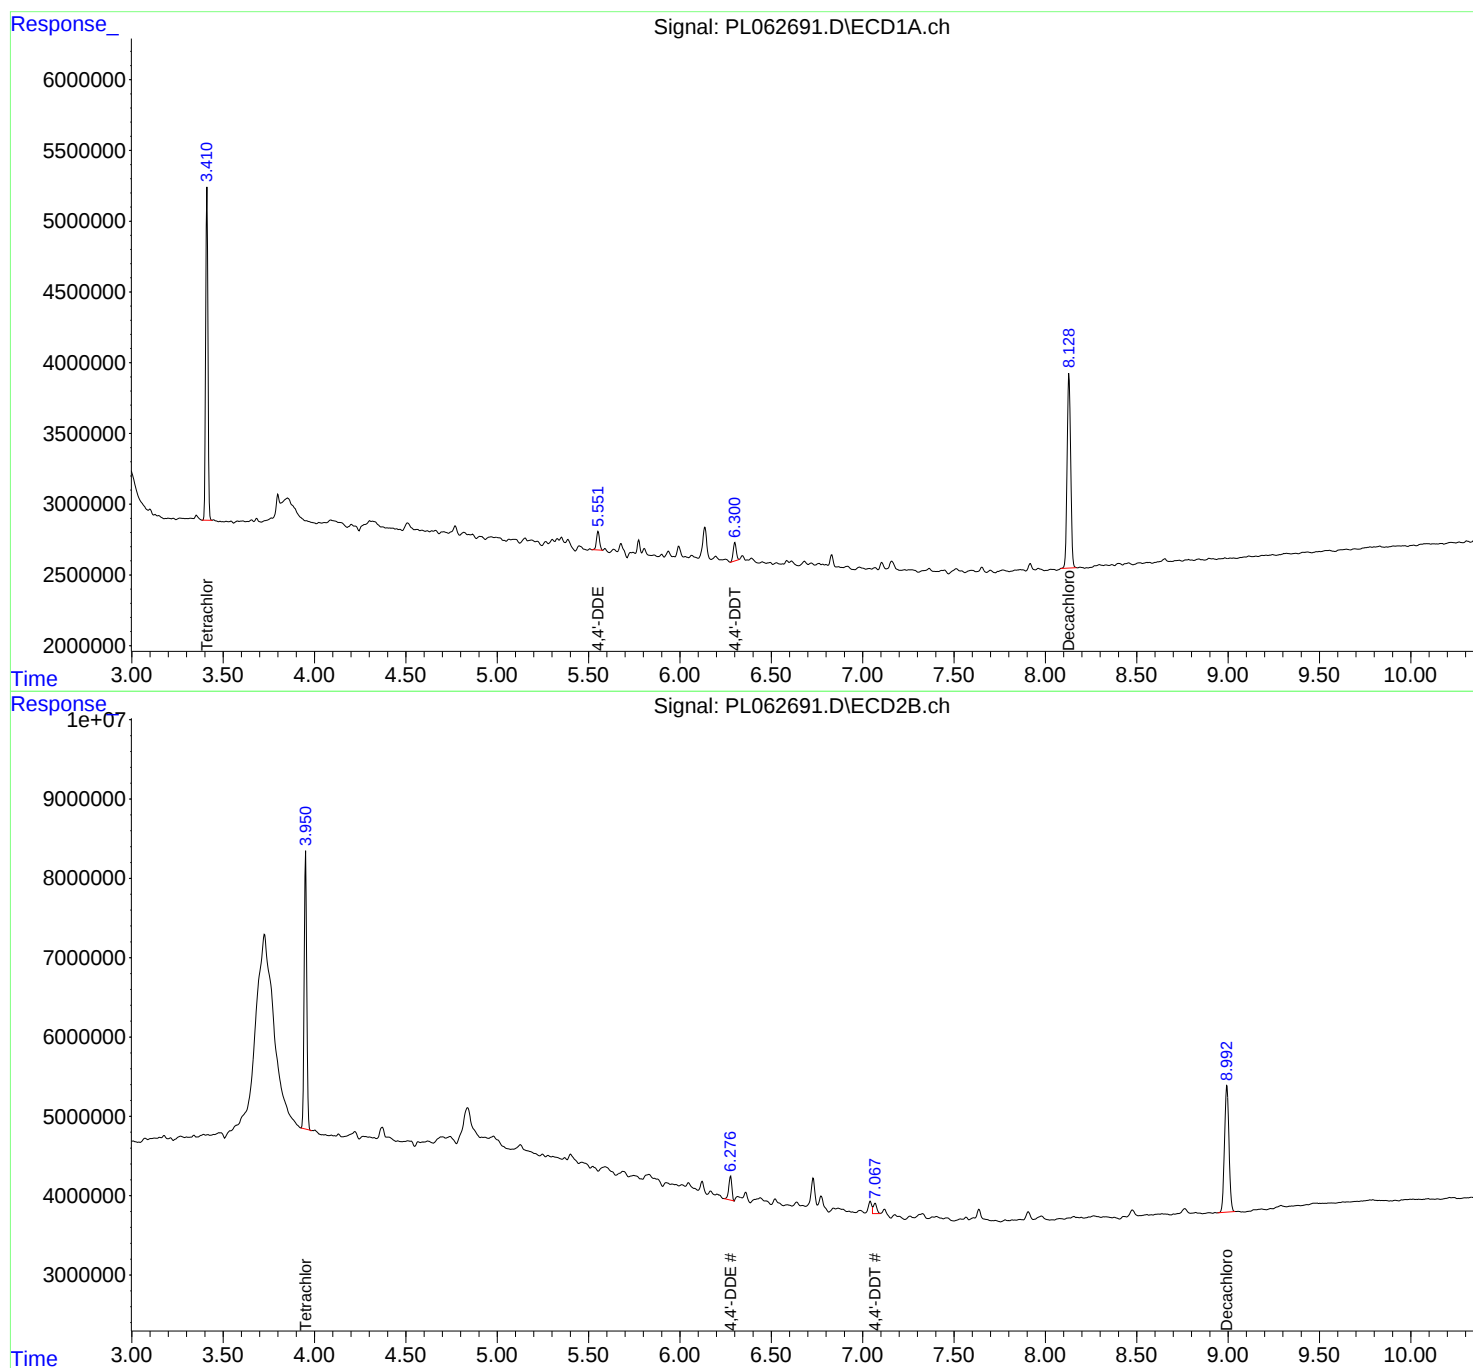

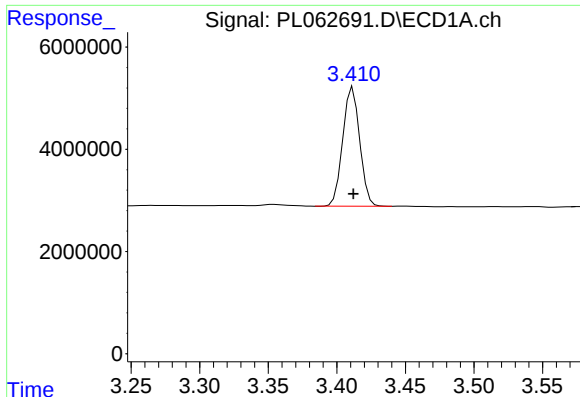


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 20112129
Conc: 11.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-01-102820


Manual Integrations
APPROVED

Ankita
10/30/2020 3:54:40 PM

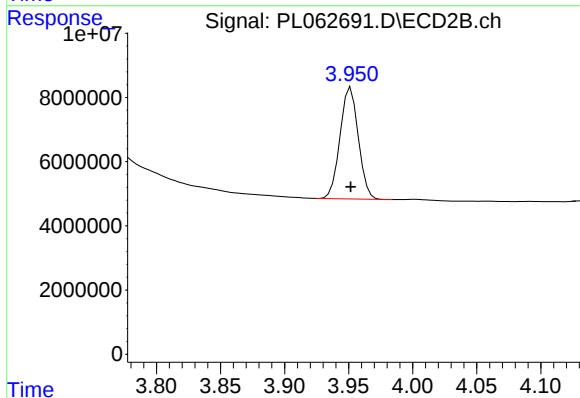


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 34428026
Conc: 11.72 ng/ml

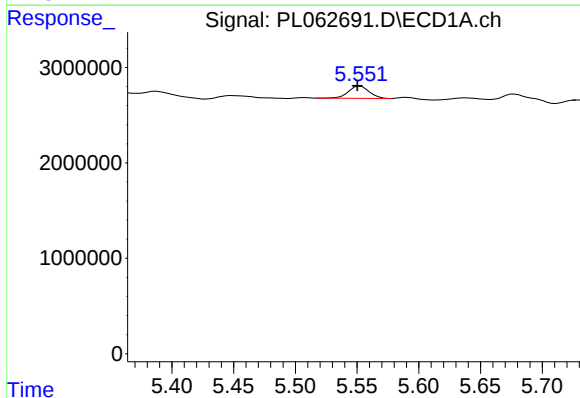


#12 4,4'-DDE

R.T.: 5.553 min
Delta R.T.: 0.002 min
Response: 1514333
Conc: 0.92 ng/ml

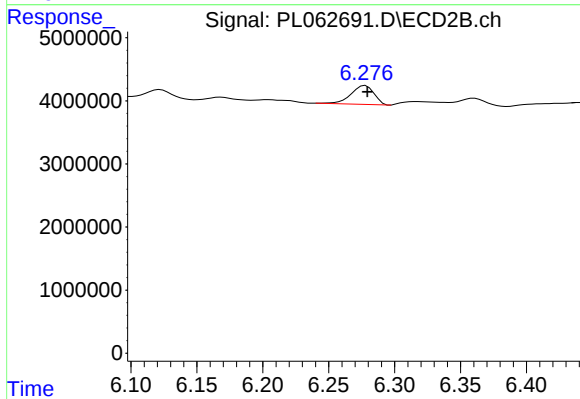

#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: -0.002 min
Response: 3606975
Conc: 1.12 ng/ml

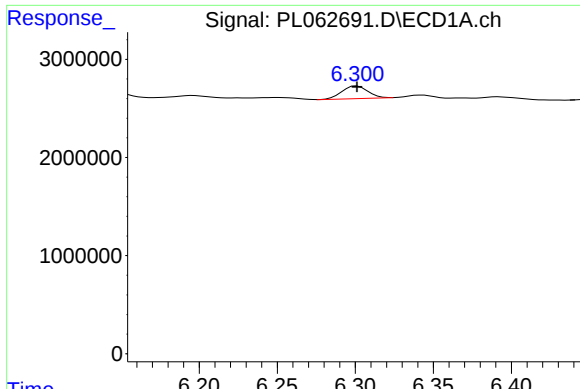


#17 4,4'-DDT

R.T.: 6.300 min
Delta R.T.: -0.002 min
Response: 1507154
Conc: 1.13 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HR-01-102820


Manual Integrations
APPROVED

Ankita
10/30/2020 3:54:40 PM

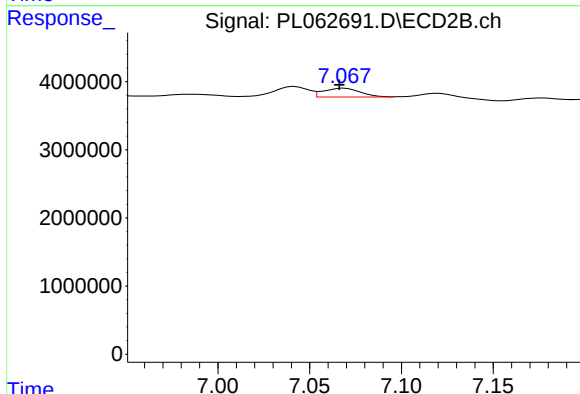


#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.001 min
Response: 1771917
Conc: 0.79 ng/ml m

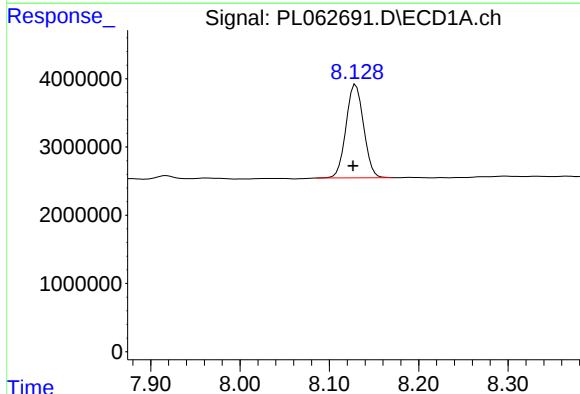

#28 Decachlorobiphenyl

R.T.: 8.130 min
Delta R.T.: 0.003 min
Response: 18709511
Conc: 11.66 ng/ml

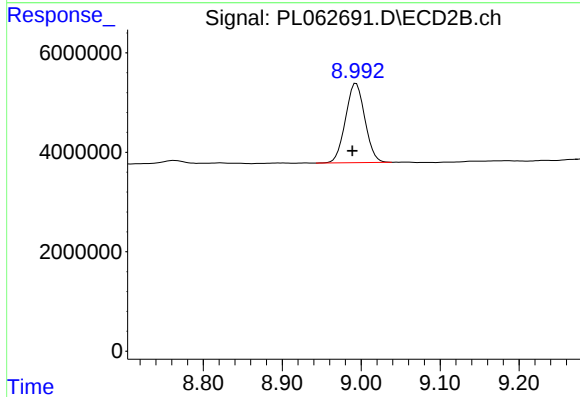

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.005 min
Response: 27196897
Conc: 12.99 ng/ml