

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
 Data File : PL070638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 02:37
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 07:49:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 29 07:43:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.583	5.518	9325664	29176987	20.682	20.975
28)	SA Decachlor...	10.347	11.419	11858030	25951520	19.863	18.154
Target Compounds							
7)	B delta-BHC	0.000	7.038f	0	7097178	N.D.	1.659 #
9)	A Endosulfan I	7.423	8.384	5376066	14963370	9.559	8.882
10)	B gamma-Chl...	7.298	8.248	5694532	15707637	9.386	8.636
12)	B 4,4'-DDE	7.582	8.518	9245539	31825871	17.741	17.637
13)	MA Dieldrin	7.709	8.673	10827792	31575571	18.863	17.922
19)	B Endosulfa...	8.731	9.519	10818448	26807919	19.193	17.886
20)	A Methoxychlor	9.024	9.861	29051725	70479620	87.442	84.189
21)	B Endrin ke...	9.249	10.016	12223782	29302745	19.273	17.933
25)	Chlordane-3	7.298	8.248	5694532	15707637	98.451	64.266 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
Data File : PL070638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 02:37
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 07:49:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
Quant Title : GC Extractables
QLast Update : Fri Oct 29 07:43:54 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

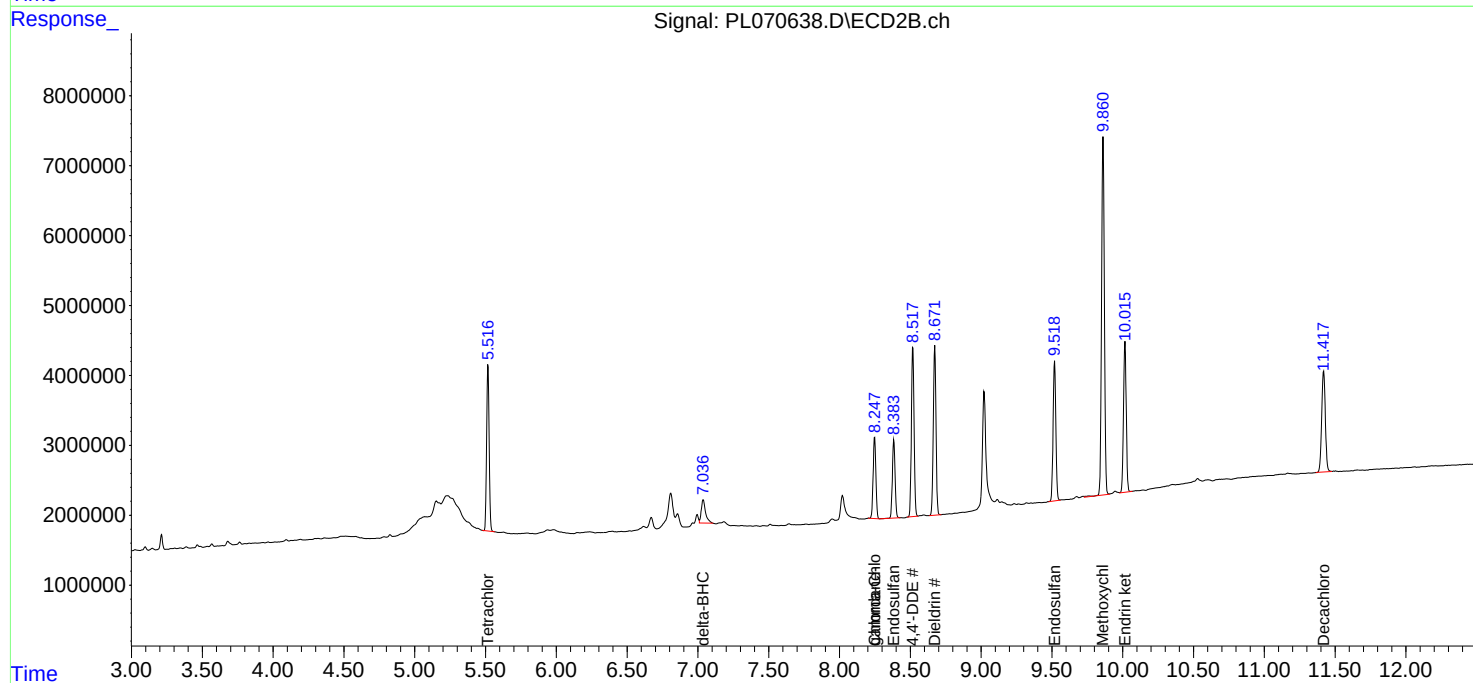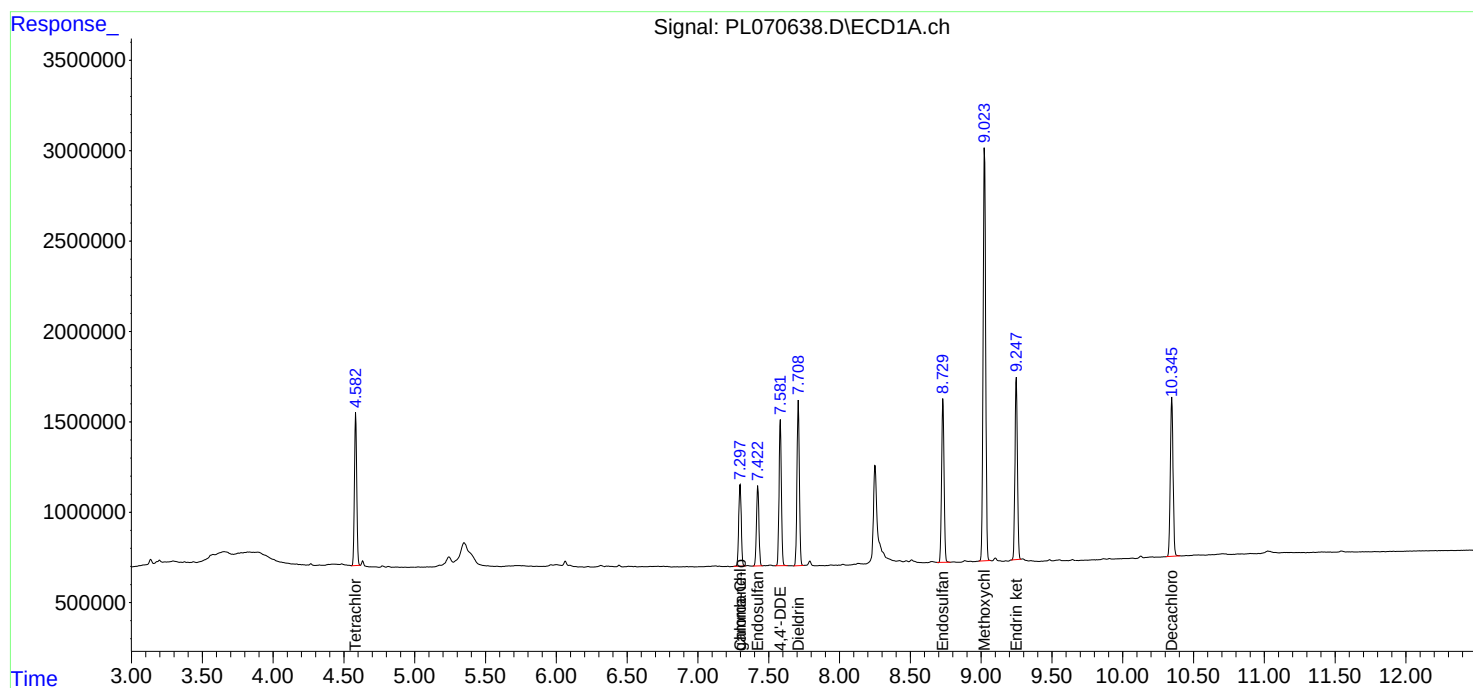

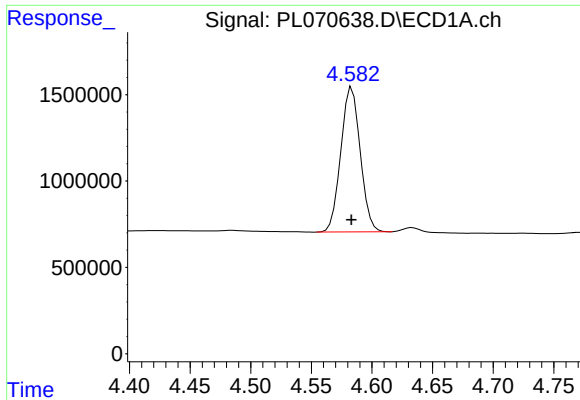


#1 Tetrachloro-m-xylene

R.T.: 4.583 min
Delta R.T.: 0.000 min
Response: 9325664
Conc: 20.68 ng/ml

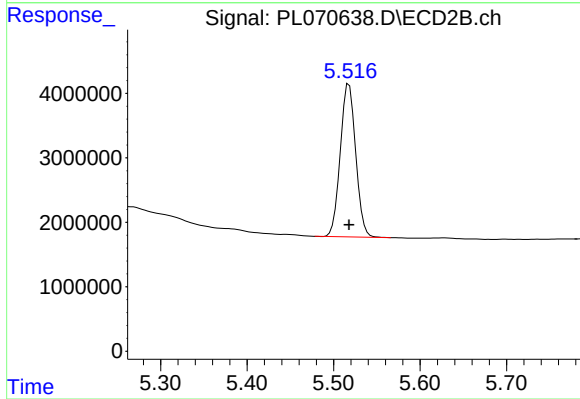


#1 Tetrachloro-m-xylene

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 29176987
Conc: 20.97 ng/ml

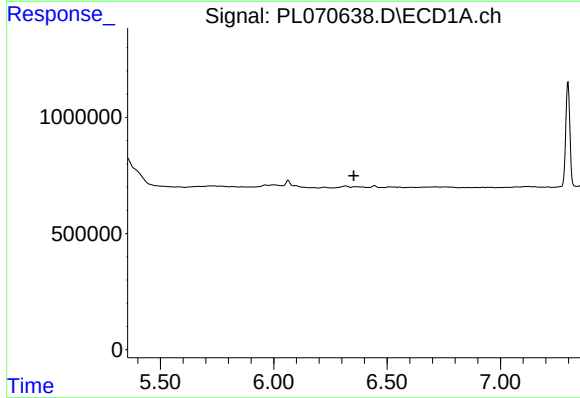


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

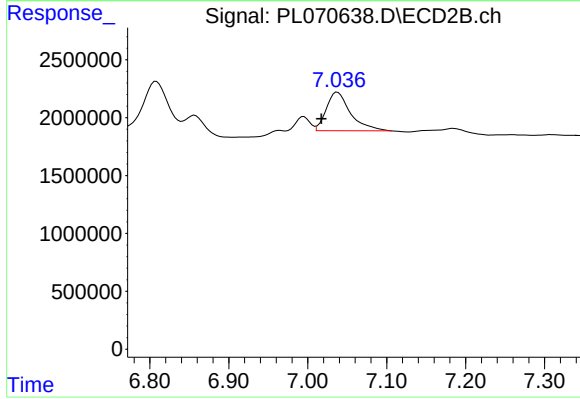


#7 delta-BHC

R.T.: 7.038 min
Delta R.T.: 0.021 min
Response: 7097178
Conc: 1.66 ng/ml

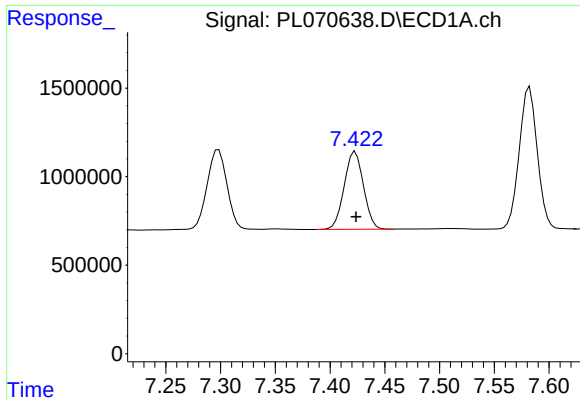


#9 Endosulfan I

R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 5376066
Conc: 9.56 ng/ml

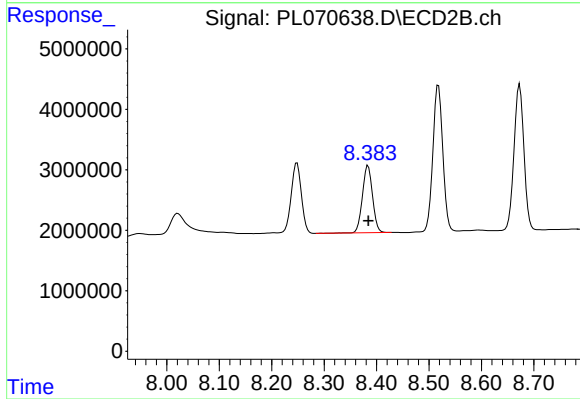


#9 Endosulfan I

R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 14963370
Conc: 8.88 ng/ml

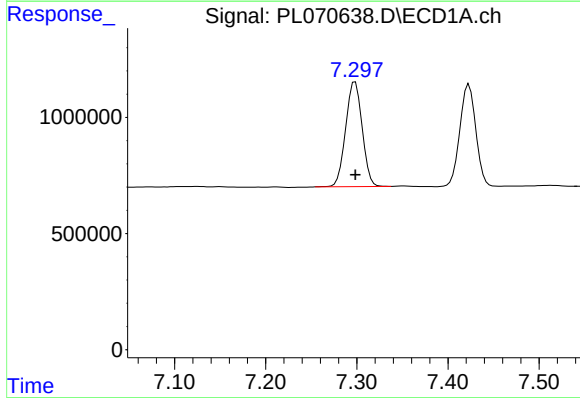


#10 gamma-Chlordane

R.T.: 7.298 min
Delta R.T.: 0.000 min
Response: 5694532
Conc: 9.39 ng/ml

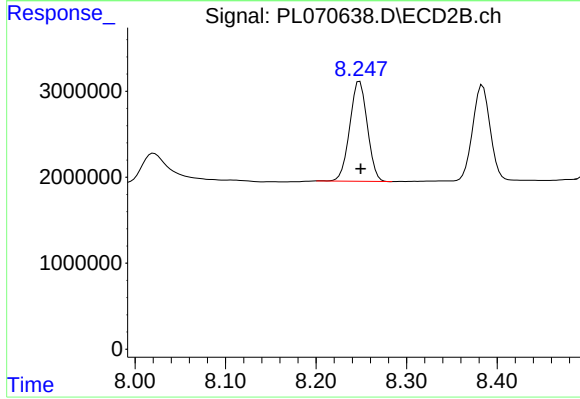


#10 gamma-Chlordane

R.T.: 8.248 min
Delta R.T.: 0.000 min
Response: 15707637
Conc: 8.64 ng/ml

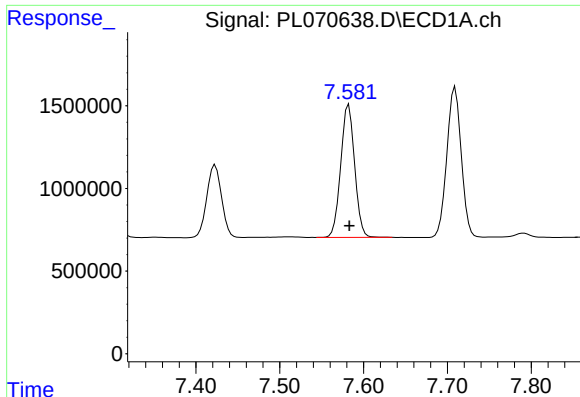


#12 4,4'-DDE

R.T.: 7.582 min
Delta R.T.: 0.000 min
Response: 9245539
Conc: 17.74 ng/ml

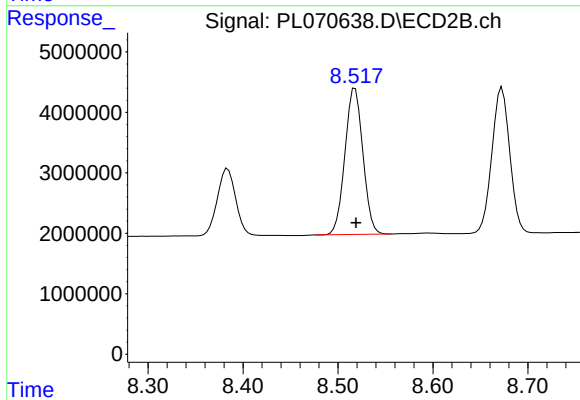


#12 4,4'-DDE

R.T.: 8.518 min
Delta R.T.: -0.001 min
Response: 31825871
Conc: 17.64 ng/ml

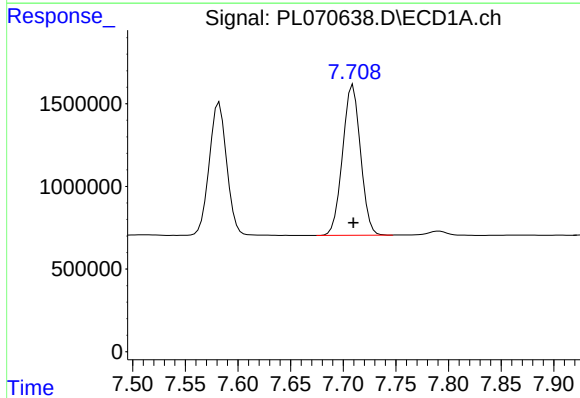


#13 Dieldrin

R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 10827792
Conc: 18.86 ng/ml

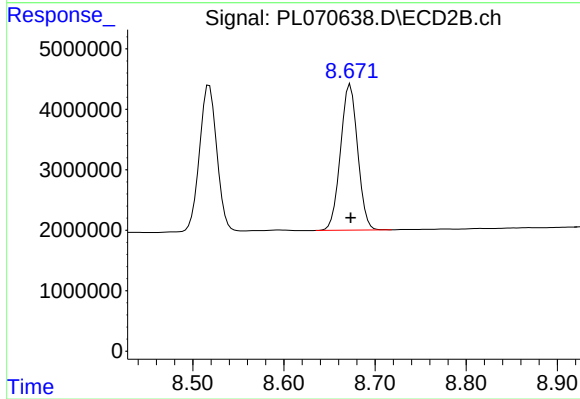


#13 Dieldrin

R.T.: 8.673 min
Delta R.T.: 0.000 min
Response: 31575571
Conc: 17.92 ng/ml

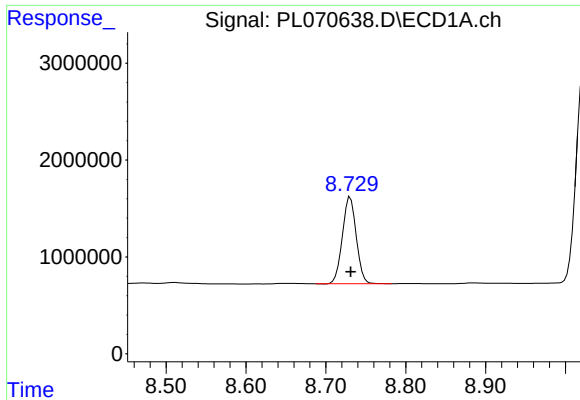


#19 Endosulfan Sulfate

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 10818448
Conc: 19.19 ng/ml

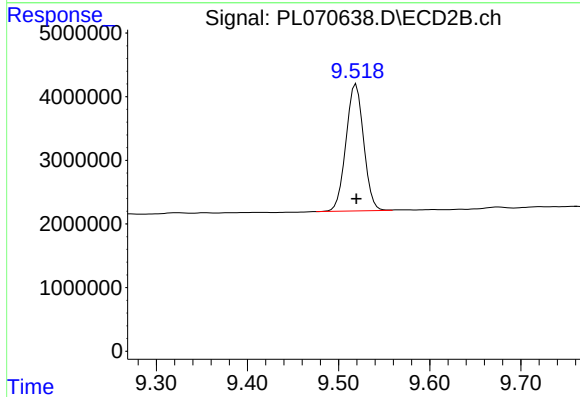


#19 Endosulfan Sulfate

R.T.: 9.519 min
Delta R.T.: 0.000 min
Response: 26807919
Conc: 17.89 ng/ml

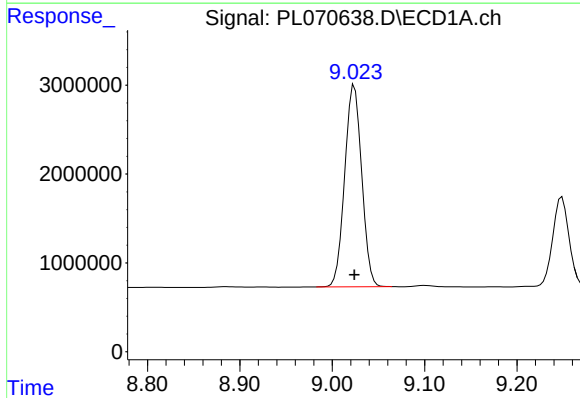


#20 Methoxychlor

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 29051725
Conc: 87.44 ng/ml

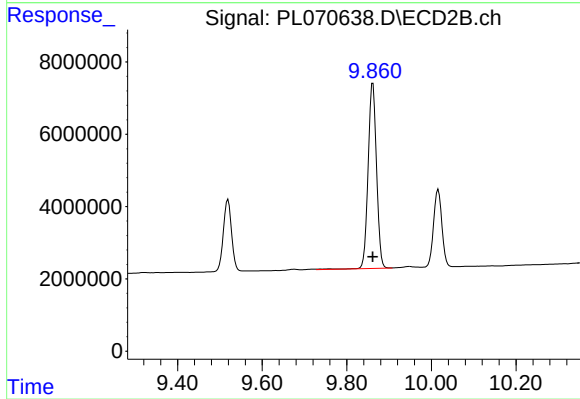


#20 Methoxychlor

R.T.: 9.861 min
Delta R.T.: 0.000 min
Response: 70479620
Conc: 84.19 ng/ml

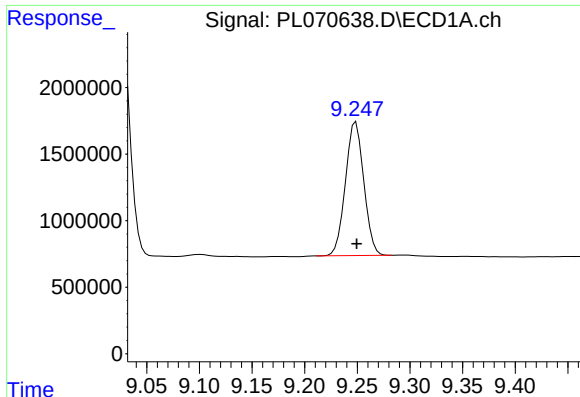


#21 Endrin ketone

R.T.: 9.249 min
Delta R.T.: 0.000 min
Response: 12223782
Conc: 19.27 ng/ml

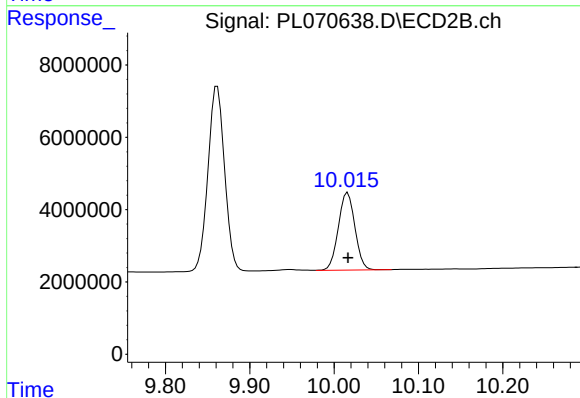


#21 Endrin ketone

R.T.: 10.016 min
Delta R.T.: 0.000 min
Response: 29302745
Conc: 17.93 ng/ml

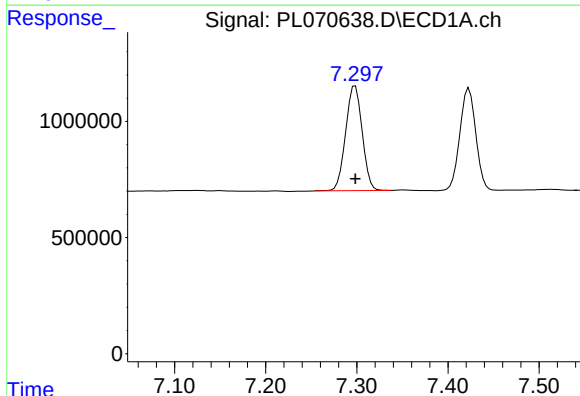


#25 Chlordane-3

R.T.: 7.298 min
Delta R.T.: 0.000 min
Response: 5694532
Conc: 98.45 ng/ml

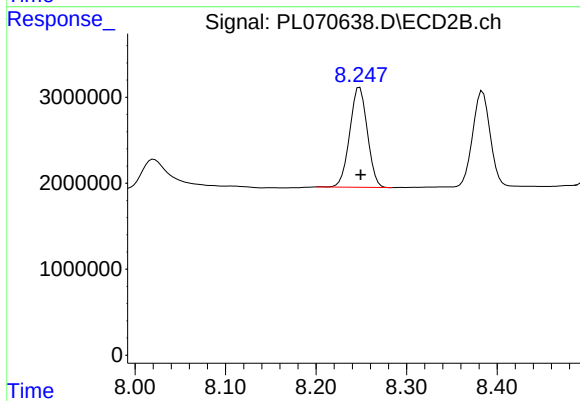


#25 Chlordane-3

R.T.: 8.248 min
Delta R.T.: 0.000 min
Response: 15707637
Conc: 64.27 ng/ml

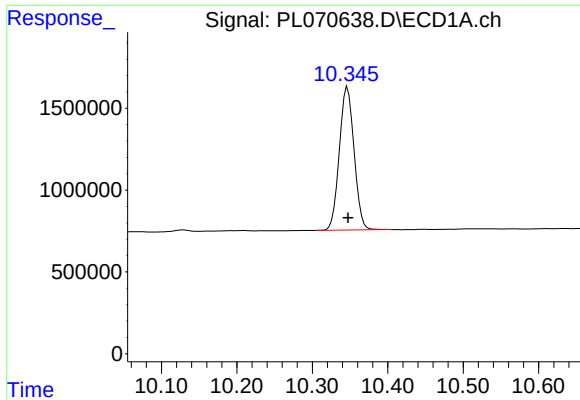

#28 Decachlorobiphenyl

R.T.: 10.347 min
Delta R.T.: 0.000 min
Response: 11858030
Conc: 19.86 ng/ml

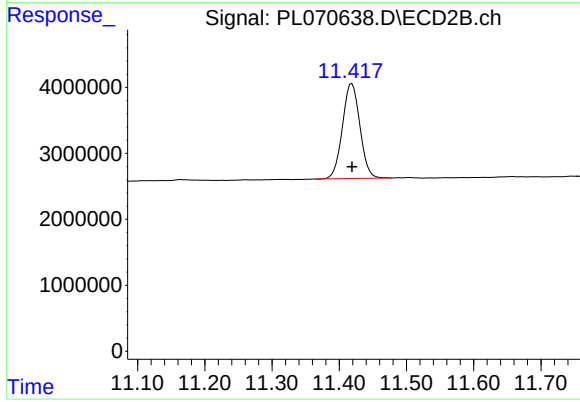

#28 Decachlorobiphenyl

R.T.: 11.419 min
Delta R.T.: 0.000 min
Response: 25951520
Conc: 18.15 ng/ml