

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
 Data File : PL070644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 04:17
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 06:33:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 29 06:27:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.584	5.518	47997504	147.6E6	96.244	97.046
28)	SA Decachlor...	10.347	11.419	55828720	144.1E6	89.736	94.183
Target Compounds							
23)	Chlordane-1	5.910	6.901	16551890	58791274	967.209	995.097
24)	Chlordane-2	6.599	7.493	21439961	62134664	924.552	952.319
25)	Chlordane-3	7.299	8.250	59010917	257.2E6	978.407	992.233
26)	Chlordane-4	7.367	8.332	63282119	302.8E6	971.917	979.017
27)	Chlordane-5	8.316	9.218	22158778	54746890	935.233	985.835



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
Data File : PL070644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 04:17
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 06:33:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
Quant Title : GC Extractables
QLast Update : Fri Oct 29 06:27:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

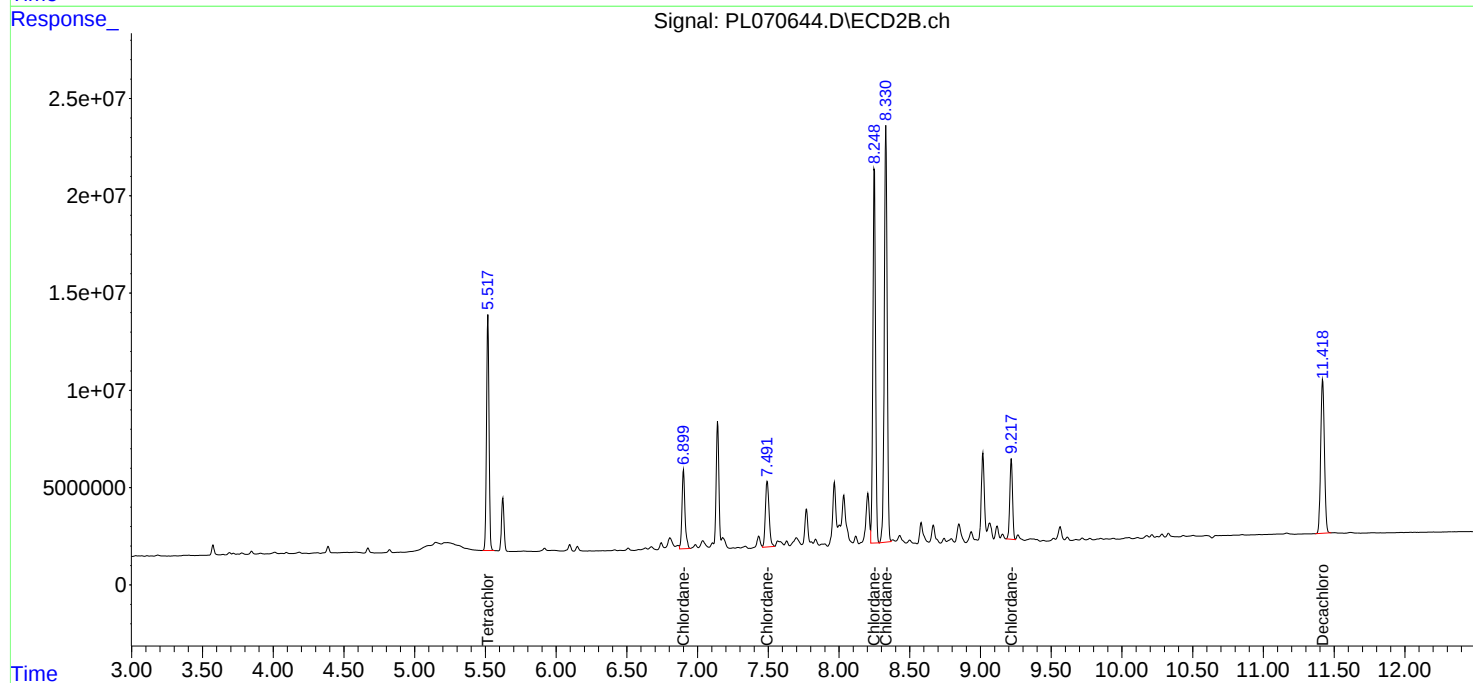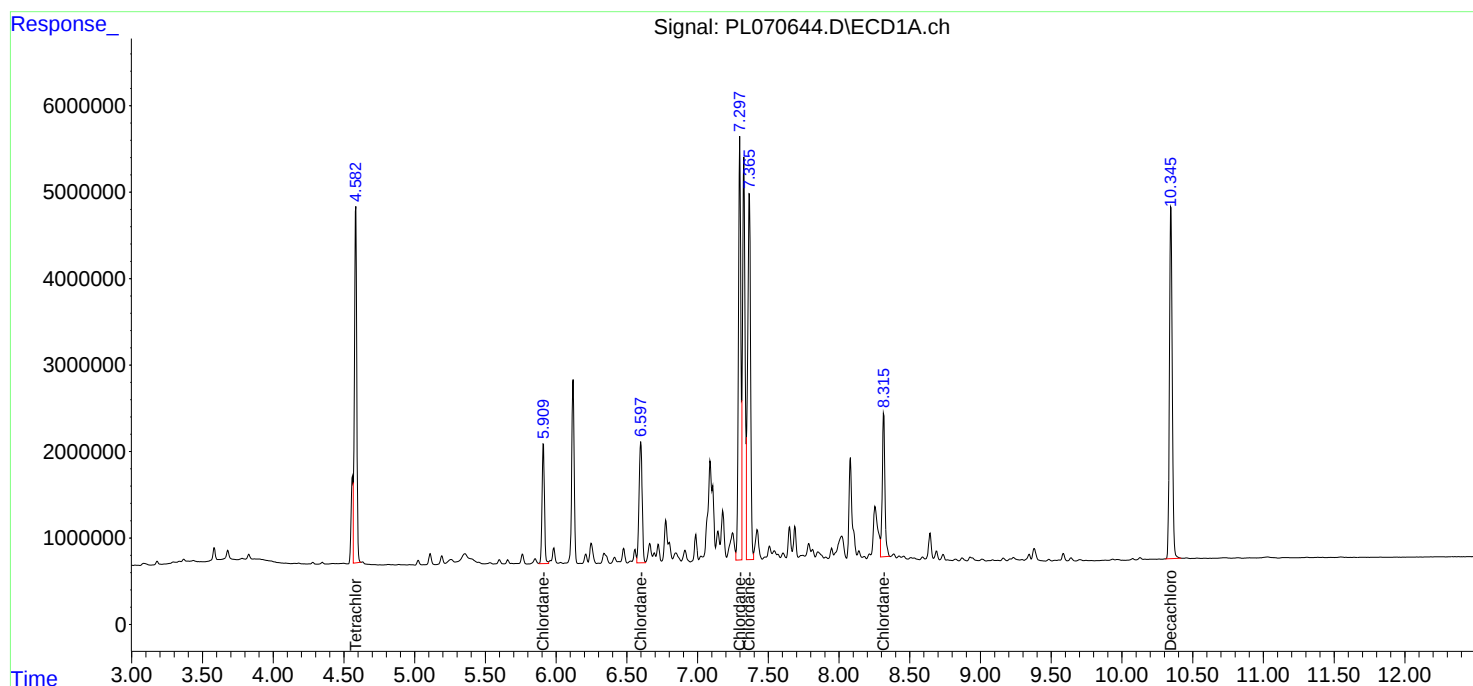


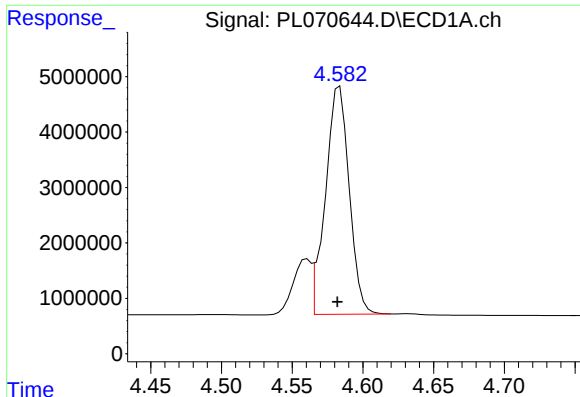

#1 Tetrachloro-m-xylene


R.T.: 4.584 min
Delta R.T.: 0.002 min
Response: 47997504
Conc: 96.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

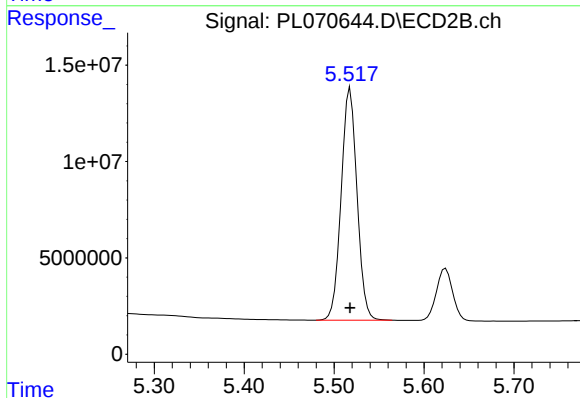


#1 Tetrachloro-m-xylene

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 147636862
Conc: 97.05 ng/ml

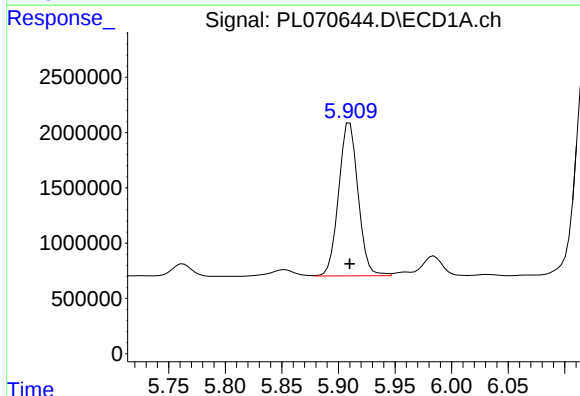


#23 Chlordane-1

R.T.: 5.910 min
Delta R.T.: 0.000 min
Response: 16551890
Conc: 967.21 ng/ml

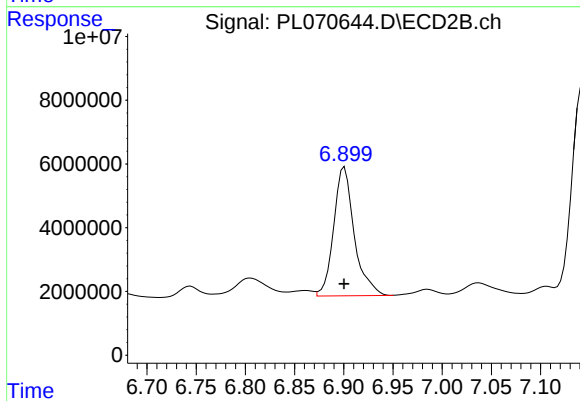

#23 Chlordane-1


R.T.: 6.901 min
Delta R.T.: 0.000 min
Response: 58791274
Conc: 995.10 ng/ml

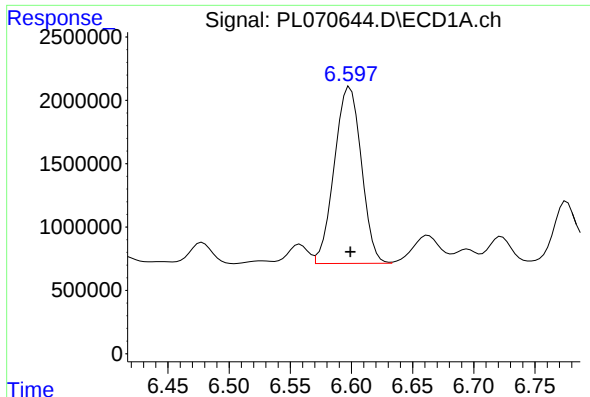

#24 Chlordane-2


R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 21439961
Conc: 924.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

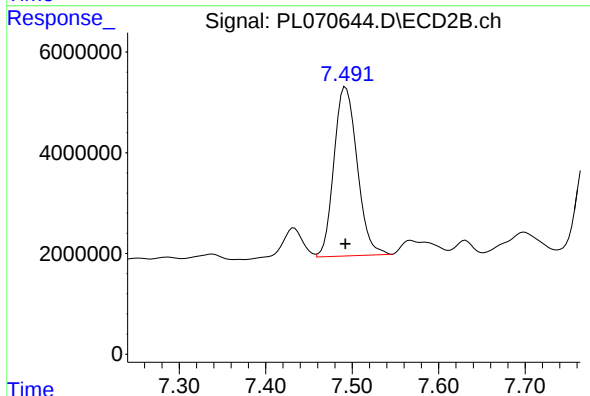


#24 Chlordane-2

R.T.: 7.493 min
Delta R.T.: 0.000 min
Response: 62134664
Conc: 952.32 ng/ml

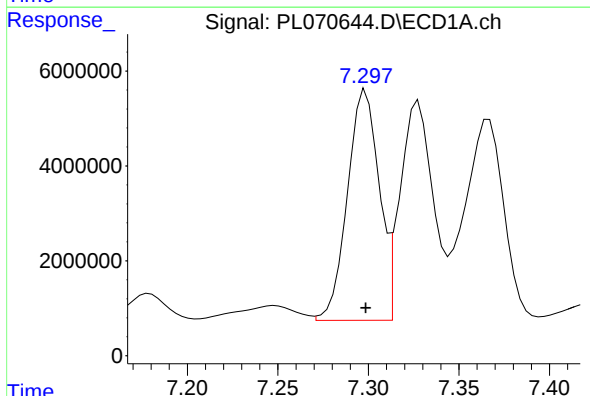


#25 Chlordane-3

R.T.: 7.299 min
Delta R.T.: 0.000 min
Response: 59010917
Conc: 978.41 ng/ml

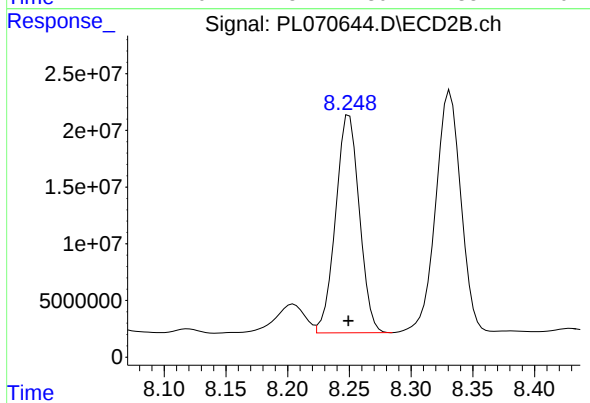

#25 Chlordane-3


R.T.: 8.250 min
Delta R.T.: 0.000 min
Response: 257178874
Conc: 992.23 ng/ml

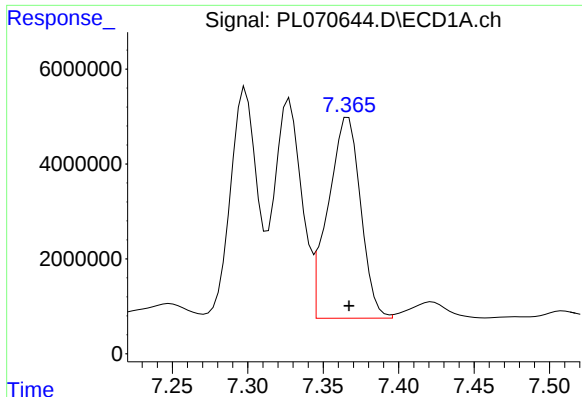

#26 Chlordane-4


R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 63282119
Conc: 971.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

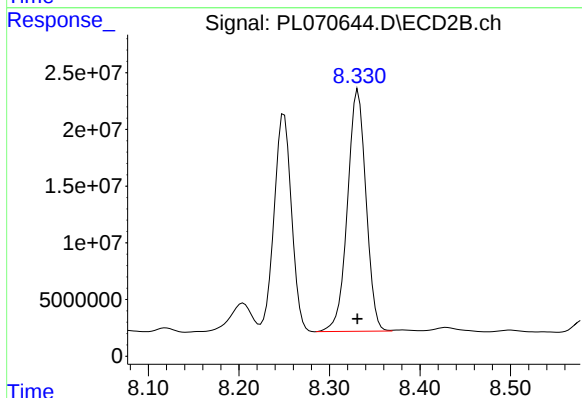


#26 Chlordane-4

R.T.: 8.332 min
Delta R.T.: 0.000 min
Response: 302782479
Conc: 979.02 ng/ml

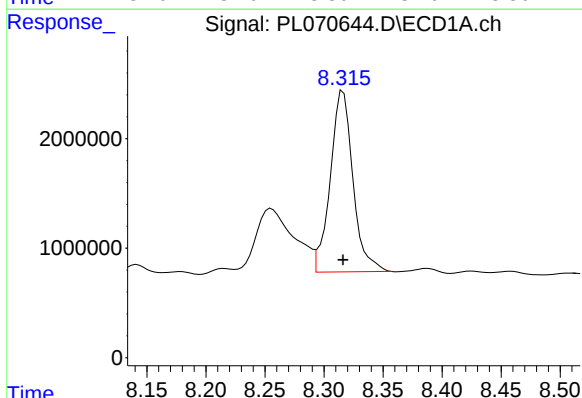


#27 Chlordane-5

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 22158778
Conc: 935.23 ng/ml

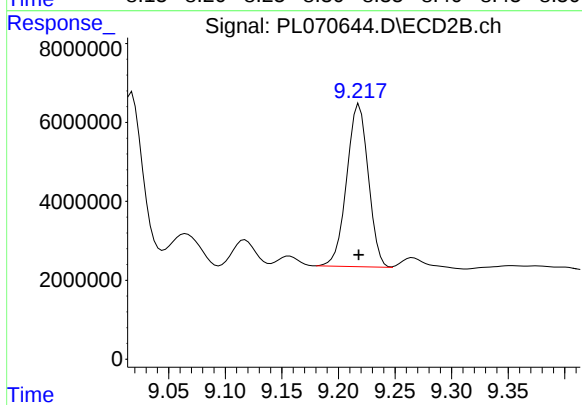

#27 Chlordane-5


R.T.: 9.218 min
Delta R.T.: 0.000 min
Response: 54746890
Conc: 985.83 ng/ml

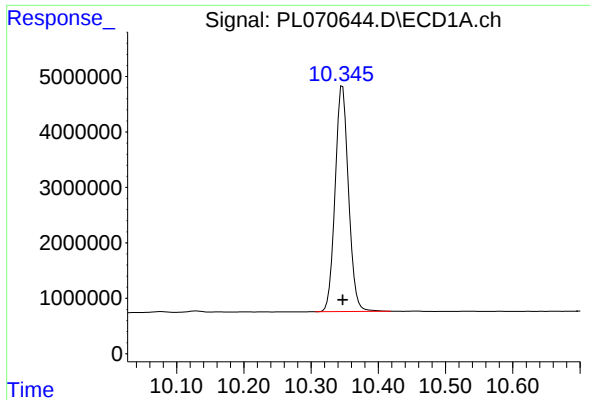

#28 Decachlorobiphenyl

R.T.: 10.347 min
Delta R.T.: 0.000 min
Response: 55828720
Conc: 89.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

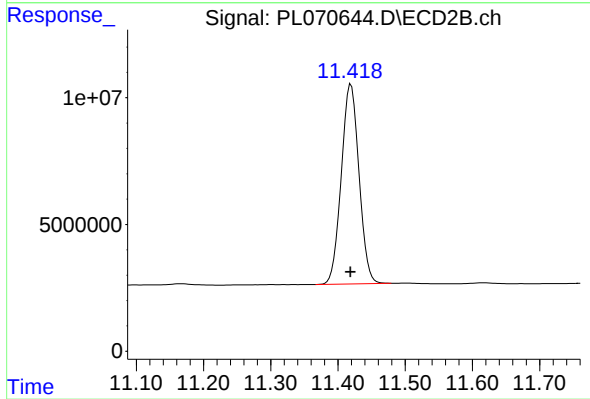

#28 Decachlorobiphenyl

R.T.: 11.419 min
Delta R.T.: 0.000 min
Response: 144117732
Conc: 94.18 ng/ml