

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
 Data File : PL070645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 04:34
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 06:33:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 29 06:27:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.583	5.518	35614315	109.7E6	71.413	72.121
28)	SA Decachlor...	10.347	11.419	42838981	109.0E6	68.857	71.263
Target Compounds							
23)	Chlordane-1	5.910	6.901	12087515	42618508	706.334	721.358
24)	Chlordane-2	6.599	7.493	16065229	46546728	692.778	713.408
25)	Chlordane-3	7.298	8.250	42925931	189.7E6	711.716	731.794
26)	Chlordane-4	7.367	8.331	46032414	224.4E6	706.988	725.736
27)	Chlordane-5	8.316	9.218	16662532	40671082	703.259	732.370



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
Data File : PL070645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 04:34
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 06:33:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
Quant Title : GC Extractables
QLast Update : Fri Oct 29 06:27:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

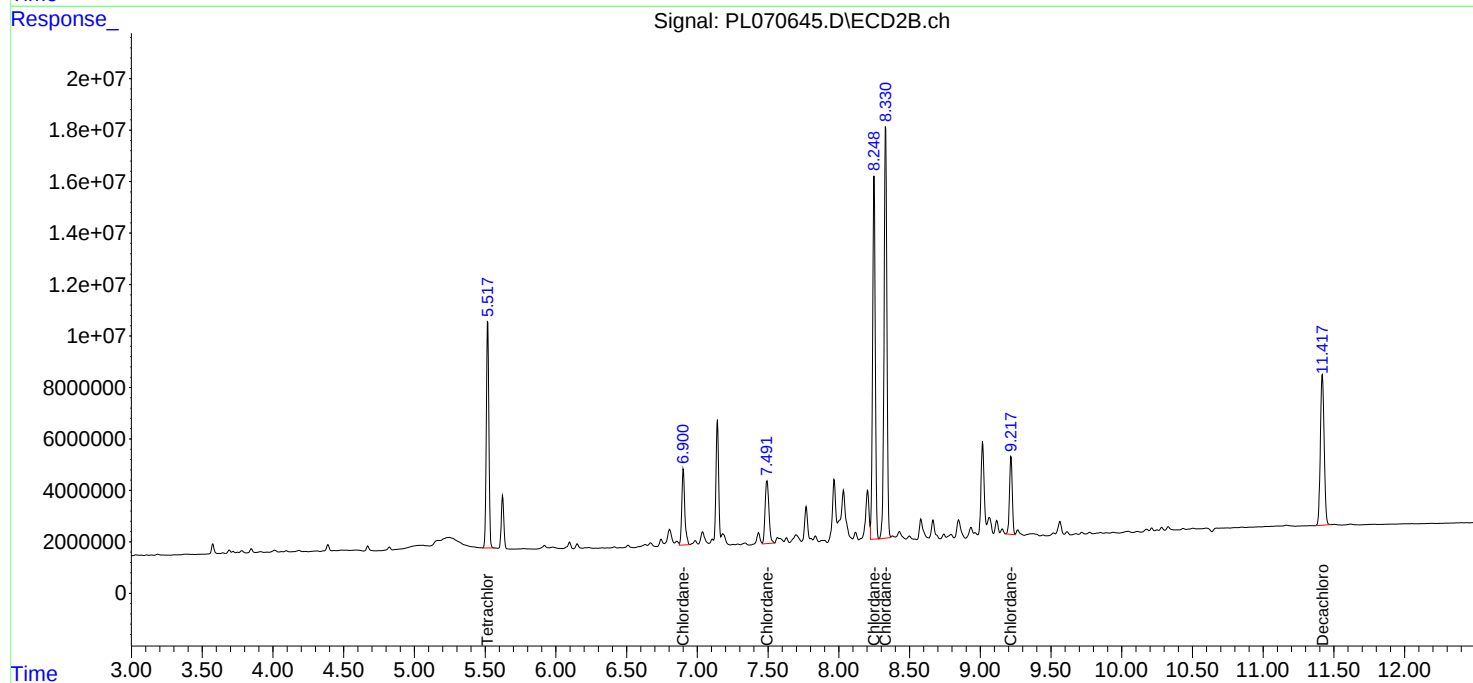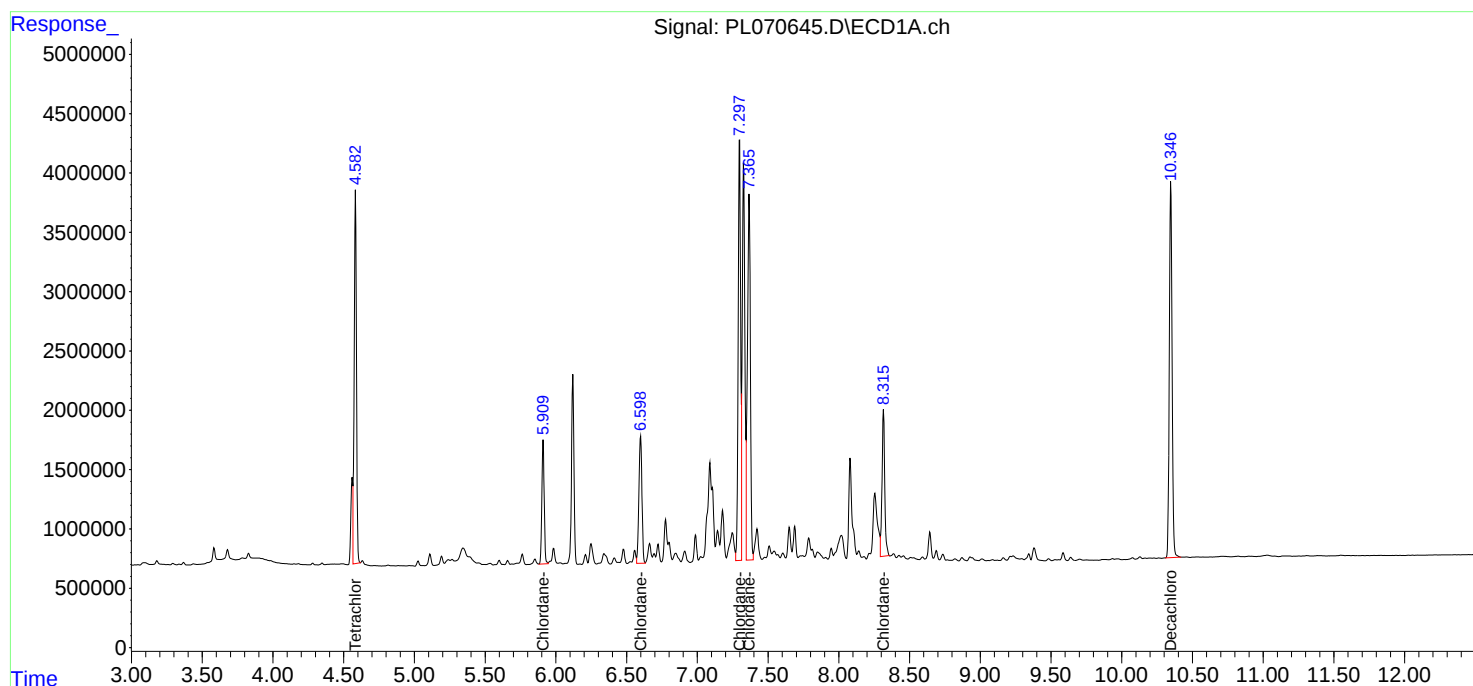


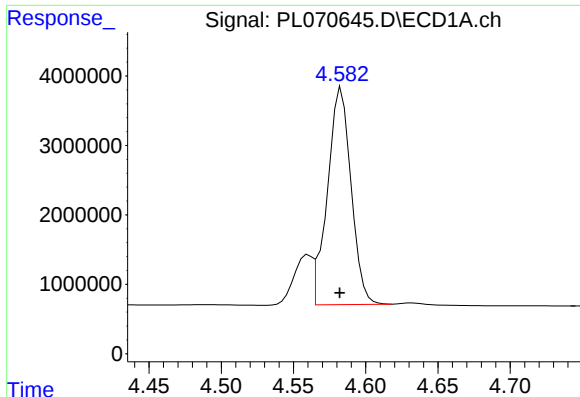

#1 Tetrachloro-m-xylene


R.T.: 4.583 min
Delta R.T.: 0.001 min
Response: 35614315
Conc: 71.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

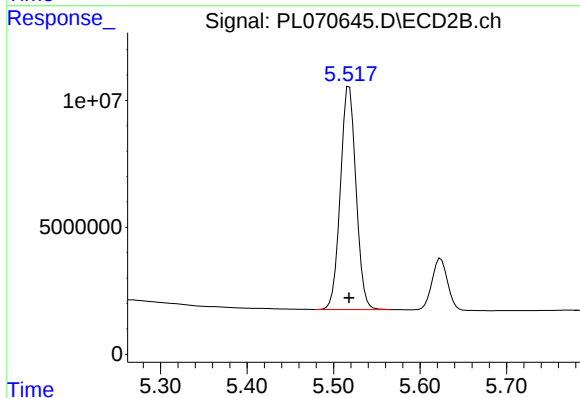


#1 Tetrachloro-m-xylene

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 109719068
Conc: 72.12 ng/ml

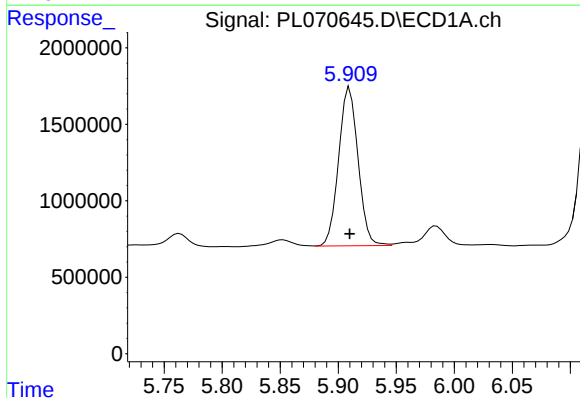


#23 Chlordane-1

R.T.: 5.910 min
Delta R.T.: 0.000 min
Response: 12087515
Conc: 706.33 ng/ml

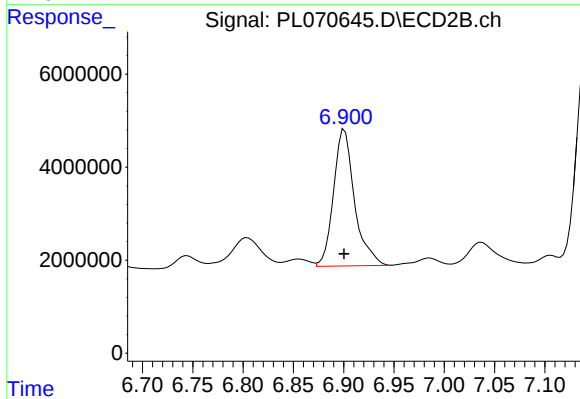

#23 Chlordane-1


R.T.: 6.901 min
Delta R.T.: 0.000 min
Response: 42618508
Conc: 721.36 ng/ml

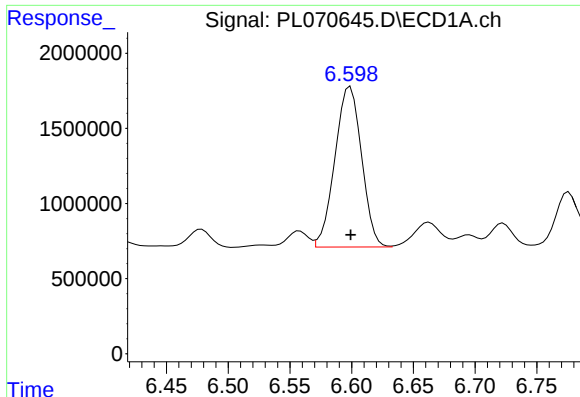

#24 Chlordane-2


R.T.: 6.599 min
Delta R.T.: 0.000 min
Response: 16065229
Conc: 692.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

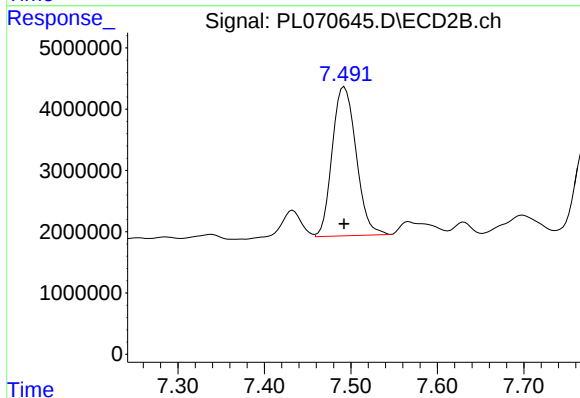


#24 Chlordane-2

R.T.: 7.493 min
Delta R.T.: 0.000 min
Response: 46546728
Conc: 713.41 ng/ml

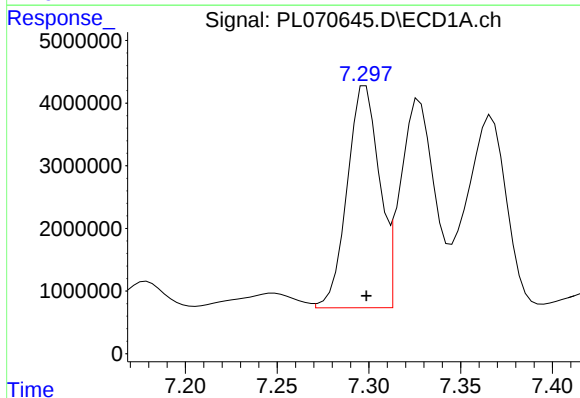


#25 Chlordane-3

R.T.: 7.298 min
Delta R.T.: 0.000 min
Response: 42925931
Conc: 711.72 ng/ml

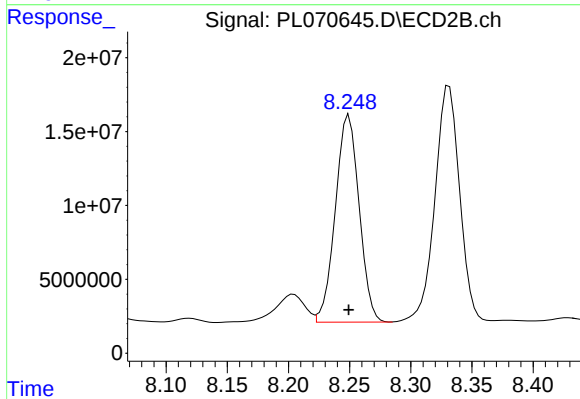

#25 Chlordane-3


R.T.: 8.250 min
Delta R.T.: 0.000 min
Response: 189675312
Conc: 731.79 ng/ml

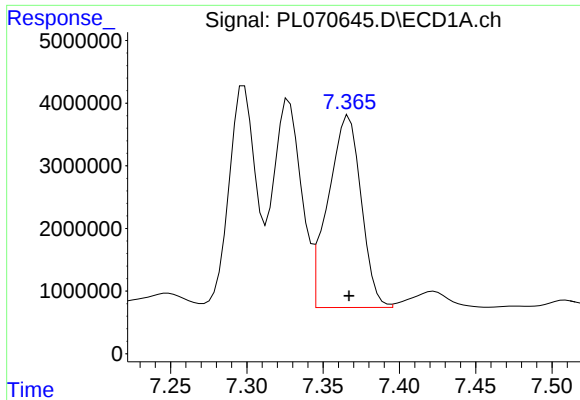

#26 Chlordane-4


R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 46032414
Conc: 706.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

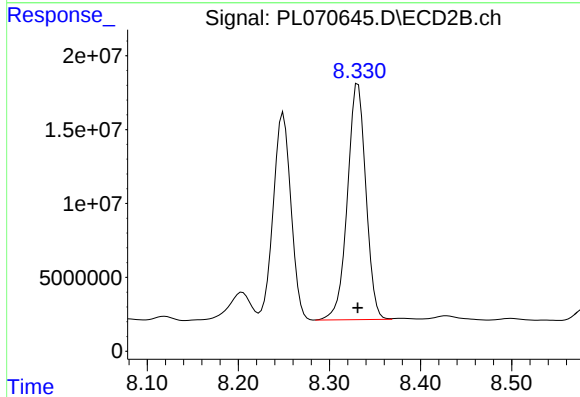


#26 Chlordane-4

R.T.: 8.331 min
Delta R.T.: 0.000 min
Response: 224449653
Conc: 725.74 ng/ml

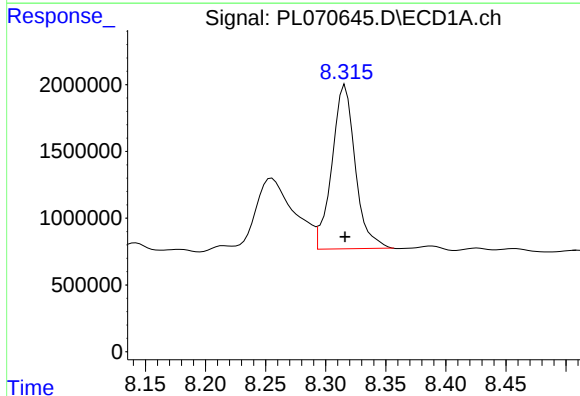


#27 Chlordane-5

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 16662532
Conc: 703.26 ng/ml

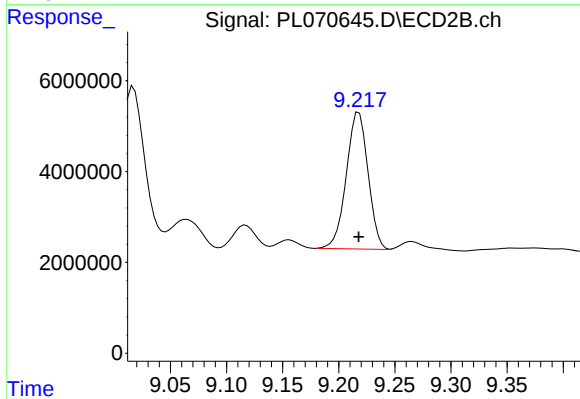

#27 Chlordane-5


R.T.: 9.218 min
Delta R.T.: 0.000 min
Response: 40671082
Conc: 732.37 ng/ml

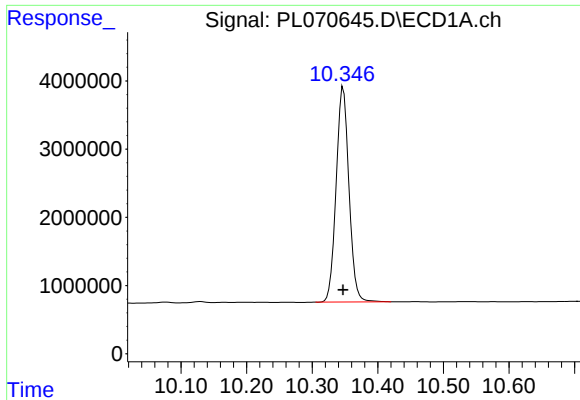

#28 Decachlorobiphenyl

R.T.: 10.347 min
Delta R.T.: 0.000 min
Response: 42838981
Conc: 68.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

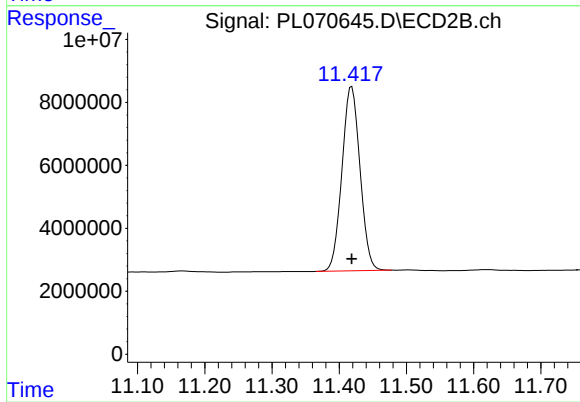

#28 Decachlorobiphenyl

R.T.: 11.419 min
Delta R.T.: 0.000 min
Response: 109045124
Conc: 71.26 ng/ml