

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
 Data File : PL070647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 05:07
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 06:31:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 29 06:27:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.584	5.518	11311047	33793009	22.681	22.213
28)	SA Decachlor...	10.347	11.418	15263285	35428207	24.533	23.153
Target Compounds							
23)	Chlordane-1	5.910	6.901	3919277	12808036	229.023	216.788
24)	Chlordane-2	6.598	7.492	5543071	14899656	239.033	228.362
25)	Chlordane-3	7.298	8.249	13610252	56017742	225.659	216.124
26)	Chlordane-4	7.366	8.332	14637045	67568149	224.803	218.475
27)	Chlordane-5	8.316	9.218	5646955	12254647	238.335	220.671



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102921\
Data File : PL070647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 05:07
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 06:31:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
Quant Title : GC Extractables
QLast Update : Fri Oct 29 06:27:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

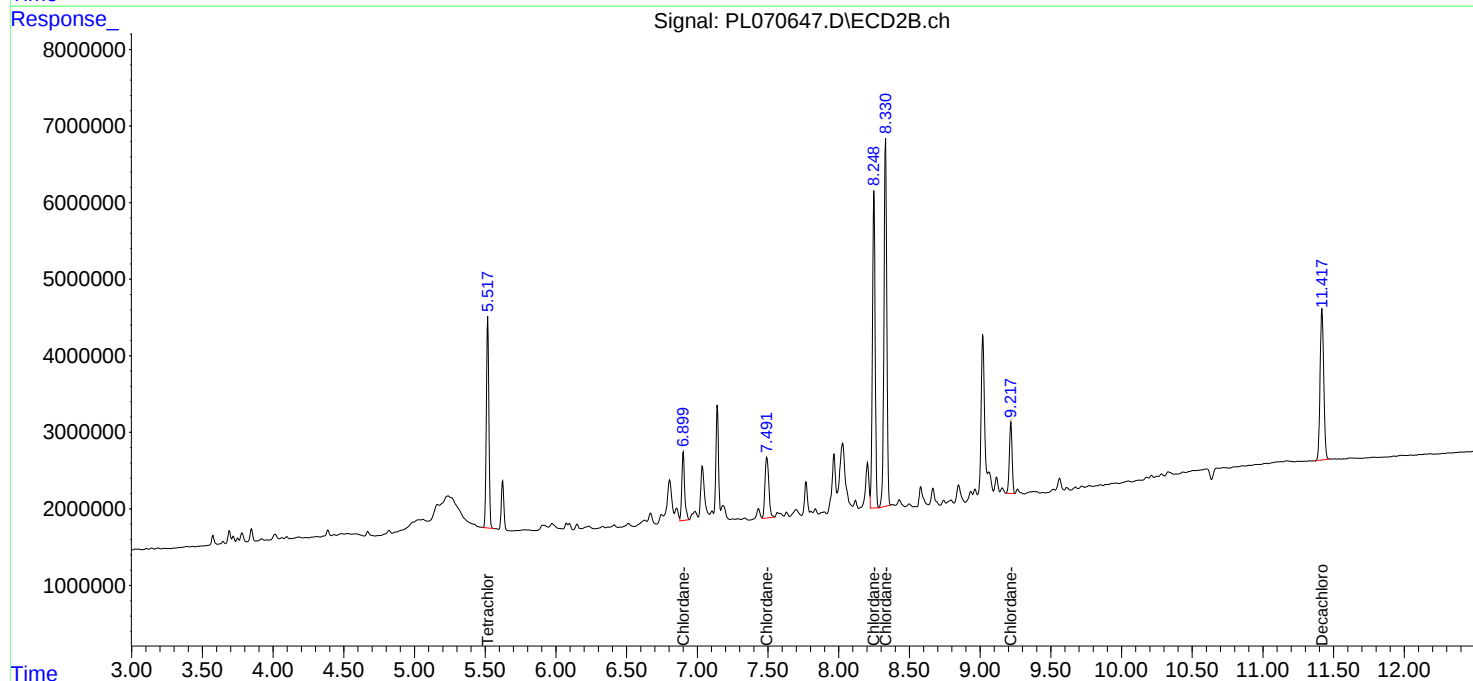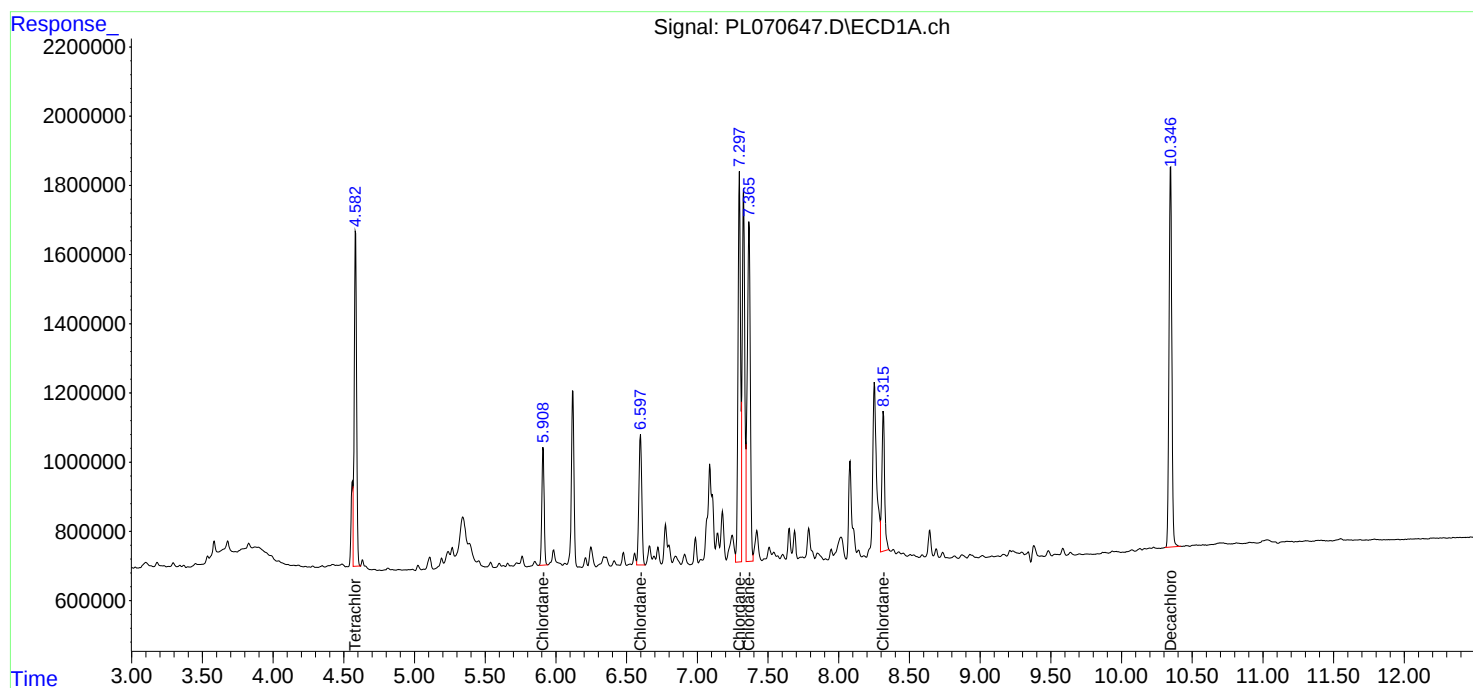


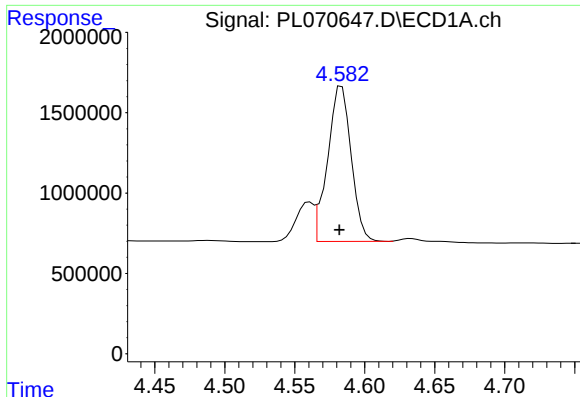

#1 Tetrachloro-m-xylene


R.T.: 4.584 min
Delta R.T.: 0.002 min
Response: 11311047
Conc: 22.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

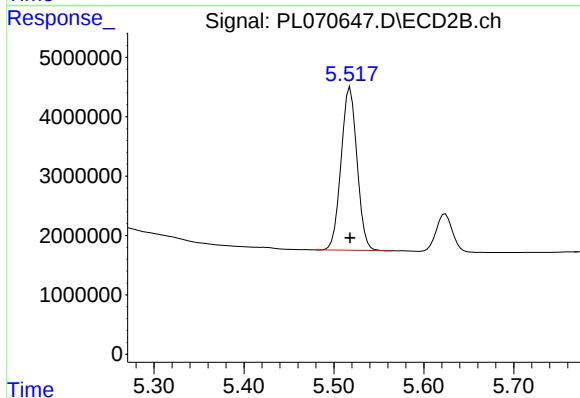


#1 Tetrachloro-m-xylene

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 33793009
Conc: 22.21 ng/ml

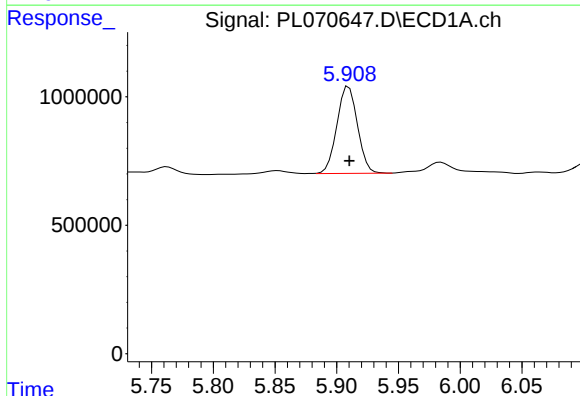


#23 Chlordane-1

R.T.: 5.910 min
Delta R.T.: 0.000 min
Response: 3919277
Conc: 229.02 ng/ml

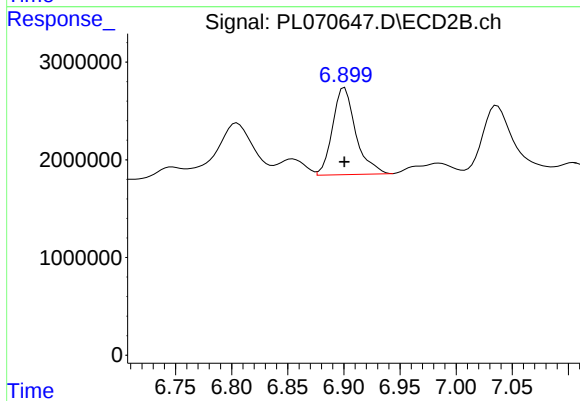

#23 Chlordane-1


R.T.: 6.901 min
Delta R.T.: 0.000 min
Response: 12808036
Conc: 216.79 ng/ml

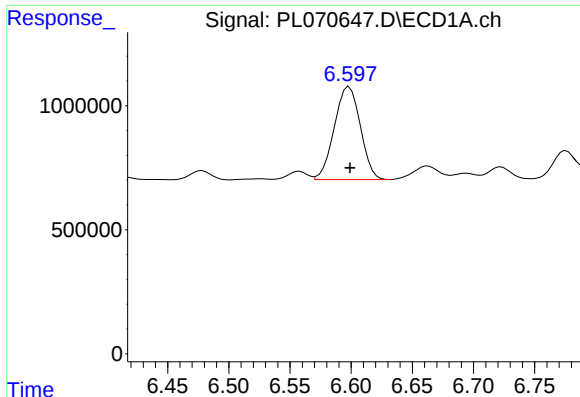

#24 Chlordane-2


R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 5543071
Conc: 239.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

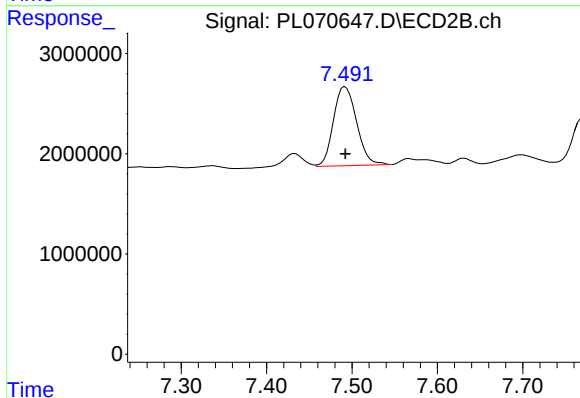


#24 Chlordane-2

R.T.: 7.492 min
Delta R.T.: 0.000 min
Response: 14899656
Conc: 228.36 ng/ml

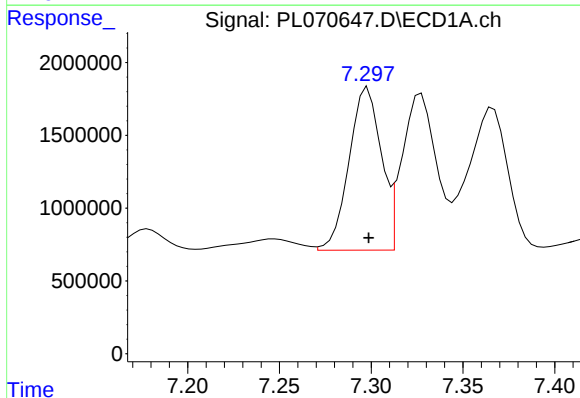


#25 Chlordane-3

R.T.: 7.298 min
Delta R.T.: 0.000 min
Response: 13610252
Conc: 225.66 ng/ml

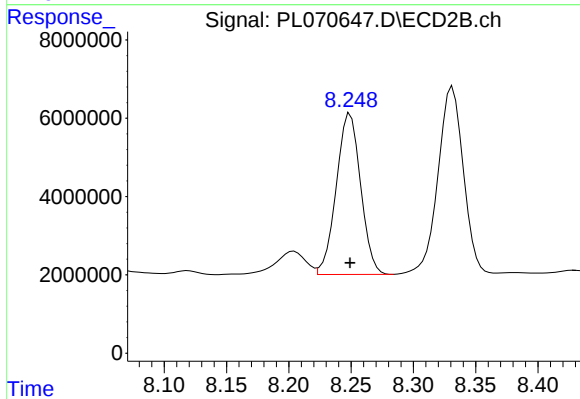

#25 Chlordane-3


R.T.: 8.249 min
Delta R.T.: 0.000 min
Response: 56017742
Conc: 216.12 ng/ml

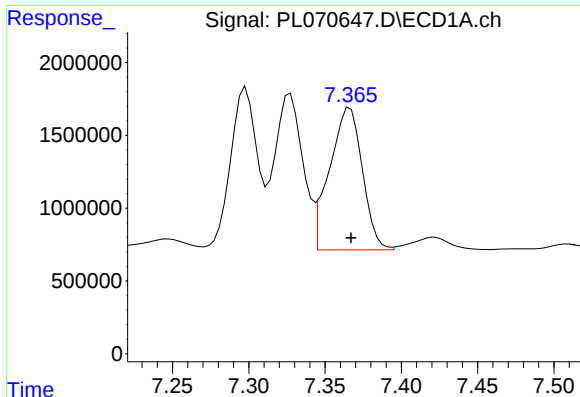

#26 Chlordane-4


R.T.: 7.366 min
Delta R.T.: 0.000 min
Response: 14637045
Conc: 224.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

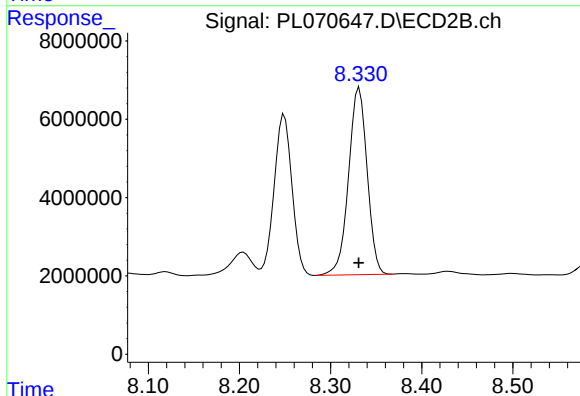


#26 Chlordane-4

R.T.: 8.332 min
Delta R.T.: 0.000 min
Response: 67568149
Conc: 218.47 ng/ml

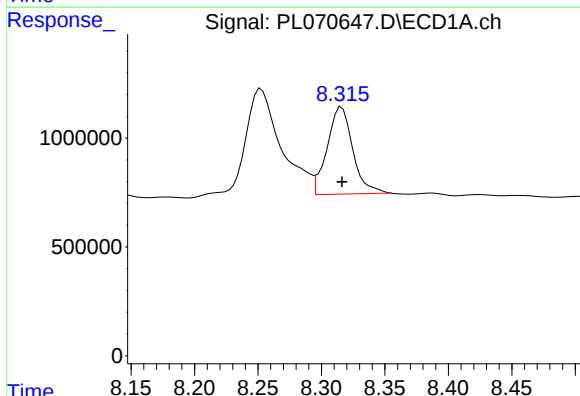


#27 Chlordane-5

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 5646955
Conc: 238.34 ng/ml

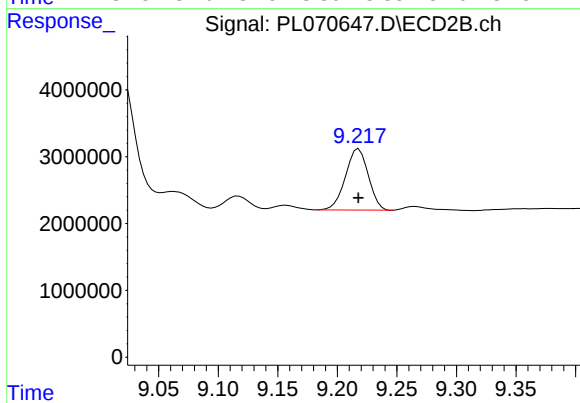

#27 Chlordane-5


R.T.: 9.218 min
Delta R.T.: 0.000 min
Response: 12254647
Conc: 220.67 ng/ml

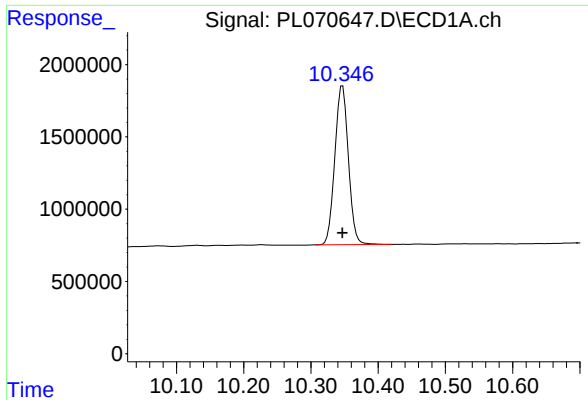

#28 Decachlorobiphenyl

R.T.: 10.347 min
Delta R.T.: 0.000 min
Response: 15263285
Conc: 24.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

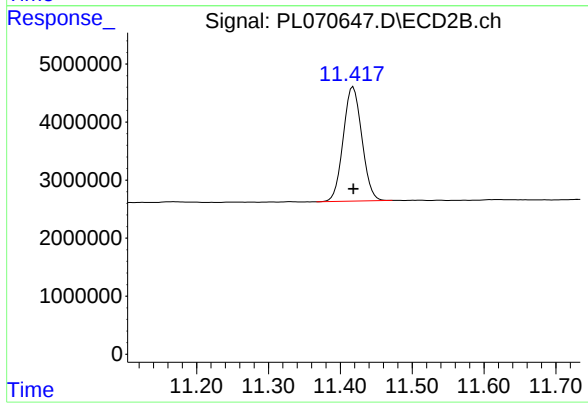

#28 Decachlorobiphenyl

R.T.: 11.418 min
Delta R.T.: 0.000 min
Response: 35428207
Conc: 23.15 ng/ml