

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 12:17
 Operator : AR\AJ
 Sample : PB164496BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164496BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:14:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.778	46412984	49207083	18.942	18.083
28)	SA Decachlor...	9.052	7.915	39150833	55848223	20.343	20.463
Target Compounds							
2)	A alpha-BHC	0.000	3.288	0	225749	N.D.	0.057 #
3)	MA gamma-BHC...	0.000	3.609	0	25248	N.D.	0.007 #
4)	MA Heptachlor	0.000	3.973f	0	59073	N.D.	0.016 #
5)	MB Aldrin	0.000	4.209f	0	45578	N.D.	0.012 #
7)	B delta-BHC	0.000	4.148	0	82024	N.D.	0.021 #
8)	B Heptachlo...	0.000	4.727	0	55141	N.D.	0.017 #
14)	MA Endrin	0.000	5.660f	0	304457	N.D.	0.105 #
22)	Mirex	0.000	7.047f	0	21553	N.D.	0.008 #
23)	Chlordane-1	0.000	3.792	0	84962	N.D.	0.800 #
24)	Chlordane-2	0.000	4.385f	0	478599	N.D.	3.864 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 12:17
Operator : AR\AJ
Sample : PB164496BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164496BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:14:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

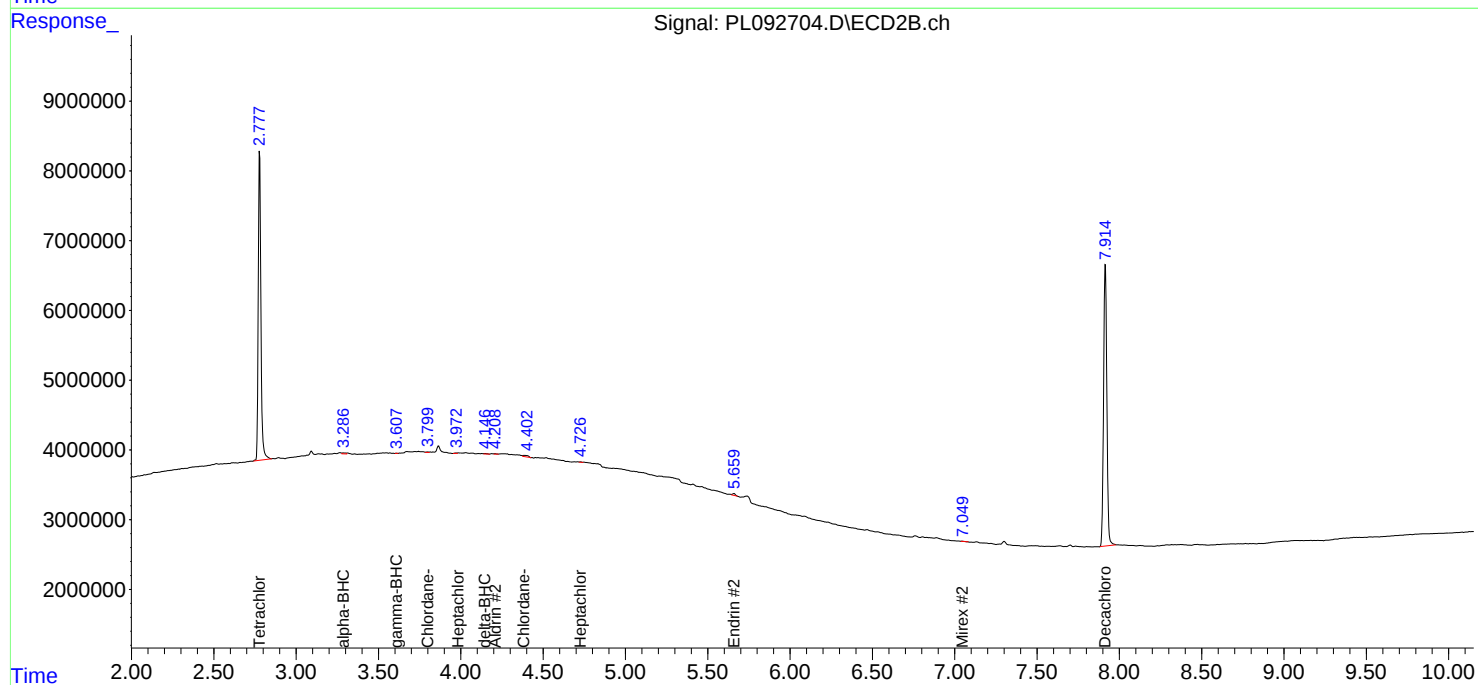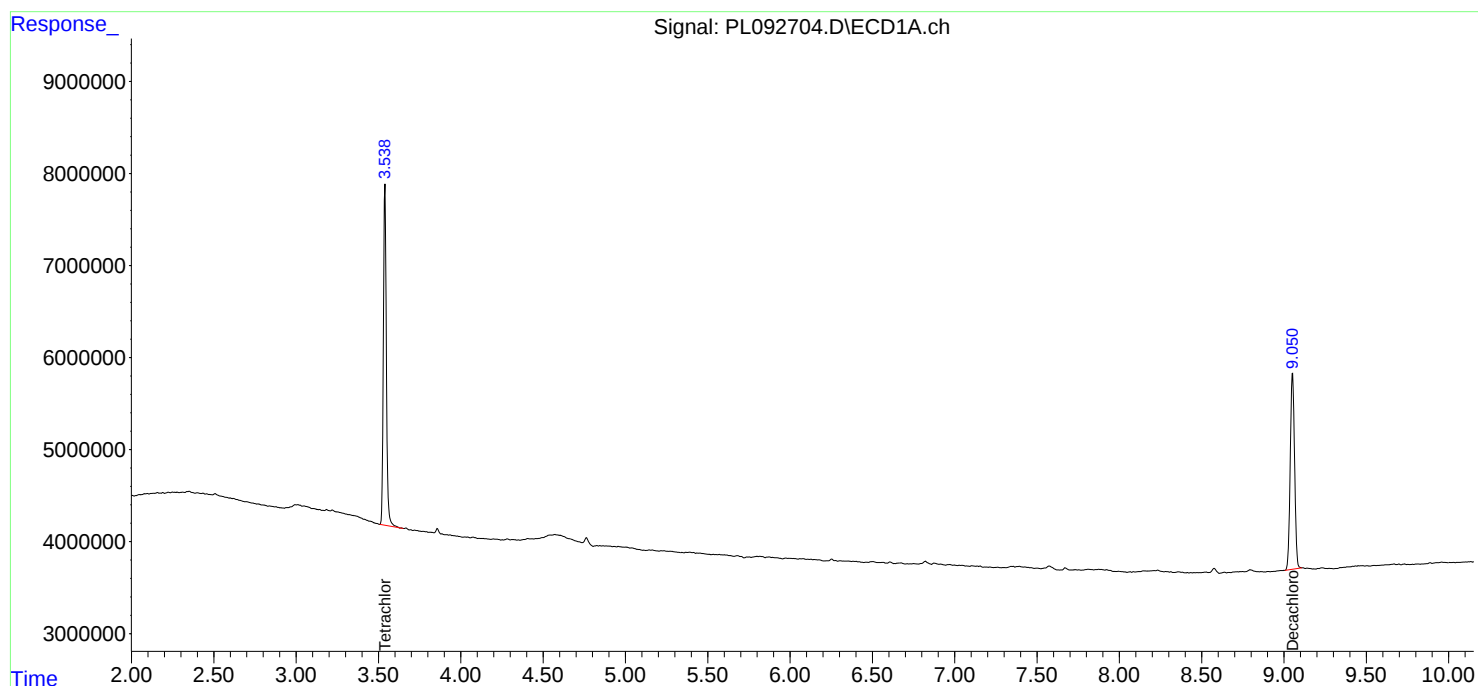


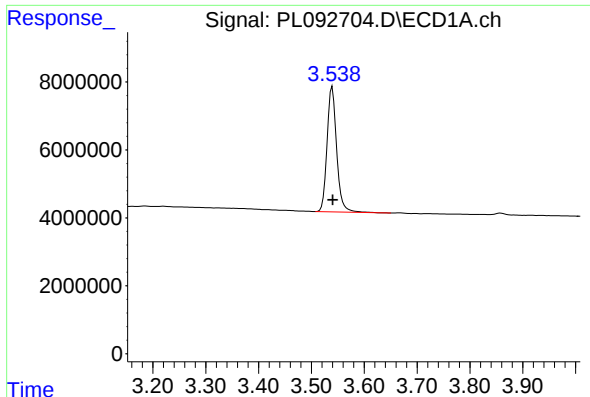

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 46412984
Conc: 18.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164496BL

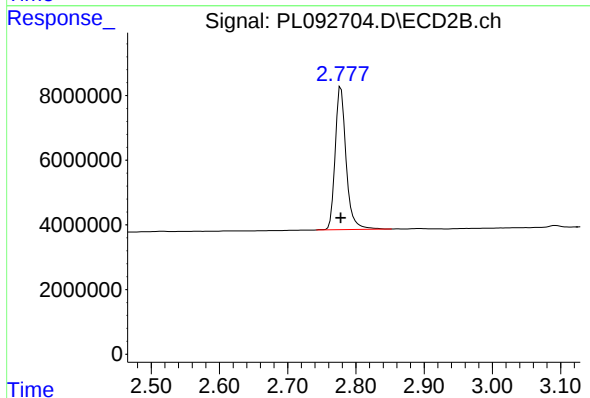


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 49207083
Conc: 18.08 ng/ml

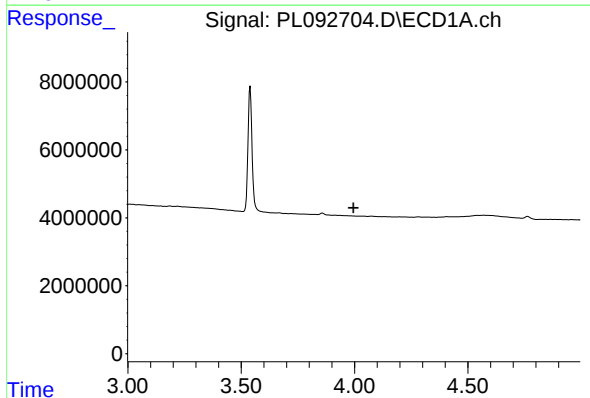


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

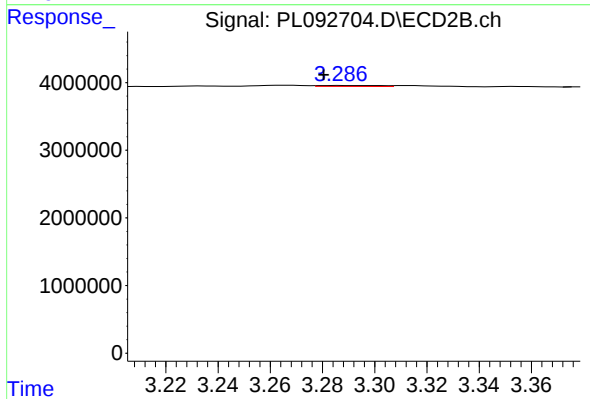

#2 alpha-BHC


R.T.: 3.288 min
Delta R.T.: 0.007 min
Response: 225749
Conc: 0.06 ng/ml

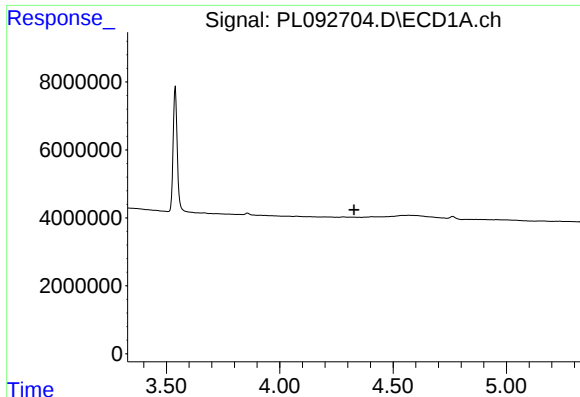

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164496BL

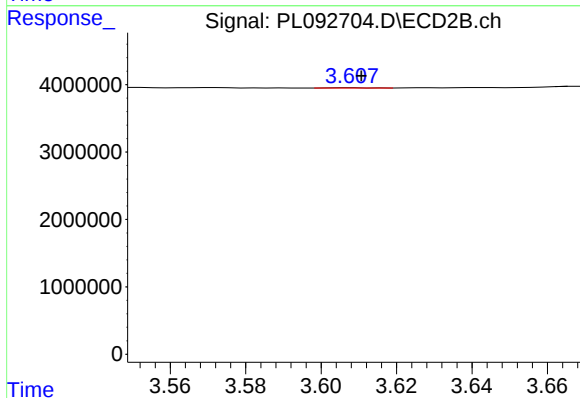


#3 gamma-BHC (Lindane)

R.T.: 3.609 min
Delta R.T.: -0.002 min
Response: 25248
Conc: 0.01 ng/ml

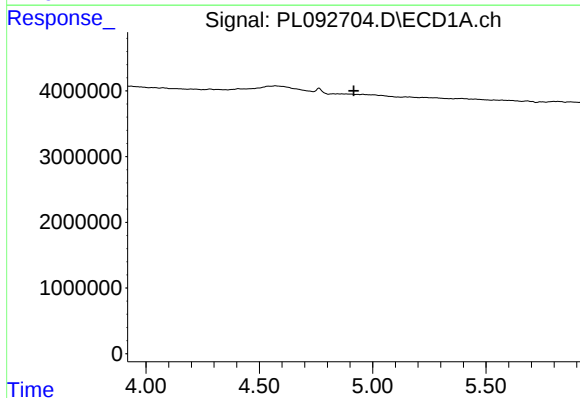


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.917 min
Response: 0
Conc: N.D.

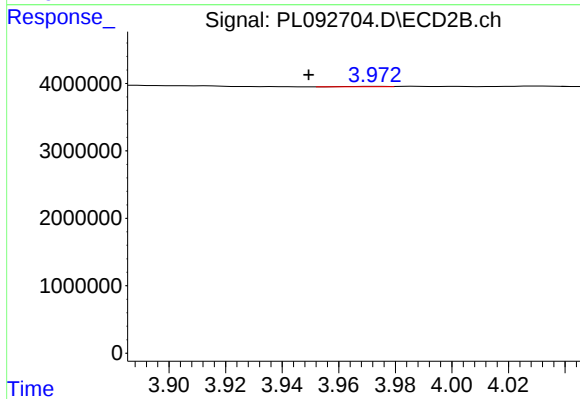

#4 Heptachlor


R.T.: 3.973 min
Delta R.T.: 0.024 min
Response: 59073
Conc: 0.02 ng/ml

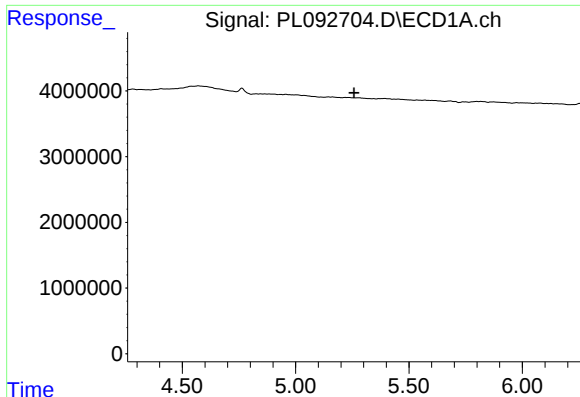

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164496BL

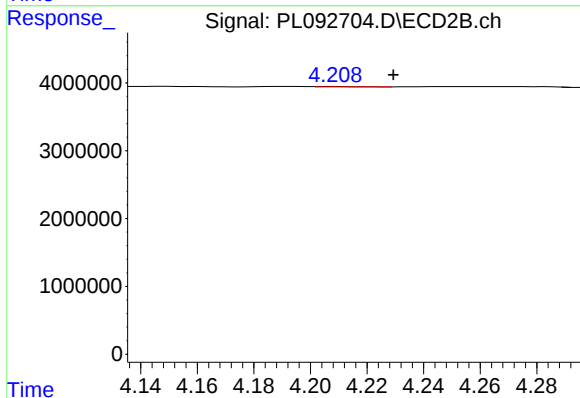


#5 Aldrin

R.T.: 4.209 min
Delta R.T.: -0.020 min
Response: 45578
Conc: 0.01 ng/ml

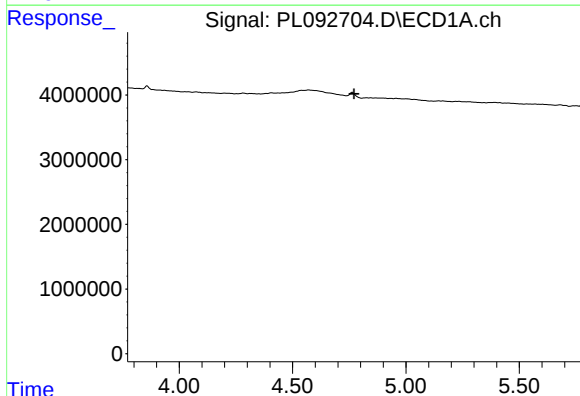


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.772 min
Response: 0
Conc: N.D.

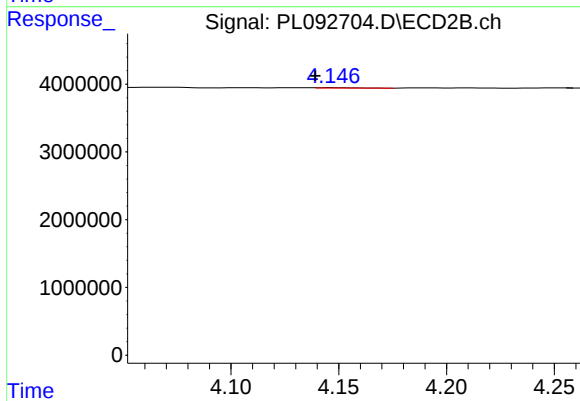

#7 delta-BHC


R.T.: 4.148 min
Delta R.T.: 0.009 min
Response: 82024
Conc: 0.02 ng/ml

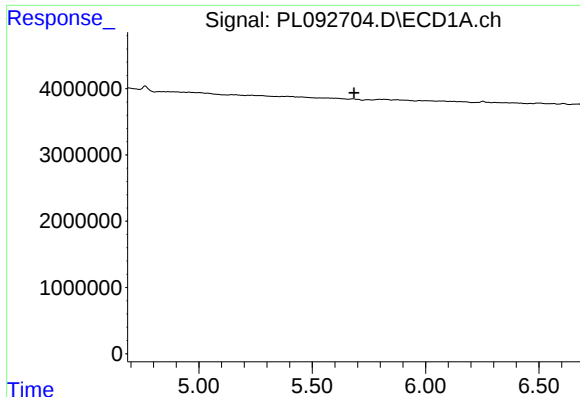

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164496BL

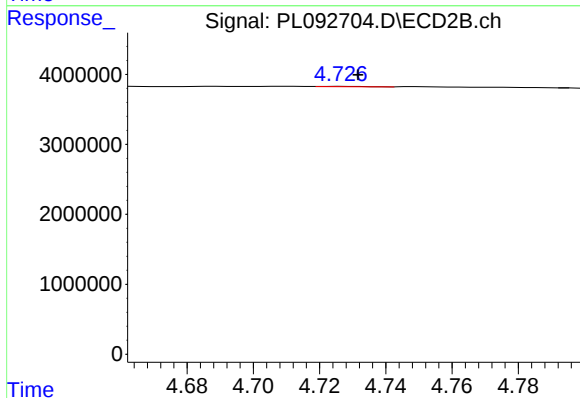


#8 Heptachlor epoxide

R.T.: 4.727 min
Delta R.T.: -0.005 min
Response: 55141
Conc: 0.02 ng/ml

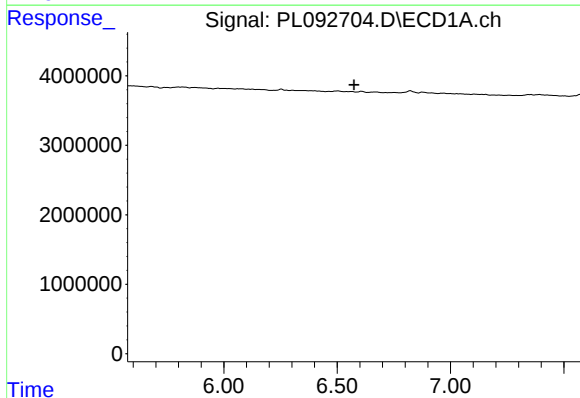


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

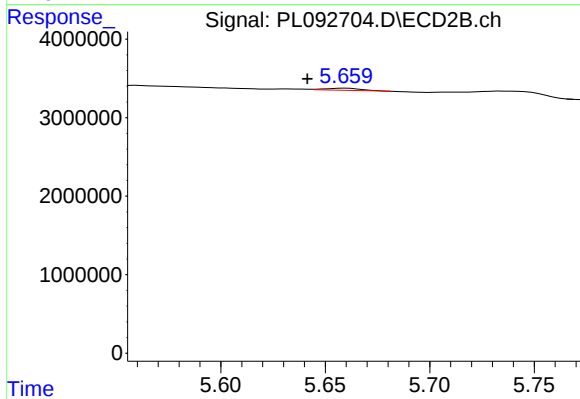

#14 Endrin


R.T.: 5.660 min
Delta R.T.: 0.019 min
Response: 304457
Conc: 0.11 ng/ml

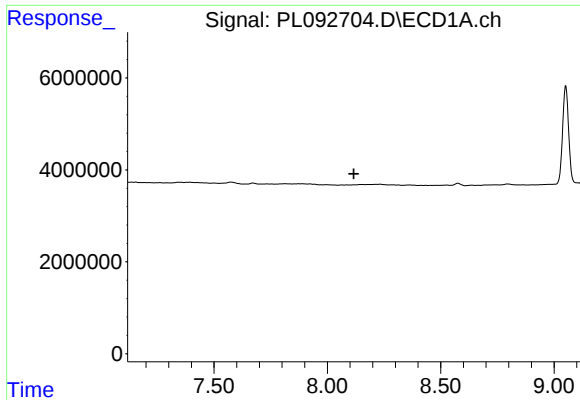

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164496BL

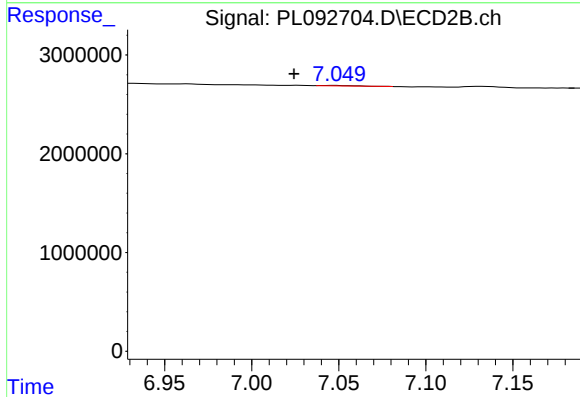


#22 Mirex

R.T.: 7.047 min
Delta R.T.: 0.023 min
Response: 21553
Conc: 0.01 ng/ml

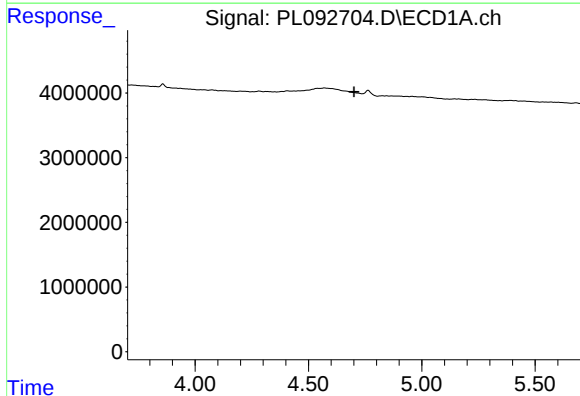


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.702 min
Response: 0
Conc: N.D.

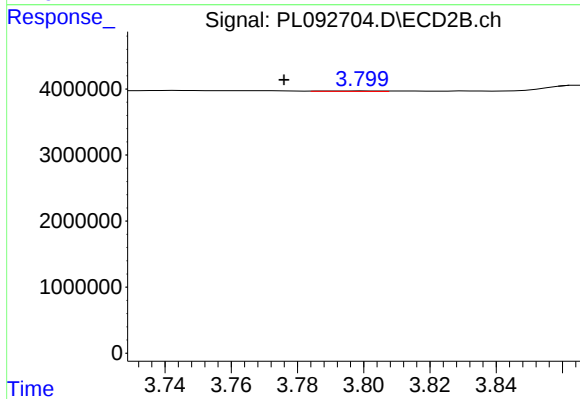

#23 Chlordane-1


R.T.: 3.792 min
Delta R.T.: 0.017 min
Response: 84962
Conc: 0.80 ng/ml

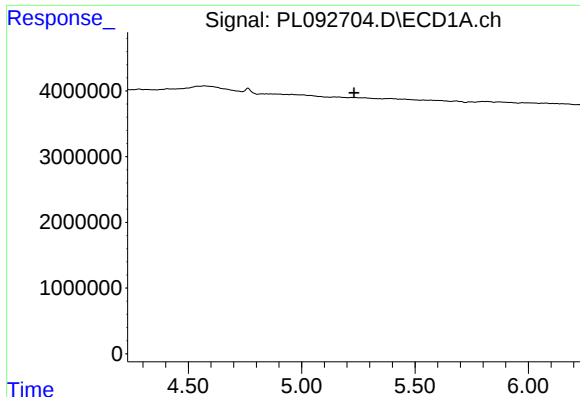

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164496BL

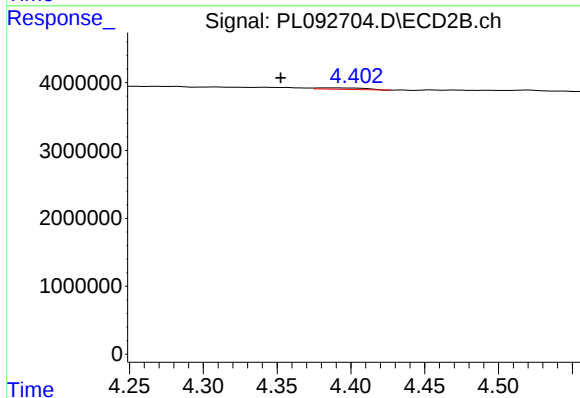


#24 Chlordane-2

R.T.: 4.385 min
Delta R.T.: 0.032 min
Response: 478599
Conc: 3.86 ng/ml

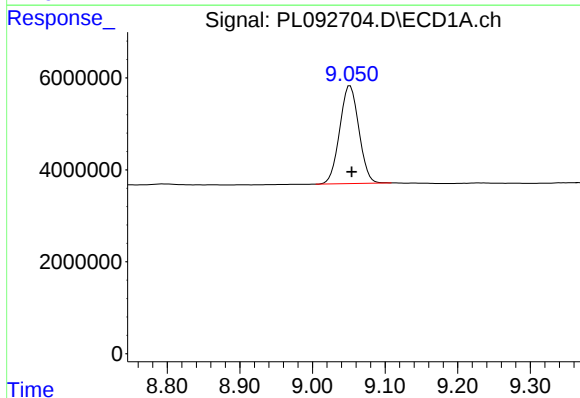

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.002 min
Response: 39150833
Conc: 20.34 ng/ml

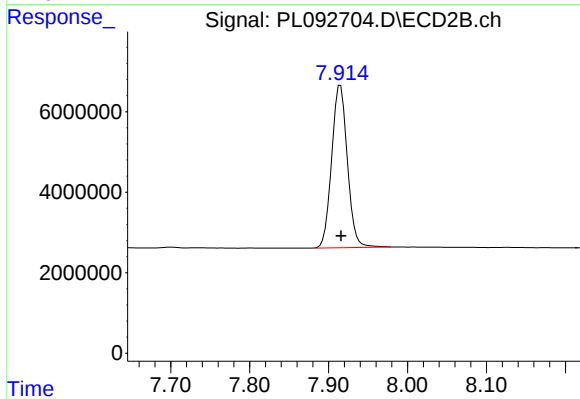

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 55848223
Conc: 20.46 ng/ml