

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
 Data File : PL041497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 13:30
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 04:01:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.104	133.6E6	63122501	20.969	20.493
28)	SA Decachlor...	8.215	9.236	125.2E6	50642017	18.899	19.765
Target Compounds							
7)	B delta-BHC	0.000	5.160	0	1988375	N.D.	0.492 #
10)	B gamma-Chl...	5.392	6.261	7337423	-802296	0.901	N.D. #
15)	B Endosulfa...	6.240f	0.000	6208166	0	0.898	N.D. #
23)	Chlordane-1	4.369	5.160	275740	1988375	0.972	14.316 #
25)	Chlordane-3	5.392	6.261	7337423	-802296	8.232	N.D. #
26)	Chlordane-4	5.451	6.261	1704633	-802296	2.177	N.D. #
27)	Chlordane-5	6.240	0.000	6208166	0	24.896	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL103018\
Data File : PL041497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 13:30
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 04:01:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

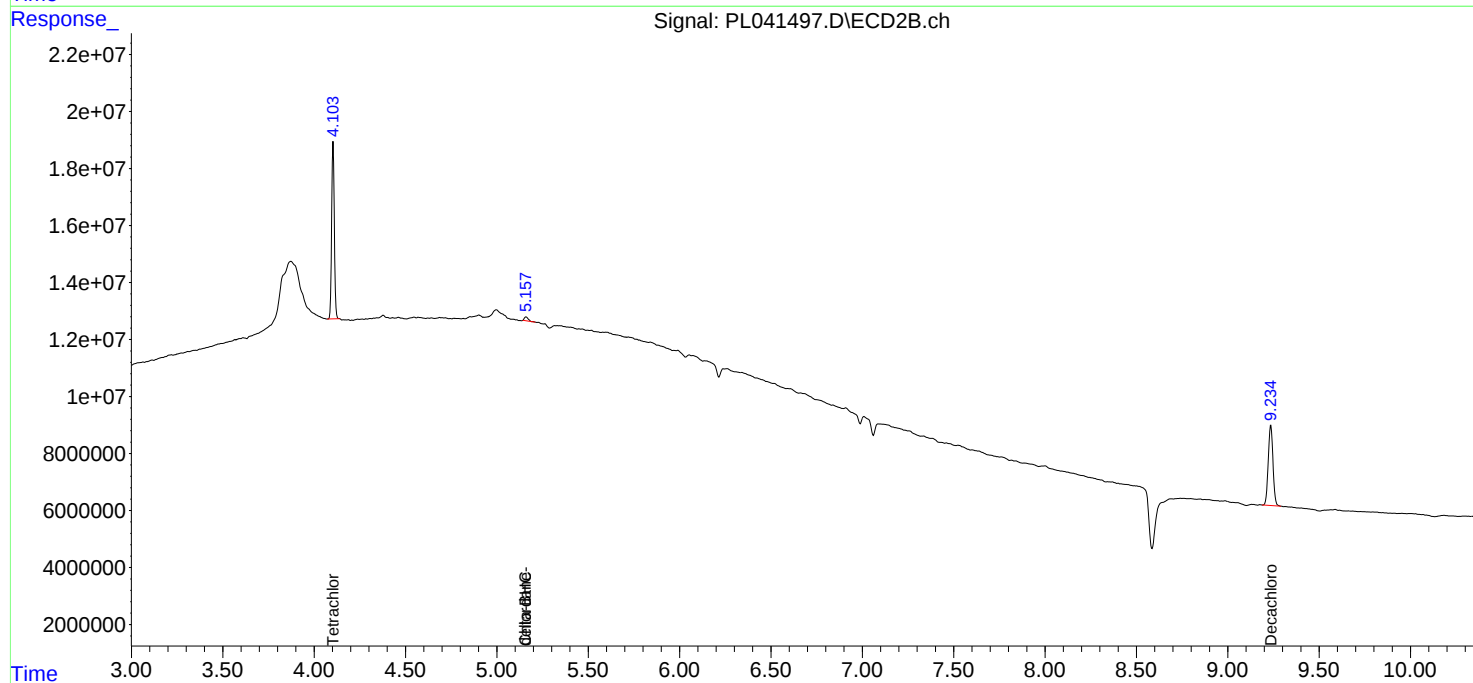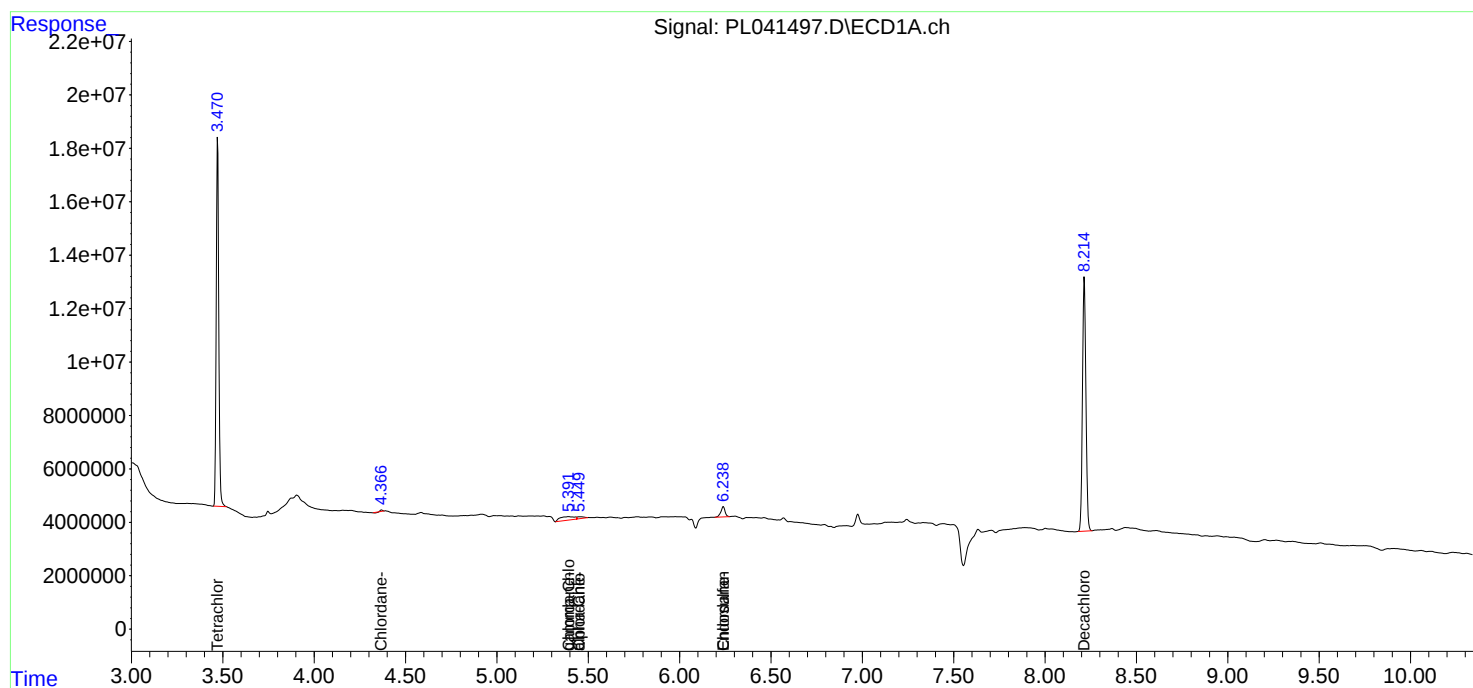


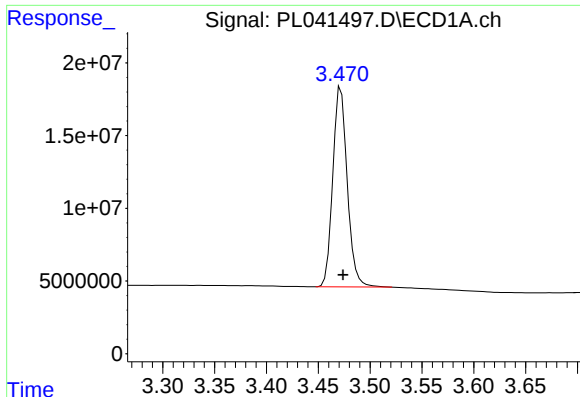

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 133578765
Conc: 20.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

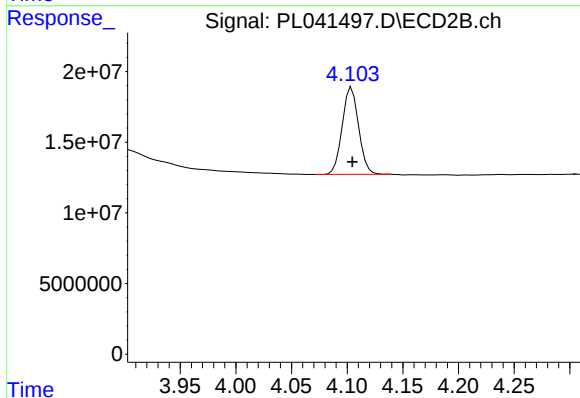


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 63122501
Conc: 20.49 ng/ml

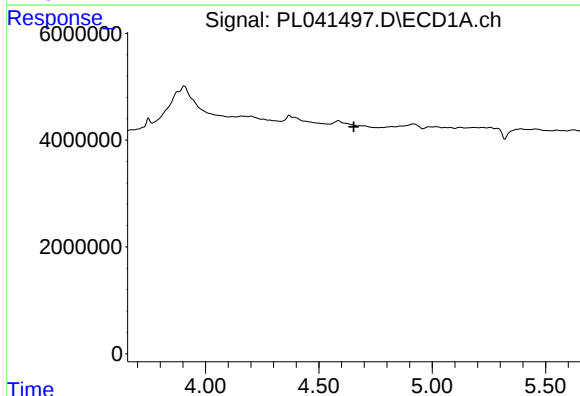


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

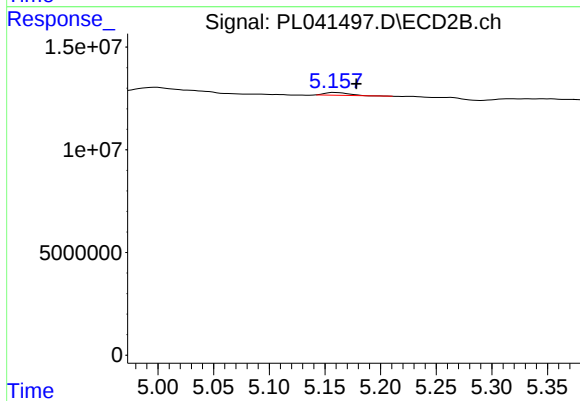

#7 delta-BHC


R.T.: 5.160 min
Delta R.T.: -0.019 min
Response: 1988375
Conc: 0.49 ng/ml

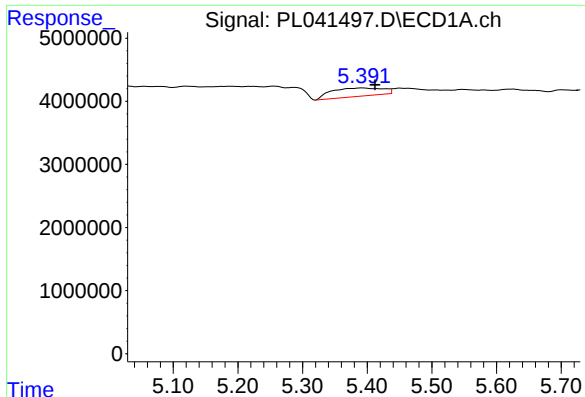

#10 gamma-Chlordane


R.T.: 5.392 min
Delta R.T.: -0.020 min
Response: 7337423
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

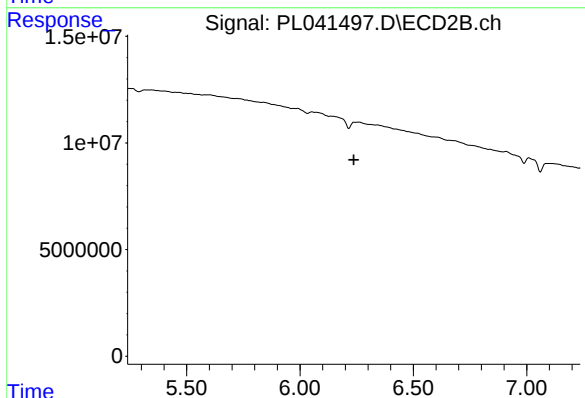


#10 gamma-Chlordane

R.T.: 6.261 min
Delta R.T.: 0.024 min
Response: -802296
Conc: N.D.

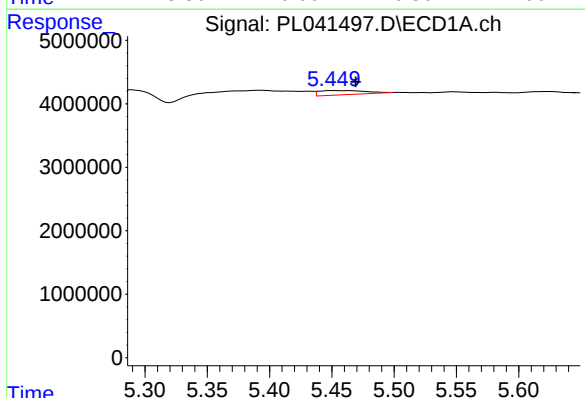


#11 alpha-Chlordane

R.T.: 5.451 min
Delta R.T.: -0.018 min
Response: 1704633
Conc: 0.21 ng/ml

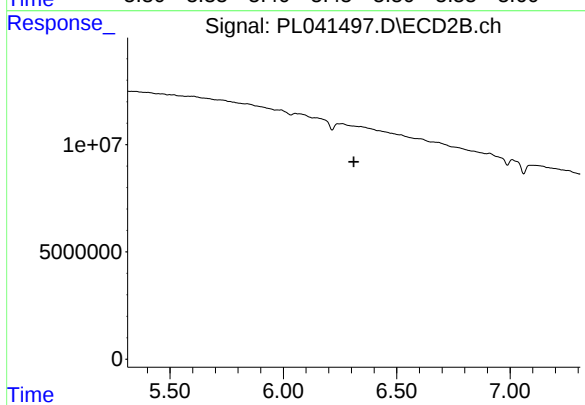

#11 alpha-Chlordane


R.T.: 6.261 min
Delta R.T.: -0.050 min
Response: -802296
Conc: N.D.

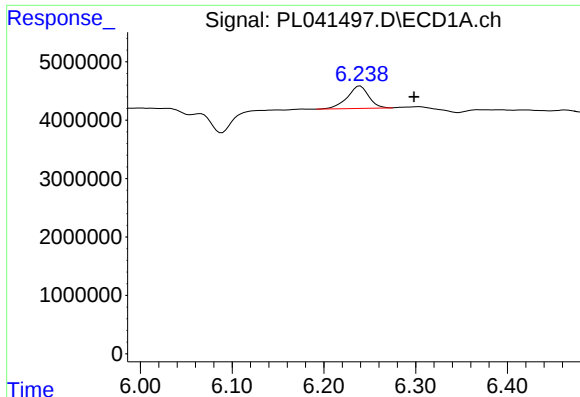

#15 Endosulfan II


R.T.: 6.240 min
Delta R.T.: -0.059 min
Response: 6208166
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

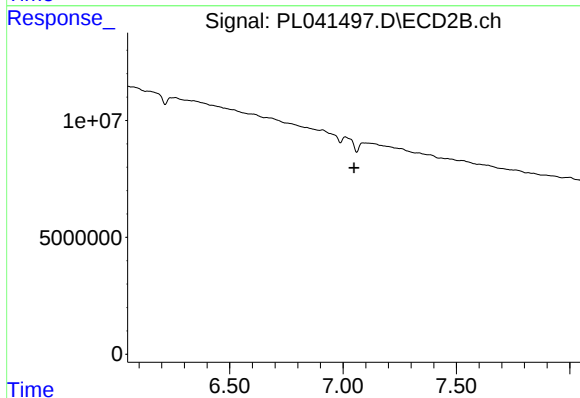


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

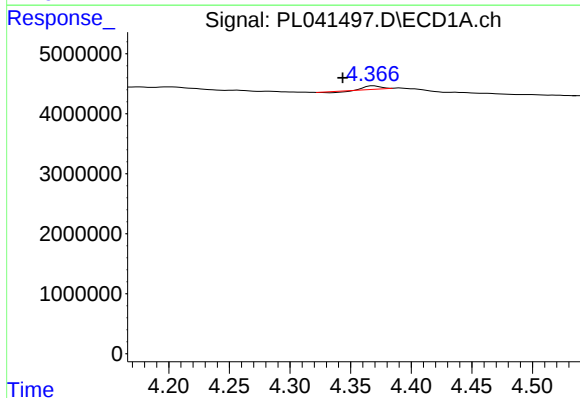


#23 Chlordane-1

R.T.: 4.369 min
Delta R.T.: 0.026 min
Response: 275740
Conc: 0.97 ng/ml

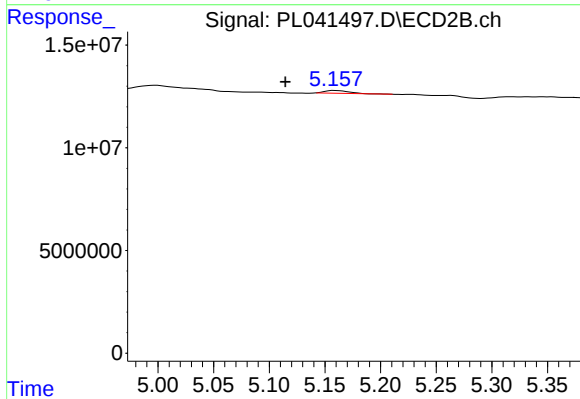

#23 Chlordane-1


R.T.: 5.160 min
Delta R.T.: 0.045 min
Response: 1988375
Conc: 14.32 ng/ml

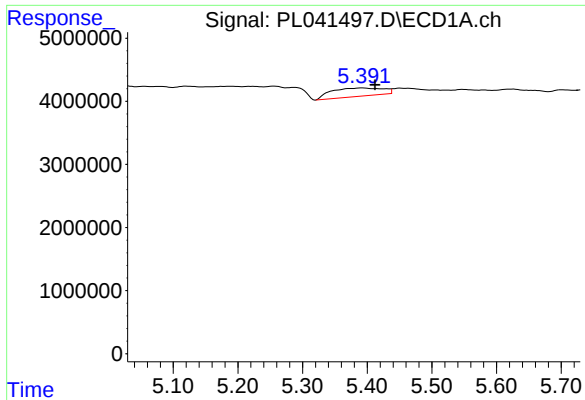

#25 Chlordane-3


R.T.: 5.392 min
Delta R.T.: -0.020 min
Response: 7337423
Conc: 8.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

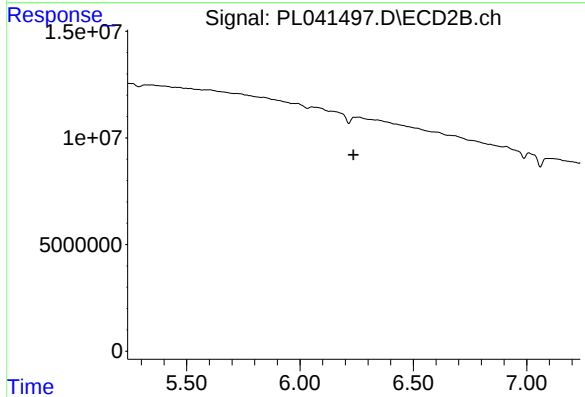


#25 Chlordane-3

R.T.: 6.261 min
Delta R.T.: 0.025 min
Response: -802296
Conc: N.D.

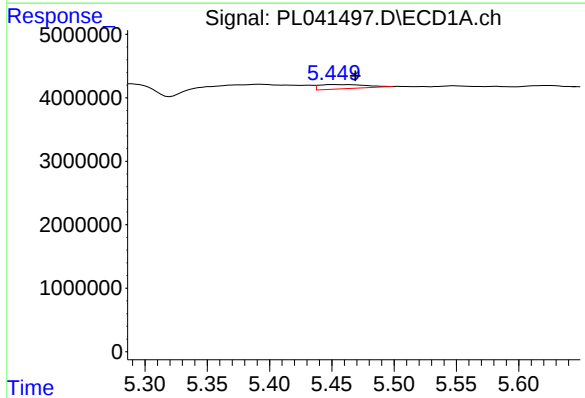


#26 Chlordane-4

R.T.: 5.451 min
Delta R.T.: -0.018 min
Response: 1704633
Conc: 2.18 ng/ml

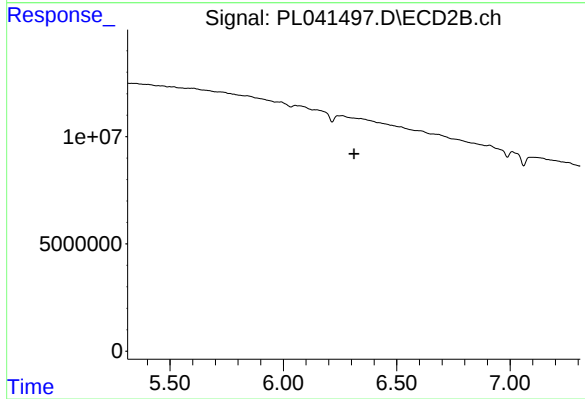

#26 Chlordane-4


R.T.: 6.261 min
Delta R.T.: -0.050 min
Response: -802296
Conc: N.D.

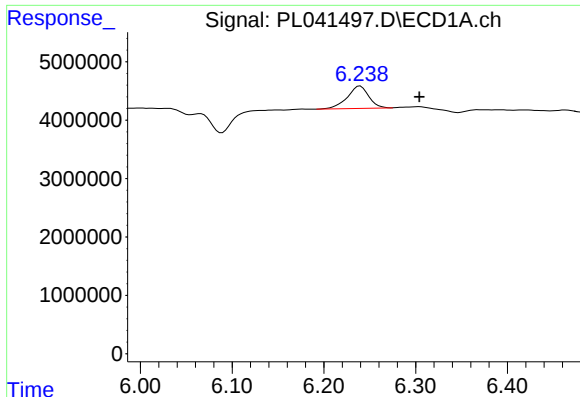

#27 Chlordane-5


R.T.: 6.240 min
Delta R.T.: -0.065 min
Response: 6208166
Conc: 24.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

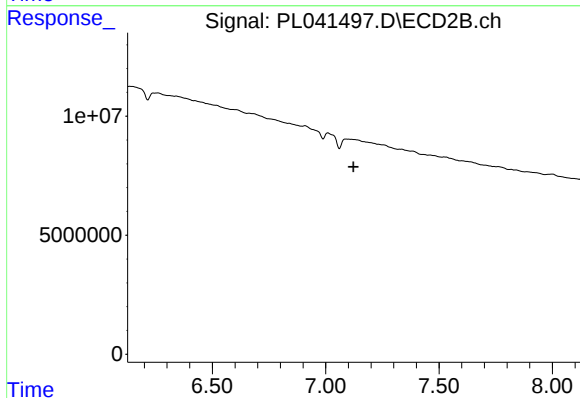


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.123 min
Response: 0
Conc: N.D.

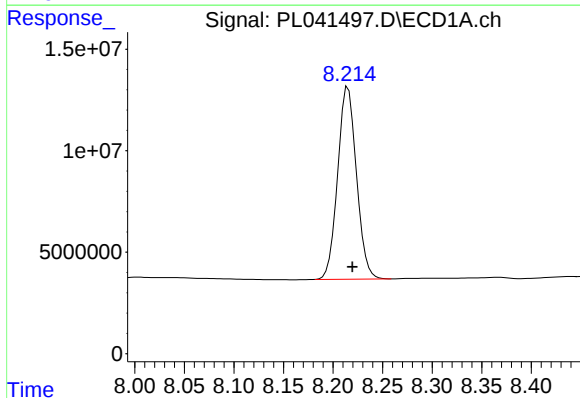

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.004 min
Response: 125184748
Conc: 18.90 ng/ml

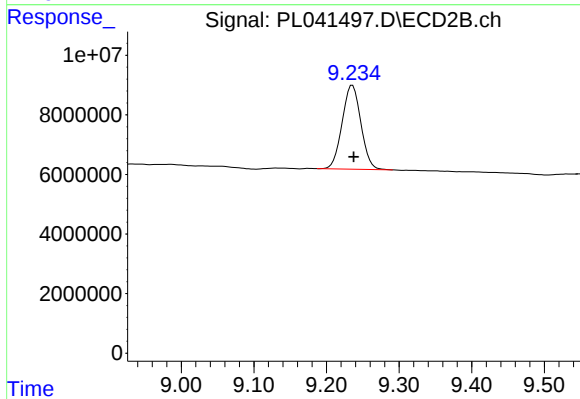

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.002 min
Response: 50642017
Conc: 19.77 ng/ml